



SIEMENS


How to scan with CARE kV

**For all SOMATOM Scanners equipped with FAST CARE
syngo CT 2011**


By B. Schmidt, R. Raupach and T. Flohr

siemens.com/healthcare

SIEMENS

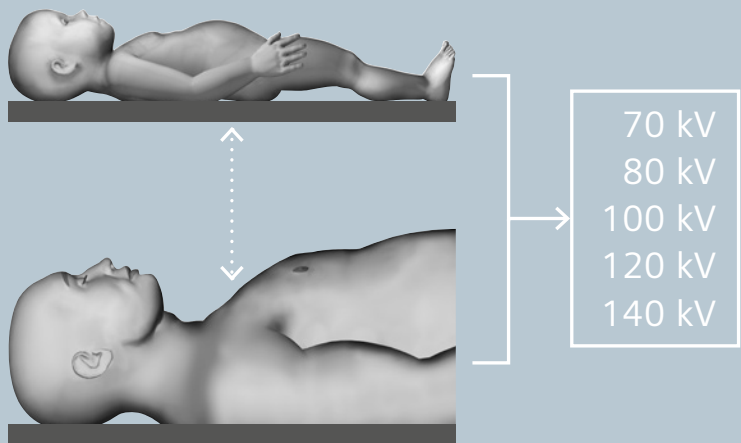

The three different modes of CARE kV in the Scan Card

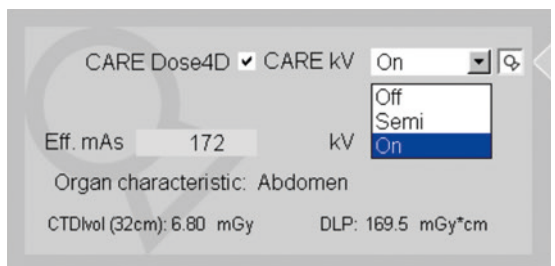

General

CARE kV is a fully automated feature that adjusts the tube voltage tailored to the individual patient, the system capabilities and the clinical task. In combination with CARE Dose4D, it allows the patient-specific adaptation of both dose relevant parameters, tube current and tube voltage.

The potential for patient dose reduction by adjusting the tube voltage (kV) is well-known. But this can be challenging as then the tube current might have to be adapted as well to maintain image quality. CARE kV is a fully automated feature integrated into the workflow at the CT scanner that optimizes tube voltage while the tube current is adapted with CARE Dose4D simultaneously.

With CARE Child Siemens now offers the possibility of scanning with 70 kV. Thus five different kV settings are available: 70 kV, 80 kV, 100 kV, 120 kV and 140 kV.

The three different modes of CARE kV

“On”: The system will propose optimized settings for tube voltage and tube current based on the patient’s topogram and your reference settings.

“Off”: The scan is performed with the kV setting defined in the respective scan protocol. Optimization of tube voltage is not performed.

“Semi”: A user specified kV setting will be used and mAs-values will be adjusted based on your specified reference values and the topogram. This is particularly helpful for follow-up exams where a constant kV-setting is desirable.


Prerequisites

Some prerequisites have to be met once before you start scanning with CARE kV. These prerequisites are then defined as your standard settings.



Configure the **“Quality reference mAs”** and **“Reference kV”** according to your clinical needs. Define values that you would use for a standard sized adult patient weighing 75 kg. Siemens standard protocols that come along with the system are a good starting point.

Select the exam type by setting the slider **“Dose saving optimized for”**. For CT Angiography examinations the slider should be positioned at 11, for non-contrast enhanced scans at 3. For contrast enhanced scans of parenchymatous organs such as the liver, a setting in between (7) is recommended.

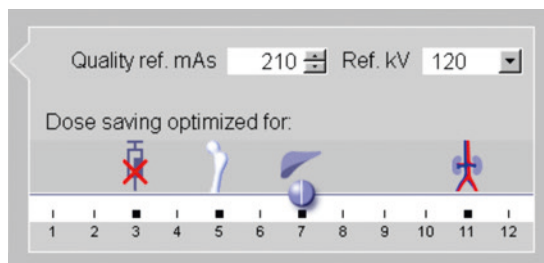

In the Scan Protocol Assistant, you can define the minimum and the maximum value for the kV setting which CARE kV should use for optimization for a specific scan range.

Guided workflow

Once your prerequisites have been defined CARE kV uses your specified standard values for “Quality reference mAs”, the “Reference kV” and the slider position in the Scan Card. These are the steps that have to be done when scanning with CARE kV.

Position the patient into the iso-center of the scanner to ensure that CARE Dose4D and CARE kV function optimally.




Ensure the topogram is long enough to cover the entire planned scan range.

Select ‘On’ in the CARE kV drop-down menu of the Scan Card.



If you need to perform subsequent acquisitions with the same kV e.g. in case of multiphase exams, you can force CARE kV to use the same kV by linking the series. The optimization is then done by considering all linked acquisitions.

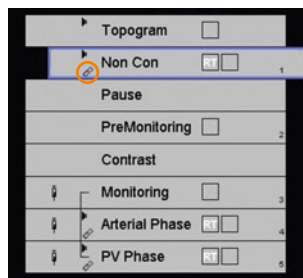

The “chain-link” icon indicates the linked acquisitions within one series. The same kV setting will be chosen.

Tips and tricks



The “Quality reference mAs” and the “Reference kV” refer to a standard 75 kg patient. Specify values that you would use in such a standard patient.

The slider position for the optimization criteria of CARE kV should not be changed for the individual patient. Set it once depending on the clinical task!

A manual adaptation of the viewing window is not necessary. This is performed automatically by CARE kV (see recon sub task card: “FAST Adjust”).



If CARE kV doesn’t perform as expected first check the “Quality reference mAs” value and CARE Dose4D settings, and if contrast was administered properly. Secondly double-check that the slider position has been correctly selected for the clinical task.



It is not necessary to modify the settings in case of an obese patient. The system not only decreases kV, but also increases kV if necessary.

Low kV selection can be limited by the power reserves of the system, especially for high-pitch values. Try reducing the pitch if you feel that CARE kV doesn’t go low enough for these cases. That might well be so for chest examinations or in very slim patients.



Choosing lower kV-settings typically requires an increase in mAs to maintain image quality. However, even with such increased mAs-settings, the dose can be reduced. Monitor the $CTDI_{vol}$ value prior to scanning to estimate the actual exposure during the scan.


For the relationship of mAs, kV and image quality see page 8/9.



CARE kV – the principle


The basis to discuss CARE kV is an understanding of image quality and how it changes when changing kV. Further on it is important to understand what is the impact of changing kV on dose.

Image quality is defined in a technical way as the contrast-to-noise ratio (CNR). To maintain the same image quality, the CNR has to be constant. Different materials respectively tissues show different behavior when the kV is changed. The plots below illustrate the scenario for contrast, noise and dose for the **example of iodine** (CT Angiography exams at a given patient size).

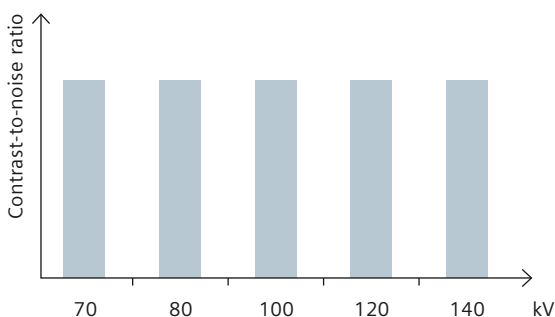


Contrast-to-noise ratio

The goal of CARE kV is to maintain a desired image quality (CNR) independent of the kV at the lowest possible dose.

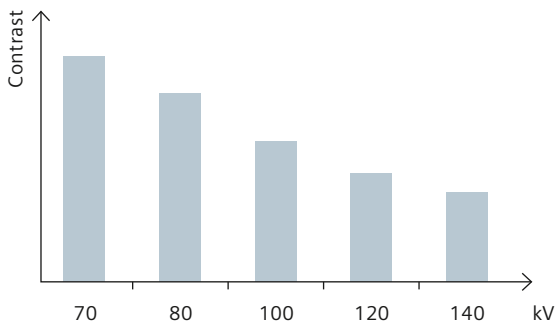

Contrast


Contrast of most materials – particularly iodine – increases for lower kV.

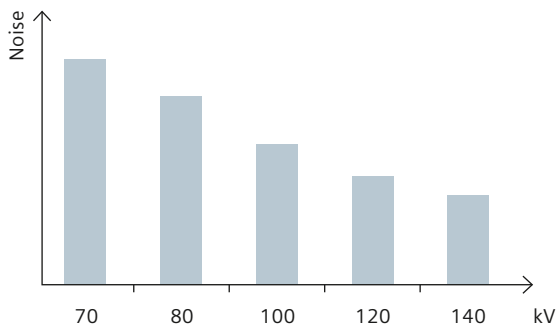

Noise

As contrast increases, noise can be allowed to increase by the same extent to maintain the CNR. For each kV level, the respective mAs required to get to the desired noise level has to be determined.

Note: Due to CT system limitations (e.g. tube load), some kV settings which theoretically provide the best performance are dismissed

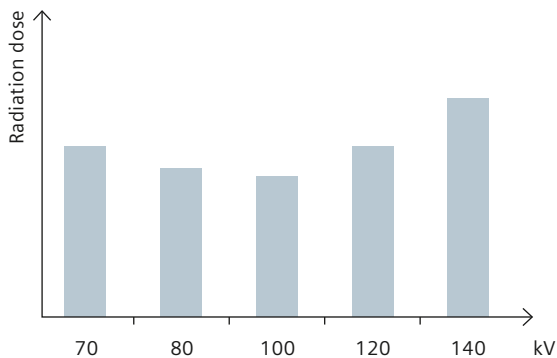

Radiation dose

Image quality can be maintained while dose is reduced when the optimal kV setting for each clinical task is chosen. In this case 100 kV with the respective mAs values would be the proposed scan technique.

Note: Lowest dose does not necessarily mean lowest kV!

CARE kV – the principle



In addition CARE kV takes the **patient size** and its changes along the patient's length axis into account. For small patients typically the CNR increases when going to lower kV, for bigger patients the optimal tube voltage is more towards higher kVs.

This is an example how CARE kV and CARE Dose4D optimize the parameters for the individual examination.

Reference setting		Actual settings with CARE Dose4D and CARE kV*	
Body CT Angiography examination of the Aorta		Adult patient, Body Mass Index 25.4 kg/m ²	
"Quality reference mAs"	110 mAs	Effective mAs	143 mAs
"Reference kV"	120 kV	kV	100 kV
CTDI _{vol}	10.59 mGy	CTDI _{vol}	6.4 mGy

* CARE Dose4D on, CARE kV on, slider position "Dose saving optimized for": 11. According to: Winklehner A et al. Automated Attenuation-Based Tube Potential Selection for Thoracoabdominal Computed Tomography Angiography: Improved Dose Effectiveness. Invest Radiol. 2011 Jul 1. [Epub ahead of print]

Thus, CARE kV enables an individualized patient care by optimizing scan parameters for each individual patient and the clinical question.



In the event that upgrades require FDA approval, Siemens cannot predict whether or when the FDA will issue its approval. Therefore, if regulatory clearance is obtained and is applicable to this package, it will be made available according to the terms of this offer.

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice. Some/All of the features and products described herein may not be available in the United States.

The information in this document contains general technical descriptions of specifications and options as well as standard and optional features which do not always have to be present in individual cases.

Siemens reserves the right to modify the design, packaging, specifications, and options described herein without prior notice. Please contact your local Siemens sales representative for the most current information.

Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Siemens Healthcare Headquarters

Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany
Phone: +49 9131 84-0
[siemens.com/healthcare](https://www.siemens.com/healthcare)

[siemens.com/healthcare](https://www.siemens.com/healthcare)