

syngo MI.PET/CT 2008A

MI

DICOM Conformance Statement

D0007769

Version 04

Release Date: December 6, 2007

Copyright by Siemens Medical Solutions USA, Inc.

Table of Contents

Table of Contents	3
List of Figures	7
List of Tables	8
1 Introduction	11
1.1 Overview	11
1.2 Audience.	11
1.3 Scope	11
1.4 Definitions, Acronyms and Abbreviations	12
1.4.1 Definitions	12
1.4.2 Acronyms and Abbreviations	12
1.5 References	12
1.6 Connectivity and Interoperability	13
Part I - Network	14
2 Implementation Models	15
2.1 Verification	15
2.1.1 Application Data Flow Diagram	15
2.1.2 Functional Definitions of Application Entities.	15
2.1.3 Sequencing of Real-World Activities	15
2.2 Storage.	16
2.2.1 Application Data Flow Diagram	16
2.2.2 Functional Definitions of Application Entities.	16
2.2.3 Sequencing of Real-World Activities	17
2.3 Storage Commitment Push Model.	18
2.3.1 Application Data Flow Diagram	18
2.3.2 Functional Definitions of Application Entities.	18
2.3.3 Sequencing of real World Activities	19
2.4 Query/Retrieve	20
2.4.1 Application Data Flow Diagram	20
2.4.2 Functional Definitions of Application Entities.	21
2.4.3 Sequencing of Real-World Activities	21
2.5 Print	22
2.5.1 Application Data Flow Diagram	22
2.5.2 Functional Definitions of Application Entities.	22
2.5.3 Sequencing of Real-World Activities	22
2.6 Worklist.	23
2.6.1 Application Data Flow Diagram	23
2.6.2 Functional Definitions of Application Entities.	23

2.6.3	Sequencing of Real-World Activities.	24
2.7	Modality Performed Procedure Step.	25
2.7.1	Application Data Flow Diagram	25
2.7.2	Functional Definitions of Application Entities	25
2.7.3	Sequencing of real World Activities	25
3	AE Specifications	26
3.1	Verification AE Specification	26
3.1.1	Association Establishment Policies.	26
3.1.2	Association Initiation by Real-World Activity	26
3.1.3	Association Acceptance Policy	27
3.2	Storage AE Specification	27
3.2.1	Association Establishment Policies.	29
3.2.2	Association Initiation by Real-World Activity	30
3.2.3	Association Acceptance Policy	35
3.3	Storage Commitment AE Specification	44
3.3.1	Association Establishment Policies.	44
3.3.2	Association Initiation Policy	45
3.3.3	Association Acceptance Policy	46
3.4	Query/Retrieve AE Specification	48
3.4.1	Association Establishment Policies.	49
3.4.2	Association Initiation Policy	50
3.4.3	Association Acceptance Policy	58
3.5	Print AE Specification	77
3.5.1	Association Establishment Policies.	78
3.5.2	Association Initiation Policy	78
3.6	Modality Worklist AE Specification.	102
3.6.1	Association Establishment Policies.	102
3.6.2	Association Initiation Policy	103
3.7	Modality Performed Procedure Step AE Specification	114
3.7.1	Association Establishment Policies.	114
3.7.2	Association Initiation Policy	115
4	Communication Profiles.	124
4.1	Supported Communication Stacks	124
4.1.1	OSI Stack	124
4.1.2	TCP/IP Stack	124
4.1.3	Point-to-Point Stack.	124
5	Extensions/Specializations/Privatizations	125
5.1	Standard Extensions	125
5.1.1	Standard Extensions of all SOP Classes	125
5.1.2	Specializations	133
5.2	Privatizations.	153

5.2.1	Private Elements for Storage SOP Classes.	153
5.2.2	Private Elements for CT Image Storage SOP Class	158
5.2.3	Private SOP class CSA Non-Image	160
5.2.4	Private SOP Classes	164
5.2.5	Private Transfer Syntaxes	165
6	Configuration	166
6.1	AE Title / Presentation Address Mapping.	166
6.1.1	DICOM Verification	166
6.1.2	DICOM Storage/StorageCommitment/QR AE Title.	166
6.1.3	DICOM Modality Worklist and MPPS AE Title	166
6.1.4	DICOM Print AE Title	166
6.1.5	Remote AE Titles and Presentation Addresses	166
6.2	Configurable Parameters	167
6.2.1	Storage, Storage Commitment and Query/Retrieve	167
6.2.2	Print.	167
6.2.3	Modality Worklist	168
6.2.4	Modality Performed Procedure Step	168
6.3	Default Parameters	168
7	Support of Extended Character Sets.	170
	Part II - Media Storage	171
8	Implementation Model	172
8.1	Application Data Flow Diagram	172
8.2	Functional definitions of AE's	172
8.3	Sequencing of Real-World Activities	173
8.4	File Meta Information Options	173
9	AE Specifications	174
9.1	DICOM Archive Specification	174
9.1.1	File Meta Information for the Application Entity	174
9.1.2	Real-World Activities for this Application Entity	174
10	Augmented and Private Profiles	178
10.1	Augmented Application Profiles	178
10.1.1	AUG-GEN-CD	178
10.1.2	AUG-CTMR-xxxx	178
10.1.3	AUG-XA1K-CD	178
10.2	syngo® private offline Media Application Profiles	179
10.2.1	Class and Profile Identification	179
10.2.2	Clinical Context	179
10.2.3	PRI-SYNGO Profiles.	181
11	Extensions, Specializations and Privatizations of SOP Classes and Trans-	

fer Syntaxes	193
11.1 SOP Specific Conformance Statement for Basic Directory	193
11.1.1 Extension, Specialization for SIEMENS Non-Image Objects	193
12 Configuration	194
12.1 AE Title Mapping	194
12.1.1 DICOM Media Storage AE Title	194
13 Support of Extended Character Sets	195
A Appendix	196
A.1 CT Standard Extended SOP Class	196
A.1.1 Examination (Spiral)	196
A.1.2 Body Perfusion	202
A.1.3 Calcium Scoring	211
A.1.4 Dental CT	217
A.1.5 DynEva	222
A.1.6 Evaluation (Average/Subtract/Filter)	228
A.1.7 Lung Care	235
A.1.8 Neuro Perfusion	240
A.1.9 Osteo CT	250
A.1.10 Pulmo CT	255
A.1.11 Vessel View	261
A.1.12 Volume CT	267
A.2 SC Standard Extended SOP Class	273
A.2.1 Care Bolus	273
A.2.2 DynEva	278
A.2.3 InSpace	283
A.2.4 Lung Care Result	289
A.2.5 Lung Care Report	294
A.2.6 Osteo	298
A.2.7 Vessel View	303
A.2.8 Volume CT	308
Index	314

List of Figures

Figure 1:	Application Data Flow Diagram Verification SCU	15
Figure 2:	Application Data Flow Diagram C-STORE SCU.....	16
Figure 3:	Application Data Flow Diagram C-STORE SCP	16
Figure 4:	Application Data Flow Diagram Storage Commitment SCU	18
Figure 5:	Application Data Flow Diagram QUERY/RETRIEVE SCU	20
Figure 6:	Application Data Flow Diagram QUERY/RETRIEVE SCP	21
Figure 7:	Application Data Flow Diagram PRINT SCU	22
Figure 8:	Application Data Flow Diagram BASIC WORKLIST SCU	23
Figure 9:	Application Data Flow Diagram MODALITY PERFORMED PROCEDURE STEP SCU	25
Figure 10:	DICOM Information Model.....	161

List of Tables

Table 1:	Siemens <i>Biograph</i> Products	11
Table 2:	Initiation presentation context Verification.....	27
Table 3:	Standard SOP Classes as an Storage SCU and an SCP.....	27
Table 4:	Private SOP Classes as an Storage SCU and an SCP	29
Table 5:	Initiation presentation context Storage.....	30
Table 6:	Acceptable presentation contexts Storage.....	36
Table 7:	Standard SOP Classes as Storage Commitment Push Model	44
Table 8:	Initiation presentation context Storage Commitment Request.....	45
Table 9:	Presentation context accepted for Storage Commitment	46
Table 10:	SOP Classes as an Query/Retrieve SCU	48
Table 11:	SOP Classes as an Query/Retrieve SCP.....	48
Table 12:	Proposed Presentation Contexts - Find SCU:	50
Table 13:	Query attributes	52
Table 14:	C-FIND response status	55
Table 15:	Proposed Presentation Contexts - Move SCU.....	56
Table 16:	C-MOVE response status	57
Table 17:	Accepted Presentation Contexts - Find SCP:.....	60
Table 18:	Patient level attributes, Patient Root Information Model.....	62
Table 19:	Study level attributes, Patient Root Information Model	62
Table 20:	Series level attributes, Patient Root Information Model	63
Table 21:	Image level attributes, Patient Root Information Model.....	64
Table 22:	Study level attributes, Study Root Information Model	66
Table 23:	Series level attributes, Study Root Information Model.....	67
Table 24:	Image level attributes, Study Root Information Model.....	68
Table 25:	Patient instance level, Patient Study Only Information Model.....	69
Table 26:	Study level attributes, Patient Study Only Information Model.....	69
Table 27:	C-FIND return status	71
Table 28:	Accepted Presentation Contexts -- Get SCP	72
Table 29:	C-GET return status	73
Table 30:	Accepted Presentation Contexts - Move SCP	74
Table 31:	C-MOVE return status	75
Table 32:	Basic Gray Scale Print Management Meta SOP-Classes.....	77
Table 33:	Basic Color Print Management Meta SOP-Classes	77
Table 34:	Presentation context - Print SCU	80
Table 35:	Used Basic Film Session N-CREATE_RQ attributes.....	82
Table 36:	Attributes of the N-DELETE-RQ on the Basic Film Session SOP Class.....	82
Table 37:	Basic Film Session SOP status.....	82
Table 38:	Used Film Box N-CREATE_RQ attributes	83
Table 39:	Attributes of the N_DELETE_RQ on the Basic Film Session SOP Class.....	85
Table 40:	Basic Film Box SOP status	85
Table 41:	Used Basic Grayscale Image Box N-SET attributes.....	85
Table 42:	Basic Grayscale Image Box SOP status.....	86
Table 43:	Used Basic Color Image Box N-SET attributes.....	87
Table 44:	Basic Color Image Box SOP status.....	87

Table 45:	Attributes of the N_CREATE_RQ on the Presentation LUT SOP Class	88
Table 46:	Attributes of the N_DELETE_RQ on the Presentation LUT SOP Class	88
Table 47:	Presentation LUT SOP status	88
Table 48:	Used Printer N-EVENT report	89
Table 49:	Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes	89
Table 50:	Used Print Job N-EVENT report	90
Table 51:	Printer Status Infos within Printer SOP Class/Execution Status Infos within Print Job SOP Class	91
Table 52:	Printer Status Infos: Additional Agfa printer status infos	98
Table 53:	Printer Status Infos: Additional Kodak infos for Pacs Link (formerly Imation cameras)	98
Table 54:	Printer Status Infos: Additional Kodak infos for Kodak 190	98
Table 55:	Printer Status Infos: Additional Kodak infos for 2180/1120	99
Table 56:	Printer Status Infos: Additional Codonics infos	99
Table 57:	SOP Classes as an SCU	102
Table 58:	Proposed presentation contexts	103
Table 59:	Search Key Attributes in a broad worklist query	104
Table 60:	Basic Worklist C_FIND_RSP Return Key Attributes	105
Table 61:	Search Key Attributes in a patient based worklist query	111
Table 62:	C-FIND Response Status	112
Table 63:	SOP Classes as an SCU	114
Table 64:	Proposed presentation contexts	115
Table 65:	Performed Procedure Step N-CREATE Attributes	116
Table 66:	N-SET Response Status	119
Table 67:	Performed Procedure Step N-SET Attributes	120
Table 68:	N-SET Response Status	123
Table 69:	Standard Extensions of all SOP Classes	125
Table 70:	Image Type (0008,0008) for objects created by PETsyngo	132
Table 71:	Image Type (0008,0008) for objects created by PETsyngo	133
Table 72:	PETsyngo CT Attribute Interpretation	137
Table 73:	PETsyngo PET Attribute Interpretation	144
Table 74:	CSA Image IOD Modules	155
Table 75:	CSA Image Header Module	155
Table 76:	CSA Series Header Module	156
Table 77:	MEDCOM Header Module	156
Table 78:	MEDCOM History Information	158
Table 79:	MEDCOM OOG Module	158
Table 80:	CSA Non-Image IOD Modules	161
Table 81:	CSA Non-Image Module	162
Table 82:	(Non-)Image Type (0008,0008) for private Non-image Objects	164
Table 83:	SOP Classes	164
Table 84:	Application profiles, Activities, and Roles for DICOM Archive	174
Table 85:	SOP Classes and Transfer Syntax	181
Table 86:	DICOMDIR keys	190
Table 87:	DICOMDIR keys for CsaNonImage	191
Table 88:	CT Acquisition/Reconstruction - Mode SPIRAL	196
Table 89:	Body Perfusion	202

Table 90: Calcium Scoring.....	211
Table 91: Dental CT	217
Table 92: DynEva created CT images.....	222
Table 93: Evaluation (Average/Subtract/Filter)	228
Table 94: LungCARE - CT Images.....	235
Table 95: Neuro Perfusion.....	240
Table 96: Osteo CT	250
Table 97: Pulmo CT	255
Table 98: Vessel View Result Images - CT	261
Table 99: Volume CT, saved CT Images	267
Table 100: Care Bolus.....	273
Table 101: DynEva created SC Images.....	278
Table 102: InSpace.....	283
Table 103: CT LungCARE - Result.....	289
Table 104: CT LungCARE - Report	294
Table 105: Osteo - SC Image	298
Table 106: VesselView - SC result image	303
Table 107: Volume CT, Result Image (CSA BLACK IMAGE)	308

1 Introduction

1.1 Overview

This DICOM Conformance Statement is written according to part PS 3.2 of [1].

The applications described in this DICOM Conformance Statement are implemented in Biograph products using software syngo MI.PET/CT 2008A (internal name: PETsyngo 6.0).

syngo MI.PET/CT 2008A is based on Somaris/5, the SW platform for CT systems, which itself is based on *syngo*¹, the common SW platform for Siemens medical devices. *syngo* is shared with other Siemens modalities in order to provide a common look and feel and common interoperability features. In this document parts of the common SW platform are referenced by the terms "syngo", "MedCom", and "CSA".

As syngo MI.PET/CT 2008A is a *syngo* based product, this DICOM Conformance Statement is based on the corresponding *syngo* template [2] and on the corresponding CT DICOM Conformance Statement [3].

The described DICOM network implementation acts as SCU and SCP for the DICOM Verification, Storage, Storage Commitment Push Model, and Query/Retrieve Services. It acts as SCU for the DICOM Print Management Service, the Modality Worklist Service, and the Performed Procedure Step Service. These services are described in "Part I".

The described DICOM Media Storage Service implementation acts as FSC, FSU, and FSR for the specified application profiles and the related SOP Class instances. These services are described in "Part II".

1.2 Audience

This document is intended for hospital staff, health system integrators, hospital IT-managers, and software designers. It is assumed that the reader has a working understanding of DICOM.

1.3 Scope

This DICOM Conformance Statement refers to Siemens Biograph products using software PETsyngo. The following table relates software names to Siemens products.

Table 1: Siemens Biograph Products

Software Name	Product Name
syngo MI.PET/CT 2008A	Biograph 6
syngo MI.PET/CT 2008A	Biograph 40
syngo MI.PET/CT 2008A	Biograph 64

1. 'syngo' and 'We speak syngo' are registered trademarks of Siemens AG

1.4 Definitions, Acronyms and Abbreviations

1.4.1 Definitions

DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite information objects

1.4.2 Acronyms and Abbreviations

ACR	American College of Radiology
AE	DICOM Application Entity
ASCII	American Standard Code for Information Interchange
FSC	File Set Creator
FSR	File Set Reader
FSU	File Set Updater
HIS	Hospital Information System
IOD	DICOM Information Object Definition
ISO	International Standard Organization
MPPS	Modality Performed Procedure Step
MWL	Modality Worklist
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
R	Required Key Attribute
RIS	Radiology Information System
RWA	Real-World Activity
PDU	DICOM Protocol Data Unit
SCU	DICOM Service Class User (DICOM client)
SCP	DICOM Service Class Provider (DICOM server)
SOP	DICOM Service-Object Pair
U	Unique Key Attribute
UID	Unique Identifier
VR	Value Representation

1.5 References

- [1] Digital Imaging and Communications in Medicine (DICOM) 3.0, NEMA PS 3.1-3.14
- [2] *syngo* VD20J DICOM Conformance Statement
- [3] Somaris/5 VB20A DICOM Conformance Statement

1.6 Connectivity and Interoperability

The implementation of the PETsyngo DICOM interface has been carefully tested to assure correspondence with this Conformance Statement. But the Conformance Statement and the DICOM standard do not guarantee interoperability of Siemens modalities and modalities of other vendors. The user must compare the relevant Conformance Statements and if a successful interconnection should be possible, the user is responsible to specify an appropriate test suite and to validate the interoperability, which is required. A network environment may need additional functions out of the scope of DICOM.

Part I - Network

2 Implementation Models

2.1 Verification


The Verification service class defines an application-level class of service which allows for the operator to verify the ability of an application on a remote node to respond to DICOM messages. The DICOM Service Tool application supports the Verification service to act as SCU.

The other direction - responding to Verification requests from remote applications - is handled by the Storage SCP application.

2.1.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation is a Windows NT application and acts as SCU for the Verification service.

Figure 1: Application Data Flow Diagram Verification SCU

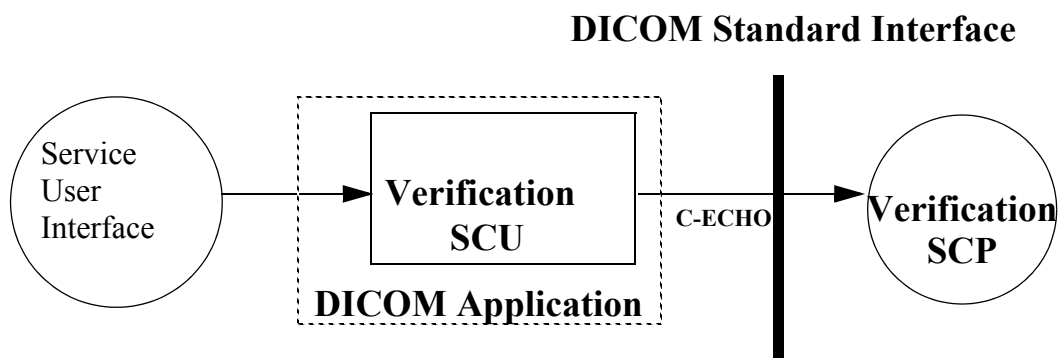

2.1.2 Functional Definitions of Application Entities

The DICOM Service Tool application opens an association to an application on the remote node and sends a Verification message to verify that the remote application can respond to DICOM messages.

2.1.3 Sequencing of Real-World Activities

Newly configured data of a remote AE have to be saved first, before a "verification" of these data is possible.

2.2 Storage

The PETsyngo DICOM Application Entity both originates associations for Storage of DICOM Composite Information Objects in Remote Application Entities and accepts association requests for Storage from Remote Application Entities.

2.2.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation acts as SCU and SCP for the C-STORE DICOM network service and as SCP for the C-ECHO DICOM network service. The product target operating system is Windows XP.

Figure 2: Application Data Flow Diagram C-STORE SCU


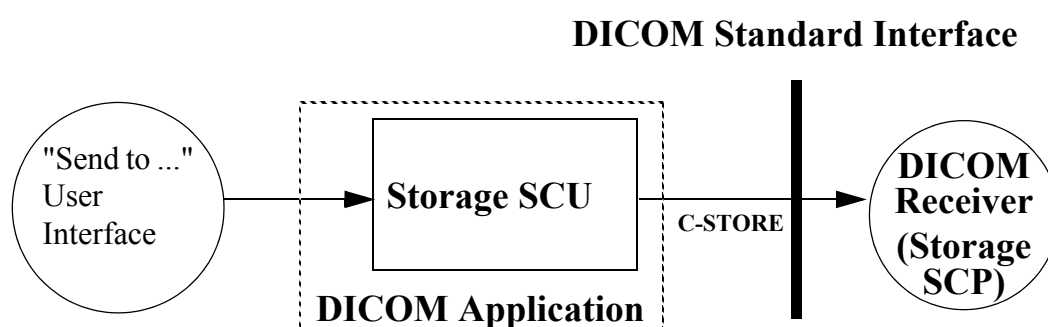


Figure 3: Application Data Flow Diagram C-STORE SCP

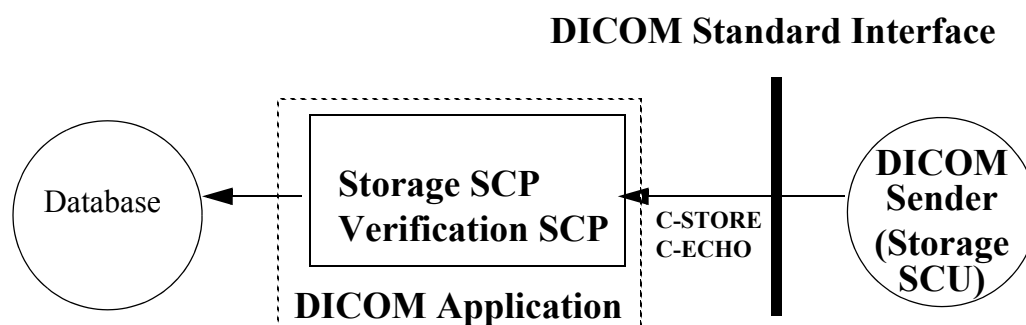

2.2.2 Functional Definitions of Application Entities

The Storage SCU is invoked by the job control interface that is responsible for processing network archiving tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

The Storage SCP component of the Siemens PETsyngo DICOM application is operating as background server process. It is existing, when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database. Verification requests will be processed and responded to by Storage SCP component, too.

2.2.3 Sequencing of Real-World Activities

not applicable.


2.3 Storage Commitment Push Model

The Storage Commitment service class defines an application-level class of service which facilitates the commitment to storage. It performs an additional task of commitment of composite objects apart from the network based storage of images as defined by the Storage Service class. The PETsyngo DICOM implementation supports the Storage Commitment Push Model as SCU.

2.3.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation acts as SCU for the Storage Commitment Push Model Service using the Storage Commitment Service Class. The product target operating system is Windows XP.

Figure 4: Application Data Flow Diagram Storage Commitment SCU

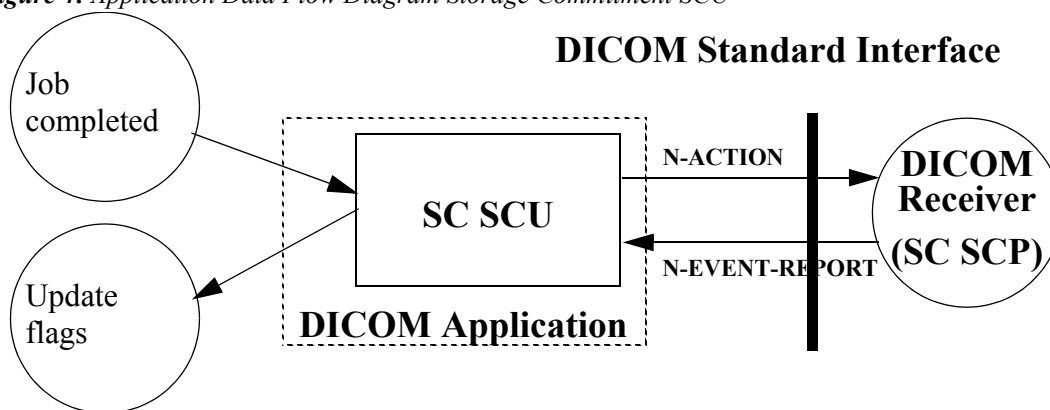

2.3.2 Functional Definitions of Application Entities

With each successfully completed send job the PETsyngo DICOM application will create a Storage Commitment Push Model Identifier from the SOP Instances sent. Then a Storage Commit Request is triggered. Depending on configuration, the PETsyngo DICOM application will keep the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the Status Flags of the related entity. It is possible to create triggers ("auto rules") from this event.

The Transaction UUIDs of the pending commitment request are kept "open" for a configurable amount in time (default: 1h). If the "open time" for a pending commitment request has elapsed without a related response from the provider, the Transaction UUID is removed and the related entities are indicated as "commit failed".

In any case, commitment will only be requested for previously and successfully sent images.

2.3.3 Sequencing of real World Activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send job.

2.4 Query/Retrieve

The query/retrieve service class defines an application-level class of services which facilitates the management of images and patient data against the well defined information model of DICOM and allows a DICOM AE to retrieve images from a remote DICOM node or to request a remote DICOM AE to initiate a transfer of images to another DICOM AE. The DICOM query/retrieve application supports the query/retrieve services to act as SCU and SCP.

2.4.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation acts as SCU and SCP for the query/retrieve network service. The product target operating system is Windows XP.

Figure 5: Application Data Flow Diagram QUERY/RETRIEVE SCU


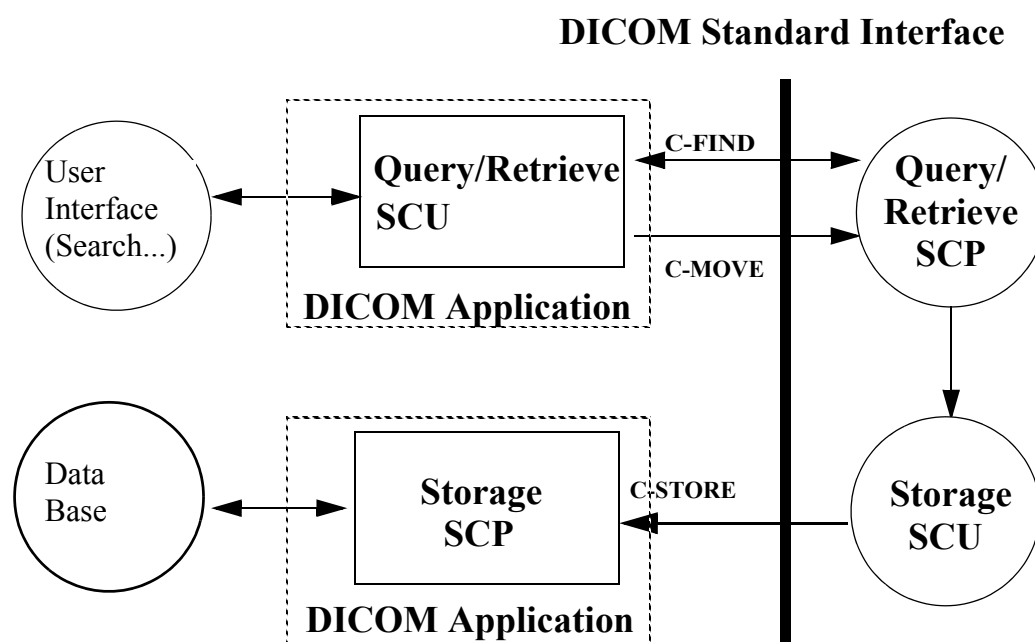


Figure 6: Application Data Flow Diagram QUERY/RETRIEVE SCP

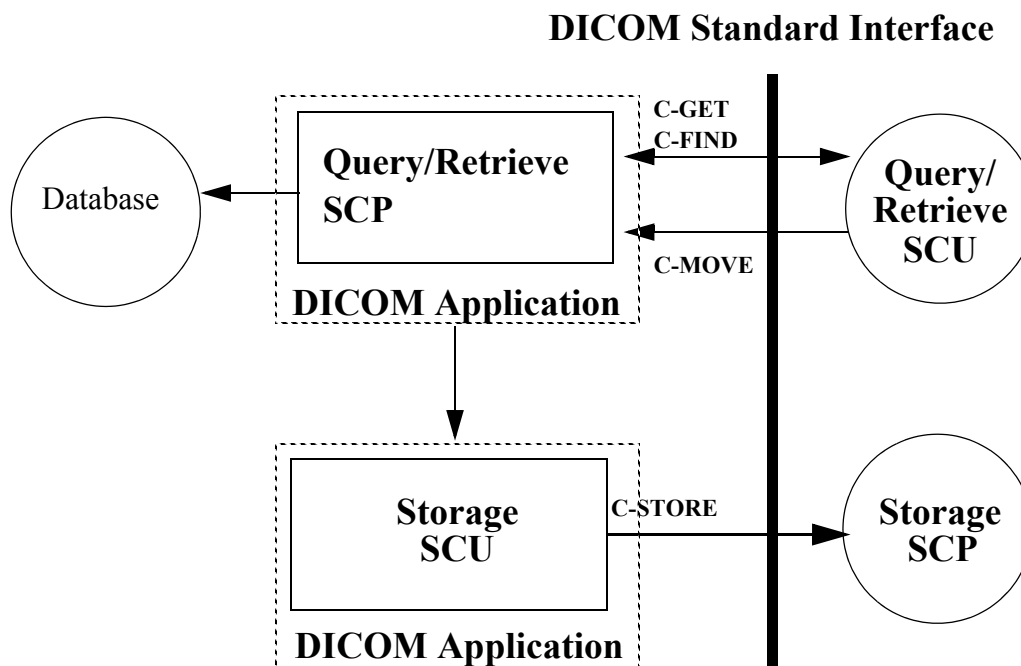

2.4.2 Functional Definitions of Application Entities

The query/retrieve SCU requests the remote query/retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in the user interface. Depending on user action (Import) the PETsyngo DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from the remote Storage SCU to the PETsyngo DICOM Storage SCP.

The query/retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote request, a C-GET or a C-MOVE involves the PETsyngo DICOM query/retrieve SCP application to initiate a C-STORE association (by triggering and parameterizing the own Storage SCU) to send image objects to a remote Storage SCP.

All components of the PETsyngo DICOM query/retrieve SCP application are operating as background server processes. They are existing when the machine is powered on and then respond to queries based on the records stored in its database.

Note

The PETsyngo DICOM query/retrieve SCU application will execute new queries based upon the data found in the higher level query. For details see 3.4.2.1.3.

2.4.3 Sequencing of Real-World Activities

Retrieve of images is only possible if results from a previous "Search..." operation exist and those entities can be selected for "Import".


2.5 Print

The Print Management Service Classes define an application-level class of services which facilitate the printing of images on a hardcopy medium. The print management SCU and print management SCP are peer DICOM print management application entities. The DICOM print application supports the print management DIMSE services to act as SCU.

2.5.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation acts as SCU for the print management network service. The product target operating system is Windows XP.

Figure 7: Application Data Flow Diagram PRINT SCU

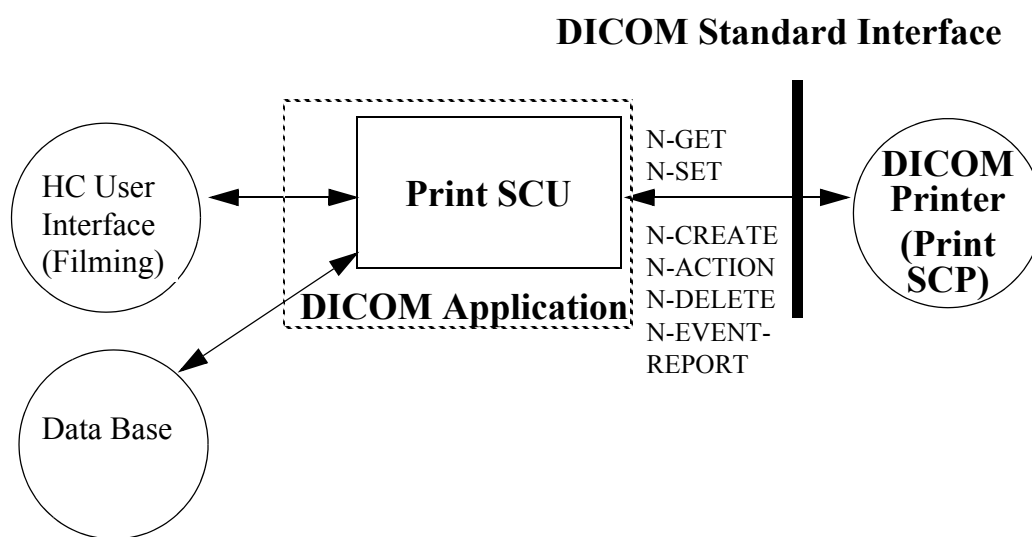

2.5.2 Functional Definitions of Application Entities

The Print SCU is invoked by the user interface to set up film sheet layout and whenever an image is ready to be printed on film. The print SCU will hold and maintain all data needed to compile a complete film sheet from the data (images, layout, configuration) received. Whenever a film sheet is ready to print, the related data is used to supply the information to the SOP Classes of the Print Management Service Class. A queue is maintained in order to intermediately store several film sheets in case of resource problems on the printer. The SCU will only supply and require the mandatory SOP Classes of the Print Management Service Class.

2.5.3 Sequencing of Real-World Activities

Not applicable.


2.6 Worklist

The Basic Worklist Service Class defines an application-level class of service which facilitates the transfer of worklists from the information system to the imaging modality. The worklist is queried by the AE and supplies the SCU with the scheduled tasks, which have to be performed on the modality. The DICOM worklist application supports the worklist service as SCU.

2.6.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation acts as SCU for the Basic Worklist Service using the Modality Worklist SOP Class. The product target operating system is Windows XP.

Figure 8: Application Data Flow Diagram BASIC WORKLIST SCU

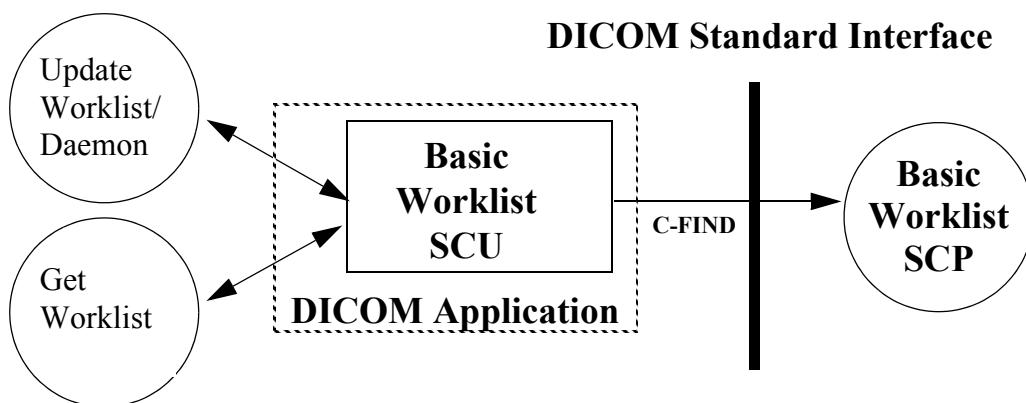

Note: It is configurable to get the worklist updates either automatically (in a configurable time interval) or manually (initiated by the user). There are two kinds of query the user can do: broad worklist query (all jobs for the own modality or own application entity) and patient based worklist query (where more search keys can be given, including Patient Name and Patient ID).

PETsyngo provides an enhanced query mode to retrieve worklists for multiple modalities. Up to three modalities can be configured and selected by the user. A separate C-FIND query is executed for each specified modality.

2.6.2 Functional Definitions of Application Entities

The worklist SCU ("broad query") is invoked from the patient browser user interface or by timer to request the worklist from a remote Information System (Modality Worklist SCP). This is done to perform a match to the internal worklist query keys specified in the C-FIND DIMSE service issued for the Modality Worklist Model.

The Worklist SCP responds to the C-FIND query and scheduled imaging service requests (scheduled procedure steps) and patient demographic information will be downloaded from the information system to the PETsyngo modality. All information retrieved will be held in the scheduling database for usage during patient registration procedure.

Furthermore the patient based query dialog from the patient browser allows to enter specific matching criteria ("narrow query") for the issue worklist query. With the response data the Patient Registration dialog can be populated according availability within the worklist response identifier.

2.6.3 Sequencing of Real-World Activities

The "narrow" (patient based) Worklist Query requires that sufficient matching keys or a unique matching key are/is entered before the query is issued. Only then a single response can be expected to complete the registration dialog.


2.7 Modality Performed Procedure Step

The Modality Performed Procedure Step service class defines an application-level class of service which facilitates the transfer of procedure and billing information from the imaging modality to the information system. The performed procedure step is created and set by the AE and supplies the SCP with the information about a real world procedure which is performed on the modality. The DICOM Modality Performed Procedure Step application supports the MPPS service as SCU.

2.7.1 Application Data Flow Diagram

The PETsyngo DICOM network implementation is a Windows XP application and acts as SCU for the performed procedure step network service.

Figure 9: Application Data Flow Diagram MODALITY PERFORMED PROCEDURE STEP SCU

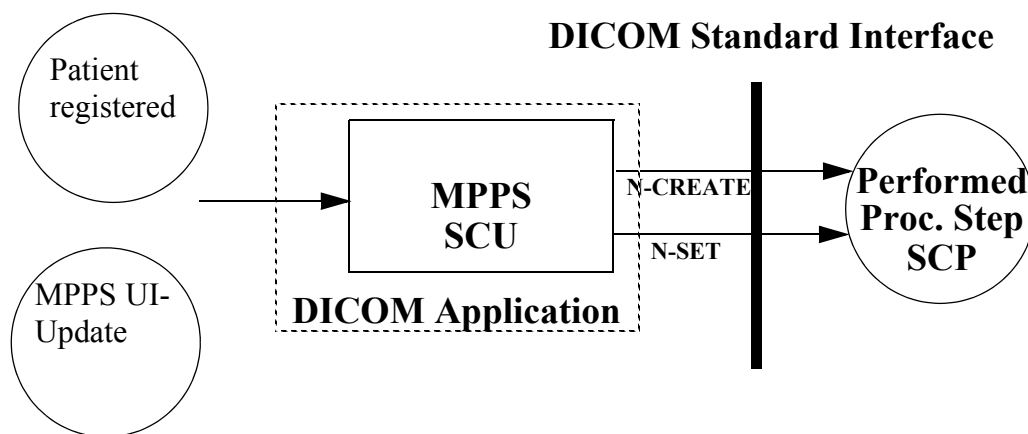

2.7.2 Functional Definitions of Application Entities

With registration of a patient (i.e. a Scheduled Procedure Step from Worklist), the PETsyngo DICOM application will create a MPPS instance and communicate it to the MPPS SCP.

Furthermore a manual update can be performed with the PETsyngo MPPS user interface. The state of the MPPS can only be set to "Completed" or "Discontinued" through the MPPS user interface. If done so, the DICOM application will no longer allow updates on the related MPPS Instance.

PETsyngo will not only allow a "1:1 relationship" of Scheduled Procedure Steps and Performed Procedure Steps, but also supports the "group case" (grouping several SPS of the same or different Requested Procedures) and "append case" from the respective IHE scenarios.

PETsyngo supports creation of "unscheduled cases" by allowing MPPS instances to be communicated for locally registered patients.

2.7.3 Sequencing of real World Activities

not applicable.

3 AE Specifications

3.1 Verification AE Specification

3.1.1 Association Establishment Policies

3.1.1.1 General

The PETsyngo DICOM Service Tool application attempts to open an association for verification request whenever the "verification" function is activated during network configuration of a remote DICOM application.

3.1.1.2 Number of Associations

The PETsyngo DICOM Service Tool application initiates one association at a time to request verification.

3.1.1.3 Asynchronous Nature

The PETsyngo DICOM Service Tool application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.1.1.4 Implementation Identifying Information

The PETsyngo DICOM Service Tool application provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- "SIEMENS_S5VB20B".

3.1.2 Association Initiation by Real-World Activity

The PETsyngo DICOM Service Tool application attempts to initiate a new association for

- DIMSE C-ECHO

service operations.

3.1.2.1 Real-World Activity - Verification SCU

3.1.2.1.1 Associated Real-World Activity - Verification SCU

The associated Real-World activity is a C-ECHO request initiated by the DICOM Service Tool application. If the process successfully establishes an association to a remote Application Entity, it will send the C-ECHO-Request via the open association to verify that the remote Application Entity is responding to DICOM messages.

3.1.2.1.2 Proposed Presentation Contexts - Verification SCU

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 2: Initiation presentation context Verification

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None

3.1.2.1.3 SOP Specific Conformance Statement - Verification SCU

The Application conforms to the definition of a Verification SCU in accordance to the DICOM Standard.

3.1.3 Association Acceptance Policy

The Verification SCP is part of the Storage SCP - see section 3.2.3 on page 35

3.2 Storage AE Specification

The PETsyngo Storage service class user applications and service class provider applications use one AE when initiating/receiving associations to/from remote DICOM nodes.

The PETsyngo DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Classes as both an SCU and SCP:

Table 3: Standard SOP Classes as an Storage SCU and an SCP

SOP Class Name	SOP Class UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1

Table 3: Standard SOP Classes as an Storage SCU and an SCP

SOP Class Name	SOP Class UID
Digital X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital MammoGraphy X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital MammoGraphy X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
UltraSound Multi-Frame Image Storage (retired) (SCP only)	1.2.840.10008.5.1.4.1.1.3
UltraSound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
UltraSound Image Storage (retired) (SCP only)	1.2.840.10008.5.1.4.1.1.6
UltraSound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray RadioFluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
PET Image Storage	1.2.840.10008.5.1.4.1.1.128

Table 3: Standard SOP Classes as an Storage SCU and an SCP

SOP Class Name	SOP Class UID
Radio Therapy Image Storage	1.2.840.10008.5.1.4.1.1.481.1
Radio Therapy Dose Storage	1.2.840.10008.5.1.4.1.1.481.2
Radio Therapy Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3
Radio Therapy Plan Storage	1.2.840.10008.5.1.4.1.1.481.5
Verification (only SCP)	1.2.840.10008.1.1

The PETsyngo DICOM implementation provides Private Conformance to the following DICOM V3.0 conform Private SOP Classes as both an SCU and SCP:

Table 4: Private SOP Classes as an Storage SCU and an SCP

SOP Class Name	SOP Class UID
CSA Non-Image Storage	1.3.12.2.1107.5.9.1

3.2.1 Association Establishment Policies

3.2.1.1 General

The existence of a job queue with network destination or an internal trigger from processing a retrieve request will activate the DICOM Storage Application. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the transfer is started.

The default PDU size will be 28 KB.

3.2.1.2 Number of Associations

The PETsyngo DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The PETsyngo DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of Simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in Configuration / DICOM / General.

3.2.1.3 Asynchronous Nature

The PETsyngo DICOM application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.2.1.4 Implementation Identifying Information

The PETsyngo DICOM implementation provides the Implementation Class UID of

- “1.3.12.2.1107.5.1.4”

and an Implementation Version Name of

- “SIEMENS_S5VB20B”.

3.2.2 Association Initiation by Real-World Activity

If a job with network destination becomes active in the job list or a retrieve sub-operation is processed the PETsyngo DICOM application attempts to initiate a new association for

- DIMSE C-STORE

service operations.

3.2.2.1 Real-World Activity - Send (Storage SCU)

3.2.2.1.1 Associated Real-World Activity - Send Image Objects to a Network Destination

The associated Real-World activities are:

- A user wants to send one or more composite objects to a remote node. A job with network destination triggers an internal process, which initiates a C-STORE request.
- A user on a remote node wants to retrieve one or more composite objects: The local C-MOVE SCP initiates C-STORE suboperations as a reaction to a C-MOVE-RQ coming from a remote node.

For both cases, if the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. If the C-STORE Response from the remote Application contains a status other than "Success" or "Warning", the association is aborted or released.

3.2.2.1.2 Proposed Presentation Contexts - Send Images (Storage SCU)

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 5: Initiation presentation context Storage

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		

Table 5: Initiation presentation context Storage

Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital Mammography X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital Mammography X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital Intra-oral X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Digital Intra-oral X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
UltraSound Multi-Frame Image	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None

Table 5: Initiation presentation context Storage

Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
UltraSound Image	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Waveform 12-lead ECG Object	1.2.840.10008.5.1.4.1.1.9.1.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform General ECG Object	1.2.840.10008.5.1.4.1.1.9.1.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Ambulatory ECG Object	1.2.840.10008.5.1.4.1.1.9.1.3	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Hemodynamic Object	1.2.840.10008.5.1.4.1.1.9.2.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Cardiac Electrophysiology Object	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Basic Audio Object	1.2.840.10008.5.1.4.1.1.9.4.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
X-Ray RadioFluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 5: Initiation presentation context Storage

PET Image	1.2.840.10008.5.1.4.1.1.128	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70	SCU	None
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
CSA Non-Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Note

Uncompressed transfer syntaxes are proposed together in a single presentation context for each abstract syntax.

PETsyngo does not support any of the compression Transfer Syntaxes for PT or NM.

The "MOVE" destinations must be configured as Storage destinations. This will include the configuration of Transfer Syntax capabilities.

Not all the listed transfer syntaxes will be proposed all the time. For some abstract syntaxes only a list of uncompressed (UC) transfer syntaxes (one or more) will be proposed, for other abstract syntaxes also JPEG Lossless (LL) syntax will be proposed and/or a list of JPEG Lossy (LY) transfer syntaxes. The contents of this lists is configurable, e.g. UC could be configured to contain only Implicit Little Endian for instance. For further configuration details see chapter 6.2.1

It is not possible to send an image that is locally stored in a Lossy compressed format using an uncompressed or lossless transfer syntax.

3.2.2.1.3 SOP Specific Conformance Statement - Storage SCU

The DICOM images created by PETsyngo DICOM application conform to the DICOM IOD definitions (Standard Extended IODs). But they will contain additional private elements which have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification

PETsyngo does not change private attributes if no modification is done. But during a *Save as* operation all non *syngo* defined private attributes will be removed. For association and DIMSE level time outs refer sec. 6.2

3.2.2.1.3.1 Image Pixel Attribute Description for Grayscale Images

The PETsyngo DICOM application supports the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. Possible values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = “MONOCHROME1”
- photometric interpretation (attribute 0028,0004) = “MONOCHROME2”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8, 16
- bits stored (attribute 0028,0101) = 8, 10, 12
- high bit (attribute 0028,0102) = 7, 9, 11

Overlay plane

- overlay type (attribute 60xx, 0040) = “G”
- overlay bits allocated (attribute 60xx, 0100) = 16
- overlay bit position (attribute 60xx, 0102) = 12, 13, 14, 15

Overlay plane

- overlay type (attribute 60xx, 0040) = “G”
- overlay bits allocated (attribute 60xx, 0100) = 1
- overlay bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported.

The PETsyngo DICOM application sends also the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integer and 16 bits allocated. Possible values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = “MONOCHROME1”
- photometric interpretation (attribute 0028,0004) = “MONOCHROME2”
- pixel representation (attribute 0028, 0103) = 1
- bits allocated (attribute 0028, 0100) = 16
- bits stored (attribute 0028,0101) = 16

- high bit (attribute 0028,0102) = 15

Overlay plane

- overlay type (attribute 60xx, 0040) = “G”
- overlay bits allocated (attribute 60xx, 0100) = 1
- overlay bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported.

3.2.2.1.3.2 Image Pixel Attribute Description for Color Images

The PETsyngo DICOM application supports the RGB color image description with the unsigned integer 24 bit color image plane pixel format:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = “RGB”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7
- planar configuration (attribute 0028,0006) = 0.

Note

The PETsyngo DICOM application extends the CT Image IOD to support RGB pixel format as described above. See section 5.1.

The PETsyngo DICOM application supports the “Palette Color” color image description with unsigned integer and 2’s complement pixel format:

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = “PALETTE COLOR”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8, 16
- bits stored (attribute 0028,0101) = 8, 16
- high bit (attribute 0028,0102) = 7, 15

Both 8bit and 16bit palettes are supported - but no Segmented Palette Color LUTs.

3.2.3 Association Acceptance Policy

The PETsyngo DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

service operations. Any Information Object transmitted on that association will be checked for conformance and stored in the database if check was successful.

3.2.3.1 Real-World Activity - Receive (Storage SCP)

3.2.3.1.1 Associated Real-World Activity - Receiving Images from a Remote Node (Storage SCP)

The daemon receiving process will accept an association and will receive any images transmitted on that association and will store the images on disk in the own database if the conformance check is performed successfully.

3.2.3.1.2 Proposed Presentation Contexts - Receiving Images (Storage SCP)

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 6: Acceptable presentation contexts Storage

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Digital X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Digital X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Digital Mammography X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None

Table 6: Acceptable presentation contexts Storage

Digital Mammography X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Digital Intra-oral X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Digital Intra-oral X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
UltraSound Multi-Frame Image	1.2.840.10008.5.1.4.1.1.3.1 1.2.840.10008.5.1.4.1.1.3 (retired) *1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
UltraSound Image	1.2.840.10008.5.1.4.1.1.6.1 1.2.840.10008.5.1.4.1.1.6 (retired) *1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None

Table 6: Acceptable presentation contexts Storage

Waveform 12-lead ECG Object	1.2.840.10008.5.1.4 .1.1.9.1.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform General ECG Object	1.2.840.10008.5.1.4 .1.1.9.1.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Ambulatory ECG Object	1.2.840.10008.5.1.4 .1.1.9.1.3	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Hemodynam- ic Object	1.2.840.10008.5.1.4 .1.1.9.2.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Cardiac Elec- trophysiolo- gy Object	1.2.840.10008.5.1.4 .1.1.9.3.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Waveform Basic Audio Object	1.2.840.10008.5.1.4 .1.1.9.4.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
X-Ray Angio- graphic Image	1.2.840.10008.5.1. 4.1.1.12.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
X-Ray Ra- dioFluoro- scopic Image	1.2.840.10008.5.1. 4.1.1.12.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
Nuclear Med- icine Image	1.2.840.10008.5.1. 4.1.1.20	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
PET Image	1.2.840.10008.5.1. 4.1.1.128	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
RT Image	1.2.840.10008.5.1. 4.1.1.481.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None
RT Dose	1.2.840.10008.5.1. 4.1.1.481.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian JPEG Lossy Baseline (Process 1) JPEG Lossy Extended (2 & 4) JPEG Lossless, Process 14 (selection value 1) RLE Lossless	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51 1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.2	SCU	None

Table 6: Acceptable presentation contexts Storage

RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
CSA Non-Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

***1:** US Retired and US Multiframe Retired images are converted to US images/US Multiframe images before storing them into the local database. The conversion creates new images, which implies new UIDs.

Note

With RLE Lossless Transfer Syntax the DICOM application will decompress the image before storing it into the database.

PETsyngo does not support any of the compression Transfer Syntaxes for PT or NM.

3.2.3.1.3 SOP Specific Conformance Statement - Storage SCP

The PETsyngo DICOM application conforms to the Full Storage Service Class at Level 2 - with the exception that private Sequences (private elements with VR=SQ) are not supported in Explicit VR Transfer syntax and will be ignored. When private Sequences are received in implicit VR then the whole sequence is stored as one binary element of VR=OW.

Upon successfully receiving a C-STORE-RQ, the PETsyngo DICOM receiver performs a quick plausibility test on the received image and available system resources. If this test succeeds, it returns the status SUCCESS, otherwise one of the following status codes is returned and the association is aborted:

- **Refused (A700):**
This error status indicates a lack of Resources (e.g. not enough disk space) on the PETsyngo modality.
- **Invalid Dataset (A900):**
The dataset is not containing one of the attributes "Study Instance UID", "Series UID" or "SOP Instance UID", or one of them has an invalid value.
- **Processing Error (0110 or C000):**
An error occurred while processing the image which makes it impossible to proceed.

Attention! Only after sending the response, the image will be saved into the database. If an error occurs during this operation, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

In order to confirm that the images sent were successfully stored into the database, the sending application should use Storage Commitment Service.

If an image with the same SOP Instance UID as the image being received is already present in the database then the received image will be ignored. The existing image is not superseded. So if a remote node sends twice the same image (same SOP Instance UID) then there will still be only one image (the first) in the database of the DICOM receiver.

The PETsyngo DICOM receiver can receive all kinds of different image formats. But RT images currently cannot be displayed. For Display of other images the following restrictions apply:

3.2.3.1.3.1 Image Pixel Attribute Acceptance Criterion for Grayscale Images

The Display application accepts the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. Accepted values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- pixel representation (attribute 0028, 0103) = 0 (unsigned)
- bits allocated (attribute 0028, 0100) = 8, 16
- bits stored (attribute 0028,0101) = 8, 10, 12
- high bit (attribute 0028,0102) = bits stored - 1
- only aspect ratio (attribute 0028,0034) 1:1 is supported

Overlay plane

- overlay type (attribute 60xx, 0040) = "G"
- overlay bits allocated (attribute 60xx, 0100) = 16
- overlay bit position (attribute 60xx, 0102) = 12, 13, 14, 15 (only bits above high bit permitted)
- Graphic Overlay will be shifted to fill Overlay Planes from Bit 12 and consecutive.

Overlay plane

- overlay type (attribute 60xx, 0040) = "G"
- overlay bits allocated (attribute 60xx, 0100) = 1
- overlay bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported.

The PETsyngo DICOM application accepts also the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integer and 16 bits allocated. Accepted values:

Pixel plane

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- pixel representation (attribute 0028, 0103) = 1 (signed)
- bits allocated (attribute 0028, 0100) = 16
- bits stored (attribute 0028,0101) = 16
- high bit (attribute 0028,0102) = 15
- only aspect ratio (attribute 0028,0034) 1:1 is supported

Overlay plane

- overlay type (attribute 60xx, 0040) = "G"
- overlay bits allocated (attribute 60xx, 0100) = 1
- overlay bit position (attribute 60xx, 0102) = 0
- overlay data (attribute 60xx, 3000) = supported.

For MOD LUT both the linear LUT (Rescale Slope/Intercept) and the MOD LUT SQ are supported and considered when pixel data is displayed. However there are two limitations. The MOD LUT SQ will be ignored in the following cases:

- 8 bit signed pixels
- The pixel format is changed by the MOD LUT (e.g. 8 bit -> 16 bit).

If the MOD LUT SQ contains multiple LUTs then only the first one is used.

For VOI LUT also both the linear LUT (Window Center/Width) and the VOI LUT SQ are supported (VOI LUT SQ with 8 or 16 bit LUT data).

But if both a VOI LUT SQ and a linear MOD LUT are specified within one image, then the value of Rescale Slope is restricted to 1.

If the VOI LUT SQ contains multiple LUTs, then only the first one is used by default. The other VOI LUTs are selectable.

In this version the Display application supports only rectangular and circular Shutters, one of each per image. Images with other shutter types will be displayed without Shutter.

3.2.3.1.3.2 Image Pixel Attribute Acceptance Criterion for Color Images

The Display application supports the RGB color image description with the unsigned integer 24 bit color image plane pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 3

- photometric interpretation (attribute 0028,0004) = “RGB”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7
- planar configuration (attribute 0028,0006) = 0 (pixel interleave) or 1 (plane interleave)
- only aspect ratio (attribute 0028,0034) 1:1 is allowed for Pixel Aspect Ratio, and Pixel Spacing must be the same for both directions.

The Display application supports the “Palette Color” color image description with unsigned integer and 2’s complement pixel format:

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = “PALETTE COLOR”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- bits allocated (attribute 0028, 0100) = 16 and bits stored (attribute 0028,0101) = 16
- high bit (attribute 0028,0102) = 7, 15

Both 8bit and 16bit palettes are supported - but no Segmented Palette Color LUTs.

The Display application supports the YBR_FULL color image description with the unsigned integer pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = “YBR_FULL”
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7

If PETsyngo software is making any persistent changes on a YBR image, the resulting new image will be saved with Photometric Interpretation “RGB”.

3.2.3.1.4 Presentation Context Acceptance Criterion - Storage SCP

The PETsyngo DICOM application will accept any number of Verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to the maximum of 127 (DICOM limit). In case the PETsyngo DICOM application runs out of resources, it will reject the association request.

3.2.3.1.5 Transfer Syntax Selection Policies - Storage SCP

The PETsyngo DICOM application supports

- the Implicit VR Little Endian, the Explicit VR Little Endian and Explicit VR Big Endian transfer syntaxes
- the JPEG Baseline and JPEG Extended transfer syntaxes (JPEG lossy)
- the JPEG lossless Non-Hierarchical transfer syntax
- the RLE Lossless Transfer Syntax

The PETsyngo DICOM application does not support compression transfer syntaxes for image types PT or NM.

Any proposed presentation context which includes one of these transfer syntaxes will be accepted. Any proposed presentation context that does not include one of these transfer syntaxes will be rejected.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

1. JPEG Lossy Extended Process 2 And 4
2. JPEG Lossless Non-hierarchical
3. JPEG Lossy Baseline
4. RLE Lossless
5. Explicit VR Little Endian
6. Explicit VR Big Endian
7. Implicit VR Little Endian

With RLE Lossless Transfer Syntax the PETsyngo DICOM application will decompress the image before storing it to the database.

With Implicit VR Little Endian Transfer Syntax the PETsyngo DICOM application will remove any private attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute dictionary of the PETsyngo DICOM application.

Therefore any Explicit VR Transfer Syntax shall preferably be used by the Storage SCUs when sending Composite Image Instances to the PETsyngo DICOM application.

3.3 Storage Commitment AE Specification

The PETsyngo DICOM application provides Standard Conformance to the following DICOM V3.0 SOP Classes as SCU.

Table 7: Standard SOP Classes as Storage Commitment Push Model

SOP Class Name	SOP Class UID
Storage Commitment Push Model	1.2.840.10008.1.20.1

3.3.1 Association Establishment Policies

3.3.1.1 General

With a Send Job successfully completed, the DICOM application will generate a Storage Commitment Identifier which references all instances of the processed job. The Commit Request is then sent over a single opened association. PETsyngo will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and time stamp, is kept. Depending on configuration, the association is closed when the configured time out has elapsed or a response was received before. If the association is closed before a response was received, the response is then expected on a different association. Multiple Storage Commitment Requests can be pending.

The default PDU size will be 28 KB.

3.3.1.2 Number of Associations

The PETsyngo DICOM application initiates several association at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The PETsyngo DICOM application is able to accept multiple association at a time. It can handle up to 10 associations in parallel.

3.3.1.3 Asynchronous Nature

The PETsyngo DICOM application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.3.1.4 Implementation Identifying Information

The PETsyngo Storage DICOM application provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- "SIEMENS_S5VB20B".

3.3.2 Association Initiation Policy

The PETsyngo Storage Commitment AE initiates an association in one case: when acting as SCU, in order to send a request for storage commitment. It will then issue a

- N-ACTION DIMSE to request commitment or a
- N-EVENT-REPORT DIMSE to respond to a received storage commitment request and the association was closed by the remote system prior to response.

3.3.2.1 Real-World Activity - Send Storage Commitment Request

3.3.2.1.1 Associated Real-World Activity - Job Completed

The PETsyngo Storage Commitment application sends the commit request (N-ACTION_RQ) message and waits for acceptance of this request (N_ACTION-RSP). After receiving this, the transaction is marked as "waiting".

Depending on a configuration value, the association will then be closed or kept open. In the first case there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N_EVENT-REPORT). In the second case, this time is the (also configurable) time out for the association. For both cases, if the commit response (N-EVENT-REPORT) does not arrive during the configured time, the transaction will be marked as failed. PETsyngo does not re-send objects because of a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as failed, else the transaction is marked as "completed"; in both cases, a message is shown to the user.

3.3.2.1.2 Proposed Presentation Contexts - Job Completed

The PETsyngo Storage Commitment AE will propose Presentation Contexts as shown in the following table:

Table 8: Initiation presentation context Storage Commitment Request

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

3.3.2.1.3 SOP Specific Conformance Statement - Job Completed

Storage Commitment is supported for all the SOP class UIDs as mentioned in 'Acceptable presentation contexts Storage' (pg. 36).

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes will not be supported in the N-ACTION primitive invoked by the Storage Commitment SCU.

3.3.3 Association Acceptance Policy

The PETsyngo Storage Commitment AE accepts an association in this case: when acting as SCU if configured to receive N-EVENT-REPORT on a separate association.

3.3.3.1 Real World Activity - Receive Storage Commitment Response

3.3.3.1.1 Associated Real World Activity - Receive Storage Commitment Response

The PETsyngo Storage Commitment AE has sent a Storage Commitment Request and, being configured to receive response on a separate association, has closed the association, and now it gets an association request from the Storage Commitment SCP that wants to send the results. The application will wait for Storage Commitment Notification triggers. Any incoming notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid, the Notification Identifier is evaluated and the related Instances marked with the related status. The overall Commit Status of the higher Information Entities is derived from propagation of all Image entities included.

The status flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of (English UI assumed):

- "AC" or "SC" - Successful Commitment. A means archived to configured archive destination, whereas S means sent to any other destination.
- "Af" or "Sf" - Commitment failed
- "A?" or "S?" - Commitment request is sent, response is pending

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

3.3.3.1.2 Accepted Presentation Contexts - Receive Storage Commitment Response

The PETsyngo Storage Commitment AE will accept Presentation Contexts as shown in the following table:

Table 9: Presentation context accepted for Storage Commitment

Presentation Context Table			
Abstract Syntax	Transfer Syntax	Role	Extended

Name	UID	Name List	UID List		Negotia- tion
Storage Com- mitment Push Model	1.2.840.10008.1.20 .1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

3.3.3.1.3 SOP Specific Conformance Statement - Receive Storage Commitment Response

If the Commitment Response (N_EVENT_REPORT) received has the status of "complete - failure exists", the transaction is marked as failed, else the transaction is marked as "completed"; In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

The PETsyngo DICOM application will NOT support the Storage Media File Set ID attributes.

3.4 Query/Retrieve AE Specification

The Query/Retrieve SCU requests that the remote SCP performs a match of all keys specified in the request against the information in its database and the identified images will be moved or retrieved to the same or a different storage destination.

The Query/Retrieve SCP responds to queries based on the records of its database and images will be sent to the requesting SCU or to a different storage destination.

The PETsyngo DICOM application provides Standard Conformance to the following DICOM V3.0 SOP Classes as SCU and SCP:

Table 10: SOP Classes as an Query/Retrieve SCU

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2

PETsyngo DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

Table 11: SOP Classes as an Query/Retrieve SCP

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Patient Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.1.3
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1

Table 11: *SOP Classes as an Query/Retrieve SCP*

SOP Class Name	SOP Class UID
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Study Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.2.3
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2
Patient/Study Only Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.3.3

Note

See also the Storage DICOM Conformance Statement (section 3.2.3 on page 35) to compare for conformance of the C-STORE sub-operation generated by the C-MOVE and C-GET DIMSE services. Furthermore compare the supported Storage Service SOP classes described in the Storage DICOM Conformance Statement of the Modality to which the images shall be transferred to.

3.4.1 Association Establishment Policies

3.4.1.1 General

With the "Search..." function the query data are entered and the DICOM Query/Retrieve application is started. A query request will be sent out to one remote node that can be selected from a list of configured Query Providers and the response data will be displayed for the user. In order to provide detailed information early additional queries are sent for the more detailed levels not yet covered by the first results. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used will be 28 KB.

3.4.1.2 Number of Associations

The PETsyngo DICOM Query/Retrieve application initiates several association at a time, one for each query/retrieve request being processed.

The PETsyngo DICOM Query/Retrieve application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

3.4.1.3 Asynchronous Nature

The PETsyngo DICOM Query/Retrieve application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.4.1.4 Implementation Identifying Information

The PETsyngo DICOM Query/Retrieve AE provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- "SIEMENS_S5VB20B".

3.4.2 Association Initiation Policy

The Query/Retrieve user interface will request the query data from the user and triggers C-FIND requests to the selected remote node. The response data will be displayed in the query UI for further data navigation.

When requesting Import of related items the browser requests the retrieve application to send a C_MOVE request to the related remote node. Images will then be received by the Storage SCP as described in the related section.

The following DIMSE-C operations are supported as SCU:

- C-FIND
- C-MOVE

3.4.2.1 Real-World Activity - Find SCU

3.4.2.1.1 Associated Real-World Activity - Find SCU "Search"

The associated Real-World activity is to fill out a query form with search data and pass it as queries to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data entries that will be passed to a browser application. When data transfer is finished the association is closed.

3.4.2.1.2 Proposed Presentation Contexts - Find SCU

The PETsyngo DICOM Query application will propose Presentation Contexts as shown in the following table

Table 12: Proposed Presentation Contexts - Find SCU:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		

Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Patient Study only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

It is configurable which of the three query models are to be used by the PETsyngo Query SCU application. If Patient and Study Root Abstract Syntaxes are configured, the C_FIND SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the STUDY Root Model.

It is highly recommended to configure only the Study Root Model if the corresponding Query SCP supports this Model. If the Query SCP does not support queries on Series Level, Patient Study Only Model should be used.

Note

C-FIND Extended Negotiation is NOT supported by the SCU.

3.4.2.1.3 SOP Specific Conformance Statement - Find SCU

The PETsyngo DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. On each level, the unique attributes of all previous levels are also sent (values are provided by the user by selection from a list). For instance for a query using the patient root model on Series level, the Patient ID of the current selected patient and the Study Instance UID of the current selected study are included in the message. The interactive querying of attributes on IMAGE level is not supported by the Query SCU, hence retrieval of individual Objects is possible.

The Query dialog in PETsyngo offers search keys on different levels (Patient, Study, Series). Depending on the used Query Model (Patient Root, Study Root, Patient Study Only) the PETsyngo DICOM Query/Retrieve SCU will execute multiple queries sequentially.

E.g. Patient Root Model:

The first query is performed on patient level with the entered patient level query keys. For each query result a new query is performed on study level with the entered study level query keys. At last for each result on study level a query is performed on series level with the entered series level keys.

The *Table 13: Query attributes* describes the search keys for the three query models (Patient Root, Study Root, Patient Study Only) that the PETsyngo Query/Retrieve application supports as an SCU. Matchings are either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is returned no matter what value it has.

Table 13: Query attributes

Attribute name	Tag	Type	Matching	user input	return value displayed
Patient level^a					
Patient name	(0010,0010)	R	wildcard ^d	enter value	yes
Patient ID	(0010,0020)	U	wildcard ^d	enter value	yes
Patient's birth date	(0010,0030)	O	universal (NULL)	enter value	yes
Patient's sex	(0010,0040)	O	universal (NULL)	enter value	yes
Number of Patient related studies	(0020,1200)	O	universal (NULL)	-	yes ^b
Number of Patient relates series	(0020,1202)	O	universal (NULL)	-	no
Number of Patient related instances	(0020,1204)	O	universal (NULL)	-	no
Study level					
Patient name ^c	(0010,0010)	R	wildcard ^d	enter value	yes
Patient ID	(0010,0020)	R	wildcard ^d	enter value	yes
Patient's birth date ^c	(0010,0030)	O	universal (NULL)	enter value	yes
Patient's sex ^c	(0010,0040)	O	universal (NULL)	enter value	yes

Table 13: Query attributes

Attribute name	Tag	Type	Matching	user input	return value displayed
Study Instance UID	(0020,000D)	U	single value	-	yes
Study ID	(0020,0010)	R	universal (NULL)	enter value ^d	yes
Study date	(0008,0020)	R	universal (NULL)	enter value ^e	yes
Study time	(0008,0030)	R	universal (NULL)	-	yes
Accession number	(0008,0050)	R	universal (NULL)	enter value ^d	yes
Study description	(0008,1030)	O	universal (NULL)	enter value ^d	yes
Referring physician's name	(0008,0090)	O	universal (NULL)	enter value ^d	yes
Name of physician reading study	(0008,1060)	O	universal (NULL)	enter value ^d	yes
Modalities in Study	(0008,0061)	O	universal (NULL)	selection ^g	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	no
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	no
Number of study related series	(0020,1206)	O	universal (NULL)	-	yes ^f
Number of study related instances	(0020,1208)	O	universal (NULL)	-	no
Series level					
Series instance UID	(0020,000E)	U	single value	-	yes
Series number	(0020,0011)	R	universal (NULL)	-	yes
Modality	(0008,0060)	R	universal (NULL)	selection ^g	yes

Table 13: Query attributes

Attribute name	Tag	Type	Matching	user input	return value displayed
Series date	(0008,0021)	O	universal (NULL)	-	yes
Series time	(0008,0031)	O	universal (NULL)	-	yes
Study ID	(0020,0010)	O	universal (NULL)	-	yes
Series description	(0008,103E)	O	universal (NULL)	enter value ^d	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	yes
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	yes
Body Part Examined	(0018,0015)	O	universal (NULL)	enter value ^d	yes
Protocol name	(0018,1030)	O	universal (NULL)	-	no
Performing Physician	(0018,1050)	O	universal (NULL)	enter value ^d	yes
Performed procedure step start date	(0040,0244)	O	universal (NULL)	-	yes
Performed procedure step start time	(0040,0245)	O	universal (NULL)	-	yes
Request Attribute Sequence	(0040,0275)	O	universal (NULL)	-	yes
>Requested Procedure ID	(0040,1001)	O	universal (NULL)	-	yes
>Scheduled Procedure ID	(0040,0009)	O	universal (NULL)	-	yes
Number of series related instances	(0020,1209)	O	universal (NULL)	-	yes
Image Level					
SOP Instance UID	(0008,0018)	U	single value	-	no

Table 13: Query attributes

Attribute name	Tag	Type	Matching	user input	return value displayed
Instance Number	(0020,0013)	R	universal (NULL)	-	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	no
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	no
Content date	(0008,0023)	O	universal (NULL)	-	no
Content time	(0008,0033)	O	universal (NULL)	-	no
Number of Frames	(0028,0008)	O	universal (NULL)	-	yes
Image comments	(0020,4000)	O	universal (NULL)	-	no

a. Only for Patient Root or Patient Study Only information model

b. Implicitly visualized in the UI if no study and series search attributes have been entered

c. Only for Study Root information model

d. Always a "*" is added to the string supplied by the user

e. Date range possible

f. Implicitly visualized in the UI if no series search attributes have been entered

g. Selection in drop down list from CT, MR, NM, PET and other modalities

The Find SCU interprets following status codes:

Table 14: C-FIND response status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None

Table 14: C-FIND response status

Service Status	Meaning	Protocol Codes	Related Fields
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.4.2.2 Real-World Activity - Move SCU

3.4.2.2.1 Associated Real-World Activity - Move SCU "Import"

The operator selects a data entry in the Query UI and activates the "Import" function.

This will generate a retrieval request to the archival application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement of the SCP describes the C-STORE service which is generated by processing the C-MOVE service.)

The transferred image data are processed as described in the storage class SCP descriptions.

The possibility to request the remote C-MOVE provider to move data to an application entity other than the C-MOVE SCU (the PETsyngo DICOM application) is NOT used.

C-MOVE operation on Patient Level is not supported by the Query UI.

3.4.2.2.2 Proposed Presentation Contexts - Move SCU "Import"

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 15: Proposed Presentation Contexts - Move SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		

Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Patient Study Only Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

Note

C-MOVE Extended Negotiation will be NOT supported by the SCU.

C-MOVE on Patient level is not supported by the application.

3.4.2.2.3 SOP Specific Conformance Statement - Move SCU "Import"

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The Move SCU interprets following status codes:

Table 16: C-MOVE response status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform suboperations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Table 16: C-MOVE response status

Service Status	Meaning	Protocol Codes	Related Fields
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
Failed	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.4.3 Association Acceptance Policy

The Query/Retrieve SCU and SCP establish an association by using the DICOM association services. During association establishment the Query/Retrieve application entities negotiate the supported SOP classes to exchange the capabilities of the SCU and the SCP.

The following DIMSE-C operations are supported as SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

3.4.3.1 Real-World Activity - Find SCP

3.4.3.1.1 Associated Real-World Activity - Find SCP

The associated Real-World activity is to respond to query requests to an SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is NOT supported. With a C-FIND-CANCEL request the running query can be cancelled at any time.

The SCP does support multiple C-FIND-requests over the same association, but not multiple C-MOVE requests.

3.4.3.1.2 Accepted Presentation Contexts - Find SCP

The PETsyngo Query/Retrieve AE will accept Presentation Contexts as shown in the following table

Table 17: Accepted Presentation Contexts - Find SCP:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

Note

C-FIND Extended Negotiation will NOT be supported by the SCP.

The order of preference in accepting a Transfer syntax is:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.1.3 SOP Specific Conformance Statement - Find SCP

The PETsyngo DICOM Query/Retrieve SCP supports hierarchical queries with all mandatory and optional search keys. The query attributes will be treated Case Sensitive.

With wildcard queries the symbol "?" is treated as "*" by the C-FIND-SCP application. As a consequence the query string of "?abc*" will be processed as "*abc*".

If the value for the patient level unique key "Patient ID" is not known, it may be returned with zero length. The attribute "Image Comments" will not be included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File Set ID, Retrieve AE Title with C-FIND-RSP message:

- The Storage Media File Set ID - if existent - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related instance.
- The Retrieve AE Title - if existent - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are NOT supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation has completed.

The supported attributes on the various levels of the three information models are listed in following tables

3.4.3.1.3.1 Patient Root Information Model**Table 18:** Patient level attributes, Patient Root Information Model

Attribute name	Tag	Type	Matching
Patient name	(0010,0010)	R	single value, wildcard, universal
Patient id	(0010,0020)	U	single value, wildcard, universal
Patient's birth date	(0010,0030)	O	single value, range, universal
Patient's birth time	(0010,0032)	O	single value, range, universal
Patient's sex	(0010,0040)	O	single value, wildcard, universal
Ethnic group	(0010,2160)	O	single value, wildcard, universal
Patient comments	(0010,4000)	O	wildcard, universal
Number of Patient related studies	(0020,1200)	O	universal
Number of Patient relates series	(0020,1202)	O	universal
Number of Patient related instances	(0020,1204)	O	universal

Table 19: Study level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Study instance UID	(0020,000D)	U	single value, list of UIDs
Study id	(0020,0010)	R	single value, wildcard, universal
Study date	(0008,0020)	R	single value, range, universal
Study time	(0008,0030)	R	single value, range, universal
Accession number	(0008,0050)	R	single value, wildcard, universal

Table 19: Study level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Referring physician's name	(0008,0090)	O	single value, wildcard, universal
Study description	(0008,1030)	O	single value, wildcard, universal
Admitting diagnoses description	(0008,1080)	O	single value, wildcard, universal
Patient's age	(0010,1010)	O	single value, wildcard, universal
Patient's size	(0010,1020)	O	single value, universal
Patient's weight	(0010,1030)	O	single value, universal
Additional patient history	(0010,21B0)	O	wildcard, universal
Name of physician reading study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of study related series	(0020,1206)	O	universal
Number of study related instances	(0020,1208)	O	universal

Table 20: Series level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Series instance UID	(0020,000E)	U	single value, list of UID
Series number	(0020,0011)	R	single value, universal
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body part examined	(0018,0015)	O	single value, wildcard, universal

Table 20: Series level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Patient position	(0018,5100)	O	single value, wildcard, universal
Smallest pixel value in series	(0028,0108)	O	single value, universal
Largest pixel value in series	(0028,0109)	O	single value, universal
Protocol name	(0018,1030)	O	single value, wildcard, universal
Series date	(0008,0021)	O	single value, range, universal
Series time	(0008,0031)	O	single value, range, universal
Series description	(0008,103E)	O	single value, wildcard, universal
Operators name	(0008,1070)	O	single value, wildcard, universal
Performing physician's name	(0008,1050)	O	single value, wildcard, universal
Performed procedure step start date	(0040,0244)	O	universal
Performed procedure step start time	(0040,0245)	O	universal
Number of series related instances	(0020,1209)	O	universal

Table 21: Image level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
SOP instance UID	(0008,0018)	U	single value, list of UID
Instance number	(0020,0013)	R	single value, universal
Content date	(0008,0023)	O	single value, range, universal

Table 21: *Image level attributes, Patient Root Information Model*

Attribute name	Tag	Usage SCU	Matching
Content time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image comments	(0020,4000)	O	universal

3.4.3.1.3.2 Study Root Information Model*Table 22: Study level attributes, Study Root Information Model*

Attribute name	Tag	Usage SCU	Matching
Patient name	(0010,0010)	R	single value, wildcard, universal
Patient id	(0010,0020)	R	single value, wildcard, universal
Patient's birth date	(0010,0030)	O	single value, range, universal
Patient's birth time	(0010,0032)	O	single value, range, universal
Patient's sex	(0010,0040)	O	single value, wildcard, universal
Patient comments	(0010,4000)	O	wildcard, universal
Number of Patient related studies	(0020,1200)	O	universal
Number of Patient relates series	(0020,1202)	O	universal
Number of Patient related instances	(0020,1204)	O	universal
Study instance UID	(0020,000D)	U	single value, list of UIDs
Study id	(0020,0010)	R	single value, wildcard, universal
Study date	(0008,0020)	R	single value, range, universal
Study time	(0008,0030)	R	single value, range, universal
Accession number	(0008,0050)	R	single value, wildcard, universal
Referring physician's name	(0008,0090)	O	single value, wildcard, universal
Study description	(0008,1030)	O	single value, wildcard, universal
Admitting diagnoses description	(0008,1080)	O	single value, wildcard, universal

Table 22: Study level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Patient's age	(0010,1010)	O	single value, wildcard, universal
Patient's size	(0010,1020)	O	single value, universal
Patient's weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal
Additional patient history	(0010,21B0)	O	wildcard, universal
Name of physician reading study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of study related series	(0020,1206)	O	universal
Number of study related instances	(0020,1208)	O	universal

Table 23: Series level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Series instance UID	(0020,000E)	U	single value, list of UID
Series number	(0020,0011)	R	single value, universal
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body part examined	(0018,0015)	O	single value, wildcard, universal
Patient position	(0018,5100)	O	single value, wildcard, universal
Smallest pixel value in series	(0028,0108)	O	single value, universal

Table 23: Series level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Largest pixel value in series	(0028,0109)	O	single value, universal
Protocol name	(0018,1030)	O	single value, wildcard, universal
Series date	(0008,0021)	O	single value, range, universal
Series time	(0008,0031)	O	single value, range, universal
Series description	(0008,103E)	O	single value, wildcard, universal
Operators name	(0008,1070)	O	single value, wildcard, universal
Performing physician's name	(0008,1050)	O	single value, wildcard, universal
Performed procedure step start date	(0040,0244)	O	universal
Performed procedure step start time	(0040,0245)	O	universal
Number of series related instances	(0020,1209)	O	universal

Table 24: Image level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
SOP instance UID	(0008,0018)	U	single value, list of UID
Instance number	(0020,0013)	R	single value, universal
Content date	(0008,0023)	O	single value, range, universal
Content time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image comments	(0020,4000)	O	universal

3.4.3.1.3.3 Patient Study Only Information Models

Table 25: Patient instance level, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Patient name	(0010,0010)	R	single value, wildcard, universal
Patient id	(0010,0020)	U	single value, wildcard, universal
Patient's birth date	(0010,0030)	O	single value, range, universal
Patient's birth time	(0010,0032)	O	single value, range, universal
Patient's sex	(0010,0040)	O	single value, wildcard, universal
Ethnic group	(0010,2160)	O	single value, wildcard, universal
Patient comments	(0010,4000)	O	wildcard, universal
Number of Patient related studies	(0020,1200)	O	universal
Number of Patient relates series	(0020,1202)	O	universal
Number of Patient related instances	(0020,1204)	O	universal

Table 26: Study level attributes, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Study instance UID	(0020,000D)	U	single value, list of UIDs
Study id	(0020,0010)	R	single value, wildcard, universal
Study date	(0008,0020)	R	single value, range, universal
Study time	(0008,0030)	R	single value, range, universal
Accession number	(0008,0050)	R	single value, wildcard, universal

Table 26: Study level attributes, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Referring physician's name	(0008,0090)	O	single value, wildcard, universal
Study description	(0008,1030)	O	single value, wildcard, universal
Admitting diagnoses description	(0008,1080)	O	single value, wildcard, universal
Patient's age	(0010,1010)	O	single value, wildcard, universal
Patient's size	(0010,1020)	O	single value, universal
Patient's weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal
Additional patient history	(0010,21B0)	O	wildcard, universal
Name of physician reading study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of study related series	(0020,1206)	O	universal
Number of study related instances	(0020,1208)	O	universal

Note

The C-FIND-RSP message will contain the following attributes:

- Specific Character Set (0008,0005) (If there is a specific character set in use)
- Query/Retrieve Level (0008,0052) from the C_FIND_RQ
- Retrieve AE Title (0008,0054) at study, series and image level.
This value is a list of AE titles from which the images can be retrieved. Will be NULL except for the lowest level of the query model (Image level for Patient Root or Study Root and Study level for Patient/Study Only)
- Storage-Media File-set ID (0088,0130) at level study, series and image. If Storage-Media File-set ID is not present a NULL value will be returned.
- attributes requested by C_FIND_RQ and supported by the SCP

Note

See also section 3.4.3.1.3 on page 60

The Find SCP returns following status codes:

Table 27: *C-FIND return status*

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.4.3.2 Real World Activity - Get SCP

3.4.3.2.1 Associated Real-World Activity - Get SCP

The associated Real-World activity is to respond to retrieve requests initiated from a foreign SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service which is generated by C-GET service. Relational retrieve operation is NOT supported.

Multiple C-GET requests over the same association are NOT supported.

3.4.3.2.2 Accepted Presentation Contexts - Get SCP

The PETsyngo DICOM application will accept Presentation Contexts as shown in the following table:

Table 28: Accepted Presentation Contexts -- Get SCP

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.1.3	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.2.3	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.3.3	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

Note

C-GET Extended Negotiation will be NOT supported by the SCP.

The order of preference in accepting a Transfer syntax is:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.2.3 SOP Specific Conformance Statement - Get SCP

At association establishment time the C-GET presentation context must be negotiated along with the C-STORE sub-operations which must be accomplished on the same association as the C-GET operation. Relational retrieve operation is NOT supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section will give information about "U" marked key attributes.

Note:

In DICOM wildcard queries the symbol '?' is treated as '*' by Find SCP.
 So a wildcard query with "?abc*" is actually treated as "*abc*"

The Get SCP returns following status codes:

Table 29: C-GET return status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform suboperations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures or Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.4.3.3 Real-World Activity - Move SCP

3.4.3.3.1 Associated Real-World Activity - Move SCP

The associated Real-World activity is to respond to retrieve requests to an SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service which is generated by the C-MOVE service. Relational retrieve operation is NOT supported.

Multiple C-MOVE requests over the same association are NOT supported.

3.4.3.3.2 Accepted Presentation Contexts - Move SCP

The PETsyngo DICOM application will accept Presentation Contexts as shown in the following table:

Table 30: Accepted Presentation Contexts - Move SCP

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCP	See Note
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

Note

C-MOVE Extended Negotiation will be NOT supported by the SCP.

The order of preference in accepting a Transfer syntax is:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.3 SOP Specific Conformance Statement - Move SCP

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations is done on a different association, specified in the C-MOVE request, to transfer images to another SCP of the Storage Service Class. Relational retrieve operation is NOT supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section will give information about "U" marked key attributes.

Note:

In DICOM wildcard queries the symbol '?' is treated as '*' by Find SCP.
 So a wildcard query with "?abc*" is actually treated as "*abc*"

The Move SCP returns following status codes:

Table 31: C-MOVE return status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform suboperations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Table 31: C-MOVE return status

Service Status	Meaning	Protocol Codes	Related Fields
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.5 Print AE Specification

The print management SCU invokes print management DIMSE services to transfer images from the local AE to the remote SCP AE to print the images with the defined film format and size on a selected network DICOM hardcopy printer. See DICOM part 4 annex H. This is done in a "full-page" print mode.

PETsyngo DICOM implementation provides Standard Conformance to the following DICOM V3.0 Basic Grayscale Print Management Meta SOP Class, Basic Color Print Management Meta SOP Class and the optional Print Job SOP Class as an SCU:

Table 32: Basic Gray Scale Print Management Meta SOP-Classes

SOP Class Name	SOP Class UID	Usage SCU/SCP
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	M/M
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	M/M
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	M/M
- Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	M/M
- Printer SOP Class	1.2.840.10008.5.1.1.16	M/M
- Print Job SOP Class	1.2.840.10008.5.1.1.14	U/U
- Presentation LUT SOP Class	1.2.840.10008.5.1.1.23	U/U

Table 33: Basic Color Print Management Meta SOP-Classes

SOP Class Name	SOP Class UID	Usage SCU/SCP
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	M/M
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	M/M
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	M/M
- Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	M/M
- Printer SOP Class	1.2.840.10008.5.1.1.16	M/M
- Print Job SOP Class	1.2.840.10008.5.1.1.14	U/U

3.5.1 Association Establishment Policies

3.5.1.1 General

Whenever a film is completely set up and printed by command or automatism, the job is prepared for processing. As soon as the queue is ready to process the job is activated and carried out according to the processing data. The related Print application will initiate an association to the print destination and process the printing of the related information.

The default PDU size will be 28 KB.

3.5.1.2 Number of Associations

The PETsyngo DICOM Print application initiates one association at a time for print device configured.

3.5.1.3 Asynchronous Nature

The PETsyngo DICOM implementation does not support asynchronous communication (multiple outstanding transactions over a single association).

3.5.1.4 Implementation Identifying Information

The PETsyngo DICOM implementation provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- "SIEMENS_S5VB20B".

3.5.2 Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. With the help of the N-GET request for the printer SOP Class the Status is determined before printing.

In case no problem is encountered with the N-CREATE/N-SET Services for the related Basic Print SOP Classes the film sheet is set up for printing and the image(s) is(are) transferred to the printer device.

After the last film is printed from the queue, the Print application will leave open the association for another 60 seconds. If a new film job is ready for printing within this time limit, the job will be processed immediately over the association still open. If there is no new job, the association is closed when the time out has elapsed. This is done to optimize automatic printing.

During the "idle time" (no open association to printer) the Print application will issue a cyclic camera status request (using N-GET of Printer SOP Class) every 5 minutes.

3.5.2.1 Real-World Activity

3.5.2.1.1 Associated Real-World Activity - Printing a Printer Job Queue Entry

Whenever a film sheet is prepared by the user, it is forwarded to the Printer Job queue. As soon as the associated Printer device is available the job is activated and an association is set up.

The film sheet is internally processed, converted to a Standard/1-1 page and then the page image is sent. Status is controlled by awaiting any N-EVENT message all through the transfer until the last image or film sheet is sent.

If the response from the remote application contains a status other than Success or Warning the association is aborted.

3.5.2.1.2 Proposed Presentation Contexts

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 34: Presentation context - Print SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Basic Gray-scale Print Management Meta SOP class	1.2.840.10008.5.1.1.9	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Basic Color Print Management Meta SOP class	1.2.840.10008.5.1.1.18	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Basic film session SOP class	1.2.840.10008.5.1.1.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Basic film box SOP class	1.2.840.10008.5.1.1.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Basic gray-scale image box SOP class	1.2.840.10008.5.1.1.4	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Basic color image box SOP class	1.2.840.10008.5.1.1.4.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		

Table 34: Presentation context - Print SCU

Printer SOP class	1.2.840.10008.5.1.1.16	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Print Job SOP class	1.2.840.10008.5.1.1.14	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		
Presentation LUT SOP class	1.2.840.10008.5.1.1.23	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax,	1.2.840.10008.1.2.2		

3.5.2.1.3 SOP Specific Conformance Statement - Meta SOP Classes

The PETsyngo DICOM Print Management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class and Basic Color Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM SCP, e.g.:

- maximum number of print jobs in the queue
- maximum number of print copies
- supported film sizes of the connected DICOM SCP
- supported film formats of the DICOM SCP
- lookup table definition.

The printing is only suspended in the case of a failure return status of the SCP.

3.5.2.1.3.1 SOP Specific Conformance to Basic Film Session SOP Class

The Basic Film Session information object definition describes all the user defined parameter which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes and that are printed on one hardcopy printer.

The PETsyngo DICOM Print application supports the following DIMSE Service Elements for the Basic Film Session SOP class as SCU:

- N-CREATE

- N-DELETE

The Basic Film Session SOP class N-CREATE-RQ (SCU) uses following attributes:

Table 35: Used Basic Film Session N-CREATE_RQ attributes

Attribute name	Tag	Usage SCU	Supported Values
Number of Copies	(2000,0010)	U	1
Medium Type	(2000,0030)	U	BLUE FILM CLEAR FILM PAPER
Film Destination	(2000,0040)	U	MAGAZINE PROCESSOR

The number of copies sent to the DICOM printer is always 1, the job is sent n times for n copies.

The affected SOP Instance UID received with N-CREATE-RSP message from SCP will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session SOP Class - see table below:

Table 36: Attributes of the N-DELETE-RQ on the Basic Film Session SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session

The N-DELETE-RQ on the Basic Film Session SOP Class is used to delete the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

Table 37: Basic Film Session SOP status

Service Status	Meaning	Protocol Codes
Failure	Film session SOP instances hierarchy does not contain film box SOP instances	C600
	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603

Table 37: Basic Film Session SOP status

Service Status	Meaning	Protocol Codes
Warning	Memory allocation not supported	B600
	Film session printing is not supported	B601
	Film box does not contain image box (empty page)	B602
Success	Film belonging to the film session are accepted for printing	0000

3.5.2.1.3.2 SOP Specific Conformance to Basic Film Box SOP Class

The Basic Film Box information object definition describes all the user defined parameter of one film of the film session. The Basic Film Box information description defines the presentation parameters which are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported as SCU are:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP class N-CREATE-RQ message uses following attributes (the used values for each attribute depend how the DICOM Printer is configured within the PETsyngo software):

Table 38: Used Film Box N-CREATE_RQ attributes

Attribute name	Tag	Usage SCU	Supported Values
Image Display Format	(2010,0010)	M	STANDARD\1-1
Referenced Film Session Sequence	(2010,0500)	M	
>Referenced SOP Class UID	(0008,1150)	M	1.2.840.10008.5.1.1.1
>Referenced SOP Instance UID	(0008,1155)	M	
Film Orientation	(2010,0040)	M	PORTRAIT LANDSCAPE

Table 38: *Used Film Box N-CREATE_RQ attributes*

Attribute name	Tag	Usage SCU	Supported Values
Film Size ID	(2010,0050)	M	8INX10IN 10INX14IN 11INX14IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM
Magnification Type	(2010,0060)	M	BILINEAR CUBIC NONE REPLICATE
Border Density	(2010,0100)	U	BLACK WHITE
Max Density	(2010,0130)	U	0 < Value
Min Density	(2010,0120)	U	0 < Value < 50
Illumination	(2010,015E)	U	Value > 0 Required if Presentation LUT is present
Reflective Ambient Light	(2010,0160)	U	Value > 0 Required if Presentation LUT is present
Referenced Presentation LUT Sequence	(2050,0500)	U	

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with its SOP Class / Instance UID pairs which will be kept internally to be further used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film sheet have been set, the PETsyngo DICOM print manager will issue a N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box (returned in N-CREATE-RSP of Basic Film Box SOP class) and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Box SOP Class - see table below:

Table 39: Attributes of the N_DELETE_RQ on the Basic Film Session SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box

The Basic Film Box SOP class interprets the following status codes :

Table 40: Basic Film Box SOP status

Service Status	Meaning	Protocol Codes
Failure	Unable to create print job; print queue is full	C602
	Image size is larger than image box size	C603
Warning	Film box does not contain image box (empty page)	B603
	Requested MinDensity or MaxDensity outside of printer's operating range	B605
Success	Film accepted for printing	0000

3.5.2.1.3.3 SOP Specific Conformance to Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data which apply to a single image of a sheet of film.

The Grayscale Image Box SOP class uses only the N-SET-RQ with the following attributes

Table 41: Used Basic Grayscale Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
Basic Grayscale Image Sequence	(2020,0110)	M	
>Samples Per Pixel	(0028,0002)	M	1

Table 41: Used Basic Grayscale Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
>Photometric Interpretation	(0028,0004)	M	MONOCHROME2 for Grayscale Images
>Rows	(0028,0010)	M	
>Columns	(0028,0011)	M	
>Pixel Aspect Ratio	(0028,0034)	M	
>Bits Allocated	(0028,0100)	M	8
>Bits Stored	(0028,0101)	M	8
>High Bit	(0028,0102)	M	7
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

The Grayscale Image Box SOP class interprets following status codes:

Table 42: Basic Grayscale Image Box SOP status

Service Status	Meaning	Protocol Codes
Warning	Requested MinDensity or MaxDensity outside of printer's operating range	B605
Failure	Image contains more pixel than printer can print in Image box	C603
	Insufficient memory in printer to store the image	C605
Success		0000

3.5.2.1.3.4 SOP Specific Conformance to Basic Color Image Box SOP Class

The Basic Color Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data which apply to a single image of a sheet of film.

The Color Image Box SOP class uses only the N-SET-RQ with the following attributes

Table 43: *Used Basic Color Image Box N-SET attributes*

Attribute name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
Basic Color Image Sequence	(2020,0111)	M	
>Samples Per Pixel	(0028,0002)	M	3
>Photometric Interpretation	(0028,0004)	M	RGB
>Planar Configuration	(0028,0006)	M	0
>Rows	(0028,0010)	M	
>Columns	(0028,0011)	M	
>Pixel Aspect Ratio	(0028,0034)	M	
>Bits Allocated	(0028,0100)	M	8
>Bits Stored	(0028,0101)	M	8
>High Bit	(0028,0102)	M	7
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

The Color Image Box SOP class interprets following status codes:

Table 44: *Basic Color Image Box SOP status*

Service Status	Meaning	Protocol Codes
Warning	Image size larger than image box size.	B604
Failure	Image contains more pixel than printer can print in Image box	C603
	Insufficient memory in printer to store the image	C605
Success		0000

3.5.2.1.3.5 SOP Specific Conformance to Presentation LUT SOP Class

The objective of the Presentation LUT is to realize image hardcopy printing tailored for specific modalities, applications, and user preferences.

The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

Table 45: Attributes of the N_CREATE_RQ on the Presentation LUT SOP Class

Attribute name	Tag	Usage SCU	Supported Values
Presentation LUT Shape	(2050,0020)	U	IDENTITY

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and is used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ) - see below.

Table 46: Attributes of the N_DELETE_RQ on the Presentation LUT SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Presentation LUT

The Presentation LUT SOP class interprets the following status codes:

Table 47: Presentation LUT SOP status

Service Status	Meaning	Protocol Codes
Warning	Requested Min Density or Max Density outside the HCD's operating range. HCD will use its respective minimum or maximum density value instead.	B605
Success	Presentation LUT successfully created	0000

3.5.2.1.3.6 SOP Specific Conformance to Printer SOP Class

The Printer SOP Class is the possibility to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The PETsyngo DICOM Print application uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way

It can directly ask the Printer (SCP) for its status or can receive Events from the Print SCP asynchronously:

- N_GET as SCU
- N_EVENT_REPORT as SCU

In both cases the following information is supported:

Table 48: *Used Printer N-EVENT report*

Event type name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

Table 49: *Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes*

Attribute name	Tag	Usage SCP	supported values
Printer Status	(2110,0010)	M	NORMAL FAILURE WARNING
Printer Status Info	(2110,0020)	M	See Sec. 3.5.2.1.3.8

For a detailed description of how PETsyngo reacts to the various messages please refer to the section: "DICOM Print SCU - detailed status displays".

3.5.2.1.3.7 SOP Specific Conformance to Print Job SOP Class

The Print Job SOP Class is the possibility to monitor the execution of the print process.

The PETsyngo DICOM Print application supports the optional N-EVENT-REPORT DIMSE service to receive the changes of the print job status in an asynchronous way.

It can receive events from the Print SCP asynchronously:

- N-EVENT-REPORT

Note

PETsyngo does not support receiving N-EVENT from the camera during print sessions, normally this is configurable in the camera.

The following information is supported:

Table 50: *Used Print Job N-EVENT report*

Event type name	Event	Attributes	Tag	Usage SCU
Normal	1	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Printing	2	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Done	3	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Failure	4	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U

For a detailed description of how PETsyngo reacts to the various messages please refer to the section: "DICOM Print SCU - detailed status displays".

3.5.2.1.3.8 DICOM Print SCU - detailed status displays

The following tables document the behavior of the PETsyngo system in response to messages received for the printer SOP class and the print job SOP class.

Definitions of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed.
- Interact: The user has to react in near future, but not immediately.
Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by N-EVENT-REPORT.
- Queue Stopped: The user has to react immediately. Either the camera needs immediate interaction or a job has been aborted.
Example: A camera is out of 8x10 clear sheets, or camera is down, or a film job is aborted.

Note

Different camera symbols are displayed according to the Printer Status Info.

The Printer Status (Success, Warning, Failure) is not evaluated, since the Printer Status Info is much more detailed and allows a more appropriate reaction of the system.

Table 51: Printer Status Infos within Printer SOP Class/Execution Status Infos within Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
NORMAL	Camera is ready.	Camera is ready.	<None>/idle
BAD RECEIVE MGZ	There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine.	Problem with receive magazine.	<None>/interact
BAD SUPPLY MGZ	There is a problem with a film supply magazine. Films from this magazine cannot be transported into the printer.	Problem with supply magazine.	<None>/interact
CALIBRATING	Printer is performing self calibration, it is expected to be available for normal operation shortly.	Self calibration. Please wait.	<None>/idle
CALIBRATION ERR	An error in the printer calibration has been detected, quality of processed films may not be optimal.	Problem in calibration. Film quality may not be optimal.	<None>/interact
CHECK CHEMISTRY	A problem with the processor chemicals has been detected, quality of processed films may not be optimal.	Problem with chemistry. Film quality may not be optimal.	<None>/interact
CHECK SORTER	There is an error in the film sorter	Error in film sorter.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
CHEMICALS EMPTY	There are no processing chemicals in the processor, films will not be printed and processed until the processor is back to normal.	Camera chemistry empty. Please check.	<None>/interact
CHEMICALS LOW	The chemical level in the processor is low, if not corrected, it will probably shut down soon.	Camera chemistry low. Please check.	<None>/interact
COVER OPEN	One or more printer or processor covers, drawers, doors are open.	Camera cover, drawer or door open.	<None>/interact
ELEC CONFIG ERR	Printer configured improperly for this job.	Camera configured improperly for this job. Queue stopped.	Queue for this camera will be STOPPED/Queue stopped
ELEC DOWN	Printer is not operating due to some unspecified electrical hardware problem.	Camera electrical hardware problem.	<None>/interact
ELEC SW ERROR	Printer not operating for some unspecified software error.	Camera software problem. Queue stopped.	Queue for this camera will be STOPPED/queue stopped
EMPTY 8x10	The 8x10 inch film supply magazine is empty.	8x10 film supply empty.	<None>/interact
EMPTY 8x10 BLUE	The 8x10 inch blue film supply magazine is empty.	8x10 blue film supply empty.	<None>/interact
EMPTY 8x10 CLR	The 8x10 inch clear film supply magazine is empty.	8x10 clear film supply empty.	<None>/interact
EMPTY 8x10 PAPR	The 8x10 inch paper supply magazine is empty.	8x10 paper supply empty.	<None>/interact
EMPTY 10x12	The 10x12 inch film supply magazine is empty.	10x12 film supply empty.	<None>/interact
EMPTY 10x12 BLUE	The 10x12 inch blue film supply magazine is empty.	10x12 blue film supply empty.	<None>/interact
EMPTY 10x12 CLR	The 10x12 inch clear film supply magazine is empty.	10x12 clear film supply empty.	<None>/interact
EMPTY 10x12 PAPR	The 10x12 inch paper supply magazine is empty.	10x12 paper supply empty.	<None>/interact
EMPTY 10x14	The 10x14 inch film supply magazine is empty.	10x14 film supply empty.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
EMPTY 10x14 BLUE	The 10x14 inch blue film supply magazine is empty.	10x14 blue film supply empty.	<None>/interact
EMPTY 10x14 CLR	The 10x14 inch clear film supply magazine is empty.	10x14 clear film supply empty.	<None>/interact
EMPTY 10x14 PAPR	The 10x14 inch paper supply magazine is empty.	10x14 paper supply empty.	<None>/interact
EMPTY 11x14	The 11x14 inch film supply magazine is empty.	11x14 film supply empty.	<None>/interact
EMPTY 11x14 BLUE	The 11x14 inch blue film supply magazine is empty.	11x14 blue film supply empty.	<None>/interact
EMPTY 11x14 CLR	The 11x14 inch clear film supply magazine is empty.	11x14 clear film supply empty.	<None>/interact
EMPTY 11x14 PAPR	The 11x14 inch paper supply magazine is empty.	11x14 paper supply empty.	<None>/interact
EMPTY 14x14	The 14x14 inch film supply magazine is empty.	14x14 film supply empty.	<None>/interact
EMPTY 14x14 BLUE	The 14x14 inch blue film supply magazine is empty.	14x14 blue film supply empty.	<None>/interact
EMPTY 14x14 CLR	The 14x14 inch clear film supply magazine is empty.	14x14 clear film supply empty.	<None>/interact
EMPTY 14x14 PAPR	The 14x14 inch paper supply magazine is empty.	14x14 paper supply empty.	<None>/interact
EMPTY 14x17	The 14x17 inch film supply magazine is empty.	14x17 film supply empty.	<None>/interact
EMPTY 14x17 BLUE	The 14x17 inch blue film supply magazine is empty.	14x17 blue film supply empty.	<None>/interact
EMPTY 14x17 CLR	The 14x17 inch clear film supply magazine is empty.	14x17 clear film supply empty.	<None>/interact
EMPTY 14x17 PAPR	The 14x17 inch paper supply magazine is empty.	14x17 paper supply empty.	<None>/interact
EMPTY 24x24	The 24x24 inch film supply magazine is empty.	24x24 film supply empty.	<None>/interact
EMPTY 24x24 BLUE	The 24x24 inch blue film supply magazine is empty.	24x24 blue film supply empty.	<None>/interact
EMPTY 24x24 CLR	The 24x24 inch clear film supply magazine is empty.	24x24 clear film supply empty.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
EMPTY 24x24 PAPR	The 24x24 inch paper supply magazine is empty.	24x24 paper supply empty.	<None>/interact
EMPTY 24x30	The 24x30 inch film supply magazine is empty.	24x30 film supply empty.	<None>/interact
EMPTY 24x30 BLUE	The 24x30 inch blue film supply magazine is empty.	24x30 blue film supply empty.	<None>/interact
EMPTY 24x30 CLR	The 24x30 inch clear film supply magazine is empty.	24x30 clear film supply empty.	<None>/interact
EMPTY 24x30 PAPR	The 24x30 inch paper supply magazine is empty.	24x30 paper supply empty.	<None>/interact
EMPTY A4 PAPR	The A4 paper supply magazine is empty.	A4 paper supply empty.	<None>/interact
EMPTY A4 TRANS	The A4 transparency supply magazine is empty.	A4 transparency supply empty.	<None>/interact
EXPOSURE FAILURE	The exposure device has failed due to some unspecified reason.	Exposure device has failed.	<None>/interact
FILM JAM	A film transport error has occurred and a film is jammed in the printer or processor.	Film jam.	<None>/interact
FILM TRANSP ERR	There is a malfunction with the film transport, there may or may not be a film jam.	Film transport problem.	<None>/interact
FINISHER EMPTY	The finisher is empty.	Finisher is empty.	<None>/interact
FINISHER ERROR	The finisher is not operating due to some unspecified reason.	Finisher problem.	<None>/interact
FINISHER LOW	The finisher is low on supplies	Finisher low.	<None>/interact
LOW 8x10	The 8x10 inch film supply magazine is low.	8x10 film supply low.	<None>/interact
LOW 8x10 BLUE	The 8x10 inch blue film supply magazine is low.	8x10 blue film supply low.	<None>/interact
LOW 8x10 CLR	The 8x10 inch clear film supply magazine is low.	8x10 clear film supply low.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
LOW 8x10 PAPR	The 8x10 inch paper supply magazine is low.	8x10 paper supply low.	<None>/interact
LOW 10x12	The 10x12 inch film supply magazine is low.	10x12 film supply low.	<None>/interact
LOW 10x12 BLUE	The 10x12 inch blue film supply magazine is low.	10x12 blue film supply low.	<None>/interact
LOW 10x12 CLR	The 10x12 inch clear film supply magazine is low.	10x12 clear film supply low.	<None>/interact
LOW 10x12 PAPR	The 10x12 inch paper supply magazine is low.	10x12 paper supply low.	<None>/interact
LOW 10x14	The 10x14 inch film supply magazine is low.	10x14 film supply low.	<None>/interact
LOW 10x14 BLUE	The 10x14 inch blue film supply magazine is low.	10x14 blue film supply low.	<None>/interact
LOW 10x14 CLR	The 10x14 inch clear film supply magazine is low.	10x14 clear film supply low.	<None>/interact
LOW 10x14 PAPR	The 10x14 inch paper supply magazine is low.	10x14 paper supply low.	<None>/interact
LOW 11x14	The 11x14 inch film supply magazine is low.	11x14 film supply low.	<None>/interact
LOW 11x14 BLUE	The 11x14 inch blue film supply magazine is low.	11x14 blue film supply low.	<None>/interact
LOW 11x14 CLR	The 11x14 inch clear film supply magazine is low.	11x14 clear film supply low.	<None>/interact
LOW 11x14 PAPR	The 11x14 inch paper supply magazine is low.	11x14 paper supply low.	<None>/interact
LOW 14x14	The 14x14 inch film supply magazine is low.	14x14 film supply low.	<None>/interact
LOW 14x14 BLUE	The 14x14 inch blue film supply magazine is low.	14x14 blue film supply low.	<None>/interact
LOW 14x14 CLR	The 14x14 inch clear film supply magazine is low.	14x14 clear film supply low.	<None>/interact
LOW 14x14 PAPR	The 14x14 inch paper supply magazine is low.	14x14 paper supply low.	<None>/interact
LOW 14x17	The 14x17 inch film supply magazine is low.	14x17 film supply low.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
LOW 14x17 BLUE	The 14x17 inch blue film supply magazine is low.	14x17 blue film supply low.	<None>/interact
LOW 14x17 CLR	The 14x17 inch clear film supply magazine is low.	14x17 clear film supply low.	<None>/interact
LOW 14x17 PAPR	The 14x17 inch paper supply magazine is low.	14x17 paper supply low.	<None>/interact
LOW 24x24	The 24x24 inch film supply magazine is low.	24x24 film supply low.	<None>/interact
LOW 24x24 BLUE	The 24x24 inch blue film supply magazine is low.	24x24 blue film supply low.	<None>/interact
LOW 24x24 CLR	The 24x24 inch clear film supply magazine is low.	24x24 clear film supply low.	<None>/interact
LOW 24x24 PAPR	The 24x24 inch paper supply magazine is low.	24x24 paper supply low.	<None>/interact
LOW 24x30	The 24x30 inch film supply magazine is low.	24x30 film supply low.	<None>/interact
LOW 24x30 BLUE	The 24x30 inch blue film supply magazine is low.	24x30 blue film supply low.	<None>/interact
LOW 24x30 CLR	The 24x30 inch clear film supply magazine is low.	24x30 clear film supply low.	<None>/interact
LOW 24x30 PAPR	The 24x30 inch paper supply magazine is low.	24x30 paper supply low.	<None>/interact
LOW A4 PAPR	The A4 paper supply magazine is low.	A4 paper supply low.	<None>/interact
LOW A4 TRANS	The A4 transparency supply magazine is low.	A4 transparency supply low.	<None>/interact
NO RECEIVE MGZ	The film receive magazine no available.	Film receiver not available.	<None>/interact
NO RIBBON	The ribbon cartridge needs to be replaced.	Replace ribbon cartridge.	<None>/interact
NO SUPPLY MGZ	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
CHECK PRINTER	The printer is not ready at this time, operator intervention is required to make the printer available.	Check camera.	<None>/interact

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
CHECK PROC	The processor is not ready at this time, operator intervention is required to make the printer available.	Check processor.	<None>/interact
PRINTER DOWN	The printer is not operating due to some unspecified reason.	Camera down.	<None>/interact
PRINTER INIT	The printer is not ready at this time, it is expected to become available without intervention, For example, it may be in a normal warm-up state.	Camera initializing.	<None>/idle
PRINTER OFFLINE	The printer has been disabled by an operator or service person.	Camera off-line.	<None>/interact
PROC DOWN	The processor is not operating due to some unspecified reason.	Processor down.	<None>/interact
PROC INIT	The processor is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Processor initializing.	<None>/idle
PROC OVERFLOW FL	Processor chemicals are approaching the overflow full mark.	Processor chemicals overflow.	<None>/interact
PROC OVERFLOW HI	Processor chemicals have reached the overflow full mark.	Processor chemicals near overflow.	<None>/interact
QUEUED	Print job in Queue	-	<None>/idle
RECEIVER FULL	The Film receive magazine is full.	Receiver full.	<None>/interact
REQ MED NOT INST	The requested film, paper, or other media supply magazine is installed in the printer, but may be available with operator intervention.	Install media supply.	<None>/interact
REQ MED NOT AVAI	The requested film, paper, or other media requested is not available on this printer.	Media supply not available on this camera. Queue stopped. Change camera.	Queue for this camera will be STOPPED/queue stopped

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
RIBBON ERROR	There is an unspecified problem with the print ribbon.	Error with print ribbon.	<None>/interact
SUPPLY EMPTY	The printer is out of film.	Camera out of film.	<None>/interact
SUPPLY LOW	The film supply is low.	Film supply low.	<None>/interact
UNKNOWN	There is an unspecified problem.	Unspecified problem with camera.	<None>/interact

Table 52: Printer Status Infos: Additional Agfa printer status infos

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
WARMING UP	Printer is in the warm-up stage. Spooling of print jobs to disk is still possible.	Camera is warming up.	<None>idle
OFFLINE	Printer is switched off-line. Spooling of print jobs to disk is still possible.	Camera is switched off-line.	<None>/interact
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	-	<None>/idle

Table 53: Printer Status Infos: Additional Kodak infos for Pacs Link (formerly Imation cameras)

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
SUPPLY MGZ ERR	The supply magazine has an error.	Film supply has an error.	<None>/interact

Table 54: Printer Status Infos: Additional Kodak infos for Kodak 190

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
PRINTER STOPPED	The printer has stopped	Camera has stopped.	<None>/interact
FATAL ERROR	Fatal error.	Fatal error. Queue stopped.	Queue for this camera will be STOPPED/queue stopped

Table 55: *Printer Status Infos: Additional Kodak infos for 2180/1120*

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
PRINTER NOT RDY	Printer not ready.	Camera not ready.	<None>/interact
CHECK PROCESSOR	Check processor.	Check processor.	<None>/interact
NO TONER	No toner.	No toner.	<None>/interact
FATAL	Fatal error.	Fatal error. Queue stopped.	Queue for this camera will be STOPPED/queue stopped

Table 56: *Printer Status Infos: Additional Codonics infos*

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
STANDARD	Printer is ready.	Camera is ready.	<None>/Normal
LOAD A-SIZE	Load A-size media.	Load A-size media.	<None>/interact
LOAD A-DVPAPER	Load A-size black and white paper.	Load A-size black and white paper.	<None>/interact
LOAD A-CVPAPER	Load A-size color paper.	Load A-size color paper.	<None>/interact
LOAD A-CVTRANS	Load A-size transparencies.	Load A-size transparencies.	<None>/interact
LOAD A4-SIZE	Load A4-size media.	Load A4-size media.	<None>/interact
LOAD A4-DVPAPER	Load A4-size black and white paper.	Load A4-size black and white paper.	<None>/interact
LOAD A4-CVPAPER	Load A4-size color paper.	Load A4-size color paper.	<None>/interact
LOAD A4-CVTRANS	Load A4-size transparencies.	Load A4-size transparencies.	<None>/interact
LOAD LA-SIZE	Load LA-size media.	Load LA-size media.	<None>/interact
LOAD LA-DVPAPER	Load LA-size black and white paper.	Load LA-size black and white paper.	<None>/interact
LOAD LA-CVPAPER	Load LA-size color paper.	Load LA-size color paper.	<None>/interact
LOAD LA-CVTRANS	Load LA-size transparencies.	Load LA-size transparencies.	<None>/interact
LOAD LA4-SIZE	Load LA4-size media.	Load LA4-size media.	<None>/interact

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
LOAD LA4-DVPAPER	Load LA4-size black and white paper.	Load LA4-size black and white paper.	<None>/interact
LOAD LA4-CVPAPER	Load LA4-size color paper.	Load LA4-size color paper.	<None>/interact
LOAD LA4-CVTRANS	Load LA4-size transparencies.	Load LA4-size transparencies.	<None>/interact
LOAD XLA-SIZE	Load XLA-size media.	Load XLA-size media.	<None>/interact
LOAD XLA-DVPAPER	Load XLA-size black and white paper.	Load XLA-size black and white paper.	<None>/interact
LOAD XLA-CVPAPER	Load XLA-size color paper.	Load XLA-size color paper.	<None>/interact
LOAD XLA-CVTRANS	Load XLA-size transparencies.	Load XLA-size transparencies.	<None>/interact
LOAD XLA4-SIZE	Load XLA4-size media.	Load XLA4-size media.	<None>/interact
LOAD XLA4-DVPAPE	Load XLA4-size black and white paper.	Load XLA4-size black and white paper.	<None>/interact
LOAD XLA4-CVPAPE	Load XLA4-size color paper.	Load XLA4-size color paper.	<None>/interact
LOAD XLA4-CVTRAN	Load XLA4-size transparencies.	Load XLA4-size transparencies.	<None>/interact
LOAD XLW-SIZE	Load XLW-size media.	Load XLW-size media.	<None>/interact
LOAD XLW-DVPAPER	Load XLW-size black and white paper.	Load XLW-size black and white paper.	<None>/interact
LOAD XLW-CVPAPER	Load XLW-size color paper.	Load XLW-size color paper.	<None>/interact
LOAD 8X10-SIZE	Load 8x10 media.	Load 8x10 media.	<None>/interact
LOAD 8X10-DVFILM	Load 8x10 black and white film.	Load 8x10 black and white film.	<None>/interact
SUPPLY MISSING	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
RIBBON MISSING	Ribbon is missing.	Ribbon is missing.	<None>/interact
RIBBON EMPTY	Ribbon is empty.	Ribbon is empty.	<None>/interact

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
TOP COVER OPEN	Top cover of printer is open.	Top cover of camera is open.	<None>/interact

Additional DICOM Execution Status Infos

Execution Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
INVALID PAGE DES	The specified page layout cannot be printed or other page description errors have been detected.	Film Job cannot be printed on this camera. Queue stopped. Please redirect film job.	Queue for this camera will be STOPPED/queue stopped
INSUFFIC MEMORY	There is not enough memory available to complete this job.	Not enough memory available in camera. Queue stopped. Please continue queue or change camera.	Queue for this camera will be STOPPED/queue stopped
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	-	<None>/idle

3.6 Modality Worklist AE Specification

The Modality Worklist SCU (patient registration in conjunction with the network application) requests that the remote SCP performs a match of all keys specified in the query against the information in its worklist database.

The PETsyngo DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

Table 57: SOP Classes as an SCU

SOP Class Name	SOP Class UID
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31

3.6.1 Association Establishment Policies

3.6.1.1 General

It is possible to configure a cyclic update of the modality scheduler database through a background worklist request with date/time and modality information.

In addition the user can request worklist update with "Update Worklist". No duplicate entries will be added in the Scheduler DB. Entries are uniquely identified by the Study Instance UID (0020,000D) for the Requested Procedure and the SPS ID (0040,0009) in the SPS Sequence (0040,0100).

An interactive worklist query can be issued with search criteria entered in the patient based Query dialog from the patient browser.

The default PDU size used will be 28 KB.

3.6.1.2 Number of Associations

The PETsyngo DICOM application initiates one association at a time to query worklist entry data.

3.6.1.3 Asynchronous Nature

The PETsyngo DICOM implementation does not support asynchronous communication (multiple outstanding transactions over a single association).

3.6.1.4 Implementation Identifying Information

The PETsyngo DICOM implementation provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- “SIEMENS_S5VB20B”.

3.6.2 Association Initiation Policy

The network application will (if configured) query the worklist periodically or by user request. Ever then it establishes an association by using the DICOM association services. During association establishment the negotiation of SOP classes to exchange the capabilities of the SCU and the SCP is not supported.

The following DIMSE-C operation is supported as SCU:

- C-FIND

3.6.2.1 Real-World Activity

3.6.2.1.1 Associated Real-World Activity - Query (Update) Worklist

A network application will perform worklist queries with the C-FIND request at regular intervals. In addition it can be triggered by immediate request. The received worklist items will be compared with the contents of the local scheduler database. New items will be inserted into scheduler database.

After each broad query all RP/SPS that were cancelled or rescheduled to another modality at the RIS will be automatically removed from the scheduler DB if

1. the Examination of this procedure has not been started or finished yet
2. the corresponding configuration item "Automatic removal of cancelled/rescheduled Request" was checked in the Service UI under DICOM / HIS/RIS Node

No automatic clean-up of the scheduler DB is performed after a Patient based Query since the worklist received does not give the complete list of all currently scheduled procedures for the modality.

3.6.2.1.2 Proposed Presentation Contexts - Query (Update) Worklist

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 58: *Proposed presentation contexts*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		

Modality	1.2.840.10008.5.1.4.31	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
Worklist Information		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
Model- FIND		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

3.6.2.1.3 SOP Specific Conformance Statement - Update Worklist

Search Key Attributes of the Worklist C-FIND

The PETsyngo DICOM worklist SCU supports "broad worklist queries" with all required search keys.

The following tables describe the search keys that the SCU supports for a broad worklist query, which is a query for all tasks scheduled for the own modality or own modality application entity defined with the following search keys:

Table 59: Search Key Attributes in a broad worklist query

Attribute name ^a	Tag	Matching Key Type	query value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	
>Scheduled Station AE Title	(0040,0001)	R	Configurable ^b : own AET or "*"
>Scheduled Procedure Step Start Date	(0040,0002)	R	Configurable: inserted in UI ^c or "today and yesterday"
>Scheduled Procedure Step Start Time	(0040,0003)	R	Configurable: inserted in UI ^d or 0:00-23:59
>Modality	(0008,0060)	R	Configurable ^b : own modality, "*" or multi- modality ^e

a. No other attributes of Register Dialog used for C-FIND

b. One and only one of the attributes "Modality" and "AE Title" is set to "*". There is a configuration parameter telling which of them. The other one is always set to the "own" value (i.e. own modality respectively own AE Title). Use Options/Configuration/PatientRegistration, "HIS/RIS" tabcard for configuration.

c. <startDate>-<endDate>

d. <startTime>-<endTime>

- e. For multi-modality worklist query one or more of the pre-configured modalities can be selected.
 If multiple modalities are selected, a C-FIND is executed for each modality.

Note

Since various SCP implementations depend on the Specific Character Set attribute to be sent with the C-FIND in order to deliver the attribute filled with the C-FIND-RSP (see below), as a default the attribute will be sent even if empty. In case this turns out to be a problem for a specific SCP in cooperation with Siemens this can be configured not to include this attribute.

Return Key Attributes used from the Worklist C-FIND-RSP

The PETsyngo DICOM worklist SCU supports worklist queries with return key attributes of all types. The following tables describe the return keys that the SCU supports.

An "x" in the UI column will indicate that the attribute is visualized when browsing the Worklist results with Patient Browser and/or during Patient Registration. The Patient Browser display is additionally influenced by the related Browser configuration.

A tag in the IOD column will indicate that the related attribute is included into the SOP Instances of the IODs created during processing of this worklist request.

A tag in the MPPS column will indicate that the related attribute is included into the SOP Instances of the MPPS objects created during processing of this worklist request. (See also the tables 'Performed Procedure Step N-CREATE Attributes' (pg. 116) and 'Performed Procedure Step N-SET Attributes' (pg. 120)).

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
SOP Common					
Specific Character Set ^a	(0008,0005)	1C	-	(0008,0005)	(0008,0005)
Scheduled Procedure Step					
Scheduled Procedure Step Sequence	(0040,0100)	1			
>Modality	(0008,0060)	1	x	(0008,0060)	(0008,0060)
>Requested Contrast Agent	(0032,1070)	2C	x	(0032,1070)	
>Scheduled Station AE Title	(0040,0001)	1	x		(0040,0241)
>Scheduled Procedure Step Start Date	(0040,0002)	1	x		
>Scheduled Procedure Step Start Time	(0040,0003)	1	x		
>Scheduled Procedure Step End Date	(0040,0004)	3	-		
>Scheduled Procedure Step End Time	(0040,0005)	3	-		

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
>Scheduled Performing Physician's Name	(0040,0006)	1	x	(0008,1050)	(0008,1050)
>Scheduled Procedure Step Description	(0040,0007)	1C	x	(0040,0007) (0040,0254)	(0040,0007) (0040,0254)
>Scheduled Protocol Code Sequence	(0040,0008)	1C	-	(0040,0008) (0040,0260)	(0040,0008) (0040,0260)
>>Code Value	(0008,0100)	1C	x		
>>Coding Scheme Designator	(0008,0102)	1C	x		
>>Coding Scheme Version	(0008,0103)	3	x		
>>Code Meaning	(0008,0104)	3	x		
>Scheduled Procedure Step ID	(0040,0009)	1	x	(0040,0009) (0040,0253)	(0040,0009) (0040,0253)
>Scheduled Station Name	(0040,0010)	2	x		
>Scheduled Procedure Step Location	(0040,0011)	2	x		(0040,0242)
>Pre-Medication	(0040,0012)	2C	x		
>Scheduled Procedure Step Status	(0040,0020)	3	x		
>Comments on the Scheduled Procedure Step	(0040,0400)	3	-		
Requested Procedure					
Referenced Study Sequence	(0008,1110)	2	-	(0008,1110)	(0008,1110)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Study Instance UID	(0020,000D)	1	-	(0020,000D)	(0020,000D)
Requested Procedure Description	(0032,1060)	1C	x	(0032,1060)	(0032,1060)
Requested Procedure Code Sequence	(0032,1064)	1C	-	(0032,1032) (0032,1064)	(0032,1032)
>Code Value	(0008,0100)	1C	x		
>Code Scheme Designator	(0008,0102)	1C	x		
>Code Scheme Version	(0008,0103)	3	x		
>Code Meaning	(0008,0104)	3	x		

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Requested Procedure ID	(0040,1001)	1	x	(0040,1001) (0020,0010)	(0040,1001) (0020,0010)
Reason for the Requested Procedure	(0040,1002)	3	-		
Requested Procedure Priority	(0040,1003)	2	x		
Patient Transport Arrangements	(0040,1004)	2	-		
Requested Procedure Location	(0040,1005)	3	-		
Confidentiality Code	(0040,1008)	3	-		
Reporting Priority	(0040,1009)	3	-		
Names of Intended Recipients of results	(0040,1010)	3	-	(0008,1048)	
Requested Procedure Comments	(0040,1400)	3	x		
Imaging Service Request					
Accession Number	(0008,0050)	2	x	(0008,0050)	(0008,0050)
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Requesting Physician	(0032,1032)	2	x	(0032,1032)	(0032,1032)
Requesting Service	(0032,1033)	3	x	(0032,1033)	
Reason for the Imaging Service Request	(0040,2001)	3	-		
Issuing Date of Imaging Service Request	(0040,2004)	3	-		
Issuing Time of Imaging Service Request	(0040,2005)	3	-		
Placer Order Number / Imaging Service Request	(0040,2016)	3	-		(0040,2016)
Filler Order Number / Imaging Service Request	(0040,2017)	3	-		(0040,2017)
Order entered by...	(0040,2008)	3	-		
Order Enterer's Location	(0040,2009)	3	-		
Order Callback Phone Number	(0040,2010)	3	-		
Imaging Service Request Comments	(0040,2400)	3	x		
Visit Identification					
Institution Name	(0008,0080)	3	x	(0008,0080)	

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Institution Address	(0008,0081)	3	-	(0008,0081)	
Institution Code Sequence	(0008,0082)	3	-		
>Code Value	(0008,0100)	1C			
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Admission ID	(0038,0010)	2	x		
Issuer of Admission ID	(0038,0011)	3	-		
Visit Status					
Visit Status ID	(0038,0008)	3	-		
Current Patient Location	(0038,0300)	2	x		
Patient's Institution Residence	(0038,0400)	3	-		
Visit Comments	(0038,4000)	3	-		
Visit Relationship					
Referenced Study Sequence	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Sequence	(0008,1120)	2	-		(0008,1120)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Visit Admission					
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Referring Physician's Address	(0008,0092)	3	-		
Referring Physician's Phone Numbers	(0008,0094)	3	-		
Admitting Diagnoses Description	(0008,1080)	3	x	(0008,1080)	
Admitting Diagnosis Code Sequence	(0008,1084)	3			
>Code Value	(0008,0100)	1C			

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Route of Admissions	(0038,0016)	3	-		
Admitting Date	(0038,0020)	3	-		
Admitting Time	(0038,0021)	3	-		
Patient Identification					
Patient's Name	(0010,0010)	1	x	(0010,0010)	(0010,0010)
Patient ID	(0010,0020)	1	x	(0010,0020)	(0010,0020)
Issuer of Patient ID	(0010,0021)	3	-	(0010,0021)	
Other Patient IDs	(0010,1000)	3	x	(0010,1000)	
Other Patient Names	(0010,1001)	3	x	(0010,1001)	
Patient's Birth Name	(0010,1005)	3	-	(0010,1005)	
Patient's Mother's Birth Name	(0010,1060)	3	-	(0010,1060)	
Medical Record Locator	(0010,1090)	3	-	(0010,1090)	
Patient Demographic					
Patients Birth Date	(0010,0030)	2	x	(0010,0030)	(0010,0030)
Patients Birth Time	(0010,0032)	3	-	(0010,0032)	
Patient's Sex	(0010,0040)	2	x	(0010,0040)	(0010,0040)
Patient's Insurance Plan Code Sequence	(0010,1050)	3	-	(0010,1050)	
>Code Value	(0008,0100)	1C			
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Patient's Age	(0010,1010)	3	x	(0010,1010)	
Patient's Size	(0010,1020)	3	x	(0010,1020)	
Patient's Weight	(0010,1030)	2	x	(0010,1030)	

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Patient's Address	(0010,1040)	3	x	(0010,1040)	
Military Rank	(0010,1080)	3	x	(0010,1080)	
Branch of Service	(0010,1081)	3	-	(0010,1081)	
Country of Residence	(0010,2150)	3	-	(0010,2150)	
Region of Residence	(0010,2152)	3	-	(0010,2152)	
Patient's Telephone Numbers	(0010,2154)	3	-	(0010,2154)	
Ethnic Group	(0010,2160)	3	x	(0010,2160)	
Occupation	(0010,2180)	3	-	(0010,2180)	
Patient's Religious Preference	(0010,21F0)	3	-	(0010,21F0)	
Patient Comments	(0010,4000)	3	x	(0010,4000)	
Patient Data Confidentiality Constraint Description	(0040,3001)	2	x	(0040,3001)	
Patient Medical					
Medical Alerts	(0010,2000)	2	x	(0010,2000)	
Contrast Allergies	(0010,2110)	2	x	(0010,2110)	
Pregnancy Status	(0010,21C0)	2	x	(0010,21C0)	
Smoking Status	(0010,21A0)	3	x	(0010,21A0)	
Last Menstrual Date	(0010,21D0)	3	x	(0010,21D0)	
Additional Patient History	(0010,21B0)	3	x	(0010,21B0)	
Special Needs	(0038,0050)	2	x	(0038,0050)	
Patient State	(0038,0500)	2	x	(0038,0500)	
Patient Relationship					
Referenced Study Sequence	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Visit Sequence	(0008,1125)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		

Table 60: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Alias Sequence	(0038,0004)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		

a. The Specific Character Set distributed via Modality Worklist by the hospital network shall reflect the global hospital context, e.g. a hospital with german context shall not restrict the worklist entries to ISO_IR 6 but supply a character set adequate to hold all german language text input.

3.6.2.1.4 Associated Real-World Activity - Get Worklist

With "Get Worklist" in the patient based Worklist Query dialog the entered attributes are used to form a worklist request identifier. With the response data the Patient Registration dialog can be updated to perform examination in advance. The response data are additionally placed in the scheduler database.

3.6.2.1.5 Proposed Presentation Contexts - Get Worklist

The same Presentation contexts as with "Update Worklist" will be proposed. Please see table 'Proposed presentation contexts' (pg. 103).

3.6.2.1.6 SOP Specific Conformance - Get Worklist

Search Key Attributes of the Worklist C-FIND

The PETsyngo DICOM worklist SCU supports "narrow worklist queries" with all required search keys.

The following table describes the search keys that the SCU supports for a patient based worklist query, which is defined by the following search keys:

Table 61: Search Key Attributes in a patient based worklist query

Attribute name	Tag	Matching Key Type	query value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	

Table 61: Search Key Attributes in a patient based worklist query

Attribute name	Tag	Matching Key Type	query value
>Scheduled Performing Physician's Name	(0040,0006)	R	inserted in UI or zero length
Requested Procedure			
Requested Procedure ID	(0040,1001)	O	inserted in UI or zero length
Imaging Service Request			
Accession Number	(0008,0050)	O	inserted in UI or zero length
Referring Physician's Name	(0008,0090)	O	inserted in UI or zero length
Visit Status			
Current Patient Location	(0038,0300)	O	inserted in UI or zero length
Patient Identification			
Patient's Name ^a	(0010,0010)	R	inserted in UI or zero length
Patient ID	(0010,0020)	R	inserted in UI or zero length

a. Please be aware that although in the UI there are different entries for First Name and Last Name of a patient these are combined into one query attribute. Querying just for the Last Name (without wildcard) or not providing a first letter for the First Name may prevent expected matches.

Return Key Attributes used from the Worklist C-FIND-RSP

Please see 'Basic Worklist C_FIND_RSP Return Key Attributes' (pg. 105).

Status Codes of the Worklist C-FIND

The worklist SCU interprets following status codes:

Table 62: C-FIND Response Status

Service Status	Meaning	Status Codes (0000,0900)	Related Fields
Refused	Out of Resources	A700	(0000,0902)

Table 62: *C-FIND Response Status*

Service Status	Meaning	Status Codes (0000,0900)	Related Fields
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.7 Modality Performed Procedure Step AE Specification

The Modality Performed Procedure Step SCU (Patient Registration and MPPS UI) provide information about a performed real-world Procedure to a remote SCP (Information System).

The PETsyngo DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

Table 63: SOP Classes as an SCU

SOP Class Name	SOP Class UID
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3

3.7.1 Association Establishment Policies

3.7.1.1 General

The creation of a MPPS Instance is done automatically by the PETsyngo DICOM application whenever a patient is registered for image acquisition through the Patient Registration dialog. Exception: In case of Emergency Patients the MPPS is created only when the user explicitly sends a corresponding message from the MPPS user interface.

Further updates on the MPPS data can be done interactively from the related MPPS user interface. The MPPS "Complete" or "Discontinued" states can only be set from user interface.

The default PDU size used will be 28 KB.

3.7.1.2 Number of Associations

The PETsyngo DICOM application initiates one association at a time, to create or set MPPS instance.

3.7.1.3 Asynchronous Nature

The PETsyngo DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

3.7.1.4 Implementation Identifying Information

The PETsyngo DICOM software provides the Implementation Class UID of

- "1.3.12.2.1107.5.1.4"

and an Implementation Version Name of

- "SIEMENS_S5VB20B".

3.7.2 Association Initiation Policy

The Modality Performed Procedure Step SCU establishes an association by using the DICOM association services.

The following DIMSE-N operations are supported as SCU:

- N-CREATE
- N-SET

3.7.2.1 Real World Activity

3.7.2.1.1 Associated Real-World Activity - Patient Registered

The associated Real-World activity is to send examination information to an SCP by using the DICOM Modality Performed Procedure Step Service.

3.7.2.1.2 Proposed Presentation Contexts - Patient Registered

The PETsyngo DICOM application will propose Presentation Contexts as shown in the following table:

Table 64: *Proposed presentation contexts*

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2	SCU	None
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1		
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2		

3.7.2.1.3 SOP Specific Conformance Statement - Patient Registered

Attributes used for the Performed Procedure Step N-CREATE

The DICOM Modality Performed Procedure Step SCU informs the remote SCP when the examination of a scheduled procedure step will be performed (i.e. the patient is registered). The N-CREATE message is sent when the examination is started with successful registration of patient data. The following table describes the supported attributes for a N-CREATE message.

Table 65: Performed Procedure Step N-CREATE Attributes

Attribute name	Tag	Required Type	Value
SOP Common			
Specific Character Set	(0008,0005)	1C	from MWL or created
Performed Procedure Step Relationship			
Scheduled Step Attribute Sequence	(0040,0270)	1	
>Study Instance UID	(0020,000D)	1	from MWL or created
>Referenced Study Sequence	(0008,1110)	2	from MWL or zero length
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Accession Number	(0008,0050)	2	from MWL or user input
>Placer Order Number / Imaging Service Request	(0040,2016)	3	from MWL or zero length
>Filler Order Number / Imaging Service Request	(0040,2017)	3	from MWL or zero length
>Requested Procedure ID	(0040,1001)	2	from MWL or user input
>Requested Procedure Description	(0032,1060)	2	from MWL or zero length
>Scheduled Procedure Step ID	(0040,0009)	2	from MWL or zero length
>Scheduled Procedure Step Description	(0040,0007)	2	from MWL or zero length
>Scheduled Protocol Code Sequence	(0040,0008)	2	from MWL or zero length
>>Code Value	(0008,0100)	1C	
>>Coding Scheme Designator	(0008,0102)	1C	
>>Code Scheme Version	(0008,0103)	3	
>>Code Meaning	(0008,0104)	3	

Table 65: *Performed Procedure Step N-CREATE Attributes*

Attribute name	Tag	Required Type	Value
Patient's Name	(0010,0010)	2	from MWL or user input
Patient ID	(0010,0020)	2	from MWL or user input or created
Patients Birth Date	(0010,0030)	2	from MWL or user input
Patient's Sex	(0010,0040)	2	from MWL or user input
Referenced Patient Sequence	(0008,1120)	2	from MWL or zero length
>Referenced SOP Class UID	(0008,1150)	1C	
>Referenced SOP Instance UID	(0008,1155)	1C	
Performed Procedure Step Information			
Performed Procedure Step ID	(0040,0253)	1	from SPS ID or created
Performed Station AE Title	(0040,0241)	1	own AE Title
Performed Station Name	(0040,0242)	2	own hostname
Performed Location	(0040,0243)	2	from SPS Location or zero length
Performed Procedure Step Start Date	(0040,0244)	1	created
Performed Procedure Step Start Time	(0040,0245)	1	created
Performed Procedure Step Status	(0040,0252)	1	IN PROGRESS
Performed Procedure Step Description	(0040,0254)	2	from SPS Description or zero length
Performed Procedure Type Description	(0040,0255)	2	zero length
Procedure Code Sequence	(0008,1032)	2	from Requested Procedure Code or zero length
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	3	

Table 65: Performed Procedure Step N-CREATE Attributes

Attribute name	Tag	Required Type	Value
>Code Meaning	(0008,0104)	3	
Performed Procedure Step End Date	(0040,0250)	2	zero length
Performed Procedure Step End Time	(0040,0251)	2	zero length
Image Acquisition Results			
Modality	(0008,0060)	1	CT ^a
Study ID	(0020,0010)	2	from Requested Procedure ID or created
Performed Protocol Code Sequence	(0040,0260)	2	from Scheduled Protocol Code SQ or zero length
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Series Sequence	(0040,0340)	2	
>Performing Physicians's Name	(0008,1050)	2C	from MWL or user input
>Protocol Name	(0008,1030)	1C	default value
>Operator's Name	(0008,1070)	2C	user input
>Series Instance UID	(0020,000E)	1C	created
>Series Description	(0008,103E)	2C	zero length
>Retrieve AE Title	(0008,0054)	2C	zero length
>Referenced Image Sequence	(0008,1140)	2C	zero length
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	zero length

a. For PET/CT acquisitions Performed Series Sequence may include PET image series even when the Modality is set to CT.

Status Codes of the Performed Procedure Step N-CREATE

The Performed Procedure Step SCU interprets the following status values:

Table 66: N-SET Response Status

Service Status	Meaning	Status Codes (0000,0900)
Failure	Processing Failure	0110
	No such attribute	0105
	Invalid attribute value	0106
	Duplicate SOP Instance	0111
	No such SOP Instance	0112
	No such SOP class	0118
	Class instance conflict	0119
	Missing attribute	0120
	Missing attribute value	0121
	Resource limitation	0213
Success	Successful Operation	0000

3.7.2.1.4 Associated Real-World Activity - Update

The associated Real-World activity is to send examination information to an SCP by using the DICOM Modality Performed Procedure Step Service either implicitly (examination) or explicitly (MPPS UI).

3.7.2.1.5 Proposed Presentation Contexts - Update

The same Presentation Contexts as in '*Proposed presentation contexts*' (pg. 115) will be proposed.

3.7.2.1.6 SOP Specific Conformance Statement - Patient Registered

Attributes used for the Performed Procedure Step N-SET

The PETsyngo DICOM performed procedure step SCU informs the remote SCP about the performed examination and its status. The N-Set message is sent once for each reconstruction of CT acquisition data with status "IN_PROGRESS". The N-SET message is sent on user input

with status "COMPLETED" or "DISCONTINUED", respectively. This is intended to be used when the examination is finished with status "COMPLETED" or when the examination could not be completed with status "DISCONTINUED" (already sent automatically when examination is ended via End Exam and no acquisition was done). The following table describes the supported attributes for a N-SET message.

Table 67: Performed Procedure Step N-SET Attributes

Attribute name	Tag	Required Type	Value
Performed Procedure Step Information			
Performed Procedure Step Status	(0040,0252)	3	IN_PROGRESS or COMPLETED or DISCONTINUED (see above)
Performed Procedure Step Description	(0040,0254)	3	from SPS Description or user input
Performed Procedure Type Description	(0040,0255)	3	zero length
Procedure Code Sequence	(0008,1032)	3	from Requested Procedure Code or empty on user change (see IHE Technical Framework Y3, App. C Note 6)
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	1C	
>Code Meaning	(0008,0104)	1C	
Performed Procedure Step End Date	(0040,0250)	3	created or zero length
Performed Procedure Step End Time	(0040,0251)	3	created or zero length
Image Acquisition Results			
Performed Protocol Code Sequence	(0040,0260)	3	from Scheduled Protocol Code SQ or user input
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	1C	

Table 67: *Performed Procedure Step N-SET Attributes*

Attribute name	Tag	Required Type	Value
>Code Meaning	(0008,0104)	1C	
Performed Series Sequence	(0040,0340)	1	
>Performing Physicians's Name	(0008,1050)	2C	from MWL or user input [empty if Study Split is used]
>Protocol Name	(0018,1030)	1C	name of Scan Protocol (Siemens standard or user defined) [dummy if Study Split is used]
>Operator's Name	(0008,1070)	2C	user input [empty if Study Split is used]
>Series Instance UID	(0020,000E)	1C	created [dummy if Study Split is used]
>Series Description	(0008,103E)	2C	range name with generated reconstruction information or user input [empty if Study Split is used]
>Retrieve AE Title	(0008,0054)	2C	from Storage Commitment RSP or zero length
>Referenced Image Sequence	(0008,1140)	2C	created [empty if Study Split is used]
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	zero length
Radiation Dose			
Total Number of Exposures	(0040,0301)	3	created (number of scans)
Distance Source to Detector (SID)	(0018,1110)	3	created
Distance Source to Entrance	(0040,0306)	3	created

Table 67: Performed Procedure Step N-SET Attributes

Attribute name	Tag	Required Type	Value
Comments on Radiation Dose	(0040,0310)	3	created (one line per scan) ^a
Billing and Material Management Code			
Film Consumption Sequence	(0040,0321)	3	created or zero length
>Number of Films	(2100,0170)	3	
>Medium Type	(2000,0030)	3	
>Film Size ID	(2010,0050)	3	
Billing Supplies and Devices Sequence	(0040,0324)	3	user input in Examination Card (example values below) or MPPS window
>Billing Item Sequence	(0040,0296)	3	
>>Code Value	(0008,0100)	1C	e.g. contrast media code
>>Code Scheme Designator	(0008,0102)	1C	e.g. contrast media catalog
>>Code Meaning	(0008,0104)	1C	e.g. contrast media name
>Quantity Sequence	(0040,0293)	1C	
>>Quantity	(0040,0294)	3	e.g. volume of contrast media
>>Measuring Units Sequence	(0040,0295)	3	
>>>Code Value	(0008,0100)	1C	e.g. cm3
>>>Code Scheme Designator	(0008,0102)	1C	e.g. UCUM
>>>Code Scheme Version	(0008,0103)	1C	e.g. 1.4
>>>Code Meaning	(0008,0104)	1C	e.g. cm3

a. The following format is used:

RangeName: kV=xxx mAs=xxx CTDIvol=xxx DLP=xxx

CTDIvol and DLP is not provided for Topogram scans.

Status Codes of the Performed Procedure Step N-SET

The Performed Procedure Step SCU interprets the following status values:

Table 68: *N-SET Response Status*

Service Status	Meaning	Status Codes (0000,0900)
Failure	Processing Failure: Performed Procedure Step Object may no longer be updated	0110
	No such attribute	0105
	Invalid attribute value	0106
	No such SOP Instance	0112
	Invalid object instance	0117
	No such SOP class	0118
	Class instance conflict	0119
	Missing attribute value	0121
	Resource limitation	0213
Success	Successful Operation	0000

4 Communication Profiles

4.1 Supported Communication Stacks

The PETsyngo DICOM application provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

The product target operating system is Windows XP.

4.1.1 OSI Stack

not supported.

4.1.2 TCP/IP Stack

The PETsyngo DICOM application uses the TCP/IP stack from the Windows XP system. It uses the MergeCOM-3 subroutine library from Merge Technologies Inc. that is based on a Berkeley socket interface.

4.1.2.1 API

The PETsyngo DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

4.1.2.2 Physical Media Support

The PETsyngo DICOM application is indifferent to the physical medium over which TCP/IP executes. It inherits it from the target operating system upon which it executes.

4.1.3 Point-to-Point Stack

not supported.

5 Extensions/Specializations/Privatizations

5.1 Standard Extensions

5.1.1 Standard Extensions of all SOP Classes

The following tables list the data dictionary of all DICOM IOD attributes where the DICOM standard definitions are extended:.

Table 69: *Standard Extensions of all SOP Classes*

Attribute Name	Tag	Private Creator	Type	Notes
Image Type	(0008,0008)	-	1	<p>See 5.1.1.1 for further explanation. additional Defined Terms:</p> <p>Defined Terms for value 3: OTHER MPR PROJECTION IMAGE UNDEFINED</p> <p>Defined Terms for value 4: CSA *^a CT_SOM4 * CT_SOM5 * CT_SOM6 * SHS *</p> <p>PETsyngo based Biograph products provide a value 5 with the Defined Terms: ADD CTL FINISHED IN_WORK MRTD OTOM OTOP PBF PBV PKET PMON TTP TTS</p>

Table 69: Standard Extensions of all SOP Classes

Attribute Name	Tag	Private Creator	Type	Notes
Patient Position	(0018,5100)	-	2C	Additional Defined Terms for the Magnetom Open HLS HLP FLS FLP HLDL HLDR FLDL FLDR
Body Part Examined	(0018,0015)		3	Additional Defined Terms for the PETsyngo based Biograph products: SPINE SPECIAL UNKNOWN SERVICE See 5.1.1.2 for further explanation.

a. For terms beginning with the stated prefix, e. g. "CSA", and ending with a "*", see 5.1.1.1 on page 126.

All SOP classes may contain additional type 3 attributes which DICOM standard defines in a different DICOM IOD or DICOM SOP class (attributes from Normalized SOP classes).

This is the case for example for

- Rescale Slope (0028,1053)
- Rescale Intercept (0028,1052)

which are also used in the MR IOD.

5.1.1.1 Image Type

The Image Type (0008,0008) attribute identifies important image identification characteristics. These characteristics are:

1. Pixel Data Characteristics:
 - is the image an ORIGINAL Image; an image whose pixel values are based on original or source data, or
 - is the image a DERIVED Image; an image whose pixel values have been derived in some manner from the pixel value of one or more other images.
2. Patient Examination Characteristics:
 - is the image a PRIMARY Image; an image created as a direct result of the Patient examination, or
 - is the image a SECONDARY Image; an image created after the initial Patient examination.
3. Modality Specific Characteristics (SOP Specific Characteristics).

4. Implementation specific identifiers; other implementation specific identifiers shall be documented in an implementation's conformance claim.

The Image Type attribute is multi-valued and shall be provided in the following manner:

- **Value 1** shall identify the Pixel Data Characteristics; Enumerated Values for the Pixel Data Characteristics are:
 - ORIGINAL = identifies an Original Image
 - DERIVED = identifies a Derived Image
- **Value 2** shall identify the Patient Examination Characteristics; Enumerated Values for the Patient Examination Characteristics are:
 - PRIMARY = identifies a Primary Image
 - SECONDARY = identifies a Secondary Image
- **Value 3** shall identify any Image IOD specific specialization, the following terms are defined in addition to the DICOM standard definitions:
 - OTHER = converted non-Axial and non-Localizer CT images; images of no special type (new syntax)
 - MPR = 3D MPR images (MR)
 - PROJECTION IMAGE = 3D MIP and SSD images (MR)
 - UNDEFINED = images of no special type (old syntax)
- **Value 4** is implementation specific. The following terms are defined:
 - original *syngo* generated data set types:
 - CSA 3D EDITOR = object created by 3D Editor
 - CSA 3D FLY PATH = object created by Fly Through Path
 - CSA 3D FLY VRT = object created by Fly Through Volume Rendering Technique
 - CSA 3D FUSION = object created by Fusion
 - CSA AVERAGE = image was created by Average
 - CSA BLACK IMAGE = SC Image with black pixels, only graphics information is of interest
 - CSA BOOKMARK = InSpace generated SC image containing bookmark information
 - CSA RESAMPLED = derived image created by zooming or panning original image
 - CSA REPORT = *syngo* Reporting (documentation of diagnosis)
 - CSA RESULT = *syngo* Reporting (post processing results)
 - CSA MIP THIN = image created by Maximum Intensity Projection
 - CSA MIP THIN CV = image created by Maximum Intensity Projection (curved cut)
 - CSA MPR = image created by Multi Planar Reconstruction
 - CSA MPR CV = image created by Multi Planar Reconstruction (curved cut)
 - CSA MPR THICK = image created by Multi Planar Reconstruction

CSA MPR THICK CV = image created by Multi Planar Reconstruction (curved cut)

CSA MPR THIN = image created by Multi Planar Reconstruction

CSA PSSD = SC image as Perspective Shaded Surface Display

CSA SSD = SC Image as Shaded Surface Display

CSA SUBTRACT = image was created by Subtraction

CSA VRT = SC Image created by Volume Rendering Technique

ECAT ACF = CTI PET Attenuation Correction

ECAT NORMAL = CTI PET Normalization

ECAT 3D SINO = CTI PET 3D Sinogram Short

ECAT 3D SINO FLT = CTI PET 3D Sinogram Float

- additional image types generated by PETsyngo based Biograph products

CT_SOM5 AVE = Averaged Image

CT_SOM5 ICD = Interventional Cine Display Image

CT_SOM5 MON = Monitoring or Premonitoring Image

CT_SOM5 MUL = Multiscan Image

CT_SOM5 PAR = Parameter Image

CT_SOM5 PROT = Protocol Image

CT_SOM5 ROT = ROT Image

CT_SOM5 RTD = Real Time Display Image

CT_SOM5 SEQ = Sequence Image

CT_SOM5 SPI = Spiral Image

CT_SOM5 SPO = Spiral Oblique Image

CT_SOM5 STA = Static Image

CT_SOM5 SUB = Subtracted Image

CT_SOM5 TOP = Topogram

CT_SOM5 DPAN = Dental Panorama Rebuilt Tomogram

CT_SOM5 DPAR = Dental Paraxial Rebuilt Tomogram

CT_SOM5 DFLM = Dental Filming Image

CT_SOM5 DYB = Dynamic Evaluation Averaged Baseline Image

CT_SOM5 DYF = Dynamic Evaluation Fused Multislice Image

CT_SOM5 PEVI = Pulmo Evaluation Image

CT_SOM5 OEVA = Osteo Evaluated Tomogram

CT_SOM5 MIP = Maximum Intensity Projection image created by a CT application

CT_SOM5 MPR = Multi Planar Reconstruction image created by a CT application

CT_SOM5 REP = Lung Care Report Image

- converted images
 - CT_SOM4 NONE = converted SOMARIS image
 - CT_SOM4 CONV = converted SOMARIS Convolution Kernel file
 - CT_SOM4 DART = converted SOMARIS Dental Artificial image
 - CT_SOM4 DEVA = converted SOMARIS Dental Evaluation image
 - CT_SOM4 DGRA = converted SOMARIS Dental Graphics image
 - CT_SOM4 DMEA = converted SOMARIS Dynamic Measurement image
 - CT_SOM4 DPAN = converted SOMARIS Dental Panorama image
 - CT_SOM4 DPAR = converted SOMARIS Dental Paraxial image
 - CT_SOM4 EBT = converted SOMARIS Evolution image
 - CT_SOM4 HIS = converted SOMARIS Histogram Graphics image
 - CT_SOM4 HISC = converted SOMARIS Histogram Graphics image
 - CT_SOM4 MUL = converted SOMARIS Multiscan image
 - CT_SOM4 OEVA = converted SOMARIS Osteo Evaluation image
 - CT_SOM4 OTOM = converted SOMARIS Osteo Tomogram image
 - CT_SOM4 OTOP = converted SOMARIS Osteo Topogram image
 - CT_SOM4 PLOT = converted SOMARIS Plot image
 - CT_SOM4 QUAL = converted SOMARIS Quality image
 - CT_SOM4 R2D = converted SOMARIS 2D Rebuild image
 - CT_SOM4 R3D = converted SOMARIS 3D Rebuild image
 - CT_SOM4 R3DE = converted SOMARIS 3D Rebuild image
 - CT_SOM4 RMAX = converted SOMARIS Maximum Intensity Projection image
 - CT_SOM4 RMIN = converted SOMARIS Minimum Intensity Projection image
 - CT_SOM4 ROT = converted SOMARIS Rotation Mode image
 - CT_SOM4 RRAD = converted SOMARIS Radiographic Projection image
 - CT_SOM4 RVIT = converted SOMARIS Vessel Image Tool image
 - CT_SOM4 RVRT = converted SOMARIS Volumetric Rendering image
 - CT_SOM4 SAVE = converted SOMARIS Evolution Screen Save image
 - CT_SOM4 SCAN = converted SOMARIS Standard Mode image
 - CT_SOM4 SEQ = converted SOMARIS Sequence Mode image
 - CT_SOM4 SER = converted SOMARIS Serial Mode image
 - CT_SOM4 SIN = converted SOMARIS Sinogram image
 - CT_SOM4 SINC = converted SOMARIS Sinogram image
 - CT_SOM4 SPI = converted SOMARIS Spiral Mode image
 - CT_SOM4 STA = converted SOMARIS Static Mode image

CT_SOM4 TAB = converted SOMARIS Correction Table image
CT_SOM4 TOP = converted SOMARIS Topogram image
CT_SOM4 GTOP = converted SOMARIS Topo Graphics image
CT_SOM4 PEVG = converted SOMARIS Pulmo Evaluation image
CT_SOM4 PEVI = converted SOMARIS Pulmo Evaluation image
CT_SOM4 PUL = converted SOMARIS Pulmo Respiration curve
CT_SOM4 PROT = converted SOMARIS Protocol image
CT_SOM4 TEXT = converted SOMARIS Text image
CT_SOM4 ICD = converted SOMARIS Interventional Cine image

SHS DENT = converted MagicView Dental Tomogram image
SHS DPAN = converted MagicView Dental Panorama image
SHS DPAR = converted MagicView Dental Paraxial image
SHS 3D_CURVED = converted MagicView image
SHS 3D_MIP = converted MagicView Maximum Intensity Projection image
SHS 3D_MPR = converted MagicView Multi Planar Reconstruction image
SHS 3D_SSD = converted MagicView Shaded Surface Display image
SHS 3D_VRT = converted MagicView Volumetric Rendering image

- **Value 5** is specific for the PETsyngo based Biograph products. In special cases (3D postprocessing) values mentioned for a lower index may appear for value 5 or higher. This will refer to 3D postprocessing base image types.

The following terms are defined:

- ADD = Additional Scan
- ALP = Arterial Liver Perfusion
- CTL = Control Scan
- HPI = Hepatic Perfusion Index
- FINISHED = Lung Care Report Image (finished)
- IN_WORK = Lung Care Report Image (not finished)
- MRTD = Multiscan Real Time Display Image
- OTOM = Osteo Scanned Tomogram
- OTOP = Osteo Scanned Topogram
- PBF = Perfusion Blood Flow Image
- PBV = Perfusion Blood Volume Image
- PKET = Peak Enhancement Parameter Image
- PMON = Premonitoring Scan
- PVP = Portal Venous Liver Perfusion

- RT3D CONFIG = InSpace Configuration Image
- TTP = Time to Peak Parameter Image
- TTS = Time to Start Parameter Image

5.1.1.2 Body Part Examined

The Body Part Examined (0018,0015) attribute provides a textual description of the part of the body examined. The PETsyngo based Biograph products extend the Defined Terms:

- SPINE = Summary term used instead of the Defined Terms CSPINE, TSPINE, LSPINE, and SSPINE
- SPECIAL = Image was acquired with acquisition modes that are not mapped to a certain part of the body
- SERVICE = Image was acquired for maintenance purpose
- UNKNOWN = No information about the body part available

See 5.1.2 for a mapping of the organ characteristics used for examination to the Body Part Examined terms.

In addition, the user interface permits the definition of new terms by the user. So in fact any syntactically correct value may be present as a value of this attribute. It is recommended, though, to use the DICOM defined terms when appropriate.

5.1.1.3 RGB color images

The PETsyngo DICOM application extends the CT Image IOD by the use of RGB color image description with the unsigned integer 24 bit color image plane pixel format:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = "RGB"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7
- planar configuration (attribute 0028,0006) = 0.

This format is used for Functional Imaging, i.e. images that meaningfully use all common CT Image attributes - however the pixel values do not represent a scaled Hounsfield value but a different value (depending on the type of image). Thus window related attributes must not be used to interpret the pixel values as scaled HU. The values used by PETsyngo are:

- window center (attribute 0028, 1050) = 128
- window width (attribute 0028,1051) = 256
- rescale intercept (attribute 0028, 1050) = 0
- rescale slope (attribute 0028,1051) = 1

The following types of images may use this format:

Table 70: Image Type (0008,0008) for objects created by PETsyngo

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Image Text
Averaged Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 AVE	none	AVE
Parameter Image (Patlak Blood Volume)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKBV	PAR
Parameter Image (Peak enhancement)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKET	PAR
Parameter Image (Perfusion Blood Flow)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBF	PAR
Parameter Image (Perfusion Blood Volume)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBV	PAR
Parameter Image (Permeability)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PMB	PAR
Parameter Image (Time to Peak)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTP	PAR
Parameter Image (Time to Start)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTS	PAR

5.1.2 Specializations

5.1.2.1 Images created by PETsyngo

The following table lists the PETsyngo image types and the corresponding combinations of the Image Type Attribute values.

Table 71: Image Type (0008,0008) for objects created by PETsyngo

Image Type Description [known creating applications]	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Image Text or Lists
Averaged Image [Average, DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 AVE	none	AVE
Interventional Cine Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 ICD	none	ICD
Monitoring Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MON	none	MON
Premonitoring Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MON	PMON	MON
Multiscan Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MUL	none	MUL
Parameter Image (Arterial Liver Perfusion) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	ALP	PAR
Parameter Image (Hepatic Perfusion Index) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	HPI	PAR
Parameter Image (Portal Venous Liver Perfusion) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PVP	PAR
Protocol Image, Time Density Curve Image [BodyPerfusion] ^a	SC	DERIVED	SECONDARY	OTHER	none	none	AC
Parameter Image (Patlak Blood Volume) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKBV	PAR

Table 71: Image Type (0008,0008) for objects created by PETsyngo

Parameter Image (Patlak Residual) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKER	PAR
Parameter Image (Patlak RSquare) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKR2	PAR
Parameter Image (Peak enhancement) [DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKET	PAR
Parameter Image (Perfusion Blood Flow) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBF	PAR
Parameter Image (Perfusion Blood Volume) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBV	PAR
Parameter Image (Permeability) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PMB	PAR
Parameter Image (Time to Peak) [DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTP	PAR
Parameter Image (Time to Start) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTS	PAR
Protocol Image	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 PROT	none	PROT (List only)
Report Image (not finished)	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 REP	IN_WORK	REP
Report Image (finished)	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 REP	FINISHED	REP
ROT Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 ROT	none	ROT
Real Time Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 RTD	none	RTD
Multiscan Real Time Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 RTD	MRTD	RTD
Sequence Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	none	SEQ

Table 71: Image Type (0008,0008) for objects created by PETsyngo

Additional Scan Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	ADD	SEQ
Control Scan Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	CTL	SEQ
Spiral Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SPI	none	SPI
Spiral Oblique Image	CT	DERIVED	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SPO	none	SPI
Static Image	CT	ORIGINAL	PRIMARY	OTHER	CT_SOM5 STA	none	STA
Subtracted Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 SUB	none	SUB
Topogram	CT	ORIGINAL	PRIMARY	LOCAL-IZER	CT_SOM5 TOP	none	TOP
Osteo Scanned Tomogram	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 SEQ	OTOM	SEQ
Osteo Scanned Topogram	CT	ORIGINAL	PRIMARY	LOCAL-IZER	CT_SOM5 TOP	OTOP	TOP
Osteo Evaluated Tomogram	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 OEVA	none	OEVA
Pulmo Evaluated Tomogram	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PEVI	none	PEVI
Calcium Scoring Table [Calcium Scoring]	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 TAB	none	TAB
Dental Filming Image	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DFLM	none	DFLM
Dental Panorama Rebuild Tomogram	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DPAN	none	DPAN
Dental Paraxial Rebuild Tomogram	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DPAR	none	DPAR
Dental/Volume Maximum Intensity Projection Image [Dental, Volume, DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MIP	none	MIP

Table 71: Image Type (0008,0008) for objects created by PETsyngo

Dental Panorama Reference Image [Dental, Volume]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	none	MPR
Dental Paraxial Reference Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	none	MPR
Dental Reference Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	none	MPR
Dynamic Evaluation Averaged Baseline	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 DYB	none	DYB
Dynamic Evaluation Fused Multi-slice	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 DYF	none	DYF
Volume reformat- ed images (sagittal and coronal)	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 MPR	none	MPR
Various result images [CalciumScoring, Colon, VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA MPR	none	MPR
Various result images [VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA MPR THICK	none	MPR
Various result images [VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA MIP	none	MIP
Various result images [CalciumScoring, VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA MIP THIN	none	MIP
Various result images [Colon]	SC	DERIVED	SECONDARY	OTHER	CSA PSSD	none	PSSD
Various result images [VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA VRT	none	VRT
Various result images [Colon]	SC	DERIVED	SECONDARY	OTHER	CSA VRT	none	VRT
Various result images [VesselView]	CT	DERIVED	SECONDARY	AXIAL	CSA RIBBON	none	RIBB

Table 71: Image Type (0008,0008) for objects created by PETsyngo

InSpace book- mark [InSpace]	SC	DERIVED	SECONDARY	OTHER	CSA BOOKMARK	RT3D CONFIG	BOOK
InSpace result images [InSpace]	SC	DERIVED	SECONDARY	OTHER	CSA 3DPROJEC TION	none	3DPR
Various Graphics [DynEva, Osteo, Pulmo, Volume, Perfusion, Argus, VesselView]	SC	DERIVED	SECONDARY	OTHER	CSA BLACK IMAGE	none	none

a. More detailed attribute information will be provided in a future version.

Note

Some applications (e.g. Argus, CalciumScoring) will create reports that are processed like a Structured Report internally. However, outside of the system they will appear as a SC image, labelled as Type 3 "OTHER" and Type 4 "CSA REPORT". This private extension is not published in detail here because it is to be replaced by real DICOM SR in future versions.

5.1.2.2 PETsyngo Attribute Interpretation

The tables below explain common attributes of created and uncompressed ORIGINAL and AXIAL CT and PET images. These tables do not intend to be a substitute for DICOM 3.0 attribute definitions. However, they will provide an impression of which attributes are in common use - and how they are related to PETsyngo examination.

Table 72: describes the attributes for CT images, Table 73: the attributes of PET images.

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0002,0012	Implementation Class UID	Value: 1.3.12.2.1107.5.1.4
0002,0013	Implementation Version Name	Value: SIEMENS_S5VB20B
0008,0005	Specific Character Set	
0008,0008	Image Type	see 5.1.2.1
0008,0016	SOP Class UID	Value: 1.2.840.10008.5.1.4.1.1.2
0008,0018	SOP Instance UID	created

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0008,0020	Study Date	For existing studies their date and time entries are copied into the corresponding entries in a new image's header. If a new study is created the date and time entries from the first series of this new study will be used.
0008,0030	Study Time	
0008,0021	Series Date	For existing series their date and time entries are copied into the corresponding entries in a new image's header. If a new series is created the current real-world date and time will be used.
0008,0031	Series Time	
0008,0022	Acquisition Date	Acquisition Date and Time is defined as the real-world beginning of the accumulation of data which contribute to a particular image. Due to the multi-slice technology several images may have the same Acquisition Date and Time.
0008,0032	Acquisition Time	
0008,0023	Image (Content) Date	For all images which result from a reconstruction of acquired data, the time stamp is the same as Acquisition Date and Time. This is true for images that were reconstructed immediately after data acquisition as well as for images that were reconstructed at any time later. For all other images created by any other means the time stamp is derived from a point in time during the creation process of these images.
0008,0033	Image (Content) Time	
0008,0050	Accession Number	Input entered from MWL or during patient registration. May be null-length.
0008,0060	Modality	Value: CT
0008,0070	Manufacturer	Value: SIEMENS
0008,0080	Institution Name	Hospital name read from configuration data or user input entered during patient registration or examination setup
0008,0081	Institution Address	Hospital address read from configuration data. Default format is 4 lines containing Street, City, District and Country.
0008,0090	Referring Physician's Name	Input from MWL or entered during patient registration or examination setup. May be null-length.
0008,1010	Station Name	Name of the computer the examination is controlled with

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0008,1030	Study Description	Is derived from information entered during patient registration or examination setup. Concatenated from Body Region and selected Scan Protocol name, separated by a "^"
0008,1050	Performing Physician's Name	Input entered from MWL or during patient registration.
0008,1070	Operator's Name	According to user input
0008,1080	Admitting Diagnoses Description	Input entered from MWL or during patient registration.
0008,103E	Series Description	According to user input (system proposes <Range Name> <Slice Thickness> <Kernel>)
0008,1090	Manufacturer's Model Name	Product Name: Biograph 6 Biograph 40 Biograph 64
0008,1140	Referenced Image Sequence	
>0008,1150	Referenced SOP Class UID	SOP Class UID of Topogram used for planning
>0008,1155	Referenced SOP Instance UID	SOP Instance UID of Topogram used for planning
0008,2112	Source Image Sequence	
>0008,1150	Referenced SOP Class UID	SOP Class UID of Rawdata used for reconstruction
>0008,1155	Referenced SOP Instance UID	SOP Instance UID of Rawdata used for reconstruction
0008,2111	Derivation Description	Lossy Image Compression will be set to 01 for Extended Field of View because of low image quality. Derivation Description: "Reconstruction field larger than scan field"
0009,00xx	Private Creator	Value: SIEMENS CT VA1 DUMMY
0010,0010	Patient's Name	Input from MWL or entered during patient registration or examination setup.
0010,0020	Patient ID	Input from MWL or entered or generated during patient registration or examination setup.

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation																								
0010,0030	Patient's Birth Date	Input from MWL or entered during patient registration or examination setup. May be calculated from age.																								
0010,0040	Patient's Sex	Input from MWL or entered during patient registration or examination setup.																								
0010,1010	Patient's Age	Input from MWL or entered during patient registration or examination setup. May be calculated from Patient’s Birth Date																								
0018,0010	Contrast/Bolus Agent	If present: The attribute is filled with the value entered in the contrast card. If nothing was entered the attribute is filled with the fixed term "APPLIED".																								
0018,0015	Body Part Examined	<p>The Body Part Examined is derived from the organ characteristic of the scan or directly entered by the operator, which overrides this default. The organ characteristic parameter is contained in the scan protocol selected for examination during patient registration or examination setup and may vary for different scans within one protocol (use System/Run/List Scan Protocols column "OrgChar" for a list of values for specific scan protocols).</p> <table><tr><th>Organ Characteristic</th><th>Body Part Examined</th></tr><tr><td>Head</td><td>HEAD</td></tr><tr><td>Neck</td><td>NECK</td></tr><tr><td>Shoulder</td><td>SHOULDER</td></tr><tr><td>Thorax</td><td>CHEST</td></tr><tr><td>Abdomen</td><td>ABDOMEN</td></tr><tr><td>Spine</td><td>SPINE</td></tr><tr><td>Pelvis</td><td>PELVIS</td></tr><tr><td>Extremities</td><td>EXTREMITY</td></tr><tr><td>Cardio</td><td>HEART</td></tr><tr><td>Service</td><td>SERVICE</td></tr><tr><td>n. a.</td><td>UNKNOWN</td></tr></table>	Organ Characteristic	Body Part Examined	Head	HEAD	Neck	NECK	Shoulder	SHOULDER	Thorax	CHEST	Abdomen	ABDOMEN	Spine	SPINE	Pelvis	PELVIS	Extremities	EXTREMITY	Cardio	HEART	Service	SERVICE	n. a.	UNKNOWN
Organ Characteristic	Body Part Examined																									
Head	HEAD																									
Neck	NECK																									
Shoulder	SHOULDER																									
Thorax	CHEST																									
Abdomen	ABDOMEN																									
Spine	SPINE																									
Pelvis	PELVIS																									
Extremities	EXTREMITY																									
Cardio	HEART																									
Service	SERVICE																									
n. a.	UNKNOWN																									
0018,0050	Slice Thickness	Resulting slice thickness. Not necessarily equal to collimated slice.																								
0018,0060	KVP	Voltage selected for scan.																								
0018,0090	Data Collection Diameter																									
0018,1000	Device Serial Number	Serial number of the CT system’s gantry.																								

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0018,1020	Software Version(s)	Software Version of Somaris/5. Only one value is used.
0018,1030	Protocol Name	Name of Scan Protocol selected during patient registration or examination setup
0018,1100	Reconstruction Diameter	Field of View selected for reconstruction
0018,1110	Distance Source to Detector	
0018,1111	Distance Source to Patient	
0018,1120	Gantry/Detector Tilt	
0018,1130	Table Height	Table height as entered for scan
0018,1140	Rotation Direction	
0018,1150	Exposure Time	The exposure time for the respective image. For spiral scan or multiscan this corresponds to the rotation time.
0018,1151	X-ray Tube Current	Tube current used for scanning
0018,1152	Exposure	(Effective) mAs. For spiral images the product of exposure time and x-ray tube current is corrected with Table Feed per Rotation. Expressed in mAs.
0018,1160	Filter Type	0: No Filter, 1: Teflon Filter
0018,1170	Generator Power	
0018,1190	Focal Spots	Size of the focal spot actually used to generate x-ray radiation for a particular image. This is a single value expressed in mm.
0018,1200	Date of Last Calibration	Date of last Base Calibration
0018,1201	Time of Last Calibration	Time of last Base Calibration
0018,1210	Convolution Kernel	4 character code of convolution kernel
0018,5100	Patient Position	As entered for scan
0019,00xx	Private Creator	Value: SIEMENS CT VA0 COAD
0019,xxB0	Feed per Rotation	Movement of table during one rotation in mm

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0020,000D	Study Instance UID	From MWL or created NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
0020,000E	Series Instance UID	From MWL or created
0020,0010	Study ID	From MWL or created NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
0020,0011	Series Number	created
0020,0012	Acquisition Number	Scan number within this examination.
0020,0013	Instance Number	created; direction within range selectable by user
0020,0032	Image Position (Patient)	The x, y, and z coordinates of the center of the first pixel, in mm.
0020,0037	Image Orientation (Patient)	
0020,0052	Frame of Reference UID	created
0020,1040	Position Reference Indicator	null-length
0020,1041	Slice Location	Topogram: Slice Location is defined as the relative table position of the very beginning of the Topogram image expressed in mm. Tomogram: Slice Location is defined as the relative position of the intersection of the image's slice with the z-axis expressed in mm. This positions is relative to the current reference point and corresponds to the table position.
0020,4000	Image Comments	According to user input. 2 lines supported.
0021,00xx	Private Creator	Value: SIEMENS MED
0021,xx11	Target	Center x/y as entered for reconstruction
0028,0002	Samples per Pixel	Value: 1
0028,0004	Photometric Interpretation	Value: MONOCHROME2
0028,0010	Rows	
0028,0011	Columns	

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0028,0030	Pixel Spacing	
0028,0100	Bits Allocated	Value: 16
0028,0101	Bits Stored	Value: 12
0028,0102	High Bit	Value: 11
0028,0103	Pixel Representation	Value: 0 (unsigned)
0028,0106	Smallest Image Pixel Value	Calculated by examination
0028,0107	Largest Image Pixel Value	Calculated by examination
0028,1050	Window Center	Last windowing center saved. First window followed by second window.
0028,1051	Window Width	Last windowing width saved. First window followed by second window.
0028,1052	Rescale Intercept	Value -1024 for images without extended CT scale
0028,1053	Rescale Slope	Value 1 for images without extended CT scale
0028,1055	Window Center & Width Explanation	Value: "WINDOW1", "WINDOW2"
0028,2110	Lossy Image Compression	Lossy Image Compression will be set to 01 for Extended Field of View because of low image quality. Derivation Description: "Reconstruction field larger than scan field"
0029,xxxx	(private data)	see section 5.2
0029,xx40	Application Header Sequence	see section 5.2
>0029,00xx	Private Creator	"SIEMENS MEDCOM HEADER"
>0029,xx41	Application Header Type	"SOM 5 TPOS"
>0029,xx42	Application Header ID	"SOM 5 NULLPOSITION"
>0029,xx43	Application Header Version	"VB10A 20030626"
>0029,xx44	Application Header Info	Table Null Position coded as a null terminated character buffer

Table 72: PETsyngo CT Attribute Interpretation

Tag	Name	Explanation
0032,1060	Requested Procedure Description	Input entered during patient registration or examination setup.
7FE0,0010	Pixel Data	

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0002,0012	Implementation Class UID	Value: 1.3.12.2.1107.5.1.4
0002,0013	Implementation Version Name	Value: SIEMENS_S5VB20B
0008,0005	Specific Character Set	
0008,0008	Image Type	Value 1: Original Value 2: Primary
0008,0016	SOP Class UID	Value: 1.2.840.10008.5.1.4.1.1.128
0008,0018	SOP Instance UID	created
0008,0020	Study Date	For existing studies their date and time entries are copied into the corresponding entries in a new image's header. If a new study is created the date and time entries from the first series of this new study will be used.
0008,0030	Study Time	
0008,0021	Series Date	Series date and time are set the earliest acquisition date and time of the scan.
0008,0031	Series Time	
0008,0022	Acquisition Date	Acquisition Date and Time is defined as the real-world beginning of the accumulation of data which contribute to a particular image. PET images belong to the same bed position share the same acquisition date and time.
0008,0032	Acquisition Time	
0008,0023	Image (Content) Date	Image (Content) Date and Time for PET images are set to the real-world date and time when the images are generated.
0008,0033	Image (Content) Time	
0008,0050	Accession Number	Input entered from MWL or during patient registration. May be null-length.
0008,0060	Modality	Value: PT

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0008,0070	Manufacturer	Value: SIEMENS
0008,0080	Institution Name	Hospital name read from configuration data or user input entered during patient registration or examination setup.
0008,0081	Institution Address	Hospital address read from configuration data. Default format is 4 lines containing Street, City, District and Country.
0008,0090	Referring Physician's Name	Input from MWL or entered during patient registration or examination setup. May be null-length.
0008,1010	Station Name	Name of the computer the examination is controlled with.
0008,1030	Study Description	Is derived from information entered during patient registration or examination setup. Concatenated from Body Region and selected Scan Protocol name, separated by a "^".
0008,1040	Institutional Department Name	According to site configuration.
0008,1050	Performing Physician's Name	Input entered from MWL or during patient registration.
0008,1070	Operator's Name	According to user input.
0008,1080	Admitting Diagnoses Description	Input entered from MWL or during patient registration.
0008,103E	Series Description	Based on user input and configured appendix.
0008,1090	Manufacturer's Model Name	PET gantry model number 1080 for Biograph HiRez 1093 for Biograph TruePoint 1094 for Biograph TruePoint with TrueV
0010,0010	Patient's Name	Input from MWL or entered during patient registration or examination setup.
0010,0020	Patient ID	Input from MWL or entered or generated during patient registration or examination setup.
0010,0030	Patient's Birth Date	Input from MWL or entered during patient registration or examination setup. May be calculated from age.

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0010,0040	Patient's Sex	Input from MWL or entered during patient registration or examination setup.
0010,1010	Patient's Age	Input from MWL or entered during patient registration or examination setup. May be calculated from Patient's Birth Date
0010,1030	Patient's Weight	Input from MWL or entered during patient registration or examination setup.
0018,0015	Body Part Examined	The Body Part Examined is directly entered by the operator.
0018,0050	Slice Thickness	Resulting slice thickness. It should be the same as the CT slice thickness if the PET reconstruction is configured to create PET image that matches CT slice location.
0018,1000	Device Serial Number	Currently is not populated with the real PET device serial number.
0018,1020	Software Version(s)	PETsyngo software version. Only one value is used.
0018,1030	Protocol Name	Name of Scan Protocol selected during patient registration or examination setup
0018,1060	Trigger Time	Time interval in ms from start of trigger to the beginning of data acquisition for this image. Gated only.
0018,1062	Nominal Interval	Average duration of accepted beats. Gated only.
0018,1063	Frame Time	Nominal duration per individual frame in ms. Gated only.
0018,1064	Framing Type	Value: PHASED Gated only.
0018,1080	Beat Rejection Flag	Value: Y Gated only.
0018,1081	Low R-R Value	R-R interval lower limit for beat rejection. Gated only.
0018,1082	High R-R Value	R-R interval upper limit for beat rejection. Gated only.
0018,1083	Intervals Acquired	Total number of accepted beat. Gated only.

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0018,1084	Intervals Rejected	Total number of rejected beats. Gated only.
0018,10xx	Skip Beats	Number of skipped beats after a detected arrhythmia. Gated only.
0018,10xx	Heart Rate	Average number of heart beats per minute for the collection period. This includes all accepted and rejected beats. Gated only.
0018,1181	Collimator Type	Value: NONE
0018,1200	Date of Last Calibration	Date of last Norm and Gantry Offset
0018,1201	Time of Last Calibration	Time of last Norm and Gantry Offset
0018,1210	Convolution Kernel	Filter type and parameters: XYZ Gauss<w> XYZ Hamm<w> XYZ Hamm<w> XYZ Parz<w> XYZ BUTW<w>.<o> XYZ SHEP<w> XYZ MEDI<w> XYZ BOX<w> where <w> is the filter width (fwhm), and <o> is the filter order, e.g. XYZ BUTW5.00-1
0018,1242	Actual Frame Duration	Actual time elapsed during acquisition
0018,5100	Patient Position	As entered for scan. This value is set despite the use of the Patient Orientation Code Sequence (0054,0410).
0020,000D	Study Instance UID	From MWL or created
0020,000E	Series Instance UID	From MWL or created
0020,0010	Study ID	From MWL or created
0020,0011	Series Number	Created
0020,0012	Acquisition Number	A combination of the scan range number within the examination and a secondary index (bed, frame, gate) within the scan. For example, for whole-body scans (Topo, Spiral CT range, PET range) , the acquisition number set to $2 * 1000 + \text{bed index}$

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0020,0013	Instance Number	Created. The order of the Instance Number is not selectable by the user.
0020,0032	Image Position (Patient)	The x, y and z coordinates of the center of the first pixel in mm in the CT coordinate system. The coordinates are generated after the PET/CT FOV offset correction and hence may be used directly by PET/CT image fusion applications.
0020,0037	Image Orientation (Patient)	Direction cosines of the first row and first column with respect to the patient.
0020,0052	Frame of Reference UID	Created
0020,1040	Position Reference Indicator	Null
0020,1041	Slice Location	Relative position of the intersection of the image slice with the z-axis in mm. This position is relative to the current reference point and corresponds to the table position. It is generated after the PET/CT FOV z-offset correction.
0020,4000	Image Comments	Concatenated string, separated by "^": - User input for comment - CT series description for attenuation correction - Flag that transformation matrix was applied (TM) - Flag for metal artefact correction (MAR)
0028,0002	Samples per Pixel	Value: 1
0028,0004	Photometric Interpretation	Value: MONOCHROME2
0028,0010	Rows	Number of rows in the image
0028,0011	Columns	Number of columns in the image
0028,0030	Pixel Spacing	Physical distance in the patient between the center of each pixel, specified by a numeric pair - adjacent row spacing (delimiter) adjacent column spacing in mm.
0028,0051	Corrected Image	Terms used: DECY, ATTN, SCAT, DTIM, RAN, NORM, RADL
0028,0100	Bits Allocated	Value: 16
0028,0101	Bits Stored	Value: 16

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0028,0102	High Bit	Value: 15
0028,0103	Pixel Representation	Value: 1 (signed)
0028,0106	Smallest Image Pixel Value	Calculated during image reconstruction.
0028,0107	Largest Image Pixel Value	Calculated during image reconstruction.
0028,1050	Window Center	Calculated during image reconstruction. Identical for all images in a frame. If Global Scaling is selected for dynamic or gated reconstructions, it will be identical for all frames in a series.
0028,1051	Window Width	Calculated during image reconstruction. Identical for all images in a frame. If Global Scaling is selected for dynamic or gated reconstructions, it will be identical for all frames in a series.
0028,1052	Rescale Intercept	Value: 0
0028,1053	Rescale Slope	Calculated during image reconstruction. Identical for all images in a frame. If Global Scaling is selected for dynamic or gated reconstructions, it will be identical for all frames in a series.
0029,xxxx	(Private data)	See section 5.2
0054,0013	Energy Window Range Sequence	Sequence containing one item describing the energy window used to acquire the PET image series.
>0054,0014	Energy Window Lower Limit	The lower limit of the energy window in keV.
>0054,0015	Energy Window Upper Limit	The upper limit of the energy window in keV.
0054,0016	Radiopharmaceutical Information Sequence	Sequence containing items describing the isotope information.
>0018,1072	Radiopharmaceutical Start Time	Time of start of injection (Since there is no attribute for the injection date , a day shift between start of injection and start if acquisition is encoded in the last 3 digits of the injection time.)

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
>0018,1074	Radionuclide Total Dose	The radiopharmaceutical dose administered to the patient measured in Becquerels (Bq) at the Radiopharmaceutical Start Time
>0018,1075	Radionuclide Half Life	The radionuclide half life, in seconds, that was used in the correction of this image.
>0018,1076	Radionuclide Positron Fraction	The radionuclide positron fraction (fraction of decays that are by positron emission) that was used in the correction of this image.
>0054,0300	Radionuclide Code Sequence	Sequence that identifies the radionuclide.
0054,0061	Number of R-R Intervals	Value: 1
0054,0071	Number of Time Slots	Number of gates (for gated)
0054,0081	Number of Slices	If PET slice location is configured to match CT slice location, this number is determined by the available number of CT slices within the PET scan range. Otherwise the value is = Number of detector rings * 2 - 1.
0054,0101	Number of Time Slices	Number of frames (for dynamic)
0054,0410	Patient Orientation Code Sequence	Sequence containing one item that describes the orientation of the patient with respect to gravity. Values: recumbent
>0054,0412	Patient Orientation Modifier Code Sequence	Sequence containing one item that modifies or enhances the orientation specified by Patient Orientation Code Sequence. Values: supine, prone, right lateral decubitus, left lateral decubitus
0054,0414	Patient Gantry Relationship Code Sequence	Sequence containing one item that describes the orientation of the patient with respect to the gantry. Values: head-first or feet-first.
0054,1000	Series Type	Value 1: WHOLE BODY, DYNAMIC or GATED Value 2: IMAGE
0054,1001	Units	BQML for quantitative images, for example WHOLE BODY, GATED or DYNAMIC PROPCPS for non-quantitative images, for example non attenuation corrected images.

Table 73: PETsyngo PET Attribute Interpretation

Tag	Name	Explanation
0054,1002	Counts Source	Value: EMISSION
0054,1100	Randoms Correction Method	Value: DLYD
0054,1101	Attenuation Correction Method	Value: CT-derived mu-map for attenuation-corrected images.
0054,1102	Decay Correction	Value: START for decay-corrected images.
0054,1103	Reconstruction Method	DIFT OSEM2D <m>i<n>s OSEM3D <m>i<n>s PSF <m>i<n>s where <m> is the number of iterations and <n> the number of subsets, e.g. OSEM2D 2i8s.
0054,1105	Scatter Correction Method	Value: Model-based for scatter-corrected images.
0054,1200	Axial Acceptance	The maximum detector ring difference instead of angle in degrees.
0054,1201	Axial Mash	
0054,1300	Frame Reference Time	Time offset from the series time in ms. This value is different for images acquired in different bed positions or dynamic frames, but is the same for all gates.
0054,1321	Decay Factor	The decay factor that was used to scale this image if decay correction is applied.
0054,1322	Dose Calibration Factor	A factor that was used to scale this image from ECAT counts/sec to Bq/ml using a dose calibrator. The value is 1 if normalization was not applied.
0054,1330	Image Index	An encoded index identifying the position of the image within the PET series which is viewed as a multi-dimensional array.
7FE0,0010	Pixel Data	

5.1.2.3 OOG, Overlays, High Bits

Graphics in PETsyngo images are stored as Object Oriented Graphics (OOG) in private attributes (see 5.2.1.2.5). Non *syngo* based systems are not expected to interpret this information.

In order to allow display access to graphics information for DICOM based systems private OOG information is converted on export into DICOM Overlay information stored in group 6000. This is the recommended way for a DICOM based system to access overlay graphics information.

The following attributes are generated:

Overlay Rows (6000,0010)

Overlay Columns (6000,0011)

Number of Frames in Overlay (6000,0015)

Overlay Description (6000,0022) = "Siemens MedCom Object Graphics"

Overlay Type (6000,0040) = "G"

Origin (6000,0050) = 1, 1

Image Frame Origin (6000,0051)

Overlay Bits Allocated (6000,0100)

Bit Position (6000,0102)

Overlay Data (6000,3000)

However, DICOM Overlay information stored in group 6000 is not supported by all systems that might be used to store PETsyngo images. These systems may not be able to display PETsyngo generated overlays. For a special group of these systems there is another way to provide graphical overlay information. A remote node can be configured to have overlay graphics converted into unused pixel data above High Bit (0028,0102) for images that fulfil the following condition:

- bits allocated (attribute 0028, 0100) = 16
- bits stored (attribute 0028,0101) = 12
- high bit (attribute 0028,0102) = 11

Some systems are known to support this coding; they are able to display this information with the images. Please note, however, that the proper and recommended way to store overlays with DICOM is the use of group 6000.

5.2 Privatizations

5.2.1 Private Elements for Storage SOP Classes

The following private attributes are defined for all Siemens *syngo* based applications.

5.2.1.1 Registry of DICOM Data Elements

Tag	Private Owner Code	Name	VR	VM
(0029,xx08)	SIEMENS CSA HEADER	CSA Image Header Type	CS	1
(0029,xx09)	SIEMENS CSA HEADER	CSA Image Header Version	LO	1
(0029,xx10)	SIEMENS CSA HEADER	CSA Image Header Info	OB	1
(0029,xx18)	SIEMENS CSA HEADER	CSA Series Header Type	CS	1
(0029,xx19)	SIEMENS CSA HEADER	CSA Series Header Version	LO	1
(0029,xx20)	SIEMENS CSA HEADER	CSA Series Header Info	OB	1
(0029,xx08)	SIEMENS CSA NON-IMAGE	CSA Data Type	CS	1
(0029,xx09)	SIEMENS CSA NON-IMAGE	CSA Data Version	LO	1
(0029,xx10)	SIEMENS CSA NON-IMAGE	CSA Data Info	OB	1
(0029,xx08)	SIEMENS MEDCOM HEADER	MedCom Header Type	CS	1
(0029,xx09)	SIEMENS MEDCOM HEADER	MedCom Header Version	LO	1
(0029,xx10)	SIEMENS MEDCOM HEADER	MedCom Header Info	OB	1
(0029,xx20)	SIEMENS MEDCOM HEADER	MedCom History Information	OB	1
(0029,xx31)	SIEMENS MEDCOM HEADER	PMTF Information 1	LO	1
(0029,xx32)	SIEMENS MEDCOM HEADER	PMTF Information 2	UL	1
(0029,xx33)	SIEMENS MEDCOM HEADER	PMTF Information 3	UL	1
(0029,xx34)	SIEMENS MEDCOM HEADER	PMTF Information 4	CS	1
(0029,xx35)	SIEMENS MEDCOM HEADER	PMTF Information 5	UL	1
(0029,xx40)	SIEMENS MEDCOM HEADER	Application Header Sequence	SQ	1
(0029,xx41)	SIEMENS MEDCOM HEADER	Application Header Type	CS	1
(0029,xx42)	SIEMENS MEDCOM HEADER	Application Header ID	LO	1
(0029,xx43)	SIEMENS MEDCOM HEADER	Application Header Version	LO	1
(0029,xx44)	SIEMENS MEDCOM HEADER	Application Header Info	OB	1
(0029,xx50)	SIEMENS MEDCOM HEADER	Workflow Control Flags	LO	8
(0029,xx51)	SIEMENS MEDCOM HEADER	Archive Management Flag Keep Online	CS	1
(0029,xx52)	SIEMENS MEDCOM HEAD	Archive Management Flag Do Not Archive	CS	1
(0029,xx53)	SIEMENS MEDCOM HEADER	Image Location Status	CS	1
(0029,xx54)	SIEMENS MEDCOM HEADER	Estimated Retrieve Time	DS	1
(0029,xx55)	SIEMENS MEDCOM HEADER	Data Size of Retrieved Images	DS	1
(0029,xx08)	SIEMENS MEDCOM OOG	MEDCOM OOG Type	CS	1
(0029,xx09)	SIEMENS MEDCOM OOG	MEDCOM OOG Version	LO	1
(0029,xx10)	SIEMENS MEDCOM OOG	MEDCOM OOG Info	OB	1
Tag	Private Owner Code	Name	VR	VM
(7FE1,xx10)	SIEMENS CSA NON-IMAGE	CSA Data	OB	1

The next subsections will explain in which IODs these private data elements are used.

5.2.1.2 All syngo Supported Image SOP Classes

5.2.1.2.1 Extended Image IOD Module Table

Table 74: CSA Image IOD Modules

IE	Module	Reference	Usage	Note
Patient	Patient	part 3 C.7.1.1	M	
Study	General Study	part 3 C.7.2.1	M	
	Patient Study	part 3 C.7.2.2	U	
Series	General Series	part 3 C.7.3.1	M	
Equipment	General Equipment	part 3 C.7.5.1	U	
Image	General Image	part 3 C.7.6.1	M	
	Image Pixel	part 3 C.7.6.3	M	
	IOD specific modules	part 3 C.8.2.1	M/U	depends on the IOD
	CSA Image Header	5.2.1.2.2	U	
	CSA Series Header	5.2.1.2.3	U	
	MEDCOM Header	5.2.1.2.4	U	private syngo information
	MEDCOM OOG	5.2.1.2.5	U	if object graphics is attached to image
	SOP Common	part 3 C.12.1	M	

5.2.1.2.2 CSA Image Header Module

The table in this section contains private IOD Attributes that describe the CSA Image Header.

Table 75: CSA Image Header Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Image Header Type	(0029,xx08)	SIEMENS CSA HEADER	1	CSA Image Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = Somaris/5
CSA Image Header Version	(0029,xx09)	SIEMENS CSA HEADER	3	Version of CSA Image Header Info (0029,xx10) format.
CSA Image Header Info	(0029,xx10)	SIEMENS CSA HEADER	3	product dependent information.

5.2.1.2.3 CSA Series Header Module

The table in this section contains private IOD Attributes that describe the CSA Series Header.

Table 76: CSA Series Header Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Series Header Type	(0029,xx18)	SIEMENS CSA HEADER	1	CSA Series Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = Somaris/5
CSA Series Header Version	(0029,xx19)	SIEMENS CSA HEADER	3	Version of CSA Series Header Info (0029,xx20) format.
CSA Series Header Info	(0029,xx20)	SIEMENS CSA HEADER	3	product dependent information.

5.2.1.2.4 MEDCOM Header Module

The table in this section contains private IOD Attributes that describe MEDCOM Header.

Table 77: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MED-COM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 Required if MedCom Header Info (0029,xx10) present.
MedCom Header Version	(0029,xx09)	SIEMENS MED-COM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. Required if MEDCOM Header Info (0029,xx10) present.
MedCom Header Info	(0029,xx10)	SIEMENS MED-COM HEADER	3	Manufacturer model dependent information. The value of the attribute MedCom Header Info (0029,xx10) can be build up in each user defined format.
MedCom History Information	(0029,xx20)	SIEMENS MED-COM HEADER	3	MedCom defined Patient Registration history information. See 5.2.1.2.4.1.
PMTF Information 1	(0029,xx31)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 2	(0029,xx32)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 3	(0029,xx33)	SIEMENS MED-COM HEADER	3	Transformation Information

Table 77: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
PMTF Information 4	(0029,xx34)	SIEMENS MED-COM HEADER	3	Transformation Information
Application Header Sequence	(0029,xx40)	SIEMENS MED-COM HEADER	3	Sequence of Application Header Items. Zero or more Items shall be included in this sequence. Encoded as a sequence of items.
>Application Header Type	(0029,xx41)	SIEMENS MED-COM HEADER	1C	Application Header identification characteristics. Required if Sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MED-COM HEADER	3	Identification of an application header.
>Application Header Version	(0029,xx43)	SIEMENS MED-COM HEADER	3	Version of Application Header Info (0029,xx43) format.
>Application Header Info	(0029,xx44)	SIEMENS MED-COM HEADER	3	Application dependent information.
Workflow Control Flags	(0029,xx50)	SIEMENS MED-COM HEADER	3	Eight free definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS MED-COM HEADER	3	Flag to control remote archive management system to keep the image always online (also when already archived). Enumerated Values: 00 = remote control not required, 01 = keep image online.
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS MED-COM HEADER	3	Flag to control remote archive management system not to archive the related image. Enumerated Values: 00 = remote control not required, 01 = don't archive image.
Image Location Status	(0029,xx53)	SIEMENS MED-COM HEADER	3	Image location status to control retrieving. Defined Terms: ONLINE = retrieving has to be done as usual, NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54), OFFLINE = invoking a retrieve operation initiates an operator request, INVALID = invoking a retrieve operation would always result in an error.
Estimated Retrieve Time	(0029,xx54)	SIEMENS MED-COM HEADER	3	Estimated retrieve time in seconds. A value less than zero (< 0) indicates location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS MED-COM HEADER	3	Data size of images in MByte.

5.2.1.2.4.1 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined in the following way:

Table 78: MEDCOM History Information

Part	Name	Type	Bytes	Notes
header	Identifier	string	32	always "CSA HISTORY"
	Version	string	32	e.g. "V1.10"
n items	Class Name	string	64	
	Modification String	string	1024	

5.2.1.2.5 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used when object graphics is drawn on the image and stores the properties of the graphics objects (Line, Circle, Rectangle, Arrow, and so on). So the graphics objects will remain re-animatable even if such an image is transferred via DICOM C-STORE SOP class.

Table 79: MEDCOM OOG Module

Attribute Name	Tag	Private Creator	Type	Notes
MedCom OOG Type	(0029,xx08)	SIEMENS MED-COM OOG	1	MEDCOM Object Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1
MedCom OOG Version	(0029,xx09)	SIEMENS MED-COM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format.
MedCom OOG Info	(0029,xx10)	SIEMENS MED-COM OOG	3	MEDCOM Object Oriented Graphics (OOG) data.

The graphics objects are also stored in one Image overlay plane for compatibility with other products which don't support the MedCom OOG module. Any system which does not support this MedCom OOG module has to remove these private attributes when modifying the image overlay data.

5.2.2 Private Elements for CT Image Storage SOP Class

The following private attributes are defined for PETsyngo.

5.2.2.1 Registry of DICOM Data Elements

Tag	Private Owner Code	Name	VR	VM	Notes
(0019,xx90)	SIEMENS CT VA0 COAD	Osteo Offset	DS	1	Offset of the water equivalent material of the Siemens Osteo phantom to real water
(0019,xx92)	SIEMENS CT VA0 COAD	Osteo Regression Line Slope	DS	1	Slope of the regression line for the ESP (=European Spine Phantom) standardization
(0019,xx93)	SIEMENS CT VA0 COAD	Osteo Regression Line Intercept	DS	1	Intercept of the regression line for the ESP (=European Spine Phantom) standardization
(0019,xx96)	SIEMENS CT VA0 COAD	Osteo Phantom Number	IS	1	Number of the Siemens Osteo phantom
(0019,xxB0)	SIEMENS CT VA0 COAD	Feed per Rotation	DS	1	Som/4 style Feed per Rotation (Backwards Compatibility)
(0019,xxBD)	SIEMENS CT VA0 COAD	Pulmo Trigger Level	IS	1	Spirometer trigger level used for the scan, given in percent of VC (= Vital Capacity) of the patient
(0019,xxBE)	SIEMENS CT VA0 COAD	Expiratoric Reserve Volume	DS	1	ERV (= Expiratoric Reserve Volume) achieved by the patient
(0019,xxBF)	SIEMENS CT VA0 COAD	Vital Capacity	DS	1	VC (= Vital Capacity) achieved by the patient
(0019,xxC0)	SIEMENS CT VA0 COAD	Pulmo Water	DS	1	Density of the water insert of the Siemens Pulmo phantom
(0019,xxC1)	SIEMENS CT VA0 COAD	Pulmo Air	DS	1	Density of the air holes of the Siemens Pulmo phantom
(0019,xxC2)	SIEMENS CT VA0 COAD	Pulmo Date	DA	1	Date of the evaluation of the Siemens Pulmo phantom
(0019,xxC3)	SIEMENS CT VA0 COAD	Pulmo Time	TM	1	Time of the evaluation of the Siemens Pulmo phantom

(0021xx11)	SIEMENS MED	Target	DS	2	Som/4 style Target (Backwards Com- patibility)
0009,00xx	SIEMENS CT VA1 DUMMY	Private Creator Data Ele- ment	LO	1	1

5.2.3 Private SOP class CSA Non-Image

This chapter includes the definition of the Siemens AG B Med CSA defined private Non-Image Object (called CsaNonImage IOD). The focus of this private Non-Image Object is to address the requirement for non-image data sets found in *syngo* based applications.

The MedCom Non-Image Information Object Definition specifies data sets that are converted from a non-DICOM format to a modality independent DICOM format.


Examples of such manufacturer model dependent data sets are:

- Raw Data
- CT Admin Data
- MR Spectroscopy Data
- etc.

5.2.3.1 CSA Non-Image IOD Entity Relationship Model

The E-R model in [DICOM] A.1.2 depicts those components of the DICOM Information Model which directly refer to the CSA Non-Image IOD. The frame of reference IE, overlay IE, modality look up table IE, VOI lookup table IE and curve IE are not components of the CSA Non-Image IOD.

Figure 10: DICOM Information Model

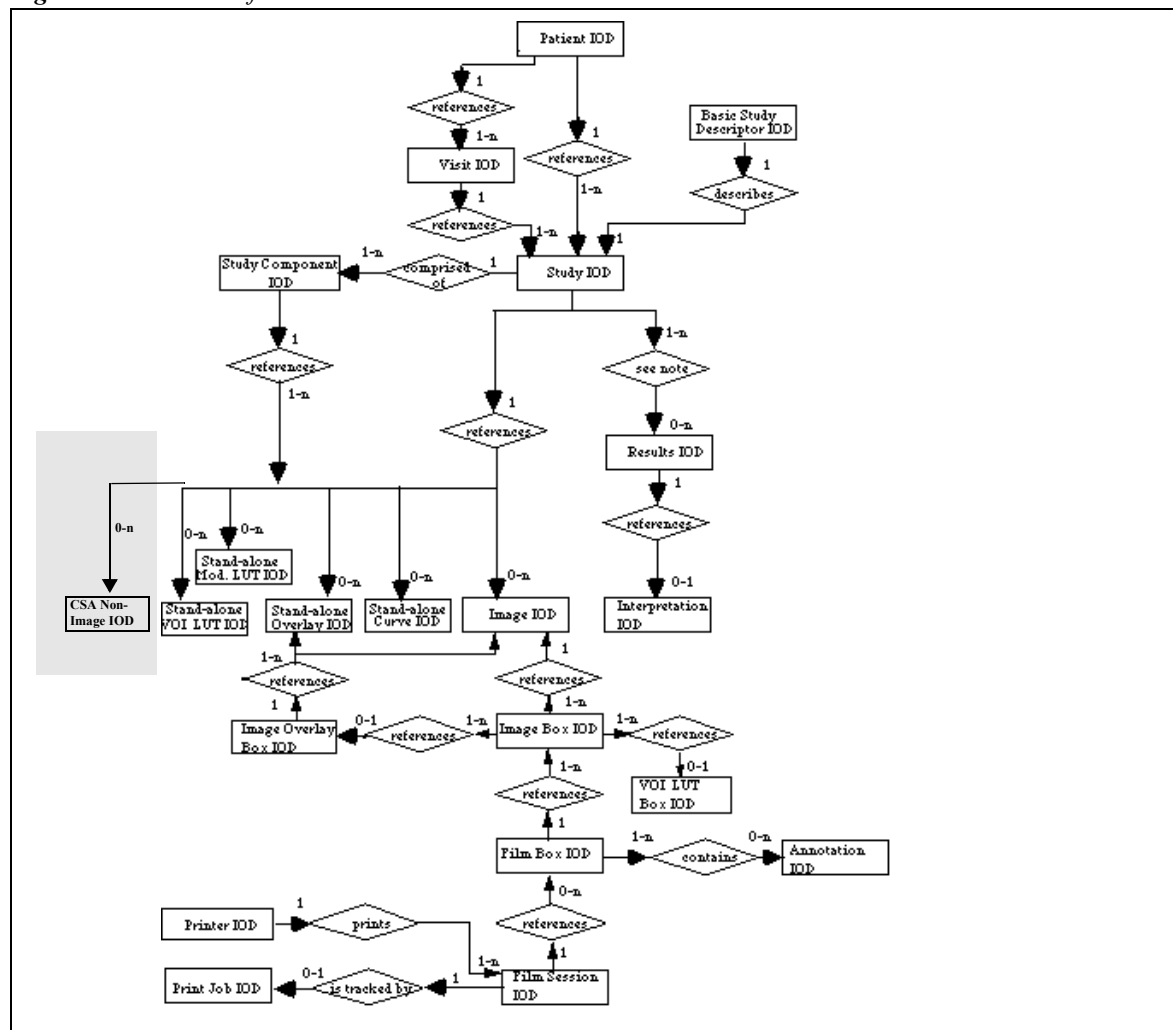

5.2.3.2 CSA Non-Image IOD Module Table

Table 80: CSA Non-Image IOD Modules

IE	Module	Reference	Usage
Patient	Patient	part 3 C.7.1.1	M
Study	General Study	part 3 C.7.2.1	M
	Patient Study	part 3 C.7.2.2	U
Series	General Series	part 3 C.7.3.1	M
Equipment	General Equipment	part 3 C.7.5.1	U
CSA	CSA Image Header	5.2.1.2.2	U
	CSA Series Header	5.2.1.2.3	U
	MEDCOM Header	5.2.1.2.4	U
	MEDCOM OOG	5.2.1.2.5	U
	CSA Non-Image	5.2.3.3	M
	SOP Common	part 3 C.12.1	M

5.2.3.3 CSA Non-Image Module

The table in this section contains private IOD Attributes that describe CSA Non-Images.

Table 81: *CSA Non-Image Module*

Attribute Name	Tag	Private Creator	Type	Notes
Image Type	(0008,0008)	-	3	Image identification characteristics. See 5.2.3.4.
Acquisition Date	(0008,0022)	-	3	The date the acquisition of data that resulted in this data set started.
Acquisition Time	(0008,0032)	-	3	The time the acquisition of data that resulted in this data set started.
Conversion Type	(0008,0064)	-	3	Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation.
Referenced Image Sequence	(0008,1140)	-	3	A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as sequence of items: (0008,1150) and (0008,1155).
Derivation Description	(0008,2111)	-	3	A text description of how this data set was derived.
Source Image Sequence	(0008,2112)	-	3	A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to derive this data set. Zero or more Items may be included in this Sequence. Encoded as sequence of items: (0008,1150) and (0008,1155).
Patient Position	(0018,5100)	-	3	Patient position descriptor relative to the equipment.
Acquisition Number	(0020,0012)	-	3	A number identifying the gathering of data over a period of time which resulted in this data set.
Instance Number	(0020,0013)	-	3	A number that identifies this data set.
Frame of Reference UID	(0020,0052)	-	3	Uniquely identifies the frame of reference for a Series.
Image Comments	(0020,4000)	-	3	User-defined comments about the image.
Quality Control Image	(0028,0300)	-	3	Indicates whether or not this image is a quality control or phantom image. If this Attribute is absent, then the image may or may not be a quality control or phantom image. Enumerated Values: YES, NO.

Table 81: CSA Non-Image Module

Attribute Name	Tag	Private Creator	Type	Notes
Burned In Annotation	(0028,0301)	-	3	Indicates whether or not image contains sufficient burned in annotation to identify the patient and date the image was acquired. If this Attribute is absent, then the image may or may not contain burned in annotation. Enumerated Values: YES, NO.
Lossy Image Compression	(0028,2110)	-	3	Specifies whether an Image has undergone lossy compression. Enumerated Values: 00 = Image has NOT been subjected to lossy compression, 01 = Image has been subjected to lossy compression.
Lossy Image Compression Ratio	(0028,2112)	-	3	Describes the approximate lossy compression ratio(s) that have been applied to this image. May be multi valued if successive lossy compression steps have been applied.
CSA Data Type	(0029,xx08)	SIEMENS CSA NON-IMAGE	1	CSA Data identification characteristics. Defined Terms: RAW DATA NUM 4 = NUMARIS/4 Raw Data SPEC NUM 4 = NUMARIS/4 Spectroscopy RAW DATA SOM 5 = Somaris/5 Raw Data BSR REPORT = BSR Study Report Data COL REPORT SOM5 = syngo Colonography Report Data
CSA Data Version	(0029,xx09)	SIEMENS CSA NON-IMAGE	3	Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format.
CSA Data Info	(0029,xx10)	SIEMENS CSA NON-IMAGE	3	Information to describe the CSA Data (7FE1,xx10). The value of the attribute CSA Data Info (0029,xx10) can be build up in each user defined format.
CSA Data	(7FE1,xx10)	SIEMENS CSA NON-IMAGE	1	Binary data as byte stream.

5.2.3.4 Extensions of the Non-Image Object

PETsyngo uses the following defined term for Image Type (0008,0008):

- Value 1: ORIGINAL, DERIVED
- Value 2: PRIMARY, SECONDARY

- Value 3: AXIAL, LOCALIZER, CPS_PT_WB, CPS_PT_LM, CPS_PT_NRM, CPS_PT_SM, OTHER
- Value4: CPS_PT_LM_CARDIAC, CPS_PT_LM_RESP, or a CT_SOM5 * enumeration
- Value5: CT specific enumeration

The following table lists the PETsyngo non-image types and the corresponding combinations of the Image Type Attribute values

Table 82: (Non-)Image Type (0008,0008) for private Non-image Objects

Description	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Image Text
ECG Data	none	none	none	none	none	none
Colonography Data	DERIVED	SECONDARY	OTHER	CT_SOM5 COL	none	none
Raw Data	Same entries as for images					
Sinogram data	ORIGINAL	PRIMARY	CPS_PT_WB	none	none	none
Listmode data	ORIGINAL	PRIMARY	CPS_PT_LM	none	none	none
Listmode data with ECG triggers	ORIGINAL	PRIMARY	CPS_PT_LM	CPS_PT_LM_CARDIAC	none	none
Listmode data with resp. triggers	ORIGINAL	PRIMARY	CPS_PT_LM	CPS_PT_LM_RESP	none	none
Attenuation correction data	DERIVED	PRIMARY	None	none	none	none
Normalization data	ORIGINAL	PRIMARY	CPS_PT_NRM	none	none	none
Protocol data	ORIGINAL	PRIMARY	CPS_PT_SM	none	none	none
ROI data	DERIVED	SECONDARY	OTHER	none	none	none

5.2.4 Private SOP Classes

Table 83: SOP Classes

SOP Class Name	SOP Class UID
CSA Non-Image	1.3.12.2.1107.5.9.1

5.2.5 Private Transfer Syntaxes

Not applicable

6 Configuration

6.1 AE Title / Presentation Address Mapping

To ensure unique identification the hostname should be part of the AE Titles (see examples below, hostname = station4). The string can be up to 16 characters long and must not contain any extended characters, only 7 bit ASCII characters (excluding control characters) are allowed according to DICOM standard. An example name is HRI_station4. Another common setting is the use of the hostname in capital letters, e.g. "STATION4".

Note

The current implementation does not support the full DICOM standard syntax. Spaces and special characters (like &<>) in the AE title string are not supported.

6.1.1 DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. E.g. Verification will use the Storage AE, if initiated to check the configuration of a remote DICOM node.

6.1.2 DICOM Storage/StorageCommitment/QR AE Title

There is a common AE Title for Storage, Storage Commitment and Query/Retrieve. It can be configured via Service UI in Configuration/DICOM/General.

The port is set to the fixed value of 104.

6.1.3 DICOM Modality Worklist and MPPS AE Title

There is a common AE Title for Modality Worklist and MPPS. It can be configured via Service UI in Configuration/DICOM/General.

6.1.4 DICOM Print AE Title

There is a separate AE Title for Print application. It can be configured via Service UI in Configuration/DICOM/General.

No input of AETs starting with a numeric character is possible.

6.1.5 Remote AE Titles and Presentation Addresses

Remote AETs, host names, IP addresses and port numbers can be configured using the Service application. For each AET a list of supported services can be configured.

6.2 Configurable Parameters

6.2.1 Storage, Storage Commitment and Query/Retrieve

The Service Configuration Tool can be used to set the AETs, port numbers, host names, IP addresses and capabilities for the remote nodes' (SCP's). The user can select transfer syntaxes, compression types and query models for each SCP separately.

- If the C-STORE is initiated by a user, only the transfer syntax will be proposed that is configured via Options -> Transfer -> Network Nodes (No Compression, Lossless JPEG, Lossy JPEG). The default transfer syntax (ILE) will be proposed in any case.
- If the C-STORE is initiated by an autotransfer rule or by the C-MOVE SCP all transfer syntaxes that are configured in the Service UI for this particular network destination will be proposed. (Compressed Transfer Syntaxes will be proposed first followed by the uncompressed Transfer Syntaxes).

Additional configurable parameters for Storage Commitment are:

When acting as SCU:

- flag to indicate whether the association will be kept open to receive the response or to close the association and be prepared to receive the response on another association.
- time-out which defines how long the association of N-ACTION is kept to receive a N-EVENT-REPORT on the same association. The same value is used to wait for a N-EVENT-REPORT on another association (applicability of transaction UID).
(default 1 h)

When acting as SCP:

- flag to indicate whether an archive system is installed.

6.2.2 Print

The Service application can be used to configure the SCP (DICOM Printer).

These parameters are mandatory to be set:

- AET
- Host name
- IP address
- Port number

These parameters have defaults as per configuration file and can be changed:

- Default camera
- Pixel size
- Additional or changed film sheet formats (e.g. inch 14x14, inch 14x17, ...)
- List with mapping pixel size to each film sheet format

- Minimal density
- Stored printed film jobs
- Media type
- Film destination

6.2.3 Modality Worklist

The Service application can be used to set the AETs, port numbers, host names, IP addresses, capabilities, and time-outs for the remote nodes (SCPs).

Additional configurable parameters for Basic Worklist Query are:

- Query Waiting time - the time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default 20 s)
- Max. Query Match Number - the maximum number of entries accepted in one worklist (default is 100)
- Query Interval - the time between two C-FIND-RQs to the Hospital Information System (default is 60 min.)
- Broad Worklist Query behaviour: two values are defined:

Set the AE Title search attribute to the own AE Title, and the Modality search attribute to "*".

Set the Modality search attribute to the own modality and the AE Title search attribute to "*".

The sending of an empty Specific Character Set in a C-FIND-RQ can be omitted by configuration. However, this is not available in the Service application but must be set by a Siemens service technician.

6.2.4 Modality Performed Procedure Step

The Service application can be used to configure the Modality Worklist SCP to be a Modality Performed Procedure Step SCP also.

Additional configurable parameters for Modality Performed Procedure Step are:

- Default Catalog Name - (0008,0102) used for items entered in MPPS UI
- Default Catalog Version - (0008,0103) used for items entered in MPPS UI

6.3 Default Parameters

This configuration tool also uses some default parameters:

- maximal PDU size set to 28672 Bytes
- time-out for accepting/rejecting an association request: 60 s
- time-out for responding to an association open/close request: 60 s

-
- time-out for accepting a message over network: 60 s
 - time-out for waiting for data between TCP/IP-packets: 60 s

The Time-outs for waiting for a Request/Response message from the remote node are as follows:

- for Storage SCP/SCU: 600 s
- for Storage Commitment SCU:
 - time-out for Response to N-ACTION: 600 s
 - time-out for N-EVENT-REPORT: configurable, see section 6.2 on page 167
- for Query/Retrieve SCP/SCU: 600 s
- for Modality Worklist SCU: configurable, see section 6.2 on page 167.
- for Print Management SCU:
 - time-out for Response to N-SET-RQ: 240 s
 - time-out for Response to other Requests: 60 s

7 Support of Extended Character Sets

The PETsyngo DICOM application supports the ISO 8859 Latin 1 (ISO-IR 100) character set family and the same family with code extensions (ISO 2022 IR 100 Latin-1). The same is valid for its subsets (ISO-IR 6, ISO 2022 IR 6).

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD coming into the system, then the following measures are taken to make the characters DICOM conform: Try to import with ISO-IR 100. If ISO-IR 100 also fails convert each illegal character to '?'.

Part II - Media Storage

This part contains the Conformance Statement to all "Offline Media Application Profiles (incl. private extensions)" supported by the PETsyngo archive options.


The application profiles supported shall be:

- Standard Application Profiles
- Augmented Application Profiles
- syngo private Application Profiles

For general introductory topics see section 1 on page 11.

8 Implementation Model

8.1 Application Data Flow Diagram

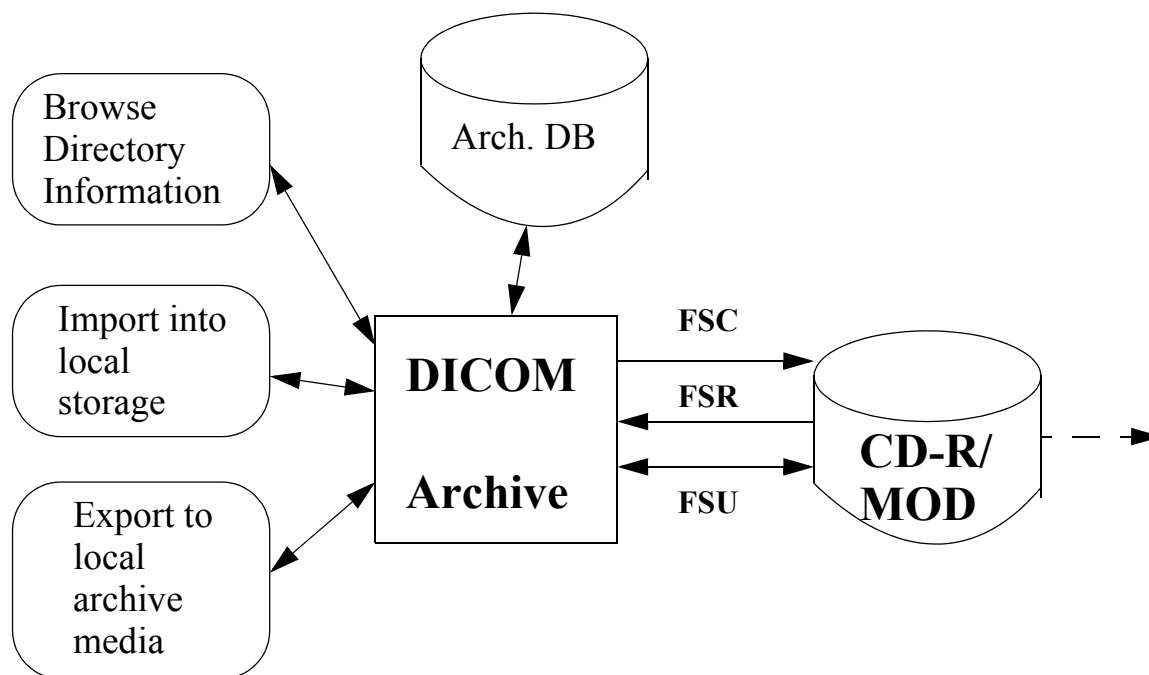

The DICOM archive application will serve as an interface to the CD-R or MOD off-line medium device. It serves interfaces to include the off-line media directory into the browser and to copy SOP instances to a medium or retrieve SOP Instances from medium into local storage.

The DICOM Archive application will support CD-R and MOD media (see Table 84:).

The FSU role will update new SOP Instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will be temporarily stored in Archive-Database.

8.2 Functional definitions of AE's

The PETsyngo DICOM off-line media storage application consists of the DICOM Archive application entity serving all interfaces to access off-line media. The DICOM Archive application is capable of

1. creating a new File-set onto an unwritten medium (Export to...)
2. updating an existing File-set by writing new SOP Instances onto the medium (Export to...)
3. copying SOP Instances from the medium onto local storage
4. reading the File-set's DICOMDIR information temporarily into database and pass it to display applications

8.3 Sequencing of Real-World Activities

The DICOM Archive application will not perform updates before the Directory information of the DicomDIR is completely read.

When performing updates, the SOP instances are checked for existence before updating. Duplicate instances will be avoided.

8.4 File Meta Information Options

The Implementation Class UID is:

- 1.3.12.2.1107.5.1.4

and an Implementation Version Name of

- "SIEMENS_S5VB20B"

9 AE Specifications

9.1 DICOM Archive Specification

The DICOM Archive provides Standard conformance to Media Storage Service Class (Interchange Option).

Table 84: Application profiles, Activities, and Roles for DICOM Archive

Application Profiles Supported	Real-World Activity	Role	SC Option
PRI-SYNGO-CD PRI-SYNGO-MOD23 PRI-SYNGO-MOD41 PRI-SYNGO-FD AUG-GEN-CD AUG-CTMR-MOD650 ^a AUG-CTMR-MOD12 ^a AUG-CTMR-MOD23 ^a AUG-CTMR-CD ^a STD-XA1K-CD ^a	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange
	Export to local archive media	FSC,FSU	Interchange
STD-GEN-CD STD-CTMR-MOD650 STD-CTMR-MOD12 STD-CTMR-MOD23 STD-CTMR-CD STD-XABC-CD STD-XA1K-CD TD-US-zz-yF-xxxxxx ^b STD-WVFM-GEN-FD	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange

a. With no private SOP Class used, the PRI-SYNGO-CD profile definitions are appropriate to describe the augmentation of the related -STD Profiles.

b. All combinations of the following values for zz, yF and xxxxxx are supported:

'yF' can take two values: SF for Single Frame and MF for Multi Frame.

'zz' can take three values: ID (Image Display), SC(Spatial Calibration) and CC (Combined Calibration)

xxxxxx can take 8 values: FLOP, MOD128, MOD230, MOD540, MOD650, MOD12, MOD23 and CDR

9.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See section 6 on page 166 for details.

9.1.2 Real-World Activities for this Application Entity

9.1.2.1 Real-World Activity: Browse Directory Information

The DICOM Archive application acts as FSR using the interchange option when requested to read the media directory.

The DICOM archive application will read the DICOMDIR and insert that directory entries, that are valid for the application profiles supported, into a local database. The database can then be used for browsing media contents.

Note:

Icon Image SQ is also supported in DICOMDIR. But only those Icon Images with Bits Allocated (0028,0100) equal to 8 and size 64 by 64 or 128 by 128 pixels are imported into database and are visible in PatientBrowser.

9.1.2.1.1 Application Profiles for the RWA: Browse Directory Information

See Table 84: for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

9.1.2.2 Real-World Activity: Import into local Storage

The DICOM Archive application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the local storage.

The SOP Instance selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported and are listed as supported by the Storage SCP Conformance section (see 3.2), can be retrieved from media storage. This is due to the fact that the Browse Directory Information will filter all SOP Instances not matching the Application profiles supported.

During operation no "Attribute Value Precedence" is applied to the SOP Instances. Detached Patient Management is not supported (please refer to DICOM part 11, Media Storage Application Profiles).

For media conforming to the STD-GEN-CD Profile the following SOP classes will be supported as a FSR:

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
SC Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Wave-form Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Elec-trophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Voice Audio Wave-form Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
XA Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Csa Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

9.1.2.2.1 Application Profiles for the RWA: Import into local Storage

See Table 84: for the Application Profiles listed that invoke this Application Entity for the Copy to Local Storage RWA.

9.1.2.3 Real-World Activity: Export to local Archive Media

The DICOM Archive application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive medium.

The DICOM Archive application will receive a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

When the DICOM archive application is requested to copy SOP Instances the preferred application profile according configuration will be used to validate and copy the referred SOP Instances. When creating a new file set no Descriptor File will be allocated and the related ID is not used.

The DICOM archive application will not close the medium.

9.1.2.3.1 Application Profiles for the RWA: Export to local Archive Media

See Table 84: for the Application Profiles listed that invoke this Application Entity for the Export to local Archive Media RWA.

10 Augmented and Private Profiles

10.1 Augmented Application Profiles

10.1.1 AUG-GEN-CD

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-GEN-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

The Siemens non-image is typically used for raw data and 3D private data. However, there are also other types of data (e.g. ECG data) that are stored using this IOD.

10.1.2 AUG-CTMR-xxxx

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-CTMR-MOD650, STD-CTMR-MOD12, STD-CTMR-MOD23, STD-CTMR-MOD41 and STD-CTMR-CD Standard Profiles.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

10.1.3 AUG-XA1K-CD

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-XA1K-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

10.2 *syngo*[®] private offline Media Application Profiles

This section will contain a syngo specific Application Profile.

The Structure of this Application Profile is defined in Part 11 of the DICOM Standard.

It is needed to describe the requirements for Offline Media Storage of the private IOD (Non-Image IOD).

10.2.1 Class and Profile Identification

This document defines an Application Profile class for "*syngo*[®] speaking"¹ modalities or applications.

The identifier for this class shall be PRI-SYNGO. This class is intended to be used for interchange of extended and private Information Objects via CD-R or re-writeable magneto-optical disk (MOD) offline media between dedicated acquisition or workstation modalities built from a common *syngo* architecture.

The specific application profiles in this class are shown in the table below:

Application Profile	Identifier	Description
" <i>syngo</i> speaking" System on CD-R	PRI-SYNGO-CD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)
" <i>syngo</i> speaking" System on 2.3 GB MOD	PRI-SYNGO-MOD23	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)
" <i>syngo</i> speaking" System on 4.1 GB MOD	PRI-SYNGO-MOD41	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)
" <i>syngo</i> speaking" System on Floppy Disk	PRI-SYNGO-FD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)

Equipment claiming conformance for this syngo Application Profile Class shall make a clear statement on handling of the private defined SOP Instances.

10.2.2 Clinical Context

This application profile facilitates the interchange of original acquired and derived images and private data related to them. Typical media interchange would be from in-lab acquisition equipment to dedicated workstations and archive systems with specific extensions to handle the private data objects (in both directions).

1. '*syngo*' and '*We speak syngo*' are registered trademarks of Siemens AG

Additionally, images used to prepare procedures, multi-modality images (e.g. integrated US) and images derived from primary diagnostic images, such as annotations, quantitative analysis images, reference images, screen capture images may be interchanged via this profile.

10.2.2.1 Roles and Service Class Options

This Application Profile uses the Media Storage Service Class defines in PS 3.4 with the Interchange Option.

The Application Entity shall support one or more of the roles of File Set Creator (FSC), File Set Reader (FSR), and File Set Updater (FSU), defined in PS3.10.

10.2.2.1.1 File Set Creator

The Application Entity acting as File Set Creator generates a File Set under the PRI-SYNGO Application Profiles.

File Set Creators shall be able to generate the Basic Directory SOP Class in the DICOMDIR file with all the subsidiary Directory Records related to the Image SOP Classes and Private SOP Classes stored in the File Set.

In case of the PRI-SYNGO-CD profile, the FSC shall offer the ability to either finalize the disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc).

Note

A multiple volume (a logical volume that can cross multiple physical media) is not supported by this Application Profile Class. If a set of Files, e.g., a Study, cannot be written entirely on one CD-R, the FSC will create multiple independent DICOM File Sets such that each File Set can reside on a single CD-R medium controlled by its individual DICOMDIR file. The user of the FSC can opt to use written labels on the discs to reflect that there is more than one disc for this set of files (e.g. a study).

10.2.2.1.2 File Set Reader

The role of the File Set Reader shall be used by Application Entities which receive the transferred File Set.

File Set Readers shall be able to read all the defined SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, using all the defined Transfer Syntaxes.

10.2.2.1.3 File Set Updater

The role of the File Set Updater shall be used by Application Entities, which receive a transferred File Set and update it by the addition of processed information.

File Set Updaters shall be able to read and update the DICOMDIR file. File Set Updaters do not have to read the image/private information objects. File Set Updaters shall be able to generate any of the SOP Instance files defined for the specific Application Profiles to which a conformance claim is made, and to read and update the DICOMDIR file.

In case of the PRI-SYNGO-CD profile, the FSU shall offer the ability to either finalize a disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information can be subsequently added to the disc).

Note (for CD-R)

If the disc has not been finalized, the File Set Updater will be able to update information assuming there is enough space on the disc to write a new DICOMDIR file, the information, and the fundamental CD-R control structures. CD-R control structures are the structures that inherent to CD-R standards; see PS 3.12

10.2.3 PRI-SYNGO Profiles

10.2.3.1 SOP Classes and Transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option. In the table below Transfer Syntax UID "RLE Lossless" applies only for decompression.

Table 85: *SOP Classes and Transfer Syntax*

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
Basic Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	M
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MR Image	1.2.840.10008.5.1.4.1.1.4	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
SC Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
SC Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
SC Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
SC Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
SC Image	1.2.840.10008.5.1.4.1.1.7	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1 1.2.840.10008.5.1.4.1.1.9.1.2 1.2.840.10008.5.1.4.1.1.9.1.3 1.2.840.10008.5.1.4.1.1.9.2.1 1.2.840.10008.5.1.4.1.1.9.3.1 1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1 1.2.840.10008.5.1.4.1.1.9.1.2 1.2.840.10008.5.1.4.1.1.9.1.3 1.2.840.10008.5.1.4.1.1.9.2.1 1.2.840.10008.5.1.4.1.1.9.3.1 1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
XA Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
XA Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
XA Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
XA Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
XA Image	1.2.840.10008.5.1.4.1.1.12.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
XRF-Image	1.2.840.10008.5.1.4.1.1.12.2	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
NM Image	1.2.840.10008.5.1.4.1.1.12.0	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
NM Image	1.2.840.10008.5.1.4.1.1.12.0	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.12.8	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
PET Image	1.2.840.10008.5.1.4.1.1.12.8	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.1481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Csa Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O

FSC, FSR, FSU - denote the requirement for those roles

O - Optional

M - Mandatory

10.2.3.2 Physical Media and Formats

The PRI-SYNGO-CD Profile requires the 120mm CD-R physical media with the ISO/IEC 9660 Media Format, as defined in PS3.12.

The PRI-SYNGO-MOD23 Profile requires the 130mm 2.3 GB R/W MOD physical medium with the PCDOS Media Format, as defined in PS3.12.

The PRI-SYNGO-MOD41 Profile requires the 130mm 4.1 GB R/W MOD physical medium with the PCDOS Media Format, as defined in PS3.12.

The PRI-SYNGO-FD Profile requires the 1.44 MB diskette physical medium with the PCDOS Media Format, as defined in PS3.12.

10.2.3.3 Directory Information in DICOMDIR

Conforming Application Entities shall include in the DICOMDIR File the Basic Directory IOD containing Directory Records at the Patient and subsidiary levels appropriate to the SOP Classes in the File Set. All DICOM files in the File Set incorporating SOP instances defined for the specific Application Profile shall be referenced by Directory Records.

Note

DICOMDIRs with no directory information are not allowed by this Application Profile
Privately defined IODs will be referenced by "PRIVATE" Directory Records.

10.2.3.3.1 Basic Directory IOD Specification

This Application Profile makes use of optional attributes of the Basic Directory IOD to support recognition of Patient's Storage Service request results in spanning multiple volumes (file sets). Therefore the File Set Descriptor File can be used and is then referenced by optional Basic Directory IOD attributes. If existent, the specified Descriptor File may be used by FSR applications. Any FSU, FSC shall make a clear statement if the Descriptor File mechanism is used according to the specialization defined in this Application Profile.

The Descriptor Files shall have the following contents:

One single line without any control characters and according to the Basic Character Set having the following defined text:

"MULTIVOLUME: xx of yy"

xx, yy are replaced by the actual number of the volume (xx) and the total number of volumes in the set (yy).

If used, the Descriptor File shall have the File ID "README" and reside in the same directory level as the DICOMDIR. It is referenced by the attribute [0004,1141] File Set Descriptor File ID having the defined contents of "README".

10.2.3.3.2 Additional Keys

File Set Creators and Updaters are required to generate the mandatory elements specified in PS 3.3, Annex F of the DICOM Standard. Table below: PRI-SYNGO-CD Additional DICOMDIR Keys specifies the additional associated keys. At each directory record level other additional data elements can be added, but it is not required that File Set Readers be able to use them as keys. Refer to the Basic Directory IOD in PS 3.3.

Table 86: DICOMDIR keys

Attribute Name	Tag	Directory Record Level	Type	Notes
Date Of Birth	(0010,0030)	PATIENT	2C	required, if present in SOP Instance
Patient's Sex	(0010,0040)	PATIENT	2C	required, if present in SOP Instance
Series Date	(0008,0021)	SERIES	3	
Series Time	(0008,0031)	SERIES	3	
Institution name	(0008,0080)	SERIES	2C	required, if present in SOP Instance
Institution Address	(0008,0081)	SERIES	2C	required, if present in SOP Instance
Series Description	(0008,103E)	SERIES	3	
Performing Physician	(0008,1050)	SERIES	2C	required, if present in SOP Instance
Image Type	(0008,0008)	IMAGE	1C	required, if present in SOP Instance
Content Date	(0008,0023)	IMAGE	3	
Content Time	(0008,0033)	IMAGE	3	
Referenced Image Sequence	(0008,1140)	IMAGE	1C	required, if present in SOP Instance
> Referenced SOP Class UID	(0008,1150)			
> Referenced SOP Instance UID	(0008,1155)			
Image Position (Patient)	(00020,0032)	IMAGE	2C	required, if present in SOP Instance
Image Orientation (Patient)	(0020,0037)	IMAGE	2C	required, if present in SOP Instance
Frame Of Reference UID	(0020,0052)	IMAGE	2C	required, if present in SOP Instance
Rows	(0028,0010)	IMAGE	3	
Columns	(0028,0011)	IMAGE	3	
Pixel Spacing	(0028,0030)	IMAGE	1C	C
Calibration Image	(0050,0004)	IMAGE	2C	required, if present in SOP Instance
Icon Image Sequence	(0088,0200)	IMAGE	3	required for Image SOP Classes
> Samples per Pixel	(0028,0002)			1
> Photometric Interpretation	(0028,0004)			MONOCHROME2
> Rows	(0028,0010)			128 for XA IOD, 64 otherwise
> Columns	(0028,0011)			128 for XA IOD, 64 otherwise

Table 86: DICOMDIR keys

Attribute Name	Tag	Directory Record Level	Type	Notes
> Bits Allocated	(0028,0100)			8
> Bits Stored	(0028,0101)			8
> High Bit	(0028,0102)			7
> Pixel Representation	(0028,0103)			0 (unsigned)
> Pixel Data	(7FE0,0010)			Icon Image pixel data
Curve Number	(0020,0024)	CURVE	1C	required, if present in SOP Instance

10.2.3.3.3 Private Directory Record Keys

Private Directory Records are supported by this Application Profile Class at the following level:
 IMAGE

The PRIVATE Directory Records will have required elements in addition to the mandatory elements specified in PS 3.3.

The following table will list the additional required keys for PRIVATE Directory Records.

Table 87: DICOMDIR keys for CsaNonImage

Attribute Name	Tag	Directory Record Level	Type	Notes
Private Record UID	(0004,1432)	PRIVATE	1	See Conformance Statement
SOP Class UID	(0008,0016)	PRIVATE	1C	required, if present in SOP Instance
SOP Instance UID	(0008,0018)	PRIVATE	1C	required, if present in SOP Instance
Image Type	(0008,0008)	PRIVATE	3	identification characteristics
Acquisition Date	(0008,0022)	PRIVATE	3	
Acquisition Time	(0008,0032)	PRIVATE	3	
Acquisition Number	(0020,0012)	PRIVATE	3	
CSA Data Type	(0029,xx08)	PRIVATE	1	private owner code = SIEMENS CSA NON-IMAGE
CSA Data Version	(0029,xx09)	PRIVATE	3	private owner code = SIEMENS CSA NON-IMAGE

10.2.3.3.4 Icon Images

Directory Records of type SERIES or IMAGE may include Icon Images. The Icon Image Pixel data shall be as specified in PS 3.3 "Icon Image Key Definition", and restricted such, that Bits Allocated (0028,0100) and Bits Stored (0028,0101) shall be equal to 8, and Rows (0028,0010) and Columns (0028,0011) shall be equal to 128 for XA Images and 64 for all other images. The Photometric interpretation (0028,0004) shall always be restricted to "MONOCHROME2".

PRIVATE Directory Records will not contain Icon Image information.

10.2.3.4 Other Parameters

This section defines other parameters common to all specific Application Profiles in the PRI-SYNGO class which need to be specified in order to ensure interoperable media interchange.

10.2.3.4.1 Multiframe JPEG Format

The JPEG encoding of pixel data shall use Interchange Format (with table specification) for all frames.

11 Extensions, Specializations and Privatizations of SOP Classes and Transfer Syntaxes

The SOP Classes listed refer in majority to those created by the equipment to which this Conformance Statement is related to. For SOP classes not listed in this section, please refer to the Storage section of the DICOM Conformance Statement of the product. This will include all SOP Instances that can be received and displayed and therefore will be included into offline media storage even though these SOP Instances are not created by the equipment serving the Media Storage Service.

11.1 SOP Specific Conformance Statement for Basic Directory

11.1.1 Extension, Specialization for SIEMENS Non-Image Objects

According to the PRI-SYNGO Application Profile Class the usage of the Private Creator UIDs and further optional keys for the Directory Records referring to SIEMENS Non-Image Objects are listed in the following table.

Attribute	Tag	Value used
Private Record UID	(0004,1432)	1.3.12.2.1107.5.9.1
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1

For the Non-Images no Icon Image Sequence will be generated.

12 Configuration

12.1 AE Title Mapping

12.1.1 DICOM Media Storage AE Title

The DICOM Storage application (Image Manager) provides the application entity title:

CsaImageManager

13 Support of Extended Character Sets

The PETsyngo DICOM application supports the ISO 8859 Latin 1 (ISO-IR 100) character set family and the same family with code extensions (ISO 2022 IR 100 Latin-1). The same is valid for its subsets (ISO-IR 6, ISO 2022 IR 6).

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD coming into the system, then the following measures are taken to make the characters DICOM conform: Try to import with ISO-IR 100. If ISO-IR 100 also fails convert each illegal character to'?'.

A Appendix

This appendix contains several attribute lists for images generated by specific applications. The subsequent fact must be kept in mind:

- Some text constants provided may be translated when using a non-English User Interface
- Private attributes are used; however, they are not listed in the tables below. Please refer to the general descriptions in chapter 5.
- Tables for applications "Colon", "Heart View", "Argus" are not included here. They will be provided in a future software version.

A.1 CT Standard Extended SOP Class

The PETsyngo application will create functional images from special applications. Some of these will be encoded as CT Standard extended SOP Class. Please see the following tables for a selected overview of supplied Standard attributes.

A.1.1 Examination (Spiral)

PETsyngo Examination will create images from reconstruction of Raw Data. As an example an overview of spiral image attributes is provided

Table 88: CT Acquisition/Reconstruction - Mode SPIRAL

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	from MWL or conf. Character Set
Image Type	(0008,0008)	"ORIGINAL\PRIMARY\AXIAL\CT_SOM5 SPI" or "ORIGINAL\SECONDARY\AXIAL\CT_SOM5 SPI"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<Date of registration>
Series Date	(0008,0021)	(Date of Creation)
Acquisition Date	(0008,0022)	(Date of Exposure resulting in this image)
Content Date	(0008,0023)	(Date of Instance Creation)
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<Time of registration>
Series Time	(0008,0031)	(Time of Creation of Series Instance)

Table 88: *CT Acquisition/Reconstruction - Mode SPIRAL*

Attribute Name	Tag	Value
Acquisition Time	(0008,0032)	(Time of Exposure resulting in this image)
Content Time	(0008,0033)	(Time of Instance Creation)
Accession Number	(0008,0050)	from MWL or Registration UI NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
Modality	(0008,0060)	“CT”
Manufacturer	(0008,0070)	“SIEMENS”
Institution Name	(0008,0080)	from Raw Data or Registration UI or Site Configuration
Institution Address	(0008,0081)	from Raw Data or Site Configuration
Referring Physician’s Name	(0008,0090)	from MWL or Registration UI
Station Name	(0008,1010)	Computer name
Study Description	(0008,1030)	<BodyRegion^ScanProtocol> NOTE: When Study Split is used, the Requested Procedure Description selected in Exam UI will be sent
Procedure Code Sequence	(0008,1032)	from MWL or empty
> (Code Sequence Macro)		from MWL or empty
Series Description	(0008,103E)	<created by system from Range Name> or <from Exam UI>
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	-
Performing Physicians’ Name	(0008,1050)	from Registration UI
Name of Physician(s) Reading Study	(0008,1060)	-
Operator’s Name	(0008,1070)	from Registration UI
Admitting Diagnoses Description	(0008,1080)	from MWL or Registration UI
Manufacturer’s Model Name	()	Product Name
Referenced Study Sequence	(0008,1110)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Study Component Sequence	(0008,1111)	MPPS reference (if MPPS is used)
> Referenced SOP Class UID	(0008,1150)	MPPS reference (if MPPS is used)
> Referenced SOP Instance UID	(0008,1155)	MPPS reference (if MPPS is used)
Referenced Patient Sequence	(0008,1120)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-

Table 88: CT Acquisition/Reconstruction - Mode SPIRAL

Attribute Name	Tag	Value
Referenced Image Sequence	(0008,1140)	Reference to corresponding Topogram
> Referenced SOP Class UID	(0008,1150)	Reference to corresponding Topogram
> Referenced SOP Instance UID	(0008,1155)	Reference to corresponding Topogram
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	Lossy image compression will be set for Extended Field of View because of low image quality. Derivation Descripton: "Reconstruction field larger than scan field". May also be set (to other values) by subsequent applications.
Source Image Sequence	(0008,2112)	Reference to corresponding Rawdata NonImage object
> Referenced SOP Class UID	(0008,1150)	Reference to corresponding Rawdata NonImage object
> Referenced SOP Instance UID	(0008,1155)	Reference to corresponding Rawdata NonImage object
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	from MWL or Registration UI or imported data
Patient ID	(0010,0020)	from MWL or Registration UI or imported data
Patient's Birth Date	(0010,0030)	from MWL or Registration UI or imported data
Patient's Birth Time	(0010,0032)	from MWL or imported data or empty
Patient's Sex	(0010,0040)	from MWL or Registration UI or imported data
Other Patient IDs	(0010,1000)	from MWL or imported data or Registration UI or empty
Other Patient Names	(0010,1001)	from MWL or imported data or empty
Patient's Age	(0010,1010)	from MWL or Registration UI or <calculated from (0010,0030)>
Patient's Size	(0010,1020)	from MWL or Registration UI
Patient's Weight	(0010,1030)	from MWL or Registration UI
Ethnic Group	(0010,2160)	from MWL or imported data or empty
Occupation	(0010,2180)	from MWL or Registration UI
Additional Patient's History	(0010,21B0)	from MWL or Registration UI?
Patient Comments	(0010,4000)	from MWL or imported data or empty
Contrast/Bolus Agent	(0018,0010)	if applicable: from Exam UI or "APPLIED"
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-

Table 88: CT Acquisition/Reconstruction - Mode SPIRAL

Attribute Name	Tag	Value
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	from Organ Characteristic or Exam UI
Slice Thickness	(0018,0050)	from Exam UI
Scan Options	(0018,0022)	special option data for cardio scans
KVP	(0018,0060)	from UI (nominal voltage)
Data Collection Diameter	(0018,0090)	Size of scan field (from configuration)
Device Serial Number	(0018,1000)	from Configuration
Software Version(s)	(0018,1020)	from Configuration
Protocol Name	(0018,1030)	Name of Scan Protocol selected during patient registration or examination setup
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	from Exam UI
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	from Exam UI
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	from Exam UI
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	From Exam UI (Field of View)
Distance Source to Detector	(0018,1110)	from Configuration
Distance Source to Patient	(0018,1111)	from Configuration
Gantry/Detector Tilt	(0018,1120)	from Exam UI
Table Height	(0018,1130)	from Exam UI
Rotation Direction	(0018,1140)	<created by system>
Exposure Time	(0018,1150)	<created by system> (Rotation Time)
X-Ray Tube Current	(0018,1151)	<created by system>
Exposure	(0018,1152)	<created by system> (eff. Exposure for image)
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	<created by system>
Generator Power	(0018,1170)	<created by system>
Focal Spot	(0018,1190)	<created by system> (Size of focus used only)

Table 88: CT Acquisition/Reconstruction - Mode SPIRAL

Attribute Name	Tag	Value
Date of last Calibration	(0018,1200)	Date of last successful Base Calibration
Time of last Calibration	(0018,1201)	Time of last successful Base Calibration
Convolution Kernel	(0018,1210)	from Exam UI
Patient Position	(0018,5100)	from Registration UI or Patient Model Dialog
Study Instance UID	(0020,000D)	from MWL or <newUID> NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	from MWL (Requested Procedure ID - if possible) or <created by system (highest available ID + 1)> NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
Series Number	(0020,0011)	<created by system>
Acquisition Number	(0020,0012)	<created by system: Scan Number>
Instance Number	(0020,0013)	<created by system>
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<calculated by system>
Image Orientation (Patient)	(0020,0037)	<calculated by system>
Frame of Reference UID	(0020,0052)	<new UID> (same within identical coordinate system)
Laterality	(0020,0060)	no value provided (CT scans are not selective)
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	Relative position of exposure expressed in terms of the patient table position (must not be used for calculations)
Image Comments	(0020,4000)	from Exam UI or <created by system> (1 or 2 lines)
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	"MONOCHROME2"
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	<calculated by system>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11

Table 88: *CT Acquisition/Reconstruction - Mode SPIRAL*

Attribute Name	Tag	Value
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	<calculated by system>
Largest Image Pixel Value	(0028,0107)	<calculated by system>
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	- (may be set by subsequent applications)
Window Center	(0028,1050)	from UI and Configuration (first window followed by second window)
Window Width	(0028,1051)	from UI and Configuration (first window followed by second window)
Rescale Intercept	(0028,1052)	-1024 or -10240
Rescale Slope	(0028,1053)	1 or 10
Window Center & Width Explanation	(0028,1055)	"WINDOW1\WINDOW2"
Pixel Padding Value	(0028,1020)	-
Lossy Image Compression	(0028,2110)	Lossy image compression will be set to 01 for Extended Field of View because of low image quality. Derivation Descriptor: "Reconstruction field larger than scan field". May also be set by subsequent applications.
Lossy Image Compression Ratio	(0028,2112)	- (may be set by subsequent applications)
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Requested Procedure Description	(0032,1060)	from MWL NOTE: When Study Split is used, the value corresponding to the Requested Procedure Description selected in Exam UI will be sent
Request Attributes Sequence	(0040,0275)	from MWL or Registration UI
> Requested Procedure ID	(0040,1001)	from MWL or Registration UI
> Scheduled Procedure Step ID	(0040,0009)	from MWL or empty
> Scheduled Procedure Step Description	(0040,0007)	from MWL or empty
> Scheduled Protocol Code Sequence	(0040,0008)	from MWL or empty
>> Code Sequence Macro		from Original
Performed Procedure Step ID	(0040,0253)	from MWL (Scheduled), if MPPS is used>
Performed Procedure Step Start Date	(0040,0244)	<created by system, if MPPS is used> or <User Input>

Table 88: CT Acquisition/Reconstruction - Mode SPIRAL

Attribute Name	Tag	Value
Performed Procedure Step Start Time	(0040,0245)	<created by system, if MPPS is used> or <User Input>
Performed Procedure Step Description	(0040,0254)	<from MWL (Scheduled), if MPPS is used> or <User Input>
Performed Protocol Code Sequence	(0040,0260)	<from MWL (Scheduled), if MPPS is used> or <User Input>
> Code Sequence Macro		<from MWL (Scheduled), if MPPS is used> or <User Input>
Comments on the Performed Procedure Step	(0040,0280)	<empty> or <User Input>
Icon Image Sequence	(0088,0200)	<created by system>
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Pixel Data	(7FE0,0010)	<created by system>

A.1.2 Body Perfusion

Perfusion will create CT result images.

This list of images will be referred to as PerfusionImageSet:

MIP, AVE, Flow, Blood Volume, Time To Start, Time To Peak, Permeability, Patlak Blood Volume, Patlak Residual, Patlak RSquare, Arterial Liver Perfusion, Portal Venuous Liver Perfusion, Hepatic Perfusion Index

The following table provides information about image attributes created:

Table 89: Body Perfusion

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	merged according to the syngo rules

Table 89: *Body Perfusion*

Attribute Name	Tag	Value
Image Type	(0008,0008)	<ul style="list-style-type: none"> • Value 1: <ul style="list-style-type: none"> • DERIVED • Value 2: <ul style="list-style-type: none"> • SECONDARY • Value 3: <ul style="list-style-type: none"> • AXIAL • Value 4: <ul style="list-style-type: none"> • MIP: CT_SOM5 MIP (Maximum Intensity Projection) • AVE: CT_SOM5 AVE (Average) • Flow, Blood Volume, Time To Start, Time To Peak, Permeability, Patlak Blood Volume, Patlak Residual, Patlak RSquare, Arterial Liver Perfusion, Portal Venous Liver Perfusion, Hepatic Perfusion Index: CT_SOM5 PAR (PAR: Parameter) • Value 5: <ul style="list-style-type: none"> • MIP, AVE: none • Flow: PBF (PBF: Perfusion Blood Flow) • Blood Volume: PBV (PBV: Perfusion Blood Volume) • Time To Start: TTS (TTS: Time To Start) • Time To Peak: TTP (TTP: Time To Peak) • Permeability: PMB (P: Permeability) • Patlak Blood Volume: PKBV (PKBV: Patlak Blood Volume) • Patlak Residual: PKER (PKER: Patlak Residual) • Patlak RSquare: PKR2 (PKR2: Patlak RSquare) • Arterial Liver Perfusion: ALP • Portal Venous Liver Perfusion: PVP • Hepatic Perfusion Index: HPI
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>
Acquisition Date	(0008,0022)	from the first image in time that is used to create the computed image

Table 89: Body Perfusion

Attribute Name	Tag	Value
Content Date	(0008,0023)	Date when the particular image is created. Supports the same sorting order as Image Number.
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	from the first image in time that is used to create the computed image
Content Time	(0008,0033)	Time when the particular image is created. Supports the same sorting order as Image Number.
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	value from the first image used to generate the computed image
Manufacturer	(0008,0070)	from the corresponding system configuration item
Institution Name	(0008,0080)	Perstring as defined for the corresponding system configuration item
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	For the series containing the results <ul style="list-style-type: none"> as gray scale images: string as defined in the corresponding configuration item as color images string as defined for the corresponding configuration item and the slice position value
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	from the corresponding system configuration item
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>

Table 89: Body Perfusion

Attribute Name	Tag	Value
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	“Som5 Perfusion Resampled”
Source Image Sequence	(0008,2112)	references to the images used to generate the computed image
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	-
Patient’s Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient’s Birth Date	(0010,0030)	<as Original>
Patient’s Birth Time	(0010,0032)	<as Original>
Patient’s Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient’s Age	(0010,1010)	<as Original>
Patient’s Size	(0010,1020)	<as Original>
Patient’s Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient’s History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	value from the first image used to generate the computed image

Table 89: *Body Perfusion*

Attribute Name	Tag	Value
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	-
Slice Thickness	(0018,0050)	PerfusionImageSet (A.1.2): effective slice thickness from the first original image
Scan Options	(0018,0022)	value from the first image used to generate the computed image
KVP	(0018,0060)	PerfusionImageSet (A.1.2): value from the first image used to generate the computed image
Data Collection Diameter	(0018,0090)	value from the first image used to generate the computed image
Device Serial Number	(0018,1000)	-
Software Version(s)	(0018,1020)	from the corresponding system configuration item
Protocol Name	(0018,1030)	-
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	value from the first image used to generate the computed image
Distance Source to Detector	(0018,1110)	value from the first image used to generate the computed image
Distance Source to Patient	(0018,1111)	value from the first image used to generate the computed image

Table 89: Body Perfusion

Attribute Name	Tag	Value
Gantry/Detector Tilt	(0018,1120)	value from the first image used to generate the computed image
Table Height	(0018,1130)	value from the first image used to generate the computed image
Rotation Direction	(0018,1140)	value from the first image used to generate the computed image
Exposure Time	(0018,1150)	value from the first image used to generate the computed image
X-Ray Tube Current	(0018,1151)	value from the first image used to generate the computed image
Exposure	(0018,1152)	value from the first image used to generate the computed image
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	value from the first image used to generate the computed image
Generator Power	(0018,1170)	value from the first image used to generate the computed image
Focal Spot	(0018,1190)	value from the first image used to generate the computed image
Date of last Calibration	(0018,1200)	-
Time of last Calibration	(0018,1201)	-
Convolution Kernel	(0018,1210)	value from the first image used to generate the computed image
Patient Position	(0018,5100)	value from the first image used to generate the computed image
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	new Series Instance UID
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	largest Series Number in the Study + 1
Acquisition Number	(0020,0012)	value from the first image used to generate the computed image
Instance Number	(0020,0013)	In an empty result series image numbers start with one, are incremented by one, and are assigned to each image to store in the order of PerfusionImageSet (A.1.2). If there are already images in a result series image number counting is continued. If there are more instances of a certain image type they are sorted according to their slice positions (from smallest slice position value to greatest).
Patient Orientation	(0020,0020)	-

Table 89: Body Perfusion

Attribute Name	Tag	Value
Image Position (Patient)	(0020,0032)	value from the first image used to generate the computed image ??
Image Orientation (Patient)	(0020,0037)	value from the first image used to generate the computed image
Frame of Reference UID	(0020,0052)	<as in first original image>
Laterality	(0020,0060)	value from the first image used to generate the computed image
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	average of the values from the images used to generate the computed image
Image Comments	(0020,4000)	string as defined for the corresponding configuration item
Samples per Pixel	(0028,0002)	For gray scale representation: value from the first image used to generate the computed image For color representation: according to the photometric representation
Photometric Interpretation	(0028,0004)	For gray scale representation: "MONOCHROME2" For color representation: "RGB"
Planar Configuration	(0028,0006)	For color representation: according to the photometric representation For gray scale representation: n. a
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	value from the first image used to generate the computed image
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image
Bits Stored	(0028,0101)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image
High Bit	(0028,0102)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image

Table 89: Body Perfusion

Attribute Name	Tag	Value
Pixel Representation	(0028,0103)	For all images: 0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	-
Window Center	(0028,1050)	<ul style="list-style-type: none"> For color representation: 128 For gray scale representation: Window Center value at the point when the image is made persistent
Window Width	(0028,1051)	<ul style="list-style-type: none"> For color representation: 256 For gray scale representation: Window Width value at the point when the image is made persistent
Rescale Intercept	(0028,1052)	value from the first image used to generate the computed image
Rescale Slope	(0028,1053)	value from the first image used to generate the computed image
Window Center & Width Explanation	(0028,1055)	-
Pixel Padding Value	(0028,1020)	-
Red Palette Color Lookup Table Descriptor	(0028,1101)	-
Green Palette Color Lookup Table Descriptor	(0028,1102)	-
Blue Palette Color Lookup Table Descriptor	(0028,1103)	-
Red Palette Color Lookup Table Data	(0028,1201)	-
Green Palette Color Lookup Table Data	(0028,1202)	-
Blue Palette Color Lookup Table Data	(0028,1203)	-
Lossy Image Compression	(0028,2110)	Set to "01" in all result images if there is a value of "01" in at least one of the images used to generate the results. Otherwise omitted.
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
(various private data)	(0029,xxxx)	the application ROI(s) as syngo object oriented graphics (MEDCOM OOG)

Table 89: *Body Perfusion*

Attribute Name	Tag	Value
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0060)	1/1
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	application ROI(s) as overlay pixel data
Pixel Data	(7FE0,0010)	values calculated as appropriate for the computed image

A.1.3 Calcium Scoring

Calcium Scoring will create Overview (MPR) and MIP images. The following table provides information about image attributes created:

Table 90: *Calcium Scoring*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100
Image Type	(0008,0008)	Type 1: "DERIVED" Type 2: "SECONDARY" Type 3: "AXIAL" or "OTHER" Type 4: "CSA MPR" or "CSA MIP" or "CSA MIP THIN"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<Date of first series>
Series Date	(0008,0021)	<Date of Creation>
Acquisition Date	(0008,0022)	<from Original>
Content Date	(0008,0023)	<from Original>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<Time of Creation of Series Instance>
Acquisition Time	(0008,0032)	<Time of Exposure resulting in this image>
Content Time	(0008,0033)	<Time of Instance Creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	"CT"
Manufacturer	(0008,0070)	"SIEMENS"
Institution Name	(0008,0080)	<from Original>
Institution Address	(0008,0081)	<from Original>
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	Computer name
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>

Table 90: Calcium Scoring

Attribute Name	Tag	Value
Series Description	(0008,103E)	<original Series name + “CaScoring” or “MPR Collection” or “MIP Collection”>
Institutional Department Name	(0008,1040)	<from Configuration>
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	<from Registration UI>
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	Somaris/5CaScoring
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	Reference to original image or empty
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Derivation Description	(0008,2111)	<from configuration>
Source Image Sequence	(0008,2112)	Reference to original image or empty
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Patient’s Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient’s Birth Date	(0010,0030)	<as Original>
Patient’s Birth Time	(0010,0032)	<as Original>
Patient’s Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>

Table 90: Calcium Scoring

Attribute Name	Tag	Value
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	-
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	<from Original>
Slice Thickness	(0018,0050)	<from Original>
Scan Options	(0018,0022)	-
KVP	(0018,0060)	<from Original>
Data Collection Diameter	(0018,0090)	<from Original>
Device Serial Number	(0018,1000)	-
Software Version(s)	(0018,1020)	<from Configuration>
Protocol Name	(0018,1030)	<from Original>
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-

Table 90: Calcium Scoring

Attribute Name	Tag	Value
Reconstruction Diameter	(0018,1100)	-
Distance Source to Detector	(0018,1110)	<from Original>
Distance Source to Patient	(0018,1111)	<from Original>
Gantry/Detector Tilt	(0018,1120)	<from Original>
Table Height	(0018,1130)	<from Original>
Rotation Direction	(0018,1140)	<from Original>
Exposure Time	(0018,1150)	<from Original>
X-Ray Tube Current	(0018,1151)	<from Original>
Exposure	(0018,1152)	<from Original>
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	<from Original>
Generator Power	(0018,1170)	<from Original>
Focal Spot	(0018,1190)	<from Original>
Date of last Calibration	(0018,1200)	-
Time of last Calibration	(0018,1201)	-
Convolution Kernel	(0018,1210)	<from Original>
Patient Position	(0018,5100)	<from Original>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<created by system>
Acquisition Number	(0020,0012)	<from Original>
Instance Number	(0020,0013)	<created by system>
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<from Original>
Image Orientation (Patient)	(0020,0037)	<application generated data>
Frame of Reference UID	(0020,0052)	<new UID> (same within identical coordinate system)
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	Relative position of exposure expressed in terms of the patient table position (must not be used for calculations)
Image Comments	(0020,4000)	<from Original>

Table 90: Calcium Scoring

Attribute Name	Tag	Value
Private Creator	(0021,00xx)	-
Target	(0021,xx11)	-
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	"MONOCHROME2"
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	<calculated by system>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	<from Original>
Window Width	(0028,1051)	<from Original>
Rescale Intercept	(0028,1052)	-1024 or -10240
Rescale Slope	(0028,1053)	1 or 10
Window Center & Width Explanation	(0028,1055)	"WINDOW1\WINDOW2"
Lossy Image Compression	(0028,2110)	<from Configuration>
Lossy Image Compression Ratio	(0028,2112)	<from Configuration>
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>

Table 90: Calcium Scoring

Attribute Name	Tag	Value
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Overlay Description	(60xx,0022)	Siemens MedCom Object Graphics
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<filled by application>
Pixel Data	(7FE0,0010)	<filled by application>

A.1.4 Dental CT

Dental CT will create Overview (MPR) and MIP as well as Paraxial (DPAR) and Panorama (DPAN) images. The following table provides information about image attributes created:

Table 91: Dental CT

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100
Image Type	(0008,0008)	Overview= "DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 MPR" MIP= "DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 MIP" Paraxial Reformats = "DERIVED", "SECONDARY", "OTHER", "CT_SOM5 DPAR" Panorama Reformats = "DERIVED", "SECONDARY", "OTHER", "CT_SOM5 DPAN"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	yes
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	yes
Acquisition Date	(0008,0022)	yes
Content Date	(0008,0023)	yes
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	yes
Acquisition Time	(0008,0032)	yes
Content Time	(0008,0033)	yes
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	yes
Manufacturer	(0008,0070)	yes
Institution Name	(0008,0080)	yes
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	yes
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>

Table 91: Dental CT

Attribute Name	Tag	Value
Series Description	(0008,103E)	yes
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	yes
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	yes
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	yes
Source Image Sequence	(0008,2112)	yes
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>

Table 91: Dental CT

Attribute Name	Tag	Value
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	-
Slice Thickness	(0018,0050)	yes
KVP	(0018,0060)	yes
Data Collection Diameter	(0018,0090)	yes
Device Serial Number	(0018,1000)	yes
Software Version(s)	(0018,1020)	-
Protocol Name	(0018,1030)	-
Spatial Resolution	(0018,1050)	-
Distance Source to Detector	(0018,1110)	yes
Distance Source to Patient	(0018,1111)	yes
Gantry/Detector Tilt	(0018,1120)	yes
Table Height	(0018,1130)	yes
Rotation Direction	(0018,1140)	yes
Exposure Time	(0018,1150)	yes
X-Ray Tube Current	(0018,1151)	yes
Exposure	(0018,1152)	yes
Exposure in μ As	(0018,1153)	-
Generator Power	(0018,1170)	yes
Focal Spot	(0018,1190)	yes
Date of last Calibration	(0018,1200)	yes
Time of last Calibration	(0018,1201)	yes
Convolution Kernel	(0018,1210)	yes
Patient Position	(0018,5100)	yes
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	yes

Table 91: Dental CT

Attribute Name	Tag	Value
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	yes
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	yes
Image Position (Patient)	(0020,0032)	yes
Image Orientation (Patient)	(0020,0037)	yes (Note: For Paraxial images the orientation of the first paraxial is used for the orientation of the CT image. A special image note will be created to hint at this fact.)
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Slice Location	(0020,1041)	yes
Image Comments	(0020,4000)	yes
Samples per Pixel	(0028,0002)	yes
Photometric Interpretation	(0028,0004)	yes
Rows	(0028,0010)	yes
Columns	(0028,0011)	yes
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	yes
Bits Stored	(0028,0101)	yes
High Bit	(0028,0102)	yes
Pixel Representation	(0028,0103)	yes
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	-
Window Center	(0028,1050)	yes
Window Width	(0028,1051)	yes
Rescale Intercept	(0028,1052)	yes
Rescale Slope	(0028,1053)	yes
Window Center & Width Explanation	(0028,1055)	yes
Pixel Padding Value	(0028,1020)	-

Table 91: Dental CT

Attribute Name	Tag	Value
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	yes
Overlay Columns	(60xx,0011)	yes
Number of Frames in Overlay	(60xx,0015)	"1"
Overlay Description	(60xx,0022)	"Siemens MedCom Object Graphics"
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	yes

Table 91: Dental CT

Attribute Name	Tag	Value
Overlay Origin	(60xx,0050)	yes
Image Frame Origin	(60xx,0051)	yes
Overlay Bits Allocated	(60xx,0100)	yes
Overlay Bit Position	(60xx,0102)	yes
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	yes
Pixel Data	(7FE0,0010)	yes

A.1.5 DynEva

DynEva application will create CT result images (see A.2 for SC result images). The following table provides information about image attributes created

Table 92: DynEva created CT images

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	"ISO_IR 100"
Image Type	(0008,0008)	"DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 DYB" or "DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 DYF"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	(Date of Creation)
Acquisition Date	(0008,0022)	-
Content Date	(0008,0023)	(Date of Instance Creation)
Acquisition Datetime	(0008,002A)	set for fused images to the date of the 1st image
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	(Date of Creation)
Acquisition Time	(0008,0032)	set for fused images to the time of the 1st image

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
Content Time	(0008,0033)	(Time of Instance Creation)
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	“CT”
Manufacturer	(0008,0070)	“SIEMENS”
Institution Name	(0008,0080)	taken from local config
Institution Address	(0008,0081)	-
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	hostname
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	“DynEva Curves”+<Evaluation Number>
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	-
Performing Physicians’ Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	-
Operator’s Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	read from modality config
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	“Som5 DynEva Resampled”

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
Source Image Sequence	(0008,2112)	reference to fused input images
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	-
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	copied from original
Slice Thickness	(0018,0050)	copied from original
Scan Options	(0018,0022)	-
KVP	(0018,0060)	copied from original
Data Collection Diameter	(0018,0090)	copied from original
Device Serial Number	(0018,1000)	read from the local config
Software Version(s)	(0018,1020)	read from modality config
Protocol Name	(0018,1030)	copied from original image series

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	copied from original mod image
Distance Source to Detector	(0018,1110)	copied from original mod image
Distance Source to Patient	(0018,1111)	copied from original mod image
Gantry/Detector Tilt	(0018,1120)	copied from original image
Table Height	(0018,1130)	copied from original image
Rotation Direction	(0018,1140)	copied from original image
Exposure Time	(0018,1150)	-
X-Ray Tube Current	(0018,1151)	-
Exposure	(0018,1152)	-
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	-
Generator Power	(0018,1170)	-
Focal Spot	(0018,1190)	-
Date of last Calibration	(0018,1200)	-
Time of last Calibration	(0018,1201)	-
Convolution Kernel	(0018,1210)	-
Patient Position	(0018,5100)	copied from original image
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<max series number>+1
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	(unknown)

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	avg of min and max imageposition (z-axis)
Image Orientation (Patient)	(0020,0037)	copied from original
Frame of Reference UID	(0020,0052)	<new UID>
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	avg of 1st and last location
Image Comments	(0020,4000)	e.g.: "DynEva MIP", "DynEva Baseline", "DynEva Peak Enhancement", "DynEva Fused MultiSlice", "DynEva Time To Peak", "DynEva Average", "DynEva Absolute Enhancement Curves",
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	"MONOCHROME2"
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	<calculated by system>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	(unknown)
Window Width	(0028,1051)	(unknown)
Rescale Intercept	(0028,1052)	-1024
Rescale Slope	(0028,1053)	1

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
Window Center & Width Explanation	(0028,1055)	“WINDOW1/WINDOW2”
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Request Attributes Sequence	(0040,0275)	-
> Requested Procedure ID	(0040,1001)	-
> Scheduled Procedure Step ID	(0040,0009)	-
> Scheduled Procedure Step Description	(0040,0007)	-
> Scheduled Protocol Code Sequence	(0040,0008)	-
>> Code Sequence Macro		-
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Overlay Description	(60xx,0022)	"Siemens MedCom Object Graphics"
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-

Table 92: *DynEva created CT images*

Attribute Name	Tag	Value
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<created by the application>
Pixel Data	(7FE0,0010)	<created by system>

A.1.6 Evaluation (Average/Subtract/Filter)

Evaluation applications will create CT result images. The following table provides information about image attributes created:

Table 93: *Evaluation (Average/Subtract/Filter)*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	copy from first Series
Image Type	(0008,0008)	Value 1: DERIVED Value 2: SECONDARY Value 3: AXIAL Value 4: CT_SOM5 AVE or CT_SOM5 SUB or from original
Instance Creation Date	(0008,0012)	will be initialized with the actual date during creation time
Instance Creation Time	(0008,0013)	will be initialized with the actual date during creation time
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	from original
SOP Instance UID	(0008,0018)	
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	current date
Acquisition Date	(0008,0022)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Content Date	(0008,0023)	-
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>

Table 93: *Evaluation (Average/Subtract/Filter)*

Attribute Name	Tag	Value
Series Time	(0008,0031)	current time
Acquisition Time	(0008,0032)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Content Time	(0008,0033)	-
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	“CT”
Manufacturer	(0008,0070)	copy from first Series
Institution Name	(0008,0080)	copy from first Series
Institution Address	(0008,0081)	copy from first Series
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	copy from first Series
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	will be initialized with the Result Series Description, default value proposed by the application after defined conventions e.g. SUBTRACTION_...
Institutional Department Name	(0008,1040)	copy from first Series
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	names will be copied, if all entries are identical, if not it will not be set
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	will not be set
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	copy from first Series
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>

Table 93: Evaluation (Average/Subtract/Filter)

Attribute Name	Tag	Value
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	-
Source Image Sequence	(0008,2112)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
> Referenced SOP Class UID	(0008,1150)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
> Referenced SOP Instance UID	(0008,1155)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
> Referenced Frame Number	(0008,1160)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	(unknown)
Contrast/Bolus Agent Sequence	(0018,0012)	-

Table 93: *Evaluation (Average/Subtract/Filter)*

Attribute Name	Tag	Value
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	copy from first Series, if identical in all participating series
Slice Thickness	(0018,0050)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Scan Options	(0018,0022)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
KVP	(0018,0060)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Data Collection Diameter	(0018,0090)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Device Serial Number	(0018,1000)	copy from first Series
Software Version(s)	(0018,1020)	copy from first Series
Protocol Name	(0018,1030)	function name (SUBTRACTION, AVERAGE, ...)
Contrast/Bolus Route	(0018,1040)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Contrast/Bolus Volume	(0018,1041)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Contrast/Bolus Start Time	(0018,1042)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Contrast/Bolus Stop Time	(0018,1043)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Contrast/Bolus Total Dose	(0018,1044)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Contrast Flow Rate(s)	(0018,1046)	unknown
Contrast Flow Duration(s)	(0018,1047)	unknown

Table 93: Evaluation (Average/Subtract/Filter)

Attribute Name	Tag	Value
Contrast/Bolus Ingredient	(0018,1048)	unknown
Contrast/Bolus Ingredient Concentration	(0018,1049)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical
Spatial Resolution	(0018,1050)	copy from first Series
Reconstruction Diameter	(0018,1100)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Distance Source to Detector	(0018,1110)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Distance Source to Patient	(0018,1111)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Gantry/Detector Tilt	(0018,1120)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Table Height	(0018,1130)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Rotation Direction	(0018,1140)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Exposure Time	(0018,1150)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
X-Ray Tube Current	(0018,1151)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Exposure	(0018,1152)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Exposure in μ As	(0018,1153)	unknown
Filter Type	(0018,1160)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Generator Power	(0018,1170)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.

Table 93: *Evaluation (Average/Subtract/Filter)*

Attribute Name	Tag	Value
Focal Spot	(0018,1190)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Date of last Calibration	(0018,1200)	copy from first Series
Time of last Calibration	(0018,1201)	copy from first Series
Convolution Kernel	(0018,1210)	If the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
<i>Patient Position</i>	(0018,5100)	copy from first Series
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	new UID
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	max plus 1
Acquisition Number	(0020,0012)	if the entries in the input images are identical, the entry will be copied. The entry remains empty, if it is not identical.
Instance Number	(0020,0013)	unknown
Patient Orientation	(0020,0020)	will not be set
Image Position (Patient)	(0020,0032)	will not be set
Image Orientation (Patient)	(0020,0037)	will not be set
Frame of Reference UID	(0020,0052)	copy from first Series
Laterality	(0020,0060)	copy from first Series, if identical in all participating series (not filled by CT meas.)
Images in <i>Acquisition</i>	(0020,1002)	copy from first image
Position <i>Reference</i> Indicator	(0020,1040)	-
Slice Location	(0020,1041)	must be the same from all images, copy from there
Image Comments	(0020,4000)	this entry is corresponding to 4.1.2.3.1 Default Result Series Description without the added number (to be unique), e.g. Subtract_S45_I10_I45
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	will be set with the biggest value of the input images
Columns	(0028,0011)	will be set with the biggest value of the input images
Pixel Spacing	(0028,0030)	copy from first image

Table 93: Evaluation (Average/Subtract/Filter)

Attribute Name	Tag	Value
Pixel Aspect Ratio	(0028,0034)	will not be set
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	smallest value of the pixel
Largest Image Pixel Value	(0028,0107)	biggest value of the pixel
Smallest Pixel Value in Series	(0028,0108)	unknown
Largest Pixel Value in Series	(0028,0109)	unknown
Pixel Padding Value	(0028,0120)	copy from first Series
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	- (may be set by subsequent applications)
Window Center	(0028,1050)	from first Image, if not set read from configuration
Window Width	(0028,1051)	from first Image, if not set read from configuration
Rescale Intercept	(0028,1052)	-1024
Rescale Slope	(0028,1053)	0
Window Center & Width Explanation	(0028,1055)	"WINDOW1\WINDOW2"
Lossy Image Compression	(0028,2110)	copy from first image
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	unkown
> LUT Descriptor	(0028,3002)	unkown
> LUT Explanation	(0028,3003)	unkown
> LUT Data	(0028,3006)	unkown
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	unkown
Performed Procedure Step Start Date	(0040,0244)	unkown
Performed Procedure Step Start Time	(0040,0245)	unkown

Table 93: *Evaluation (Average/Subtract/Filter)*

Attribute Name	Tag	Value
Performed Procedure Step Description	(0040,0254)	unkown
Performed Protocol Code Sequence	(0040,0260)	unkown
> Code Sequence Macro		unkown
Comments on the Performed Procedure Step	(0040,0280)	unkown
Icon Image Sequence	(0088,0200)	unkown
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Pixel Data	(7FE0,0010)	calculated by application

A.1.7 Lung Care

Lung Care will create CT result images (for SC result images see A.2). The following table provides information about image attributes created:

Table 94: *LungCARE - CT Images*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	<yes>
Image Type	(0008,0008)	“DERIVED\SECONDARY\OTHER\MPR” or “DERIVED\SECONDARY\OTHER\CT_SOM5 SPI”
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	-
Acquisition Date	(0008,0022)	<yes>
Content Date	(0008,0023)	<yes>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	-
Acquisition Time	(0008,0032)	<yes>
Content Time	(0008,0033)	<yes>
Accession Number	(0008,0050)	<as Original>

Table 94: LungCARE - CT Images

Attribute Name	Tag	Value
Modality	(0008,0060)	“CT”
Manufacturer	(0008,0070)	<yes>
Institution Name	(0008,0080)	<yes>
Institution Address	(0008,0081)	“_”
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	e.g. “SCREENING #1_result_1_1_VRT” or “SCREENING #1_result_1_2_MPR”
Institutional Department Name	(0008,1040)	from Site Configuration
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	“DR. CHACHOUA”
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	from Registration UI
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	<yes>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Derivation Description	(0008,2111)	- (may be set by subsequent applications)

Table 94: LungCARE - CT Images

Attribute Name	Tag	Value
Source Image Sequence	(0008,2112)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	(unknown)
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	<yes>
Slice Thickness	(0018,0050)	<yes>
Scan Options	(0018,0022)	<yes>
KVP	(0018,0060)	<yes>
Data Collection Diameter	(0018,0090)	<yes>
Device Serial Number	(0018,1000)	<yes>
Software Version(s)	(0018,1020)	<yes>
Protocol Name	(0018,1030)	-

Table 94: LungCARE - CT Images

Attribute Name	Tag	Value
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	<yes>
Distance Source to Detector	(0018,1110)	<yes>
Distance Source to Patient	(0018,1111)	<yes>
Gantry/Detector Tilt	(0018,1120)	<yes>
Table Height	(0018,1130)	<yes>
Rotation Direction	(0018,1140)	<yes>
Exposure Time	(0018,1150)	<yes>
X-Ray Tube Current	(0018,1151)	<yes>
Exposure	(0018,1152)	<yes>
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	<yes>
Generator Power	(0018,1170)	<yes>
Focal Spot	(0018,1190)	<yes>
Date of last Calibration	(0018,1200)	<yes>
Time of last Calibration	(0018,1201)	<yes>
Convolution Kernel	(0018,1210)	<yes>
Patient Position	(0018,5100)	<yes>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<yes>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<yes>
Acquisition Number	(0020,0012)	<yes>
Instance Number	(0020,0013)	<yes>

Table 94: LungCARE - CT Images

Attribute Name	Tag	Value
Patient Orientation	(0020,0020)	
Image Position (Patient)	(0020,0032)	<yes>
Image Orientation (Patient)	(0020,0037)	<yes>
Frame of Reference UID	(0020,0052)	<yes>
Laterality	(0020,0060)	
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	<yes>
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	"MONOCHROME2"
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	<yes>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	-
Window Center	(0028,1050)	<yes>
Window Width	(0028,1051)	<yes>
Rescale Intercept	(0028,1052)	-1024
Rescale Slope	(0028,1053)	1
Window Center & Width Explanation	(0028,1055)	<yes>
Pixel Padding Value	(0028,1020)	-
Lossy Image Compression	(0028,2110)	- (may be set by subsequent applications)
Lossy Image Compression Ratio	(0028,2112)	- (may be set by subsequent applications)

Table 94: LungCARE - CT Images

Attribute Name	Tag	Value
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
(various private data)	(0029,xxxx)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	
Performed Procedure Step Start Date	(0040,0244)	
Performed Procedure Step Start Time	(0040,0245)	
Performed Procedure Step Description	(0040,0254)	
Performed Protocol Code Sequence	(0040,0260)	
> Code Sequence Macro		
Comments on the Performed Procedure Step	(0040,0280)	
Icon Image Sequence	(0088,0200)	
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Pixel Data	(7FE0,0010)	<yes>

A.1.8 Neuro Perfusion

Perfusion will create CT result images.

This list of images will be referred to as NPerfusionImageSet:

MIP, AVE, Peak Enhancement, Time To Start, Time To Peak, Flow, Blood Volume, Permeability, Patlak Blood Volume, Patlak Residual, Patlak RSquare

The following table provides information about image attributes created:

Table 95: Neuro Perfusion

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	merged according to the syngo rules

Table 95: *Neuro Perfusion*

Attribute Name	Tag	Value
Image Type	(0008,0008)	<ul style="list-style-type: none"> • Value 1: <ul style="list-style-type: none"> • NPerfusionImageSet (A.1.8): DERIVED • other: from the original images • Value 2: <ul style="list-style-type: none"> • NPerfusionImageSet (A.1.8): SECONDARY • other: from the original images • Value 3: <ul style="list-style-type: none"> • NPerfusionImageSet (A.1.8): AXIAL • other: from the original images • Value 4: <ul style="list-style-type: none"> • MIP: CT_SOM5 MIP (Maximum Intensity Projection) • AVE: CT_SOM5 AVE (Average) • Peak Enhancement, Time To Start, Time To Peak, Flow, Blood Volume, Permeability, Patlak Blood Volume, Patlak Residual, Patlak RSquare: CT_SOM5 PAR (PAR: Parameter) • other: from the original images • Value 5: <ul style="list-style-type: none"> • MIP, AVE: none • Peak Enhancement: PKET (PKET: Peak Enhancement) • Time To Start: TTS (TTS: Time To Start) • Time To Peak: TTP (TTP: Time To Peak) • Flow: PBF (PBF: Perfusion Blood Flow) • Blood Volume: PBV (PBV: Perfusion Blood Volume) • Permeability: PMB (P: Permeability) • Patlak Blood Volume: PKBV (PKBV: Patlak Blood Volume) • Patlak Residual: PKER (PKER: Patlak Residual) • Patlak RSquare: PKR2 (PKR2: Patlak RSquare) • other: from the original images
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>

Table 95: *Neuro Perfusion*

Attribute Name	Tag	Value
Acquisition Date	(0008,0022)	NPerfusionImageSet (A.1.8): from the first image in time that is used to create the computed image other: from the original images
Content Date	(0008,0023)	Date when the particular image is created. Supports the same sorting order as Image Number.
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	NPerfusionImageSet (A.1.8): from the first image in time that is used to create the computed image other: from the original images
Content Time	(0008,0033)	Time when the particular image is created. Supports the same sorting order as Image Number.
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	value from the first image used to generate the computed image
Manufacturer	(0008,0070)	from the corresponding system configuration item
Institution Name	(0008,0080)	NPerfusionImageSet (A.1.8): string as defined for the corresponding system configuration item other: from the original images
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	For the series containing the results <ul style="list-style-type: none"> as gray scale images: string as defined in the corresponding configuration item as color images string as defined for the corresponding configuration item and the slice position value
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>

Table 95: Neuro Perfusion

Attribute Name	Tag	Value
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	from the corresponding system configuration item
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	"Som5 Perfusion Resampled"
Source Image Sequence	(0008,2112)	references to the images used to generate the computed image
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>

Table 95: *Neuro Perfusion*

Attribute Name	Tag	Value
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	value from the first image used to generate the computed image
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus stration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	-
Slice Thickness	(0018,0050)	NPerfusionImageSet (A.1.8): effective slice thickness from the first original image other: from the original images
Scan Options	(0018,0022)	value from the first image used to generate the computed image
KVP	(0018,0060)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Data Collection Diameter	(0018,0090)	value from the first image used to generate the computed image
Device Serial Number	(0018,1000)	-
Software Version(s)	(0018,1020)	from the corresponding system configuration item
Protocol Name	(0018,1030)	-
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-

Table 95: Neuro Perfusion

Attribute Name	Tag	Value
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	value from the first image used to generate the computed image
Distance Source to Detector	(0018,1110)	value from the first image used to generate the computed image
Distance Source to Patient	(0018,1111)	value from the first image used to generate the computed image
Gantry/Detector Tilt	(0018,1120)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Table Height	(0018,1130)	value from the first image used to generate the computed image
Rotation Direction	(0018,1140)	value from the first image used to generate the computed image
Exposure Time	(0018,1150)	baseline, NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
X-Ray Tube Current	(0018,1151)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Exposure	(0018,1152)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	value from the first image used to generate the computed image
Generator Power	(0018,1170)	value from the first image used to generate the computed image
Focal Spot	(0018,1190)	value from the first image used to generate the computed image
Date of last Calibration	(0018,1200)	-
Time of last Calibration	(0018,1201)	-

Table 95: *Neuro Perfusion*

Attribute Name	Tag	Value
Convolution Kernel	(0018,1210)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Patient Position	(0018,5100)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	new Series Instance UID
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	largest Series Number in the Study + 1
Acquisition Number	(0020,0012)	NPerfusionImageSet (A.1.8): value from the first image used to generate the computed image other: from the original images
Instance Number	(0020,0013)	NPerfusionImageSet (A.1.8): none other: from the original images Note: an Image Number will be assigned during storing to database In an empty result series image numbers start with one, are incremented by one, and are assigned to each image to store in the order of NPerfusionImageSet (A.1.8). If there are already images in a result series image number counting is continued. If there are more instances of a certain image type they are sorted according to their slice positions (from smallest slice position value to greatest).
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	value from the first image used to generate the computed image ??
Image Orientation (Patient)	(0020,0037)	value from the first image used to generate the computed image
Frame of Reference UID	(0020,0052)	<as in first original image>
Laterality	(0020,0060)	value from the first image used to generate the computed image
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-

Table 95: Neuro Perfusion

Attribute Name	Tag	Value
Slice Location	(0020,1041)	NPerfusionImageSet (A.1.8): average of the values from the images used to generate the computed image other: from the original images
Image Comments	(0020,4000)	NPerfusionImageSet (A.1.8): string as defined for the corresponding configuration item other: from the original images
Samples per Pixel	(0028,0002)	For gray scale representation: value from the first image used to generate the computed image For color representation: according to the photometric representation
Photometric Interpretation	(0028,0004)	For gray scale representation: "MONOCHROME2" For color representation: "RGB"
Planar Configuration	(0028,0006)	For color representation: according to the photometric representation For gray scale representation: n. a
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	value from the first image used to generate the computed image
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image
Bits Stored	(0028,0101)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image
High Bit	(0028,0102)	<ul style="list-style-type: none"> For color representation: according to the photometric representation For gray scale representation: value from the first image used to generate the computed image
Pixel Representation	(0028,0103)	For all images: 0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-

Table 95: *Neuro Perfusion*

Attribute Name	Tag	Value
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	-
Window Center	(0028,1050)	<ul style="list-style-type: none"> For color representation: 128 For gray scale representation: Window Center value at the point when the image is made persistent
Window Width	(0028,1051)	<ul style="list-style-type: none"> For color representation: 256 For gray scale representation: Window Width value at the point when the image is made persistent
Rescale Intercept	(0028,1052)	value from the first image used to generate the computed image
Rescale Slope	(0028,1053)	value from the first image used to generate the computed image
Window Center & Width Explanation	(0028,1055)	-
Pixel Padding Value	(0028,1020)	-
Red Palette Color Lookup Table Descriptor	(0028,1101)	-
Green Palette Color Lookup Table Descriptor	(0028,1102)	-
Blue Palette Color Lookup Table Descriptor	(0028,1103)	-
Red Palette Color Lookup Table Data	(0028,1201)	-
Green Palette Color Lookup Table Data	(0028,1202)	-
Blue Palette Color Lookup Table Data	(0028,1203)	-
Lossy Image Compression	(0028,2110)	Set to "01" in all result images if there is a value of "01" in at least one of the images used to generate the results. Otherwise omitted.
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
(various private data)	(0029,xxxx)	the application ROI(s) as syngo object oriented graphics (MEDCOM OOG)
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>

Table 95: Neuro Perfusion

Attribute Name	Tag	Value
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0060)	1/1
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	application ROI(s) as overlay pixel data
Pixel Data	(7FE0,0010)	values calculated as appropriate for the computed image

A.1.9 Osteo CT

Osteo CT will create CT result images (for SC result images see A.2). The following table provides information about image attributes created:

Table 96: *Osteo CT*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100
Image Type	(0008,0008)	"DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 OEVA"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>
Acquisition Date	(0008,0022)	-
Content Date	(0008,0023)	<date of content creation>
Acquisition Datetime	(0008,002A)	<from Original>
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	<from Original>
Content Time	(0008,0033)	<time of content creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	<from Original>
Manufacturer	(0008,0070)	<from Original>
Institution Name	(0008,0080)	<from Original>
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	<from Original>
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	<Contours + "Evaluation Number"> <Tables + "Evaluation Number"> <Summary + "Evaluation Number"> <(explicit)>

Table 96: Osteo CT

Attribute Name	Tag	Value
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	<from Original>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>

Table 96: *Osteo CT*

Attribute Name	Tag	Value
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	-
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus Administration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	-
Slice Thickness	(0018,0050)	<from Original>
Scan Options	(0018,0022)	-
KVP	(0018,0060)	<from Original>
Data Collection Diameter	(0018,0090)	<from Original>
Device Serial Number	(0018,1000)	<from Original>
Software Version(s)	(0018,1020)	-
Protocol Name	(0018,1030)	-
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	-

Table 96: Osteo CT

Attribute Name	Tag	Value
Distance Source to Detector	(0018,1110)	<from Original>
Distance Source to Patient	(0018,1111)	<from Original>
Gantry/Detector Tilt	(0018,1120)	<from Original>
Table Height	(0018,1130)	<from Original>
Rotation Direction	(0018,1140)	<from Original>
Exposure Time	(0018,1150)	<from Original>
X-Ray Tube Current	(0018,1151)	-
Exposure	(0018,1152)	<from Original>
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	-
Generator Power	(0018,1170)	<from Original>
Focal Spot	(0018,1190)	<from Original>
Date of last Calibration	(0018,1200)	<from Original>
Time of last Calibration	(0018,1201)	<from Original>
Convolution Kernel	(0018,1210)	<from Original>
Patient Position	(0018,5100)	<from Original>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<same series number for each examination>
Acquisition Number	(0020,0012)	<same series number for each examination>
Instance Number	(0020,0013)	<from Original>
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<from Original>
Image Orientation (Patient)	(0020,0037)	<from Original>
Frame of Reference UID	(0020,0052)	<new UID>
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	<from Original>
Image Comments	(0020,4000)	<from Original>
Samples per Pixel	(0028,0002)	<from Original>
Photometric Interpretation	(0028,0004)	<from Original>

Table 96: *Osteo CT*

Attribute Name	Tag	Value
Rows	(0028,0010)	<from Original>
Columns	(0028,0011)	<from Original>
Pixel Spacing	(0028,0030)	<calculated by system>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	<from UI and Configuration>
Window Width	(0028,1051)	<from UI and Configuration>
Rescale Intercept	(0028,1052)	<from Original>
Rescale Slope	(0028,1053)	<from Original>
Window Center & Width Explanation	(0028,1055)	"WINDOW1\WINDOW2"
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
(various private data)	(0029,xxxx)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>

Table 96: Osteo CT

Attribute Name	Tag	Value
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	Siemens MedCom Object Graphics
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<created by system>
Pixel Data	(7FE0,0010)	<as Original>

A.1.10 Pulmo CT

Pulmo CT will create CT result images. The following table provides information about image attributes created:

Table 97: Pulmo CT

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100

Table 97: Pulmo CT

Attribute Name	Tag	Value
Image Type	(0008,0008)	"DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 PEVI"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<yes>
Acquisition Date	(0008,0022)	<yes>
Content Date	(0008,0023)	<yes>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<yes>
Acquisition Time	(0008,0032)	<yes>
Content Time	(0008,0033)	<yes>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	CT
Manufacturer	(0008,0070)	SIEMENS
Institution Name	(0008,0080)	<yes>
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	<from Original>
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	"Colored Subranges" or "Colored Percentiles" or "Segment Images" or "Histograms" or "3D Prep"
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>

Table 97: Pulmo CT

Attribute Name	Tag	Value
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	<from Original>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	-
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>

Table 97: Pulmo CT

Attribute Name	Tag	Value
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	-
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus Administration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	-
Slice Thickness	(0018,0050)	<yes>
Scan Options	(0018,0022)	-
KVP	(0018,0060)	<yes>
Data Collection Diameter	(0018,0090)	<yes>
Device Serial Number	(0018,1000)	<yes>
Software Version(s)	(0018,1020)	-
Protocol Name	(0018,1030)	-
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	-
Distance Source to Detector	(0018,1110)	<yes>
Distance Source to Patient	(0018,1111)	<yes>
Gantry/Detector Tilt	(0018,1120)	<yes>
Table Height	(0018,1130)	<yes>

Table 97: Pulmo CT

Attribute Name	Tag	Value
Rotation Direction	(0018,1140)	<yes>
Exposure Time	(0018,1150)	<yes>
X-Ray Tube Current	(0018,1151)	-
Exposure	(0018,1152)	<yes>
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	<yes>
Generator Power	(0018,1170)	<yes>
Focal Spot	(0018,1190)	<yes>
Date of last Calibration	(0018,1200)	<yes>
Time of last Calibration	(0018,1201)	<yes>
Convolution Kernel	(0018,1210)	<yes>
Patient Position	(0018,5100)	<yes>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<yes>
Acquisition Number	(0020,0012)	<yes>
Instance Number	(0020,0013)	<yes>
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<yes>
Image Orientation (Patient)	(0020,0037)	<yes>
Frame of Reference UID	(0020,0052)	<yes>
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	-
Slice Location	(0020,1041)	<from Original>
Image Comments	(0020,4000)	<from Original>
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Spacing	(0028,0030)	<calculated by system>
Pixel Aspect Ratio	(0028,0034)	-

Table 97: Pulmo CT

Attribute Name	Tag	Value
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	<yes>
Window Width	(0028,1051)	<yes>
Rescale Intercept	(0028,1052)	<yes>
Rescale Slope	(0028,1053)	<yes>
Window Center & Width Explanation	(0028,1055)	<yes>
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-

Table 97: Pulmo CT

Attribute Name	Tag	Value
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	<yes>
Overlay Columns	(60xx,0011)	<yes>
Overlay Description	(60xx,0022)	<yes>
Overlay Subtype	(60xx,0045)	<yes>
Overlay Type	(60xx,0040)	<yes>
Overlay Origin	(60xx,0050)	<yes>
Overlay Bits Allocated	(60xx,0100)	<yes>
Overlay Bit Position	(60xx,0102)	<yes>
ROI Area	(60xx,1301)	<yes>
ROI Mean	(60xx,1302)	<yes>
ROI Standard Deviation	(60xx,1303)	<yes>
Overlay Label	(60xx,1500)	<yes>
Overlay Data	(60xx,3000)	<yes>
Pixel Data	(7FE0,0010)	<yes>

A.1.11 Vessel View

VesselView application will create CT result images (for SC result images see A.2). The following table provides information about image attributes created

Table 98: Vessel View Result Images - CT

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	from MWL
Image Type	(0008,0008)	"DERIVED/SECONDARY/AXIAL/CSA MPR" (MPRs) or "DERIVED/SECONDARY/AXIAL/CSA MIP" (MIPs) "DERIVED/SECONDARY/AXIAL/CSA MIP THIN" (thin MIPs) "DERIVED/SECONDARY/AXIAL/CSA MPR THICK" (thick MPRs)

Table 98: *Vessel View Result Images - CT*

Attribute Name	Tag	Value
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	(Date of Creation)
Acquisition Date	(0008,0022)	(Date of Exposure resulting in FIRST image of loaded series)
Content Date	(0008,0023)	(unknown)
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	(Time of Creation of Series Instance)
Acquisition Time	(0008,0032)	(Time of Exposure resulting in FIRST image of loaded series)
Content Time	(0008,0033)	(unknown)
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	from original
Manufacturer	(0008,0070)	“Siemens”
Institution Name	(0008,0080)	from original
Institution Address	(0008,0081)	from Site Configuration
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	Computer name
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	“[ORIG] MPR Collection” for MPRs “[ORIG] MIP Collection” for MIPs “[ORIG] MPR Thick Collection” for thick MPRs “[ORIG] MIP Thin Collection” for thin MIPs (where [ORIG] is the loaded series’ description)
Institutional Department Name	(0008,1040)	from Site Configuration
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>

Table 98: Vessel View Result Images - CT

Attribute Name	Tag	Value
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	"[Product Name] Vessel View"
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	(unknown)
> Referenced SOP Class UID	(0008,1150)	(unknown)
> Referenced SOP Instance UID	(0008,1155)	(unknown)
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	"MEDCOM RESAMPLED"
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>

Table 98: Vessel View Result Images - CT

Attribute Name	Tag	Value
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	(unknown)
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus Administration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	from original
Slice Thickness	(0018,0050)	For MPRs: the minimum slice distance of loaded series. For MIPs: - For thick MPRs and thinMIPs: actual thickness
Scan Options	(0018,0022)	(from first loaded image)
KVP	(0018,0060)	(from first loaded image)
Data Collection Diameter	(0018,0090)	-
Device Serial Number	(0018,1000)	-
Software Version(s)	(0018,1020)	from Configuration
Protocol Name	(0018,1030)	from original
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	-
Reconstruction Diameter	(0018,1100)	-
Distance Source to Detector	(0018,1110)	from original
Distance Source to Patient	(0018,1111)	from original
Gantry/Detector Tilt	(0018,1120)	from original

Table 98: *Vessel View Result Images - CT*

Attribute Name	Tag	Value
Table Height	(0018,1130)	from original
Rotation Direction	(0018,1140)	from original
Exposure Time	(0018,1150)	-
X-Ray Tube Current	(0018,1151)	-
Exposure	(0018,1152)	-
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	from original
Generator Power	(0018,1170)	from original
Focal Spot	(0018,1190)	from original
Date of last Calibration	(0018,1200)	-
Time of last Calibration	(0018,1201)	-
Convolution Kernel	(0018,1210)	from original
Patient Position	(0018,5100)	from original
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<created by system>
Acquisition Number	(0020,0012)	from original
Instance Number	(0020,0013)	(unknown)
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<calculated by system>
Image Orientation (Patient)	(0020,0037)	<calculated by system>
Frame of Reference UID	(0020,0052)	from original
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	from original
Slice Location	(0020,1041)	-
Image Comments	(0020,4000)	-
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	"MONOCHROME2"
Rows	(0028,0010)	from original
Columns	(0028,0011)	from original
Pixel Spacing	(0028,0030)	<calculated by system>

Table 98: *Vessel View Result Images - CT*

Attribute Name	Tag	Value
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	from original
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	0
Largest Pixel Value in Series	(0028,0109)	Modality dependent (4095 for CT)
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	Current setting when image saved
Window Width	(0028,1051)	Current setting when image saved
Rescale Intercept	(0028,1052)	Modality dependent, -1024 for CT data
Rescale Slope	(0028,1053)	1
Window Center & Width Explanation	(0028,1055)	“WINDOW1”
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
(various private data)	(0029,xxxx)	
Request Attributes Sequence	(0040,0275)	-
> Requested Procedure ID	(0040,1001)	-
> Scheduled Procedure Step ID	(0040,0009)	-
> Scheduled Procedure Step Description	(0040,0007)	-
> Scheduled Protocol Code Sequence	(0040,0008)	-
>> Code Sequence Macro		-
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-

Table 98: *Vessel View Result Images - CT*

Attribute Name	Tag	Value
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	(unknown)
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Pixel Data	(7FE0,0010)	<created by system>

A.1.12 Volume CT

Volume application will create CT result images (for SC result images see A.2). The following table provides information about image attributes created:

Table 99: *Volume CT, saved CT Images*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	<from original series or study>
Image Type	(0008,0008)	axial MIP or MinIP: "DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 MIP"; axial MPR: "DERIVED", "SECONDARY", "AXIAL", "CT_SOM5 MPR"; coronal/sagittal MPR: "DERIVED", "SECONDARY", "OTHER", "CT_SOM5 MPR"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>
Acquisition Date	(0008,0022)	<from original image>
Content Date	(0008,0023)	<date of instance creation>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	<from original image>

Table 99: *Volume CT, saved CT Images*

Attribute Name	Tag	Value
Content Time	(0008,0033)	<time of instance creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	“CT”
Manufacturer	(0008,0070)	<from original equipment>
Institution Name	(0008,0080)	<from original equipment>
Institution Address	(0008,0081)	<from original equipment>
Referring Physician’s Name	(0008,0090)	<from original study>
Station Name	(0008,1010)	<from original equipment>
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	“VolumeResult<i>” and “VolumeAxial<i>“, where <i> is an integer >= 1
Institutional Department Name	(0008,1040)	<from original equipment>
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	<from original series>
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	<from original series> + “meduser“
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	<from original equipment>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	<from original series>
> Referenced SOP Class UID	(0008,1150)	<from original series>
> Referenced SOP Instance UID	(0008,1155)	<from original series>
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-

Table 99: *Volume CT, saved CT Images*

Attribute Name	Tag	Value
Derivation Description	(0008,2111)	"Som5 Volume Resampled"
Source Image Sequence	(0008,2112)	<Reference to an original image>
> Referenced SOP Class UID	(0008,1150)	<Reference to an original image>
> Referenced SOP Instance UID	(0008,1155)	<Reference to an original image>
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Contrast/Bolus Agent	(0018,0010)	-
Contrast/Bolus Agent Sequence	(0018,0012)	-
> Code Sequence Macro		-
Contrast/Bolus Administration Route Sequence	(0018,0012)	-
> Code Sequence Macro		-
>Additional Drug Sequence	(0018,002A)	-
>> Code Sequence Macro		-
Body Part Examined	(0018,0015)	<from original series>
Slice Thickness	(0018,0050)	<from Volume configuration or UI>
Scan Options	(0018,0022)	<from original image>
KVP	(0018,0060)	<from original image>
Data Collection Diameter	(0018,0090)	<from original image>
Device Serial Number	(0018,1000)	<from original equipment>

Table 99: Volume CT, saved CT Images

Attribute Name	Tag	Value
Software Version(s)	(0018,1020)	<from original equipment>
Protocol Name	(0018,1030)	<from original series>
Contrast/Bolus Route	(0018,1040)	-
Contrast/Bolus Volume	(0018,1041)	-
Contrast/Bolus Start Time	(0018,1042)	-
Contrast/Bolus Stop Time	(0018,1043)	-
Contrast/Bolus Total Dose	(0018,1044)	-
Contrast Flow Rate(s)	(0018,1046)	-
Contrast Flow Duration(s)	(0018,1047)	-
Contrast/Bolus Ingredient	(0018,1048)	-
Contrast/Bolus Ingredient Concentration	(0018,1049)	-
Spatial Resolution	(0018,1050)	<from original equipment>
Reconstruction Diameter	(0018,1100)	<from original image>
Distance Source to Detector	(0018,1110)	<from original image>
Distance Source to Patient	(0018,1111)	<from original image>
Gantry/Detector Tilt	(0018,1120)	<from original image>
Table Height	(0018,1130)	<from original image>
Rotation Direction	(0018,1140)	<from original image>
Exposure Time	(0018,1150)	<from original image>
X-Ray Tube Current	(0018,1151)	<from original image>
Exposure	(0018,1152)	<from original image>
Exposure in μ As	(0018,1153)	-
Filter Type	(0018,1160)	<from original image>
Generator Power	(0018,1170)	<from original image>
Focal Spot	(0018,1190)	<from original image>
Date of last Calibration	(0018,1200)	<from original equipment>
Time of last Calibration	(0018,1201)	<from original equipment>
Convolution Kernel	(0018,1210)	<first value from original image>
Patient Position	(0018,5100)	<from original series>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<(highest available ID + 1)>

Table 99: *Volume CT, saved CT Images*

Attribute Name	Tag	Value
Acquisition Number	(0020,0012)	<from original image>
Instance Number	(0020,0013)	axial MIP/MPR: 1 coronal MPR: 2 sagittal MPR: 3 current axial image: 5
Patient Orientation	(0020,0020)	-
Image Position (Patient)	(0020,0032)	<calculated by application>
Image Orientation (Patient)	(0020,0037)	<calculated by application>
Frame of Reference UID	(0020,0052)	<from original series>
Laterality	(0020,0060)	<from original series>
Images in Acquisition	(0020,1002)	-
Position Reference Indicator	(0020,1040)	<from original series>
Slice Location	(0020,1041)	axial MIP/MPR: <calculated by application> coronal/sagittal MPR: -
Image Comments	(0020,4000)	<from original image, or null length if not available>
Samples per Pixel	(0028,0002)	<from original image>
Photometric Interpretation	(0028,0004)	<from original image>
Rows	(0028,0010)	<from original image>
Columns	(0028,0011)	<from original image>
Pixel Spacing	(0028,0030)	<from original image, or calculated by application>
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	<from original image>
Bits Stored	(0028,0101)	<from original image>
High Bit	(0028,0102)	<from original image>
Pixel Representation	(0028,0103)	<from original image>
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	<from original equipment>
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	<from current widow setting in UI>
Window Width	(0028,1051)	<from current widow setting in UI>

Table 99: Volume CT, saved CT Images

Attribute Name	Tag	Value
Rescale Intercept	(0028,1052)	<from original images>
Rescale Slope	(0028,1053)	<from original images>
Window Center & Width Explanation	(0028,1055)	“WINDOW1”
Lossy Image Compression	(0028,2110)	01 if original image was lossy compressed 00 otherwise
Lossy Image Compression Ratio	(0028,2112)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Requested Procedure Description	(0032,1060)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	<from original series>
Performed Procedure Step Start Date	(0040,0244)	<from original series>
Performed Procedure Step Start Time	(0040,0245)	<from original series>
Performed Procedure Step Description	(0040,0254)	<from original series>
Performed Protocol Code Sequence	(0040,0260)	<from original series>
> Code Sequence Macro		<from original series>
Comments on the Performed Procedure Step	(0040,0280)	<from original series>
Icon Image Sequence	(0088,0200)	(unknown) -
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	<image rows (normally 512)>
Overlay Columns	(60xx,0011)	<image columns (normally 512)>
Number of Frames in Overlay	(60xx,0015)	1
Overlay Description	(60xx,0022)	“Siemens MedCom Object Graphics“ or -
Overlay Type	(60xx,0040)	“G”
Overlay Subtype	(60xx,0045)	-

Table 99: Volume CT, saved CT Images

Attribute Name	Tag	Value
Origin	(60xx,0050)	“1”, “1”
Image Frame Origin	(60xx,0051)	“1”
Overlay Origin	(60xx,0060)	-
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<binary data>
Pixel Data	(7FE0,0010)	<binary data>

A.2 SC Standard Extended SOP Class

The application will create functional images from special applications. Those will be encoded as SC Standard extended SOP Class. Please see the following tables for a selected overview of supplied Standard and Private attributes.

A.2.1 Care Bolus

Care Bolus application will create SC result images. The following table provides information about image attributes created:

Table 100: Care Bolus

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	<as defined with Study>
Image Type	(0008,0008)	“DERIVED\SECONDARY\OTHER\CSA BLACK IMAGE”
Instance Creation Date	(0008,0012)	
Instance Creation Time	(0008,0013)	
Instance Creator UID	(0008,0014)	
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<yyyymmdd>

Table 100: Care Bolus

Attribute Name	Tag	Value
Acquisition Date	(0008,0022)	
Content Date	(0008,0023)	<yyyymmdd>
Acquisition Datetime	(0008,002A)	
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<hhmmss.xxxxxx>
Acquisition Time	(0008,0032)	
Content Time	(0008,0033)	<hhmmss.xxxxxx>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	CT
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	Siemens
Institution Name	(0008,0080)	
Institution Address	(0008,0081)	
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	Enhancement curve
Institutional Department Name	(0008,1040)	
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
Referenced Patient Sequence	(0008,1120)	<as Original>

Table 100: Care Bolus

Attribute Name	Tag	Value
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Derivation Description	(0008,2111)	
Source Image Sequence	(0008,2112)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	
Device Serial Number	(0018,1000)	
Secondary Capture Device ID	(0018,1010)	
Date of Secondary Capture	(0018,1012)	<yyyymmdd>
Time of Secondary Capture	(0018,1014)	<hhmmss.xxxxxx>
Secondary Capture Device Manufacturer	(0018,1016)	
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	

Table 100: Care Bolus

Attribute Name	Tag	Value
Secondary Capture Device Software Version	(0018,1019)	
Software Version(s)	(0018,1020)	
Video Image Format Acquired	(0018,1022)	
Digital Image Format Acquired	(0018,1023)	
Protocol Name	(0018,1030)	
Spatial Resolution	(0018,1050)	
Patient Position	(0018,5100)	
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	401
Acquisition Number	(0020,0012)	
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	-
Laterality	(0020,0060)	
Images in Acquisition	(0020,1002)	
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Aspect Ratio	(0028,0034)	
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	
Largest Image Pixel Value	(0028,0107)	
Smallest Pixel Value in Series	(0028,0108)	
Largest Pixel Value in Series	(0028,0109)	
Pixel Padding Value	(0028,0120)	
Quality Control Image	(0028,0300)	
Burned In Annotation	(0028,0301)	

Table 100: Care Bolus

Attribute Name	Tag	Value
Window Center	(0028,1050)	
Window Width	(0028,1051)	
Rescale Intercept	(0028,1052)	
Rescale Slope	(0028,1053)	
Rescale Type	(0028,1054)	
Window Center & Width Explanation	(0028,1055)	
Lossy Image Compression	(0028,2110)	
Lossy Image Compression Ratio	(0028,2112)	
Modality LUT Sequence	(0028,3000)	
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
>Modality LUT Type	(0028,3004)	
> LUT Data	(0028,3006)	
VOI LUT Sequence	(0028,3010)	
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
> LUT Data	(0028,3006)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	
Performed Procedure Step Start Date	(0040,0244)	
Performed Procedure Step Start Time	(0040,0245)	
Performed Procedure Step Description	(0040,0254)	
Performed Protocol Code Sequence	(0040,0260)	
> Code Sequence Macro		
Comments on the Performed Procedure Step	(0040,0280)	
Icon Image Sequence	(0088,0200)	
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	

Table 100: *Care Bolus*

Attribute Name	Tag	Value
Overlay Rows	(60xx,0010)	
Overlay Columns	(60xx,0011)	
Overlay Description	(60xx,0022)	
Overlay Subtype	(60xx,0045)	
Overlay Type	(60xx,0040)	
Overlay Origin	(60xx,0060)	
Overlay Bits Allocated	(60xx,0100)	
Overlay Bit Position	(60xx,0102)	
ROI Area	(60xx,1301)	
ROI Mean	(60xx,1302)	
ROI Standard Deviation	(60xx,1303)	
Overlay Label	(60xx,1500)	
Overlay Data	(60xx,3000)	
Pixel Data	(7FE0,0010)	

A.2.2 DynEva

DynEva application will create SC result images (for CT result images see A.1). The following table provides information about image attributes created:

Table 101: *DynEva created SC Images*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100
Image Type	(0008,0008)	"DERIVED", "SECONDARY", "OTHER", "CSA BLACK IMAGE"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	date of series creation
Acquisition Date	(0008,0022)	-
Content Date	(0008,0023)	date of content creation

Table 101: *DynEva created SC Images*

Attribute Name	Tag	Value
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	time of series creation
Acquisition Time	(0008,0032)	-
Content Time	(0008,0033)	time of content creation
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	CT
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	Siemens
Institution Name	(0008,0080)	(taken from the local config)
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	name of computer
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	"DynEva Curves+<Examination Number>", "DynEva Parameters+<Examination Number>"
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	from original
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	from original
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>

Table 101: DynEva created SC Images

Attribute Name	Tag	Value
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	Som5 DynEva Resampled
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Private Creator	(0009,00xx)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	(source unknown)
Device Serial Number	(0018,1000)	taken from the local config
Secondary Capture Device ID	(0018,1010)	-
Date of Secondary Capture	(0018,1012)	date of SC creation
Time of Secondary Capture	(0018,1014)	time of SC creation
Secondary Capture Device Manufacturer	(0018,1016)	-
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	-

Table 101: *DynEva created SC Images*

Attribute Name	Tag	Value
Secondary Capture Device Software Version	(0018,1019)	-
Software Version(s)	(0018,1020)	set to the current version (source unknown)
Video Image Format Acquired	(0018,1022)	-
Digital Image Format Acquired	(0018,1023)	-
Protocol Name	(0018,1030)	protocolname of the current series
Spatial Resolution	(0018,1050)	-
Patient Position	(0018,5100)	position of the patient
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<highest series number + 1>
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	1 (source unknown)
Patient Orientation	(0020,0020)	created by application
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Image Comments	(0020,4000)	-
Private Creator	(0021,00xx)	-
Target	(0021,xx11)	-
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-

Table 101: DynEva created SC Images

Attribute Name	Tag	Value
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	-
Window Width	(0028,1051)	-
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	“WINDOW1”
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Pixel Padding Value	(0028,1020)	-
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-

Table 101: *DynEva created SC Images*

Attribute Name	Tag	Value
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	-
Overlay Columns	(60xx,0011)	-
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	-
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	-
Overlay Bit Position	(60xx,0102)	-
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	-
Pixel Data	(7FE0,0010)	binary (524288 bytes)

A.2.3 InSpace

InSpace application will create SC result images. The following table provides information about image attributes created:

Table 102: *InSpace*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	“DERIVED\SECONDARY\OTHER\CSA 3DPROJECTION” or “DERIVED\SECONDARY\OTHER\ CSA BOOKMARK\RT3D CONFIG”
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new UID>

Table 102: InSpace

Attribute Name	Tag	Value
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	-
Content Date	(0008,0023)	<yyyymmdd>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<hhmmss>
Acquisition Time	(0008,0032)	-
Content Time	(0008,0033)	<hhmmss>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	CT or OT
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	"HipGraphics"
Institution Name	(0008,0080)	from Configuration
Institution Address	(0008,0081)	from Configuration
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	from WS Configuration
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	created
Institutional Department Name	(0008,1040)	from Original
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	(input only via "Correct")
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	from Original or InSpace
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-

Table 102: InSpace

Attribute Name	Tag	Value
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	"MEDCOM RESAMPLED" or "INSPACE RECORD"
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	-
Device Serial Number	(0018,1000)	from Configuration
Secondary Capture Device ID	(0018,1010)	from Configuration
Date of Secondary Capture	(0018,1012)	<yyyymmdd>
Time of Secondary Capture	(0018,1014)	<hhmmss>
Secondary Capture Device Manufacturer	(0018,1016)	"HipGraphics"

Table 102: InSpace

Attribute Name	Tag	Value
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	"InSpace Postprocessing"
Secondary Capture Device Software Version	(0018,1019)	created
Software Version(s)	(0018,1020)	from WS Configuration
Video Image Format Acquired	(0018,1022)	-
Digital Image Format Acquired	(0018,1023)	-
Protocol Name	(0018,1030)	-
Spatial Resolution	(0018,1050)	-
Patient Position	(0018,5100)	-
Private Creator	(0019,00xx)	-
Feed per Rotation	(0019,xxB0)	-
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new Uid>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	from Original
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	from Original
Patient Orientation	(0020,0020)	
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Image Comments	(0020,4000)	
Private Creator	(0021,00xx)	-
Target	(0021,xx11)	-
Samples per Pixel	(0028,0002)	3
Photometric Interpretation	(0028,0004)	RGB
Rows	(0028,0010)	
Columns	(0028,0011)	
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	8
Bits Stored	(0028,0101)	8
High Bit	(0028,0102)	7
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-

Table 102: InSpace

Attribute Name	Tag	Value
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	from Original
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	-
Window Width	(0028,1051)	-
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	-
Red Palette Color Lookup Table Descriptor	(0028,1101)	-
Green Palette Color Lookup Table Descriptor	(0028,1102)	-
Blue Palette Color Lookup Table Descriptor	(0028,1103)	-
Red Palette Color Lookup Table Data	(0028,1201)	-
Green Palette Color Lookup Table Data	(0028,1202)	-
Blue Palette Color Lookup Table Data	(0028,1203)	-
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Private information	(0029,xxxx)	
Request Attributes Sequence	(0040,0275)	<as Original> (not for Bookmark images)
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>

Table 102: InSpace

Attribute Name	Tag	Value
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	-
Overlay Columns	(60xx,0011)	-
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	-
Overlay Type	(60xx,0040)	-
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	-
Overlay Bit Position	(60xx,0102)	-
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	-
Pixel Data	(7FE0,0010)	

A.2.4 Lung Care Result

Lung Care will create SC result images (for CT result images see A.1). They are not intended for viewing but for reporting purposes - and they can be stored/transferred via DICOM. The following table provides information about image attributes created:

Table 103: CT LungCARE - Result

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	<yes>
Image Type	(0008,0008)	“DERIVED\SECONDARY\OTHER\MPR” or “DERIVED\SECONDARY\OTHER\MIP” or “DERIVED\SECONDARY\OTHER\PVRT”
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new Uid>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	-
Acquisition Date	(0008,0022)	<yes>
Content Date	(0008,0023)	<yes>
Acquisition Datetime	(0008,002A)	
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	-
Acquisition Time	(0008,0032)	<yes>
Content Time	(0008,0033)	<yes>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	“SC”
Conversion Type	(0008,0064)	
Manufacturer	(0008,0070)	“Siemens Med CT”
Institution Name	(0008,0080)	<yes>
Institution Address	(0008,0081)	-
Referring Physician’s Name	(0008,0090)	
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>

Table 103: *CT LungCARE - Result*

Attribute Name	Tag	Value
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	e.g. "SCREENING #1_report" or "SCREENING #1_result_1_3_SPI" or "SCREENING #1_result_1_4_MPR"
Institutional Department Name	(0008,1040)	
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	<yes>
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	<yes>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Derivation Description	(0008,2111)	
Source Image Sequence	(0008,2112)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>

Table 103: CT LungCARE - Result

Attribute Name	Tag	Value
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	
Device Serial Number	(0018,1000)	
Secondary Capture Device ID	(0018,1010)	
Date of Secondary Capture	(0018,1012)	
Time of Secondary Capture	(0018,1014)	
Secondary Capture Device Manufacturer	(0018,1016)	
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	
Secondary Capture Device Software Version	(0018,1019)	
Software Version(s)	(0018,1020)	<yes>
Video Image Format Acquired	(0018,1022)	
Digital Image Format Acquired	(0018,1023)	
Protocol Name	(0018,1030)	
Spatial Resolution	(0018,1050)	
Patient Position	(0018,5100)	
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UId>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<yes>
Acquisition Number	(0020,0012)	
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	

Table 103: CT LungCARE - Result

Attribute Name	Tag	Value
Laterality	(0020,0060)	
Images in Acquisition	(0020,1002)	
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1 or 3
Photometric Interpretation	(0028,0004)	“MONOCHROME2” or “RGB”
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16 or 8
Bits Stored	(0028,0101)	12 or 8
High Bit	(0028,0102)	11 or 7
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	-400\50
Window Width	(0028,1051)	1200\400
Rescale Intercept	(0028,1052)	- or -1024
Rescale Slope	(0028,1053)	- or 1
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	WINDOW1\WINDOW2
Lossy Image Compression	(0028,2110)	
Lossy Image Compression Ratio	(0028,2112)	
Modality LUT Sequence	(0028,3000)	
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
>Modality LUT Type	(0028,3004)	
> LUT Data	(0028,3006)	
VOI LUT Sequence	(0028,3010)	

Table 103: CT LungCARE - Result

Attribute Name	Tag	Value
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
> LUT Data	(0028,3006)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	
Performed Procedure Step Start Date	(0040,0244)	
Performed Procedure Step Start Time	(0040,0245)	
Performed Procedure Step Description	(0040,0254)	
Performed Protocol Code Sequence	(0040,0260)	
> Code Sequence Macro		
Comments on the Performed Procedure Step	(0040,0280)	
Icon Image Sequence	(0088,0200)	
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	
Overlay Rows	(60xx,0010)	
Overlay Columns	(60xx,0011)	
Overlay Description	(60xx,0022)	
Overlay Subtype	(60xx,0045)	
Overlay Type	(60xx,0040)	
Overlay Origin	(60xx,0060)	
Overlay Bits Allocated	(60xx,0100)	
Overlay Bit Position	(60xx,0102)	
ROI Area	(60xx,1301)	
ROI Mean	(60xx,1302)	
ROI Standard Deviation	(60xx,1303)	
Overlay Label	(60xx,1500)	
Overlay Data	(60xx,3000)	
Pixel Data	(7FE0,0010)	<yes>

A.2.5 Lung Care Report

Lung Care will create SC result images (for CT result images see A.1). They are not intended for viewing but for reporting purposes - and they can be stored/transferred via DICOM. The following table provides information about image attributes created:

Table 104: CT LungCARE - Report

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	<yes>
Image Type	(0008,0008)	"DERIVED\SECONDARY\OTHER\REPORT" Type 5: "IN_WORK" or "FINISHED"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	-
Acquisition Date	(0008,0022)	<yes>
Content Date	(0008,0023)	<yes>
Acquisition Datetime	(0008,002A)	
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	-
Acquisition Time	(0008,0032)	<yes>
Content Time	(0008,0033)	<yes>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	"SC"
Conversion Type	(0008,0064)	
Manufacturer	(0008,0070)	"Siemens Med CT"
Institution Name	(0008,0080)	<yes>
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	e.g. "SCREENING #1_report"

Table 104: CT LungCARE - Report

Attribute Name	Tag	Value
Institutional Department Name	(0008,1040)	
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	<yes>
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	<yes>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Derivation Description	(0008,2111)	
Source Image Sequence	(0008,2112)	
> Referenced SOP Class UID	(0008,1150)	
> Referenced SOP Instance UID	(0008,1155)	
> Referenced Frame Number	(0008,1160)	
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>

Table 104: CT LungCARE - Report

Attribute Name	Tag	Value
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	
Device Serial Number	(0018,1000)	
Secondary Capture Device ID	(0018,1010)	
Date of Secondary Capture	(0018,1012)	
Time of Secondary Capture	(0018,1014)	
Secondary Capture Device Manufacturer	(0018,1016)	
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	
Secondary Capture Device Software Version	(0018,1019)	
Software Version(s)	(0018,1020)	<yes>
Video Image Format Acquired	(0018,1022)	
Digital Image Format Acquired	(0018,1023)	
Protocol Name	(0018,1030)	
Spatial Resolution	(0018,1050)	
Patient Position	(0018,5100)	-
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UId>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<yes>
Acquisition Number	(0020,0012)	
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	-
Laterality	(0020,0060)	
Images in Acquisition	(0020,1002)	
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	3
Photometric Interpretation	(0028,0004)	"RGB"

Table 104: CT LungCARE - Report

Attribute Name	Tag	Value
Rows	(0028,0010)	64
Columns	(0028,0011)	64
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0300)	-
Window Center	(0028,1050)	100
Window Width	(0028,1051)	100
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	-
Pixel Padding Value	(0028,1020)	
Lossy Image Compression	(0028,2110)	
Lossy Image Compression Ratio	(0028,2112)	
Modality LUT Sequence	(0028,3000)	
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
>Modality LUT Type	(0028,3004)	
> LUT Data	(0028,3006)	
VOI LUT Sequence	(0028,3010)	
> LUT Descriptor	(0028,3002)	
> LUT Explanation	(0028,3003)	
> LUT Data	(0028,3006)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>

Table 104: *CT LungCARE - Report*

Attribute Name	Tag	Value
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	
Performed Procedure Step Start Date	(0040,0244)	
Performed Procedure Step Start Time	(0040,0245)	
Performed Procedure Step Description	(0040,0254)	
Performed Protocol Code Sequence	(0040,0260)	
> Code Sequence Macro		
Comments on the Performed Procedure Step	(0040,0280)	
Icon Image Sequence	(0088,0200)	
> Image Pixel Module		
Presentation LUT Shape	(2050,0020)	
Pixel Data	(7FE0,0010)	<yes>

A.2.6 Osteo

Osteo will create SC result images (for CT result images see A.1). The following table provides information about image attributes created:

Table 105: *Osteo - SC Image*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	ISO_IR 100
Image Type	(0008,0008)	"DERIVED", "SECONDARY", "OTHER", "CSA BLACK IMAGE"
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new Uid>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<Date of series creation>
Acquisition Date	(0008,0022)	-

Table 105: Osteo - SC Image

Attribute Name	Tag	Value
Content Date	(0008,0023)	<Date of image creation>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<Time of series creation>
Acquisition Time	(0008,0032)	-
Content Time	(0008,0033)	<Time of image creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	CT
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	SIEMENS
Institution Name	(0008,0080)	-
Institution Address	(0008,0081)	-
Referring Physician's Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	-
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	< one of: Contours, Tables, Summary>
Institutional Department Name	(0008,1040)	-
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians' Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator's Name	(0008,1070)	-
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	-
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>

Table 105: Osteo - SC Image

Attribute Name	Tag	Value
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	-
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	-
Device Serial Number	(0018,1000)	-
Secondary Capture Device ID	(0018,1010)	-
Date of Secondary Capture	(0018,1012)	<Date of instance creation>
Time of Secondary Capture	(0018,1014)	<Time of instance creation>
Secondary Capture Device Manufacturer	(0018,1016)	-
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	-
Secondary Capture Device Software Version	(0018,1019)	-

Table 105: Osteo - SC Image

Attribute Name	Tag	Value
Software Version(s)	(0018,1020)	-
Video Image Format Acquired	(0018,1022)	-
Digital Image Format Acquired	(0018,1023)	-
Protocol Name	(0018,1030)	-
Spatial Resolution	(0018,1050)	-
Patient Position	(0018,5100)	-
Private Creator	(0019,00xx)	-
Feed per Rotation	(0019,xxB0)	-
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new Uid>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<last existing series + 1>
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	-
Patient Orientation	(0020,0020)	-
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Image Comments	(0020,4000)	-
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	512
Columns	(0028,0011)	512
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-

Table 105: *Osteo - SC Image*

Attribute Name	Tag	Value
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	-
Window Width	(0028,1051)	-
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	-
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	-
> Image Pixel Module		-

Table 105: Osteo - SC Image

Attribute Name	Tag	Value
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	<yes>
Overlay Columns	(60xx,0011)	<yes>
Overlay Description	(60xx,0022)	-
Overlay Subtype	(60xx,0045)	<yes>
Overlay Type	(60xx,0040)	<yes>
Overlay Origin	(60xx,0050)	<yes>
Overlay Bits Allocated	(60xx,0100)	<yes>
Overlay Bit Position	(60xx,0102)	<yes>
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<yes>
Pixel Data	(7FE0,0010)	<created by system>

A.2.7 Vessel View

VesselView application will create SC result images (for CT result images see A.1). The following table provides information about image attributes created:

Table 106: VesselView - SC result image

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	"ISO_IR 100"
Image Type	(0008,0008)	"DERIVED/SECONDARY/OTHER/CSA RIBBON/CSA MPR CURVED" (VN images) or "DERIVED/SECONDARY/OTHER/CSA VRT/VVMANIPULATED" (VRTs) or "DERIVED/SECONDARY/MPR/CSA MPR" (axial cuts) or "DERIVED/SECONDARY/OTHER/CSA BLACK IMAGE" (reports)
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7

Table 106: *VesselView - SC result image*

Attribute Name	Tag	Value
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>
Acquisition Date	(0008,0022)	(Date of Exposure resulting in FIRST image of loaded series)
Content Date	(0008,0023)	(unknown)
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	(Time of Exposure resulting in FIRST image of loaded series)
Content Time	(0008,0033)	<time of instance creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	from original
Conversion Type	(0008,0064)	“WSD”
Manufacturer	(0008,0070)	Siemens
Institution Name	(0008,0080)	<from original equipment>
Institution Address	(0008,0081)	(from Site Configuration)
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	Computer name
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	“[ORIG] RENDERINGS Collection” for VRT and VN or “[ORIG] REPORTS Collection” for reports or “[ORIG] ANGIOMPRS Collection” for axial cuts (where [ORIG] is the loaded series’ description)
Institutional Department Name	(0008,1040)	<from configuration>
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	-
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	“meduser“
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer’s Model Name	(0008,1090)	“[Product Name] Vessel View”

Table 106: *VesselView - SC result image*

Attribute Name	Tag	Value
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	(unknown)
> Referenced SOP Class UID	(0008,1150)	(unknown)
> Referenced SOP Instance UID	(0008,1155)	(unknown)
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	"MEDCOM RESAMPLED"
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	<from original series>

Table 106: *VesselView - SC result image*

Attribute Name	Tag	Value
Device Serial Number	(0018,1000)	-
Secondary Capture Device ID	(0018,1010)	Computer name
Date of Secondary Capture	(0018,1012)	First loaded image's acquisition date
Time of Secondary Capture	(0018,1014)	First loaded image's acquisition time
Secondary Capture Device Manufacturer	(0018,1016)	Siemens
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	[Product Name] Vessel View
Secondary Capture Device Software Version	(0018,1019)	[Product Version] (e.g "syngo CT 2005A-W")
Software Version(s)	(0018,1020)	From configuration
Video Image Format Acquired	(0018,1022)	-
Digital Image Format Acquired	(0018,1023)	-
Protocol Name	(0018,1030)	<from original series>
Spatial Resolution	(0018,1050)	-
Date of Last Calibration	(0018,1200)	
Time of Last Calibration	(0018,1201)	
Patient Position	(0018,5100)	<from original series>
Private Creator	(0019,00xx)	-
Feed per Rotation	(0019,xxB0)	-
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<created by system>
Acquisition Number	(0020,0012)	from original
Instance Number	(0020,0013)	(unknown)
Patient Orientation	(0020,0020)	Orientation of image for VRT and VN, else -
Laterality	(0020,0060)	-
Images in Acquisition	(0020,1002)	-
Image Comments	(0020,4000)	-
Samples per Pixel	(0028,0002)	3 for VN and VRT (color images) 1 for axial cuts (b/w images) and reports (black images)
Photometric Interpretation	(0028,0004)	"RGB" for VN and VRT "MONOCHROME2" for axial cuts and reports

Table 106: *VesselView - SC result image*

Attribute Name	Tag	Value
Rows	(0028,0010)	512 for VRT depending on ribbon size for VN 512 for reports (black images) 256 for axial cuts
Columns	(0028,0011)	512 for VRT depending on ribbon size for VN 512 for reports (black images) 256 for axial cuts
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16 for axial cuts and reports 8 for VN and VRT
Bits Stored	(0028,0101)	12 for axial cuts and reports 8 for VN and VRT
High Bit	(0028,0102)	11 for axial cuts and reports 7 for VN and VRT
Pixel Representation	(0028,0103)	from original
Smallest Image Pixel Value	(0028,0106)	“0” for reports, - otherwise
Largest Image Pixel Value	(0028,0107)	“0” for reports, - otherwise
Smallest Pixel Value in Series	(0028,0108)	0
Largest Pixel Value in Series	(0028,0109)	Modality dependent (4095 for CT) for reports and axial cuts 0 for VN and VRT
Pixel Padding Value	(0028,0120)	-
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	Current setting when image saved (for VN and axial cuts), 100 (for VRT and reports)
Window Width	(0028,1051)	Current setting when image saved (for VN and axial cuts), 100 (for VRT and reports)
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	-
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-

Table 106: *VesselView - SC result image*

Attribute Name	Tag	Value
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Requested Procedure Description	(0032,1060)	
Request Attributes Sequence	(0040,0275)	-
> Requested Procedure ID	(0040,1001)	-
> Scheduled Procedure Step ID	(0040,0009)	-
> Scheduled Procedure Step Description	(0040,0007)	-
> Scheduled Protocol Code Sequence	(0040,0008)	-
>> Code Sequence Macro		-
Performed Procedure Step ID	(0040,0253)	-
Performed Procedure Step Start Date	(0040,0244)	-
Performed Procedure Step Start Time	(0040,0245)	-
Performed Procedure Step Description	(0040,0254)	-
Performed Protocol Code Sequence	(0040,0260)	-
> Code Sequence Macro		-
Comments on the Performed Procedure Step	(0040,0280)	-
Icon Image Sequence	(0088,0200)	(unknown) -
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Pixel Data	(7FE0,0010)	<binary data>

A.2.8 Volume CT

Volume application will create SC result images (for CT result images see A.1). The following table provides information about image attributes created:

Table 107: *Volume CT, Result Image (CSA BLACK IMAGE)*

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	"ISO_IR 100"

Table 107: Volume CT, Result Image (CSA BLACK IMAGE)

Attribute Name	Tag	Value
Image Type	(0008,0008)	“DERIVED”, “SECONDARY”, “OTHER”, “CSA BLACK IMAGE”
Instance Creation Date	(0008,0012)	-
Instance Creation Time	(0008,0013)	-
Instance Creator UID	(0008,0014)	-
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	<new UID>
Study Date	(0008,0020)	<as Original>
Series Date	(0008,0021)	<date of series creation>
Acquisition Date	(0008,0022)	-
Content Date	(0008,0023)	<date of instance creation>
Acquisition Datetime	(0008,002A)	-
Study Time	(0008,0030)	<as Original>
Series Time	(0008,0031)	<time of series creation>
Acquisition Time	(0008,0032)	-
Content Time	(0008,0033)	<time of instance creation>
Accession Number	(0008,0050)	<as Original>
Modality	(0008,0060)	“CT”
Conversion Type	(0008,0064)	“WSD”
Manufacturer	(0008,0070)	<from original equipment>
Institution Name	(0008,0080)	<from original equipment>
Institution Address	(0008,0081)	<from original equipment>
Referring Physician’s Name	(0008,0090)	<as Original>
Station Name	(0008,1010)	<from original equipment>
Study Description	(0008,1030)	<as Original>
Procedure Code Sequence	(0008,1032)	<as Original>
> (Code Sequence Macro)		<as Original>
Series Description	(0008,103E)	“VolumeResult<i>”, where <i> is an integer >= 1
Institutional Department Name	(0008,1040)	<from original equipment>
Physician(s) of Record	(0008,1048)	<as Original>
Performing Physicians’ Name	(0008,1050)	<from original series>
Name of Physician(s) Reading Study	(0008,1060)	<as Original>
Operator’s Name	(0008,1070)	<from original series> + “meduser“

Table 107: Volume CT, Result Image (CSA BLACK IMAGE)

Attribute Name	Tag	Value
Admitting Diagnoses Description	(0008,1080)	<as Original>
Manufacturer's Model Name	(0008,1090)	<from original equipment>
Referenced Study Sequence	(0008,1110)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Study Component Sequence	(0008,1111)	<from original series>
> Referenced SOP Class UID	(0008,1150)	<from original series>
> Referenced SOP Instance UID	(0008,1155)	<from original series>
Referenced Patient Sequence	(0008,1120)	<as Original>
> Referenced SOP Class UID	(0008,1150)	<as Original>
> Referenced SOP Instance UID	(0008,1155)	<as Original>
Referenced Image Sequence	(0008,1140)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Derivation Description	(0008,2111)	-
Source Image Sequence	(0008,2112)	-
> Referenced SOP Class UID	(0008,1150)	-
> Referenced SOP Instance UID	(0008,1155)	-
> Referenced Frame Number	(0008,1160)	-
Private Creator	(0009,00xx)	-
Patient's Name	(0010,0010)	<as Original>
Patient ID	(0010,0020)	<as Original>
Patient's Birth Date	(0010,0030)	<as Original>
Patient's Birth Time	(0010,0032)	<as Original>
Patient's Sex	(0010,0040)	<as Original>
Other Patient IDs	(0010,1000)	<as Original>
Other Patient Names	(0010,1001)	<as Original>
Patient's Age	(0010,1010)	<as Original>
Patient's Size	(0010,1020)	<as Original>
Patient's Weight	(0010,1030)	<as Original>
Ethnic Group	(0010,2160)	<as Original>
Occupation	(0010,2180)	<as Original>

Table 107: Volume CT, Result Image (CSA BLACK IMAGE)

Attribute Name	Tag	Value
Additional Patient's History	(0010,21B0)	<as Original>
Patient Comments	(0010,4000)	<as Original>
Body Part Examined	(0018,0015)	<from original series>
Device Serial Number	(0018,1000)	<from original equipment>
Secondary Capture Device ID	(0018,1010)	-
Date of Secondary Capture	(0018,1012)	<date of instance creation> ?
Time of Secondary Capture	(0018,1014)	<date of instance creation> ?
Secondary Capture Device Manufacturer	(0018,1016)	-
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	-
Secondary Capture Device Software Version	(0018,1019)	-
Software Version(s)	(0018,1020)	<from original equipment>
Video Image Format Acquired	(0018,1022)	-
Digital Image Format Acquired	(0018,1023)	-
Protocol Name	(0018,1030)	<from original series>
Spatial Resolution	(0018,1050)	<from original equipment>
Date of Last Calibration	(0018,1200)	<from original equipment>
Time of Last Calibration	(0018,1201)	<from original equipment>
Patient Position	(0018,5100)	<from original series>
Study Instance UID	(0020,000D)	<as Original>
Series Instance UID	(0020,000E)	<new UID>
Study ID	(0020,0010)	<as Original>
Series Number	(0020,0011)	<(highest available ID + 1)>
Acquisition Number	(0020,0012)	-
Instance Number	(0020,0013)	4
Patient Orientation	(0020,0020)	(null length)
Laterality	(0020,0060)	<from original series>
Images in Acquisition	(0020,1002)	-
Image Comments	(0020,4000)	-
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	512
Columns	(0028,0011)	512

Table 107: Volume CT, Result Image (CSA BLACK IMAGE)

Attribute Name	Tag	Value
Pixel Aspect Ratio	(0028,0034)	-
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	-
Largest Image Pixel Value	(0028,0107)	-
Smallest Pixel Value in Series	(0028,0108)	-
Largest Pixel Value in Series	(0028,0109)	-
Pixel Padding Value	(0028,0120)	<from original equipment>
Quality Control Image	(0028,0300)	-
Burned In Annotation	(0028,0301)	-
Window Center	(0028,1050)	-
Window Width	(0028,1051)	-
Rescale Intercept	(0028,1052)	-
Rescale Slope	(0028,1053)	-
Rescale Type	(0028,1054)	-
Window Center & Width Explanation	(0028,1055)	“WINDOW1“
Lossy Image Compression	(0028,2110)	-
Lossy Image Compression Ratio	(0028,2112)	-
Modality LUT Sequence	(0028,3000)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
>Modality LUT Type	(0028,3004)	-
> LUT Data	(0028,3006)	-
VOI LUT Sequence	(0028,3010)	-
> LUT Descriptor	(0028,3002)	-
> LUT Explanation	(0028,3003)	-
> LUT Data	(0028,3006)	-
Requested Procedure Description	(0032,1060)	
Request Attributes Sequence	(0040,0275)	<as Original>
> Requested Procedure ID	(0040,1001)	<as Original>
> Scheduled Procedure Step ID	(0040,0009)	<as Original>

Table 107: Volume CT, Result Image (CSA BLACK IMAGE)

Attribute Name	Tag	Value
> Scheduled Procedure Step Description	(0040,0007)	<as Original>
> Scheduled Protocol Code Sequence	(0040,0008)	<as Original>
>> Code Sequence Macro		<as Original>
Performed Procedure Step ID	(0040,0253)	<from original series>
Performed Procedure Step Start Date	(0040,0244)	<from original series>
Performed Procedure Step Start Time	(0040,0245)	<from original series>
Performed Procedure Step Description	(0040,0254)	<from original series>
Performed Protocol Code Sequence	(0040,0260)	<from original series>
> Code Sequence Macro		<from original series>
Comments on the Performed Procedure Step	(0040,0280)	<from original series>
Icon Image Sequence	(0088,0200)	(unknown) -
> Image Pixel Module		-
Presentation LUT Shape	(2050,0020)	-
Overlay Rows	(60xx,0010)	512
Overlay Columns	(60xx,0011)	512
Number of Frames in Overlay	(60xx,0015)	1
Overlay Description	(60xx,0022)	“Siemens MedCom Object Graphics“
Overlay Type	(60xx,0040)	“G”
Overlay Subtype	(60xx,0045)	-
Origin	(60xx,0050)	“1”, “1”
Image Frame Origin	(60xx,0051)	“1”
Overlay Origin	(60xx,0050)	-
Overlay Bits Allocated	(60xx,0100)	1
Overlay Bit Position	(60xx,0102)	0
ROI Area	(60xx,1301)	-
ROI Mean	(60xx,1302)	-
ROI Standard Deviation	(60xx,1303)	-
Overlay Label	(60xx,1500)	-
Overlay Data	(60xx,3000)	<binary data>
Pixel Data	(7FE0,0010)	<binary data>

Index

B

Basic Color Print Management 81
 Basic Worklist 102
 Body Part Examined 131, 140

C

Case Sensitive 60
 C-ECHO 16, 26, 27, 35
 C-FIND 21, 23, 50, 51, 58, 59, 60, 103,
 104, 111, 112
 C-FIND-CANCEL 58
 C-FIND-RQ 168
 C-FIND-RSP 168
 C-GET 21, 49, 58, 71, 72
 C-GET-CANCEL 58
 C-MOVE 21, 49, 50, 56, 57, 58, 59, 74,
 75
 C-MOVE-CANCEL 58
 Color Images 35, 41
 Color Print Management 77
 Configuration 166, 194
 C-STORE 16, 21, 30, 35, 56, 57, 71, 72,
 74, 75, 158
 C-STORE-RQ 39

D

Data Flow 15, 18, 172
 Display 40

E

Extended Character Set 195

Extended Character Sets 170
 Extended Negotiation 51, 57, 60, 72, 74

F

Film Box 77, 81, 83, 84, 85
 Film Session 77, 81, 82, 83

G

Graphic overlay 34, 40
 Grayscale Images 34, 40, 86
 Grayscale Print Management 77, 81

I

Image Box 77, 83, 84, 85, 86

M

Match 48
 MOD LUT SQ 41
 Modality Worklist 168
 MONOCHROME1 34, 40, 41
 MONOCHROME2 34, 40, 41, 190

N

N_EVENT_REPORT 88
 N-ACTION 83
 N-CREATE 81, 83, 115
 N-DELETE 82, 83
 N-SET 115

O

Organ Characteristic **140**
Overlay plane . . . **34, 35, 40, 41, 158**

P

PALETTE COLOR **35, 42**
Performed Procedure Step **25**
Pixel plane **34, 41**
Presentation LUT **77**
Print Job SOP Class **77**
Printer SOP Class **77**

R

RGB **35, 41, 42, 131**

S

SOP Classes **44**

V

Verification **15, 26, 39, 42**
VOI LUT SQ **41**

Y

YBR_FULL **42**

