

DICOM Conformance Statement *syngo* MammoReport

SP



The DICOM functionalities in the *syngo* MammoReport system are based on the libraries from Merge Technologies Inc.

Softcopy reading software by MeVis BreastCare.

Copyright © 2001 - 2010 by MeVis BreastCare.



Bremen, März 2010

Table of Contents

<i>Introduction.....</i>	<i>8</i>
Overview	8
Scope and Field.....	8
Audience.....	8
Remarks.....	8
Definitions, Terms and Abbreviations	8
References.....	9
Structure	9
<i>Implementation Model Verification</i>	<i>10</i>
Application Data Flow Diagram.....	10
Functional Definitions of Applications	10
Sequencing of Real-World Activities	10
<i>Application Entity Specification Verification</i>	<i>11</i>
Verification AE Specification.....	11
Association Establishment Policies	11
Association Initiation Policy.....	11
Association Acceptance Policy	12
<i>Implementation Model Storage</i>	<i>13</i>
Application Data Flow Diagram.....	13
Functional Definitions of Application Entities	13
Sequencing of Real-World Activities	13
<i>Application Entity Specification Storage.....</i>	<i>14</i>
Storage AEs Specification.....	14
Association Establishment Policies	16
Association Initiation Policy.....	17
Association Acceptance Policy	20
<i>Implementation Model Storage Commitment.....</i>	<i>29</i>
Application Data Flow Diagram.....	29
Functional Definitions of Application Entities	29
Sequencing of real World Activities	30
<i>AE Specification Storage Commitment.....</i>	<i>31</i>
Storage Commitment AE Specification	31
Association Establishment Policies	31
Association Initiation Policy.....	31
Association Acceptance Policy	33
<i>Implementation Model Query / Retrieve</i>	<i>35</i>
Application Data Flow Diagram.....	35
Functional Definitions of Application Entities	35

Sequencing of Real-World Activities	36
Query/Retrieve Service AEs Specification	36
Association Establishment Policies	37
Association Initiation Policy	37
Association Acceptance Policy	42
Implementation Model Print.....	49
Application Data Flow Diagram.....	49
Functional Definition of Application Entities	49
Sequencing of Real-World Activities	49
Application Entity Specification Print.....	50
Print Management AE Specification	50
1.1.1 Association Establishment Policies	50
Association Initiation Policy	51
Association Acceptance Policy	57
Communication Profiles	58
Supported Communication Stacks	58
TCP/IP Stack.....	58
Extensions / Specializations / Privatizations	59
Standard Extended / Specialized / Private SOPs	59
Private Transfer Syntaxes.....	59
Configuration	59
AE Title/Presentation Address Mapping.....	59
DICOM Verification.....	59
DICOM Storage AE Title	59
DICOM Query/Retrieve AE Title	59
DICOM Print AE Title	59
Configurable Parameters.....	59
Storage, Storage Commitment and Query/Retrieve	60
Print	60
Modality Worklist	61
Default Parameters	61
Support of Extended Character Sets	61
Media Storage Conformance Statement.....	63
Introduction.....	64
Purpose	64
Scope	64
Definitions, Abbreviations.....	64
Definitions.....	64
Abbreviations.....	64
References.....	64
Remarks.....	65
Implementation Model.....	66
Application Data Flow Diagram.....	66
Functional Definitions of AEs	66

Sequencing of Real-World Activities	66
File Meta Information Options	67
AE Specifications	68
DICOM Archive Specification	68
File Meta Information for the Application Entity	68
Real-World Activities for this Application Entity	68
2 Augmented and Private Profiles	71
Augmented Application Profiles	71
AUG-GEN-CD	71
AUG-CTMR-xxxxx	71
AUG-XA1K-CD	71
syngo® private offline Media Application Profile	71
Class and Profile Identification	71
Clinical Context	72
PRI-SYNGO Profiles	73
Basic Directory IOD Specialization	80
Additional Keys	80
Icon Images	82
Extensions, Specialization and Privatization of SOP Classes and Transfer Syntaxes 83	
SOP Specific Conformance Statement for Basic Directory	83
Extension, Specialization for SIEMENS Non-Image Objects	83
Configuration	83
AE Title Mapping	83
DICOM Media Storage AE Title	83
Support of Extended Character Sets	83
ImageRouting Conformance Statement	84
Introduction	84
Purpose	84
Scope	85
Definitions, Abbreviations	85
Implementation Model	86
Application Data Flow	86
Functional Definition of AE	86
Sequencing of Real World Activities	86
AE Specification	87
Service Class User Part	87
Service Class Provider Part	90
Network Interfaces	93
Physical Network Interface	93
Configuration	93
AE Titles / Presentation Address Mapping	93
Media Interchange	93
Support of Character Sets	93
Security	93
IOD Contents	93
ImagePrefetching Conformance Statement	94

Introduction	95
Purpose	95
Scope	95
Definitions, Abbreviations.....	95
Implementation Model	97
Application Data Flow.....	97
Functional Definition of AE	99
Sequencing of Real World Activities	100
AE Specification	102
Service Class User Part	102
Service Class Provider Part	107
Network Interfaces	112
Physical Network Interface.....	112
Configuration	112
AE Titles / Presentation Address Mapping	112
Media Interchange.....	112
Support of Character Sets	112
Security	112
IOD Contents	112

Introduction

Overview

The Conformance Statement describes the DICOM interface for the Siemens *syngo* MammoReport in terms of part 2 of [DICOM].

This introduction describes the application's implemented DICOM functionality in general terms.

Scope and Field

The *syngo* MammoReport is a “*syngo*®-speaking” Imaging Modality or workstation. The *syngo* MammoReport is designed to be integrated into an environment of medical DICOM-based devices. The *syngo* MammoReport DICOM network implementation acts as SCU and SCP for the DICOM Storage, Storage Commitment and Query/Retrieve services and as SCU for the DICOM Print Service. Verification is supported in SCU (only via Service environment) and SCP role. Furthermore the handling of CD/MOD offline media is supported as a FSC, FSU and FSR.

Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

ACR	American College of Radiology
AE	DICOM Application Entity
ASCII	American Standard Code for Information Interchange
CSE	Customer Service Engineer
DB	Database
DCS	DICOM Conformance Statement
DSA	Digital Subtraction Angiography
IIDC	Image-Intensifier Distortion Correction
IOD	DICOM Information Object Definition
ISO	International Standard Organization
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
RIS	Radiology Information System
RWA	Real-World Activity
SCU	DICOM Service Class User (DICOM client)
SCP	DICOM Service Class Provider (DICOM server)
SOP	DICOM Service-Object Pair
SR	Structured Report
U	Unique Key Attribute
UTF-16	Unicode Transformation Format-16 (used internally by Microsoft Windows)

References

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.18, 2009

The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>

Structure

This Conformance Statement is subdivided into multiple Parts, which relate to individual documents needed to declare Conformance according to the requirements of “Part 2 - Conformance” of the DICOM Standard.

Those parts are:

- “Network Conformance Statement” for Network related Services
 - Storage - User/Provider (includes Verification - User/Provider)
 - Storage Commitment - User/Provider
 - Query/Retrieve - User/Provider
 - Basic Grayscale/Color Print - User
 - Basic Worklist - User
 - Modality Performed Procedure Step - User
- “Offline Media Conformance Statement” to support local archive media.
- A general Appendix.

Implementation Model Verification

The *syngo* MammoReport DICOM Service Tool application requests Verification to verify the ability of a foreign DICOM application on a remote node to respond to DICOM messages.

Responding to Verification requests from remote nodes is handled by the Storage SCP application and therefore described in chapter *Implementation Model Storage*.

Application Data Flow Diagram

The *syngo* MammoReport DICOM network implementation acts as SCU for the C-ECHO DICOM network service. The product target Operating System is Windows XP®.

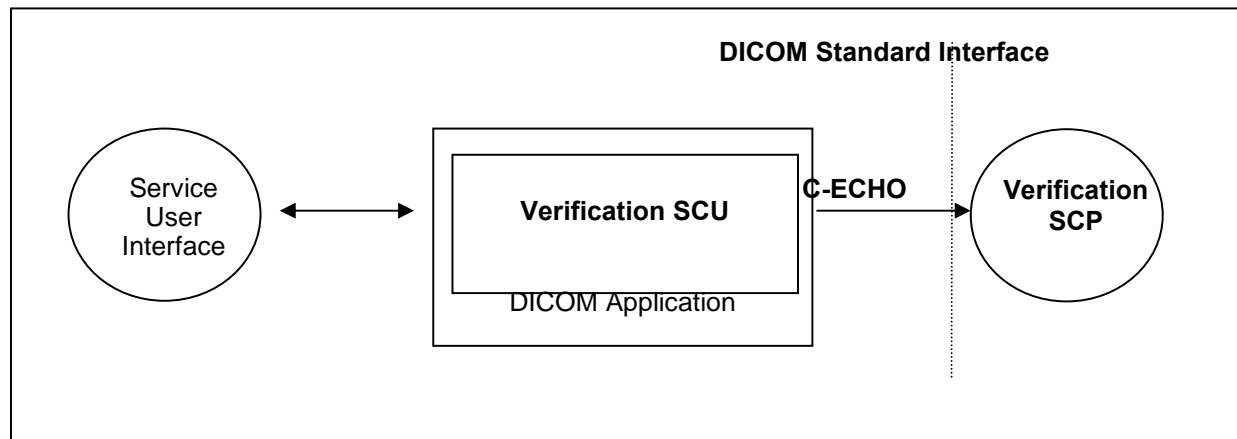


Figure 1: Application Data Flow Diagram - Verification SCU

Functional Definitions of Applications

The *syngo* MammoReport DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

Sequencing of Real-World Activities

Newly entered data have to be saved first, before a "verification" of these data is possible.

Application Entity Specification Verification

Verification AE Specification

Association Establishment Policies

General

The *syngo* MammoReport DICOM Service Tool application attempts to open an association for verification request whenever the “verification” function is activated during network configuration of a remote DICOM application.

Number of Associations

The *syngo* MammoReport DICOM Service Tool application initiates one association at a time to request verification.

Asynchronous Nature

The *syngo* MammoReport DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

Implementation Identifying Information

Implementation Class UID	1.3.12.2.1107.5.12
Implementation Version Name	“MBC_SCR-5-1-0”

Association Initiation Policy

The *syngo* MammoReport DICOM Service Tool application attempts to initiate a new association for DIMSE C-ECHO service operations.

Associated Real-World Activity - Verification

Associated Real-World Activity – Request Verification “verification”

The associated Real-World activity is a C-ECHO request initiated by Service and Configuration SW environment whenever a “verification” is requested. If an association to a remote Application Entity is successfully established, Verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application contains a status other than “Success” this will be indicated in the service environment and the association is closed.

Proposed Presentation Contexts

The *syngo* MammoReport DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table – Verification SCU					
Abstract Syntax		Transfer Syntax		Extended	
Name	UID	Name List	UID List	Role	Negotiation
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

SOP Specific Conformance – Verification SCU

The Application conforms to the definitions of the Verification SCU in accordance to the DICOM Standard.

Association Acceptance Policy

The Verification SCP is part of the Storage SCP – see chapter *Implementation Model Storage*.

Implementation Model Storage

The *syngo* MammoReport DICOM Application Entity both originates associations for Storage of DICOM Composite Information Objects in Remote Application Entities and accepts association requests for Storage from Remote Application Entities.

Application Data Flow Diagram

The *syngo* MammoReport DICOM network implementation acts as SCU and SCP for the C-STORE DICOM network service and as SCP for the C-ECHO DICOM network service. The product target Operating System is Windows XP.

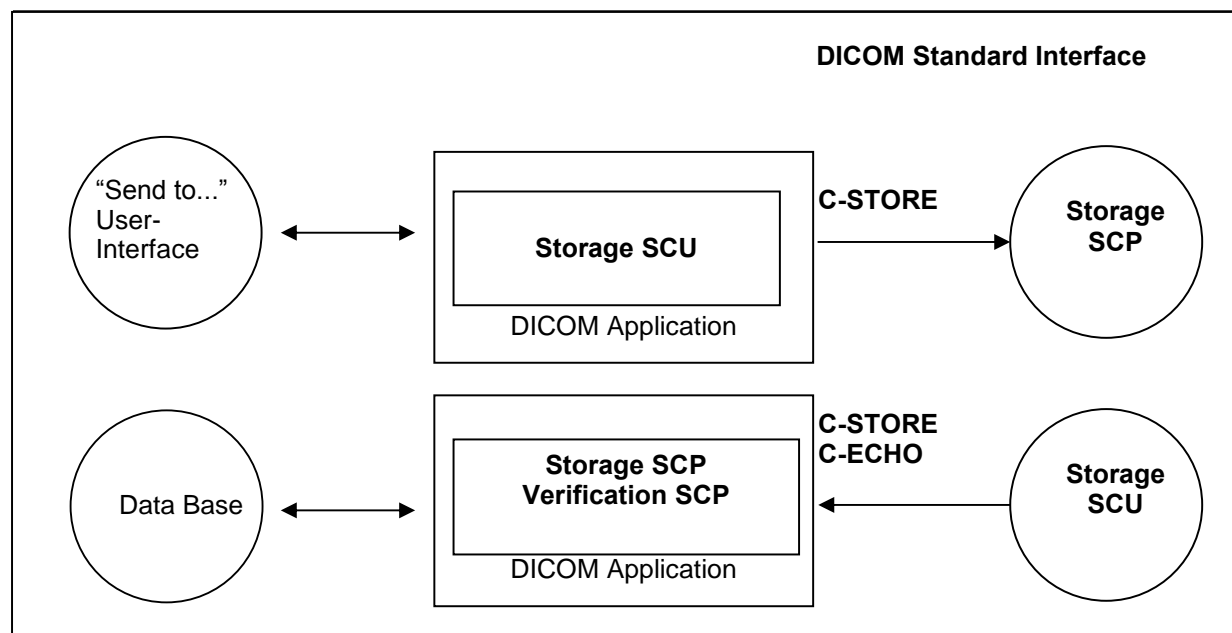


Figure 2: Application Data Flow Diagram – Storage SCU/SCP

Functional Definitions of Application Entities

The Storage SCU is invoked by the job control interface that is responsible for processing network send/storage tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

The Storage SCP component of the *syngo* MammoReport DICOM application is operating as background server process. It is existing when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database. Verification requests will be processed and responded by Storage SCP component too.

Sequencing of Real-World Activities

not applicable

Application Entity Specification Storage

Storage AEs Specification

The *syngo* MammReport Storage service class user/service class provider applications use one AE when initiating/receiving associations to/from remote DICOM nodes.

SIEMENS *syngo* MammReport DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCU:

SOP Class Name	SOP Class UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Digital X-Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital MammoGraphy Image Storage – for Processing (only if configured in registry!)	1.2.840.10008.5.1.4.1.1.1.2.1
Digital MammoGraphy Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3.1
Digital Intra-oral X-Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
PET Image Storage	1.2.840.10008.5.1.4.1.1.128
RadioTherapy Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3
RadioTherapy Dose Storage	1.2.840.10008.5.1.4.1.1.481.2
RadioTherapy Image Storage	1.2.840.10008.5.1.4.1.1.481.1
RadioTherapy Plan Storage	1.2.840.10008.5.1.4.1.1.481.5
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
UltraSound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
UltraSound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray RadioFluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1

General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22
Verification	1.2.840.10008.1.1
Key Object Selection	1.2.840.10008.5.1.4.1.1.88.59

SIEMENS syngo MammoReport DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

SOP Class Name	SOP Class UID
Computed R adiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed T omography Image Storage	1.2.840.10008.5.1.4.1.1.2
Digital X -Ray Image Storage – for Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital X -Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital M ammo G raphy Image Storage – for Processing (only if configured in registry!)	1.2.840.10008.5.1.4.1.1.1.2.1
Digital M ammo G raphy Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital I ntra- o ral X -Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3.1
Digital I ntra- o ral X -Ray Image Storage – for Presentation	1.2.840.10008.5.1.4.1.1.1.3
M agnetic R esonance Image Storage	1.2.840.10008.5.1.4.1.1.4
N uclear M edicine Image Storage	1.2.840.10008.5.1.4.1.1.20
PET Image Storage	1.2.840.10008.5.1.4.1.1.128
R adio T herapy S tructure S et Storage	1.2.840.10008.5.1.4.1.1.481.3
R adio T herapy D ose Storage	1.2.840.10008.5.1.4.1.1.481.2
R adio T herapy I mage Storage	1.2.840.10008.5.1.4.1.1.481.1
R adio T herapy P lan Storage	1.2.840.10008.5.1.4.1.1.481.5
S econdary C apture Image Storage	1.2.840.10008.5.1.4.1.1.7
U ltra S ound Multi-Frame Image Storage (retired)	1.2.840.10008.5.1.4.1.1.3
U ltra S ound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
U ltra S ound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
U ltra S ound Image Storage (retired)	1.2.840.10008.5.1.4.1.1.6
X -Ray A ngiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X -Ray R adio F luoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3

SOP Class Name	SOP Class UID
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22
Verification	1.2.840.10008.1.1
Key Object Selection	1.2.840.10008.5.1.4.1.1.88.59

Association Establishment Policies

General

The existence of a job queue entry with network destination or an internal trigger from processing a retrieve request will activate the DICOM Storage Application. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the transfer is started.

The default PDU size used will be 28 KB.

Number of Associations

The *syngo* MammoReport DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The *syngo* MammoReport DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of Simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in Configuration / DICOM / General.

Asynchronous Nature

The *syngo* MammoReport DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

Implementation Identifying Information

Implementation Class UID

1.3.12.2.1107.5.12

Implementation Version Name

"MBC_SCR-5-1-0"

Association Initiation Policy

If a job with network destination gets active in the job list or a retrieve sub-operation is processed the *syngo MammoReport* DICOM application attempts to initiate a new association for

- DIMSE C-STORE service operations.

Associated Real-World Activity - Send

Associated Real-World Activity – Send Image Objects to a Network Destination

The associated Real-World activity is a C-STORE request initiated by an internal daemon process triggered by a job with network destination or the processing of an external C-MOVE retrieve request. If the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. If the C-STORE Response from the remote Application contains a status other than “Success” or “Warning”, the association is aborted.

Proposed Presentation Context – Send Images

The *syngo MammoReport* DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Digital X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Digital X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
MammoGraphy Image for processing (only if configured in registry!)	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
MammoGraphy Image for presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Digital Intra-oral X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossy Extended *1 (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCU	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		

Presentation Context Table					
Digital Intra-oral X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Ultra-Sound Multi-Frame Image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Ultra-Sound Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
X-Ray RadioFluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless, Process 14 (selection value 1) Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.4.70 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None

Presentation Context Table					
Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform 12-Lead ECG Object	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform General ECG Object	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform Ambulatory ECG Object	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform Hemodynamic Object	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform Cardiac Electro- physiology Object	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Waveform Basic Audio Object	1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCU	None
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Key Object Selection Document SOP Class	1.2.840.10008.5.1.4.1.1.88.59	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None

Note:

1. The compression is only supported for images with pixel representation (0028, 0103) equal to 0 (=unsigned)

The "MOVE destinations" must be configured as Storage destinations. This would include the configuration of Transfer Syntax capabilities.

Not all the listed transfer syntaxes will be proposed all the time. For some abstract syntaxes only a list of uncompressed (UC) transfer syntaxes (one or more) will be proposed, for other abstract syntaxes also JPEG Lossless (LL) syntax will be proposed and/or a list of JPEG Lossy (LY) transfer syntaxes. The contents of this lists is configurable, e.g. UC could be configured to contain only Implicit Little Endian for instance.

Depending on the real world activity initiating the C-STORE, we have the following behaviors:

- if the C-STORE is initiated by a user, a configuration parameter called QualityFactor(Q) will be used to decide which transfer syntax lists will be proposed. Q can take values between 0 and 100. If Q=0, only UC will be proposed. If Q = 100, UC and LL will be proposed. Else UC and LY will be proposed.
- if the C-STORE is initiated by the C-MOVE SCP, there is another configuration parameter called Compression Types Supported (CTS) which will be used to decide what transfer syntaxes are proposed. CTS can take integer values. If CTS=0 or CTS > 3, UC will be proposed. If CTS=1, UC and LY will be proposed. If CTS = 2, UC and LL will be proposed. If CTS >= 3, UC, LL and LY will be proposed.

The compression types JPEG lossy and JPEG lossless are parameters, which are part of the Application Entity Properties configuration (storage checked). It can be reached via the Service-UI: Configuration / DICOM / Network nodes

SOP specific Conformance to Storage SOP classes

The *syngo* MammoReport (DICOM) application will not change private attributes as long as no modification is done. During a "Save as ..." operation all private attributes not defined within the *syngo* MammoReport DICOM application will be removed when the new object instance is created.

For association and DIMSE level time-outs, please refer to Configuration section of this document.

1.1.1.1.1.1 Optional Attributes

- Data Dictionary of DICOM Type 2 and 3 IOD Attributes

Please see the related Image Object definition tables in the Annex for a list of all DICOM IOD attributes of type 2 and 3, which are encoded by the *syngo* MammoReport applications.

1.1.1.1.1.2 Specialized Information Object Definitions

The DICOM images created by *syngo* MammoReport DICOM application conform to the DICOM IOD definitions (Standard extended IODs). But they will contain additional private elements, which have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification!

- Data Dictionary of applied private IOD Attributes

Please see chapter „IOD Contents“ for a list of possible private IOD attributes.

1.1.1.1.1.3 Specific requirements for DICOM attributes

It is required that the patient identifying type 2 attributes Patient's Name (0010,0010) and Patients ID (0010,0020) must not have zero length to allow appropriate further processing of the SOP class instances.

1.1.1.1.1.4 Enhanced SR

For creating a Breast Imaging Report Enhanced SR is used.

Association Acceptance Policy

The *syngo* MammoReport DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

Service operations. Any Information Objects transmitted on that association will be checked on conformance and stored in database if check was successful.

Associated Real-World Activity - Receive

Associated Real-World Activity – Receiving Images from a Remote Node

The daemon receiving process will accept an association and will receive any images transmitted on that association and will store the images on disk in the own database if the conformance check is performed successfully.

Accepted Presentation Context – Receiving Image Objects

The *syngo* MammoReport DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Digital X-Ray Image	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
MammoGraphy Image (For Processing only if configured in registry)	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
Digital Intra-oral X-Ray Image	1.2.840.10008.5.1.4.1.1.1.3.1	RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		

Presentation Context Table					
Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90		
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	JPEG 2000 Lossless	1.2.840.10008.1.2.4.90		
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Presentation Context Table					
Ultra-Sound Multi-Frame Image (retired) ‡	1.2.840.10008.5.1.4.1.1.3	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Ultra-Sound Image (retired) ‡	1.2.840.10008.5.1.4.1.1.6	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Ultra-Sound Multi-Frame Image §	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	SCP	None
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
Ultra-Sound Image §	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	RLE Lossless	1.2.840.10008.1.2.5	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
X-Ray RadioFluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70	SCP	None
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Implicit VR Little Endian	1.2.840.10008.1.2		
Waveform	1.2.840.10008.5.1.4.1.1.9.1.1 1.2.840.10008.5.1.4.1.1.9.1.2 1.2.840.10008.5.1.4.1.1.9.1.3 1.2.840.10008.5.1.4.1.1.9.2.1 1.2.840.10008.5.1.4.1.1.9.3.1 1.2.840.10008.5.1.4.1.1.9.4.1	JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	SCP	None
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

‡ US Retired and US Multi-frame Retired images are converted to US Images/US Multi-frame images before storing them into the local database. The conversion creates new images, which implies new UIDs.

§ Color images are converted to gray scale for display on high resolution viewer. A warning is displayed on the image in such a case

Presentation Context Table					
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCP	None
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Key Object Selection	1.2.840.10008.5.1.4.1.1.88.59	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None

Note:

With RLE Lossless Transfer Syntax the DICOM application will decompress the image before storing it into the database.

SOP-specific Conformance Statement – Receiving Images

The *syngo* MammoReport DICOM application conforms to the Full Storage Class at Level 2.

In the event of a successful C-Store operation, the image has successfully been written on disk. For private attributes with VR=SQ only a nesting level of one is supported. This means that private attributes containing another sequence will be removed from the image header during storage.

Upon successful receiving a C-STORE-RQ, the Siemens *syngo* MammoReport DICOM receiver performs a quick plausibility test on the received image and available system resources. If this test succeeds, it returns the status SUCCESS, otherwise one of the following status codes is returned and the association is aborted:

- **Refused (A700):**
This error status indicates a lack of Resources (e.g. not enough disk space) on the *syngo* MammoReport modality.
- **Invalid Dataset (0xA900):**
The dataset is not containing one of the Attributes “Study Instance UID”, “Series Instance UID” or “SOP Instance UID”, or one of them has an invalid value.
- **Processing Error (0110):**
An error occurred while processing the image, which makes it impossible to proceed

Attention! Only after sending the response, the image will be saved into the database. If during this operation an error occurs, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

In order to confirm that the sent images were successfully stored in the database, the sending application should use Storage Commitment Service.

If an image instance is received that is identified by a SOP Instance UID which is already used by an Instance stored in database then the actual received image will be discarded. The existing Instance is not superseded.

Currently the following modalities can be configured to be shown on the high resolution monitors:

- MG images
- CR images
- CT images
- DX images

- SC images
- US images
- MR images
- RT images
- SR CAD (only if referenced image is available)
- Key Object Selection with Document Title:
 - Rejected for Patient Safety Reasons or
 - Rejected for Quality Reasons

More may be added in the future.

The following sections will differentiate the attribute contents required for Image Viewing. The *syngo* MammoReport DICOM application supports more formats for Storage of Images than Viewing.

Number of Associations

The *syngo* MammoReport DICOM application is able to accept multiple associations at a time. However Storage Class User should not send images of a single study simultaneously on different associations.

1.1.1.1.1.5 Image Pixel Attribute Acceptance Criterion for Grayscale Images - Viewing

The *syngo* MammoReport Multi-Modality Viewing application accepts the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. Accepted values:

- Pixel plane
 - samples per pixel (attribute 0028, 0002) = 1
 - photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
 - photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
 - pixel representation (attribute 0028, 0103) = 0
 - bits allocated (attribute 0028, 0100) = 8, 16
 - bits stored (attribute 0028,0101) = 8, 10, 12, 14, 15, 16
 - high bit (attribute 0028,0102) = 7, 9, 11, 13, 14, 15
 - only aspect ratio 1:1 is supported
- Overlay plane
 - overlay type (attribute 60xx, 0040) = "G"
 - bits allocated (attribute 60xx, 0100) = 16
 - bit position (attribute 60xx, 0102) = 12, 13, 14, 15 (only bits above high bit permitted)
 - Graphic Overlay will be shifted to fill Overlay Planes from Bit 12 and consecutive.

- Overlay plane
 - overlay type (attribute 60xx, 0040) = "G"
 - bits allocated (attribute 60xx, 0100) = 1
 - bit position (attribute 60xx, 0102) = 0
 - overlay data (attribute 60xx, 3000) = supported

The *syngo* MammoReport Multi-Modality Viewing application accepts also the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integer and 16 bits allocated. Accepted values:

- Pixel plane
 - samples per pixel (attribute 0028, 0002) = 1
 - photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
 - photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
 - pixel representation (attribute 0028, 0103) = 1 (signed)
 - bits allocated (attribute 0028, 0100) = 16
 - bits stored (attribute 0028,0101) = 16
 - high bit (attribute 0028,0102) = 15
 - only aspect ratio 1:1 is supported
- Overlay plane
 - overlay type (attribute 60xx, 0040) = "G"
 - bits allocated (attribute 60xx, 0100) = 1
 - bit position (attribute 60xx, 0102) = 0
 - overlay data (attribute 60xx, 3000) = supported
 - For MOD LUT, both the linear LUT (Rescale Slope/Intercept) and the MOD LUT SQ are supported and considered when pixel data is displayed. However there are two limitations. The MOD LUT SQ will be ignored in the following cases:

- 8-Bit signed pixels
 - the pixel format is changed by the MOD LUT (e.g. 8bit -> 16bit)
- If the MOD LUT SQ contains multiple LUTs, then only the first one is used.

For VOI LUT, both the linear LUT (Window Center/Width) and the VOI LUT SQ are supported (VOI LUT SQ with 8 or 16 bit LUT data)

But if both, a VOI LUT SQ and a linear MOD LUT, are specified within one image, then the value for Rescale Slope is restricted to 1.

If multiple VOI LUTs are available (linear LUT and/or VOI LUT SQ) it can be configured which one is used by default. The other VOI LUTs are selectable.

Only Rectangular and Circular Shutter Shape is supported in this version. Images containing other Shutter Shapes will be displayed w/o shutter.

1.1.1.1.1.6 Image Pixel Attribute Acceptance Criterion for Color Images - Viewing

The *syngo* MammoReport Multi-Modality Viewing application supports the RGB color image description with the unsigned integer 24-bit color image plane pixel format.

Accepted values:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = "RGB"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8
- bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7
- planar configuration (attribute 0028,0006) = 0 (pixel interleave) or 1 (plane interleave).

The *syngo* MammoReport Multi-modality Viewing application supports the "Palette Color" color image description with the unsigned integer and 2's complement pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 1
- photometric interpretation (attribute 0028,0004) = "PALETTE COLOR"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- bits allocated (attribute 0028, 0100) = 16 and bits stored (attribute 0028,0101) = 16
- high bit (attribute 0028,0102) = 7, 15

Both 8-bit and 16-bit palettes are supported, but NO Segmented Palette Color LUTs.

The *syngo* MammoReport Multi-modality Viewing application supports the YBR_FULL color image description with the unsigned integer pixel format. Accepted values:

- samples per pixel (attribute 0028, 0002) = 3
- photometric interpretation (attribute 0028,0004) = "YBR_FULL"
- pixel representation (attribute 0028, 0103) = 0
- bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- high bit (attribute 0028,0102) = 7

If *syngo* MammoReport software is making any persistent changes on a YBR image, the resulting new image will be saved with Photometric Interpretation = "RGB".

Presentation Context Acceptance Criterion

The *syngo* MammoReport DICOM application will accept any number of verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to the maximum of 127 (DICOM limit). In the event that the *syngo* MammoReport DICOM application runs out of resources, it will reject the association request.

Transfer Syntax Selection Policies

The *syngo* MammoReport DICOM application currently supports

- the Implicit VR Little Endian, the Explicit VR Little Endian and Explicit VR Big Endian Transfer Syntaxes
- the JPEG Lossless Non-hierarchical Transfer Syntax
- the JPEG Baseline and JPEG Extended Transfer Syntaxes (JPEG Lossy).
- the RLE Lossless Transfer Syntax

Any proposed presentation context including one of these Transfer Syntaxes will be accepted. Any proposed presentation context that does not include one of these Transfer Syntaxes will be rejected.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

1. JPEG Lossy Extended
2. JPEG Lossless non-hierarchical
3. JPEG Lossy Baseline
4. RLE Lossless
5. Explicit VR Little Endian
6. Explicit VR Big Endian
7. Implicit VR Little Endian

With RLE Lossless Transfer Syntax the *syngo* MammoReport DICOM application will decompress the image before storing it into the database.

With Implicit VR Little Endian Transfer Syntax the *syngo* MammoReport DICOM application will remove any Private Attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute-dictionary of the *syngo* MammoReport DICOM application.

Therefore any Explicit VR Transfer Syntax shall preferably be used by the Storage SCU's when sending Composite Image Instances to the *syngo* MammoReport DICOM application.

Implementation Model Storage Commitment

The Storage Commitment service class defines an application-level class of service which facilitates the commitment to storage. It performs an additional task of commitment of composite objects apart from the network based storage of images as defined by the Storage Service class. The *syngo* MammoReport DICOM implementation supports the Storage Commitment Push Model as SCU and SCP.

Application Data Flow Diagram

The *syngo* MammoReport DICOM network implementation acts as SCU for the Storage Commitment Push Model Service using the Storage Commitment Service Class. The product target Operating System is Windows XP.

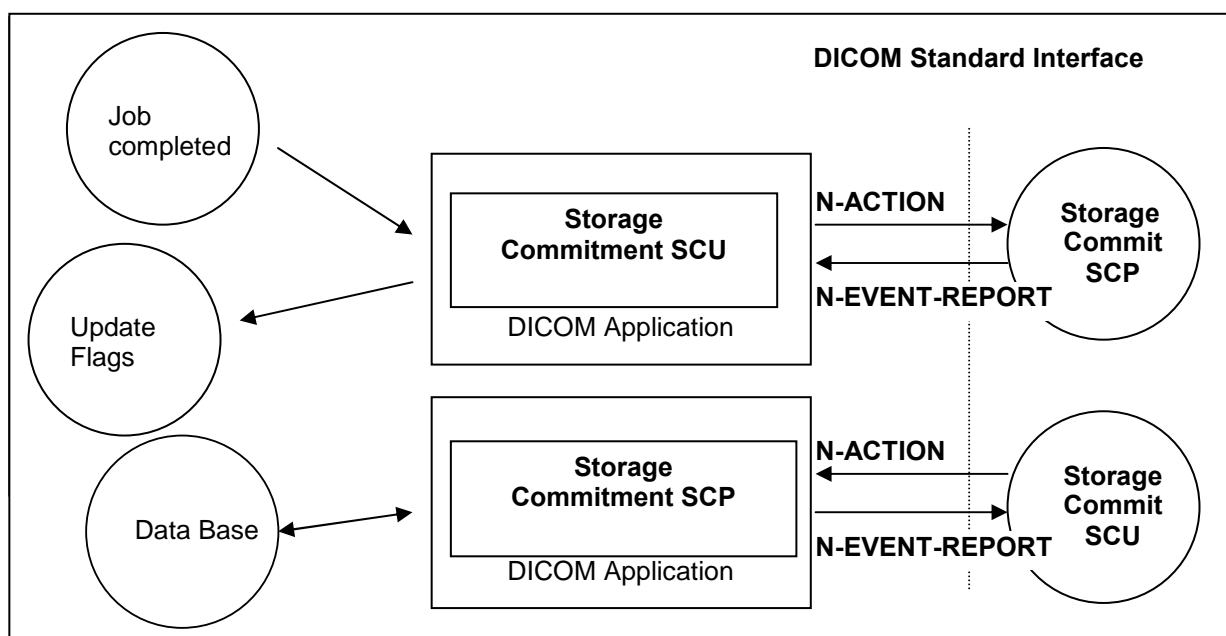


Figure 3: Application Data Flow Diagram – Storage Commitment SCU/SCP

Functional Definitions of Application Entities

With each successfully completed send job to a node that is configured to be a Storage Commitment SCP, the *syngo* MammoReport DICOM Application will create a Storage Commitment request Push Model Identifier from the SOP Instances sent. Then a Storage Commit Request is triggered. Depending on configuration, the *syngo* MammoReport DICOM application will keep the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the related Status Flags of the related entity. It is possible to create triggers ("auto rules") from this event.

The Transaction UUIDs of the pending commitment request are kept "open" for a configurable amount in time (default: 1h). If the "open time" for a pending commitment request has elapsed w/o a related response from the provider, the Transaction UUID is removed and the related entities are indicated as "commit failed".

In any case, commitment will only be requested for previously and successfully sent images.

Sequencing of real World Activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

AE Specification Storage Commitment

Storage Commitment AE Specification

SIEMENS *syngo* MammoReport DICOM application provides Standard Conformance to the following DICOMV3.0 SOPClass as an SCU:

SOP Class Name	SOP Class UID
Storage Commitment Push Model	1.2.840.10008.1.20.1

Association Establishment Policies

General

With a Send Job successfully completed to a node that is configured to be a Storage Commitment SCP, the DICOM application will generate a Storage Commitment Identifier which references to all Instances of the processed job. The Commit Request is then sent over a single opened association. The *syngo* MammoReport will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and a time-stamp, is kept. Depending on configuration, the association is closed when the configured time-out has elapsed or a response was received before. If the association is closed before a response was received, the response is then expected on a different association. Multiple Storage Commitment Requests can be pending.

The default PDU size used will be 28 KB.

Number of Associations

The *syngo* MammoReport DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The *syngo* MammoReport DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

Asynchronous Nature

The *syngo* MammoReport DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

Implementation Identifying Information

Implementation Class UID

1.3.12.2.1107.5.12

Implementation Version Name

"MBC_SCR-5-1-0"

Association Initiation Policy

The *syngo* MammoReport DICOM Application Entity acts as a Service Class User (SCU) for the

- Storage Commitment Push Model Service Class (to request commitment for storage of instances previously sent).
To do so, the *syngo* MammoReport will issue a
- N-ACTION DIMSE to request commitment or a
- N-EVENT-REPORT DIMSE to respond to a received storage commitment request and the association was closed by the remote system prior to response.

Real World Activity – Storage Commitment

Associated Real-World Activity - Job Completed

The *syngo* MammoReport Storage Commitment application sends the commit request (N-ACTION-RQ) message and waits for acceptance of this request (N-ACTION-RSP). After receiving this, the transaction is marked as “waiting”.

Depending on a configuration value, the association will then be closed or kept open. In the first case, there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N-EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association. For both cases, if the commit response (N-EVENT-REPORT) does not arrive during the configured time, the transaction will be marked as failed. The *syngo* MammoReport does not re-send objects from a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”; In both cases, a message is shown to the user.

Proposed Presentation Contexts - Job Completed

The *syngo* MammoReport DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

SOP Specific Conformance Statement- Job Completed

Storage Commitment is supported for all the SOP class UIDs as mentioned in 'Acceptable presentation contexts - Storage' in the Storage SCP section of this document.

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes will not be supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

Associated Real-World Activity - Send Commit Response

Acting as a Storage Commitment Provider, the *syngo* MammoReport Storage Commitment AE received a Storage Commitment request, carried out the request, and is ready to send back the response, but the association is not open anymore. In this case it will by itself initiate an association to send the storage commitment response (N-EVENT-REPORT) to the SCU.

Proposed Presentation Contexts - Send Commitment Response

The Siemens *syngo* MammoReport DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

SOP Specific Conformance Statement - Send Commitment Response

Storage Media File-Set ID and UID Attributes will not be supported in the N-EVENT-REPORT primitive invoked by the Storage Commitment SCP.

Association Acceptance Policy

The *syngo* MammoReport DICOM Application Entity acts as a Service Class Provider (SCP) for the

- Storage Commitment Push Model Service Class (Give a commitment to store previously received instances).
To do so, the *syngo* MammoReport attempts to accept a
- N-ACTION DIMSE to receive a commitment request for the instance included or a
- N-EVENT-REPORT DIMSE to receive a storage commitment response from a previous request and the SCP behavior requires a different association than the commit request.

Associated Real-World Activity - Commit SCU

Associated Real-World Activity - Update Flags

The *syngo* MammoReport Storage Commitment DICOM Application has sent a Storage Commitment Request and, being configured to receive response on a separate association, has closed the association, and now it gets an association request from the Storage Commitment SCP that want to send the results. The *syngo* MammoReport DICOM application will await Storage commitment Notification triggers. Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid, the Notification Identifier is evaluated and the related Instances marked with the related status. The over-all Commit Status of the higher Information Entities is derived from propagation of the States of all Image entities included in a study.

The Status Flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of

- “AC” or “SC” - Successful Commitment, A means archived to configured Archive destination, whereas S means sent to any other destination
- “Af” or “Sf” - Commitment failed.
- “A?” or “S?” - Commitment request is sent, response is pending.

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

Accepted Presentation Contexts - Update Flags

The Siemens *syngo* MammoReport DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

SOP-specific Conformance Statement - Update Flags

If the Commitment response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”; In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

The *syngo* MammoReport DICOM application will NOT support the Storage Media File Set ID attributes.

Implementation Model Query / Retrieve

The query/retrieve service class defines an application-level class of services which facilitates the management of images and patient data against the well-defined information model of DICOM and allows a DICOM AE to retrieve images from a remote DICOM node or to request a remote DICOM AE to initiate a transfer of images to another DICOM AE. The *syngo* MammomReport DICOM query/retrieve application supports the query/retrieve services to act as SCU and SCP.

Application Data Flow Diagram

The *syngo* MammomReport DICOM network implementation acts as SCU and SCP for the query/retrieve network service. The product target Operating System is Windows XP®.

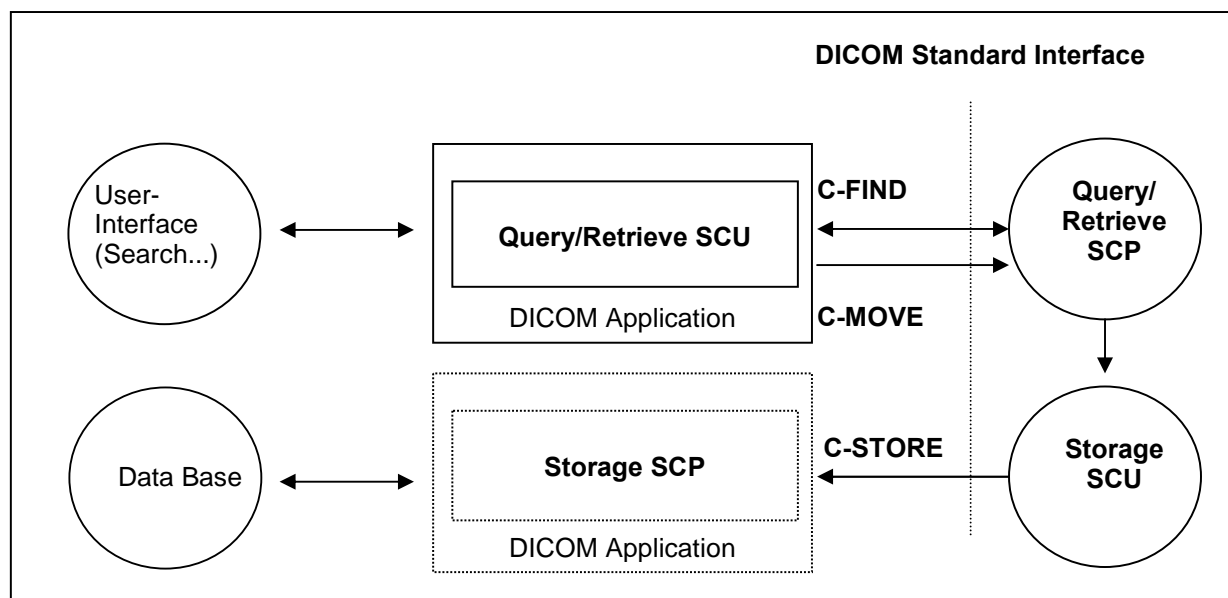


Figure 4: *syngo* MammomReport Application Data Flow Diagram – Query/Retrieve SCU

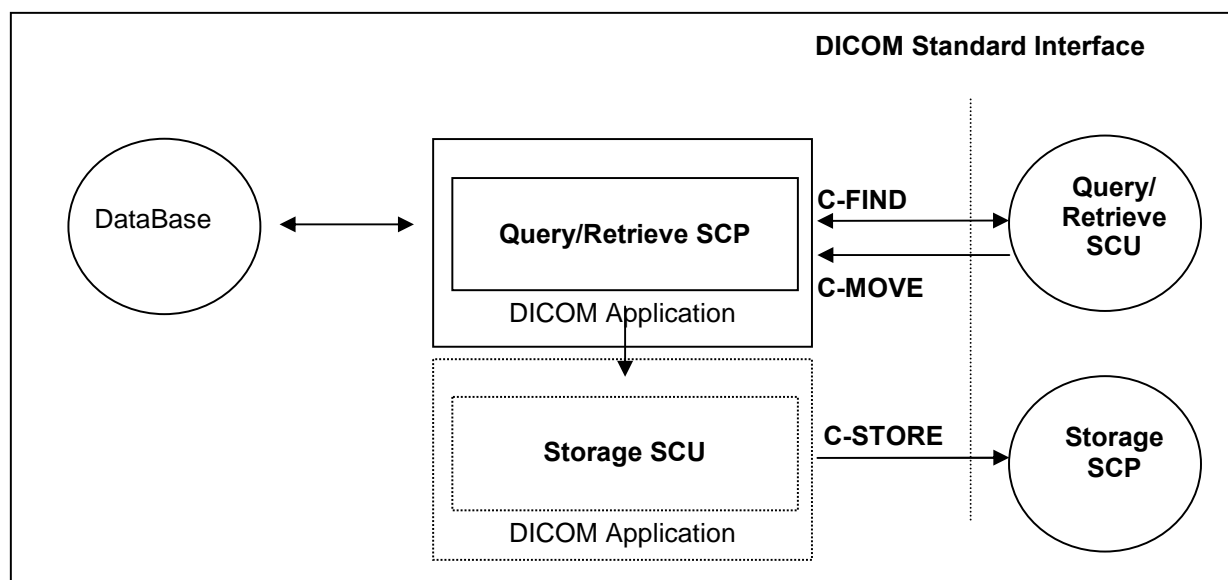


Figure 5: *syngo* MammomReport Application Data Flow Diagram – Query/Retrieve SCP

Functional Definitions of Application Entities

The *syngo* MammomReport DICOM query/retrieve SCU requests the remote query/retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in

the *syngo* MammoReport user interface. Depending on user action (Import) the *syngo* MammoReport DICOM SCU sends a C-MOVE request DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the *syngo* MammoReport Storage SCP.

The *syngo* MammoReport DICOM query/retrieve SCP responds to C-FIND request DIMSE services from remote SCU applications. Depending on further remote request, a C-MOVE involves the *syngo* MammoReport DICOM query/retrieve SCP application to initiate a C-STORE association (by triggering and parametrizing the own Storage SCU) to send image objects to a remote Storage SCP.

All components of the DICOM query/retrieve SCP application are operating as background server processes. They are existing when the machine is powered on and then respond to queries based on the records stored in its database.

Sequencing of Real-World Activities

Retrieve of images is only possible if results from a previous “Search...” operation exists and those entities can be selected for “Import”.

Application Entity Specification Query/Retrieve

Query/Retrieve Service AEs Specification

The Query/Retrieve SCU requests that the remote SCP performs a match of all keys specified in the request, against the information in its database and the identified images will be moved over a different (C-MOVE) storage association.

The Query/Retrieve SCP responds to queries based on the records based on its database and images will be sent to the requesting SCU or to a different storage destination.

SIEMENS *syngo* MammoReport DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as SCU:

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2

SIEMENS *syngo* MammoReport DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1

Study Root Query/Retrieve Information Model - MOVE 1.2.840.10008.5.1.4.1.2.2.2

Patient/Study Only Query/Retrieve Information Model - FIND 1.2.840.10008.5.1.4.1.2.3.1

Patient/Study Only Query/Retrieve Information Model – MOVE 1.2.840.10008.5.1.4.1.2.3.2

Note: See also the Storage DICOM Conformance Statement of the *syngo* MammoReport DICOM application to compare for conformance of the C-STORE sub-operation generated by the C-MOVE DIMSE services. Furthermore compare the supported Storage Service SOP classes described in the Storage DICOM Conformance Statement of the Modality to which the images shall be transferred to.

Association Establishment Policies

General

With the “Search...” function the query data are input and the DICOM query/retrieve application is started. A query request will be sent out to one remote node that can be selected from a list of configured Query Providers and the response data will be displayed for the user. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used will be 28 KB.

Number of Associations

The *syngo* MammoReport DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The *syngo* MammoReport DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

Asynchronous Nature

The *syngo* MammoReport DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

Implementation Identifying Information

Implementation Class UID

1.3.12.2.1107.5.12

Implementation Version Name

“MBC_SCR-5-1-0”

Association Initiation Policy

The query user interface will request the query-data from user and triggers one C-FIND request to the selected remote node. The response data will be displayed in the query UI for further data navigation.

When requesting Import of related items the browser requests the retrieve application to send a C-MOVE request to the related remote node. Images will then be received by the Storage SCP as described in the related section.

Real World Activity - Find SCU

Associated Real-World Activity - Find SCU “Search”

The associated Real-World activity is to fill out a query form with search data and pass it as query to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. When data transfer is finished the association is closed.

Proposed Presentation Contexts - Find SCU

The syngo MammomReport DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

It is configurable which of the two query models (or both) are to be used by the syngo MammomReport DICOM Query SCU application. If both Abstract Syntaxes are configured, The C-FIND SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the STUDY root model.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient/Study Only Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Conformance Statement - Find SCU

The syngo MammomReport DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. The interactive querying of attributes on IMAGE level is not supported by the Query SCU, hence retrieval of individual Objects is possible. The following table describes the search keys for the different query models that the SCU supports. Matching is either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is requested as return value.

Attribute name	Tag	Type	Matching	User input	return value display
Patient Level					
**					
Patient Name	(0010,0010)	R	Wildcard ^{††}	enter value	yes
Patient ID	(0010,0020)	U	Wildcard ^b	enter value	yes

** Patient Root Information Model only

†† Always a '*' is appended to the user-supplied string

Attribute name	Tag	Type	Matching	User input	return value display
Patient's Birth date	(0010,0030)	O	universal (Null)	enter value	yes
Patient's Sex	(0010,0040)	O	universal (Null)	enter value	yes
Number of Patient related Studies	(0020,1200)	O	universal (Null)	-	yes ⁺⁺
Number of Patient related Series	(0020,1202)	O	universal (Null)	-	no
Number of Patient related Instances	(0020,1204)	O	universal (Null)	-	no
Study Level					
Patient Name ^{\$\$}	(0010,0010)	R	Wildcard ^b	enter value	yes
Patient ID ^d	(0010,0020)	R	Wildcard ^b	enter value	yes
Patient's Birth date ^d	(0010,0030)	O	universal (Null)	enter value	yes
Patient's Sex ^d	(0010,0040)	O	universal (Null)	enter value	yes
Study Instance UID	(0020,000D)	U	single value	-	yes
Study ID	(0020,0010)	R	universal (Null)	enter value	yes
Study Date	(0008,0020)	R	universal (Null)	enter value ^{***}	yes
Study Time	(0008,0030)	R	universal (Null)	-	yes
Accession Number	(0008,0050)	R	universal (Null)	-	yes
Study Description	(0008,1030)	O	universal (Null)	-	yes
Referring Physician's Name	(0008,0090)	O	universal (Null)	-	yes
Name of Physician	(0008,1060)	O	universal (Null)	-	yes
Reading Study Modalities in Study	(0008,0061)	O	universal (Null)	-	yes
Storage Media File-Set ID	(0008,0130)	O	universal (Null)	-	no
Retrieve AE Title	(0008,0054)	O	universal (Null)	-	no
Number of Study related Series	(0020,1206)	O	universal (Null)	-	yes ⁺⁺⁺
Number of Study related Instances	(0020,1208)	O	universal (Null)	-	no
Series Level					
Series Instance UID	(0020,000E)	U	single value	-	yes
Series Number	(0020,0011)	R	universal (Null)	-	yes
Modality	(0008,0060)	R	universal (Null)	enter value	yes
Series Description	(0008,103E)	O	universal (Null)	enter value	yes
Body Part Examined	(0018,0015)	O	universal (Null)	enter value	yes
Performing Physician	(0008,1050)	O	universal (Null)	enter value	yes
Storage Media File-Set ID	(0008,0130)	O	universal (Null)	-	yes
Retrieve AE Title	(0008,0054)	O	universal (Null)	-	yes
Protocol Name	(0018,1030)	O	universal (Null)	-	no

⁺⁺ Implicitly visualized in the UI if no study and series search attributes have been entered

^{\$\$} Study Root Information Model only

^{***} Date range also possible

⁺⁺⁺ Implicitly if no series search attributes have been entered

Attribute name	Tag	Type	Matching	User input	return value display
Perf. Procedure Step (0040,0244)		O	universal (Null)	-	yes
Start Date					
Perf. Procedure Step (0040,0245)		O	universal (Null)	-	yes
Start Time					
Requested Attribute (0040,0275)		O	universal (Null)	-	yes
Sequence					
> Requested	(0040,1001)	O	universal (Null)	-	yes
Procedure ID					
> Scheduled	(0040,0009)	O	universal (Null)	-	yes
Procedure ID					
Number of Series	(0020,1209)	O	universal (Null)	-	yes
related Instances					

The Find SCU interprets following status codes:

C-FIND response status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901)
	Unable to process	Cxxx	(0000,0902)
			(0000,0901)
			(0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied	FF00	Identifier
	and any Optional Keys were supported in the same manner as Required Keys		
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

Real-World Activity – Move SCU

Associated Real-World Activity – Move SCU “Import”

When selecting a data entry in the Query UI and activate the “Import” function, a retrieval request is passed to the archival application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by processing the C-MOVE service.)

The transferred image data are processed as described in the storage class SCP descriptions.

The possibility to request the remote C-MOVE provider (remote application that responded to the C-FIND) to move data to an application entity other than the C-MOVE SCU (the *syngo* MammoReport DICOM application) is NOT USED.

C-MOVE operation on Patient Level is not supported by the Query UI.

Proposed Presentation Contexts - Move SCU "Import"

The syngo MammoReport DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Note: C-MOVE extended negotiation will not be supported by the SCU

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient/Study OnlyQuery/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

SOP Specific Conformance Statement - Move SCU "Import"

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The Move SCU interprets following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	CXXX	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures or Warnings	B000	(0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Pending

Sub-operations are continuing

FF00

(0000,1020)
(0000,1021)
(0000,1022)
(0000,1023)

Association Acceptance Policy

The *syngo* MammoReport DICOM application will accept associations for the following DIMSE-C operations as SCP:

- C-FIND
- C-MOVE
- C-FIND-CANCEL
- C-MOVE-CANCEL

Real-World Activity - Find SCP

Associated Real-World Activity - Find SCP

The associated Real-World activity is to respond query requests to an SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is NOT supported. With a C-FIND-CANCEL request the running query can be canceled at any time.

Multiple C-FIND requests over the same association are supported.

Accepted Presentation Contexts - Find SCP

The *syngo* MammoReport DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – FIND		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – FIND		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – FIND		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Note: C-FIND Extended Negotiation will NOT be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian

SOP Specific Conformance Statement - Find SCP

The *syngo* MammoReport DICOM Query/Retrieve SCP supports hierarchical queries with all mandatory and optional search keys.

The query attribute contents will be treated case-sensitive.

With wildcard queries the symbol “?” is treated as “*” by the C-FIND SCP application. As a consequence the query string of “?abc*” will be processed as “*abc*”.

If the value for the patient-level unique key “Patient ID” is not known, it may be returned with zero length. The attribute “Image Comments” will not be included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File-Set ID, Retrieve AE Title with C-FIND-RSP message:

- The C-FIND SCP may return the DICOM attributes StorageMediaFileSetID (0088,0130) and StorageMediaFileSetUID (0088,0140) as empty or not at all. The Storage Media File-Set ID - if existent - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related Instance.
- The C-FIND SCP may return the DICOM attribute Retrieve AE Title (0008,0054) as empty or not at all. The Retrieve AE Title - if existent - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are **not** supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation has completed.

The supported attributes on the various query levels of the three supported information models are list in the tables of the following sections.

1.1.1.1.1.7 Patient Root Information Model

Attribute Name	Tag	Usage SCU	Matching
Patient Level			
Patient Name	(0010,0010)	R	single value, wildcard, universal
Patient ID	(0010,0020)	U	single value, wildcard, universal
Patient's Birth Date	(0010,0030)	O	single value, range, universal
Patient's Birth Time	(0010,0032)	O	single value, range, universal
Patient's Sex	(0010,0040)	O	single value, wildcard, universal
Ethnic Group	(0010,2160)	O	single value, wildcard, universal
Patient Comments	(0010,4000)	O	wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Level			
Study Instance UID	(0020,000D)	U	single value, list of UIDs
Study ID	(0020,0010)	R	single value, wildcard, universal
Study Date	(0008,0020)	R	single value, range, universal
Study Time	(0008,0030)	R	single value, range, universal
Accession Number	(0008,0050)	R	single value, wildcard, universal
Referring Physician's Name	(0008,0090)	O	single value, wildcard, universal
Study Description	(0008,1030)	O	single value, wildcard, universal
Admitting Diagnoses Description	(0008,1080)	O	single value, wildcard, universal
Patient's Age	(0010,1010)	O	single value, wildcard, universal
Patient's Size	(0010,1020)	O	single value, universal
Patient's Weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal

Attribute Name	Tag	Usage SCU	Matching
Additional Patient History	(0010,21B0)	O	wildcard, universal
Name of Physician reading Study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of Study related Series	(0020,1206)	O	universal
Number of Study related Instances	(0020,1208)	O	universal
Series Level			
Series Instance UID	(0020,000E)	U	single value, list of UID
Series Number	(0020,0011)	R	single value, universal
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body Part Examined	(0018,0015)	O	single value, wildcard, universal
Patient Position	(0018,5100)	O	single value, wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	single value, universal
Largest Pixel Value in Series	(0028,0109)	O	single value, universal
Protocol Name	(0018,1030)	O	single value, wildcard, universal
Series Date	(0008,0021)	O	single value, range, universal
Series Time	(0008,0031)	O	single value, range, universal
Series Description	(0008,103E)	O	single value, wildcard, universal
Operators Name	(0008,1070)	O	single value, wildcard, universal
Performing Physician's Name	(0008,1050)	O	single value, wildcard, universal
Perf. Procedure Step Start Date	(0040,0244)	O	universal
Perf. Procedure Step Start Time	(0040,0245)	O	universal
Number of Series related Instances	(0020,1209)	O	universal
Image Level			
SOP Instance UID	(0008,0018)	U	single value, list of UID
SOP Class UID	(0008,0016)	O	Single value
Image Number	(0020,0013)	R	single value, universal
Image Date	(0008,0023)	O	single value, range, universal
Image Time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image Comments	(0020,4000)	O	Universal
Concept Name Code Sequence	(0040,A043)	O	Sequence matching
>Code Value	(0008,0100)	O	single value, wildcard, universal
>Coding Scheme Designator	(0008,0102)	O	single value, wildcard, universal
>Coding Scheme Version	(0008,0103)	O	single value, wildcard, universal
>Code Meaning	(0008,0104)	O	single value, wildcard, universal
Template Identifier	(0040,DB00)	O	single value, wildcard, universal
Completion Flag	(0040,A491)	O	single value, wildcard, universal
Verification Flag	(0040,A493)	O	single value, wildcard, universal
Verifying Observer Sequence	(0040,A073)	O	Sequence matching
>Verifying Organization	(0040,A027)	O	single value, wildcard, universal
>Verifying DateTime	(0040,A030)	O	single value, range matching, universal
>Verifying Observer Name	(0040,A075)	O	single value, wildcard, universal
>Verifying Observer Identification Code Sequence	(0040,A088)	O	Sequence matching
>>Code Value	(0008,0100)	O	single value, wildcard, universal
>>Coding Scheme Designator	(0008,0102)	O	single value, wildcard, universal
>>Coding Scheme Version	(0008,0103)	O	single value, wildcard, universal

Attribute Name	Tag	Usage SCU	Matching
>>Code Meaning	(0008,0104)	O	single value, wildcard, universal
Supported Query attributes sorted by Query Level – Patient Root Information Model			

1.1.1.1.1.8 Study Root Information Model

Attribute Name	Tag	Usage SCU	Matching
Study Level			
Patient Name	(0010,0010)	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	R	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Instance UID	(0020,000D)	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	Single Value, Wildcard, universal
Study Date	(0008,0020)	R	Single Value, Range, universal
Study Time	(0008,0030)	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	Single Value, universal
Patient's Weight	(0010,1030)	O	Single Value, universal
Occupation	(0010,2180)	O	Single Value, Wildcard, universal
Additional Patient History	(0010,21B0)	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	universal
Number of Study Related Instances	(0020,1208)	O	universal
Series Level			
Series Instance UID	(0020,000E)	U	Single Value, List of UIDs
Series Number	(0020,0011)	R	Single Value, universal
Modality	(0008,0060)	R	Single Value, Wildcard, universal
Laterality	(0020,0060)	O	Single Value, Wildcard, universal
Body Part Examined	(0018,0015)	O	Single Value, Wildcard, universal
Patient Position	(0018,5100)	O	Single Value, Wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	Single Value, universal
Largest Pixel Value in Series	(0028,0109)	O	Single Value, universal
Protocol Name	(0018,1030)	O	Single Value, Wildcard, universal
Series Date	(0008,0021)	O	Single Value, Range, universal
Series Time	(0008,0031)	O	Single Value, Range, universal
Series Description	(0008,103E)	O	Single Value, Wildcard, universal
Operator's Name	(0008,1070)	O	Single Value, Wildcard, universal
Performing Physician's Name	(0008,1050)	O	Single Value, Wildcard, universal
Performed Procedure Step Start Date	(0040,0244)	O	universal
Performed Procedure Step Start Time	(0040,0245)	O	universal
Number of Series related Instances	(0020,1209)	O	universal
Image Level			
SOP Instance UID	(0008,0018)	U	Single Value, List of UIDs
SOP Class UID	(0008,0016)	O	Single value
Image Number	(0020,0013)	R	Single Value, universal
Image Date	(0008,0023)	O	Single Value, Range, universal
Image Time	(0008,0033)	O	Single Value, Range, universal

Attribute Name	Tag	Usage SCU	Matching
Modality	(0008,0060)	O	Single Value, Wildcard, universal
Image Comments	(0020,4000)	O	universal
>Accession Number	(0008,0050)	O	Single value, universal
>Requested Procedure ID	(0040,1000)	O	Single value, universal
Concept Name Code Sequence	(0040,A043)	O	Sequence matching
>Code Value	(0008,0100)	O	single value, wildcard, universal
>Coding Scheme Designator	(0008,0102)	O	single value, wildcard, universal
>Coding Scheme Version	(0008,0103)	O	single value, wildcard, universal
>Code Meaning	(0008,0104)	O	single value, wildcard, universal
Template Identifier	(0040,DB00)	O	single value, wildcard, universal
Completion Flag	(0040,A491)	O	single value, wildcard, universal
Verification Flag	(0040,A493)	O	single value, wildcard, universal
Verifying Observer Sequence	(0040,A073)	O	Sequence matching
>Verifying Organization	(0040,A027)	O	single value, wildcard, universal
>Verifying DateTime	(0040,A030)	O	single value, range matching, universal
>Verifying Observer Name	(0040,A075)	O	single value, wildcard, universal
>Verifying Observer Identification Code Sequence	(0040,A088)	O	Sequence matching
>>Code Value	(0008,0100)	O	single value, wildcard, universal
>>Coding Scheme Designator	(0008,0102)	O	single value, wildcard, universal
>>Coding Scheme Version	(0008,0103)	O	single value, wildcard, universal
>>Code Meaning	(0008,0104)	O	single value, wildcard, universal

Supported Query attributes sorted by Query Level – Study Root Information Model

1.1.1.1.1.9 Patient/Study Only Information Model

Attribute Name	Tag	Usage SCU	Matching
Patient Level			
Patient Name	(0010,0010)	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	U	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	Single Value, Wildcard, universal
Ethnic Group	(0010,2160)	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Level			
Study Instance UID	(0020,000D)	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	Single Value, Wildcard, universal
Study Date	(0008,0020)	R	Single Value, Range, universal
Study Time	(0008,0030)	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	Single Value, universal
Patient's Weight	(0010,1030)	O	Single Value, universal
Occupation	(0010,2180)	O	Single Value, Wildcard, universal
Additional Patient History	(0010,21B0)	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	universal
Number of Study Related Instances	(0020,1208)	O	universal

Supported Query attributes sorted by Query Level – Patient/Study Only Information Model

The Find SCP returns following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901)
			(0000,0902)
	Unable to process	C001	(0000,0901)
Cancel	Matching terminated due to Cancel request	FE00	(0000,0902)
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

Real-World Activity - Move SCP

Associated Real-World Activity - Move SCP

The associated Real-World activity is to respond to retrieve requests to an SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by the C-MOVE service. Relational retrieve operation is NOT supported.

Multiple C-MOVE requests over the same association are NOT supported.

Accepted Presentation Contexts - Move SCP

The syngo MammoReport DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root		Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root		Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only		Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Note: C-MOVE Extended negotiation will NOT be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

SOP Specific Conformance Statement - Move SCP

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations is done on a different association, specified in the C-MOVE request, to transfer images to a remote SCP of the Storage Service Class. Relational retrieve operation is NOT supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section will give information about "U" marked key attributes.

The Move SCP returns following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
			(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Implementation Model Print

The Print Management Service Classes define an application-level class of services, which facilitate the printing of images on a hardcopy medium. The print management SCU and print management SCP are peer DICOM print management application entities. The *syngo* DICOM print application supports the print management DIMSE services to act as SCU.

Application Data Flow Diagram

The *syngo* DICOM network implementation acts as SCU for the print management network service. The product target Operating System is Windows XP®.

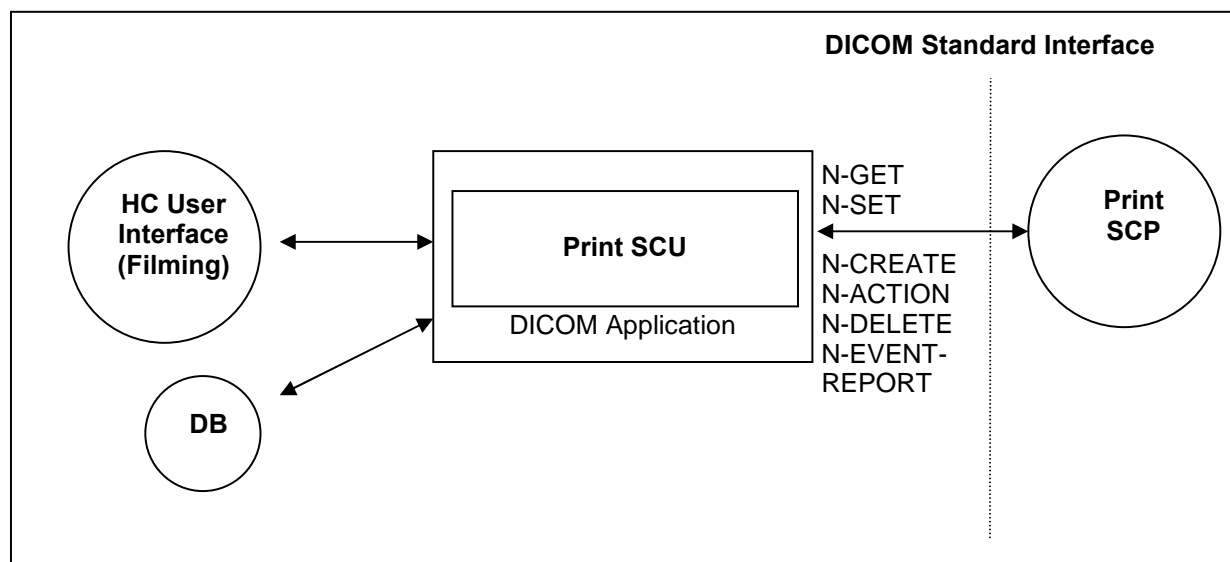


Figure 6: DICOM Application Data Flow Diagram – Print SCU

Functional Definition of Application Entities

The Print SCU is invoked by the user interface to setup film-sheet layout and whenever an image is ready to be printed on film. The Print SCU will hold and maintain all data needed to compile a complete film-sheet from the data (images, layout, configuration) received. Whenever a film-sheet is ready to print the related data is used to supply the Information to the SOP Classes of the Print Management Service Class. A queue is maintained, in order to intermediately store several film-sheets in case of resource problems on printer. The SCU will only supply and require the mandatory SOP Classes of the Print Management Service Class.

Sequencing of Real-World Activities

Not applicable

Application Entity Specification Print

Print Management AE Specification

The *syngo* print management SCU (HCS) invokes print management DIMSE services to transfer images from the local AE to the remote SCP AE to print images with defined layout on a selected network-based DICOM hardcopy printer. This is done in a “full-page” print mode.

SIEMENS *syngo* DICOM products provide Standard Conformance to the following DICOM V3.0 Print Management Meta SOP Classes as an SCU:

SOP Class Name	SOP Class UID
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
- Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4
- Printer SOP Class	1.2.840.10008.5.1.1.16
Print Job SOP Class	1.2.840.10008.5.1.1.14
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23

SOP Class Name	SOP Class UID
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
- Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1
- Printer SOP Class	1.2.840.10008.5.1.1.16
Print Job SOP Class	1.2.840.10008.5.1.1.14

1.1.1 Association Establishment Policies

General

Whenever a film is completely set up and printed by command or automatism, the job is prepared for processing. As soon as the queue is ready to process the job is activated and worked according the processing data. The related Print application will initiate an association to the print destination and process the printing of the related information.

The default PDU size used will be 28 KB.

Number of Associations

The *syngo* DICOM Print application initiates one association at a time for each different print device configured.

Asynchronous Nature

The *syngo* DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

Implementation Identifying Information

Implementation Class UID

1.3.12.2.1107.5.12

Implementation Version Name

"MBC_SCR-5-1-0"

Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. With the help of the N-GET request for the Printer SOP Class the Status is determined before printing.

With no problem encountered with the N-CREATE/N-SET Services for the related Basic Print SOP Classes the film sheet is set up for printing and the image(s) is(are) transferred to the printer device.

After the last film is printed from queue, the Print application will leave open the association for another 60 seconds. If a new film job is ready for printing within this time-limit, the job will be immediately processed over the still open association. If there is no new job, the association is closed if the time-out elapsed. This is done to optimize automated printing.

During the "idle-time" (no open association to printer) the Print application will issue a cyclic camera status request (using N-GET of Printer SOP Class) every 5 minutes.

Associated Real-World Activity

Associated Real-World Activity – Printing a Printer Job Queue Entry

Whenever a film-sheet is prepared by the user, it is forwarded to the Printer Job queue. As soon as the associated Printer device is available the job is activated and association is set up.

The film sheet is internally processed, converted to a Standard/1-1 page and then the page image is sent. Status is controlled by awaiting any N-EVENT message all through the transfer until the last image or film-sheet is sent.

If the response from the remote application contains a status other than Success or Warning the association is aborted.

Proposed Presentation Context (Presentation Context Table)

The Siemens *syngo* DICOM Print application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		

Basic Grayscale Print Management Meta SOP class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Color Print Management Meta SOP class	1.2.840.10008.5.1.1.18	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic film session SOP class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Film Box SOP class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Grayscale Image Box SOP class	1.2.840.10008.5.1.1.4	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Color Image Box SOP class	1.2.840.10008.5.1.1.4.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Printer SOP class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Print Job SOP class	1.2.840.10008.5.1.1.14	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Presentation LUT SOP class	1.2.840.10008.5.1.1.23	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

SOP specific Conformance Statement – Meta SOP Classes

The *syngo* DICOM print management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class and the Basic Color Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM SCP, e.g.:

- maximum number of print jobs in the queue
- maximum number of print copies
- supported film sizes of the connected DICOM SCP
- supported film formats of the DICOM SCP
- lookup table definition.

The printing is only suspended in the case of a failure return status of the SCP.

1.1.1.1.10 Basic Film Session SOP class

The Basic Film Session information object definition describes all the user-defined parameters, which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes and that are printed on one hardcopy printer.

The *syngo* DICOM print management SCU supports the following DIMSE Service elements for the Basic Film Session SOP Class as SCU:

- N-CREATE, N-DELETE

The Basic Film Session SOP Class N-CREATE-RQ (SCU) uses the following attributes:

Attribute Name	Tag	Usage SCU	Supported Values
Number of Copies	(2000,0010)	U	1
Medium Type	(2000,0030)	U	BLUE FILM CLEAR FILM PAPER
Film Destination	(2000,0040)	U	MAGAZINE PROCESSOR

The number of Copies sent to the DICOM Printer is always 1, the job is sent n times for n copies.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session – see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) → (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session

The N-DELETE-RQ on the Basic Film Session SOP Class is used to remove the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

Service Status	Meaning	Error Codes
Failed	Film session SOP instances hierarchy does not contain film box SOP instances	C600
	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603
Warning	Memory allocation not supported	B600
	Film session printing is not supported	B601
	Film box does not contain image box (empty page)	B602
Success	Film belonging to the film session are accepted for printing	0000

1.1.1.1.1.11 Basic Film Box SOP class

The Basic Film Box information object definition describes all the user-defined parameter of one film of the film session. The Basic Film Box information description defines the presentation parameters, which are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported Service Elements as SCU are:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP class N-CREATE-RQ message uses the following attributes (the actual values for each attribute depend on DICOM printer configuration within the *syngo* DICOM print management SCU):

Attribute Name	Tag	Usage SCU	Supported Values
Image Display Format	(2010,0010)	M	STANDARD\1,1
Referenced Film Session Sequence	(2010,0500)	M	
> Referenced SOP Class UID	(0008,1150)	M	1.2.840.10008.5.1.1.1
> Referenced SOP Instance UID	(0008,1155)	M	
Film Orientation	(2010,0040)	M	PORTRAIT

Film Size ID	(2010,0050)	M	8INX10IN, 10INX12IN, 10INX14IN, 11INX14IN,, 14INX14IN, 14INX17IN, 24CMX24CM, 24CMX30CM
Magnification Type	(2010,0060)	M	BILINEAR, CUBIC, NONE, REPLICATE
Border Density	(2010,0100)	U	BLACK, WHITE
Max Density	(2010,0130)	U	0 < Value
Min Density	(2010,0120)	U	0 < Value < 50
Illumination	(2010,015E)	U	0 < Value Required if Presentation LUT is present.
Reflective Ambient Light	(2010,0160)	U	0 < Value Required if Presentation LUT is present.
Referenced Presentation LUT Sequence	(2050,0500)	U	

For Page Mode printing, the Image Display format used is Standard\1,1. For Image Mode Printing, the Image Display format used is Standard\C,R where C is the number of Columns and R is the number of Rows as specified in the Hardcopy Layout.

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with SOP Class/Instance UID pairs which will be kept internally to be further used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film-sheet have been set, the *syngo* DICOM print manager will issue a N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Box - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) → (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box

The Basic Film Box SOP class interprets the following status codes:

Service Status	Meaning	Error Codes
Failure	Unable to create print job, print queue is full	C602
	Image size is larger than images box size	C603
Warning	Film box does not contain image box (empty page)	B603
	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success	Film accepted for printing	0000

1.1.1.1.12 Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Grayscale Image Box SOP Class uses only the N-SET-RQ with the following attributes:

Attribute Name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
BASIC Grayscale Image Sequence	(2020,0110)	M	
> Samples per Pixel	(0028,0002)	M	1
> Photometric Interpretation	(0028,0004)	M	MONOCHROME2
> Rows	(0028,0010)	M	

Attribute Name	Tag	Usage SCU	Supported Values
> Columns	(0028,0011)	M	
> Pixel Aspect Ratio	(0028,0034)	M	
> Bits Allocated	(0028,0100)	M	8/16
> Bits Stored	(0028,0101)	M	8,12
> High Bit	(0028,0102)	M	7,11
> Pixel Representation	(0028,0103)	M	0
> Pixel Data	(7FE0,0010)	M	

The Grayscale Image Box SOP class interpret the following status codes:

Service Status	Meaning	Error Codes
Failure	Image contains more pixel than printer can print in Image Box	C603
Warning	Insufficient memory in printer to store the image Requested MinDensity or MaxDensity outside of Printer's operating range	C605 B605
Success		0000

1.1.1.1.13 Basic Color Image Box SOP Class

The Basic Color Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Color Image Box SOP Class uses only the N-SET-RQ with the following attributes:

Attribute Name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
BASIC Color Image Sequence	(2020,0111)	M	
> Samples per Pixel	(0028,0002)	M	3
> Photometric Interpretation	(0028,0004)	M	RGB
> Planar Configuration	(0028,0006)	M	0
> Rows	(0028,0010)	M	
> Columns	(0028,0011)	M	
> Pixel Aspect Ratio	(0028,0034)	M	
> Bits Allocated	(0028,0100)	M	8
> Bits Stored	(0028,0101)	M	8
> High Bit	(0028,0102)	M	7
> Pixel Representation	(0028,0103)	M	0
> Pixel Data	(7FE0,0010)	M	

The Color Image Box SOP class interpret the following status codes:

Service Status	Meaning	Error Codes
Failure	Image contains more pixel than printer can print in Image Box	C603
Warning	Insufficient memory in printer to store the image Image size larger than image box size	C605 B604
Success		0000

1.1.1.1.14 Presentation LUT SOP Class

The objective of the Presentation LUT is to realize image hardcopy printing tailored for specific modalities, applications and user preferences.

The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

The Presentation LUT SOP Class uses only the N-CREATE-RQ with the following attributes:

Attribute Name	Tag	Usage SCU	Supported Values
Presentation LUT Shape	(2050,0020)	U	IDENTITY

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and is used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ) - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) → (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Presentation LUT

The Presentation LUT SOP class interprets the following status codes:

Service Status	Meaning	Error Codes
Warning	Requested MinDensity or MaxDensity outside of HCD's operating range. HCD will use its respective minimum or maximum density value instead.	B605
Success	Presentation LUT successfully created	0000

1.1.1.1.1.15 Printer SOP Class

The Printer SOP Class is the possibility to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The SCU uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way.

It can directly ask the Printer (SCP) for its status or receive Events from the Printer asynchronously:

- N-GET as SCU

N-EVENT-REPORT as SCU In both cases the following information is supported:

Used Printer N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

Attribute Name	Tag	Usage SCP	Supported Values
Printer Status	(2110,0010)	M	NORMAL, FAILURE, WARNING
Printer Status Info	(2110,0020)	M	See tables in Annex for details.

Note: For a detailed description on how syngo reacts on different printer status messages, please refer to the Annex section "DICOM Print SCU – detailed status displays".

1.1.1.1.1.16 Print Job SOP Class

The Print Job SOP Class is the possibility to monitor the execution of the print process.

The *syngo* DICOM Print Management application supports the optional N-EVENT-REPORT DICMSE Service to receive the changes of the Print Job Status in an asynchronous way.

It can receive Events from the Print SCP asynchronously

Note: *syngo* does not support receiving N-EVENT from camera during print sessions, normally this is configurable in the camera.

N-EVENT-REPORT The following information is supported:

Used Print Job N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1	Execution Status Info	(2100,0030)	U
				--
		Print Job ID	(2100,0010)	(Print Queue Management SOP Class not supported)
Printing	2	Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
				--
		Print Job ID	(2100,0010)	(Print Queue Management SOP Class not supported)
Done	3	Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
				--
		Print Job ID	(2100,0010)	(Print Queue Management SOP Class not supported)
Failure	4	Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
				--
		Print Job ID	(2100,0010)	(Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U

Note: For a detailed description on how *syngo* reacts on different printer status messages, please refer to the Annex section "DICOM Print SCU – detailed status displays".

Association Acceptance Policy

Not applicable

Communication Profiles

Supported Communication Stacks

The Siemens *syngo* MammoReport DICOM application provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.
The product target Operating System is Windows XP®.

TCP/IP Stack

The *syngo* MammoReport DICOM application uses the TCP/IP stack from the target operating system upon which it executes. It uses the MergeCOM-3 subroutine library from Merge Technologies Inc. that is based on a Berkeley socket interface.

API

The *syngo* MammoReport DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

Physical Media Support

The *syngo* MammoReport DICOM application is indifferent to the physical medium over which TCP/IP executes; it inherits this from the target operating system upon which it executes.

Extensions / Specializations / Privatizations

Standard Extended / Specialized / Private SOPs

Please refer to Annex for further information on these topics. A detailed overview is given there.

Private Transfer Syntaxes

Not applicable

Configuration

AE Title/Presentation Address Mapping

To ensure unique identification within the network the hostname should be used as part of the AE Titles (see examples below, hostname = name1). The string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters) are allowed according to DICOM Standard.

Note: the current implementation of syngo does not support the full DICOM Standard. Spaces and special characters (like &<> ") in the AE title string are not supported.

DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. E.g. Verification will use the Storage AE, if initiated to check the configuration of a remote DICOM node.

DICOM Storage AE Title

Within syngo there are local application entity titles for HIS/RIS, Study Transfer and Print. They can be configured via Service-UI in Configuration / DICOM / General (e.g. STU_NAME1).

The port number is set to the default value of 5104.

DICOM Query/Retrieve AE Title

The DICOM Query/Retrieve application uses the same application entity title as the DICOM Storage AE.

DICOM Print AE Title

The DICOM Print application provides the application entity title:

e.g. PRI_NAME1 *(No input of AETs starting with a numeric character is possible)*

Configurable Parameters

The Application Entity Titles, host names and port numbers for remote AE are configured using the syngo MammoReport Service/Installation Tool. For each AET the list of services supported can be configured.

Storage, Storage Commitment and Query/Retrieve

The *syngo* MammoReport Service/Installation Tool can be used to set the AETs, port-numbers, host-names, IP-addresses and capabilities for the remote nodes (SCPs). The user can select transfer syntaxes, compression modes and query models for each SCP separately.

- a quality factor which determines the proposed transfer syntax in case that an user has initiated the C-STORE. By convention, 0 means: Only Uncompressed Transfer Syntax(es) are proposed, 100 means: Lossless Transfer Syntax is proposed, and any other value between 1 and 99 means that an JPEG Lossy Transfer Syntax is proposed. One Uncompressed Transfer Syntax will be proposed in any case. This parameter is general for all destination nodes.
- a "compression type supported" which determines the proposed transfer syntax in case that the C-STORE was initiated as a sub-operation of an incoming C-MOVE-RQ. By convention, 0 means: Only Uncompressed Transfer Syntax(es) are proposed, 1 means: Lossless Transfer Syntax is proposed, and 2 means that an JPEG Lossy Transfer Syntax is proposed. One uncompressed transfer syntax will be proposed in any case. This parameter can be set for each configured destination node.

Note:

y default association requests are accepted by the SCP regardless of the value of DICOM Application Context Name set in the requests.

This behavior can be changed by modifying the value of the entry `ACCEPT_ANY_CONTEXT_NAME` in the configuration file `mergecom.pro` of MergeCOM-3 Tool Kit. If the value is `FALSE`, association requests are accepted only when DICOM Application Context Name is set to "1.2.840.10008.3.1.1.1" (see DICOM specification PS 3.7-2003, A.2.1)

Additional configurable parameters for Storage Commitment are:

When acting as SCU:

- flag to indicate whether the association will be kept open to receive the response or to close the association and be prepared to receive the response on another association.
- time-out which defines how long the association of N-ACTION is kept to receive a N-EVENT-REPORT on the same association. The same value is used to wait for an N-EVENT-REPORT on an other association. (default 1 h)

When acting as SCP:

- flag to indicate if an archive system is installed

Print

The *syngo* MammoReport Service/Installation Tool can be used to configure the SCP (DICOM-Printer).

These parameters are mandatory to set:

- AET,
- host-name,
- IP-address and
- Port-number.

These parameters have defaults as per configuration file and can be changed:

- default camera (yes/no),
- pixel size,
- additional or changed film sheet formats (e.g. inch 14x14, inch 14x17, ...),
- list with mapping pixel size to each film sheet format,

- minimal density,
- stored printed film jobs,
- media type,
- film destination.

Modality Worklist

The Service application can be used to set the AETs, port numbers, host names, IP addresses, capabilities and time-outs for the remote nodes (SCPs)

Additional configurable parameters for Modality Worklist Query are:

- Query Waiting time - the time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default 20 sec.)
- Max Query Match Number - the maximum number of entries accepted in one worklist (default is 200)
- Query Interval: the time between two C-FIND-RQ to the Hospital Information system (default is 60 min.)
- Broad Worklist Query behaviour (two values are defined):
 - Set the AE Title search attribute to the own AE Title, and the Modality search attribute to “*”.
 - Set the Modality search attribute to the own modality and the AE Title search attribute to “*”.

Default Parameters

This installation tool also uses some default parameters:

- max PDU size set to 262144 Bytes (256 kB)
- time-out for accepting/rejecting an association request: 60 s
- time-out for responding to an association open/close request: 60 s
- time-out for accepting a message over network: 60 s
- time-out for waiting for data between TCP/IP-packets: 60 s

The time-outs for waiting for a Service Request/Response message from the remote node are as follows:

- for Storage SCP/SCU: 600 s
- for Storage Commitment SCU:
time-out for Response to N-ACTION: 600 s
- for Query/Retrieve SCP/SCU: 600 s
- for Print Management SCU:
 - time-out for Response to N-SET-RQ: 240 s
 - time-out for Response to other Requests: 60 s

Support of Extended Character Sets

The *syngo* MammoReport DICOM application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?'.

Media Storage Conformance Statement

This chapter will contain the Conformance Statement to all “Offline Media Application Profiles (incl. private extensions)” supported by the *syngo* MammoReport archive options.

Those application profiles supported shall be:

- Standard Application Profiles
- *syngo* private Application Profile
- General Purpose CDR Profile

Introduction

Purpose

This DICOM Conformance Statement is written according to part PS 3.2 of [1].

The applications described in this conformance statement are the SIEMENS *syngo* MammoReport based on *syngo*® software⁺⁺⁺. The *syngo* MammoReport DICOM offline media storage service implementation acts as FSC, FSU and/or FSR for the specified application profiles and the related SOP Class instances.

Scope

This DICOM Conformance Statement refers to SIEMENS *syngo* MammoReport based products using *syngo* MammoReport software. The following table relates *syngo* MammoReport software names to SIEMENS products:

Software Name	SIEMENS <i>syngo</i> -based Product
SCR-SIE-3-2-1 / VB23	<i>syngo</i> MammoReport

Definitions, Abbreviations

Definitions

DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite information objects

Abbreviations

ACR	American College of Radiology
AE	DICOM Application Entity
ASCII	American Standard Code for Information Interchange
DB	Database
DCS	DICOM Conformance Statement
FSC	File Set Creator
FSR	File Set Reader
FSU	File Set Updater
IOD	DICOM Information Object Definition
ISO	International Standard Organization
LEONARDO	AX-Workstation (for Angiographic/Radiographic viewing)
MOD	Magneto-optical Disk
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
RWA	Real-World Activity
U	Unique Key Attribute

References

- [1] Digital Imaging and Communications in Medicine (DICOM) 3.0, NEMA PS 3.1-18, 2006

⁺⁺⁺ *syngo* is a registered trademark of Siemens AG.

Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.


The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

Implementation Model

Application Data Flow Diagram

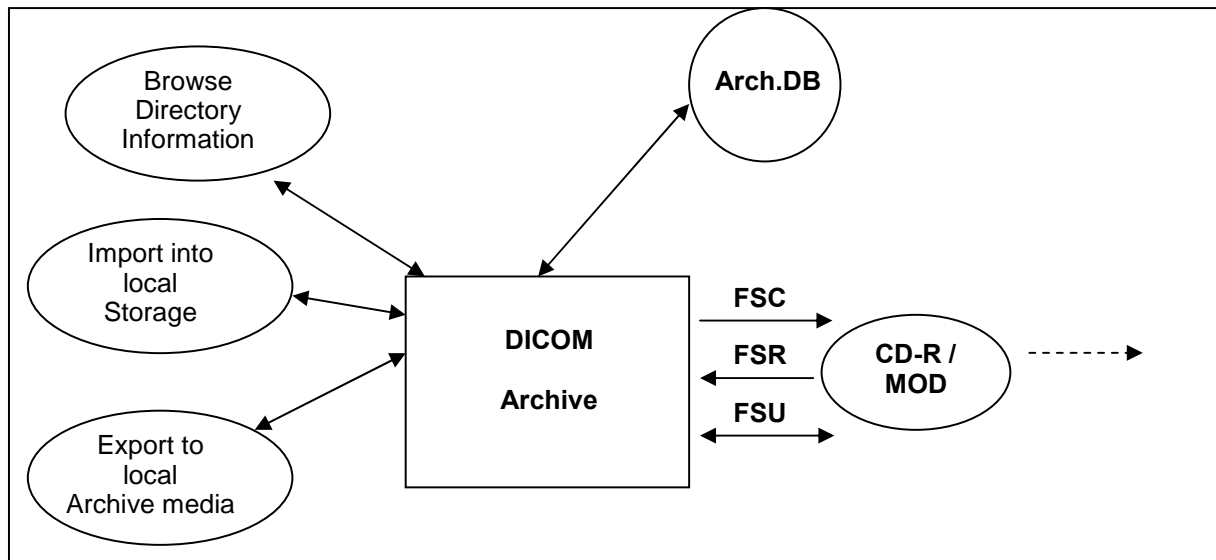

The DICOM archive application will serve as an interface to the CD-R offline medium device. It serves interfaces to include the offline media directory into the browser and to copy SOP instances to a medium or retrieve SOP Instances from medium into local storage.

The DICOM Archive application will support the 120mm CD-R medium, the 130mm 2.3 GB R/W MOD.

The FSU role will update new SOP Instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will be temporarily stored in Archive-Database.

Functional Definitions of AEs

The *syngo* MammoReport DICOM offline media storage application consists of the DICOM Archive application entity serving all interfaces to access offline media. The DICOM Archive application is capable of

1. creating a new File-set onto an unwritten medium (Export to...).
2. updating an existing File-set by writing new SOP Instances onto the medium (Export to...).
3. importing SOP Instances from the medium onto local storage
4. reading the File-sets DICOMDIR information into temporary database and pass it to display applications.

Sequencing of Real-World Activities

The DICOM Archive application will not perform updates before the Directory information of the DICOMDIR is completely read.

When performing updates, the SOP instances are checked for existence before updating. Duplicate instances will be avoided.

File Meta Information Options

Implementation Class UID

1.3.12.2.1107.5.12

Implementation Version Name

"MBC_SCR-5-1-0"

AE Specifications

DICOM Archive Specification

The DICOM Archive provides Standard conformance to Media Storage Service Class (Interchange Option). In addition augmented conformance is provided to store extra data attributes important for the full feature support of the *syngo* MammoReport. Details are listed in following Table:

Application Profiles Supported	Real-World Activity	Role	SC Option
AUG-STD-GEN-CD AUG-STD-XA1K-CD	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange
	Export to local Archive Media	FSC, FSU	Interchange
STD-GEN-CD STD-CTMR-CD STD-XA1K-CD STD-US-zz-yF-xxxxxx *2	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange

*2 - All combinations of the following values for zz, yF and xxxxxx are supported: yF={SF|MF}, zz={ID|SC|CC}

On syngo-based products the augmented profiles will be preferably used by the system. The General Purpose Interchange Profile (STD-GEN-CD), Ultrasound Profile (STD-US-xxx), CT and MR Image Profile (STD-CTMR-xxx) and 1024 X-Ray Angiographic Profile (STD-XA1K-CD) will be supported with read capability of the related media.

File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See Chapter "Configuration" for details.

Real-World Activities for this Application Entity

Real-World Activity: Browse Directory Information

The DICOM Archive application acts as FSR using the interchange option when requested to read the media directory.

The DICOM archive application will read the DICOMDIR and insert those directory entries, that are valid for the application profiles supported, into a local database. The database can then be used for browsing media contents.

- Note

IconImageSQ is also supported in DICOMDIR. But only those Icon Images with BitsAllocated (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

Application Profiles for the RWA: Browse Directory Information

See Table in section 3.1 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

Real-World Activity: Import into local Storage

The DICOM Archive application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the local storage.

The SOP Instance selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported and are listed as supported by the Storage SCP Conformance section (Network DCS, 5.1.3), can be retrieved from media storage. This is due to the fact that the Browse Directory Information will filter all SOP Instances not matching the Application profiles supported.

During operation no “Attribute Value Precedence” is applied to the SOP Instances. Detached Patient Management is not supported (please refer to DICOM Part 11, Media Storage Application Profiles).

For media conforming to the STD-GEN-CD Profile the following SOP classes will be supported as an FSR:

Information Object Definition	SOP Class UID	Transfer Syntax UID
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CT image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image-For Processing	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image-For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image-For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image-For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CSA Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Application Profiles for the RWA: Import into local Storage

See Table in section 0 for the Application Profiles listed that invoke this Application Entity for the Import into Local Storage RWA.

Real-World Activity: Export to local Archive Media

The DICOM Archive application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium.

The DICOM Archive application will receive a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

When the DICOM archive application is requested to copy SOP Instances the preferred application profile according configuration will be used to validate and copy the referred SOP Instances. When creating a new file-set no Descriptor File will be allocated and the related ID is not used.

The DICOM archive application will not close the medium.

Application Profiles for the RWA: Export to local Archive Media

See Table in section 0 for the Application Profiles listed that invoke this Application Entity for the Export to local Archive Media RWA.

2 Augmented and Private Profiles

Augmented Application Profiles

AUG-GEN-CD

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-GEN-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

The Siemens non-image is typically used for raw data and 3D private data.

AUG-CTMR-xxxxx

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-CTMR-MOD650, STD-CTMR-MOD12, STD-CTMR-MOD23 and STD-CTMR-CDR Standard Profiles.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

AUG-XA1K-CD

With no private Siemens Non-Images stored onto Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-XA1K-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see other section).

syngo® private offline Media Application Profile

Will contain a *syngo* specific Application Profile.

Structure of this Application Profile is defined in Part 11 of the 2000 DICOM Standard.

It is needed to describe the requirements for Offline Media Storage of the private IOD (Non-Image IOD).

Class and Profile Identification

This document defines an Application Profile Class for “*syngo*® speaking^a” modalities or applications.

The identifier for this class shall be PRI-SYNGO. This class is intended to be used for interchange of extended and private Information Objects via CD-R or re-writeable magneto-optical disk (MOD) offline media between dedicated acquisition or workstation modalities build from a common *syngo* architecture.

^a *syngo* is a registered trademark of Siemens AG.

The specific application profiles in this class are shown in Table below:

Application Profile	Identifier	Description
"syngo speaking" System on CD-R	PRI-SYNGO-CD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD).
"syngo speaking" System on 2.3 GB MOD	PRI-SYNGO-MOD23	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD).
"syngo speaking" System on 4.1 GB MOD ^a	PRI-SYNGO-MOD41	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD).
"syngo speaking" System on DVD R	PRI-SYNGO-DVD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD).

Equipment claiming conformance for this syngo Application Profile Class shall make a clear statement on handling of the private defined SOP Instances.

Clinical Context

This application profile facilitates the interchange of original acquired and derived images and private data related to them. Typical media interchange would be from in-lab acquisition equipment to dedicated workstations and archive systems with specific extensions to handle the private data objects (in both directions).

Additionally, images (from MR,CT,US,NM,DX,RF) used to prepare procedures, multi-modality images (e.g. integrated US) and images derived from primary diagnostic images, such as annotations, quantitative analysis images, reference images, screen capture images may be interchanged via this profile.

Roles and Service Class Options

This Application Profile uses the Media Storage Service Class defined in PS 3.4 with the Interchange Option.

The Application Entity shall support one or more of the roles of File Set Creator (FSC), File Set Reader (FSR), and File Set Updater (FSU), defined in PS 3.10.

File Set Creator

The Application Entity acting as a File-Set Creator generates a File Set under the PRI-SYNGO Application Profiles.

File Set Creators shall be able to generate the Basic Directory SOP Class in the DICOMDIR file with all the subsidiary Directory Records related to the Image SOP Classes and Private SOP Classes stored in the File Set.

In case of the PRI-SYNGO-CD profile, the FSC shall offer the ability to either finalize the disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc). In case of the PRI-SYNGO-DVD profile only multi-session is supported. For both profile a multi-session media can be finalized.

Note

A multiple volume (a logical volume that can cross multiple physical media) is not supported by this Application Profile Class. If a set of Files, e.g., a Study, cannot be written entirely on one CD-

^a Definition of this profile is done due to approval of DICOM Supplement 62.

R, the FSC will create multiple independent DICOM File-Set such that each File-Set can reside on a single CD-R medium controlled by its individual DICOMDIR file. The user of the FSC can opt to use written labels on the discs to reflect that there is more than one disc for this set of files (e.g., a Study).

File Set Reader

The role of the File Set Reader shall be used by Application Entities which receive the transferred File Set.

File Set Readers shall be able to read all the defined SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, using all the defined Transfer Syntaxes.

File Set Updater

The role of the File Set Updater shall be used by Application Entities, which receive a transferred File Set and update it by the addition of processed information.

File Set Updaters shall be able to read and update the DICOMDIR file. File-Set Updaters do not have to read the image/private information objects. File-Set Updaters shall be able to generate any of the SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, and to read and update the DICOMDIR file.

In case of the PRI-SYNGO-CD profile, the FSU shall offer the ability to either finalize a disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc). In case of the PRI-SYNGO-DVD profile only multi-session is supported. For both profile a multi-session media can be finalized.

Note (for CD-R and DVD-R)

If the disc has not been finalized, the File-Set Updater will be able to update information assuming there is enough space on the disc to write a new DICOMDIR file, the information, and the fundamental CD-R/DVD-R control structures. CD-R/DVD-R control structures are the structures that inherent to the CD-R/DVD-R standards; see PS 3.12

PRI-SYNGO Profiles

SOP Classes and transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option. In the table below Transfer Syntax UID "RLE Lossless " applies only for decompression.

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
Basic Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	M
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
CR Image	1.2.840.10008.5.1.4.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
CT image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
DX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
DX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
MG Image – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MG Image – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
MG Image – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
MG Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
IOX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
IOX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
IOX Image – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
IOX Image – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MR Image	1.2.840.10008.5.1.4.1.1.4	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed	M	M	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
		1.2.840.10008.1.2.1			
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	O	O
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	O	O
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	-	M	-
Ultrasound Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	-	M	-
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50	O	M	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
		1.2.840.10008.1.2.4.51			
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	M	O
Ultrasound Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	M	O
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	-	M	-
Ultrasound Multi-frame Image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	-	M	-
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	M	O
Ultrasound Multi-frame Image	1.2.840.10008.5.1.4.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	M	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	M	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50	O	O	O

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR	FSU
		1.2.840.10008.1.2.4.51			
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90	O	M	O
X-Ray Radiofluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91	O	M	O
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1 1.2.840.10008.5.1.4.1.1.9.1.2 1.2.840.10008.5.1.4.1.1.9.1.3 1.2.840.10008.5.1.4.1.1.9.2.1 1.2.840.10008.5.1.4.1.1.9.3.1 1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1 1.2.840.10008.5.1.4.1.1.9.1.2 1.2.840.10008.5.1.4.1.1.9.1.3 1.2.840.10008.5.1.4.1.1.9.2.1 1.2.840.10008.5.1.4.1.1.9.3.1 1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.1 1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.1 1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.2 2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.2 2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.3 3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.3 3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.5 0	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.5 0	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.6 5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.6 5	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CSA Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O

FSC, FSR, FSU – denote the requirements for those roles

O – Optional

M - Mandatory

Physical Media and Formats

The PRI-SYNGO-CD Profile requires the 120mm CD-R physical media with the ISO/IEC 9660 Media Format, as defined in PS3.12.

The PRI-SYNGO-DVD Profile requires the 120mm DVD physical media with the UDF 2.01 Media Format, as defined in PS3.12.

The PRI-SYNGO-MOD23 Profile requires the 130mm 2.3 GB R/W MOD physical medium with the PC DOS Media Format, as defined in PS3.12.

The PRI-SYNGO-MOD41 Profile requires the 130mm 4.1 GB R/W MOD physical medium with the PC DOS Media Format, as defined in PS 3.12.

The PRI-SYNGO-FD Profile requires the 1.44 MB diskette physical medium with the PC DOS Media Format, as defined in PS3.12.

Directory Information in DICOMDIR

Conforming Application Entities shall include in the DICOMDIR File the Basic Directory IOD containing Directory Records at the Patient and subsidiary levels appropriate to the SOP Classes in the File-set. All DICOM files in the File-set incorporating SOP Instances defined for the specific Application profile, shall be referenced by Directory Records.

Note

DICOMDIRs with no directory information are not allowed by this Application Profile

Privately defined IODs will be referenced by "PRIVATE" Directory Records.

Basic Directory IOD Specialization

This Application Profile makes use of optional attributes of the Basic Directory IOD to support recognition of Patient's Storage Service request results in spanning multiple volumes (file sets). Therefore the File Set Descriptor File can be used and is then referenced by optional Basic Directory IOD attributes. If existent, the specified Descriptor File may be used by FSR applications. Any FSU, FSC shall make a clear Statement if the Descriptor File mechanism is used according to the specialization defined in this Application Profile.

The Descriptor Files shall have the following contents:

One single Line without any control-characters and according to the Basic Character-Set having the following defined text:

"MULTIVOLUME: xx of yy"

xx, yy are replaced by the actual Number of the volume (xx) and the Total Number of Volumes in the set (yy).

If used, the Descriptor File shall have the File ID "README" and reside in same directory level as the DICOMDIR. It is referenced by the attribute [0004,1141] File-set Descriptor File ID having the defined content of "README".

Additional Keys

File-set Creators and Updaters are required to generate the mandatory elements specified in PS 3.3, Annex F of the DICOM Standard. Table below: Additional DICOMDIR Keys specifies the additional associated keys. At each directory record level other additional data elements can be added, but it is not required that File Set Readers be able to use them as keys. Refer to the Basic Directory IOD in PS 3.3.

Key Attribute	Tag	Directory Record Level	Type	Notes
Date of Birth	(0010,0030)	PATIENT	2C	required, if present in SOP Instance
Patient's Sex	(0010,0040)	PATIENT	2C	required, if present in SOP Instance

Key Attribute	Tag	Directory Record Level	Type	Notes
Series Date	(0008,0021)	SERIES	3	
Series Time	(0008,0031)	SERIES	3	
Institute Name	(0008,0080)	SERIES	2C	required, if present in SOP Instance
Institution Address	(0008,0081)	SERIES	2C	required, if present in SOP Instance
Series Description	(0008,103E)	SERIES	3	
Performing Physician's Name	(0008,1050)	SERIES	2C	required, if present in SOP Instance
Image Type	(0008,0008)	IMAGE	1C	required, if present in SOP Instance
SOP Class UID	(0008,0016)	IMAGE	3	
SOP Instance UID	(0008,0018)	IMAGE	3	
Content Date	(0008,0023)	IMAGE	3	
Content Time	(0008,0033)	IMAGE	3	
Referenced Image Sequence	(0008,1140)	IMAGE	1C	required, if present in SOP Instance
> Referenced SOP Class UID	(0008,1150)			
> Referenced SOP Instance UID	(0008,1155)			
Image Position (Patient)	(0020,0032)	IMAGE	2C	required, if present in SOP Instance
Image Orientation (Patient)	(0020,0037)	IMAGE	2C	required, if present in SOP Instance
Frame of Reference UID	(0020,0052)	IMAGE	2C	required, if present in SOP Instance
Rows	(0028,0010)	IMAGE	3	
Columns	(0028,0011)	IMAGE	3	
Pixel Spacing	(0028,0030)	IMAGE	1C	required, if present in SOP Instance
Calibration Image	(0050,0004)	IMAGE	2C	required, if present in SOP Instance
Icon Image Sequence	(0088,0200)	IMAGE	3	required for Image SOP Classes
> Samples per Pixel	(0028,0002)			1
> Photometric Interpretation	(0028,0004)			MONOCHROME2
> Rows	(0028,0010)			64 , 128
> Columns	(0028,0011)			64 , 128
> Bits Allocated	(0028,0100)			8
> Bits Stored	(0028,0101)			8
> High Bit	(0028,0102)			7
> Pixel Representation	(0028,0103)			0
> Pixel Data	(7FE0,0010)			Icon Image
Curve Number	(0020,0024)	CURVE	1C	required, if present in SOP Instance

Private Directory Record Keys

Private Directory Records are supported by this Application Profile Class at the following Level - IMAGE. The PRIVATE Directory Records will have required elements in addition to the mandatory elements specified in PS 3.3.

The following table will list the additional required keys for PRIVATE Directory Records:

Key Attribute	Tag	Directory Record Level	Type	Notes
Private Record UID	(0004,1432)	PRIVATE	1	See Conformance Statement
SOP Class UID	(0008,0016)	PRIVATE	1C	required, if present in SOP Instance
SOP Instance UID	(0008,0018)	PRIVATE	1C	required, if present in SOP Instance
Image Type	(0008,0008)	PRIVATE	3	
Acquisition Date	(0008,0022)	PRIVATE	3	
Acquisition Time	(0008,0032)	PRIVATE	3	
Acquisition Number	(0020,0012)	PRIVATE	3	
CSA Data Type	(0029,xx08)	PRIVATE	1	private owner code = SIEMENS CSA NON-IMAGE
CSA Data Version	(0029,xx09)	PRIVATE	3	private owner code = SIEMENS CSA NON-IMAGE

Icon Images

Directory Records of type SERIES or IMAGE may include Icon Images. The Icon Image pixel data shall be as specified in PS 3.3 "Icon Image Key Definition", and restricted such, that Bits Allocated (0028,0100) and Bits Stored (0028,0101) shall be equal 8, and Rows (0028,0010) and Columns (0028,0011) shall be equal to 128 for XA Images and 64 for all other Images. The Photometric Interpretation (0028,0004) shall always be restricted to "MONOCHROME2".

Extensions, Specialization and Privatization of SOP Classes and Transfer Syntaxes

The SOP Classes listed refer in majority to those created by the equipment to which this conformance Statement is related to. For SOP classes not listed in this section, please refer to the Storage section of the DICOM Conformance Statement of the product. This will include all SOP Instances that can be received and displayed and therefore will be included into offline media storage even though these SOP Instances are not created by the equipment serving the Media Storage Service.

SOP Specific Conformance Statement for Basic Directory

Extension, Specialization for SIEMENS Non-Image Objects

According to the PRI-SYNGO Application Profile Class the usage of the Private Creator UIDs and further optional keys for the Directory Records referring to SIEMENS Non-Image Objects are listed in the following tables.

Attribute	Tag	Value used
Private Record UID	(0004,1432)	1.3.12.2.1107.5.9.1
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1

For those “Non-Images” no Icon Image Sequence will be generated.

Configuration

AE Title Mapping

DICOM Media Storage AE Title

The DICOM Storage application provides the application entity title:

CsalmageManager

Support of Extended Character Sets

The Siemens *syngo* MammoReport DICOM archive application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?’.

ImageRouting Conformance Statement

This chapter contains the Conformance Statement for the Image Routing part of the *syngo* MammoReport.

Image Routing is used to distribute incoming DICOM images and related information to other DICOM nodes. It implements the necessary DICOM services to receive and store images and related information from / to networked devices.

For completeness of the DICOM standard conformance ImageRouting answers Verification requests.

SOP Classes	User of Service SCU	Provider of Service
Verification	No	Yes

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Secondary Capture Image Storage	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image Storage	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage	Yes	Yes
Computed Radiography Image Storage	Yes	Yes
CT Image Storage	Yes	Yes
Enhanced CT Image Storage	Yes	Yes
Digital X-Ray Image Storage – For Presentation	Yes	Yes
Digital X-Ray Image Storage – For Processing	Yes	Yes
Digital Mammography X-Ray Image Storage – For Presentation	Yes	Yes
Digital Mammography X-Ray Image Storage – For Processing	Yes	Yes
MR Image Storage	Yes	Yes
Enhanced MR Image Storage	Yes	Yes
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
<i>Ultrasound Image Storage (Retired)</i>	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Positron Emission Tomography Image Storage	Yes	Yes
Grayscale Softcopy Presentation State Storage	Yes	Yes
Mammography CAD SR Storage	Yes	Yes
Enhanced SR Storage	Yes	Yes
Key Object Selection Document SOP Class	Yes	Yes

Only the SOP Classes mentioned above are supported.

Introduction

Purpose

This DICOM Conformance Statement is written according to part PS 3.2 of [1].

The applications described in this conformance statement are the SIEMENS *syngo* MammoReport Image Routing based on *syngo*® software^a.

Scope

This DICOM Conformance Statement refers to SIEMENS *syngo* MammoReport based products using *syngo* MammoReport software. The following table relates *syngo* MammoReport software names to SIEMENS products:

Software Name	SIEMENS <i>syngo</i> -based Product
SCR-SIE-5-1-0 / VB40	<i>syngo</i> MammoReport

Definitions, Abbreviations

Definitions

100BASE-T Ethernet	Computer networking technology standardized by IEEE
10BASE-T Ethernet	Computer networking technology standardized by IEEE
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite information objects

Abbreviations

AE	Application Entity
IEEE	Institute of Electrical and Electronics Engineers
IOD	Information Object Definition
PACS	Picture Archive and Communication System
SCP	Service Class Provider
SCU	Service Class User
SOP	Service Object Pair
TCP/IP	Transmission Control Protocol / Internet Protocol
UID	Unique Identifier

References

- [1] Digital Imaging and Communications in Medicine (DICOM) 3.0, NEMA PS 3.1-18, 2009

The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>

Remarks

A DICOM conformance statement – the structure and content of which are stipulated by the DICOM standard – is intended to aid in determining the suitability of interconnecting digital imaging devices. References to specific functionality in a conformance statement are not sufficient to guarantee interoperability between components. The following should be considered when evaluating interoperability:

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.


- The *syngo* MammoReport ImageRouting conformance statement provides a starting point for ascertaining whether the product can communicate with other systems.

^a *syngo* is a registered trademark of Siemens AG.

- The only way to know for certain whether *syngo* MammoReport ImageRouting can interoperate with other systems is to perform connectivity tests.
- This document represents a best effort to document the functionality of commercial versions of *syngo* MammoReport ImageRouting and is not a functional specification of any component or product.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

Implementation Model

Application Data Flow

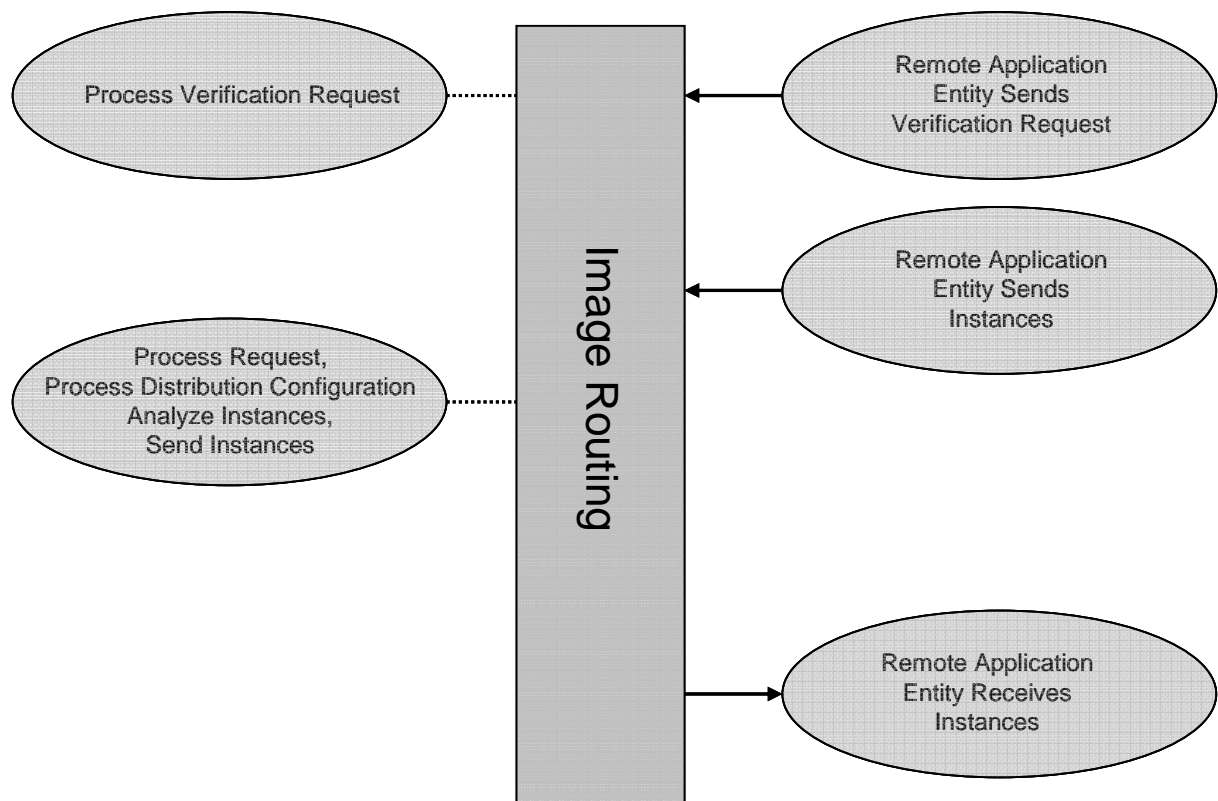


Functional Definition of AE

The SCU Application Entity and SCP Application Entity of *syngo* MammoReport ImageRouting are implemented as separate threads. They are part of the ImageRouting process.

- The SCU part initiates Storage Requests as needed by *syngo* MammoReport ImageRouting.
- The SCP part accepts Storage and Verification requests whenever *syngo* MammoReport ImageRouting is running. ImageRouting stores received instances locally.

Sequencing of Real World Activities

An instance is being sent from a DICOM node to *syngo* MammoReport ImageRouting. According to the current configuration this instance is forwarded to a remote *syngo* MammoReport ImageRouting instance or any other DICOM.

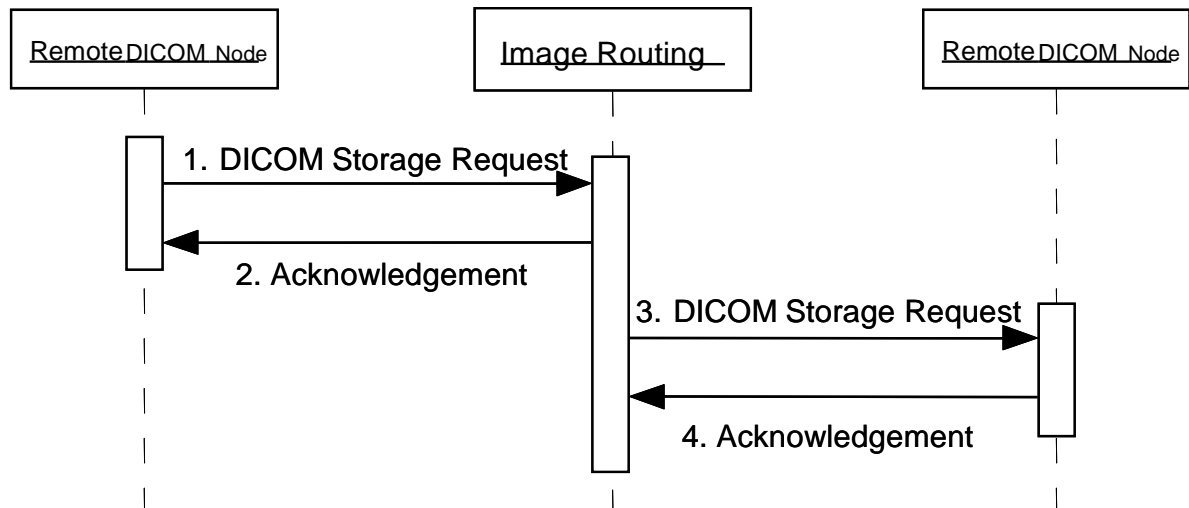

AE Specification

Service Class User Part

SOP Classes

syngo MammoReport ImageRouting provides Standard Conformance to the following SOP Classes as Service Class User:

SOP Class Name	SOP Class UID
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
CT Image Storage	1.2.840.10008.5.1.4.1.1.2
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1
Digital Mammography X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mammography X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
MR Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Ultrasound Multi-Frame Image Storage (retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Image Storage (retired)	1.2.840.10008.5.1.4.1.1.6
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128

Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22
Key Object Selection SOP Class	1.2.840.10008.5.1.4.1.1.88.59

Association Policies

The DICOM standard Application context shall be specified.

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

syngo MammoReport ImageRouting supports multiple associations as Service Class User. There are no enforced limits for the number of open associations.

syngo MammoReport ImageRouting does not support asynchronous operations as Service Class User.

Implementation Class UID	1.3.12.2.1107.5.12
Implementation Version Name	MBC_DXC-3-0-2

Association Initiation Policy

Send DICOM Objects is triggered when routed DICOM Objects are received from a remote DICOM node (e.g. a *syngo* MammoReport ImageRouting instance). When the received object should be sent to another DICOM node according to the current configuration, a DICOM Storage to the node is initiated.

The Presentation Contexts are (Transfer Syntax values are explained below):

Abstract Syntax	UID	Transfer Syntax
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Extended
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Extended
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Extended
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Extended
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Extended
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Extended
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Extended
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1	Extended
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Extended
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Extended
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Extended
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Extended
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Extended
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.3	Extended
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Extended
<i>Ultrasound Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.6	Extended

Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Extended
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Extended
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Basic
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Basic
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Basic
Key Object Selection SOP Class	1.2.840.10008.5.1.4.1.1.88.59	Basic

Dependent on the configuration *syngo* MammoReport ImageRouting supports the following Transfer Syntaxes as Service Class User:

Basic:

Transfer Syntax	UID
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

Extended (default):

Transfer Syntax	UID
JPEG_EXTENDED_2_4	1.2.840.10008.1.2.4.51
JPEG_LOSSLESS_HIER_14	1.2.840.10008.1.2.4.70
JPEG_BASELINE	1.2.840.10008.1.2.4.50
RLE	1.2.840.10008.1.2.5
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

As SCU *syngo* MammoReport ImageRouting uses the following transfer syntax scheme:

- If the image was received with one of the basic transfer syntaxes all **basic** transfer syntaxes are negotiated.
- If the image was received with a non basic transfer syntax only this transfer syntax will be used.

The behaviour of the Service Class User Part when encountering status codes in a C-Store response is summarized in the table below:

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0	The remote Store SCP has successfully stored the SOP instance. Job complete.
Warning or Failure	Any	Any	The Service Class User Part releases the association.

The behaviour of the Service Class User Part during communication failure is summarized in the table below:

Exception	Behaviour
-----------	-----------

Timeout The Service Class User Part releases the association. The error is reported
 Association rejected or aborted by SCP The error is reported.

Service Class Provider Part

SOP Classes

syngo MammoReport ImageRouting provides Standard Conformance for the following SOP Classes as Service Class Provider:

SOP Class Name	SOP Class UID
Verification	1.2.840.10008.1.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-Frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2
Multi-Frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-Frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
CT Image Storage	1.2.840.10008.5.1.4.1.1.2
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1
Digital Mammography X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital Mammography X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
MR Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Ultrasound Multi-Frame Image Storage (retired)	1.2.840.10008.5.1.4.1.1.3
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
Ultrasound Image Storage (retired)	1.2.840.10008.5.1.4.1.1.6
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22
Key Object Selection SOP Class	1.2.840.10008.5.1.4.1.1.88.59

Association Policies

The DICOM standard Application context is always accepted.

Application Context Name 1.2.840.10008.3.1.1.1

syngo MammoReport ImageRouting supports multiple associations as Service Class Provider. There are no enforced limits on the number of open associations.

syngo MammoReport ImageRouting does not support asynchronous operations as Service Class Provider.

Implementation Class UID 1.3.12.2.1107.5.12

Implementation Version Name MBC_DXC-3-0-2

Association Acceptance Policy

As soon as the software has been started the Service Class Provider Part is available. Received DICOM objects may be routed to remote DICOM nodes according to the current configuration.

The instances are deleted as soon as all open send operations are done.

The Presentation Contexts are:

Abstract Syntax	UID	Transfer Syntax
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Extended
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Extended
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Extended
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Extended
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Extended
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Extended
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Extended
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1	Extended
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Extended
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Extended
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Extended
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Extended
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Extended
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.3	Extended
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Extended
<i>Ultrasound Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.6	Extended
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Extended
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Extended
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Basic
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Basic
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Basic
Verification	1.2.840.10008.1.1	Basic

Dependent on the configuration syngo MammoReport ImageRouting supports the following Transfer Syntaxes as Service Class Provider:

Basic:

Transfer Syntax	UID
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2

Implicit Little Endian 1.2.840.10008.1.2

Extended (default):

Transfer Syntax	UID
JPEG_EXTENDED_2_4	1.2.840.10008.1.2.4.51
JPEG_LOSSLESS_HIER_14	1.2.840.10008.1.2.4.70
JPEG_BASELINE	1.2.840.10008.1.2.4.50
RLE	1.2.840.10008.1.2.5
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

The Service Class Provider Part provides Level 2 (full) conformance to all of the accepted Storage SOP Classes. All received attributes of Type 1, 2, 3 and Private Attributes are stored without modification.

In addition to the proper encoded Private Tags according to DICOM Standard 2007 *syngo* MammoReport ImageRouting allows some more variants of Private Tags:

- Empty Private Creator Codes are accepted / kept
- Invalid Private Creator Codes are accepted / kept
- Multiple times the same Creator Codes within one group are accepted / kept

The return values that can be sent in a C-Store response are:

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0x0000	Storage was successful.
Failure	Processing Failure	0x0110	Directory to store message does not exist or storage procedure failed.
Failure	Out of Resources	0xA700	Available disk space is less than the configured minimum.

syngo MammoReport ImageRouting is always available to respond to verification requests from any remote application entity:

Abstract Syntax	UID	Transfer Syntax
Verification	1.2.840.10008.1.1	Basic

syngo MammoReport ImageRouting provides standard conformance to the verification service class.

When *syngo* MammoReport ImageRouting accepts an association it will respond to storage and verification requests.

Network Interfaces

Physical Network Interface

syngo MammoReport ImageRouting has been tested using the following physical networks:

- 10Base-T Ethernet
- 100Base-T Ethernet

Configuration

AE Titles / Presentation Address Mapping

AE title, TCP/IP parameter etc. are configurable. *syngo* MammoReport ImageRouting uses one AE title for all Service Class User Part and Service Class Provider Part TCP/IP ports and services.

Media Interchange

Media interchange is not supported by *syngo* MammoReport ImageRouting.

Support of Character Sets

No restriction for the main functionality.

Security

syngo MammoReport ImageRouting does not support any specific DICOM security measures.

IOD Contents

No SOP-Instances are created by *syngo* MammoReport ImageRouting.

Attributes with incorrect values may cause undesirable behaviors. In most cases it is not possible for *syngo* MammoReport ImageRouting to detect incorrect values.

The following attributes and values are expected for successful interpretation of received SOP Instances:

Attribute Name	Tag	Expected Value
SOP Instance UID	(000,0018)	Unique Worldwide
Rows	(0028,0010)	Matches Pixel Data
Columns	(0028,0011)	Matches Pixel Data
Bits Allocated	(0028,0100)	Matches Pixel Data
Bits Stored	(0028,0101)	Matches Pixel Data
Pixel Data	(7FE0,0010)	Consistent with values above

No other tags are checked.

No valid DICOM tags get coerced / modified during transmission.

No private transfer syntaxes are used.

ImagePrefetching Conformance Statement

This chapter contains the Conformance Statement for the Image Prefetching part of the syngo MammReport.

Image Prefetching is used to prefetch DICOM images and reports based on incoming DICOM images and modality worklists, or based on incoming query/retrieve requests. It implements the necessary DICOM services to query, retrieve, receive and store images and related information from / to networked devices.

For completeness of the DICOM standard conformance ImagePrefetching answers Verification requests. During performance of an initial automatic configuration check, ImagePrefetching requests Verification from other DICOM nodes.

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Secondary Capture Image Storage	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image Storage	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage	Yes	Yes
Computed Radiography Image Storage	Yes	Yes
CT Image Storage	Yes	Yes
Enhanced CT Image Storage	Yes	Yes
Digital X-Ray Image Storage – For Presentation	Yes	Yes
Digital X-Ray Image Storage – For Processing	Yes	Yes
Digital Mammography X-Ray Image Storage – For Presentation	Yes	Yes
Digital Mammography X-Ray Image Storage – For Processing	Yes	Yes
MR Image Storage	Yes	Yes
Enhanced MR Image Storage	Yes	Yes
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
<i>Ultrasound Image Storage (Retired)</i>	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Positron Emission Tomography Image Storage	Yes	Yes
Grayscale Softcopy Presentation State Storage	Yes	Yes
Mammography CAD SR Storage	Yes	Yes
Enhanced SR Storage	Yes	Yes
Verification	Yes	Yes
Key Object Selection Document SOP Class	Yes	Yes
Patient Root Query/Retrieve Information Model – FIND	Yes ¹⁾	Yes
Patient Root Query/Retrieve Information Model – MOVE	Yes ¹⁾	Yes
Study Root Query/Retrieve Information Model – FIND	Yes	Yes
Study Root Query/Retrieve Information Model – MOVE	Yes	Yes
Patient/Study Only Query/Retrieve Information Model – FIND (retired)	Yes ¹⁾	Yes
Patient/Study Only Query/Retrieve Information Model – MOVE (retired)	Yes ¹⁾	Yes
Modality Worklist Information Model - FIND	Yes	No

¹⁾ These SOP classes will be used only when forwarding query/retrieve requests that were received from other DICOM nodes using the respective Information Model.

Only the SOP Classes mentioned above are supported.

Relational Queries are not supported either as an SCU or SCP.

Introduction

Purpose

This DICOM Conformance Statement is written according to part PS 3.2 of [1].

The applications described in this conformance statement are the SIEMENS *syngo* MammoReport Image Prefetching based on *syngo*® software^a.

Scope

This DICOM Conformance Statement refers to SIEMENS *syngo* MammoReport based products using *syngo* MammoReport software. The following table relates *syngo* MammoReport software names to SIEMENS products:

Software Name	SIEMENS <i>syngo</i> -based Product
SCR-SIE-5-1-0 / VB40	<i>syngo</i> MammoReport

Definitions, Abbreviations

Definitions

100BASE-T Ethernet	Computer networking technology standardized by IEEE
10BASE-T Ethernet	Computer networking technology standardized by IEEE
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite information objects

Abbreviations

ADSL	Asymmetric Digital Subscriber Line, computer networking technology standardized by ITU
AE	Application Entity
ETSI	European Telecommunications Standards Institute
IEEE	Institute of Electrical and Electronics Engineers
IOD	Information Object Definition
ITU	International Telecommunication Union
PACS	Picture Archive and Communication System
SCP	Service Class Provider
SCU	Service Class User
SOP	Service Object Pair
TCP/IP	Transmission Control Protocol / Internet Protocol
UID	Unique Identifier

References

- [1] Digital Imaging and Communications in Medicine (DICOM) 3.0, NEMA PS 3.1-18, 2009

^a *syngo* is a registered trademark of Siemens AG.

The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>

Remarks


A DICOM conformance statement – the structure and content of which are stipulated by the DICOM standard – is intended to aid in determining the suitability of interconnecting digital imaging devices. References to specific functionality in a conformance statement are not sufficient to guarantee interoperability between components. The following should be considered when evaluating interoperability:


This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

- The *syngo* MammoReport ImagePrefetching conformance statement provides a starting point for ascertaining whether the product can communicate with other systems.
- The only way to know for certain whether *syngo* MammoReport ImagePrefetching can interoperate with other systems is to perform connectivity tests.
- This document represents a best effort to document the functionality of commercial versions of *syngo* MammoReport ImagePrefetching and is not a functional specification of any component or product.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.


Implementation Model

Application Data Flow

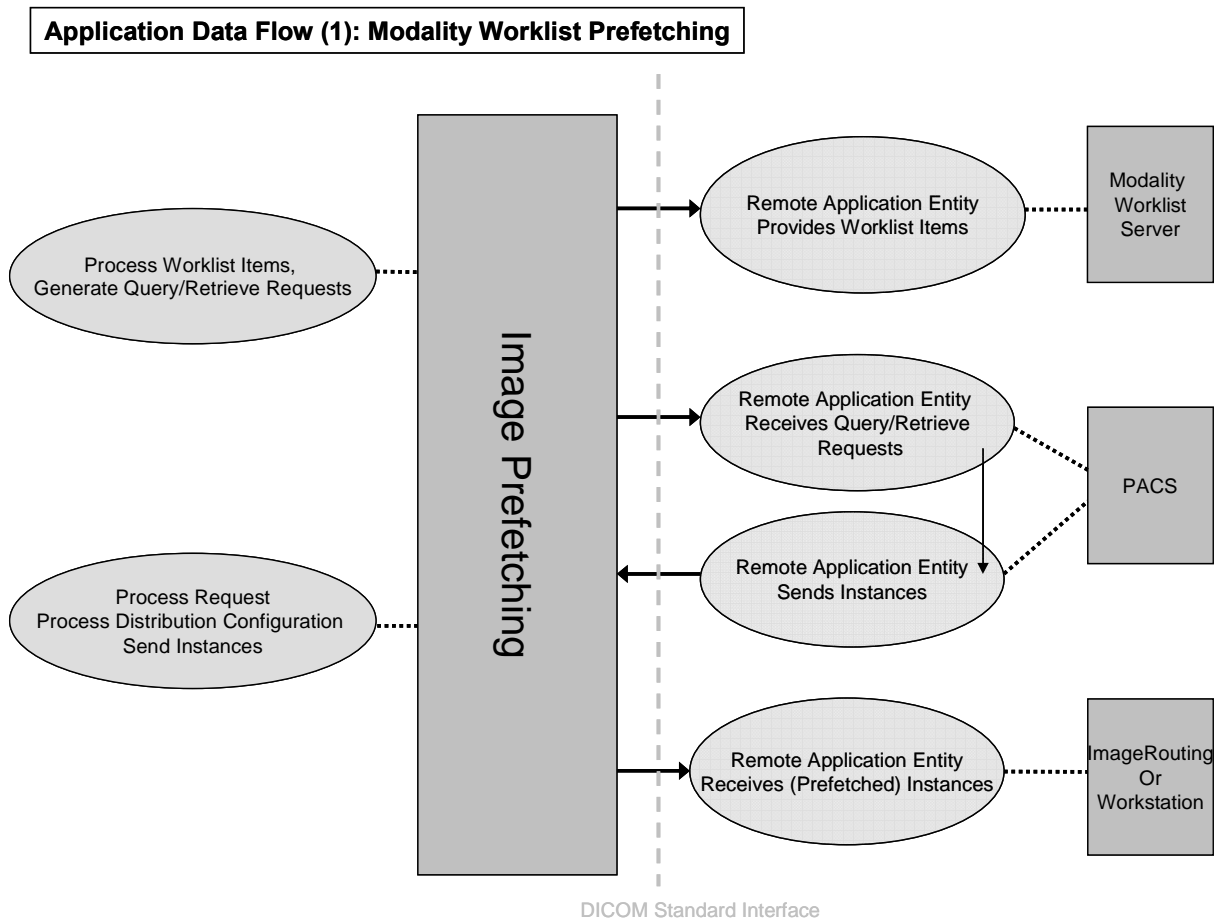

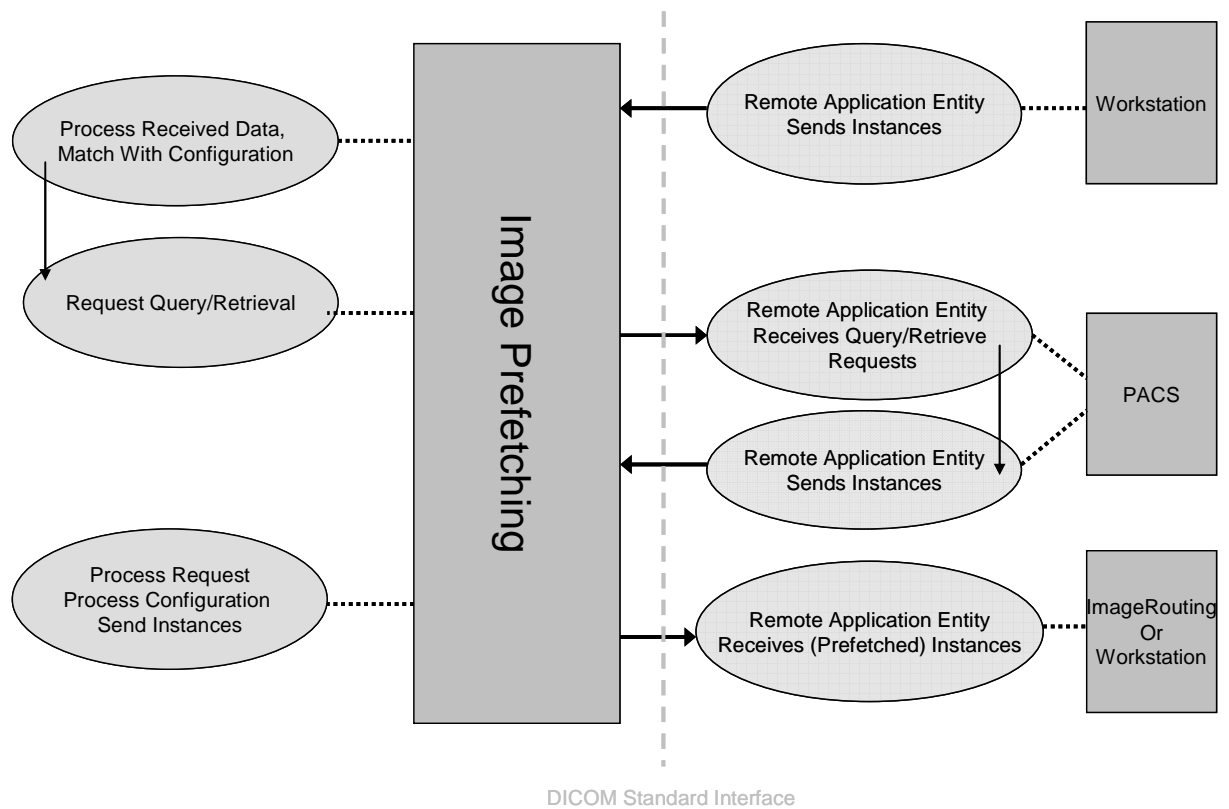Application Data Flow (2): Automatic Prefetching

Application Data Flow (3): Manual Query/Retrieve

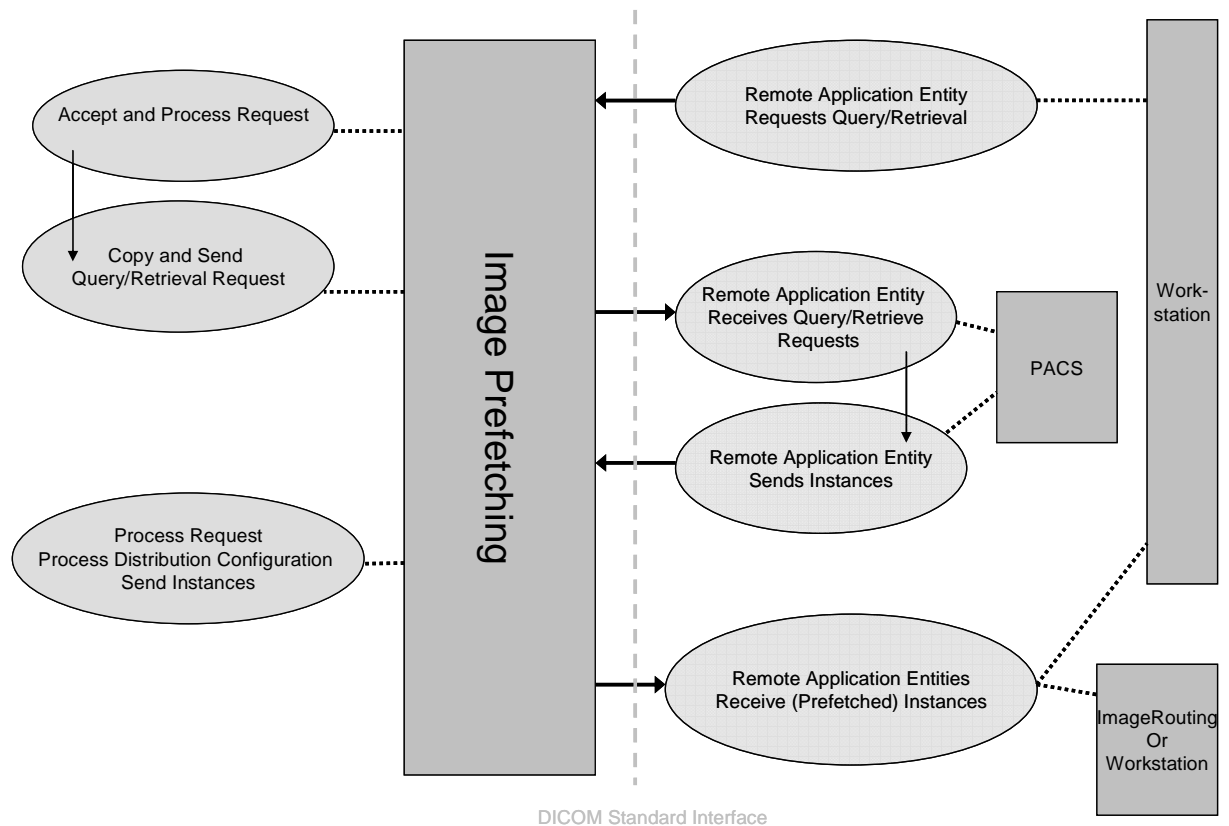

Functional Definition of AE

Several different Application Entities, implemented in separate threads, are part of the ImagePrefetching process, externally identified by one single Application Entity Title.

Instance Forwarder Application Entity (1):

The Storage SCU part initiates Storage Requests as needed by *syngo* MammoReport ImagePrefetching for transferring the prefetched data to the configured target nodes.

Automatic Prefetching Image Acceptor Application Entity (2):

One Storage SCP part accepts Storage Requests as needed by *syngo* MammoReport ImagePrefetching for the Automatic Prefetching functionality (incoming instances triggering prefetching of other instances).

Prefetched Instances Acceptor Application Entity (3):

Another Storage SCP part accepts Storage Requests as a result of a Retrieve Request of a Query/Retrieve SCU of *syngo* MammoReport ImagePrefetching (→ 5) or 6)).

Modality Worklist Polling Application Entity (4):

One Query SCU part initiates Modality Worklist Find Requests as needed by *syngo* MammoReport ImagePrefetching for the Modality Worklist Prefetching functionality.

Query/Retrieve Application Entity (5):

One Query/Retrieval SCU part initiates Query and Retrieval Requests as needed by *syngo* MammoReport ImagePrefetching for prefetching prior images from configured network devices (e.g. PACS). It is triggered internally by the processing of either worklist items (modality worklist prefetching) or received (current) instances (autofetching).

Query/Retrieve Forwarder Application Entity (6):

One Query/Retrieval part (SCP and SCU) accepts Query and Retrieval Requests as needed by *syngo* MammoReport ImagePrefetching for the Manual Query/Retrieve functionality and initiates Query and Retrieval Requests to configured network nodes (forwarding of Query/Retrieval requests).


All those parts are available whenever *syngo* MammoReport ImagePrefetching is running as far as they are configured. If a part of the functionality is not used and thus not configured, the respective Application Entity is not available.

Sequencing of Real World Activities


There are three different types of prefetching:

- Current study based prefetching (autofetching, AF): An instance is being sent from a DICOM node to *syngo* MammoReport ImagePrefetching. According to the current configuration, ImagePrefetching will query configured DICOM nodes (PACSe) for prior studies and forward the retrieved studies to the configured destination.
- Modality worklist based prefetching (MWL): According to the configuration, ImagePrefetching will poll one or more modality worklist servers and query/retrieve the prior studies according to the modality worklists.
- Manual Query/Retrieve (MQR): According to the configuration, ImagePrefetching will accept Query/Retrieve requests from other DICOM nodes and forward the requests to other DICOM nodes.


Sequencing of Real-World Activities (1): MWL

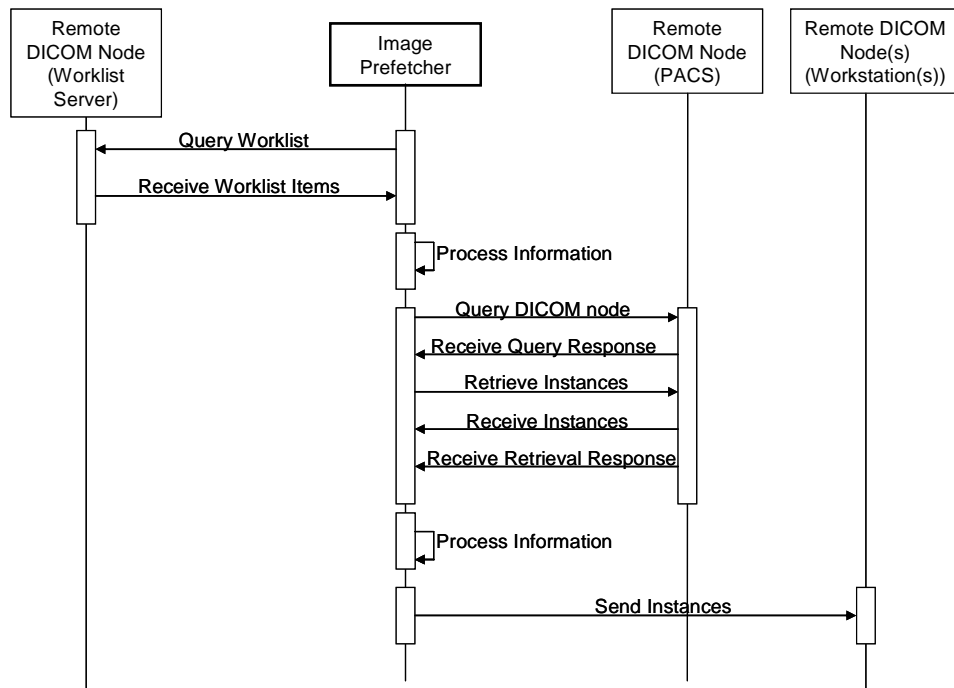

Sequencing of Real-World Activities (2): AF

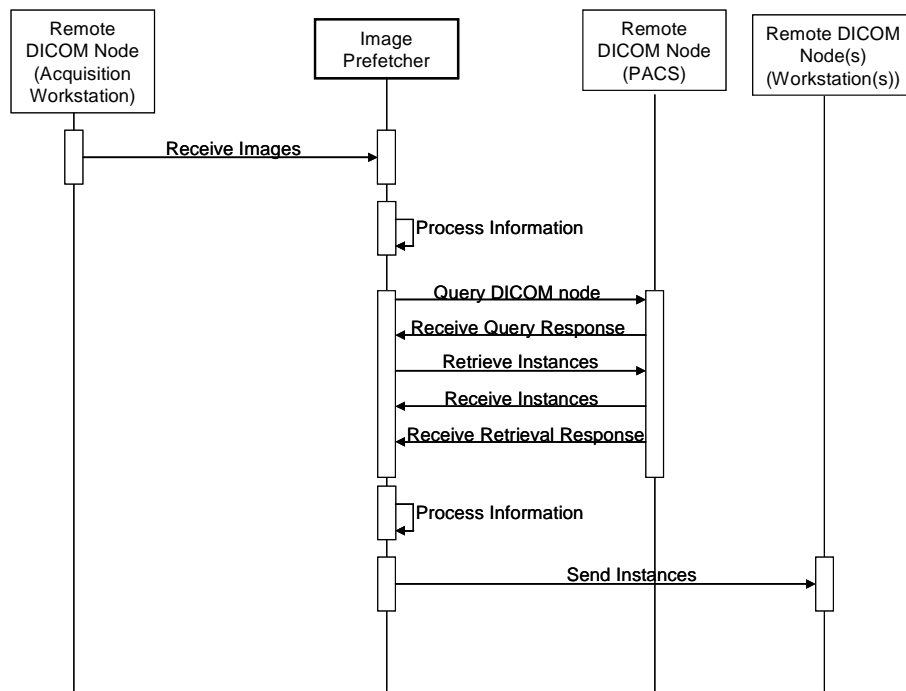

Sequencing of Real-World Activities (3): MQR

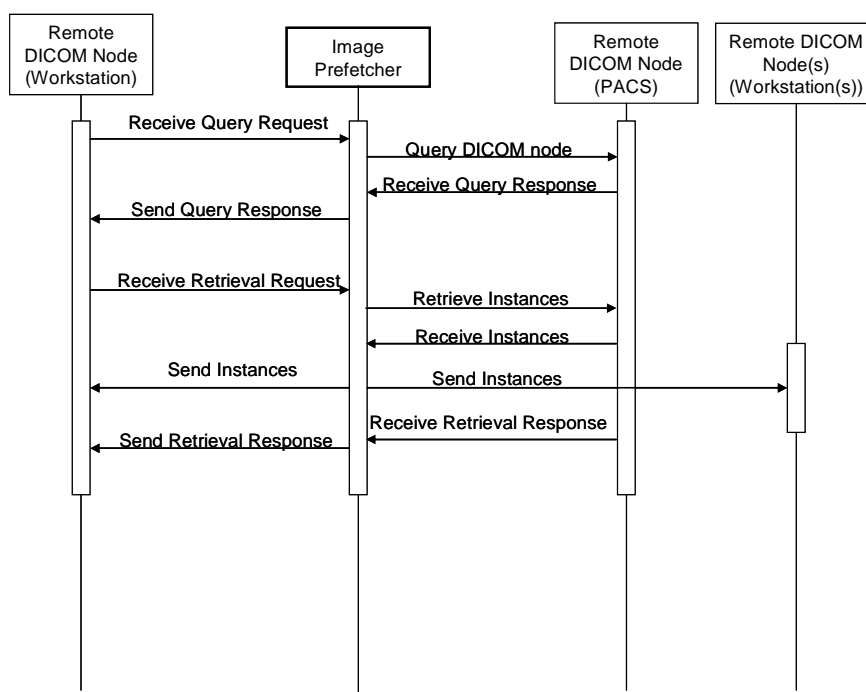

AE Specification

Service Class User Part

SOP Classes

syngo MammoReport ImagePrefetching provides Standard Conformance to the following SOP Classes as Service Class User:

SOP Class Name	SOP class UID	Prefetching Type
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	AF, MWL, MQR
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	AF, MWL, MQR
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	AF, MWL, MQR
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	AF, MWL, MQR
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	AF, MWL, MQR
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	AF, MWL, MQR
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	AF, MWL, MQR
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1	AF, MWL, MQR
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	AF, MWL, MQR
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	AF, MWL, MQR
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	AF, MWL, MQR
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	AF, MWL, MQR
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	AF, MWL, MQR
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.3	AF, MWL, MQR
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	AF, MWL, MQR
<i>Ultrasound Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.6	AF, MWL, MQR
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	AF, MWL, MQR

Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	AF, MWL, MQR
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	AF, MWL, MQR
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	AF, MWL, MQR
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	AF, MWL, MQR
Verification	1.2.840.10008.1.1	AF, MWL, MQR
Key Object Selection Document SOP Class	1.2.840.10008.5.1.4.1.1.88.59	AF, MWL, MQR
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	MQR
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	MQR
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	AF, MWL, MQR
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	AF, MWL, MQR
Patient/Study Only Query/Retrieve Information Model – FIND (retired)	1.2.840.10008.5.1.4.1.2.3.1 (retired)	MQR
Patient/Study Only Query/Retrieve Information Model – MOVE (retired)	1.2.840.10008.5.1.4.1.2.3.2 (retired)	MQR
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	MWL

Association Policies

The DICOM standard Application context shall be specified.

Application Context Name 1.2.840.10008.3.1.1.1

syngo MammoReport ImagePrefetching supports multiple associations as Service Class User. There are no enforced limits for the number of open associations.

syngo MammoReport ImagePrefetching does not support asynchronous operations as Service Class User.

Implementation Class UID 1.3.12.2.1107.5.12

Implementation Version Name MBC_DXC-3-0-2

Association Initiation Policy

A Modality Worklist Information Model C-FIND request is sent periodically to every configured modality worklist server. The polling interval is configurable.

Query/Retrieve of DICOM Objects is triggered when

- current studies are received from a remote DICOM node (e.g. an acquisition workstation) (AF)
- modality worklist items have been polled from a remote Modality Worklist Server (MWL)
- query/retrieve requests are received from a remote DICOM node (e.g. a *syngo MammoReport* instance) (MQR)

When the retrieved object(s) should be sent to another DICOM node according to the current configuration, a DICOM Storage to the node is initiated when the instance has been received.

No CANCEL requests are issued.

The Presentation Contexts are (Transfer Syntax values are explained below):

Abstract Syntax	UID	Transfer Syntax
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Extended
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Extended
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Extended
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Extended
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Extended
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Extended
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Extended
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1	Extended
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Extended
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Extended
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Extended
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Extended
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Extended
<i>Ultrasound Multi-frame Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.3	Extended
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Extended
<i>Ultrasound Image Storage (Retired)</i>	1.2.840.10008.5.1.4.1.1.6	Extended
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Extended
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Extended
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Basic
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Basic
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Basic
Verification	1.2.840.10008.1.1	Basic
Key Object Selection Document SOP Class	1.2.840.10008.5.1.4.1.1.88.59	Basic
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Basic
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Basic
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Basic
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Basic
Patient/Study Only Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.3.1 (retired)	Basic
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2 (retired)	Basic
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Basic

Dependent on the configuration *syngo* MammoReport ImagePrefetching supports the following Transfer Syntaxes as Service Class User:

Basic:

Transfer Syntax	UID
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

Extended (default):

Transfer Syntax	UID
JPEG_EXTENDED_2_4	1.2.840.10008.1.2.4.51
JPEG_LOSSLESS_HIER_14	1.2.840.10008.1.2.4.70
JPEG_BASELINE	1.2.840.10008.1.2.4.50
RLE	1.2.840.10008.1.2.5
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

As SCU *syngo* MammoReport ImagePrefetching uses the following transfer syntax scheme:

- If the image was received with one of the basic transfer syntaxes all basic transfer syntaxes are negotiated.
- If the image was received with a non basic transfer syntax only this transfer syntax will be used.

The C-FIND/C-MOVE SCU part of *syngo* MammoReport ImagePrefetching does not support optional keys. No extended negotiation is performed. In particular, relational queries are not supported. The C-FIND/C-MOVE SCU uses ISO-IR 100 as specific character set (0008,0005) or, when forwarding requests, it may also use the specific character set which is set in the received request.

Behavior according to the Status Code value returned in C-STORE/C-FIND/C-MOVE Responses

The behaviour of the Service Class User Part when encountering status codes in a C-FIND response is summarized below:

Case 1: C-FIND as part of AF or MWL:

Service Status	Further Meaning	Error Code (hex)	Behaviour
Success	Success	0	Job complete. Received data will be processed. Successful completion is shown to user via ImagePrefetching Status GUI.
Pending	Pending (more suboperations to be completed)	FF00, FF01	Keep on listening
Warning or Error	Any Other	Any Other	The error code is logged in the detailed logfile; the ServiceLog (visible to User) shows message "DICOM node returned error on C-FIND" with information about the requested patient/study and the DICOM node. Job will be retried according to configuration (retry interval configured, limited number of retries configured). If max. number of retries exceeded, job is set to status 'completed with errors' which is signaled to the user via ImagePrefetching Status GUI.

Case 2: C-FIND as part of MQR (forwarded C-FIND request):

The responses are sent to the original issuer as received from the C-FIND SCP(s); therefore, ImagePrefetching does not do any error handling in this case, as this feature represents a simple forwarding of Query Requests.

The behaviour of the Service Class User Part when encountering status codes in a C-MOVE response is summarized in the tables below:

Case 1: C-MOVE as part of AF or MWL:

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0	Job complete. Received data will be processed. Successful completion is shown to user via ImagePrefetching Status GUI.
Warning	Warning (one or more failed suboperations)	B100	Job complete with partial failures. Received data will be processed. Completion is shown as 'completed with errors' to user via ImagePrefetching Status GUI.
Pending	Pending (more suboperations to be completed)	FF00	Keep on listening
Warning or Error	Any Other	Any Other	The error code is logged in the detailed logfile; the ServiceLog (visible to User) shows message "DICOM node returned error on C-MOVE" with information about the requested patient/study and the DICOM node. Job will be retried according to configuration (retry interval configured, limited number of retries configured). If max. number of retries exceeded, job is set to status 'completed with errors' which is signaled to the user via ImagePrefetching Status GUI.

Case 2: C-MOVE as part of MQR (forwarded C-MOVE request):

The responses are sent to the original issuer as received from the C-MOVE SCP(s). ImagePrefetching does not do any error handling in this case, as this feature represents a simple forwarding of Retrieval Requests.

The behaviour of the Service Class User Part during communication failure in a C-FIND or C-MOVE request is summarized in the table below:

C-FIND as part of MQR

Exception	Behaviour
Association cannot be established.	The Service Class User Part releases the association. The error is reported in the logfiles.
Request cannot be sent after successful establishing connection.	
Response cannot be read.	

C-MOVE as part of MQR

Exception	Behaviour
Association cannot be established.	The Service Class User Part releases the association. An error is reported in the logfiles.
Request cannot be sent after successful establishing connection.	The Service Class User Part releases the association. An error is reported in the logfiles.
Response cannot be read.	The Service Class User Part releases the association. An error is reported in the logfiles. An internal error count is increased and the final response to the issuer of the request will show „one or more failures“.

C-FIND as part of MWL/AF

Exception	Behaviour
Association cannot be established.	The error is reported in the logfiles.
Request cannot be sent after successful establishing connection.	Job will be retried according to configuration (retry interval configured, limited number of retries configured). If max. number of retries exceeded, job is set to status 'completed with errors' which is signaled to the user via ImagePrefetching Status GUI.
Response cannot be read.	

C-MOVE as part of MWL/AF

Exception	Behaviour
Association cannot be established.	The error is reported in the logfiles.
Request cannot be sent after successful establishing connection.	Job will be retried according to configuration (retry interval configured, limited number of retries configured). If max. number of retries exceeded, job is set to status 'completed with errors' which is signaled to the user via ImagePrefetching Status GUI.
Response cannot be read.	

The behaviour of the Service Class User Part when encountering status codes in a C-Store response is summarized in the table below:

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0	The remote Store SCP has successfully stored the SOP instance. Job complete. C-Store in context of AF/MWL:
Warning or Failure	Any	Any	The Service Class User Part releases the association. The error is reported in the logfile. Failed request is set on retry list. C-Store to issuer of C-MOVE request: No specific error handling, i.e. no retries.

The behaviour of the Storage Service Class User Part during communication failure is summarized in the table below:

Exception	Behaviour
Timeout	The Service Class User Part releases the association. The error is reported.
Association rejected or aborted by SCP	The error is reported.

Service Class Provider Part

SOP Classes

syngo MammoReport ImagePrefetching provides Standard Conformance for the following SOP Classes as Service Class Provider:

SOP Class Name	SOP Class UID	Prefetching Type
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	AF, MWL, MQR
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	AF, MWL, MQR
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	AF, MWL, MQR
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	AF, MWL, MQR

Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	AF, MWL, MQR
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	AF, MWL, MQR
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	AF, MWL, MQR
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	AF, MWL, MQR
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	AF, MWL, MQR
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	AF, MWL, MQR
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	AF, MWL, MQR
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	AF, MWL, MQR
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	AF, MWL, MQR
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	AF, MWL, MQR
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	AF, MWL, MQR
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	AF, MWL, MQR
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	AF, MWL, MQR
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	AF, MWL, MQR
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	AF, MWL, MQR
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	AF, MWL, MQR
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	AF, MWL, MQR
Verification	1.2.840.10008.1.1	AF, MWL, MQR
Key Object Selection Document SOP Class	1.2.840.10008.5.1.4.1.1.88.59	AF, MWL, MQR
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	MQR
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	MQR
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	MQR
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	MQR
Patient/Study Only Query/Retrieve Information Model – FIND (retired)	1.2.840.10008.5.1.4.1.2.3.1 (retired)	MQR
Patient/Study Only Query/Retrieve Information Model – MOVE (retired)	1.2.840.10008.5.1.4.1.2.3.2 (retired)	MQR

Association Policies

The DICOM standard Application context is always accepted.

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

syngo MammoReport ImagePrefetching supports multiple associations as Service Class Provider. There are no enforced limits on the number of open associations.

syngo MammoReport ImagePrefetching does not support asynchronous operations as Service Class Provider.

Implementation Class UID	1.3.12.2.1107.5.12
Implementation Version Name	MBC_DXC-3-0-2

Association Acceptance Policy

As soon as the software has been started the Service Class Provider Part is available, if the respective features are configured.

Two different ports are used to receive C-Store requests:

- DICOM objects received on the port specified for autofetching may trigger query/retrieve requests to remote DICOM nodes according to the current configuration (AF).
- DICOM objects received as a result of a retrieve request may be routed to remote DICOM nodes according to the current configuration.

The instances received in context of a C-MOVE request are deleted as soon as all open send operations are done. The instances received as a trigger for AF are deleted as soon as the data has been processed, i.e. according to the configuration, a query/retrieve request has been generated from the received instance.

One port is used to receive C-FIND/C-MOVE requests:

- Query/Retrieve requests received on the port configured for manual query/retrieve may trigger query/retrieve requests to remote DICOM nodes according to the current configuration (MQR).

The Presentation Contexts are:

Abstract Syntax	UID	Transfer Syntax
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Extended
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Extended
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Extended
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Extended
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Extended
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Extended
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Extended
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1.1	Extended
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1	Extended
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Extended
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Extended
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Extended
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Extended
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Extended
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Extended
Ultrasound Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Extended
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Extended
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Extended
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Basic
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Basic
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Basic
Verification	1.2.840.10008.1.1	Basic
Key Object Selection Document SOP Class	1.2.840.10008.5.1.4.1.1.88.59	Basic

Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Basic
Patient Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Basic
Study Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Basic
Study Root Query/Retrieve Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Basic
Patient/Study Only Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.3.1 (retired)	Basic
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2 (retired)	Basic

Dependent on the configuration *syngo* MammoReport ImagePrefetching supports the following Transfer Syntaxes as Service Class Provider:

Basic:

Transfer Syntax	UID
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

Extended (default):

Transfer Syntax	UID
JPEG_EXTENDED_2_4	1.2.840.10008.1.2.4.51
JPEG_LOSSLESS_HIER_14	1.2.840.10008.1.2.4.70
JPEG_BASELINE	1.2.840.10008.1.2.4.50
RLE	1.2.840.10008.1.2.5
Explicit Little Endian	1.2.840.10008.1.2.1
Explicit Big Endian	1.2.840.10008.1.2.2
Implicit Little Endian	1.2.840.10008.1.2

The Service Class Provider Part provides Level 2 (full) conformance to all of the accepted Storage SOP Classes. All received attributes of Type 1, 2, 3 and Private Attributes are stored without modification.

In addition to the proper encoded Private Tags according to DICOM Standard 2007 *syngo* MammoReport ImagePrefetching allows some more variants of Private Tags:

- Empty Private Creator Codes are accepted / kept
- Invalid Private Creator Codes are accepted / kept
- Multiple times the same Creator Codes within one group are accepted / kept

C-FIND/C-MOVE SCP: No extended negotiation is performed. In particular, relational queries are not supported. The C-FIND/C-MOVE SCP may set the specific character set (0008,0005) to ISO-IR 100 or use the value from the original (received) message.

Behavior according to the Status Code value returned in C-STORE/C-FIND/C-MOVE Responses

The return values that can be sent in a C-Store response are:

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0x0000	DICOM object was accepted. Directory to store message does not exist.
Failure	Processing Failure	0x0110	In the context of AF (receiving an instance as a trigger for autofetching), this error code may also be sent if storing the instance to the local file system failed.
Failure	Out of Resources	0xA700	Available disk space is less than the configured minimum.

The return values that can be sent in a C-FIND response are:

As *syngo* MammoReport ImagePrefetching is a C-FIND SCP only in case of MQR, i.e. does not process the request itself but only forwards them to other C-FIND SCP(s), all possible C-FIND responses can be sent, as the responses are forwarded from the queried DICOM nodes back to the issuer of the original C-FIND request.

Note: Depending on the configuration, the received C-FIND request may be forwarded to more than one other C-FIND SCP. Thus, the final C-FIND response (after completion of all sub-operations of all target C-FIND SCPs), is sent only after all target SCPs have sent their final response. The final response is always a C-FIND success, as there is no possibility to sent a "partial success" in case that the query failed on part of the target SCPs only.

The return values that can be sent in a C-MOVE response are:

The final response sent by *syngo* MammoReport ImagePrefetching to the issuer of the request is

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0x0000	All queried nodes returned a final success.
Warning	One or More Failures	0xB000	At least one of the queried nodes returned a failure code other than success.

As it might be possible that the request is forwarded to more than one C-MOVE SCP, the final C-MOVE responses are not directly forwarded back to the original issuer of the request, but *syngo* MammoReport ImagePrefetching sends the final response only after having received a final response from all queried C-MOVE SCPs.

syngo MammoReport ImagePrefetching is always available to respond to verification requests from any remote application entity:

Abstract Syntax	UID	Transfer Syntax
Verification	1.2.840.10008.1.1	Basic

syngo MammoReport ImagePrefetching provides standard conformance to the verification service class.

When *syngo* MammoReport ImagePrefetching accepts an association it will respond to storage and verification requests, except when the association was initiated via the port configured for manual query/retrieve (MQR).

When *syngo* MammoReport ImagePrefetching accepts an association it will respond to query/retrieve requests when the association was initiated via the port configured for manual query/retrieve (MQR).

Network Interfaces

Physical Network Interface

syngo MammoReport ImagePrefetching has been tested using the following physical networks:

- 10Base-T Ethernet
- 100Base-T Ethernet

Configuration

AE Titles / Presentation Address Mapping

AE title, TCP/IP parameter etc. are configurable. syngo MammoReport ImagePrefetching uses one AE title for all Service Class User Part and Service Class Provider Part TCP/IP ports and services.

Media Interchange

Media interchange is not supported by syngo MammoReport ImagePrefetching.

Support of Character Sets

No restriction for the main functionality.

Security

syngo MammoReport ImagePrefetching does not support any specific DICOM security measures.

IOD Contents

Attributes with incorrect values may cause undesirable behaviors. In most cases it is not possible for syngo MammoReport ImagePrefetching to detect incorrect values.

The following attributes and values are expected for successful interpretation of received SOP Instances:

Attribute Name	Tag	Expected Value
SOP Instance UID	(000,0018)	Unique Worldwide
Rows	(0028,0010)	Matches Pixel Data
Columns	(0028,0011)	Matches Pixel Data
Bits Allocated	(0028,0100)	Matches Pixel Data
Bits Stored	(0028,0101)	Matches Pixel Data
Pixel Data	(7FE0,0010)	Consistent with values above

No other tags are checked.

No valid DICOM tags get coerced / modified during transmission.

No private transfer syntaxes are used.

ANNEX

A.1 DICOM Print SCU – detailed status displays

The following tables document the behavior of the syngo MammoReport DICOM Print AE in response to messages received for the printer SOP class and the print job SOP class.

Definitions of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed.
- Interact: The user has to react in near future, but not immediately.
Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by n-event-report.
- Queue Stopped: The user has to react immediately. Either the camera needs immediate interaction or a job has been aborted.
Example: A camera is out of 8x10 clear sheets, or camera is down, or a film job is aborted.

Note: different camera symbols are displayed according to the Printer Status Info.

A.1.1 Common Status Information

“Common Status Info evaluation”

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
NORMAL	Camera is ready	Camera is ready	<None>/idle
BAD RECEIVE MGZ	There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine.	Problem with receive magazine.	<None>/interact
BAD SUPPLY MGZ	There is a problem with the film supply magazine. Films from this magazine cannot be transported into the printer.	Problem with supply magazine.	<None>/interact
CALIBRATING	Printer is performing self calibration, it is expected to be available for normal operation shortly.	Self calibration. Please wait.	<None>/idle
CALIBRATION ERR	An error in the printer calibration has been detected, quality of processed films may not be optimal.	Problem in calibration. Film quality may not be optimal.	<None>/interact
CHECK CHEMISTRY	A problem with the processor chemicals has been detected, quality of processed films may not be optimal.	Problem with chemistry. Film quality may not be optimal.	<None>/interact
CHECK SORTER	There is an error in the film sorter	Error in film sorter.	<None>/interact
CHEMICALS EMPTY	There are no processing chemicals in the processor, films will not be printed and processed until the processor is back to normal.	Camera chemistry empty. Please check.	<None>/interact
CHEMICALS LOW	The chemical level in the processor is low, if not corrected, it will probably shut down soon.	Camera chemistry low. Please check.	<None>/interact
COVER OPEN	One or more printer or processor covers, drawers, doors are open.	Camera cover, drawer or door open.	<None>/interact
ELEC CONFIG ERR	Printer configured improperly for this job.	Camera configured improperly for this job. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
ELEC DOWN	Printer is not operating due to some unspecified electrical hardware problem.	Camera electrical hardware Problem.	<None>/interact
ELEC SW ERROR	Printer not operating for some unspecified software error.	Camera software problem. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
EMPTY 8x10	The 8x10 inch film supply magazine is empty.	8x10 film supply empty.	<None>/interact
EMPTY 8x10 BLUE	The 8x10 inch blue film supply magazine is empty.	8x10 blue film supply empty.	<None>/interact
EMPTY 8x10 CLR	The 8x10 inch clear film supply magazine is empty.	8x10 clear film supply empty.	<None>/interact
EMPTY 8x10 PAPR	The 8x10 inch paper supply magazine is empty.	8x10 paper supply empty.	<None>/interact
EMPTY 10x12	The 10x12 inch film supply magazine is empty.	10x12 film supply empty.	<None>/interact
EMPTY 10x12 BLUE	The 10x12 inch blue film supply magazine is empty.	10x12 blue film supply empty.	<None>/interact
EMPTY 10x12 CLR	The 10x12 inch clear film supply magazine is empty.	10x12 clear film supply empty.	<None>/interact
EMPTY 10x12 PAPR	The 10x12 inch paper supply magazine is empty.	10x12 paper supply empty.	<None>/interact
EMPTY 10x14	The 10x14 inch film supply magazine is empty.	10x14 film supply empty.	<None>/interact
EMPTY 10x14 BLUE	The 10x14 inch blue film supply magazine is empty.	10x14 blue film supply empty.	<None>/interact
EMPTY 10x14 CLR	The 10x14 inch clear film supply magazine is empty.	10x14 clear film supply empty.	<None>/interact
EMPTY 10x14 PAPR	The 10x14 inch paper supply magazine is empty.	10x14 paper supply empty.	<None>/interact
EMPTY 11x14	The 11x14 inch film supply magazine is empty.	11x14 film supply empty.	<None>/interact
EMPTY 11x14 BLUE	The 11x14 inch blue film supply magazine is empty.	11x14 blue film supply empty.	<None>/interact
EMPTY 11x14 CLR	The 11x14 inch clear film supply magazine is empty.	11x14 clear film supply empty.	<None>/interact
EMPTY 11x14 PAPR	The 11x14 inch paper supply magazine is empty.	11x14 paper supply empty.	<None>/interact
EMPTY 14x14	The 14x14 inch film supply magazine is empty.	14x14 film supply empty.	<None>/interact
EMPTY 14x14 BLUE	The 14x14 inch blue film supply magazine is empty.	14x14 blue film supply empty.	<None>/interact
EMPTY 14x14 CLR	The 14x14 inch clear film supply magazine is empty.	14x14 clear film supply empty.	<None>/interact
EMPTY 14x14 PAPR	The 14x14 inch paper supply magazine is empty.	14x14 paper supply empty.	<None>/interact
EMPTY 14x17	The 14x17 inch film supply magazine is empty.	14x17 film supply empty.	<None>/interact
EMPTY 14x17 BLUE	The 14x17 inch blue film supply magazine is empty.	14x17 blue film supply empty.	<None>/interact
EMPTY 14x17 CLR	The 14x17 inch clear film supply magazine is empty.	14x17 clear film supply empty.	<None>/interact
EMPTY 14x17 PAPR	The 14x17 inch paper supply magazine is empty.	14x17 paper supply empty.	<None>/interact
EMPTY 24x24	The 24x24 inch film supply magazine is empty.	24x24 film supply empty.	<None>/interact
EMPTY 24x24 BLUE	The 24x24 inch blue film supply magazine is empty.	24x24 blue film supply empty.	<None>/interact
EMPTY 24x24 CLR	The 24x24 inch clear film supply magazine is empty.	24x24 clear film supply empty.	<None>/interact
EMPTY 24x24 PAPR	The 24x24 inch paper supply magazine is empty.	24x24 paper supply empty.	<None>/interact
EMPTY 24x30	The 24x30 inch film supply magazine is empty.	24x30 film supply empty.	<None>/interact
EMPTY 24x30 BLUE	The 24x30 inch blue film supply magazine is empty.	24x30 blue film supply empty.	<None>/interact
EMPTY 24x30 CLR	The 24x30 inch clear film supply magazine is empty.	24x30 clear film supply empty.	<None>/interact
EMPTY 24x30 PAPR	The 24x30 inch paper supply magazine is empty.	24x30 paper supply empty.	<None>/interact
EMPTY A4 PAPR	The A4 paper supply magazine is empty.	A4 paper supply empty	<None>/interact
EMPTY A4 TRANS	The A4 transparency supply magazine is empty.	A4 transparency supply empty.	<None>/interact
EXPOSURE FAILURE	The exposure device has failed due to some unspecified reason.	Exposure device has failed.	<None>/interact
FILM JAM	A film transport error has occurred and a film is jammed in the printer or processor.	Film jam.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
FILM TRANSP ERR	There is a malfunction with the film transport, there may or may not be a film jam.	Film transport problem.	<None>/interact
FINISHER EMPTY	The finisher is empty.	Finisher is empty.	<None>/interact
FINISHER ERROR	The finisher is not operating due to some unspecified reason	Finisher problem.	<None>/interact
FINISHER LOW	The finisher is low on supplies.	Finisher low.	<None>/interact
LOW 8x10	The 8x10 inch film supply magazine is low.	8x10 film supply low.	<None>/interact
LOW 8x10 BLUE	The 8x10 inch blue film supply magazine is low.	8x10 blue film supply low.	<None>/interact
LOW 8x10 CLR	The 8x10 inch clear film supply magazine is low.	8x10 clear film supply low.	<None>/interact
LOW 8x10 PAPR	The 8x10 inch paper supply magazine is low.	8x10 paper supply low.	<None>/interact
LOW 10x12	The 10x12 inch film supply magazine is low.	10x12 film supply low.	<None>/interact
LOW 10x12 BLUE	The 10x12 inch blue film supply magazine is low.	10x12 blue film supply low.	<None>/interact
LOW 10x12 CLR	The 10x12 inch clear film supply magazine is low.	10x12 clear film supply low.	<None>/interact
LOW 10x12 PAPR	The 10x12 inch paper supply magazine is low.	10x12 paper supply low.	<None>/interact
LOW 10x14	The 10x14 inch film supply magazine is low.	10x14 film supply low.	<None>/interact
LOW 10x14 BLUE	The 10x14 inch blue film supply magazine is low.	10x14 blue film supply low.	<None>/interact
LOW 10x14 CLR	The 10x14 inch clear film supply magazine is low.	10x14 clear film supply low.	<None>/interact
LOW 10x14 PAPR	The 10x14 inch paper supply magazine is low.	10x14 paper supply low.	<None>/interact
LOW 11x14	The 11x14 inch film supply magazine is low.	11x14 film supply low.	<None>/interact
LOW 11x14 BLUE	The 11x14 inch blue film supply magazine is low.	11x14 blue film supply low.	<None>/interact
LOW 11x14 CLR	The 11x14 inch clear film supply magazine is low.	11x14 clear film supply low.	<None>/interact
LOW 11x14 PAPR	The 11x14 inch paper supply magazine is low.	11x14 paper supply low.	<None>/interact
LOW 14x14	The 14x14 inch film supply magazine is low.	14x14 film supply low.	<None>/interact
LOW 14x14 BLUE	The 14x14 inch blue film supply magazine is low.	14x14 blue film supply low.	<None>/interact
LOW 14x14 CLR	The 14x14 inch clear film supply magazine is low.	14x14 clear film supply low.	<None>/interact
LOW 14x14 PAPR	The 14x14 inch paper supply magazine is low.	14x14 paper supply low.	<None>/interact
LOW 14x17	The 14x17 inch film supply magazine is low.	14x17 film supply low.	<None>/interact
LOW 14x17 BLUE	The 14x17 inch blue film supply magazine is low.	14x17 blue film supply low.	<None>/interact
LOW 14x17 CLR	The 14x17 inch clear film supply magazine is low.	14x17 clear film supply low.	<None>/interact
LOW 14x17 PAPR	The 14x17 inch paper supply magazine is low.	14x17 paper supply low.	<None>/interact
LOW 24x24	The 24x24 inch film supply magazine is low.	24x24 film supply low.	<None>/interact
LOW 24x24 BLUE	The 24x24 inch blue film supply magazine is low.	24x24 blue film supply low.	<None>/interact
LOW 24x24 CLR	The 24x24 inch clear film supply magazine is low.	24x24 clear film supply low.	<None>/interact
LOW 24x24 PAPR	The 24x24 inch paper supply magazine is low.	24x24 paper supply low.	<None>/interact
LOW 24x30	The 24x30 inch film supply magazine is low.	24x30 film supply low.	<None>/interact
LOW 24x30 BLUE	The 24x30 inch blue film supply magazine is low.	24x30 blue film supply low.	<None>/interact
LOW 24x30 CLR	The 24x30 inch clear film supply magazine is low.	24x30 clear film supply low.	<None>/interact
LOW 24x30 PAPR	The 24x30 inch paper supply magazine is low.	24x30 paper supply low.	<None>/interact
LOW A4 PAPR	The A4 paper supply magazine is low.	A4 paper supply low.	<None>/interact
LOW A4 TRANS	The A4 transparency supply magazine is low..	A4 transparency supply low.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
NO RECEIVE MGZ	The film receive magazine is not available.	Film receiver not available.	<None>/interact
NO RIBBON	The ribbon cartridge needs to be replaced.	Replace ribbon cartridge.	<None>/interact
NO SUPPLY MGZ	The film supply magazine is not available.	Film supply not available.	<None>/interact
CHECK PRINTER	The printer is not ready at this time, operator intervention is required to make the printer available.	Check camera.	<None>/interact
CHECK PROC	The processor is not ready at this time, operator intervention is required to make the printer available.	Check processor.	<None>/interact
PRINTER DOWN	The printer is not operating due to some unspecified reason.	Camera down.	<None>/interact
PRINTER INIT	The printer is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Camera initializing.	<None>/Idle
PRINTER OFFLINE	The printer has been disabled by an operator or service person.	Camera off-line.	<None>/interact
PROC DOWN	The processor is not operating due to some unspecified reason.	Processor down.	<None>/interact
PROC INIT	The processor is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Processor initializing.	<None>/Idle
PROC OVERFLOW FL	Processor chemicals are approaching the overflow full mark.	Processor chemicals near overflow.	<None>/interact
PROC OVERFLOW HI	Processor chemicals have reached the overflow full mark.	Processor chemicals overflow.	<None>/interact
QUEUED	Print job in Queue	--	<None>/Idle
RECEIVER FULL	The film receive magazine is full.	Receiver full.	<None>/interact
REQ MED NOT INST	The requested film, paper, or other media supply magazine is installed in the printer, but may be available with operator intervention.	Install media supply.	<None>/interact
REQ MED NOT AVAI	The requested film, paper, or other media requested is not available on this printer.	Media supply not available on this camera. Queue stopped. Change camera.	Queue for this camera will be STOPPED/ Queue stopped
RIBBON ERROR	There is an unspecified problem with the print ribbon.	Error with print ribbon.	<None>/interact
SUPPLY EMPTY	The printer is out of film.	Camera out of film.	<None>/interact
SUPPLY LOW	The film supply is low.	Film supply low.	<None>/interact
UNKNOWN	There is an unspecified problem.	Unspecified problem with camera.	<None>/interact

A.1.2 Additional Status Information – AGFA printers

“Additional Agfa printer Status Info evaluation”

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
WARMING UP	Printer is in the warm-up stage. Spooling of print jobs to disk is still possible.	Camera is warming up.	<None>/idle
OFFLINE	OFFLINE Printer is switched off-line. Spooling of print jobs to disk is still possible.	Camera is switched off-line.	<None>/interact
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	--	<None>/idle

A.1.3 Additional Status Information – Kodak PACS Link (formerly Imation)

“Additional Kodak PACS Link (Imation) printer Status Info evaluation”

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
SUPPLY MGZ ERR	The supply magazine has an error.	Film supply has an error.	<None>/interact
LOAD XLA4- CVTRANS	Load XLA4-Size transparencies.	Load XLA4-Size transparencies.	<None>/interact
LOAD XLW-SIZE	Load XLW-Size media.	Load XLW-Size media.	<None>/interact
LOAD XLW-DVPAPER	Load XLW-Size black and white paper.	Load XLW-Size black and white paper.	<None>/interact
LOAD XLW-CVPAPER	Load XLW-Size color paper.	Load XLW-Size color paper.	<None>/interact
LOAD 8X10-SIZE	Load 8x10 media.	Load 8x10 media.	<None>/interact
LOAD 8X10-DVFILM	Load XLW-Size black and white film.	Load XLW-Size black and white film.	<None>/interact
SUPPLY MISSING	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
RIBBON MISSING	Ribbon is missing.	Ribbon is missing.	<None>/interact
RIBBON EMPTY	Ribbon is empty.	Ribbon is empty.	<None>/interact
TOP COVER OPEN	Top cover of printer is open.	Top cover of camera is open.	<None>/interact

A.1.4 Additional DICOM Execution Status Information

"Additional DICOM Execution Status Info evaluation"

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
INVALID PAGE DES	The specified page layout cannot be printed or other page description errors have been detected.	Film Job cannot be printed on this camera. Queue stopped. Please redirect film job.	Queue for this camera will be STOPPED/ Queue stopped
INSUFFICIENT MEMORY	There is not enough memory available to complete this job.	Not enough memory available in camera. Queue stopped. Please continue queue or change camera.	Queue for this camera will be STOPPED/ Queue stopped
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	--	<None>/Idle

A.5 Implementation Breast Imaging Report

For creating Breast Imaging Report structured reports the following templates are supported. The complete definition can be found at DICOM Supplement 79: Breast Imaging Report Templates and DICOM Correctional Proposal CP527. All Mandatory items shall be present. The following templates are supported:

TID 4200

Breast Imaging Report

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV(111400, DCM, „Breast Imaging Report“)	1	M		
2	>	HAS CONCEPT MOD	INCLUDE	DTID(1204) Language of Content Item and Descendants	1	M		See Tailored description
3	>	CONTAINS	INCLUDE	DTID(4202) Breast Imaging Report Narrative	1	M		See Tailored description
4	>	CONTAINS	INCLUDE	DTID(4208) Breast Imaging Report Supplementary Data	1	U		See Tailored description

Note: The DICOM object created by syngo MammReport DICOM application conform to the DICOM IOD definitions and is extended by Study Status ID (0032,000A). Possible values for Study Status ID are “rea” which stands for READ, or <null>.

TID 4201

Breast Imaging Procedure Reported

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CODE	EV(121058, DCM, “Procedure Reported”)	1	M		DCID(6050) Breast Procedure Reported
3	>	HAS CONCEPT MOD	CODE	EV(G-C171, SRT, “Laterality”)	1	M		DCID(6022) Side
8	>	HAS PROPERTIES	DATE	EV(111060, DCM, “Study Date”)	1	U		

TID 4202

Breast Imaging Report Narrative

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV(111412, DCM, „Narrative Summary“)	1	M		
2	>	CONTAINS	CONTAINER	BCID(6052) Breast Imaging Report Section	1-n	M		
3	>>	HAS OBS CONTEXT	INCLUDE	DTID(1002) Observer Context	1-n	U		See Tailored description
4	>>	CONTAINS	TEXT	BCID(6053) Breast Imaging Report Elements	1	M		
5	>>>	INFERRED FROM	INCLUDE	DTID(350) References to Supporting Evidence	1	U		See Tailored description

TID 4203

Breast Imaging Assessment

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CODE	EV(111005, DCM, „Assessment Category“)	1	M		DCID(6026) Mammography Assessment
3	>	HAS CONCEPT MOD	CODE	EV(G-C171, SRT, „Laterality“)	1	U		DCID(6022) Side

TID 4205

Breast Composition Section

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV(F-01710, SRT, „Breast Composition“)	1	M		
3	>	CONTAINS	CODE	EV(F-01710, SRT, „Breast Composition“)	1-n	MC	At least one of row 3, 5 shall be present	DCID(6000) Overall Breast Composition
4	>>	HAS CONCEPT MOD	CODE	EV(G-C171, SRT, „Laterality“)	1	M		DCID(6022) Side

TID 4206

Breast Imaging Report Finding Section

Type: Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV(121070, SRT, „Findings“)	1	M		
3	>	CONTAINS	INCLUDE	DTID(4201) Breast Imaging Procedure Reported	1	M		
4	>	CONTAINS	CODE	EV(121071, DCM, “Finding”)	1-n	M		DCID(6054) Breast Imaging Findings
6	>>	HAS PROPERTIES	INCLUDE	DTID(4203) Breast Imaging Assessment	1	U		See Tailored description
9	>>	HAS PROPERTIES	INCLUDE	DTID(1400) Linear Measurement	1-n	U		
13	>>	HAS PROPERTIES	CODE	EV(111035, DCM, “Lesion Density”)	1	U		DCID(6008) Density Modifier
14	>>	HAS PROPERTIES	CODE	EV(M-020F9, SRT, “Shape”)	1-n	U		DCID(6004) Mammography Characteristics of Shape
15	>>	HAS PROPERTIES	CODE	EV(111037, DCM, “Margins”)	1-n	U		DCID(6006) Mammography Characteristics of Margin
16	>>	HAS PROPERTIES	CODE	EV(111009, DCM, “Calcification Type”)	1-n	U		DCID(6010) Mammography Calcification Types
17	>>	HAS PROPERTIES	CODE	EV(111008, DCM, “Calcification Distribution”)	1	U		DCID(6012) Calcification Distribution Modifier
20	>>	HAS PROPERTIES	CODE	EV(G-C189, SRT, “Associated Finding”)	1-n	U		DCID(6056) Associated Findings for Breast
27	>>	HAS PROPERTIES	CODE	EV(CP52706-00, DCM, “Identifiable effect on surrounding tissues”)	1	U		DCID(6015) Single Image Finding From BIRADS®
30	>>	INFERRED FROM	INCLUDE	DTID(350) Referenced to Supporting Evidence	1	U		
31 ^a	>>	CONTAINS	TEXT	BCID(6053) Breast	1	U		

^a This row is a Siemens extension to the DICOM standard.

				Imaging Report Elements				
--	--	--	--	--	--	--	--	--

TID 4208**Breast Imaging Report Supplementary Data**

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			CONTAINER	EV(111414, DCM, „Supplementary Data“)	1	M		
2	>	CONTAINS	INCLUDE	DTID(4201) Breast Imaging Procedure Reported	1-n	M		See Tailored description
5	>	CONTAINS	INCLUDE	DTID(4205) Breast Composition Section	1	U		See Tailored description
6	>	CONTAINS	INCLUDE	DTID(4206) Breast Imaging Report Finding Section	1-n	U		See Tailored description
8	>	CONTAINS	INCLUDE	EV(111413, DCM, “Overall Assessment”)	1	U		
9	>>	CONTAINS	INCLUDE	DTID(4203) Breast Imaging Assessment	1	M		See Tailored description

TID 350**References to Supporting Evidence**

Type: Non-Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			IMAGE	BCID(7003) Diagnostic Imaging Report Purposes of Reference ^a	1-n	U		

TID 1002**Observer Context**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1		HAS OBS CONTEXT	CODE	EV(121005, DCM, “Observer Type”)	1-n	U		EV(121006, DCM, “Person”) EV(121007, DCM,

^a Only EV(121080, DCM, “Best illustration of finding”) is used, contains references to images including icon images.

								"Device") Defaults to Person ^a
2		HAS OBS CONTEXT	INCLUDE	DTID(1003) "Person observer identifying attributes"	1-n	MC	IFF(121005, DCM , "Observer Type") = (121006, DCM, "Person")	

TID 1003**Person Observer Identifying Attributes**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1			PNAME	EV(121008, DCM, "Person Observer Name")	1	M		

TID 1204**Language of Content Item and Descendants**

	NL	Rel with Parent	VT	Concept Name	VM	Req Type	Condition	Value Set Constraint
1		HAS CONCEPT MOD	CODE	EV(121049, DCM, "Language of Content Item and Descendants")	1	M		DCID(5000) ^b
2	>	HAS CONCEPT MOD	CODE	EV(121046, DCM, "Country of Language")	1	U		DCID(5001) ^c

^a Only the value EV(121006, DCM, "Person") is used.^b Only the value EV(eng, ISO639_2, "English") is used^c Only the value EV(us, ISO639_2, "United States") is used