


SIEMENS

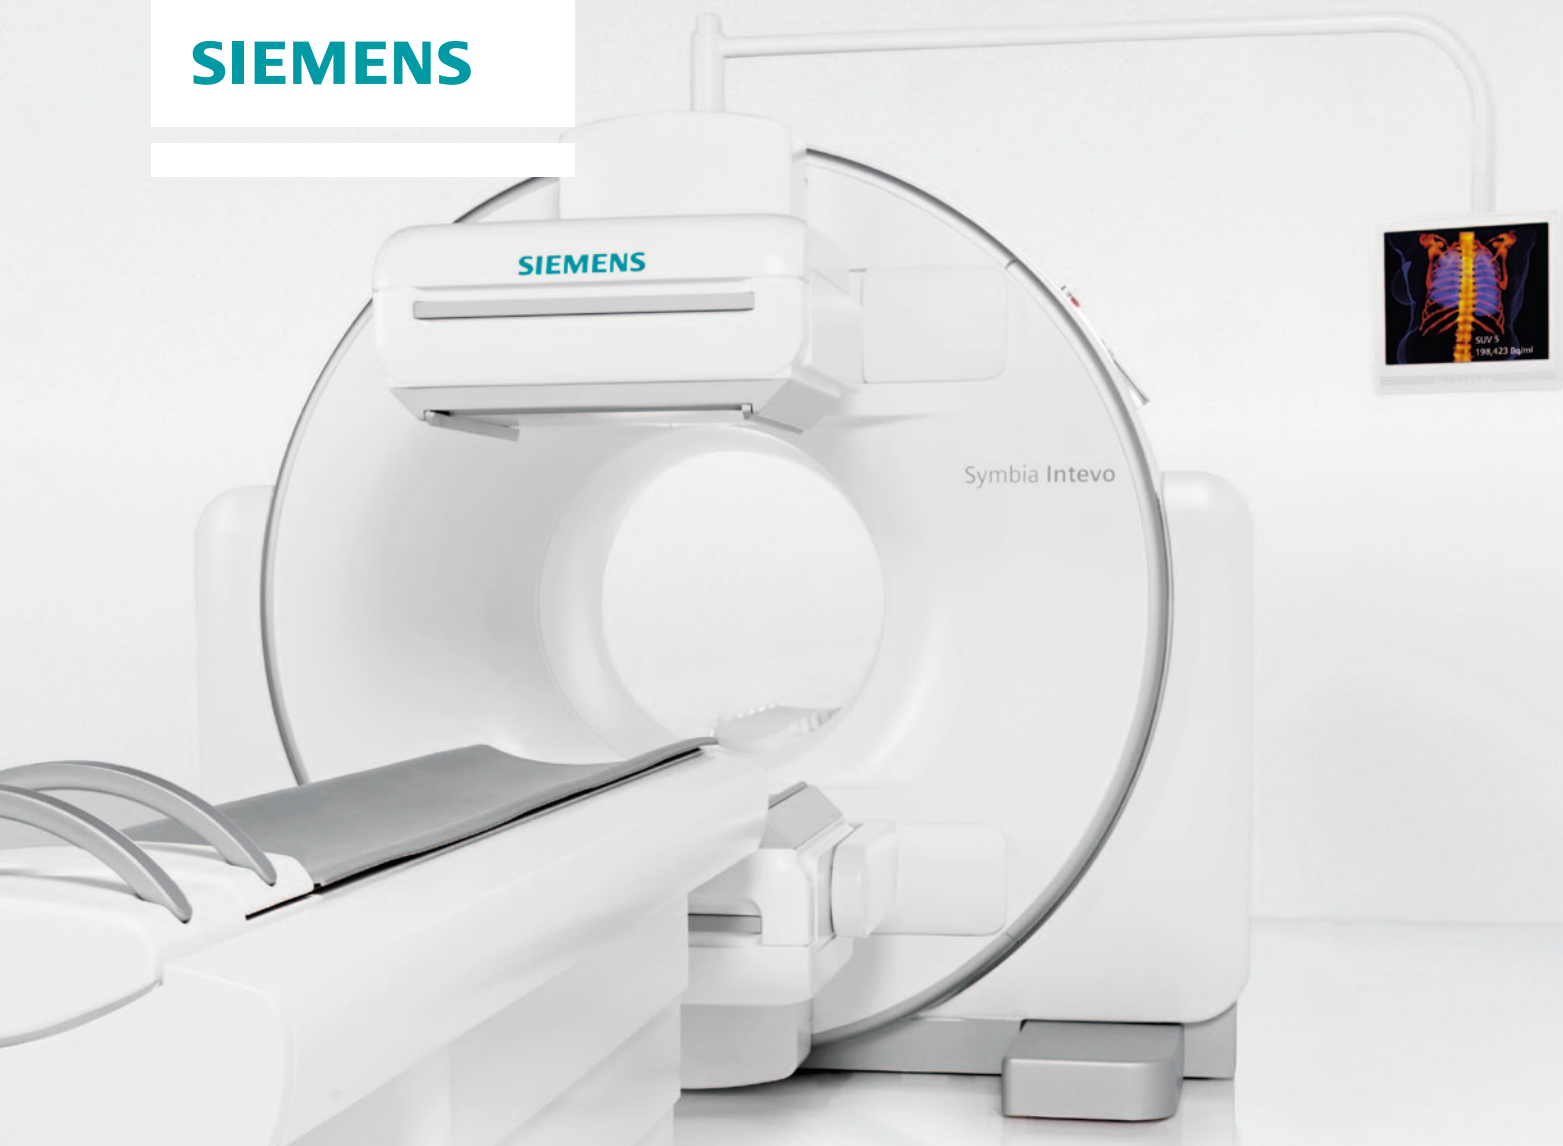

www.siemens.com/symbia-intevo


Symbia Intevo

xSPECT, the difference between seeing and knowing.

Answers for life.


Overcoming Today's SPECT/CT Limitations

Conventional SPECT/CT is limited in its ability to deliver definitive and timely answers to clinical questions in the most effective and efficient way possible. Siemens is addressing these challenges with Symbia Intevo™*, the world's first xSPECT*—a new modality that completely integrates SPECT and CT data during image reconstruction.

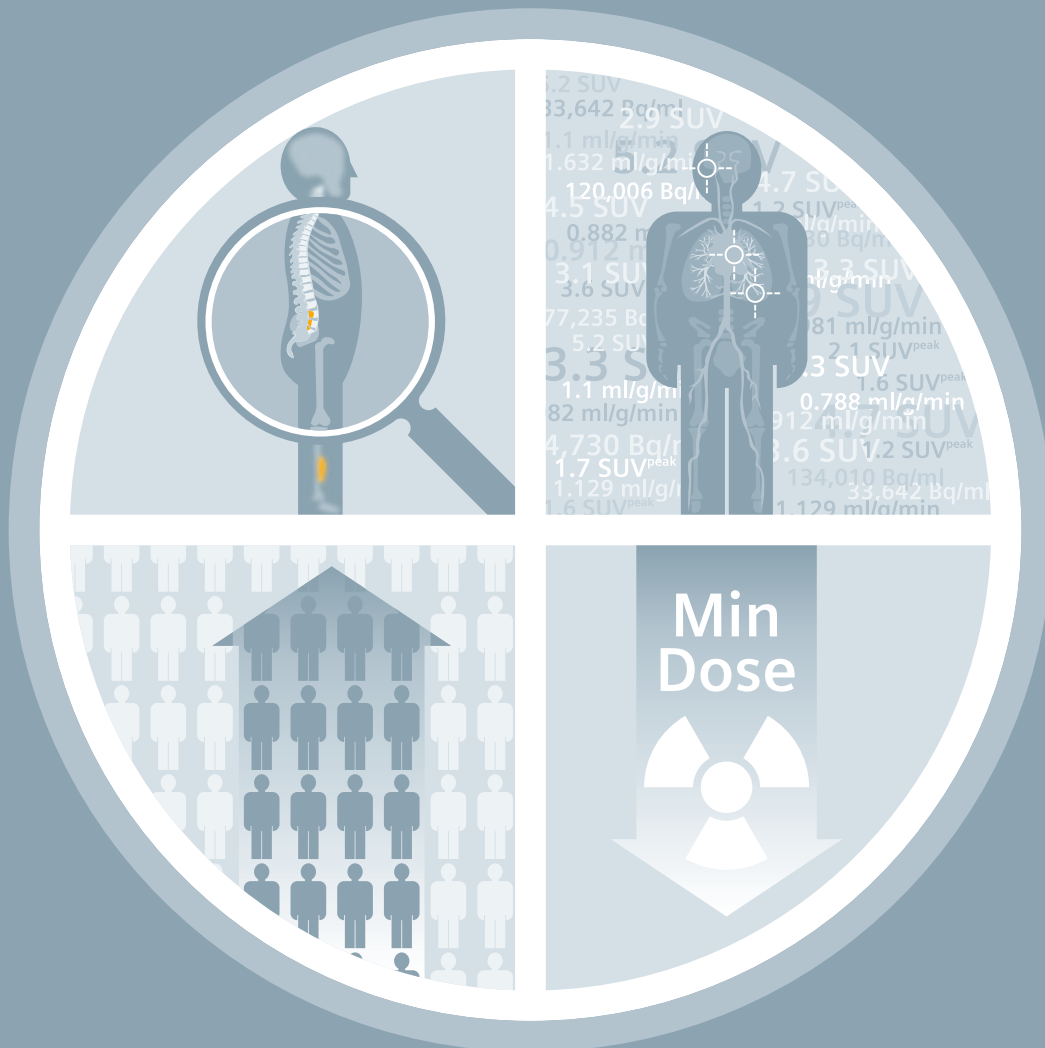


See the Unseen

| | |
|------------------|--|
| Challenge | Conventional SPECT/CT image quality is limited by the minimal amount of CT data used during reconstruction. |
| Solution | xSPECT uses CT as the frame-of-reference for image reconstruction, preserving the 512x512 resolution of the CT matrix and elevating the SPECT resolution for accurate alignment of both data sets during reconstruction. |
| Benefit | The higher resolution and clinical detail of xSPECT supports physicians' ability to more confidently distinguish between degenerative disease and cancer, reducing the need for follow-up exams (e.g., MR, biopsies). |



Quantify the Difference

| | |
|------------------|---|
| Challenge | With conventional SPECT/CT technology, assessment of disease severity and response to therapy can only be quantified through a manual, multi-step process. |
| Solution | Through a new and simple proprietary calibration method, xSPECT generates quantitative measurements** of disease uptake that are both accurate and reproducible. |
| Benefit | Symbia Intevo's quantitative capabilities support physician therapy planning and early modification of patient treatment to reduce costs associated with ineffective therapies. |



Adapt the Lowest Dose

| | |
|------------------|--|
| Challenge | To achieve sufficient image quality or faster scan times, conventional SPECT/CT systems require high dose levels. |
| Solution | With Siemens CARE (Combined Applications to Reduce Exposure) features, lower dose levels can be achieved while maintaining high image quality and fast scan times. |
| Benefit | By offering unique dose reduction features, Symbia Intevo enables 74%*** lower CT dose radiation and up to 80%*** reduction in injected dose to minimize long-term patient radiation exposure. |



Double the Throughput

| | |
|------------------|--|
| Challenge | With conventional SPECT/CT systems, long exam times and routine manual procedures can limit workflow efficiency. |
| Solution | Symbia Intevo automates routine manual tasks with exclusive features, such as Automated Quality Control and Automated Collimator Changer. Additionally, scan times have the potential for great improvement with IQ•SPECT. |
| Benefit | With Symbia Intevo's unique productivity features, institutions can save up to 50%*** more time and have the potential to double patient throughput. |




** For ^{99m}Tc and LEHR only.

*** Based on competitive literature available at time of publication. Data on file.


See the Unseen

By using the CT as the frame-of-reference for image reconstruction, xSPECT Bone* is able to extract a zone map with five different tissue segments (cortical bone, spongy bone, adipose tissue, soft tissue and air/lung) that is used to delineate the boundaries of the nuclear activity uptake during SPECT reconstruction. Through this deep integration of SPECT and CT data, xSPECT Bone is able to clearly identify post-transplant ossification disease that is not easily seen with conventional SPECT.


Conventional 3D Iterative Reconstruction

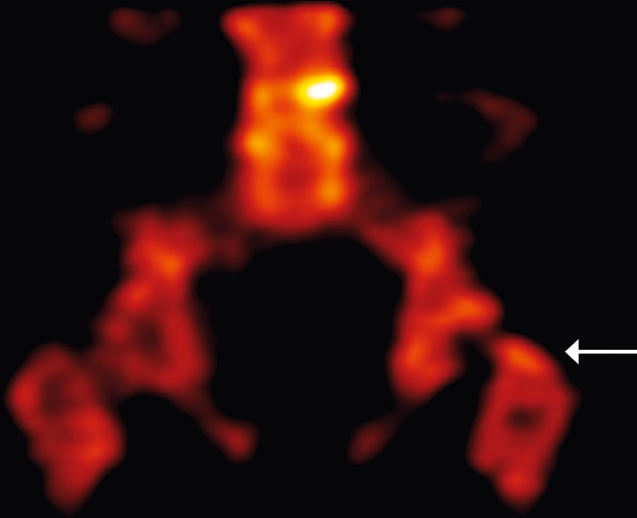


xSPECT Bone

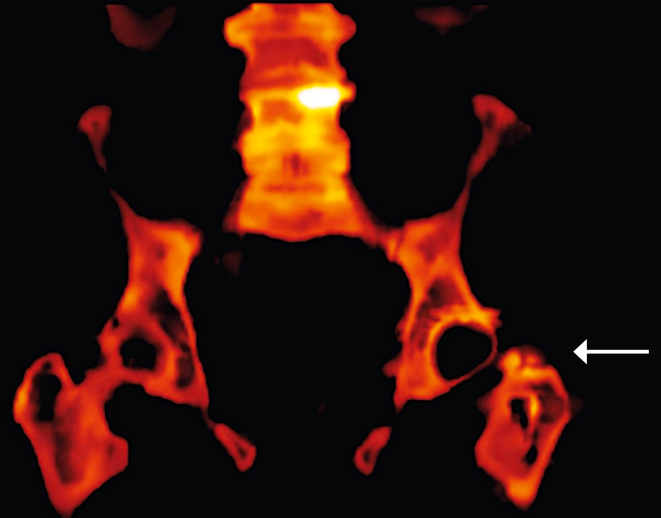

Conventional SPECT/CT

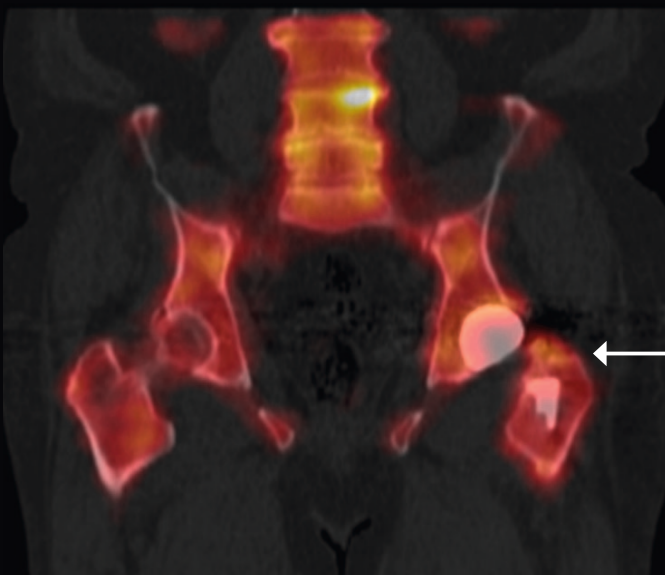

xSPECT/CT

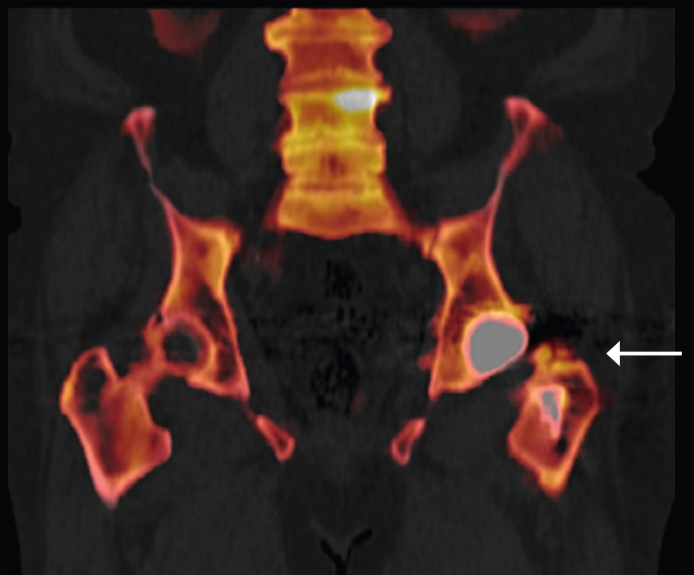

Data courtesy of Friedrich Alexander University, Erlangen, Germany
Parameters: sex: male; weight: 93 kg (205 lbs); height: 168 cm (5' 5");
injected dose: 604 MBq (16.3 mCi); 40 mAs, 130 kV; slice thickness: 3.0 mm


Quantify the Difference

Symbia Intevo employs a proprietary quantitative quality control method using a high-precision ^{57}Co source that, when combined with xSPECT reconstruction, generates accurate and reproducible quantitative images. xSPECT improves visual assessment of disease, as seen in this patient with parathyroid disease, and enables for the first time absolute quantification with xSPECT Quant*.

Max: 38.150 Bq/ml

Min: 8.770 Bq/ml

Avg.: 16.324 Bq/ml

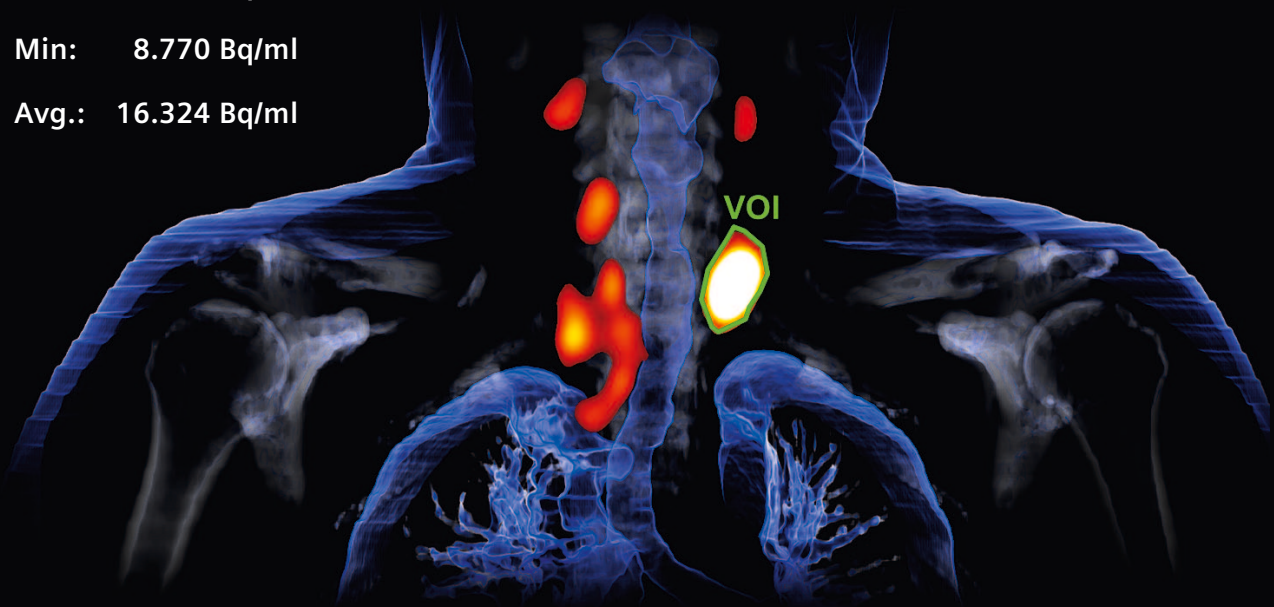


Data courtesy of Friedrich Alexander University, Erlangen, Germany
Parameters: sex: male; weight: 92 kg (120 lbs); height: 172 cm (5' 8");
injected dose: 104 MBq (2.8 mCi); 43 mAs, 130 kV; slice thickness: 3.0 mm


Adapt the Lowest Dose



Following principles such as ALARA (As Low as Reasonably Achievable) to help limit exposure to the lowest level possible, Siemens innovations significantly reduce dose compared to conventional SPECT/CT systems.

Conventional SPECT/CT*



Symbia Intevo




| |  |  | % Lower Dose |
|-----------------|---|--|--------------|
| SPECT | LEHR | 160 cpm/μCi | 26% |
| | | SMARTZOOM | 810 cpm/μCi |
| CT AC Abdomen | 120 kV | 4.35 mGy | 59% |
| | | 130 kV | 1.80 mGy |
| CT AC Cardiac | 120 kV | 1.59 mGy | 2% |
| | | 110 kV | 1.00 mGy |
| CT AC WholeBody | 120 kV | 4.35 mGy | 74% |
| | | 80 kV | 0.40 mGy |


Double the Throughput

Manual tasks require time and resources that could be focused on patient preparation, scanning and processing. Siemens solutions optimize operational efficiency and increase utilization, while offering the potential to double patient throughput.

Conventional SPECT/CT

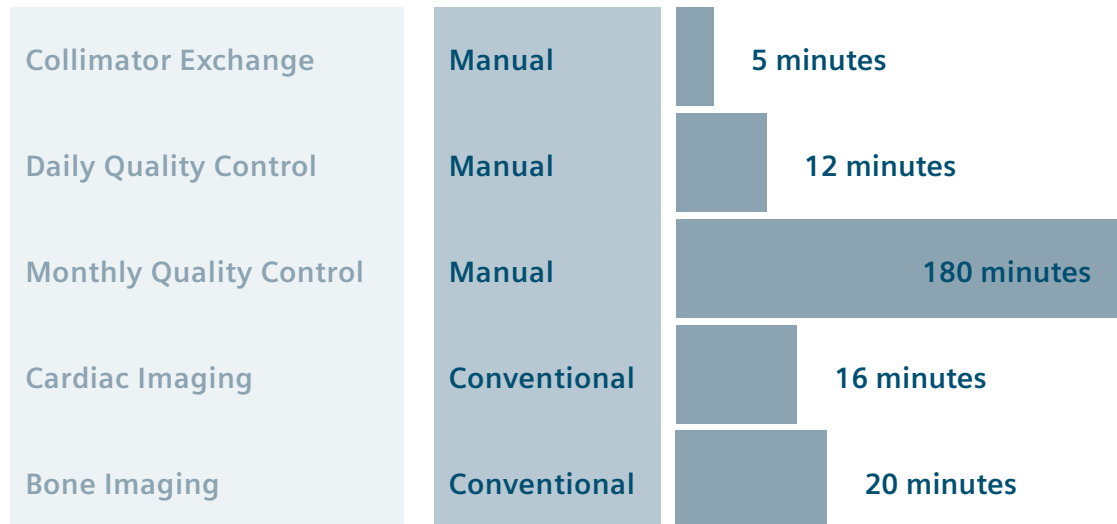

Symbia Intevo

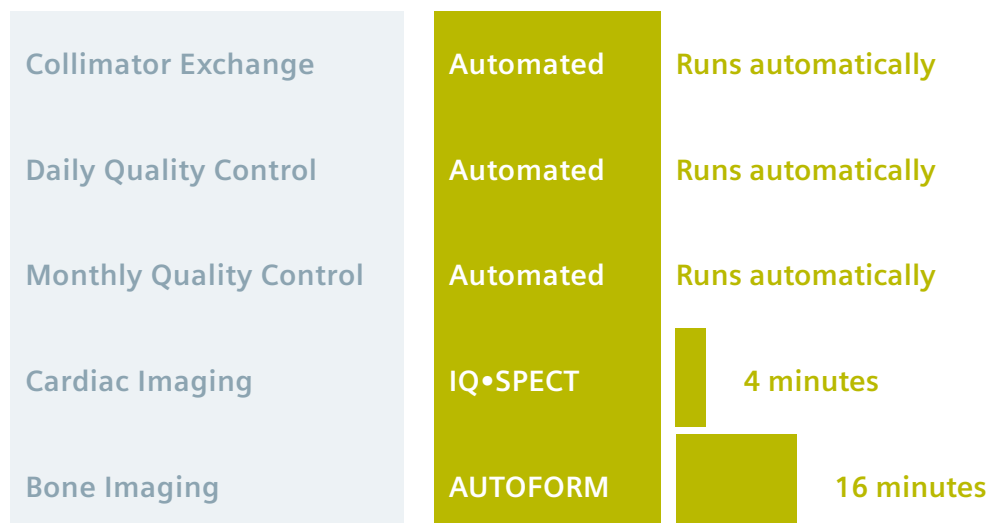

Customer Testimonials



Clinical Benefits

“With the increased image resolution and anatomical clarity from xSPECT, we’ve been able to characterize patients with just this one exam.

*With xSPECT the answers are in the images themselves, so I won’t have to do additional studies outside of the department.”**



Jerry Froelich, MD

Director of Nuclear Medicine and
Molecular Imaging, University of
Minnesota

Minneapolis, Minnesota, USA

“We have the potential to be more accurate in assessing disease severity through quantification.

*And we will be able to quantify the response to therapy.”**



Zsolt Szabo, MD, PhD

Professor of Radiology,
The Johns Hopkins Hospital

Baltimore, Maryland, USA



Torsten Kuwert, MD
Director of Nuclear Medicine
and Molecular Imaging,
University Hospital of Erlangen
Erlangen, Germany

Operational Benefits

“The system offers much improved spatial resolution. It has now become easy to precisely locate whether a focus of increased uptake is related to the cortex of the bone or to the bone marrow.

*Putting images together in your mind is a nice exercise and might be intellectually very rewarding, but having them both in one image speeds up the diagnostic process.”**



Guillaume Bouchard, MD
Nuclear Medicine Department,
Hôpital de la Cité-de-la-Santé
Laval, Quebec, Canada

Financial Benefits

*“Prior to IQ•SPECT, we had cardiac exams running on two cameras. This freed four to five hours of camera time. Now, we have reduced our wait-time and can perform more patient scans.”**



Base System Highlights

Diagnostic Spiral CT

2-, 6- and 16-slice CT configurations

Intuitive Hand Controller

Easy-to-use with descriptive controls

Autocontour

Infrared body contour system that minimizes patient-to-detector distance

Open Gantry

Patient-friendly integrated gantry design with 70 cm (27.5 in) opening for greater patient comfort

Detector Tilt

Wide variety of detector configurations adjustable to any study and patient type (e.g., gurney imaging, 76° cardiac)



HD Detectors

High-definition digital detectors that provide energy-independent performance

Patient Positioning Monitor


Self-guided, touch screen user interface with intuitive icons

Internal Electrocardiogram

Fully integrated ECG in patient bed for fast setup and less cumbersome cable

Innovative Bed Design


Low patient bed for easy access with ergonomic patient comfort accessories

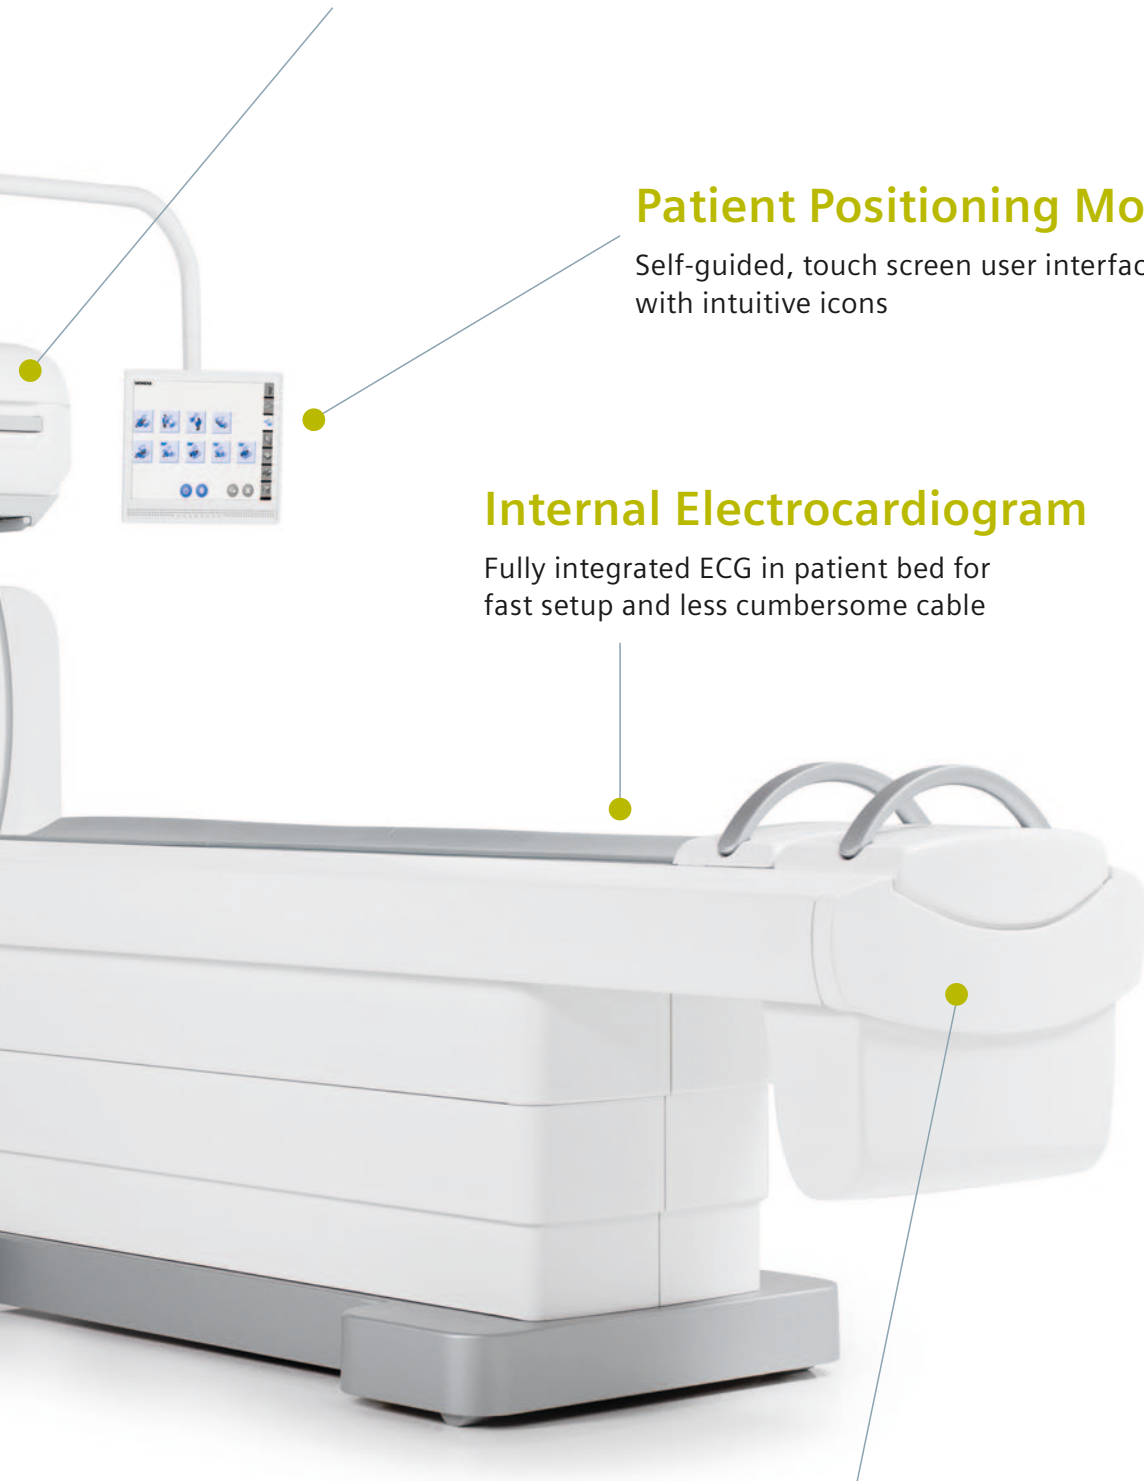

Standard Features


AUTOFORM

- Unique LEHR collimators
- 26%* higher sensitivity



UFC Detectors

- Ultra-fast ceramic CT
- Short afterglow enables up to 30%* less dose




Detector Flexibility

- Gurney and hospital bed imaging
- Detector tilt
- 76° cardiac configuration




Flash 3D

- 3D iterative reconstruction
- 50%* dose or time savings




CARE Dose4D™

- Automated real-time dose modulation
- Up to 68%* dose savings



Pediatric Friendly

- Flexible kV settings
- 80 kV, 110 kV, 130 kV




Dose Monitoring

- Structured dose reports
- Definable patient dose alerts



SureView

- Automated pitch selection
- Shorter scan times and up to 20%* dose savings

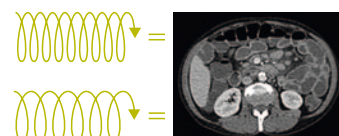

Optional Features

AQC

- Automated Quality Control
- Saves up to 1 hour each day




ACC

- Automated Collimator Changer
- 4 collimators integrated into system bed




xSPECT Bone

- High-resolution bone imaging
- Up to 80%* higher diagnostic quality




xSPECT Quant

- Quantitative imaging
- Measures activity concentration in units of Bq/ml or SUVs



IQ•SPECT

- Ultra-fast cardiac imaging
- Up to 80%* lower injected dose or faster imaging



e.media

- Integrated entertainment solution
- Helps keep patients still and comfortable




Specialty Pallets

- Pediatric
- Mammography




Symbia.net

- Anywhere**, anytime image processing and reconstruction solution



Minimum Room Size

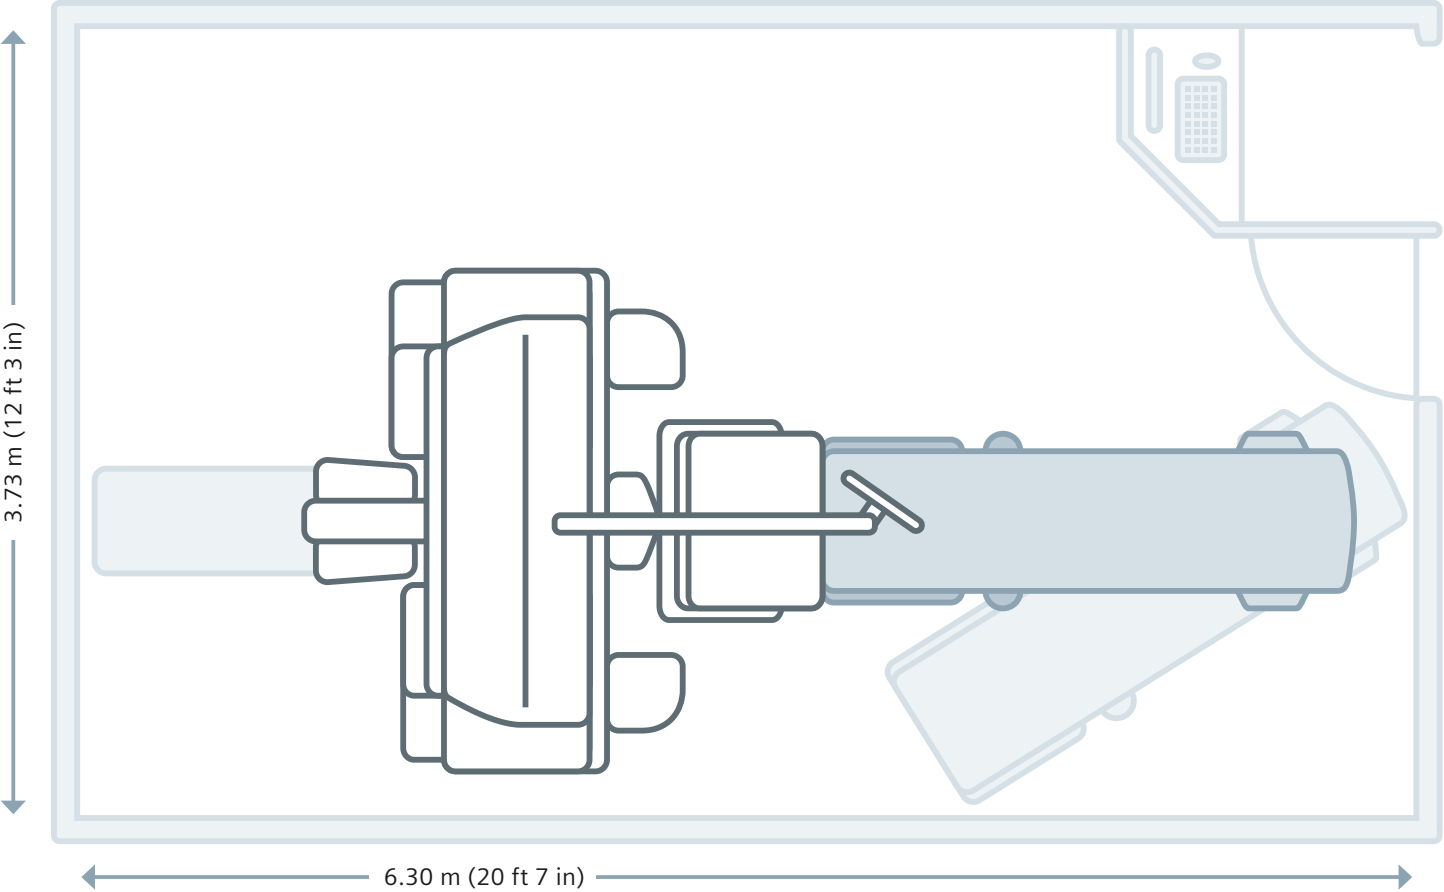

| | |
|---------------------|---|
| Room Size | 3.73 m (12 ft 3 in) x 6.30 m (20 ft 7 in) |
| Ceiling Height | 2.44 m (8 ft 0 in) |
| Hung Ceiling Height | 2.29 m (7 ft 5 in) |

Technical Specifications

| | Feature | Symbia Intevo 2, 6 and 16 |
|-------------------------|--|---|
| See the Unseen | Reconstruction frame-of-reference | CT frame-of-reference |
| | SPECT reconstruction matrix size | 256x256, 128x128, 64x64 |
| | Advanced reconstruction | xSPECT Iterative or Flash3D Iterative |
| | Zone Map (tissue classification) | Yes, with xSPECT Bone |
| | Detectors rotational uniformity | Yes |
| | Detectors rotational accuracy | 0.1° |
| | Detector caudal tilt | Yes, +16°/-16° |
| | CT focal spot size | Symbia Intevo 2: 0.8 x 0.7 mm/8° Symbia Intevo 6: 0.8 x 0.5 mm/7° and 0.8 x 0.7 mm/7° Symbia Intevo 16: 0.8 x 0.5 mm/7° and 0.8 x 0.7 mm/7° |
| | Diagnostic CT | Multi-slice spiral stand-alone diagnostic CT imaging capabilities |
| | Generator power | 40 kW with 2-slice CT and 50 kW with 6- and 16-slice CT |
| | Collimators | Low Energy and High Resolution (LEHR), Low Energy and All Purpose (LEAP), Low Energy and Ultra High Resolution, (LEUHR), Low Energy Fan Beam (LEFB), Medium Energy (ME), High Energy (HE) and SMARTZOOM (IQ•SPECT) |
| | Table flex | Rear bed support prevents flex |
| | Reconstruction workstation | 64-bit architecture |
| | CT continuous scan length | Symbia Intevo 2: 166 cm Symbia Intevo 6: 168 cm Symbia Intevo 16: 186 cm |
| | Gantry deflection matrix | Yes, 3D fully adaptive gantry deflection matrix |
| | Point spread function | Yes, 3D measured point spread function |
| | Collimator characterization | Yes, 3D measured collimator hole, shape and size |
| Quantify the Difference | Automated quantification | Yes, xSPECT Quant |
| | Quantitative volumetric analysis | Yes, in units of Bq/ml or SUV or HU units or counts-per-voxel |
| | Quantitative uncertainty % | ≤10%* |
| | Reproducible quantification | Yes, with a unique monthly quantitative calibration |
| | Quantitative calibration source | Yes, NIST precision ⁵⁷ Co source, unique to Siemens |
| Adapt the Lowest Dose | CT Dose modulation | Yes, 4D and fully automatic |
| | Flexible CT voltage settings | Yes, 80 kV, 110 kV, 130 kV |
| | CTDI Dose Values – Abdomen AC | 1.20 mGy @130 kV |
| | CTDI Dose Values – Cardiac AC | 1.56 mGy @130 kV or 1.00 mGy @110 kV or 0.4 @80 kV |
| | CTDI Dose Values – Parathyroid AC | 1.80 mGy @130 kV |
| | LEHR collimator sensitivity @10 cm | 202 cpm/μCi** |
| | SMARTZOOM collimator sensitivity @28 cm (recommended) | 810 cpm/μCi at 28 cm*** (unique to Siemens) |
| | Average Autocontour distance | 1.1 cm (0.45 in) |
| Double the Throughput | Quality control | Yes, fully automated with 2 shielded sources embedded in the patient bed |
| | Unique cardiac collimator | Yes, SMARTZOOM with 810 cpm/μCi*** |
| | Collimator exchange | Fully automatic with integrated set of collimators |

* Accuracy data validated using phantom studies for objects larger than 3 times system resolution.


** Values measured in accordance with NEMA Standards Publication NU-1 2007 using 3/8" crystal and a 5 cm diameter phantom.

*** Values measured in accordance with NEMA Standards Publication NU-1 2007 using 3/8" crystal.


xSPECT Bone

xSPECT offers easy differentiation between spongy bone and cortical bone in lumbar vertebra, enabling easy determination of lumbar disc degeneration.


Conventional 3D Iterative Reconstruction

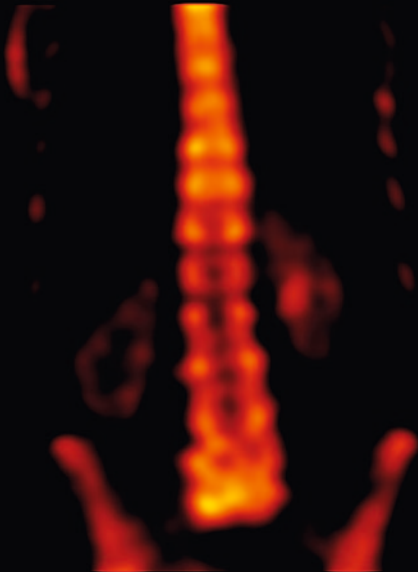


xSPECT Bone

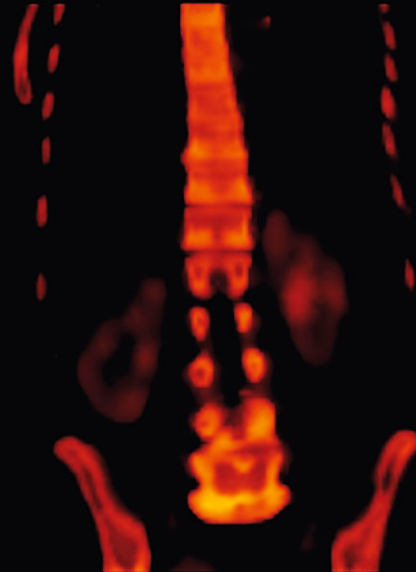

Conventional SPECT/CT

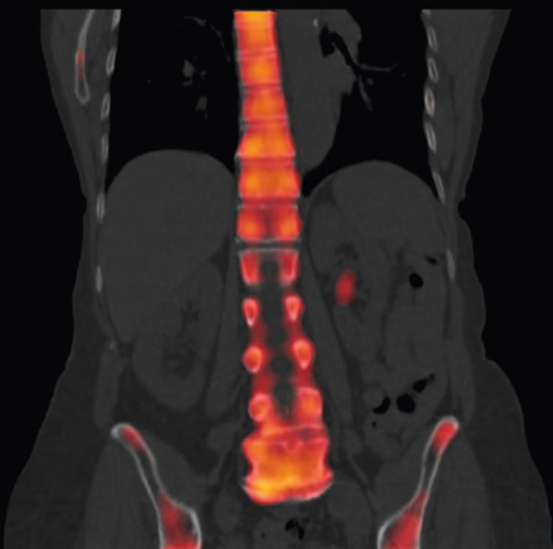


xSPECT/CT

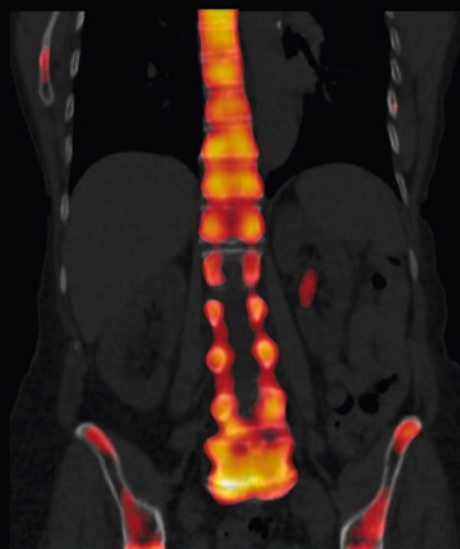


Data courtesy of Johns Hopkins University, Baltimore, Maryland, USA
Parameters: sex: female; weight: 150 kg (330 lbs); height: 170 cm (5' 6");
injected dose: 851 MBq (23 mCi); 60 mAs, 130 kV; slice thickness: 2.0 mm

Patient complained of persistent pain following vertebroplasty implantation. xSPECT Bone shows sharp delineation of increased vertebral hypermetabolism around the hypointense cemented area within the vertebrae, as well as in the vertebral pedicles, compared to the conventional SPECT reconstruction.


Conventional 3D Iterative Reconstruction

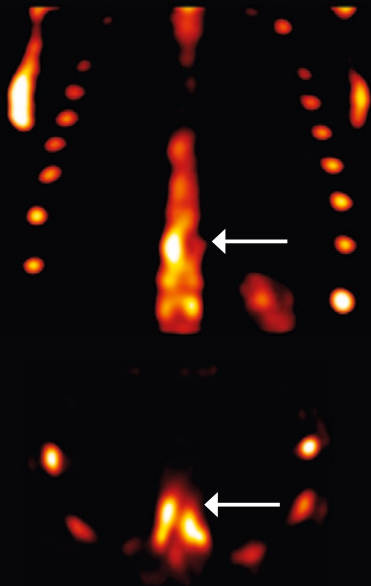


xSPECT Bone

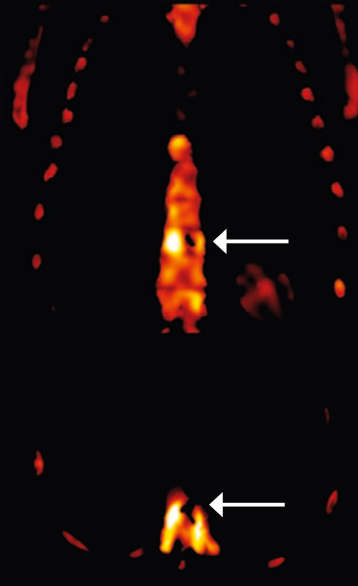

Conventional SPECT/CT

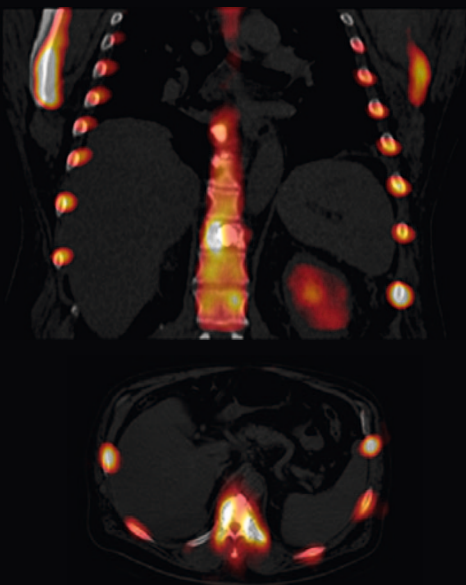


xSPECT/CT

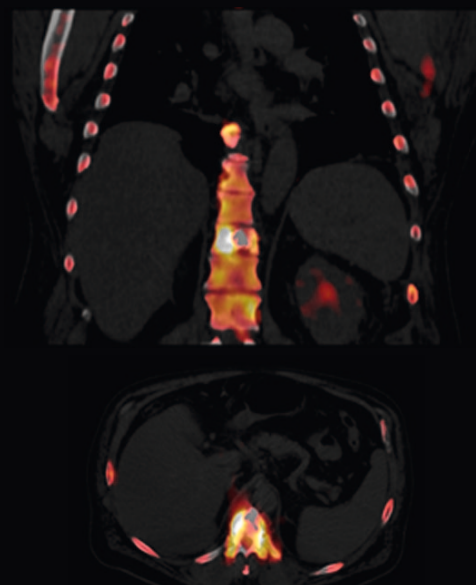

Data courtesy of University of Minnesota, Minneapolis, Minnesota, USA
 Parameters: sex: male; weight: 89 kg (196 lbs); height: 180 cm (5' 9");
 injected dose: 1011 MBq (27.32 mCi); 70 mAs, 130 kV; slice thickness: 2.5 mm


xSPECT Quant

Lumbar vertebral metastases in a patient with lung cancer. xSPECT Quant reveals high SUV in metastatic zones with low SUV in uninvolved vertebrae, suggesting osteoporosis.

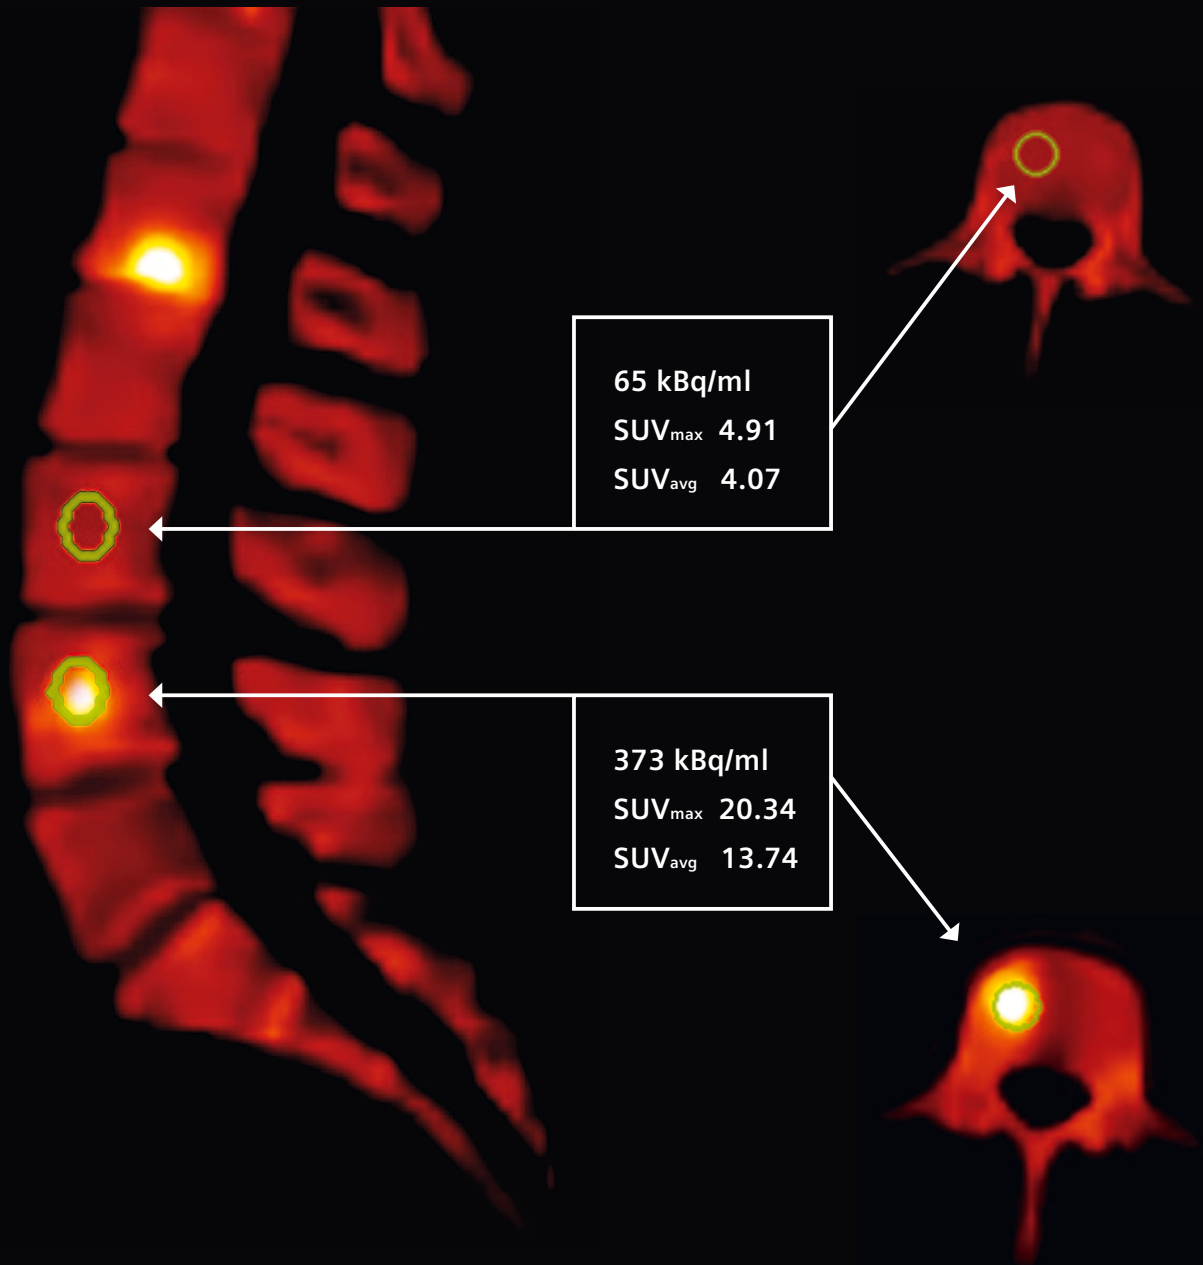

Data courtesy of Johns Hopkins University, Baltimore, Maryland, USA
Parameters: sex: female; weight: 53 kg (117 lbs); height: 160 cm (5' 2");
injected dose: 972 MBq (26.3 mCi); 60 mAs, 130 kV; slice thickness: 2.0 mm

Lumbar vertebral collapse reconstructed with xSPECT Bone and xSPECT Quant. Quantification shows high SUV in the edge of collapsed vertebrae with high SUV related to expected high skeletal metabolism, but with normal SUV in spongy bone of the normal vertebrae. xSPECT Bone shows sharp delineation of spinal canal and posterior margin of collapsed vertebrae, suggesting spinal canal compromise with possible cord compression.

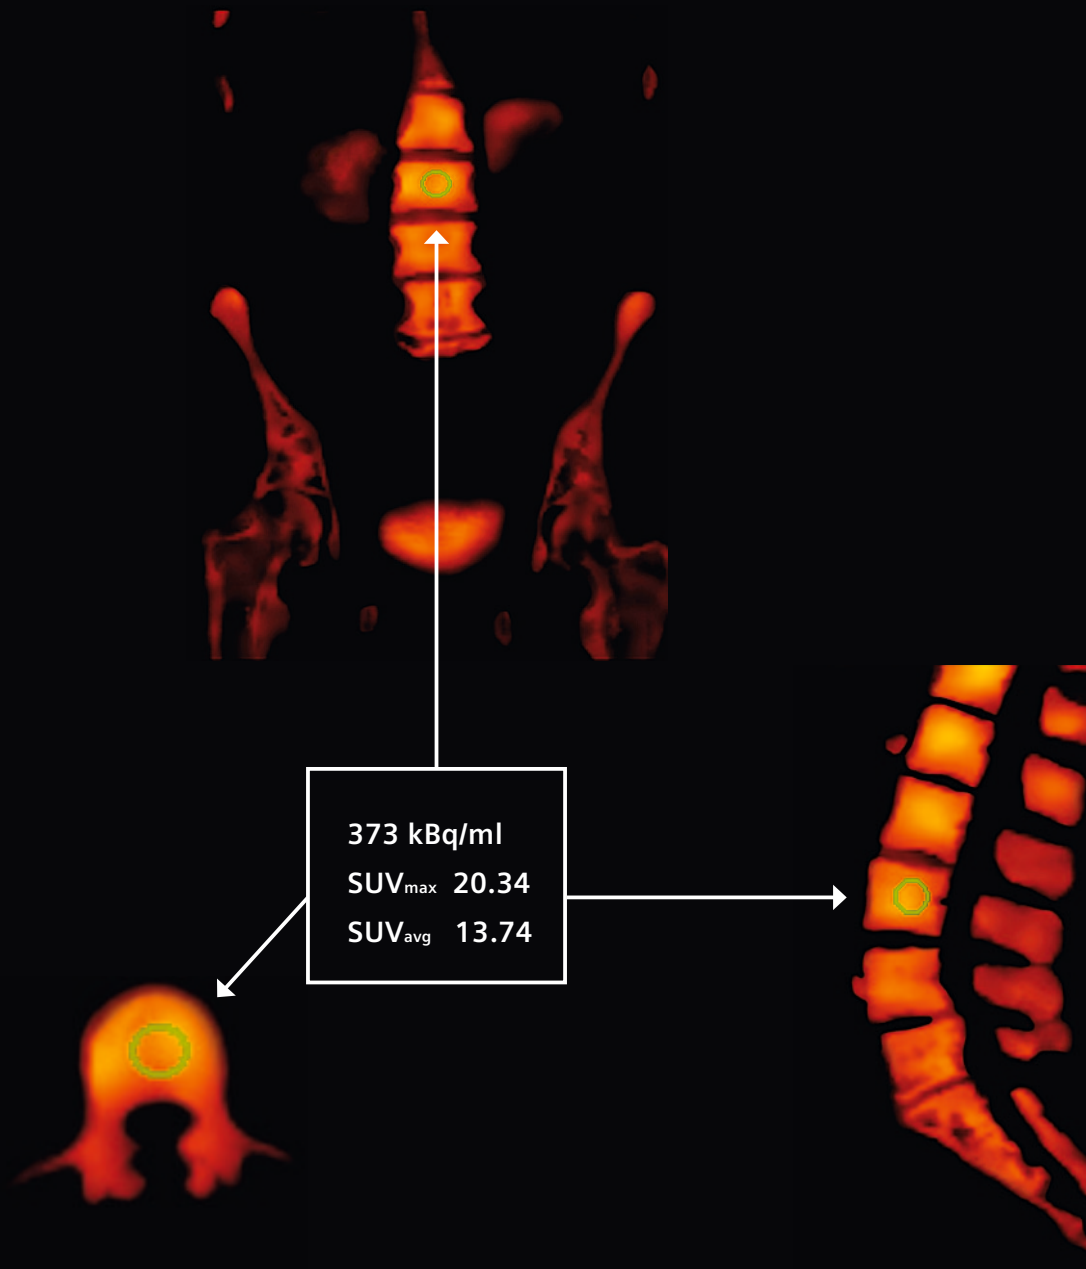

Data courtesy of University of Minnesota, Minneapolis, Minnesota, USA
Parameters: sex: female; weight: 80 kg (176 lbs); height: 170 cm (5' 6");
injected dose: 793 MBq (21.4 mCi); 50 mAs, 130 kV; slice thickness: 2.5 mm

Global Siemens Headquarters

Siemens AG
Wittelsbacherplatz 2
80333 Muenchen
Germany

Global Siemens Healthcare Headquarters

Siemens AG
Healthcare Sector
Henkestr. 127
91052 Erlangen
Germany
Telephone: +49 9131 84-0
www.siemens.com/healthcare

Global Business Unit

Siemens Medical Solutions USA, Inc.
Molecular Imaging
2501 N. Barrington Road
Hoffman Estates, IL 60192-2061
USA
Telephone: +1 847 304 7700
www.siemens.com/mi

Legal Manufacturer

Siemens Medical Solutions USA, Inc.
Molecular Imaging
2501 N. Barrington Road
Hoffman Estates, IL 60192-2061
USA
Telephone: +1 847 304 7700
www.siemens.com/mi

Order No. A91MI-10410-2C-7600 | Printed in USA | MI-2171.KF.WB.1500 | © 11.2014, Siemens AG

Trademarks and service marks used in this material are property of Siemens Medical Solutions USA or Siemens AG. All other company, brand, product and service names may be trademarks or registered trademarks of their respective holders.

All comparative claims derived from competitive data at the time of printing. Data on file. Siemens reserves the right to modify the design and specifications contained herein without prior notice. As is generally true for technical specifications, the data contained herein varies within defined tolerances. Some configurations are optional. Product performance depends on the choice of system configuration.

Please contact your local Siemens Sales Representative for the most current information or contact one of the addresses listed below. Note: Original images always lose a certain amount of detail when reproduced.

All photographs © 2014 Siemens Medical Solutions USA, Inc. All rights reserved.