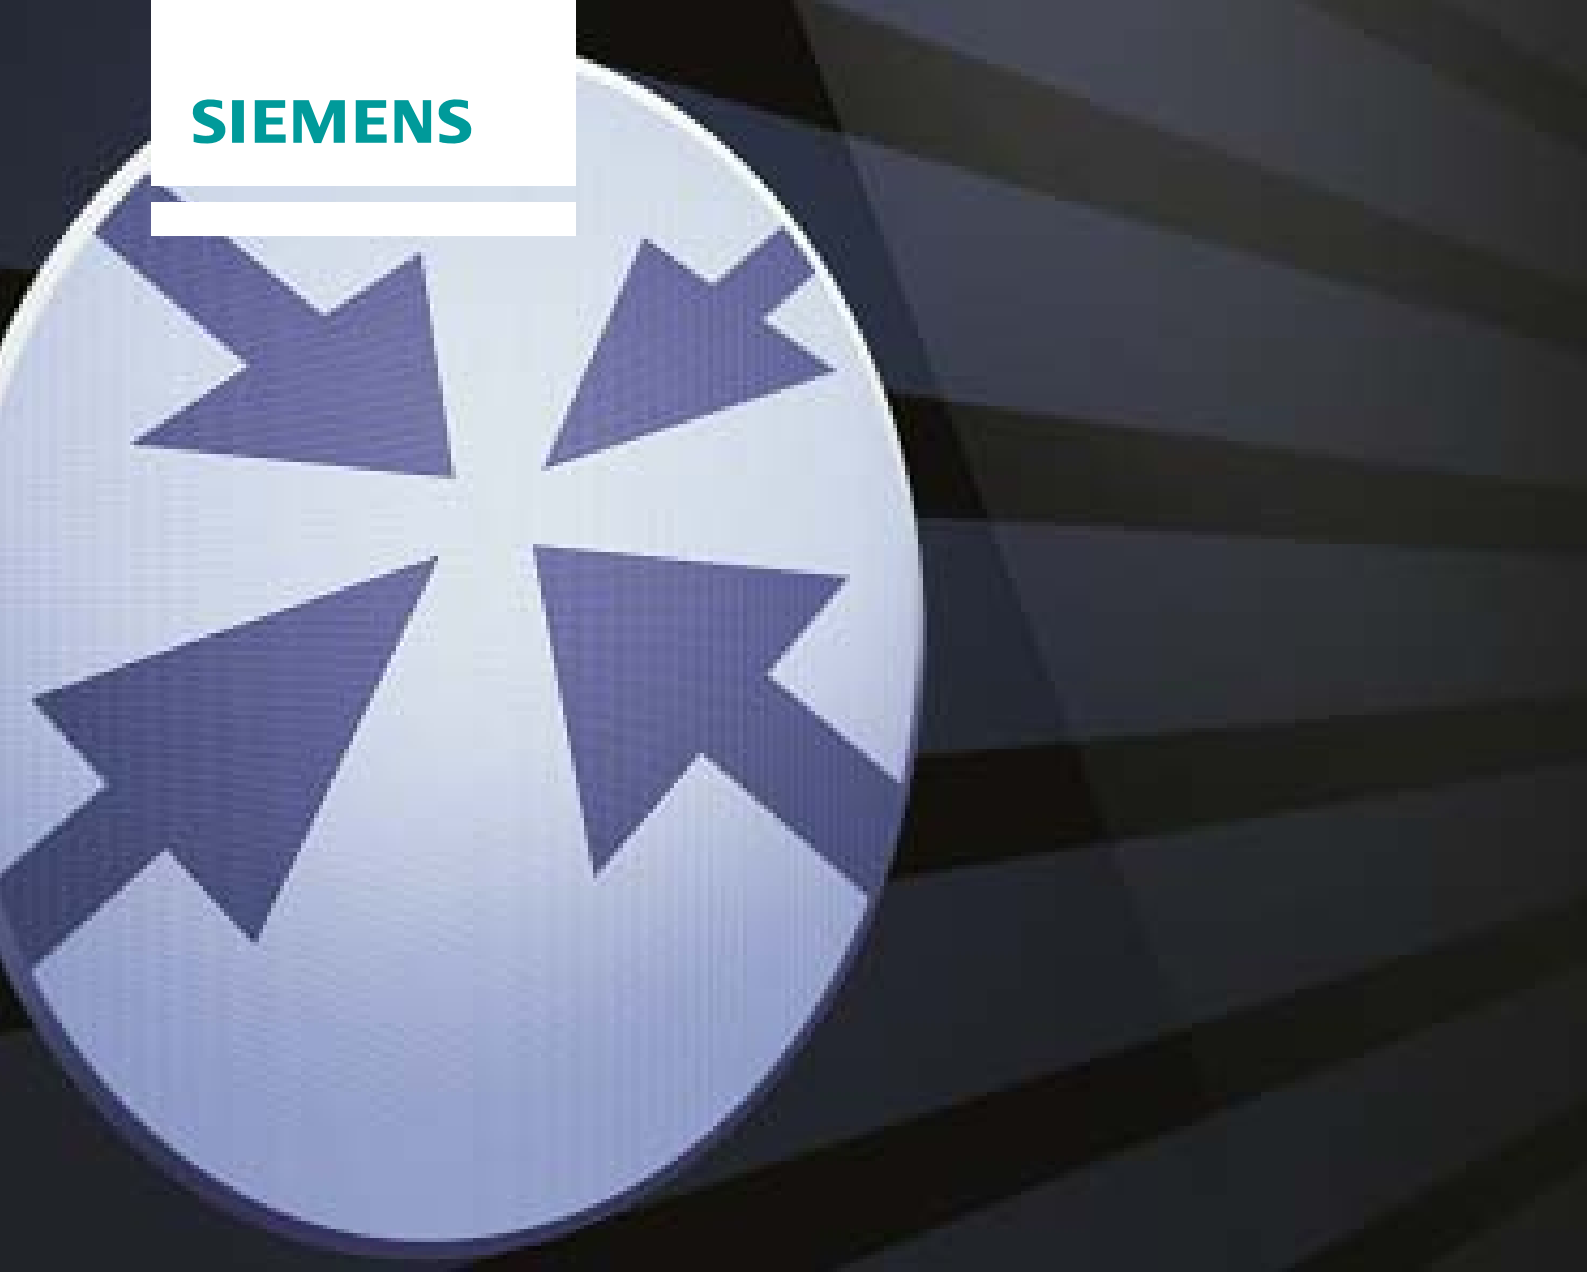

DICOM Conformance Statement

syngo.plaza

Software Version VB10B

© Siemens Healthcare GmbH, 2015

Conformance Statement Overview

***syngo*.plaza** supports eight different DICOM Application Entities:

- Main AE
- Query Spanning AE
- Retrieve Spanning AE
- MPPS Manager AE
- Modality Worklist Provider AE
- Temp AE[1]
- MPPS Image Manager AE
- Media Handling AE

The Main AE of ***syngo*.plaza** can be used to store images, query and retrieve these images. This AE also provides functionality for Storage Commitment, Printing, Modality Worklist and Mitra Report Management as listed in Table 1.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
Main AE	Verification	Yes	Yes
	Storage	Yes	Yes
	Storage Commitment	Yes	Yes
	Query/Retrieve	Yes	Yes
	Modality Worklist	Yes	No
	Print Management	Yes	No
	Mitra Report Management	Yes	No

Table 1: Supported DICOM services for Main AE

For further information on the specific SOP Classes supported by the Main AE, please refer to Table 86 and Table 87.

[1] Used in case ***syngo*®.plaza** acts as a DICOM Archive User.

The **Query Spanning AE** is a gateway for C-FIND requests. It forwards the received C-FIND requests to a set of configured query providers and merges the C-FIND responses for the query user.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
Query Spanning AE	Query[1]	Yes	Yes

Table 2: Supported DICOM services for Query Spanning AE

For further information on the specific SOP Classes supported by the Query Spanning AE, please refer to Table 88.

The **Retrieve Spanning AE** is a gateway for C-MOVE requests. It forwards the received C-MOVE requests to a set of configured retrieve providers.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
Retrieve Spanning AE	Retrieve[2]	Yes	Yes

Table 3: Supported DICOM services for Retrieve Spanning AE

For further information on the specific SOP Classes supported by the Retrieve Spanning AE, please refer to Table 89.

The **MPPS Manager AE** can receive PPS notifications from modalities and forward them to the RIS or any other capable system. It conforms to the PPS Manager defined in IHE [2].

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
MPPS Manager AE	Modality Performed Procedure Step (MPPS)	Yes	Yes

Table 4: Supported DICOM services for MPPS Manager AE

For further information on the specific SOP Classes supported by the MPPS Manager AE, please refer to Table 90.

The **Modality Worklist Provider AE** supports Modality Worklist as a Service Class Provider. It is part of the Modality Worklist Scheduler and needs to be licensed (and installed) separately.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
Modality Worklist Provider AE	Modality Worklist	No	Yes

Table 5: Supported DICOM services for Modality Worklist Provider AE

For further information on the specific SOP Classes supported by the Modality Worklist Provider AE, please refer to Table 91.

[1] The Query Spanning AE does not support Retrieve requests (C-MOVE).
[2] The Retrieve Spanning AE does not support Query requests (C-FIND).

The **Temp AE** is used in case ***syngo*.plaza** acts as a DICOM Archive User (DAU). It will be used as the destination for the DICOM objects to be de-archived. These objects will later be deleted from online storage without being archived again.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
Temp AE	Storage	No	Yes

Table 6: Supported DICOM services for Temp AE

For further information on the specific SOP Classes supported by the Temp AE, please refer to Table 86 and Table 87.

The **MPPS Image Manager AE** can receive PPS notifications from modalities and store them into the database of ***syngo*.plaza** for recording.

Application Entity	DICOM Service supported	User of Service (SCU)	Provider of Service (SCP)
MPPS Image Manager AE	Modality Performed Procedure Step (MPPS)	No	Yes

Table 7: Supported DICOM services for MPPS Image Manager AE

For further information on the specific SOP Classes supported by the MPPS Manager AE, please refer to Table 92.

The **Media Handling AE** can be used to import and export images to offline media (e.g. CD, DVD) and browse directory information from a media to be displayed at the Viewing application.

Media Storage Application Profile	Real World Activity	Role
STD-GEN-CD STD-GEN-DVD-RAM PRI-PLAZA-CD PRI-PLAZA-DVD-RAM PRI-PLAZA-DVD	Browse Directory Information	FSR
	Import Into Application	FSR
	Export To Exchange Media	FSC

Table 8: Supported DICOM Media services for Media Handling AE

For further information on the specific SOP Classes supported by the **Media Handling AE**, please refer to chapter 3.

Table of Contents

Conformance Statement Overview 2
Table of Contents 5
List of Tables 7
List of Figures 9
1 Introduction 10
1.1 General 10
1.2 Audience 10
1.3 Remarks 10
1.4 Definitions, Terms and Abbreviations 10
1.5 References 11
1.6 Structure 11
1.7 Scope and Field 12
2 Networking 13
2.1 Implementation Models 13
2.1.1 Application Data Flow 13
2.1.2 Functional Definition of Application Entities 18
2.1.3 Sequencing of Real-World Activities of the Main AE 21
2.1.4 Sequencing of Real-World Activities of the Query Spanning AE 21
2.1.5 Sequencing of Real-World Activities of the Retrieve Spanning AE 21
2.1.6 Sequencing of Real-World Activities of the MPPS Manager AE 21
2.1.7 Sequencing of Real-World Activities of the Modality Worklist Provider AE 21
2.1.8 Sequencing of Real-World Activities of the Temp AE 21
2.1.9 Sequencing of Real-World Activities of the MPPS ImageManager AE 21
2.2 AE Specifications 22
2.2.1 Main AE 22
2.2.2 Query Spanning AE 41
2.2.3 Retrieve Spanning AE 44
2.2.4 MPPS Manager AE 47
2.2.5 Modality Worklist Provider AE 49
2.2.6 Temp AE 51
2.2.7 MPPS ImageManager AE 52
2.3 Network Interfaces 55
2.3.1 Physical Network Interface 55
2.4 Configuration 56
2.4.1 AE Title / Presentation Address Mapping 56
2.4.2 Configurable parameters 56
3 Media Interchange 57
3.1 Implementation Models 57
3.1.1 Application Data Flow 57
3.1.2 Functional Definitions of AEs 57
3.1.3 Sequencing of Real-World Activities 57

3.1.4 File Meta Information for Implementation Class and Version 57

3.2 AE Specifications 58
3.2.1 Media Handling AE 58

3.3 Augmented and Private Profiles 59
3.3.1 Augmented Application Profiles 59
3.3.2 Private Application Profiles 59

3.4 Media Configuration 60

4 Support of Character Sets 61

4.1 Character Sets for *syngo*.plaza 61

5 Extensions / Specializations / Privatizations 62

5.1 Standard Extended / Specialized / Private SOPs 62
5.1.1 SIEMENS Private Non-Image IOD 62

Annex A Tables 71

A.1. Supported Storage SOP Classes of Main AE and Media Handling AE 71

A.2. Supported Non-Storage SOP Classes of Main AE 74

A.3. Supported SOP Classes of Query Spanning AE 74

A.4. Supported SOP Classes of Retrieve Spanning AE 75

A.5. Supported SOP Classes of MPPS Manager AE 75

A.6. Supported SOP Classes of Modality Worklist Provider AE 75

A.7. Supported SOP Classes of MPPS Image Manager AE 75

A.8. Supported Query attributes 75

A.9. Supported Presentation Contexts for Storage service and PRI-PLAZA SOP Classes and Transfer Syntaxes 77

A.10. Registry of DICOM Private Data Elements 91

A.11. Requirements for Viewing of DICOM Images 91

A.12. Restrictions for Viewing of DICOM Images 91

A.13. Private MITRA Report Management Query 92

List of Tables

Table 1: Supported DICOM services for Main AE 2
Table 2: Supported DICOM services for Query Spanning AE 3
Table 3: Supported DICOM services for Retrieve Spanning AE 3
Table 4: Supported DICOM services for MPPS Manager AE 3
Table 5: Supported DICOM services for Modality Worklist Provider AE 3
Table 6: Supported DICOM services for Temp AE 4
Table 7: Supported DICOM services for MPPS Image Manager AE 4
Table 8: Supported DICOM Media services for Media Handling AE 4
Table 9: Association policies for Main AE 22
Table 10: Implementation Identifying Information 22
Table 11: Association Initiation Policy – Main AE 23
Table 12: Proposed Presentation Contexts – “Send Verify” 23
Table 13: Proposed Presentation Contexts – “Send Commitment” 24
Table 14: Proposed Presentation Contexts – “Request Commitment” 25
Table 15: Proposed Presentation Contexts – “Query Objects” 26
Table 16: Status codes for Query C-FIND 26
Table 17: Proposed Presentation Contexts – “Retrieve Objects” 27
Table 18: Status codes for Retrieve C-MOVE 27
Table 19: Proposed Presentation Contexts – “Query Worklist” 28
Table 20: Modality Worklist search and return key attributes used in C-FIND request and response 28
Table 21: Status codes for Modality Worklist C-FIND 29
Table 22: Proposed Presentation Contexts – “Retrieve Reports” 29
Table 23: Proposed Presentation Contexts – “Print Job” 30
Table 24: Basic Grayscale Print Management SOP Classes 30
Table 25: Basic Color Print Management SOP Classes 31
Table 26: Default values for timing demands 31
Table 27: Attributes used to create a Film Session (N-CREATE) 31
Table 28: Status codes for Basic Film Session N-CREATE and N-DELETE 32
Table 29: Attributes used to create a Film Box (N-CREATE) 33
Table 30: Status codes for Basic Film Box N-CREATE and N-ACTION 34
Table 31: Attributes used to set a Grayscale Image Box (N-SET) 34
Table 32: Attributes used to set a Color Image Box (N-SET) 35
Table 33: Attributes used to get the printer status (N-GET) 35
Table 34: Attributes used to set a Presentation LUT (N-CREATE) 36
Table 35: Association Acceptance Policy – Main AE 36
Table 36: Accepted Presentation Contexts – “Receive Verify” 36
Table 37: Accepted Presentation Contexts – “Request Commitment” 38
Table 38: Accepted Presentation Contexts – “Provide Commitment” 38
Table 39: Accepted Presentation Contexts – “Receive Query” 39
Table 40: C-FIND SCP Return Status Codes 40
Table 41: Accepted Presentation Contexts – “Receive Retrieve” 41
Table 42: C-MOVE Return Status 41
Table 43: Association policies for Query Spanning AE 42
Table 44: Implementation Identifying Information 42
Table 45: Association Initiation Policy – Query Spanning AE 42
Table 46: Proposed Presentation Contexts – Forward Query 43
Table 47: Association Acceptance Policy – Query Spanning AE 43
Table 48: Accepted Presentation Contexts – Provide Query 44
Table 49: Association policies for Retrieve Spanning AE 44
Table 50: Implementation Identifying Information 45
Table 51: Association Initiation Policy – Retrieve Spanning AE 45
Table 52: Proposed Presentation Contexts – Forward Retrieve 46
Table 53: Association Acceptance Policy – Retrieve Spanning AE 46
Table 54: Accepted Presentation Contexts – Provide Retrieve 46

© Siemens Healthcare GmbH, 2015

Table 55: Association policies for MPPS Manager AE 47
Table 56: Implementation Identifying Information 47
Table 57: Association Initiation Policy – MPPS Manager AE 47
Table 58: Proposed Presentation Contexts – Forward MPPS 48
Table 59: Association Acceptance Policy – MPPS Manager AE 48
Table 60: Accepted Presentation Contexts – “Receive MPPS” 49
Table 61: Association policies for Modality Worklist Provider AE 49
Table 62: Implementation Identifying Information 49
Table 63: Accepted Presentation Contexts – “Provide Modality Worklist” 50
Table 64: Query matching and return key attributes for Modality Worklist Provider AE 51
Table 65: Association policies for Temp AE 51
Table 66: Implementation Identifying Information 52
Table 67: Association Acceptance Policy – Temp AE 52
Table 68: Association policies for MPPS ImageManager AE 52
Table 69: Implementation Identifying Information 53
Table 70: Association Acceptance Policy – MPPS ImageManager AE 53
Table 71: Accepted Presentation Contexts – Receive MPPS 54
Table 72: Performed Procedure Step N-CREATE Attributes 55
Table 73: N-CREATE / N-SET return codes for MPPS ImageManager AE 55
Table 74: Implementation Identifying Information 58
Table 75: PRI-PLAZA Application Profiles 59
Table 76: Siemens Non-Image IOD Module Table 64
Table 77: CSA Non-Image Module 65
Table 78: Siemens Standard Extended Modules 65
Table 79: CSA Image Header Module 66
Table 80: CSA Series Header Module 66
Table 81: MEDCOM Header Module 68
Table 82: MEDCOM History Information 68
Table 83: MEDCOM OOG Module 68
Table 84: *syngo* Report Data 69
Table 85: Registry of DICOM Data Elements 70
Table 86: Storage SOP Classes supported by Main AE and Media Handling AE 74
Table 87: Non-Storage SOP Classes supported by Main AE 74
Table 88: SOP Classes supported by Query Spanning AE 74
Table 89: SOP Classes supported by Retrieve Spanning AE 75
Table 90: SOP Classes supported by MPPS Manager AE 75
Table 91: SOP Classes supported by Modality Worklist Provider AE 75
Table 92: SOP Classes supported by MPPS Image Manager AE 75
Table 93: Supported Patient Level attributes 75
Table 94: Supported Study Level attributes 76
Table 95: Supported Series Level attributes 77
Table 96: Supported Image Level attributes 77
Table 97: Supported Presentation Contexts for Storage service 91
Table 98: Registry of Private Data Elements 91
Table 99: Grayscale Presentation State Attributes not supported 92
Table 100: Attributes for Report Content Query 93

List of Figures

Figure 1: Application Data Flow Diagram – Main AE 13
Figure 2: Application Data Flow Diagram – Query Spanning AE 15
Figure 3: Application Data Flow Diagram – Retrieve Spanning AE 16
Figure 4: Application Data Flow Diagram – MPPS Manager AE 16
Figure 5: Application Data Flow Diagram – Modality Worklist Provider AE 17
Figure 6: Application Data Flow Diagram – Temp AE 17
Figure 7: Application Data Flow Diagram – MPPS ImageManager AE 18
Figure 8: Application Data Flow Diagram – Media Handling AE 57
Figure 9: Information Model 63

1 Introduction

1.1 General

The Conformance Statement describes the DICOM interface for the Siemens PACS ***syngo*.plaza** in terms of part 2 of the DICOM Standard [1].

1.2 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

1.3 Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [1]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.

Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

1.4 Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

ACR	**A**merican **C**ollege of **R**adiology
AE	DICOM **A**pplication **E**ntity
ASCII	**A**merican **S**tandard **C**ode for **I**nformation **I**nterchange
DAP	**D**ICOM **A**rchive **P**rovider
DAU	**D**ICOM **A**rchive **U**ser
DBP	**D**icom **B**asic **P**rint
DCS	**D**ICOM **C**onformance **S**tatement
DQRY	**D**ICOM **Q**ue**ry**

DQUS	**D**ICOM **Q**uery **Us**er
DSA	**D**igital **S**ubtraction **A**ngiography
FSC	**F**ile **S**et **C**reator
FSR	**F**ile **S**et **R**eader
FSU	**F**ile **S**et **U**pdater
IOD	DICOM **I**nformation **O**bject **D**efinition
ISO	**I**nternational **S**tandard **O**rganization
LTS	**L**ong **T**erm **S**torage
MCM	**M**agic **C**ompatibility **M**odule
MPPS	**M**odality **P**erformed **P**rocedure **S**tep
MWL	**M**odality **W**ork**l**ist
NEMA	**N**ational **E**lectrical **M**anufacturers **A**ssociation
NI	**N**etwork **I**nterface
O	**O**ptional Key Attribute
PACS	**P**icture **A**rchiving and **C**ommunication **S**ystem
PDU	**P**rotocol **D**ata **U**nit
PDI	**P**ortable **D**ocument **I**maging
PPS	**P**erformed **P**rocedure **S**tep
QC	**Q**uality **C**ontrol
R	**R**equired Key Attribute
RIS	**R**adiology **I**nformation **S**ystem
SC	**S**torage **C**ommitment
SCU	DICOM **S**ervice **C**lass **U**ser (DICOM client)
SCP	DICOM **S**ervice **C**lass **P**rovider (DICOM server)
SOP	DICOM **S**ervice **O**bject **P**air
U	**U**nique Key Attribute
UI	**U**ser **I**nterface

1.5 References

[1] Digital Imaging and Communications in Medicine (DICOM), PS 3.1-2011 – PS 3.20-2011, National Electrical Manufacturers Association (NEMA).

[2] IHE Radiology Technical Framework, Vol. I – IV, http://www.ihe.net/Technical_Framework.

The Conformance Statement is based on a template taken from [1].

All DICOM Conformance Statements can be obtained from www.siemens.com/dicom.

1.6 Structure

This Conformance Statement is subdivided into multiple parts, which relate to individual documents needed to declare Conformance according to the requirements of “Part 2 - Conformance” of the DICOM Standard.

Those parts are:

- **“Network Conformance Statement” for Network related Services:**
  - Storage - User/Provider (includes Verification - User/Provider)
  - Storage Commitment - User/Provider
  - Query/Retrieve - User/Provider
  - Modality Performed Procedure Step – User/Provider
  - Modality Worklist - User/Provider

  - Print - User
  - *Private MITRA Report Management - User*
- **"Media Interchange Conformance Statement"**
- **A general Appendix.**

1.7 Scope and Field

***syngo*.plaza** offers advanced PACS functionality in a comprehensive package for all imaging needs in radiology and cardiology.

***syngo*.plaza** delivers a wide array of functional benefits that address customer needs and focus on innovation. The solution is suitable for institutions performing a low amount of procedures such as in Diagnostic Imaging Centers (DIC) and is also able to handle high procedure volumes.

2 Networking

2.1 Implementation Models

2.1.1 Application Data Flow

2.1.1.1 Main AE

The Main AE of ***syngo*.plaza** is started automatically upon startup of the application.

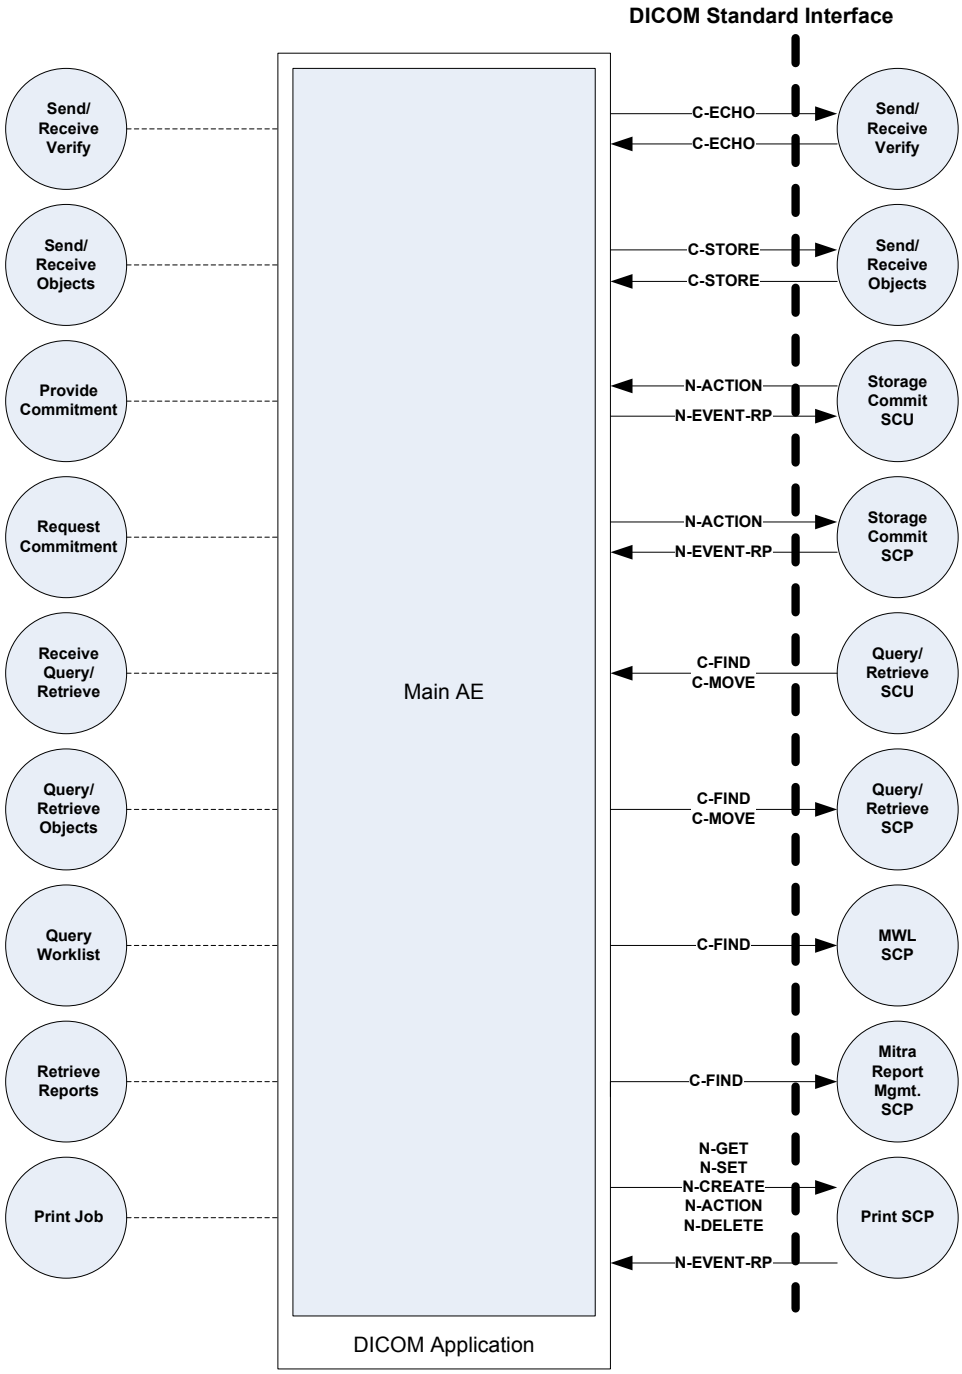

Figure 1: Application Data Flow Diagram – Main AE

The Main AE supports the following real-world activities:

- Send/Receive Verify
  - C-ECHO requests are responded in order to verify DICOM communication
  - With the help of a command line tool ***syngo*.plaza** can send C-ECHO requests to verify DICOM communication
- Send Objects (Sending of DICOM objects, e.g. Images, Structured Reports, Presentation States)
  - The objects to be transferred are selected within the ***syngo.p*laza** UI and transfer is manually activated by the user. The referenced objects are then sent to the remote DICOM node (Storage SCP).
  - For archiving purposes to a DICOM Archive the transfer to the DICOM Archive is automatically triggered by internal rules.
  - In case of autoroute (e.g. new images are forwarded after storage, images are sent after a change of the exam status) the relevant series are forwarded to the configured DICOM node.
  - As a response to retrieve event from an external DICOM node.
- Receive Objects (Receiving of DICOM objects (e.g. Images, Structured Reports, Presentation States)
  - Configured DICOM nodes may send at any time supported DICOM objects to the Main AE. After an object is received, the transfer to the ***syngo*.plaza** Short Term Storage (STS) is initiated.
- Request Commitment
  - After transmitting the images to a remote DICOM node ***syngo*.plaza** can be configured to requests a Storage Commitment.
  - It is also possible to configure ***syngo*.plaza** to send Storage Commitment requests after user triggered send operation and autoroute.
- Provide Commitment
  - If the sending system (see above) is supporting Storage Commitment, it also may send a Storage Commitment request (N-ACTION-RQ) for the stored objects. ***syngo*.plaza** can act as Storage Commitment provider only if it is configured as an archiving node.
- Receive Query/Retrieve (Replying to query and retrieval requests)
  - ***syngo*.plaza** responds to query requests based on the available DICOM meta data stored in the database. If a remote node sends retrieval requests for one or more available objects, ***syngo*.plaza** sends the referenced objects to the remote node. The requesting node may also ask to forward the objects to a third node. This is possible as far as the third node is correctly configured within ***syngo*.plaza.**
- Query/Retrieve Objects (Initiating Query / Retrieve)
  - ***syngo*.plaza** may query a remote node for its internal managed DICOM objects.

- ***syngo.*plaza** may request a remote node to retrieve a set of referenced DICOM objects. Therefore ***syngo.*plaza** initiates a move request to the remote node, which in turn stores the requested objects to ***syngo.*plaza**.

- Query Worklist (querying Modality Worklist Information)
  - ***syngo.*plaza** supports querying worklist information from a Modality Worklist SCP in order to update patient demographics while importing images, saving copies of existing data or for QC operations.

- Retrieve Reports (Retrieving reports via MITRA service)
  - ***syngo.*plaza** requests the Report Manager (typically the RIS) using a private SOP class to retrieve the content of a report.

- Print Job (Printing DICOM objects)
  - The user can load relevant images to the “filming” application of ***syngo.*plaza.**
  - The layout print settings may be adapted and the print job is sent to the printer.

2.1.1.2 Query Spanning AE

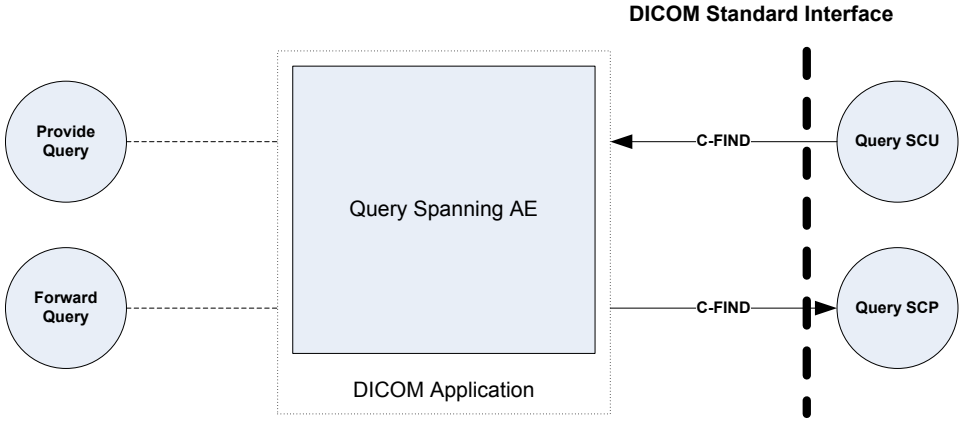

Figure 2: Application Data Flow Diagram – Query Spanning AE

The Query Spanning AE supports the following real-world activities:

- Provide Query (Receiving Query requests: C-FIND)
  - Workstations or other devices may send C-FIND requests to ***syngo.*plaza**. These messages may be forwarded to a set of configured Query SCP nodes.

- Forward Query (Forwarding Query requests: C-FIND)
  - ***syngo.*plaza** may be configured to forward C-FIND messages received from any Query SCU to a set of configured nodes (supporting Query SCP). The responses from the different Query SCP nodes are collected together to provide the original Query SCU a consolidated view on the matches of all Query SCPs.

2.1.1.3 Retrieve Spanning AE

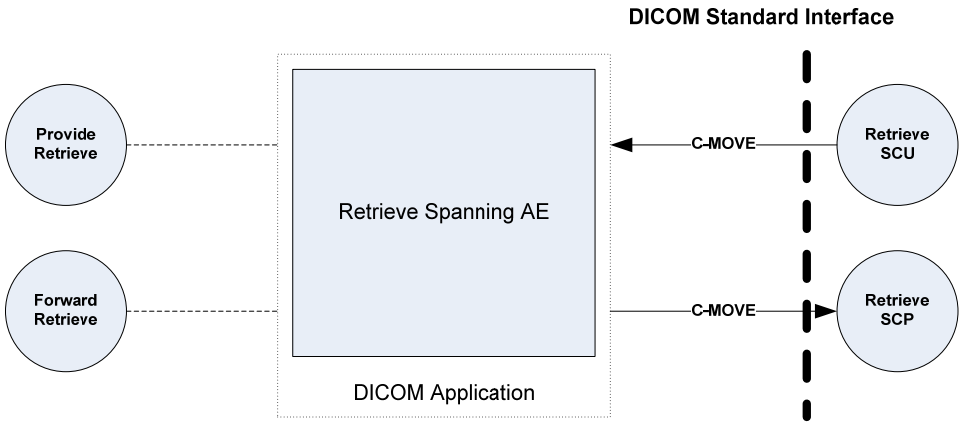

Figure 3: Application Data Flow Diagram – Retrieve Spanning AE

The Retrieve Spanning AE supports the following real-world activities:

- Provide Retrieve (Receiving Retrieve requests: C-MOVE)
  - Workstations or other devices may send C-MOVE requests to ***syngo*.plaza**. These messages may be forwarded to a set of configured Retrieve SCP nodes.
- Forward Retrieve (Forwarding Retrieve requests: C-MOVE)
  - ***syngo*.plaza** may be configured to forward C-MOVE messages received from any Retrieve SCU to a set of configured nodes (supporting Retrieve SCP). This provides the original Retrieve SCU a central entry point for all Retrieve SCPs.

2.1.1.4 MPPS Manager AE

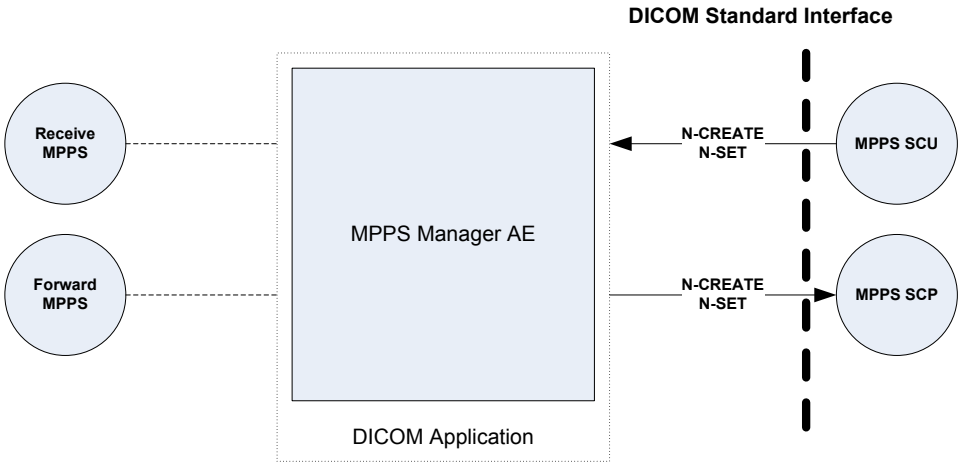

Figure 4: Application Data Flow Diagram – MPPS Manager AE

The MPPS Manager AE supports the following real-world activities:

- Receive Modality Performed Procedure Steps

- Modalities may send MPPS to ***syngo.*plaza**. This MPPS messages may be forwarded to any configured node.

- Forward Modality Performed Procedure Steps

  - ***syngo.*plaza** may be configured to forward MPPS messages received from the modality to any configured node (typically the RIS). It is possible to configure multiple destinations.

2.1.1.5 Modality Worklist Provider AE

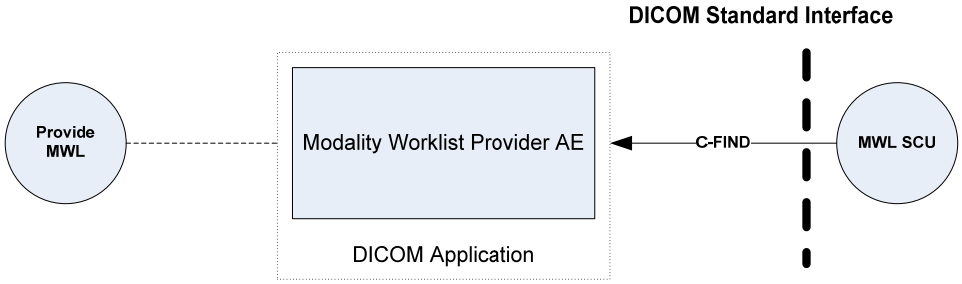

Figure 5: Application Data Flow Diagram – Modality Worklist Provider AE

The Modality Worklist Provider AE supports the following real-world activities:

- Provide Modality Worklist

  - The MWL Scheduler is a web based planning system of ***syngo.*plaza** that enables you to schedule appointments for examinations. Based on this information ***syngo.*plaza** provides worklists for modalities.

2.1.1.6 Temp AE

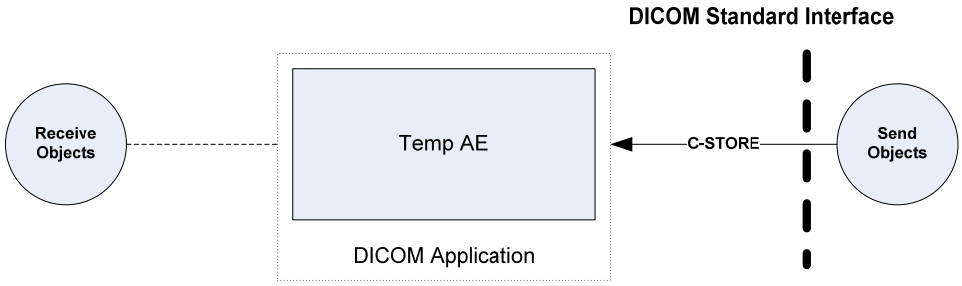

Figure 6: Application Data Flow Diagram – Temp AE

The Temp AE supports the following real-world activities:

- Receive Objects (Receiving of DICOM objects (e.g. Images, Structured Reports, Presentation States)

  - The Temp AE is only used in case ***syngo.*plaza** acts as a DICOM Archive User (DAU). When images that are archived on a DICOM Archive Provider (DAP) need to be de-archived, ***syngo.*plaza** will send a C-MOVE request with the TEMP AE as the move destination.

2.1.1.7 MPPS Image Manager AE

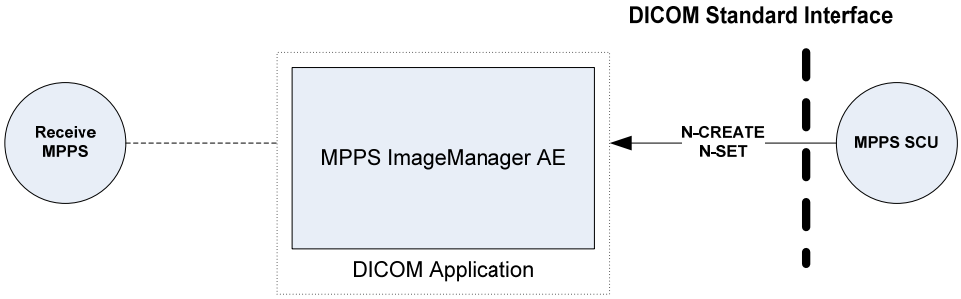

Figure 7: Application Data Flow Diagram – MPPS ImageManager AE

The MPPS ImageManager AE supports the following real-world activities:

- Receive Modality Performed Procedure Steps
  - Modalities may send MPPS to ***syngo*.plaza**. These MPPS messages are recorded in the internal database and can be displayed for the user.

2.1.2 Functional Definition of Application Entities

The SCP components of the Application Entities of ***syngo*.plaza** are operating as background server processes. They exist as soon as the system is powered up and wait for association requests. Upon accepting an association with a negotiated Presentation Context they start to receive and process the request described in the following sections.

2.1.2.1 Functional Definition of Main AE

2.1.2.1.1 Verification

Verification requests will be processed and responded by the Main AE.

2.1.2.1.2 Storage

The **Storage SCU** of the Main AE is invoked in the following cases:

- If it is internally triggered by the Retrieve Application that is responsible for processing retrieve requests.
- By a trigger of the internal communication system in case of autoroute or a change to the examination status.
- In case ***syngo*.plaza** is configured to archive its images to an external DICOM Archive (***syngo*.plaza** is Dicom Archive User), the Storage SCU is invoked if the archiving is triggered by an internal event. If the images could successfully be stored to the DICOM Archive, a subsequent Storage Commitment is necessary to secure the storage of these images at the DICOM Archive.
- In case a user manually selects images from the ***syngo*.plaza** UI and initiates transfer to a remote node.

The request consists of data describing the composite image objects selected for storage and the destination AET. An association is negotiated with the destination AE and the image data is transferred using the C-STORE DIMSE-Service. The transfer status is reported to the initiator of the Storage request.

The **Storage SCP** of the Main AE starts to receive the Composite Image Objects and store them into the STS after accepting an association with a negotiated Presentation Context.

Please be aware that in case ***syngo*.plaza** acts as a DICOM Archive User all Storage SOP Classes that are sent to ***syngo*.plaza** and that are generated by ***syngo*.plaza** (e.g. Presentation States) must also be supported by the DICOM Archive Provider. This is important in order to ensure that all DICOM objects sent to ***syngo*.plaza** can be archived.

Also the AET and port of the DICOM Archive Provider must be the same for Storage and Storage Commitment.

2.1.2.1.3 Storage Commitment

Additional to each successfully completed send job, modalities can trigger a Storage Commitment request for the safekeeping of the images sent to ***syngo*.plaza**.

The **Storage Commitment SCP** of the Main AE is only enabled if ***syngo*.plaza** is configured as an archiving node. It will send the commitment response (N-EVENT-RP) on a new association. A successful commitment is only sent back, if the stored objects were successfully archived.

In case images were sent to a remote DICOM Archive node for archiving purpose, ***syngo*.plaza** as **Storage Commitment SCU** will subsequently send a Storage Commitment request (N-ACTION-RQ) to the DICOM Archive. After the request has been sent, the association is closed. It is expected that the Storage Commitment Provider sends the commitment (N-EVENT-RP) through a new association to the Main AE.

2.1.2.1.4 Query/Retrieve

The DICOM **Query SCU** of ***syngo*.plaza** is waiting for requests from the User via the UI of ***syngo*.plaza**. When a request is started, the Main AE initiates an association with a remote Query SCP.

The DICOM **Retrieve SCU** of ***syngo*.plaza** initiates a C-MOVE DIMSE request to the remote Retrieve SCP. The remote Retrieve SCP in turn starts C-STORE sub-operations to the ***syngo*.plaza** Storage SCP.

The DICOM **Query/Retrieve SCP** of ***syngo*.plaza** responds to C-FIND DIMSE services from a remote SCU. C-MOVE requests involve the ***syngo*.plaza** DICOM Query/Retrieve SCP application to initiate a C-STORE sub-operation to send image objects to a remote Storage SCP.

2.1.2.1.5 Print

The ***syngo*.plaza** DICOM print application supports the print management DIMSE services as SCU.

The ***syngo*.plaza Print SCU** is invoked by the user interface to setup film-sheet layout and whenever an image is ready to be printed on film. Whenever a film-sheet is ready to print the related data is used to supply the Information to the SOP Classes of the Print Management Service Class.

2.1.2.1.6 Query Worklist

In order to assign correct patient demographics while importing images, saving copies of existing data or for QC operations, ***syngo*.plaza** acts as a **Modality Worklist SCU** to support querying worklist information from a Modality Worklist SCP.

2.1.2.1.7 MITRA Report Management

***syngo*.plaza** uses the Report Management service class to fetch reports from the RIS acting as a **Mitra Report Management SCU**.

Usually ***syngo*.plaza** is actively notified by the RIS about new or updated reports via HL7 messages. This can be used to fetch reports from RIS via DICOM, if configured. Else, new received examinations or the request of a user to display a report can be used as trigger to fetch reports from RIS via DICOM.

2.1.2.2 Functional Definition of Query Spanning AE

2.1.2.2.1 Query

The Query Spanning AE of ***syngo*.plaza** receives C-FIND requests from the Query SCU. These are forwarded to a set of other configurable Query SCPs. The C-FIND responses from all Query SCPs are merged together and sent back to the Query SCU.

2.1.2.3 Functional Definition of Retrieve Spanning AE

2.1.2.3.1 Retrieve

The Retrieve Spanning AE of ***syngo*.plaza** receives C-MOVE requests from the Retrieve SCU. These are forwarded to a set of other configurable Retrieve SCPs.

This is normally used for RIS triggered Prefetch jobs in case the RIS doesn't know about the exact location of the priors.

2.1.2.4 Functional Definition of MPPS Manager AE

2.1.2.4.1 MPPS

The ***syngo*.plaza** MPPS SCP stores information from the MPPS SCU. The received MPPS messages can be forwarded to a single target destination.

2.1.2.5 Functional Definition of Modality Worklist Provider AE

2.1.2.5.1 Modality Worklist

The **Modality Worklist Scheduler** is an option in ***syngo*.plaza** that provides a web-based user interface for the scheduling of resources (e.g. Modality) as well as planning of procedures in these resources. The Modality Worklist Provider AE is part of it and provides Worklist Information for modalities based on the information from the Scheduler.

2.1.2.6 Functional Definition of Temp AE

2.1.2.6.1 Storage

The Storage SCP of the Temp AE is used in case ***syngo*.plaza** acts as a DIOCM Archive User (DAU). It will receive the Composite Image Objects from the DICOM Archive Provider (DAP) after ***syngo*.plaza** has submitted a C-MOVE request to the DAP with the Temp AE as the destination. When these objects are received they are stored as temporary objects. They will be deleted at a later point in time without being archived again.

2.1.2.7 Functional Definition of MPPS Image Manager AE

2.1.2.7.1 MPPS

The MPPS ImageManager AE is able to receive MPPS requests from modalities. These messages are recorded in the database for informational purposes and can be reviewed via ***syngo*.plaza** client applications. However they are not evaluated for changing the status of a procedure in the internal database.

2.1.3 Sequencing of Real-World Activities of the Main AE

N.a.

2.1.4 Sequencing of Real-World Activities of the Query Spanning AE

N.a.

2.1.5 Sequencing of Real-World Activities of the Retrieve Spanning AE

N.a.

2.1.6 Sequencing of Real-World Activities of the MPPS Manager AE

N.a.

2.1.7 Sequencing of Real-World Activities of the Modality Worklist Provider AE

N.a.

2.1.8 Sequencing of Real-World Activities of the Temp AE

N.a.

2.1.9 Sequencing of Real-World Activities of the MPPS ImageManager AE

N.a.

2.2 AE Specifications

2.2.1 Main AE

2.2.1.1 SOP Classes

The Main AE provides Standard Conformance to the SOP Classes listed in Table 86 and Table 87.

2.2.1.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1	
Max PDU size	64512	
Maximum number of simultaneous associations as an association acceptor	Storage	40
	Query	40
	Retrieve	40
Maximum number of simultaneous associations as an association initiator	Storage	4
	Query	20
	Retrieve	10
	Print[1]	1
	Modality Worklist	1
	Report Management	1
	Storage Commitment	unlimited

Table 9: Association policies for Main AE

2.2.1.2.1 Asynchronous Nature

This version of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.1.2.2 Implementation Identifying Information

The Main AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name as listed in Table 10.

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 10: Implementation Identifying Information

2.2.1.3 Association Initiation Policy

The Main AE of ***syngo*.plaza** initiates associations as shown in Table 11.

[1] Each Print job opens a fresh association and the association is closed after the job is done.

Operation or Real-World Activity	Association for
Send Verify	C-ECHO
Send Objects	C-STORE
Provide Commitment	N-EVENT-REPORT
Request Commitment	N-ACTION
Query/Retrieve Objects	C-FIND, C-MOVE
Retrieve Reports	C-FIND (private MITRA SOP class)
Query Worklist	C-FIND
Print Job	N-CREATE, N-GET, N-SET, N-ACTION, N-DELETE

Table 11: Association Initiation Policy – Main AE

2.2.1.3.1 Activity "Send Verify"

2.2.1.3.1.1 Description and Sequencing of Activities

The DICOM communication can be verified with a service utility, which is part of the software delivered with ***syngo*.plaza**. If the process successfully establishes an association to a remote AE, it will send the C-ECHO request via the open association to verify that the remote AE is responding to DICOM messages.

2.2.1.3.1.2 Proposed Presentation Contexts

***syngo*.plaza** will propose Presentation Contexts for DICOM SOP classes as shown in Table 12.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 12: Proposed Presentation Contexts – "Send Verify"

2.2.1.3.1.3 SOP specific Conformance

***syngo*.plaza** conforms to the definition of a Verification SCU in accordance to the DICOM Standard.

2.2.1.3.2 Activity "Send Objects"

2.2.1.3.2.1 Description and Sequencing of Activities

Storage of DICOM objects is either triggered by a C-MOVE request initiated by an external DICOM AE to ***syngo*.plaza**, by the user of the Viewing Station or internally (e.g. autoroute, archiving to DAP). If an association to a remote Application Entity could successfully be established, each image will be transferred one after another. The Send facility is multi threaded and it can have parallel associations to the DICOM Store SCP with each association handling images belonging to one DICOM series. If the C-STORE response from the remote Application contains a status other than SUCCESS, the association is aborted. After a configurable time period, the transfer of the images is started again. The Send jobs will be marked as failed if it is added manually by a user. Otherwise the jobs will be tried indefinitely.

2.2.1.3.2.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts for DICOM Storage SOP classes as shown in Table 97.

The order of Transfer Syntaxes proposed depends on the Transfer Syntax of the images when they were received, on the configuration and on the licensed modules.

2.2.1.3.2.3 SOP specific Conformance

***syngo*.plaza** conforms to the definition of a Storage SCU in accordance to the DICOM Standard.

2.2.1.3.3 Activity "Provide Commitment"

2.2.1.3.3.1 Description and Sequencing of Activities

In case ***syngo*.plaza** has received a Storage Commitment request from an external node and the external node has closed the association, the Main AE of ***syngo*.plaza** initiates a new association in order to send the N-EVENT-REPORT-RQ to the SCU.

Storage Commitment is send only after the images arewere successfully archived. In case the images were sent to a DAP (***syngo*.plaza** acts as a DAU) Storage Commitment is sent after the DAP has sent successful Storage Commitment.

2.2.1.3.3.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 13.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 13: Proposed Presentation Contexts – "Send Commitment"

2.2.1.3.3.3 SOP specific Conformance

***syngo*.plaza** conforms to the definition of a Storage Commitment SCP in accordance to the DICOM Standard.

2.2.1.3.4 Activity "Request Commitment"

2.2.1.3.4.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** acts as a Service Class User for the Storage Commitment Push Model Service Class. It requests commitment for storage of instances previously sent. In this case an association is opened to the Storage Commitment SCP and an N-ACTION-RQ message is sent. It is expected that the commitment (N-EVENT-REPORT) is sent back through a new association.

The following conditions must be true in order to enable ***syngo*.plaza** to send Storage Commitment requests:

- configuration setting "Automatic request for Storage Commitment" enabled
- send destination configured as a Storage Commitment SCP

***syngo*.plaza** requests for a Storage Commitment only, if the instances to be committed have been successfully sent.

As soon as a commitment is requested for a set of instances, these instances will be marked as "For Commitment" in the local database. When the corresponding notification status (N-EVENT-REPORT) is received, these instances will be marked as "Committed" in case of success and "Commitment Failure" in case of failure.

***syngo*.plaza** waits for a configurable time for the commitment notification from the Storage Commitment SCP. If no notification could be received within this duration, the referenced instances are marked as "Not Archived" and the commitment request failed. This timeout is termed as "Event Receipt Timeout" and the default value is 1 day.

2.2.1.3.4.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 13.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 14: Proposed Presentation Contexts – "Request Commitment"

2.2.1.3.4.3 SOP specific Conformance

***syngo*.plaza** conforms to the definition of a Storage Commitment SCU in accordance to the DICOM Standard.

2.2.1.3.5 Activity "Query Objects"

2.2.1.3.5.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** opens an association to a remote node in order to issue C-FIND requests. This is initiated by a user at the Viewing Station.

2.2.1.3.5.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 15.

Presentation Context Table			
Abstract Syntax	**Transfer Syntax**	**Role**	**Ext. Neg.**

Name	UID	Name List	UID List		
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes
Patient Study Only Query/Retrieve Information Model – FIND - Retired	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes

Table 15: Proposed Presentation Contexts – "Query Objects"

The default proposed Transfer Syntax is "Implicit VR Little Endian". The default SOP Class UID is "Patient Root Query/Retrieve Information Model".

2.2.1.3.5.3 SOP specific Conformance

The Main AE of ***syngo*.plaza** proposes Extended Negotiation for all the Query SOP classes. If the Query SCP rejects the Extended Negotiation, ***syngo*.plaza** provides Standard Conformance to the Query SOP classes and uses hierarchical queries with Query/Retrieve Level "Patient", "Study", "Series" or "Image". If the Query SCP accepts Extended Negotiation, ***syngo*.plaza** performs relational queries.

***syngo*.plaza** only supports a single sub-field for the Service-class-application-information field (relational-query support). No support for combined date and time range matching or fuzzy semantic matching of person names is requested.

The Main AE of ***syngo*.plaza** checks for the status codes listed in Table 16 that are contained in the response to the C-FIND request.

Service Status	Meaning	Protocol Codes
Success	Matching is complete	0000
Canceled	Sub-operations terminated due to Cancel Indication	FE00
Pending	Matches are continuing	FF00
Pending	Matches are continuing, no optional key support	FF01
Refused	Out of Resources	A700

Table 16: Status codes for Query C-FIND

The Main AE of ***syngo*.plaza** uses the attributes listed in Table 93, Table 94, Table 95and Table 96 to issue C-FIND requests.

In order to limit the query time, ***syngo*.plaza** displays up to 20 C-FIND response entries by default. A message gives information, if more entries are available. The maximum value for the displayed response entries can be changed by configuration up to 999.

2.2.1.3.6 Activity "Retrieve Objects"

2.2.1.3.6.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** opens an association to a remote node in order to issue C-MOVE requests. This is initiated by a user at the Viewing Station. The user selects one entry from a list generated as a result of the previous C-FIND operation. If ***syngo*.plaza** successfully establishes an association to the remote node, it will trigger the Retrieve SCP via a C-MOVE request to transfer the images to the Main AE in a new association. The transfer of the corresponding images will be done by subsequent C-STORE requests.

2.2.1.3.6.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 17.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1. 4.1.2.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1. 4.1.2.2.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Patient Study Only Query/Retrieve Information Model - MOVE - Retired	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 17: Proposed Presentation Contexts – "Retrieve Objects"

The default proposed Transfer Syntax is "Implicit VR Little Endian".

2.2.1.3.6.3 SOP specific Conformance

The status codes listed in Table 18 are checked in the response to a C-MOVE request.

Service Status	Meaning	Protocol Codes
Success	Matching is complete	0000
Canceled	Sub-operations terminated due to Cancel Indication	FE00
Warning	Sub-operations Complete - One or more failures	B000
Pending	Sub-operations are continuing	FF00

Table 18: Status codes for Retrieve C-MOVE

2.2.1.3.7 Activity "Query Worklist"

2.2.1.3.7.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** opens an association to a remote node in order to issue C-FIND requests. This is initiated by a user at the Viewing Station.

2.2.1.3.7.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 19.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 19: Proposed Presentation Contexts – "Query Worklist"

The default proposed Transfer Syntax is "Implicit VR Little Endian".

2.2.1.3.7.3 SOP specific Conformance

The Main AE of ***syngo*.plaza** sends and reads the attributes listed in Table 20 to the Modality Worklist SCP.

Attribute Name	Attribute Tag	Query Matching Key	Query Return Key
Specific Character Set	(0008,0005)	-	Y
Accession Number	(0008,0050)	Y	Y
Study Date	(0008,0020)	-	Y
Study Time	(0008,0030)	-	Y
Referring Physician's Name	(0008,0090)	Y	Y
Study Description	(0008,1030)	-	Y
Patient's Name	(0010,0010)	Y	Y
Patient's Birth Date	(0010,0030)	Y	Y
Patient ID	(0010,0020)	Y	Y
Patient's Sex	(0010,0040)	Y	Y
Study Instance UID	(0020,000D)	-	Y
Study ID	(0020,0010)	-	Y
Requested Procedure Description	(0031,1060)	-	Y
Scheduled Procedure Step Description	(0040,0007)	-	Y
Scheduled Procedure Step Sequence	(0040,0100)	Y	Y
>Scheduled Station AE Title	(0040,0001)	Y	Y
>Scheduled Procedure Step Start Date	(0040,0002)	Y	Y
>Scheduled Procedure Step Start Time	(0040,0003)	-	Y
>Scheduled Performing Physician's Name	(0040,0006)	-	Y
>Scheduled Procedure Step ID	(0040,0009)	-	Y
>Modality	(0008,0060)	Y	Y
Requested Procedure ID	(0040,1001)	Y	Y

Table 20: Modality Worklist search and return key attributes used in C-FIND request and response

The Main AE of ***syngo*.plaza** checks for the status codes listed in Table 21 that are contained in the response to the C-FIND request.

Service Status	Meaning	Protocol Codes
Success	Matching is complete	0000
Canceled	Sub-operations terminated due to Cancel Indication	FE00
Pending	Matches are continuing	FF00
Pending	Matches are continuing, no optional key support	FF01

Table 21: Status codes for Modality Worklist C-FIND

2.2.1.3.8 Activity "Retrieve Reports"

2.2.1.3.8.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** can request reports via DICOM C-FIND. The private Service Class "MITRA Report Management" is used for this.

2.2.1.3.8.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 22.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
MITRA Report Management	1.2.840.113532.3500.8	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Table 22: Proposed Presentation Contexts – "Retrieve Reports"

2.2.1.3.8.3 SOP Specific Conformance

The issued C-FIND request only contains values for the attributes and

Matching keys for the issued C-FIND-RQ can be a combination of "Patient's Name", "Patient ID", "Study Instance UID", "Accession Number" and "Requested Procedure ID". Other attributes are not requested (i.e. no universal matching). However it is expected that all of the attributes listed in Table 100 are returned. This contrasts to the usual behavior of DICOM query handling but conforms to the description of this SOP class.

***syngo*.plaza** is able to use the "Requested Procedure ID" as matching key even if the SCP only supports it as return key.

2.2.1.3.9 Activity "Print Job"

2.2.1.3.9.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** acts as a Service Class User for the Print Management Services Class.

If the Main AE of ***syngo*.plaza** successfully establishes an association to the remote printer, it will send N-GET, N-CREATE, N-SET, N-ACTION and N-DELETE requests. The status of the printer is monitored by sending N-GET requests on the Printer SOP Class. The statuses of the print jobs are monitored by sending N-GET requests on the Print Job SOP Class.

***syngo*.plaza** is able to send appropriate data to both grayscale and color printers. To have uniform support for true size printing, irrespective of the printer support for true size printing through the Requested Image Size (2020, 0030) attribute, ***syngo*.plaza** stores the printer pixel spacing in configuration files specific for each printer model. It then maps the image pixel spacing to that of the printer, scales the image to its true size, clips the image if necessary to fit to the film sheet and sends this data to the printer.

2.2.1.3.9.2 Proposed Presentation Contexts

The Main AE of ***syngo*.plaza** will propose Presentation Contexts as shown in Table 23.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Table 23: Proposed Presentation Contexts – "Print Job"

The Main AE of ***syngo*.plaza** supports the mandatory SOP Classes as defined by the Basic Grayscale Print Management Meta SOP Class listed in Table 24. ***syngo*.plaza** does not support any optional SOP Classes for Basic Grayscale Print Management Meta SOP Class.

SOP Class Name	SOP Class UID
Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4
Printer SOP Class	1.2.840.10008.5.1.1.16
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23

Table 24: Basic Grayscale Print Management SOP Classes

The Main AE of ***syngo*.plaza** supports the mandatory SOP Classes as defined by the Basic Color Print Management Meta SOP Class listed in Table 25. ***syngo*.plaza** does not support any optional SOP Classes for Basic Color Print Management Meta SOP Class.

SOP Class Name	SOP Class UID
Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1
Printer SOP Class	1.2.840.10008.5.1.1.16

Table 25: Basic Color Print Management SOP Classes

2.2.1.3.9.3 SOP specific Conformance

***syngo*.plaza** conforms to the definition of a Print Management SCU in accordance to the DICOM Standard.

Only one association will be processed at a time. In case of a failure return status of the Print SCP, the current job will be suspended and retried as described in Table 26.

Definition	Registry Entry	Default Value
No. of retries on Print Error	PrintRetryNumber	5
Retry starts after a specified time interval in seconds	PrintRetryTimeDelay	180
Timeout on Printing in seconds	PrintReadMessageTimeout	300

Table 26: Default values for timing demands

Basic Film Session SOP Class

The Basic Film Session information object definition describes all the user defined parameters which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes that are printed on a hardcopy printer.
The Main AE of ***syngo*.plaza** uses the N-CREATE DIMSE service in order to create a Film Session. The attributes listed in Table 27 are supported. After use the Basic Film Session is closed with N-DELETE.

The “Affected SOP Instance UID” received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session. It will also be used for the Basic Film Box N-CREATE message to refer to the created Film Session (see below).

Attribute Name	Attribute Tag	Usage SCU/SCP	Supported Values
Number of Copies	(2000,0010)	U/M	>0
Print Priority	(2000,0020)	U/M	HIGH MED LOW
Medium Type	(2000,0030)	U/M	CLEAR FILM BLUE FILM PAPER
Film Destination	(2000,0040)	U/M	PROCESSOR
Film Session Label	(2000,0050)	U/M	

Table 27: Attributes used to create a Film Session (N-CREATE)

The status codes listed in Table 28 are evaluated by ***syngo*.plaza**.

Service Status	Meaning	Protocol Codes
Success	Film Session successfully created	0000
Warning	Memory allocation not supported	B600

Warning	Attribute Value Out of Range	0116
Warning	Film session printing (collation) is not supported	B601
Warning	Film session SOP Instance hierarchy does not contain Image Box SOP Instance (empty page)	B602
Warning	Image size is larger than image box size, the image has been demagnified.	B604
Failure	Missing attribute value	0121
Failure	Unable to create print job, print queue is full (Film Session)	C601
Failure	Image size is larger than image box size	C603
Failure	Insufficient memory in printer to store the image	C605
Failure	More than one VOI LUT Box contained in image	C606
Failure	No such argument	0114
Failure	Processing Failure	0110
Failure	Unrecognized Operation	0211

Table 28: Status codes for Basic Film Session N-CREATE and N-DELETE

Basic Film Box SOP Class

The Basic Film Box information object definition describes all the user defined parameters of one film of the film session. The Basic Film Box information description defines the presentation parameters which are common for all images on a given sheet of film.

The Main AE of ***syngo*.plaza** uses the N-CREATE DIMSE service in order to create a Film Box. The attributes listed in Table 29 are supported. . The “Affected SOP Instance UID” returned from the creation of the Film Session is used as reference to the Film Session. N-ACTION-RQ is used to start printing.

The N-CREATE-RSP message from the Print SCP includes the “Referenced Image Box Sequence” with SOP Class/Instance UID pairs which will be kept internally to be further used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

Attribute Name	Attribute Tag	Usage SCU/SCP	Supported Values
Image Display Format	(2010,0010)	M/M	STANDARD\1,1 STANDARD\2,1 STANDARD\1,2 STANDARD\2,2 STANDARD\2,3 STANDARD\3,3 STANDARD\3,4 STANDARD\4,4 STANDARD\4,5 STANDARD\5,6 ROW\2,3,3,3 ROW\3,4,4,4,4
Referenced Film Session	(2010,0500)	M/M	

Sequence			
>Referenced SOP Class UID	(0008,1150)	M/M	
>Referenced SOP Instance UID	(0008,1155)	M/M	
Referenced Image Box Sequence	(2010,0510)	-/M	
>Referenced SOP Class UID	(0008,1150)	-/M	
>Referenced SOP Instance UID	(0008,1155)	-/M	
Film Orientation	(2010,0040)	M/M	PORTRAIT, LANDSCAPE
Film Size ID	(2010,0050)	M/M	8INX10IN 8_5INX11IN 10INX12IN 10INX14IN 11INX14IN 11INX17IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM
Magnification Type	(2010,0060)	M/M	REPLICATE BILINEAR CUBIC NONE
Smoothing Type	(2010,0080)	M/M	
Border Density	(2010,0100)	M/M	BLACK WHITE
Empty Image Density	(2010,0110)	M/M	BLACK WHITE
Min Density	(2010,0120)	M/M	>=0
Max Density	(2010,0130)	M/M	>0
Trim	(2010,0140)	M/M	YES NO
Configuration Information	(2010,0150)	M/M	CS000-CS999

Table 29: Attributes used to create a Film Box (N-CREATE)

The status codes listed in Table 30 are evaluated by ***syngo*.plaza**.

Service Status	Meaning	Protocol Codes
Success	Film Box successfully created	0000
Warning	Requested Min Density or Max Density outside of printer's operating range. The printer will use its respective minimum or maximum density value instead.	B605
Warning	Film box does not contain image box (empty page).	B603
Warning	Image size is larger than image box size, the image has been demagnified.	B604

Failure	Invalid attribute value	0106
Failure	Unable to create print job SOP Instance, print queue is full (Film Box)	C602
Failure	Image size is larger than image box size	C603
Failure	Resource limitation	0213
Failed	Unrecognized Operation	0211

Table 30: Status codes for Basic Film Box N-CREATE and N-ACTION

Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information description describes the presentation parameters and image pixel data which apply to a single image of a sheet of film.

The Main AE of ***syngo*.plaza** uses the N-SET DIMSE service in order to set the attributes of an Image Box that was formerly created (N-CREATE response of a Film Box). The attributes listed in Table 31 are supported.

Attribute Name	Attribute Tag	Usage SCU/SCP	Supported Values
Image Position	(2020,0010)	M/M	Dependent on Display Format
Basic Grayscale Image Sequence	(0020,0110)	M/M	
>Sample Per Pixel	(0028,0002)	M/M	1
>Photometric Interpretation	(0028,0004)	M/M	MONOCHROME2
>Rows	(0028,0010)	M/M	Dependant on Printer and Format
>Columns	(0028,0011)	M/M	Dependant on Printer and Format
>Pixel Aspect Ratio	(0028,0034)	M/M	
>Bits Allocated	(0028,0100)	M/M	8[1]
>Bits Stored	(0028,0101)	M/M	8[1]
>High Bit	(0028,0102)	M/M	7[1]
>Pixel Representation	(0028,0103)	M/M	0
>Pixel Data	(7FE0,0010)	M/M	

Table 31: Attributes used to set a Grayscale Image Box (N-SET)

Basic Color Image Box SOP Class

The Basic Color Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information description describes the presentation parameters and image pixel data which apply to a single image of a sheet of film.

[1] The images with a higher resolution (e.g. 12/16-bit images) are converted to 8 Bit by default. It is also possible by configuration to send the images “as they are” to the printer,

The Main AE of ***syngo*.plaza** uses the N-SET DIMSE service in order to set the attributes of an Image Box that was formerly created (N-CREATE response of a Film Box). The attributes listed in Table 32 are supported.

Attribute Name	Attribute Tag	Usage SCU/SCP	Supported Values
Image Position	(2020,0010)	M/M	Dependant on Display Format
Basic Color Image Sequence	(0020,0111)	M/M	
>Sample Per Pixel	(0028,0002)	M/M	3
>Photometric Interpretation	(0028,0004)	M/M	
>Planar Configuration	(0028,0006)	M/M	
>Rows	(0028,0010)	M/M	Dependant on Printer and Format
>Columns	(0028,0011)	M/M	Dependant on Printer and Format
>Pixel Aspect Ratio	(0028,0034)	M/M	
>Bits Allocated	(0028,0100)	M/M	8
>Bits Stored	(0028,0101)	M/M	8
>High Bit	(0028,0102)	M/M	7
>Pixel Representation	(0028,0103)	M/M	0
>Pixel Data	(7FE0,0010)	M/M	

Table 32: Attributes used to set a Color Image Box (N-SET)

Printer SOP Class

The Printer SOP Class provides the possibility to monitor the status of the hardcopy printer in a synchronous way. The Main AE of ***syngo*.plaza** uses the N-GET DIMSE service in order to get the printer status. The attributes listed in Table 33 are supported. All warning and failure messages are written into a log file.

Attribute Name	Attribute Tag	Usage SCU/SCP
Printer Status	(2110,0010)	U/M
Printer Status Info	(2110,0020)	U/M

Table 33: Attributes used to get the printer status (N-GET)

Presentation LUT SOP Class

The objective of the Presentation LUT is to realize image hardcopy printing tailored for specific modalities, applications and user preferences. The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

The Main AE of ***syngo*.plaza** uses the N-CREATE DIMSE service in order to set a Presentation LUT. The attributes listed in Table 34 are supported. It also uses the N-DELETE DIMSE service to delete the Presentation LUT.

Attribute Name	Attribute Tag	Usage SCU/SCP	Supported Values

Presentation LUT Shape	(2050,0020)	U/M	IDENTITY

Table 34: Attributes used to set a Presentation LUT (N-CREATE)

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and is used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ).

2.2.1.4 Association Acceptance Policy

The Main AE of ***syngo*.plaza** attempts to accept a new association for service operations listed in Table 35.

Operation or Real-World Activity	Association for
Receive Verify	C-ECHO
Receive Objects	C-STORE
Provide Commitment	N-ACTION
Request Commitment	N-EVENT-REPORT
Receive Query/Retrieve	C-FIND, C-MOVE

Table 35: Association Acceptance Policy – Main AE

2.2.1.4.1 Activity "Receive Verify"

2.2.1.4.1.1 Description and Sequencing of Activities

The ***syngo*.plaza** receiving process will accept an association and respond to C-ECHO request for DICOM communication verification.

2.2.1.4.1.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts as specified in Table 36.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 36: Accepted Presentation Contexts – "Receive Verify"

2.2.1.4.1.3 SOP-specific Conformance

The Main AE of ***syngo*.plaza** provides standard conformance to the DICOM Verification Service Class as SCP.

2.2.1.4.2 Activity "Receive Objects"

2.2.1.4.2.1 Description and Sequencing of Activities

The ***syngo*.plaza** receiving process will accept an association, receive any images transmitted on that association and store the images on disk. It will store some header attributes in the database in order to allow clients to query these attributes.

Images are stored into the ***syngo*.plaza** database as soon as they are received. After an image is stored into the database, ***syngo*.plaza** sends a successful C-STORE response back to the sender.

This process repeats until

- the association is closed by the sender or
- the storage fails due to some reason (in this case ***syngo*.plaza** sends a failure response and aborts the association) or
- the association is lost (because of timeouts, network unexpectedly shutdown, ...).

2.2.1.4.2.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts for DICOM Storage SOP classes as shown in Table 97.

2.2.1.4.2.3 SOP-specific Conformance

The Main AE of ***syngo*.plaza** conforms to the Full Storage Class at Level 2.

2.2.1.4.2.4 Other SOP specific behavior

***syngo*.plaza** is incorporating the actor “Image Manager/Archive” within the IHE Profile “Patient Information and Reconciliation” (PIR). Therefore patient and study information might be updated after successful storage based on IHE Use Case scenarios. For further information please refer to IHE [2].

***syngo*.plaza** validates incoming DICOM objects and rejects them in the following cases:

- DICOM attribute of type 1 is not present or contains an empty value
- DICOM attribute of type 2 is not present (exception: patient attributes - see below)
- Value Representation of DICOM attribute is not correct.

There are some additional rejection criteria for patient level attributes. The checks vary slightly for different Patient Identifier configurations:

Patient Identifier configurations is "Patient Name + Patient ID"

***syngo*.plaza** will not allow the storage of DICOM objects, if

- Patient ID (0010, 0020) is missing or empty
- Patient Name (0010, 0010) is missing or empty
- there is a conflict in the hierarchy (e.g. same SOP Instance UID is sent again as registered before, but contains different information for Patient ID (0010, 0020) or Patient Name (0010, 0010))

Patient Identifier configurations is "Patient ID Only"

***syngo*.plaza** will not allow the storage of DICOM objects, if

- Patient ID (0010, 0020) attribute is missing or empty
- there is a conflict in the hierarchy (e.g. same SOP Instance UID is sent again as registered before, but contains different information for Patient ID (0010, 0020))

Note: In case the DICOM attributes for Patient’s Birth Date (0010, 0030) and Patient’s Sex (0010, 0040) are missing these are created on the fly in the DICOM header. Hence they are not considered for the validation as listed above.

2.2.1.4.3 Activity "Request Commitment"

2.2.1.4.3.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** acts as a Service Class User (SCU) for the Storage Commitment Push Model Service Class (it requests commitment to previously stored instances). It attempts to accept an association for N-EVENT-RP requests.

2.2.1.4.3.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts as shown in Table 37.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 37: Accepted Presentation Contexts – "Request Commitment"

2.2.1.4.3.3 SOP-Specific Conformance

***syngo*.plaza** conforms to the definition of a Storage Commitment SCP in accordance to the DICOM Standard.

2.2.1.4.4 Activity "Provide Commitment"

2.2.1.4.4.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** acts as a Service Class Provider (SCP) for the Storage Commitment Push Model Service Class (it gives commitment to previously received and archived instances). It attempts to accept an association for N-ACTION requests.

For further description of the handling please refer to chapter 2.2.1.3.3.

2.2.1.4.4.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts as shown in Table 38.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 38: Accepted Presentation Contexts – "Provide Commitment"

2.2.1.4.4.3 SOP-Specific Conformance

***syngo*.plaza** conforms to the definition of a Storage Commitment SCP in accordance to the DICOM Standard.

2.2.1.4.5 Activity "Receive Query"

2.2.1.4.5.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** responds to requests issued by an SCU with the query model Patient Root, Study Root and Patient/Study Only. Hierarchical and relational retrieve operations are both supported. With a C-FIND-CANCEL request the running query can be canceled at any time by the Query SCU.

2.2.1.4.5.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts as shown in Table 39.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	Yes
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	Yes
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Information Mode l- FIND - Retired	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	Yes
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 39: Accepted Presentation Contexts – "Receive Query"

2.2.1.4.5.3 SOP Specific Conformance

The query matching is case insensitive.

For relational and hierarchical queries at series level or below no result matches will be returned for MCM data that was not de-archived yet, since this information is unavailable at the archive.

***syngo*.plaza** only supports a single sub-field of the Service-class-application-information field (relational-query support). No support for combined date and time range matching and fuzzy semantic matching of person names is provided.

2.2.1.4.5.4 Hierarchical and Relational Queries

Relational queries are supported. The fields supported for relational queries are “Study Date” on study level and “Modality”, “Body Part Examined”, “Series Description”, “Exam Status” and “Rebuild Status” on series level.

Patient Root Q/R Information Model

The attributes listed in Table 93 are supported for the Patient Root Q/R Information Model on patient level.

The attributes listed in Table 94 are supported for the Patient Root Q/R Information Model on study level.

The attributes listed in Table 95 are supported for the Patient Root Q/R Information Model on series level.

The attributes listed in Table 96 are supported for the Patient Root Q/R Information Model on image level.

Study Root Q/R Information Model

The attributes listed in Table 93 and Table 94 are supported for the Study Root Q/R Information Model on study level.

The same Series level attributes as in listed in Table 95 are supported.
The same Image level attributes as listed in Table 96 are supported.

Patient/Study Only Q/R Information Model

The same Patient level attributes as in listed in Table 93 are supported.
The same Study level attributes as listed in Table 94 are supported.

2.2.1.4.5.5 Return Codes

The status codes listed in Table 40 may be returned in C-FIND responses.

Service Status	Meaning	Protocol Codes
Success	Matching is complete - No final Identifier is supplied	0000
Cancel	Matching terminated due to a Cancel request	FE00
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00
Failed	Invalid Parameters	A900
Refused	Out of Resources	A700

Table 40: C-FIND SCP Return Status Codes

2.2.1.4.6 Activity “Receive Retrieve”

2.2.1.4.6.1 Description and Sequencing of Activities

The Main AE of ***syngo*.plaza** responds to retrieve requests of an SCU. It supports the query models "Patient Root", "Study Root" and "Patient/Study Only". After accepting an association from a remote DICOM AE, the Main AE receives the move request via the open association and queries the database. The requested images are sent to the requested remote node.

2.2.1.4.6.2 Accepted Presentation Contexts

The Main AE of ***syngo*.plaza** will accept Presentation Contexts as shown in Table 41.

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes
Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes
Patient/Study Only Query/Retrieve Model – MOVE - Retired	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes

Table 41: Accepted Presentation Contexts – "Receive Retrieve"

2.2.1.4.6.3 SOP Specific Conformance

The Main AE of ***syngo*.plaza** returns the status codes listed in Table 42.

Service Status	Meaning	Protocol Codes
Success	Sub-operations Complete - No Failures or Warning	0000
Cancel	Sub-operations terminated due to Cancel Indication	FE00
Pending	Sub-operations are continuing	FF00
Refused	Move Destination unknown	A801
Failed	Invalid parameters	A900
Failed	Unable to process	C001

Table 42: C-MOVE Return Status

2.2.2 Query Spanning AE

The Query Spanning AE of ***syngo*.plaza** will listen for C-FIND requests. Whenever it gets a request, it will send the same C-FIND request to a set of configured Query SCPs in separate associations. Once it gets the results from these SCPs, it forwards them as pending C-FIND response messages to the Query SCU. Each response will also contain the attribute "Retrieve AET" (0008,0054) in the query result, which indicates the AET of the remote query SCP node the result was received from. The results are not merged (e.g. if different SCPs provide the same information or contradictory information this will be forwarded).

Whatever Information Model is used by the Query SCU will also be used for the associations to the Query SCPs.

If the query to a Query SCP fails, the next node in chain will be queried until all configured Query SCPs were processed. When a query is in progress and the Query SCU sends a C-CANCEL request,

then the same request will be sent to all Query SCPs. The query results from different nodes will not be merged. The Query Spanning AE will just get the results from various Query SCPs and forward them to the Query SCU.

The Query Spanning AE role is limited to only querying. Once the Query SCU gets the query results and the user requests for a retrieve, the Retrieve SCU will send a C-MOVE-RQ directly to the Retrieve SCP (defined by “Retrieve AET”) instead of sending it through the Query Spanning AE.

2.2.2.1 SOP Classes

The Query Spanning AE provides Standard Conformance to the SOP Classes listed in Table 88.

2.2.2.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
Max PDU size	64512
Maximum number of simultaneous associations as an association acceptor	10
Maximum number of simultaneous associations as an association initiator	configurable

Table 43: Association policies for Query Spanning AE

2.2.2.2.1 Asynchronous Nature

The Query Spanning AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.2.2.2 Implementation Identifying Information

The Query Spanning AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 44: Implementation Identifying Information

2.2.2.3 Association Initiation Policy

The Query Spanning AE of ***syngo*.plaza** initiates associations as shown in Table 45.

Operation or Real-World Activity	Association for
Forward Query	C-FIND

Table 45: Association Initiation Policy – Query Spanning AE

2.2.2.3.1 Activity “Forward Query”

2.2.2.3.1.1 Description and Sequencing of Activities

Please refer to chapter 2.2.2.

2.2.2.3.1.2 Proposed Presentation Contexts

***syngo*.plaza** will propose Presentation Contexts for DICOM SOP classes as shown in Table 46.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes
Patient Study Only Query/Retrieve Information Model – FIND - Retired	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	Yes

Table 46: Proposed Presentation Contexts – Forward Query

2.2.2.3.1.3 SOP specific Conformance

If the destination node is not reachable or an error is returned, ***syngo*.plaza** will not try to send the message again.

2.2.2.4 Association Acceptance Policy

The Query Spanning AE of ***syngo*.plaza** accepts associations as shown in Table 59.

Operation or Real-World Activity	Association for
Provide Query	C-FIND

Table 47: Association Acceptance Policy – Query Spanning AE

2.2.2.4.1 Activity "Provide Query"

2.2.2.4.1.1 Description and Sequencing of Activities

Please refer to chapter 2.2.2.

2.2.2.4.1.2 Accepted Presentation Contexts

The Query Spanning AE of ***syngo*.plaza** will accepts Presentation Contexts for DICOM SOP classes as shown in Table 48.

Presentation Context Table

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	**UID**	**Name List**	**UID List**		
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes
Patient Study Only Query/Retrieve Information Model - FIND - Retired	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	Yes

Table 48: Accepted Presentation Contexts – Provide Query

2.2.2.4.1.3 SOP-specific Conformance Statement

The Query Spanning AE of ***syngo*.plaza** will add the attribute “Retrieve AET” (0008,0054) to each of the C-FIND responses. The “Retrieve AET” indicates the remote node that returned the corresponding C-FIND response.

2.2.3 Retrieve Spanning AE

The Retrieve Spanning AE of ***syngo*.plaza** will listen for C-MOVE requests. Whenever it gets a request, it will send the same C-MOVE request to a set of configured Retrieve SCPs in separate associations.

Whatever Information Model is used by the Retrieve SCU will also be used for the associations to the Retrieve SCPs.

If the request to a Retrieve SCP fails, the C-MOVE request will be sent to the next node in chain until all configured Retrieve SCPs were processed. When a retrieve job is in progress and the Retrieve SCU sends a C-CANCEL request, then the same request will be sent to all Retrieve SCPs.

2.2.3.1 SOP Classes

The Retrieve Spanning AE provides Standard Conformance to the SOP Classes listed in Table 89.

2.2.3.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
Max PDU size	64512
Maximum number of simultaneous associations as an association acceptor	1
Maximum number of simultaneous associations as an association initiator	configurable

Table 49: Association policies for Retrieve Spanning AE

2.2.3.2.1 Asynchronous Nature

The Retrieve Spanning AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.3.2.2 Implementation Identifying Information

The Retrieve Spanning AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 50: Implementation Identifying Information

2.2.3.3 Association Initiation Policy

The Retrieve Spanning AE of ***syngo*.plaza** initiates associations as shown in Table 51.

Operation or Real-World Activity	Association for
Forward Retrieve	C-MOVE

Table 51: Association Initiation Policy – Retrieve Spanning AE

2.2.3.3.1 Activity "Forward Retrieve"

2.2.3.3.1.1 Description and Sequencing of Activities

Please refer to chapter 2.2.3.

2.2.3.3.1.2 Proposed Presentation Contexts

***syngo*.plaza** will propose Presentation Contexts for DICOM SOP classes as shown in Table 52.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4 .1.2.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4 .1.2.2.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Patient Study Only Query/Retrieve Information Model - MOVE - Retired	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 52: Proposed Presentation Contexts – Forward Retrieve

2.2.3.3.1.3 SOP specific Conformance

If the destination node is not reachable or an error is returned, ***syngo*.plaza** will not try to send the message again.

2.2.3.4 Association Acceptance Policy

The Retrieve Spanning AE of ***syngo*.plaza** accepts associations as shown in Table 53.

Operation or Real-World Activity	Association for
Provide Retrieve	C-MOVE

Table 53: Association Acceptance Policy – Retrieve Spanning AE

2.2.3.4.1 Activity "Provide Retrieve"

2.2.3.4.1.1 Description and Sequencing of Activities

Please refer to chapter 2.2.3.

2.2.3.4.1.2 Accepted Presentation Contexts

The Retrieve Spanning AE of ***syngo*.plaza** will accepts Presentation Contexts for DICOM SOP classes as shown in Table 54.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4 .1.2.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4 .1.2.2.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None
Patient Study Only Query/Retrieve Information Model - MOVE - Retired	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 54: Accepted Presentation Contexts – Provide Retrieve

2.2.3.4.1.3 SOP-specific Conformance Statement

N.a.

2.2.4 MPPS Manager AE

2.2.4.1 SOP Classes

The MPPS Manager AE provides Standard Conformance to the SOP Classes listed in Table 90.

2.2.4.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
Max PDU size	64512
Maximum number of simultaneous associations as an association acceptor	No maximum defined
Maximum number of simultaneous associations as an association initiator	No maximum defined

Table 55: Association policies for MPPS Manager AE

2.2.4.2.1 Asynchronous Nature

The MPPS Manager AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.4.2.2 Implementation Identifying Information

The MPPS Manager AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 56: Implementation Identifying Information

2.2.4.3 Association Initiation Policy

The MPPS Manager AE of ***syngo*.plaza** initiates associations as shown in Table 57.

Operation or Real-World Activity	Association for
Forward MPPS	N-SET, N-CREATE

Table 57: Association Initiation Policy – MPPS Manager AE

2.2.4.3.1 Activity "Forward MPPS"

2.2.4.3.1.1 Description and Sequencing of Activities

***syngo*.plaza** is able to receive Modality Performed Procedure Step messages from modalities. These MPPS messages can be forwarded to a further remote node; in this case ***syngo*.plaza** directly opens an association to the node and transmits the MPPS message unchanged. The forwarding of the MPPS messages is a requirement for the PPS Manager specified by IHE [2].

2.2.4.3.1.2 Proposed Presentation Contexts

The MPPS Manager AE of ***syngo*.plaza** will propose Presentation Contexts for DICOM SOP classes as shown in Table 12.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

Table 58: Proposed Presentation Contexts – Forward MPPS

2.2.4.3.1.3 SOP specific Conformance

All attributes received by ***syngo*.plaza** will be sent without any changes, interpretation or validation.

If the destination node is not reachable or an error is returned, ***syngo*.plaza** will not try to send the message again.

2.2.4.4 Association Acceptance Policy

The MPPS Manager AE of ***syngo*.plaza** accepts associations as shown in Table 59.

Operation or Real-World Activity	Association for
Receive MPPS	N-CREATE, N-SET

Table 59: Association Acceptance Policy – MPPS Manager AE

2.2.4.4.1 Activity "Receive MPPS"

2.2.4.4.1.1 Description and Sequencing of Activities

The modality can send Modality Performed Procedure Steps to the MPPS Manager AE of ***syngo*.plaza**. Multiple N-CREATE, N-SET requests over the same association are supported.

2.2.4.4.1.2 Accepted Presentation Contexts

The MPPS Manager AE of ***syngo*.plaza** will accepts Presentation Contexts for DICOM SOP classes as shown in Table 60.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 60: Accepted Presentation Contexts – "Receive MPPS"

2.2.4.4.1.3 SOP-specific Conformance Statement

The MPPS messages are simply forwarded to the destination node. There are no checks on the validity of the attributes on the incoming messages.

2.2.5 Modality Worklist Provider AE

***syngo*.plaza** provides a Modality Worklist Scheduler with basic Patient Administration functions as an option. In order to give modalities access to this scheduling information the Modality Worklist Provider AE acts as an SCP for the DICOM Modality Worklist service class.

2.2.5.1 SOP Classes

This Application Entity provides Standard Conformance to the SOP Classes listed in Table 91.

2.2.5.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
PDU size	64512
Maximum number of simultaneous associations as an association acceptor	20[1]

Table 61: Association policies for Modality Worklist Provider AE

2.2.5.2.1 Asynchronous Nature

The Modality Worklist Provider AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.5.2.2 Implementation Identifying Information

The Modality Worklist Provider AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 62: Implementation Identifying Information

2.2.5.3 Association Initiation Policy

The Modality Worklist Provider AE of ***syngo*.plaza** does not initiate associations to remote nodes.

2.2.5.4 Association Acceptance Policy

The Modality Worklist Provider AE of ***syngo*.plaza** accepts new associations for DIMSE C-FIND service operations.

[1] default, configurable

2.2.5.4.1 Activity "Provide Modality Worklist"

2.2.5.4.1.1 Description and Sequencing of Activities

After accepting an association from a remote DICOM node, the Modality Worklist Provider AE of ***syngo*.plaza** receives the Worklist C-FIND requests via the open association and queries the database. For each match a response is sent to the requesting node.

2.2.5.4.1.2 Accepted Presentation Contexts

The Modality Worklist Provider AE of ***syngo*.plaza** will accept Presentation Contexts as shown in Table 63.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 63: Accepted Presentation Contexts – "Provide Modality Worklist"

2.2.5.4.1.3 SOP Specific Conformance

The Modality Worklist Provider AE of ***syngo*.plaza** supports the query matching and return key attributes listed in Table 64.

Attribute Name	Attribute Tag	Query Matching Key	Query Return Key
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)		Y
>Scheduled Station AE Title	(0040,0001)	Y	Y
>Scheduled Procedure Step Start Date	(0040,0002)	Y	Y
>Scheduled Procedure Step Start Time	(0040,0003)		Y
>Modality	(0008,0060)	Y	Y
>Scheduled Performing Physician's Name	(0040,0006)	Y	Y
>Scheduled Procedure Step ID	(0040,0009)		Y
>Scheduled Procedure Step Description	(0040,0007)		Y
>Scheduled Station Name	(0040,0010)		Y (always blank)
>Scheduled Procedure Step Status	(0040,0020)		Y
>Scheduled Procedure Step Location	(0040,0011)		Y
Requested Procedure			
Requested Procedure ID	(0040,1001)	Y	Y
Study Instance UID	(0020,000D)		Y
Requested Procedure Comments	(0040,1400)		Y
Requested Procedure Description	(0032,1060)		Y
Names of Intended Recipients of Results	(0040,1010)		Y
Imaging Service Request			
Accession Number	(0008,0050)	Y	Y
Referring Physician's Name	(0008,0090)		Y
Requesting Physician	(0032,1032)		Y
Imaging Service Request Comments	(0040,2400)		Y
Visit Identification			

Admission ID	(0038,0100)		Y
Visit Status			
Current Patient Location	(0038,0300)		Y
Patient Identification			
Patient's Name	(0010,0010)	Y	Y
Patient ID	(0010,0020)	Y	Y
Patient Demographic			
Patient's Birth Date	(0010,0030)		Y
Patient's Sex	(0010,0040)		Y
Confidentiality Constraint on Patient Data	(0040,3001)		Y
Ethnic Group	(0010,2160)		Y
Patient Comment	(0010,4000)		Y
Patient Medical			
Patient State	(0038,0500)		Y
Pregnancy Status	(0010,21C0)		Y
Medical Alerts	(0010,2000)		Y
Additional Patient History	(0010,21B0)		Y
Contrast Allergies	(0010,2110)		Y
Patient Weight	(0010,1030)		Y
Special Needs	(0038,0050)		Y

Table 64: Query matching and return key attributes for Modality Worklist Provider AE

2.2.6 Temp AE

2.2.6.1 SOP Classes

The Temp AE provides Standard Conformance to the SOP Classes listed in Table 86 and Table 87 as SCP.

2.2.6.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
Max PDU size	64512
Maximum number of simultaneous associations as an association acceptor	20[1]

Table 65: Association policies for Temp AE

2.2.6.2.1 Asynchronous Nature

The Temp AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.6.2.2 Implementation Identifying Information

The Temp AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2

[1] default, configurable

Implementation Version Name	SHC_PLAZA_VB10A

Table 66: Implementation Identifying Information

2.2.6.3 Association Initiation Policy

The Temp AE of ***syngo*.plaza** does not initiate any DICOM associations.

2.2.6.4 Association Acceptance Policy

The Temp AE of ***syngo*.plaza** accepts associations as shown in Table 67.

Operation or Real-World Activity	Association for
Receive Objects	C-STORE

Table 67: Association Acceptance Policy – Temp AE

2.2.6.4.1 Activity "Receive Objects"

2.2.6.4.1.1 Description and Sequencing of Activities

The Temp AE of ***syngo*.plaza** is used in case ***syngo*.plaza** acts as a DIOCM Archive User (DAU). It will receive the Composite Image Objects from the DICOM Archive Provider (DAP) after ***syngo*.plaza** has submitted a C-MOVE request with the Temp AE as the destination. This is internally done in case ***syngo*.plaza** needs to de-archive DICOM objects from DAP.

2.2.6.4.1.2 Accepted Presentation Contexts

The Temp AE of ***syngo*.plaza** will accept Presentation Contexts for DICOM Storage SOP classes as shown in Table 97.

2.2.6.4.1.3 SOP-specific Conformance Statement

The Temp AE of ***syngo*.plaza** conforms to the Full Storage Class at Level 2.

2.2.7 MPPS ImageManager AE

2.2.7.1 SOP Classes

The MPPS ImageManager AE of ***syngo*.plaza** provides Standard Conformance to the SOP Classes listed in Table 92.

2.2.7.2 Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
Max PDU size	64512
Maximum number of simultaneous associations as an association acceptor	20[1]

Table 68: Association policies for MPPS ImageManager AE

[1] default, configurable

2.2.7.2.1 Asynchronous Nature

The MPPS ImageManager AE of ***syngo*.plaza** does not support asynchronous communication (multiple outstanding transactions over a single association).

2.2.7.2.2 Implementation Identifying Information

The MPPS ImageManager AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name:

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 69: Implementation Identifying Information

2.2.7.3 Association Initiation Policy

The MPPS ImageManager AE of ***syngo*.plaza** does not initiate any associations to remote nodes.

2.2.7.4 Association Acceptance Policy

The MPPS ImageManager AE of ***syngo*.plaza** accepts associations as shown in Table 70.

Operation or Real-World Activity	Association for
Receive MPPS	N-CREATE, N-SET

Table 70: Association Acceptance Policy – MPPS ImageManager AE

2.2.7.4.1 Activity "Receive MPPS"

2.2.7.4.1.1 Description and Sequencing of Activities

The modality can send Modality Performed Procedure Steps to the MPPS ImageManager AE of ***syngo*.plaza**. Multiple N-CREATE, N-SET requests over the same association are supported. The attributes of the MPPS messages listed in Table 72 are displayed to the user for informational purpose.

2.2.7.4.1.2 Accepted Presentation Contexts

The MPPS ImageManager AE of ***syngo*.plaza** will accepts Presentation Contexts for DICOM SOP classes as shown in Table 71.

Presentation Context Table					
Abstract Syntax		**Transfer Syntax**		**Role**	**Ext. Neg.**
Name	**UID**	**Name List**	**UID List**		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCP	None

Table 71: Accepted Presentation Contexts – Receive MPPS

2.2.7.4.1.3 SOP-specific Conformance Statement

Table 72 describes the supported attributes from N-CREATE and N-SET requests, which are stored in a history queue and displayed to the user.

Attribute Name	Attribute Tag	Value N-CREATE	Value N-SET
Performed Procedure Step Relationship			
Scheduled Step Attribute Sequence	(0040,0270)		-
>Study Instance UID	(0020,000D)		-
>Referenced Study Sequence	(0008,1110)		-
>>Referenced SOP Class UID	(0008,1150)		-
>>Referenced SOP Instance UID	(0008,1155)		-
>Accession Number	(0008,0050)		-
>Requested Procedure ID	(0040,1001)		-
>Requested Procedure Description	(0032,1060)		-
>Scheduled Procedure Step ID	(0040,0009)		-
>Scheduled Procedure Step Description	(0040,0007)		-
>Scheduled Action Item Sequence	(0040,0008)		-
>>Code Value	(0008,0100)		-
>>Coding Scheme Designator	(0008,0102)		-
>>Coding Scheme Version	(0008,0103)		-
>>Code Meaning	(0008,0104)		-
Patient's Name	(0010,0010)		-
Patient ID	(0010,0020)		-
Patient's Birth Date	(0010,0030)		-
Patient's Sex	(0010,0040)		-
Performed Procedure Step Informations			
Performed Station AE Title	(0040,0241)		-
Performed Station Name	(0040,0242)		-
Performed Location	(0040,0243)		-
Performed Procedure Step Start Date	(0040,0244)		-
Performed Procedure Step Start Time	(0040,0245)		-
Performed Procedure Step Status	(0040,0252)	"IN PROGRESS"	"COMPLETED" or "DISCONTINUED"
Performed Procedure Step ID	(0040,0253)		
Performed Procedure Step Description	(0040,0254)		
Performed Procedure Type Description	(0040,0255)		
Procedure Code Sequence	(0008,1032)		
>Code Value	(0008,0100)		
>Coding Scheme Designator	(0008,0102)		
>Coding Scheme Version	(0008,0103)		
>Code Meaning	(0008,0104)		
Performed Procedure Step End Date	(0040,0250)		
Performed Procedure Step End Time	(0040,0251)		
Image Acquisition Results			
Modality	(0008,0060)		
Study ID	(0020,0010)		
Performed Action Item Code Sequence	(0040,0260)		
>Code Value	(0008,0100)		
>Coding Scheme Designator	(0008,0102)		
>Coding Scheme Version	(0008,0103)		

>Code Meaning	(0008,0104)		
Performed Series Sequence	(0040,0340)		
>Performing Physician's Name	(0008,1050)		
>Operators Name	(0008,1070)		
>Series Instance UID	(0020,000E)		
>Series Description	(0008,103E)		
>Retrieve AE Title	(0008,0054)		
>Referenced Image Sequence	(0008,1140)		
>>Referenced SOP Class UID	(0008,1150)		
>>Referenced SOP Instance UID	(0008,1155)		
>Referenced Standalone SOP Instance Sequence	(0040,0220)		

Table 72: Performed Procedure Step N-CREATE Attributes

The MPPS ImageManager AE expects a complete set of attributes in the N-SET request message. If an attribute is missing or filled with a different value, the old values will be overwritten.

2.2.7.4.1.4 Return Codes

The return codes the MPPS ImageManager AE sends back to the MPPS SCU are listed in Table 73.

Service Status	Status Code	Meaning	Related Fields
Processing failure	0x0110	Application processing failure MPPS already completed	(0000,0902) (0000,0903) = 0xA710
Duplicate SOP instance	0x0111	The optional field contains the SOP Instance UID which was already allocated to another SOP Instance	(0000,1000)
Missing attribute	0x0120		Attribute List
Invalid attribute value	0x0106		Attribute List
Missing attribute value	0x0121		Attribute List
Success	0x0000	Matching is complete - No final Identifier is supplied	None

Table 73: N-CREATE / N-SET return codes for MPPS ImageManager AE

2.3 Network Interfaces

2.3.1 Physical Network Interface

***syngo*.plaza** is independent to the physical medium over which TCP/IP executes; it inherits this from the OS system upon which it executes.

Currently only IPv4 networks are supported (no support for IPv6).

2.4 Configuration

2.4.1 AE Title / Presentation Address Mapping

***syngo*.plaza** maps Application Entity Titles to host name and port number via an internal configuration method. The IP address for the host name is determined using standard system calls.

The AE Titles, hostnames and port numbers can be changed with the configuration.

2.4.2 Configurable parameters

The following parameters for time-outs can be configured in the ***syngo*.plaza** application.

- time-out for accepting/rejecting an association request: 300 sec
- time-out for responding to an association open/close request: 300 sec
- time-out for accepting a message over the network: 300 sec
- Query timeout : 300 sec
- Retrieve timeout : 300 sec
- Send Retry Interval : 180 sec

Further configuration possibilities:

- Number of max. accepted Query Matches
- automatic request for Storage Commitment

3 Media Interchange

3.1 Implementation Models

3.1.1 Application Data Flow

3.1.1.1 Media Handling AE

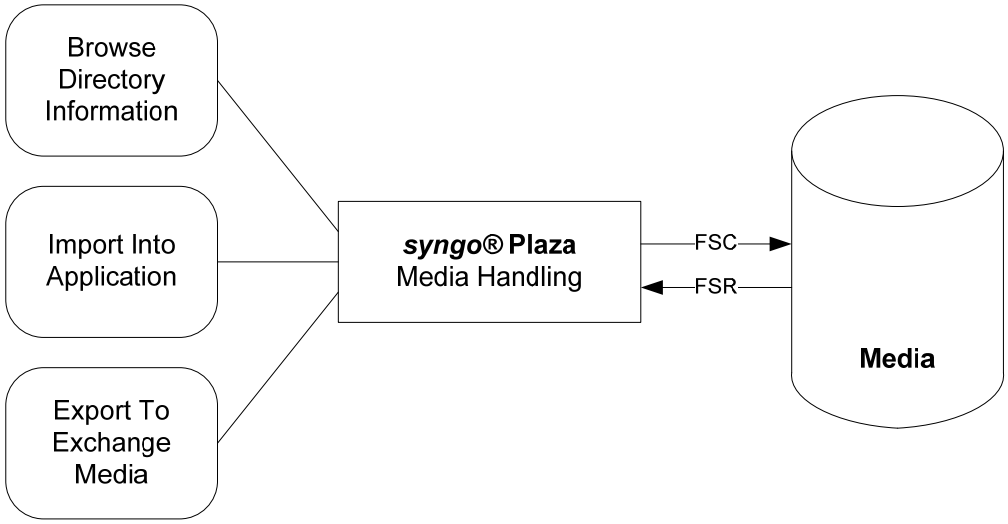

Figure 8: Application Data Flow Diagram – Media Handling AE

The Media Handling AE of ***syngo*.plaza** will serve as an interface to the CD-R, DVD-R and DVD-RAM medium device (see Table 8 for supported media services). It serves interfaces to include the off-line media directory into the browser and to copy SOP instances to a medium or retrieve SOP Instances from medium into local storage.

3.1.2 Functional Definitions of AEs

3.1.2.1 Media Handling AE

The Media Handling AE of ***syngo*.plaza** is capable of

- creating a new File-set onto an unwritten medium,
- copying SOP Instances from the medium onto local storage and loading them into viewer and
- reading the File-set's DICOMDIR information temporarily into database and pass it to display applications.

3.1.3 Sequencing of Real-World Activities

The Media Handling AE of ***syngo*.plaza** will not perform updates before the Directory information of the DICOMDIR is completely read.

3.1.4 File Meta Information for Implementation Class and Version

The Media Handling AE of ***syngo*.plaza** provides a single Implementation Class UID and Version Name as listed in Table 74.

Implementation Class UID	1.3.12.2.1107.5.8.2
Implementation Version Name	SHC_PLAZA_VB10A

Table 74: Implementation Identifying Information

3.2 AE Specifications

3.2.1 Media Handling AE

The Media Handling AE of ***syngo*.plaza** provides standard conformance to Media Storage Service Class. Please refer to Table 8 for a listing of the supported DICOM Media services.

3.2.1.1 Real World Activities

3.2.1.1.1 Activity “Browse Directory Information”

The Media Handling AE of ***syngo*.plaza** acts as an FSR using the interchange option when requested to read the media directory.

The Media Handling AE of ***syngo*.plaza** will read the DICOMDIR and insert that directory entries, which are supported, into a local database. The database can then be used for browsing media contents.

3.2.1.1.1.1 Media Storage Application Profiles

Please refer to Table 8 and Table 86 for the supported DICOM Media services and SOP classes.

3.2.1.1.2 Activity “Import Into Application”

The Media Handling AE of ***syngo*.plaza** acts as an FSR using the interchange option when requested to read SOP Instances from the medium into the local storage or the viewer. The SOP Instance selected from the media directory will be copied into the local storage or loaded into the viewer. Only SOP Instances that are supported can be retrieved from media storage.

The Media import works as specified for “Media Importer” actor defined in IHE [2] under the PDI profile.

3.2.1.1.2.1 Media Storage Application Profiles

Please refer to Table 8 and Table 86 for the supported DICOM Media services and SOP classes.

3.2.1.1.3 Activity “Export To Exchange Media”

The Media Handling AE of ***syngo*.plaza** acts as an FSC for uninitialized media. It is using the interchange option when requested to copy SOP Instances from the local storage to an exchange medium.

The Media Handling AE of ***syngo*.plaza** will receive a list of SOP Instances to be copied to the exchange medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the SOP Instances are either updated or created on the media. Only valid SOP Instances are accepted.

***syngo*.plaza** needs an external media burning software to write the exported folder contents to the target media.

3.2.1.1.3.1 Media Storage Application Profiles

Please refer to Table 8 and Table 86 for the supported DICOM Media services and SOP classes. The files are exported in the Transfer Syntax of the STS. In case of IHE PDI [2] compliant media, images are uncompressed before they are exported.

3.3 Augmented and Private Profiles

3.3.1 Augmented Application Profiles

N.a.

3.3.2 Private Application Profiles

3.3.2.1 Class and Profile Identification

This section defines an Application Profile Class for the Media Handling AE of ***syngo*.plaza**. The identifier for this class shall be PRI-PLAZA. This class is intended to be used for interchange of extended and private Information Objects via CD-R, DVD and DVD-RAM.

The specific application profiles in this class are shown in Table 75.

Application Profile	Identifier	Description
CD-R Interchange of standard & private SOP Classes with Compression	PRI-PLAZA-CD	Handles interchange of Composite SOP Instances and privately defined SOP instances(Siemens CSA NonImage IOD)
DVD Interchange of standard & private SOP Classes with Compression	PRI-PLAZA-DVD	Handles interchange of Composite SOP Instances and privately defined SOP instances(Siemens CSA NonImage IOD)
DVD-RAM Interchange of standard & private SOP Classes with Compression	PRI-PLAZA-DVD-RAM	Handles interchange of Composite SOP Instances and privately defined SOP instances(Siemens CSA NonImage IOD)

Table 75: PRI-PLAZA Application Profiles

Equipment claiming conformance for this Application Profile Class shall make a clear statement on handling of the private defined SOP Instances.

3.3.2.2 Clinical Context

This application profile facilitates the interchange of original acquired and derived images and private data related to them. Typical media interchange would be from export of ***syngo*.plaza** to dedicated systems capable of handling the private data objects.

3.3.2.2.1 Roles and Service Class Options

These Application Profiles use the Media Storage Service Class defined in PS 3.4 of [1] with the Interchange Option. The Application Entity shall support one or more of the roles of File Set Creator (FSC) and File Set Reader (FSR) defined in PS 3.10 of [1].

3.3.2.2.1.1 File Set Creator

The AE acting as a File Set Creator generates a File Set under the PRI-PLAZA Application Profiles. File Set Creators shall be able to generate the Basic Directory SOP Class in the DICOMDIR file with all the subsidiary Directory Records related to the Image SOP Classes and Private SOP Classes stored in the File Set.

The FSC shall offer the ability to either finalize the disc at the completion of the most recent write session (no additional information can be subsequently added to the disc) or to allow multi-session (additional information may be subsequently added to the disc).

3.3.2.2.1.2 File Set Reader

The role of the File Set Reader shall be used by Application Entities which receive the transferred File Set. File Set Readers shall be able to read all the defined SOP Instances files defined for the specific Application Profiles to which a conformance claim is made, using all the defined Transfer Syntaxes.

3.3.2.3 PRI-PLAZA Profile Class

3.3.2.3.1 SOP Classes and Transfer Syntaxes

The allowed SOP Classes and Transfer Syntaxes for the PRI-PLAZA Profile Class are listed in Table 97. Private attributes that are used are listed in Annex A.10.

3.3.2.3.2 Physical Media and Media Formats

The PRI-PLAZA-CD Profile requires the 120mm CD-R physical media with the ISO/IEC 9660 Media Format as defined in PS3.12 of [1].

The PRI-PLAZA-DVD-RAM application profiles require the 120 mm DVD-RAM medium as defined in PS 3.12 of [1].

The PRI-PLAZA-DVD application profile re-quires any of the 120 mm DVD media other than DVD-RAM as defined in PS 3.12 of [1].

3.3.2.3.3 Directory Information in DICOMDIR

Conforming Application Entities shall include in the DICOMDIR File the Basic Directory IOD containing Directory Records at the Patient and subsidiary levels appropriate to the SOP Classes in the File-set. All DICOM files in the File-set incorporating SOP Instances defined for the specific Application profile shall be referenced by Directory Records.

Note: DICOMDIRs with no directory information are not allowed by this Application Profile
Privately defined IODs will be referenced by "PRIVATE" Directory Records.

3.4 Media Configuration

N.a.

4 Support of Character Sets

4.1 Character Sets for *syngo*.plaza

***syngo*.plaza** supports the following character sets:

- **Single Byte Character sets without Code Extensions**
    - ISO-IR 6
    - ISO-IR 100
    - ISO-IR 101
    - ISO-IR 109
    - ISO-IR 110
    - ISO-IR 144
    - ISO-IR 127
    - ISO-IR 126
    - ISO-IR 138
    - ISO-IR 148
    - ISO-IR 13 (ISO-IR 14 as G0 invoked in GL)
    - ISO-IR 166
- **Single Byte Character sets with ISO 2022 Code Extensions**
    - ISO 2022 IR 6
    - ISO 2022 IR 100
    - ISO 2022 IR 101
    - ISO 2022 IR 109
    - ISO 2022 IR 110
    - ISO 2022 IR 144
    - ISO 2022 IR 127
    - ISO 2022 IR 126
    - ISO 2022 IR 138
    - ISO 2022 IR 148
    - ISO 2022 IR 13(ISO-IR 14 as G0 invoked in GL)
    - ISO 2022 IR 166
- **MultiByte Character sets with ISO 2022 Code Extensions**
    - ISO 2022 IR 87
    - ISO 2022 IR 159
    - ISO 2022 IR 149
- **MultiByte Character sets without Code Extensions**
    - ISO_IR 192
    - GB18030

5 Extensions / Specializations / Privatizations

5.1 Standard Extended / Specialized / Private SOPs

5.1.1 SIEMENS Private Non-Image IOD

For encoding binary data-streams not representing image data, Siemens has created a private “Non-Image IOD” according to the rules governed by the DICOM Standard. The following section will roll-out the definition of this Private IOD. It can be communicated with Network Storage Service and Offline Media Storage Services.
The Siemens “Non-Image IOD” is identified by a private Non-Image Storage SOP Class UID of „1.3.12.2.1107.5.9.1“

5.1.1.1 Siemens Non-Image IOD – E-R Model

The E-R model in A.1.2 depicts those components of the DICOM Information Model which directly refer to the Siemens Non-Image IOD. The Frame of Reference IE, Overlay IE, Modality Lookup-Table IE, VOI Lookup-Table IE and Curve IE are not components of the Siemens Non-Image IOD.

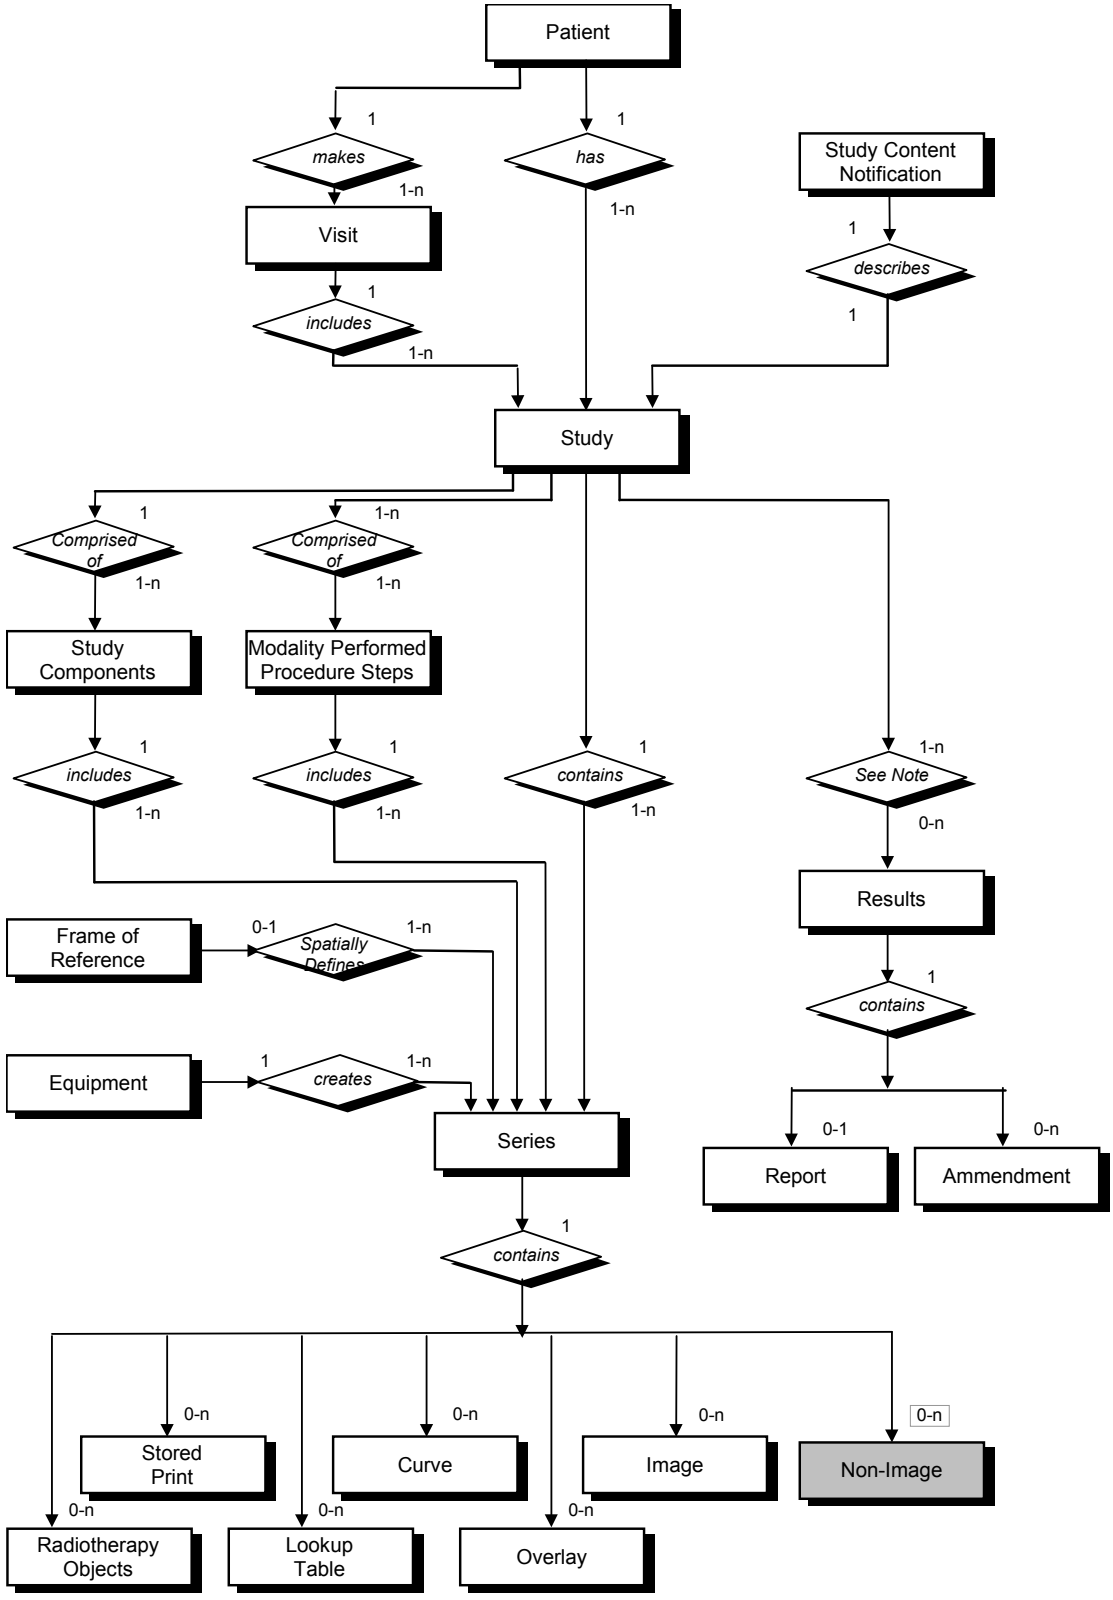

Figure 9: Information Model

5.1.1.2 Siemens Non-Image IOD - Module Table

IE	Module	Reference	Usage
Patient	Patient	[1] PS3.3 C.7.1.1	M
Study	General Study	[1] PS3.3 C.7.2.1	M
	Patient Study	[1] PS3.3 C.7.2.2	U
Series	General Series	[1] PS3.3 C.7.3.1	M
Equipment	General Equipment	[1] PS3.3 C.7.5.1	U
CSA	CSA Image Header	A.2.1	U
	CSA Series Header	A.2.2	U
	MEDCOM Header	A.2.3	U
	CSA Non-Image	A.1.3.1	M
	SOP Common	[1] PS3.3 C.12.1	M

Table 76: Siemens Non-Image IOD Module Table

5.1.1.3 Siemens Non-Image IOD - Modules

5.1.1.3.1 CSA Non-Image Module

The table in this section contains private IOD Attributes that describe CSA Non-Images.

Attribute Name	Tag	Owner	Type	Notes
Image Type	(0008,0008)	-	3	Image identification characteristics.
Acquisition Date	(0008,0022)	-	3	The date the acquisition of data that resulted in this data set started.
Acquisition Time	(0008,0032)	-	3	The time the acquisition of data that resulted in this data set started.
Conversion Type	(0008,0064)	-	3	Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation.
Referenced Image Sequence	(0008,1140)	-	3	A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as sequence of items: (0008,1150) and (0008,1155).
Derivation Description	(0008,2111)	-	3	A text description of how this data set was derived.
Source Image Sequence	(0008,2112)	-	3	A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to derive this data set. Zero or more Items may be included in this Sequence. Encoded as sequence of items: (0008,1150) and (0008,1155).
Patient Position	(0018,5100)	-	3	Patient position descriptor relative to the equipment.
Acquisition Number	(0020,0012)	-	3	A number identifying the single continuous gathering of data over a period of time which resulted in this data set.
Image Number	(0020,0013)	-	3	A number that identifies this data set.
Frame of Reference UID	(0020,0052)	-	3	Uniquely identifies the frame of reference for a Series.
Image Comments	(0020,4000)	-	3	User-defined comments about the image.
Quality Control Image	(0028,0300)	-	3	Indicates whether or not this image is a quality control or phantom image.

Attribute Name	Tag	Owner	Type	Notes
				If this Attribute is absent, then the image may or may not be a quality control or phantom image. Enumerated Values: YES, NO.
Burned in Annotation	(0028,0301)	-	3	Indicates whether or not image contains sufficient burned in annotation to identify the patient and date the image was acquired. If this Attribute is absent, then the image may or may not contain burned in annotation. Enumerated Values: YES, NO.
Lossy Image Compression	(0028,2110)	-	3	Specifies whether an Image has undergone lossy compression. Enumerated Values: 00 = Image has NOT been subjected to lossy compression, 01 = Image has been subjected to lossy compression.
Lossy Image Compression Ratio	(0028,2112)	-	3	Describes the approximate lossy compression ratio(s) that have been applied to this image. May be multi valued if successive lossy compression steps have been applied.
CSA Data Type	(0029,xx08)	SIEMENS CSA NON-IMAGE	1	CSA Data identification characteristics. Defined Terms: BSR REPORT = Study Report Data 3D EDITOR 3D FLY PATH = Fly Through Data 3D FLY VRT = Fly Through Data 3D FUSION MATRIX = Fusion Data RAW DATA NUM 4 = NUMARIS/ Raw Data RAW DATA SOM 5 = SOMARIS/ Raw Data RT3D CONFIG = InSpaceIS Data SPEC NUM 4 = NUMARIS/4 Spectroscopy
CSA Data Version	(0029,xx09)	SIEMENS CSA NON-IMAGE	3	Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format.
CSA Data Info	(0029,xx10)	SIEMENS CSA NON-IMAGE	3	Information to describe the CSA Data (7FE1,xx10).
CSA Data	(7FE1,xx10)	SIEMENS CSA NON-IMAGE	2	Binary data as byte stream.

Table 77: CSA Non-Image Module

5.1.1.4 Siemens Standard Extended Modules

IE	Module	Reference	Usage	Note
Image	CSA Image Header	A.2.1	U	private GG information
	CSA Series Header	A.2.2	U	
	MEDCOM Header	A.2.3	U	private ***syngo*** information
	MEDCOM OOG	A.2.4	U	if object graphics is attached to image

Table 78: Siemens Standard Extended Modules

5.1.1.4.1 CSA Image Header Module

The table in this section contains private IOD Attributes that describe the CSA Image Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Image Header Type	(0029,xx08)	SIEMENS CSA HEADER	1	CSA Image Header identification

				characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = SOMARIS/5
CSA Image Header Version	(0029,xx09)	SIEMENS CSA HEADER	3	Version of CSA Image Header Info (0029,xx10) format.
CSA Image Header Info	(0029,xx10)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

Table 79: CSA Image Header Module

5.1.1.4.2 CSA Series Header Module

The table in this section contains private IOD Attributes that describe the CSA Series Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Series Header Type	(0029,xx18)	SIEMENS CSA HEADER	1	CSA Series Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4
CSA Series Header Version	(0029,xx19)	SIEMENS CSA HEADER	3	Version of CSA Series Header Info (0029,xx20) format.
CSA Series Header Info	(0029,xx20)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

Table 80: CSA Series Header Module

5.1.1.4.3 MEDCOM Header Module

The table in this section contains private IOD Attributes that describe MEDCOM Header:

Attribute Name	Tag	Owner	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MEDCOM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 (Required if MedCom Header Info (0029,xx10) present.)
MedCom Header Version	(0029,xx09)	SIEMENS MEDCOM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. (Required if MEDCOM Header Info (0029,xx10) present.)
MedCom Header Info	(0029,xx10)	SIEMENS MEDCOM HEADER	3	Manufacturer model dependent information. The value of the attribute MedCom Header Info (0029,xx10) can be build up in each user defined format.
MedCom History Information	(0029,xx20)	SIEMENS MEDCOM HEADER	3	MedCom defined Patient Registration history information. See A.2.3.1.
PMTF Information 1	(0029,xx31)	SIEMENS MEDCOM HEADER	3	Transformation Information
PMTF Information 2	(0029,xx32)	SIEMENS MEDCOM HEADER	3	Transformation Information
PMTF Information 3	(0029,xx33)	SIEMENS MEDCOM HEADER	3	Transformation Information
PMTF Information 4	(0029,xx34)	SIEMENS MEDCOM HEADER	3	Transformation Information
PMTF Information 5	(0029,xx35)	SIEMENS MEDCOM HEADER	3	Transformation Information
Application Header Sequence	(0029,xx40)	SIEMENS MEDCOM HEADER	3	Sequence of Application Header items. Zero or more items are possible.
>Application Header Type	(0029,xx41)	SIEMENS MEDCOM HEADER	1C	Application Header identification characteristics. Required, if Sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MEDCOM HEADER	3	Identification of an application header
>Application Header Version	(0029,xx43)	SIEMENS MEDCOM HEADER	3	Version of CSA Series Header Info (0029,xx44) format.
>Application Header Info	(0029,xx44)	SIEMENS MEDCOM	3	Application dependent information.

Attribute Name	Tag	Owner	Type	Notes
		HEADER		
Workflow Control Flags	(0029,xx50)	SIEMENS MEDCOM HEADER	3	Eight free definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS MEDCOM HEADER	3	Flag to control remote archive management system to keep the image always online (also when already archived). Enumerated Values: 00 = remote control not required 01 = keep image online
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS MEDCOM HEADER	3	Flag to control remote archive management system not to archive the related image. Enumerated Values: 00 = remote control not required 01 = don't archive image
Image Location Status	(0029,xx53)	SIEMENS MEDCOM HEADER	3	Image location status to control retrieving. Defined Terms: ONLINE = retrieving has to be done as usual, NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54), OFFLINE = invoking a retrieve operation initiates an operator request, INVALID = invoking a retrieve operation would always result in an error.
Estimated Retrieve Time	(0029,xx54)	SIEMENS MEDCOM HEADER	3	Estimated retrieve time in seconds. A value less then zero (< 0) indicates location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS MEDCOM HEADER	3	Data size of images in MByte.
Siemens Link Sequence	(0029,xx70)	SIEMENS MEDCOM HEADER	3	Sequence of link items. Each item identify the location of one missing tag. One or more items can be included in this sequence.
Referenced Tag	(0029,xx71)	SIEMENS MEDCOM HEADER	1	The referenced tag. The value of this tag is in the Child Data Object (CDO). Currently it is always Pixel Data (7FE0,0010).
Referenced Tag Type	(0029,xx72)	SIEMENS MEDCOM HEADER	1	The Value Representation (type) of the missing tag (e.g. OW). Enumerated values are all DICOM defined Value Representations.
Referenced Value Length	(0029,xx73)	SIEMENS MEDCOM HEADER	1	The length of the referenced tag value in bytes.
Referenced Object Device Type	(0029,xx74)	SIEMENS MEDCOM HEADER	1	The Device Type that stores the Child Data Object (CDO) with the referenced tag value. Currently it should be "SHMEM". In future, "SDM", "LOID" or "FILE" are also imaginable. Defined Terms are SHMEM = Shared Memory SDM = Series Data Management LOID = Database FILE
Referenced Object Device Location	(0029,xx75)	SIEMENS MEDCOM HEADER	2	The Location of the device that stores the Child Data Object (CDO) with the referenced tag value. For the "SHMEM" case, it is the shared memory directory. Can be empty, then the default directory will be taken. In future, for "SDM" this will be the SDM_ID, for FILE it will be the directory name and for "LOID" it will be the database name.
Referenced Object ID	(0029,xx76)	SIEMENS MEDCOM HEADER	1	The ID of the object that contains the Child Data Object (CDO) with the referenced tag value. In case of "SHMEM" it is the shared memory ID. In future, for "SDM" this will be a Sirius

Attribute Name	Tag	Owner	Type	Notes
				OID, for “FILE” the file name, for “DB” the LOID.
Series Work Flow Status	(0029,xx60)	SIEMENS MEDCOM HEADER2	3	***syngo*** Patient Browser specific flags used for clinical work: • com = completed • rea = read • ver = verified

Table 81: MEDCOM Header Module

5.1.1.4.4 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined as follows.

Part	Name	Type	Bytes	Notes
header	Identifier	string	32	Always “CSA HISTORY”
	Version	string	32	e.g. “V1.10”
n Items	Class Name	string	64	
	Modification String	string	1024	

Table 82: MEDCOM History Information

5.1.1.4.5 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used whenever object graphics is drawn on the image and need to be stored as graphic object properties. Given the condition that the module contents was not removed by other modalities, the graphic objects remain re-animatable if such an image was transferred and is then retrieved back.

Attribute Name	Tag	Owner	Type	Notes
MedCom OOG Type	(0029,xx08)	SIEMENS MEDCOM OOG	1	MEDCOM Object Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1 MEDCOM OOG 2
MedCom OOG Version	(0029,xx09)	SIEMENS MEDCOM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format.
MedCom OOG Info	(0029,xx10)	SIEMENS MEDCOM OOG	3	MEDCOM Object Oriented Graphics (OOG) data.

Table 83: MEDCOM OOG Module

The graphics objects are also fully drawn in the Image Overlay Plane for compatibility with other products, which do not support the MedCom OOG module. Any system not supporting the MedCom OOG module shall remove the OOG module and its contents when modifying the image overlay plane content.

5.1.1.4.6 syngo Report Data

The module contains private IOD Attributes that describe ***syngo*** reports. This module is used when ***syngo*** report data are added to DICOM SR and DICOM SC objects.

Attribute Name	Tag	Owner	Type	Notes
syngo Report Type	(0029,xx08)	SIEMENS CSA REPORT	1	***syngo*** report characteristics, e.g. report creating application. Defined Terms: CT_LUNGCARE MR_ARGUS This attribute value will be used to identify the corresponding application during generic

				extension dll management. A restricted character set is used: only A-Z and underscore are supported.
syngo Report Version	(0029,xx09)	SIEMENS CSA REPORT	3	Version of ***syngo*** Report Data (0029,xx10) format.
syngo Report Data	(0029,xx10)	SIEMENS CSA ENVELOPE	3	A representation of DICOM SR Attribute Content Sequence (0040,A730). This includes the document relationship and document content. This data will typically be represented using an XML encoding according to a Siemens private scheme.
syngo Report Presentation	(0029,xx11)	SIEMENS CSA ENVELOPE	3	A representation of the recommended presentation for the ***syngo*** Report Data (0029,xx10). This presentation will typically be encoded in XSLT.
SR Variant	(0029,xx15)	SIEMENS CSA REPORT		DICOM SR variant. Enumerated Values: 0 = Basic Text SR (1.2.840.10008.5.1.4.1.1.88.11) 1 = Enhanced SR (1.2.840.10008.5.1.4.1.1.88.22) 2 = Comprehensive SR (1.2.840.10008.5.1.4.1.1.88.33) 3 = Mammography CAD SR (1.2.840.10008.5.1.4.1.1.88.50) 4 = Key Object Selection Document (1.2.840.10008.5.1.4.1.1.88.59) 5 = 4 = Chest CAD SR (1.2.840.10008.5.1.4.1.1.88.65)
SC SOP Instance UID	(0029,xx17)	SIEMENS CSA REPORT	3	DICOM SOP Instance UID of ***syngo*** based SC Image representing the ***syngo*** report object. This UID will be used to identify the Resulting SC object after SR to SC conversion.

Table 84: *syngo* Report Data

5.1.1.4.7 *syngo* Report Info

The module ***syngo*** Report Info contains all DICOM SR attributes except the Contents Sequence 0040,A730). This module is only used during SR to SC conversion.

Tag	Private Owner Code	Name	VR	VM
(0029,xx08)	SIEMENS CSA NON-IMAGE	CSA Data Type	CS	1
(0029,xx09)	SIEMENS CSA NON-IMAGE	CSA Data Version	LO	1
(0029,xx10)	SIEMENS CSA NON-IMAGE	CSA Data Info	OB	1
(0029,xx08)	SIEMENS CSA HEADER	CSA Image Header Type	CS	1
(0029,xx09)	SIEMENS CSA HEADER	CSA Image Header Version	LO	1
(0029,xx10)	SIEMENS CSA HEADER	CSA Image Header Info	OB	1
(0029,xx18)	SIEMENS CSA HEADER	CSA Series Header Type	CS	1
(0029,xx19)	SIEMENS CSA HEADER	CSA Series Header Version	LO	1
(0029,xx20)	SIEMENS CSA HEADER	CSA Series Header Info	OB	1
(0029,xx08)	SIEMENS CSA REPORT	***syngo*** Report Type	CS	1
(0029,xx09)	SIEMENS CSA REPORT	***syngo*** Report	LO	1
(0029,xx15)	SIEMENS CSA REPORT	SR Variant	US	1
(0029,xx17)	SIEMENS CSA REPORT	SC SOP Instance UID	UI	1
(0029,xx10)	SIEMENS CSA ENVELOPE	***syngo*** Report Data	OB	1
(0029,xx11)	SIEMENS CSA ENVELOPE	***syngo*** Report Presentation	OB	1
(0029,xx08)	SIEMENS MEDCOM HEADER	MedCom Header Type	CS	1
(0029,xx09)	SIEMENS MEDCOM HEADER	MedCom Header Version	LO	1

(0029,xx10)	SIEMENS MEDCOM HEADER	MedCom Header Info	OB	1
(0029,xx20)	SIEMENS MEDCOM HEADER	MedCom History Information	OB	1
(0029,xx31)	SIEMENS MEDCOM HEADER	PMTF Information 1	LO	1
(0029,xx32)	SIEMENS MEDCOM HEADER	PMTF Information 2	UL	1
(0029,xx33)	SIEMENS MEDCOM HEADER	PMTF Information 3	UL	1
(0029,xx34)	SIEMENS MEDCOM HEADER	PMTF Information 4	CS	1
(0029,xx35)	SIEMENS MEDCOM HEADER	PMTF Information 5	UL	1
(0029,xx40)	SIEMENS MEDCOM HEADER	Application Header Sequence	SQ	1
(0029,xx41)	SIEMENS MEDCOM HEADER	Application Header Type	CS	1
(0029,xx42)	SIEMENS MEDCOM HEADER	Application Header ID	LO	1
(0029,xx43)	SIEMENS MEDCOM HEADER	Application Header Version	LO	1
(0029,xx44)	SIEMENS MEDCOM HEADER	Application Header Info	OB	1
(0029,xx50)	SIEMENS MEDCOM HEADER	Workflow Control Flags	LO	8
(0029,xx51)	SIEMENS MEDCOM HEADER	Arch. Management Flag Keep Online	CS	1
(0029,xx52)	SIEMENS MEDCOM HEADER	Arch. Mgmnt Flag Do Not Archive	CS	1
(0029,xx53)	SIEMENS MEDCOM HEADER	Image Location Status	CS	1
(0029,xx54)	SIEMENS MEDCOM HEADER	Estimated Retrieve Time	DS	1
(0029,xx55)	SIEMENS MEDCOM HEADER	Data Size of Retrieved Images	DS	1
(0029,xx70)	SIEMENS MEDCOM HEADER	Siemens Link Sequence	SQ	1
(0029,xx71)	SIEMENS MEDCOM HEADER	Referenced Tag	AT	1
(0029,xx72)	SIEMENS MEDCOM HEADER	Referenced Tag Type	CS	1
(0029,xx73)	SIEMENS MEDCOM HEADER	Referenced Value Length	UL	1
(0029,xx74)	SIEMENS MEDCOM HEADER	Referenced Object Device Type	CS	1
(0029,xx75)	SIEMENS MEDCOM HEADER	Referenced Object Device Location	OB	1
(0029,xx76)	SIEMENS MEDCOM HEADER	Referenced Object ID	OB	1
(0029,xx60)	SIEMENS MEDCOM HEADER2	Series Work Flow Status	LO	1
(0029,xx08)	SIEMENS MEDCOM OOG	MedCom OOG Type	CS	1
(0029,xx09)	SIEMENS MEDCOM OOG	MedCom OOG Version	LO	1
(0029,xx10)	SIEMENS MEDCOM OOG	MedCom OOG Info	OB	1
(7FE1,xx10)	SIEMENS CSA NON-IMAGE	CSA Data	OB	1

Table 85: Registry of DICOM Data Elements

Annex A Tables

A.1. Supported Storage SOP Classes of Main AE and Media Handling AE

SOP Class Name	SOP Class UID	SCU	SCP	Display[1]	Media
Supported Storage SOP Classes					
Computed Radiography Object Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes	Yes	STD-GEN[2]
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes	Yes	STD-GEN[2]
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes	No	STD-GEN[2]
Digital Mammography X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes	Yes	STD-GEN[2]
Digital Mammography X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes	No	STD-GEN[2]
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	Yes	Yes	STD-GEN[2]
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	Yes	Yes	STD-GEN[2]
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	Yes	Yes	STD-GEN[2]
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	Yes	No	STD-GEN[2]
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	Yes	No	STD-GEN[2]
Enhanced MR Color Image Storage	1.2.840.10008.5.1.4.1.1.4.3	Yes	Yes	No	STD-GEN[2]
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes	Yes	STD-GEN[2]
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes	Yes	STD-GEN[2]
US Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	Yes	Yes	STD-GEN[2]
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes	Yes	STD-GEN[2]
US Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Yes	Yes	Yes	STD-GEN[2]
SC Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes	Yes	STD-GEN[2]
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes	Yes	STD-GEN[2]
Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	Yes	Yes	No	STD-GEN[2]
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Yes	Yes	No	STD-GEN[2]
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes	Yes	STD-GEN[2]
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes	Yes	STD-GEN[2]

[1] Please refer to annex A.11 and A.12 for further requirements and restrictions on viewing
[2] STD-GEN-CD and STD-GEN-DVD-RAM as FSR,FSC,FSU

SOP Class Name	SOP Class UID	SCU	SCP	Display[1]	Media
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Yes	Yes	Yes	STD-GEN[2]
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	Yes	No	STD-GEN[2]
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	Yes	Yes	STD-GEN[2]
Stored Print Storage	1.2.840.10008.5.1.1.27	Yes	Yes	No	STD-GEN[2]
Hardcopy Grayscale Image Storage	1.2.840.10008.5.1.1.29	Yes	Yes	Yes	STD-GEN[2]
Hardcopy Color Image Storage	1.2.840.10008.5.1.1.30	Yes	Yes	Yes	STD-GEN[2]
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	Yes	Yes	STD-GEN[2]
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	Yes	Yes	STD-GEN[2]
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	Yes	No	STD-GEN[2]
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	Yes	Yes	STD-GEN[2]
Video Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	Yes	Yes	STD-GEN[2]
Video Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	Yes	Yes	STD-GEN[2]
Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	Yes	Yes	STD-GEN[2]
Ophthalmic Photography 8 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	Yes	Yes	STD-GEN[2]
Ophthalmic Photography 16 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	Yes	Yes	STD-GEN[2]
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	Yes	Yes	STD-GEN[2]
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes	Yes	STD-GEN[2]
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	Yes	Yes	No	STD-GEN[2]
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Yes	Yes	No	STD-GEN[2]
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Yes	Yes	No	STD-GEN[2]
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Yes	Yes	No	STD-GEN[2]
RT Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6	Yes	Yes	No	STD-GEN[2]
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	Yes	Yes	No	STD-GEN[2]
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	Yes	No	STD-GEN[2]
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	Yes	No	STD-GEN[2]
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Yes	Yes	Yes	STD-GEN[2]
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	Yes	No	STD-GEN[2]

SOP Class Name	SOP Class UID	SCU	SCP	Display[1]	Media
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes	Yes	STD-GEN[2]
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Yes	Yes	Yes	STD-GEN[2]
Key Object Selection Storage	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes	No	STD-GEN[2]
Chest CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.65	Yes	Yes	No	STD-GEN[2]
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes	No	STD-GEN[2]
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	Yes	No	
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes	Yes	STD-GEN[2]
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	Yes	Yes	STD-GEN[2]
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes	Yes	STD-GEN[2]
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	Yes	No	STD-GEN[2]
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes	No	STD-GEN[2]
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	Yes	No	STD-GEN[2]
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	Yes	No	STD-GEN[2]
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	Yes	No	STD-GEN[2]
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	Yes	No	STD-GEN[2]
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	Yes	Yes	No	STD-GEN[2]
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Yes	Yes	No	STD-GEN[2]
Enhanced XA Image Storage	1.2.840.10008.5.1.4.1.1.12.1.1	Yes	Yes	No	STD-GEN[2]
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Yes	Yes	No	STD-GEN[2]
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	Yes	No	STD-GEN[2]
X-Ray Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes	No	STD-GEN[2]
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Yes	Yes	No	STD-GEN[2]
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	Yes	Yes	No	STD-GEN[2]
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	Yes	No	STD-GEN[2]
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Yes	Yes	No	STD-GEN[2]
Media Storage Directory Storage	1.2.840.10008.1.3.10	No	No	No	STD-GEN[2]
Supported private Storage SOP Classes					

SOP Class Name	SOP Class UID	SCU	SCP	Display[1]	Media
Siemens Private CSA Non-Image Storage	1.3.12.2.1107.5.9.1	Yes	Yes	No	
Philips Private Gyroscan MR Storage	1.3.46.670589.11.0.0.12.2	Yes	Yes	No	

Table 86: Storage SOP Classes supported by Main AE and Media Handling AE

A.2. Supported Non-Storage SOP Classes of Main AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported Verification SOP Classes			
Verification	1.2.840.10008.1.1	Yes[1]	Yes
Supported Storage Commitment SOP Classes			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	Yes
Supported Query/Retrieve SOP Classes			
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Patient/Study Only Query/Retrieve Information Model - FIND (Retired)	1.2.840.10008.5.1.4.1.2.3.1	Yes	Yes
Patient/Study Only Query/Retrieve Information Model – MOVE (Retired)	1.2.840.10008.5.1.4.1.2.3.2	Yes	Yes
Supported private Report Management SOP Classes			
MITRA Report Management	1.2.840.113532.3500.8	Yes	No
Supported Print Management SOP Classes			
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management Meta	1.2.840.10008.5.1.1.18	Yes	No
Print Job	1.2.840.10008.5.1.1.14	Yes	No
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23	Yes	No
Supported Basic Worklist Management SOP Classes			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Yes	No

Table 87: Non-Storage SOP Classes supported by Main AE

A.3. Supported SOP Classes of Query Spanning AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported Query Spanning SOP Classes			
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Patient/Study Only Query/Retrieve Information Model - FIND - Retired	1.2.840.10008.5.1.4.1.2.3.1	Yes	Yes

Table 88: SOP Classes supported by Query Spanning AE

[1] The SCU for the Verification SOP Class is included in a service utility that is part of the ***syngo*®.plaza** software.

A.4. Supported SOP Classes of Retrieve Spanning AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported Retrieve Spanning SOP Classes			
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Patient/Study Only Query/Retrieve Information Model - MOVE - Retired	1.2.840.10008.5.1.4.1.2.3.2	Yes	Yes

Table 89: SOP Classes supported by Retrieve Spanning AE

A.5. Supported SOP Classes of MPPS Manager AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported MPPS SOP Classes			
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Yes	Yes

Table 90: SOP Classes supported by MPPS Manager AE

A.6. Supported SOP Classes of Modality Worklist Provider AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported Basic Worklist Management SOP Classes			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	No	Yes

Table 91: SOP Classes supported by Modality Worklist Provider AE

A.7. Supported SOP Classes of MPPS Image Manager AE

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported MPPS SOP Classes			
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	No	Yes

Table 92: SOP Classes supported by MPPS Image Manager AE

A.8. Supported Query attributes

Attribute Name	Attribute Tag	Query Matching Key (SCP)	Query Matching Key (SCU)	Query Return Key (SCP)	Query Return Key (SCU)
Specific Character Set	(0008,0005)	N	N	Y	Y
Patient's Name	(0010,0010)	Y	Y	Y	Y
PatientID	(0010,0020)	Y	Y	Y	Y
Patient's Birth Date	(0010,0030)	Y	Y	Y	Y
Patient's Sex	(0010,0040)	Y	N	Y	Y
Storage Media File Set ID	(0088,0130)	N	N	Y	Y
Storage Media File Set UID	(0088,0140)	N	N	Y	Y

Table 93: Supported Patient Level attributes

Attribute Name	Attribute Tag	Query Matching Key (SCP)	Query Matching Key (SCU)	Query Return Key (SCP)	Query Return Key (SCU)
Specific Character Set	(0008,0005)	N	N	Y	Y
Study Date	(0008,0020)	Y	Y	Y	Y
Study Time	(0008,0030)	Y	Y	Y	Y
Accession Number	(0008,0050)	Y	Y	Y	Y
Modalities In Study	(0008,0061)	Y	N	Y	N
Institution Name	(0008,0080)	Y	Y	Y	Y
Referring Physician's Name	(0008,0090)	Y	Y	Y	Y
Study Description	(0008,1030)	Y	N	Y	N
Name of Physician Reading Study	(0008,1060)	N	Y	Y	Y
Study ID	(0020,0010)	Y	Y	Y	Y
Study Instance UID	(0020,000D)	Y	Y	Y	Y
Number of Study related Series	(0020,1206)	N	N	Y	Y
Number of Study related Images	(0020,1208)	N	N	Y	Y
Current Patient Location	(0038,0300)	Y	Y	Y	Y
Storage Media File Set ID	(0088,0130)	N	N	Y	Y
Storage Media File Set UID	(0088,0140)	N	N	Y	Y

Table 94: Supported Study Level attributes

Attribute Name	Attribute Tag	Query Matching Key (SCP)	Query Matching Key (SCU)	Query Return Key (SCP)	Query Return Key (SCU)
Series Date	(0008,0021)	Y	Y	Y	Y
Series Time	(0008,0031)	Y	Y	Y	Y
Modality	(0008,0060)	Y	Y	Y	Y
Series Description	(0008,103E)	Y	N	Y	Y
Body Part Examined	(0018,0015)	Y	Y	Y	Y
Series Instance UID	(0020,000E)	Y	Y	Y	Y
Series Number	(0020,0011)	Y	Y	Y	Y
Number of Series Related Images	(0020,1209)	N	N	Y	Y
Performed Procedure Step Start Date	(0040,0244)	Y	Y	Y	Y
Performed Procedure Step Start Time	(0040,0245)	Y	Y	Y	Y
Request Attribute Sequence	(0040,0275)				
> Requested Procedure ID	(0040,1001)	Y	Y	Y	Y
> Scheduled Procedure Step ID	(0040,0009)	Y	Y	Y	Y
Performed Procedure Start Date	(0040,0244)	Y	Y	Y	Y
Performed Procedure Start Time	(0040,0245)	Y	Y	Y	Y
Exam Status	(0095,”SIENET”,0004)	Y	Y	Y	Y
Rebuild Status	(0095,”SIENET”,000C)	Y	Y	Y	Y
Storage Media File Set ID	(0088,0130)	N	N	Y	Y
Storage Media File Set	(0088,0140)	N	N	Y	Y

UID					

Table 95: Supported Series Level attributes

Attribute Name	Attribute Tag	Query Matching Key (SCP)	Query Matching Key (SCU)	Query Return Key (SCP)	Query Return Key (SCU)
SOP Instance UID	(0008,0018)	Y	Y	Y	Y
Instance Number	(0020,0013)	Y	Y	Y	Y
SOP Class UID	(0008,0016)	Y	N	Y	Y
Number of Frames	(0028,0008)	N	N	Y	Y
Rows	(0028,0010)	N	N	Y	Y
Columns	(0028,0011)	N	N	Y	Y
Bits Allocated	(0028,0100)	N	N	Y	Y
Presentation State Specific Attributes					
Presentation Label	(0070,0080)	N	N	Y	Y
Presentation Description	(0070,0081)	N	N	Y	N
Presentation Creation Date	(0070,0082)	N	N	Y	Y
Presentation Creation Time	(0070,0083)	N	N	Y	Y
Presentation Creator.s Name	(0070,0084)	N	N	Y	Y
Referenced Series Sequence	(0008,1115)				
>Series Instance UID	(0020,000E)	N	N	Y	N
>Referenced Image Sequence	(0008,1140)				
>>Referenced SOP Class UID	(0008,1150)	N	N	Y	N
>>Referenced SOP Instance UID	(0008,1155)	N	N	Y	N

Table 96: Supported Image Level attributes

A.9. Supported Presentation Contexts for Storage service and PRI-PLAZA SOP Classes and Transfer Syntaxes

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
Computed Radiography Object Storage	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4)[2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Digital X-Ray	1.2.840.10008.5.1.	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/	None

[1] If Lossy is selected in the Send dialog for 8 Bit images
[2] If Lossy is selected in the Send dialog for 12 Bit images
[3] If Lossless is selected in the Send dialog

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
Image Storage - For Presentation	4.1.1.1.1	Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-	SCP	
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Digital X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Digital Mammography X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Digital Mammography X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
Digital Intra-oral X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Digital Intra-oral X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
US Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
US Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Implicit VR Little Endian	1.2.840.10008.1.2			SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	-	-		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	M		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
US Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
US Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.6	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Stored Print Storage	1.2.840.10008.5.1.1.27	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Hardcopy Grayscale Image Storage	1.2.840.10008.5.1.1.29	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Hardcopy Color Image Storage	1.2.840.10008.5.1.1.30	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Enhanced MR Color Image Storage	1.2.840.10008.5.1.4.1.1.4.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Key Object Selection Storage	1.2.840.10008.5.1.4.1.1.88.59	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Chest CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.65	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Enhanced XA Image Storage	1.2.840.10008.5.1.4.1.1.12.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
X-Ray Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.67	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
Ophthalmic Photography 8 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Ophthalmic Photography 16 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	O	M		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	O	M		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	O	M		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	O	O		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	**UID**	**Name List**	**UID List**				
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Video Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	-	-		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	-	-		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	-	-		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	-	-		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	-	-		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Video Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	-	-		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	-	-		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	-	-		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	-	-		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	-	-		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	-	-		
		JPEG Baseline[1]	1.2.840.10008.1.2.4.50	-	-		
		JPEG Extended (Process 2 & 4) [2]	1.2.840.10008.1.2.4.51	-	-		
		JPEG Lossless[3]	1.2.840.10008.1.2.4.70	-	-		
		JPEG 2000 Lossless Only	1.2.840.10008.1.2.4.90	-	-		
		JPEG 2000	1.2.840.10008.1.2.4.91	-	-		
		RLE Lossless	1.2.840.10008.1.2.5	O	M		
		MPEG2 Main Profile @ Main Level	1.2.840.10008.1.2.4.100	O	M		
Media Storage Directory Storage	1.2.840.10008.1.3.10	Explicit VR Little Endian	1.2.840.10008.1.2.1	M	M	---	---
Supported private Storage SOP Classes							
CSA Non Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		

Abstract Syntax		Transfer Syntax		FSC	FSR	Role	Ext. Neg.
Name	UID	Name List	UID List				
Philips Private Gyroscan MR Storage	1.3.46.670589.11.0.0.12.2	Implicit VR Little Endian	1.2.840.10008.1.2	-	-	SCU/ SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2	-	-		
		Explicit VR Little Endian	1.2.840.10008.1.2.1	O	M		

Table 97: Supported Presentation Contexts for Storage service

A.10. Registry of DICOM Private Data Elements

Attribute Name	Attribute Tag	Private Creator Code	VR	VM
Zoom Factor	(0029,xx01)	SHS MagicView 300	FD	1-N
Pan Factor X	(0029,xx02)	SHS MagicView 300	FD	1
Pan Factor Y	(0029,xx03)	SHS MagicView 300	FD	1
NmPalette	(0029,xx04)	SHS MagicView 300	LO	1
Folder Reported Status	(0095,xx04)	SIENET	UL	1
Folder Rebuild Status	(0095,xx0C)	SIENET	UL	1
Key Images	(0099,xx02)	SIENET	UL	1
Private Image Number	(0099,xx05)	SIENET	SL	1

Table 98: Registry of Private Data Elements

The Private Creator Code "SHS MagicView 300" is used to enable interoperability with old versions of syngo Imaging XS.

The Private Creator Code "SIENET" is used to enable interoperability with old versions of syngo Imaging XS and SIENET systems.

A.11. Requirements for Viewing of DICOM Images

This annex of the ***syngo*.plaza** DICOM Conformance Statement documents the required DICOM Tags for the Viewing application.

Requirements for Display and Evaluation

- Proper values for the following DICOM tags:
  - (0028,1050) – Window Center
  - (0028,1051) – Window Width
  - (0028,1051) – Rescale Intercept
  - (0028,1053) – Rescale Slope
- Maximum Image Size: 10000 Rows and 10000 Columns. Bigger images cannot be loaded to Viewer.
- Maximum number of frames for Multiframe: 1000.

A.12. Restrictions for Viewing of DICOM Images

SOP Classes

Only the images of the SOP Classes marked in Table 86 can be displayed by the Viewer.

Restrictions for compression

Images compressed in Transfer Syntax RLE Lossless (1.2.840.10008.1.2.5) can only be displayed, if they don't have a Photometric Interpretation of MONOCHROME1 or MONOCHROME2.

Unsupported Grayscale Presentation State Modules

The following Grayscale Presentation State Modules are not supported for display:

- Mask Subtraction Module
- Displayed Area Module (Zoom, Pan, …) at Frame level

Unsupported Grayscale Presentation State Attributes

The Grayscale Presentation State Attributes listed in Table 99 are not supported for display.

Attribute Name	Attribute Tag	Module Name
Graphic Layer Recommended Display Grayscale Value	(0070,0066)	Graphic Layer Module
Graphic Layer Recommended Display CIELab Value	(0070,0401)	Graphic Layer Module
Compound Graphic Sequence	(0070,0209)	Graphic Annotation Module

Table 99: Grayscale Presentation State Attributes not supported

A distinct warning icon is displayed in Viewer's Image segments if an error occurs while processing the Presentation State objects.

Unsupported macros/modules for Enhanced SOP Classes

The following modules/macros are not supported for Enhanced SOP Classes:

- Frame VOI LUT Macro
- Multi-frame Dimension Module

A.13. Private MITRA Report Management Query

Attribute Name	Attribute Tag	Matching Key SCU	Return Key SCU
Patient's Name	(0010,0010)	Yes	Yes
Patient ID	(0010,0020)	Yes	Yes
Patient's Birth Date	(0010,0030)	Yes	Yes
Accession Number	(0008,0050)	Yes	Yes
Requested Procedure ID	(0040,1001)	Yes	Yes
Study Instance UID	(0020,000D)	Yes	Yes

Attribute Name	Attribute Tag	Matching Key SCU	Return Key SCU
Requested Procedure Description	(0032,1060)	No	Yes
Requested Procedure Code Sequence	(0032,1064)	No	Yes
>Code Value	(0008,0100)	No	Yes
>Coding Scheme Designator	(0008,0102)	No	Yes
>Code Meaning	(0008,0104)	No	Yes
Result ID Issuer	(4008, 0042)	No	Yes
Interpretation Approval Time	(4008,0013)	No	Yes
Physicians Approving Interpretation	(4008,0014)	No	Yes
Interpretation Recorded Date	(4008,0100)	No	Yes
Interpretation Recorded Time	(4008,0101)	No	Yes
Interpretation Recorder	(4008,0102)	No	Yes
Interpretation Transcriber	(4008,010A)	No	Yes
Interpretation Author	(4008,010C)	No	Yes
Approver Sequence	(4008,0111)	No	Yes
> Approval Date	(4008,0112)	No	Yes
> Approval Time	(4008,0113)	No	Yes
> Physicians Approving Interpretation	(4008,0114)	No	Yes
Interpretation Text	(4008,0115)	No	Yes
Interpretation ID	(4008,0200)	No	Yes
Interpretation Status ID	(4008,0212)	No	Yes

Table 100: Attributes for Report Content Query

Siemens Healthcare Headquarters
Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany
Phone: +49 9131 84-0
siemens.com/healthcare

Siemens Healthcare GmbH 2015

All rights reserved