



DICOM Conformance Statement

syngo.via View&GO
VA10A

CONFORMANCE STATEMENT OVERVIEW

The **syngo.via View&GO** is lightweight reading workstations with connectivity to DICOM modalities and healthcare information systems. By default one **syngo.via View&GO (AE)** is used. It is possible to configure usage of multiple different AEs for the individual DICOM services.

The **syngo.via View&GO**:

- o requests storage of objects (images, reports, encapsulated PDF)
- o support query and retrieval of objects from a remote node
- o displays images to a user
- o imports objects from portable interchange media
- o exports objects to non-optical storage device (e.g. USB stick)

The **syngo.via View&GO** conforms to the DICOM Standard and supports the network services as described in Table 0-1 and the media services as described in Table 0-2.

Table 0-1 Network Services

SOP Classes	Service Class User (SCU)	Service Class Provider (SCP)
Verification		
Verification Service	Yes	Yes
Transfer(Image SOP Class)		
Breast Tomosynthesis Image Storage	Yes	Yes
Computed Radiography Image Storage	Yes	Yes
CT Image Storage	Yes	Yes
Digital Mammography X-Ray Image Storage - For Presentation	Yes	Yes
Digital Mammography X-Ray Image Storage - For Processing	Yes	Yes
Digital X-Ray Image Storage - For Presentation	Yes	Yes
Digital X-Ray Image Storage - For Processing	Yes	Yes
Enhanced CT Image Storage	Yes	Yes
Enhanced MR Image Storage	Yes	Yes
Enhanced MR Color Image Storage	Yes	Yes
Enhanced XA Image Storage	Yes	Yes
Enhanced XRF Image Storage	Yes	Yes
MR Image Storage	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image Storage	Yes	Yes
Multi-frame Single Bit Secondary Capture Image Storage	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage	Yes	Yes

SOP Classes	Service Class User (SCU)	Service Class Provider (SCP)
Nuclear Medicine Image Storage	Yes	Yes
PET Image Storage	Yes	Yes
RT Image Storage	Yes	Yes
Secondary Capture Image Storage	Yes	Yes
Segmentation Storage	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Ultrasound Image Storage (Retired)	Yes	Yes
Ultrasound Multi-Frame Image Storage	Yes	Yes
Ultrasound Multi-Frame Image Storage (Retired)	Yes	Yes
X-Ray 3D Angiographic Image Storage	Yes	Yes
X-Ray Angiographic Image Storage	Yes	Yes
X-Ray Radio-Fluoroscopic Image Storage	Yes	Yes
Transfer(Non-Image SOP Class)		
12-lead ECG Waveform Storage	Yes	Yes
Ambulatory ECG Waveform Storage	Yes	Yes
Basic Text SR Storage	Yes	Yes
Blending Softcopy Presentation State Storage	Yes	Yes
Cardiac Electrophysiology Waveform Storage	Yes	Yes
Color Softcopy Presentation State Storage (store & forward only)	Yes	Yes
Comprehensive SR Storage	Yes	Yes
Deformable Spatial Registration Storage	Yes	Yes
Encapsulated PDF Storage	Yes	Yes
Enhanced SR Storage	Yes	Yes
General ECG Waveform Storage	Yes	Yes
Grayscale Softcopy Presentation State Storage (store & forward only)	Yes	Yes
Hemodynamic Waveform Storage	Yes	Yes
Key Object Selection Document Storage	Yes	Yes
Mammography CAD SR Storage	Yes	Yes
MR Spectroscopy Storage	Yes	Yes
Pseudo-Color Softcopy Presentation State Storage	Yes	Yes
Procedure Log Storage	Yes	Yes
Raw DataStorage	Yes	Yes
Real World Value Mapping Storage	Yes	Yes
RT Beams Treatment Record Storage	Yes	Yes
RT Dose Storage	Yes	Yes
RT Ion Beams Treatment Record Storage	Yes	Yes
RT Ion Plan Storage	Yes	Yes
RT Plan Storage	Yes	Yes
RT Structure Set Storage	Yes	Yes
RT Treatment Summary Record Storage	Yes	Yes
Spatial Fiducials Storage	Yes	Yes
Spatial Registration Storage	Yes	Yes
Surface Segmentation Storage	Yes	Yes

SOP Classes	Service Class User (SCU)	Service Class Provider (SCP)
X-Ray Radiation Dose SR Storage	Yes	Yes
Transfer(Private SOP Class)		
CSA Non-Image Storage	Yes	Yes
Query / Retrieve		
Patient Root – Query/Retrieve Information Model – FIND	Yes	No
Patient Root – Query/Retrieve Information Model – MOVE	Yes	No
Study Root – Query/Retrieve Information Model – FIND	Yes	No
Study Root – Query/Retrieve Information Model – MOVE	Yes	No
Patient/Study Only – Query/Retrieve Information Model – FIND	Yes	No
Patient/Study Only – Query/Retrieve Information Model – MOVE	Yes	No
Workflow Management		
Storage Commitment Push Model	No	No
Modality Worklist Information Model – FIND	No	No
Print Management		
Basic Grayscale Print Management Meta SOP Class	No	No
Basic Film Session SOP Class	No	No
Basic Film Box SOP Class	No	No
Basic Grayscale Image Box SOP Class	No	No
Printer SOP Class	No	No
Print Job SOP Class	No	No
Presentation LUT SOP Class	No	No
Basic Color Print Management Meta SOP Class	No	No
Basic Color Image Box SOP Class	No	No

Table 0-2 Media Services

Media Storage Application Profile	Write Files (FSC)	Read Files (FSR)
Compact Disk – Recordable		
STD-GEN-CD (augmented, see 3.2.1)	No	Yes
DVD – Recordable		
STD-GEN-DVD (augmented, see 3.2.1)	No	Yes
STD-GEN-DVD-J2K (augmented, see 3.2.1)	No	Yes
USB		
STD-GEN-USB-J2K (augmented, see 3.2.1)	Yes	Yes

TABLE OF CONTENTS

CONFORMANCE STATEMENT OVERVIEW	3
TABLE OF CONTENTS	7
List of Tables	9
List of Figures	10
1 INTRODUCTION	11
1.1 REVISION HISTORY	11
1.2 GENERAL	11
1.3 AUDIENCE	11
1.4 REMARKS	11
1.5 TERMS AND DEFINITIONS	12
1.6 ABBREVIATIONS	12
1.7 REFERENCES	12
1.8 SCOPE AND FIELD OF APPLICATION	13
2 NETWORKING	14
2.1 IMPLEMENTATION MODEL	14
2.1.1 Application Data Flow	14
2.1.2 Functional Definition of AE's	14
2.1.3 Sequencing of Real-World Activities	16
2.2 AE SPECIFICATIONS	18
2.2.1 syngo.via View&GO AE	18
2.3 NETWORK INTERFACES	32
2.3.1 Physical Network Interface	32
2.3.2 Additional Protocols	32
2.3.3 IPv4 and IPv6 Support	32
2.4 CONFIGURATION	32
2.4.1 AE Title/Presentation Address Mapping	32
3 MEDIA INTERCHANGE	34
3.1 IMPLEMENTATION MODELS	34
3.1.1 Application Data Flow Diagram	34
3.1.2 Functional definitions of AEs	35
3.1.3 Sequencing of Real-World Activities	35
3.1.4 File Meta Information for Implementation Class and Version	36
3.2 AE SPECIFICATIONS	36
3.2.1 Media Storage AE – Specification	36
3.3 AUGMENTED AND PRIVATE APPLICATION PROFILES	46
3.3.1 Augmented Application Profiles	46
3.4 MEDIA CONFIGURATION	47
3.5 Attribute confidentiality profiles	47
3.5.1 De-identification	47
4 SUPPORT OF CHARACTER SETS	52
4.1 CHARACTER SETS FOR syngo.via View&GO	52

5	SECURITY	55
5.1	SECURITY PROFILES	55
5.2	ASSOCIATION LEVEL SECURITY	55
6	Annexes	56
6.1	SOP Classes supported	56
6.2	IOD CONTENTS	59
6.2.1	Created SOP Instance(s)	59
6.2.2	Data Dictionary of Private Attributes	59
6.2.3	Usage of Attributes from received IODs	60
6.2.4	Coerced / Modified fields	60
6.3	CODED TERMINOLOGY AND TEMPLATES	60
6.3.1	Context Groups	60
6.3.2	Template Specifications	60
6.3.3	Private Code definitions	61
6.4	GRAYSCALE IMAGE CONSISTENCY	61
6.5	STANDARD EXTENDED / SPECIALIZED / PRIVATE SOP CLASSES	61

List of Tables

Table 0-1 Network Services	3
Table 0-2 Media Services	6
Table 2-1: Association Policies	19
Table 2-2: Asynchronous Nature as an Association Initiator	19
Table 2-3: DICOM Implementation Class and Version	19
Table 2-4: Association initiation policies	19
Table 2-5: Acceptable Presentation Contexts for Verification Activity	20
Table 2-6: Proposed Presentation Contexts for Storage	21
Table 2-7: DICOM Command Response Status Handling Behavior	22
Table 2-8: DICOM Command Communication Failure Behavior	22
Table 2-9: Proposed Presentation Contexts for Query	24
Table 2-10: Extended Negotiation as an SCU	25
Table 2-11: DICOM Command Response Status Handling Behavior	25
Table 2-12: DICOM Command Communication Failure Behavior	25
Table 2-13: Attributes supported for instance Query - SCU	26
Table 2-14: Proposed Presentation Contexts for Retrieve and Activity "MOVE SCU"	28
Table 2-15: DICOM Command Response Status Handling Behavior	28
Table 2-16: DICOM Command Communication Failure Behavior	30
Table 2-17: Acceptable Presentation Contexts for Verification Activity	30
Table 2-18: Storage C-STORE Response Status	31
Table 3-1: Implementation Class/Version Name - Media Interchange	36
Table 3-2: Media - Application Profiles and Real-World Activities	36
Table 3-3: SOP Classes and Transfer Syntaxes for STD-GEN-DVD-J2K and STD-GEN-USB-J2K	38
Table 3-4: SOP Classes and Transfer Syntaxes for STD-GEN-CD and STD-GEN-DVD Profile	44
Table 3-5: Private SOP Classes and Transfer Syntaxes for Augmented Media Profiles	47
Table 3-6: Application Level Confidentiality Profile Attributes (standard tags)	47
Table 4-1: Single-Byte Character Sets without Code Extension	52
Table 4-2: Single-Byte Characters Sets with Code Extension	53
Table 4-3: Multi-Byte Character Sets without Code Extension	53
Table 4-4: Multi-Byte Character Sets with Code Extension	53
Table 6-1 SOP CLASSES for Storage	56
Table 6-2: Supported Non-Storage SOP Classes	58
Table 6-3: List of created SOP Classes	59
Table 6-4: Private Data Element Dictionary	59

List of Figures

Figure 1.8-1: Overview about DICOM capabilities of <i>syngo.via</i> View&GO VA10A	13
Figure 2.1-1: Application Data Flow Diagram.....	14
Figure 2.1-2: Sequence diagram – Verify	16
Figure 2.1-3: Sequence diagram – Storage	17
Figure 2.1-4: Sequence diagram – Query/Retrieve	18
Figure 3.1-1: Media Interchange Application Data Flow Diagram.....	34
Figure 3.1-2: Sequence diagram – Media creation on USB.....	35

1 INTRODUCTION

1.1 REVISION HISTORY

Version/ Status	Date of Issue	Product / Version	Author	Change & Reason of Change
2.0	2018-07-17	<i>syngo.via</i> View&GO VA10A	CT DD DS EU HU O 4 3	Release version.
1.1	2018-07-11	<i>syngo.via</i> View&GO VA10A	CT DD DS EU HU O 4 3	DICOM version set to 2016a.
1.0	2018-06-07	<i>syngo.via</i> View&GO VA10A	CT DD DS EU HU O 4 3	Release version.
0.2	2018-06-05	<i>syngo.via</i> View&GO VA10A	CT DD DS EU HU O 4 3	Draft version for <i>syngo.via</i> View&GO VA10A.
0.1	2018-06-01	<i>syngo.via</i> View&GO VA10A	CT DD DS EU HU O 4 3	Draft version for <i>syngo.via</i> View&GO VA10A.

1.2 GENERAL

The Conformance Statement describes the DICOM interface for the Siemens ***syngo.via*** **View&GO** in terms of DICOM Part PS3.2 2016a [1].

1.3 AUDIENCE

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

1.4 REMARKS

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM PS3.1-3.20 2016a Standard [1]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.

- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.

Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

1.5 TERMS AND DEFINITIONS

Terms used in this document shall be interpreted as defined in the DICOM Standard.

1.6 ABBREVIATIONS

ACR	American College of Radiology
AE	DICOM Application Entity
ASCII	American Standard Code for Information Interchange
DB	Database
DCS	DICOM Conformance Statement
DSA	Digital Subtraction Angiography
IIDC	Image-Intensifier Distortion Correction
IOD	DICOM Information Object Definition
ISO	International Standard Organization
FSC	File-set Creator
FSR	File-set Reader
FSU	File-set Updater
MWL	Modality Worklist
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
RIS	Radiology Information System
SC	Storage Commitment
SCU	DICOM Service Class User
SCP	DICOM Service Class Provider
SOP	DICOM Service-Object Pair
SCS	Specific Character Set
U	Unique Key Attribute

1.7 REFERENCES

- [1] Digital Imaging and Communications in Medicine (DICOM PS3.1-3.20 2016a), National Electrical Manufacturers Association (NEMA), <http://medical.nema.org/>
- [2] IHE Radiology Technical Framework, Vol. I – IV, http://www.ihe.net/Technical_Frameworks

1.8 SCOPE AND FIELD OF APPLICATION

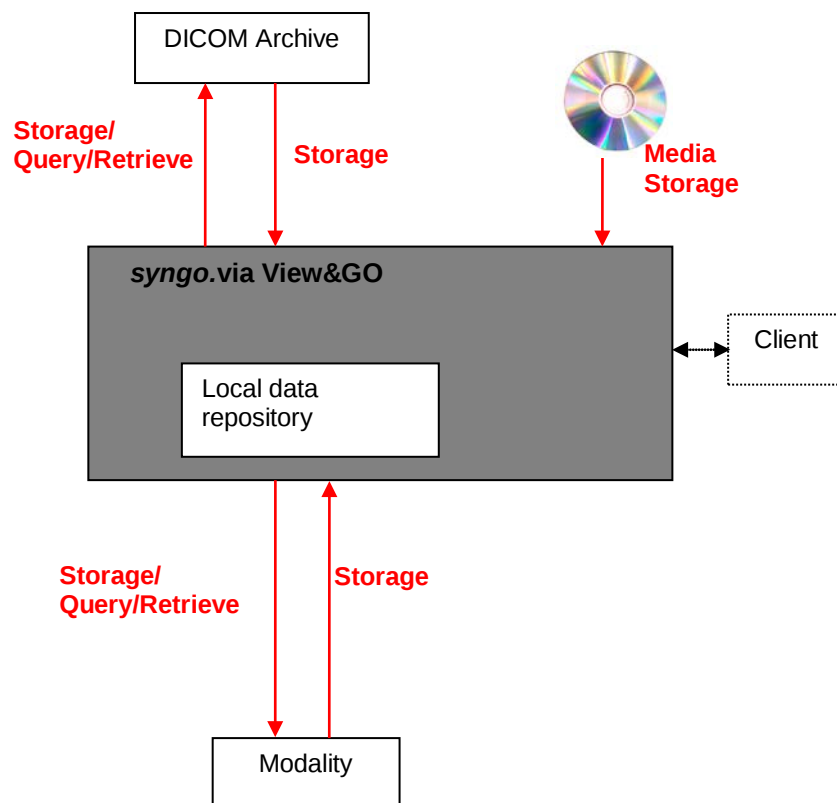


Figure 1.8-1: Overview about DICOM capabilities of *syngo.via View&GO VA10A*

2 NETWORKING

2.1 IMPLEMENTATION MODEL

2.1.1 Application Data Flow

The Application Data Flow diagram in Figure 2.1-1 depicts the DICOM data flow to and from the individual applications within **syngo.via View&GO**.

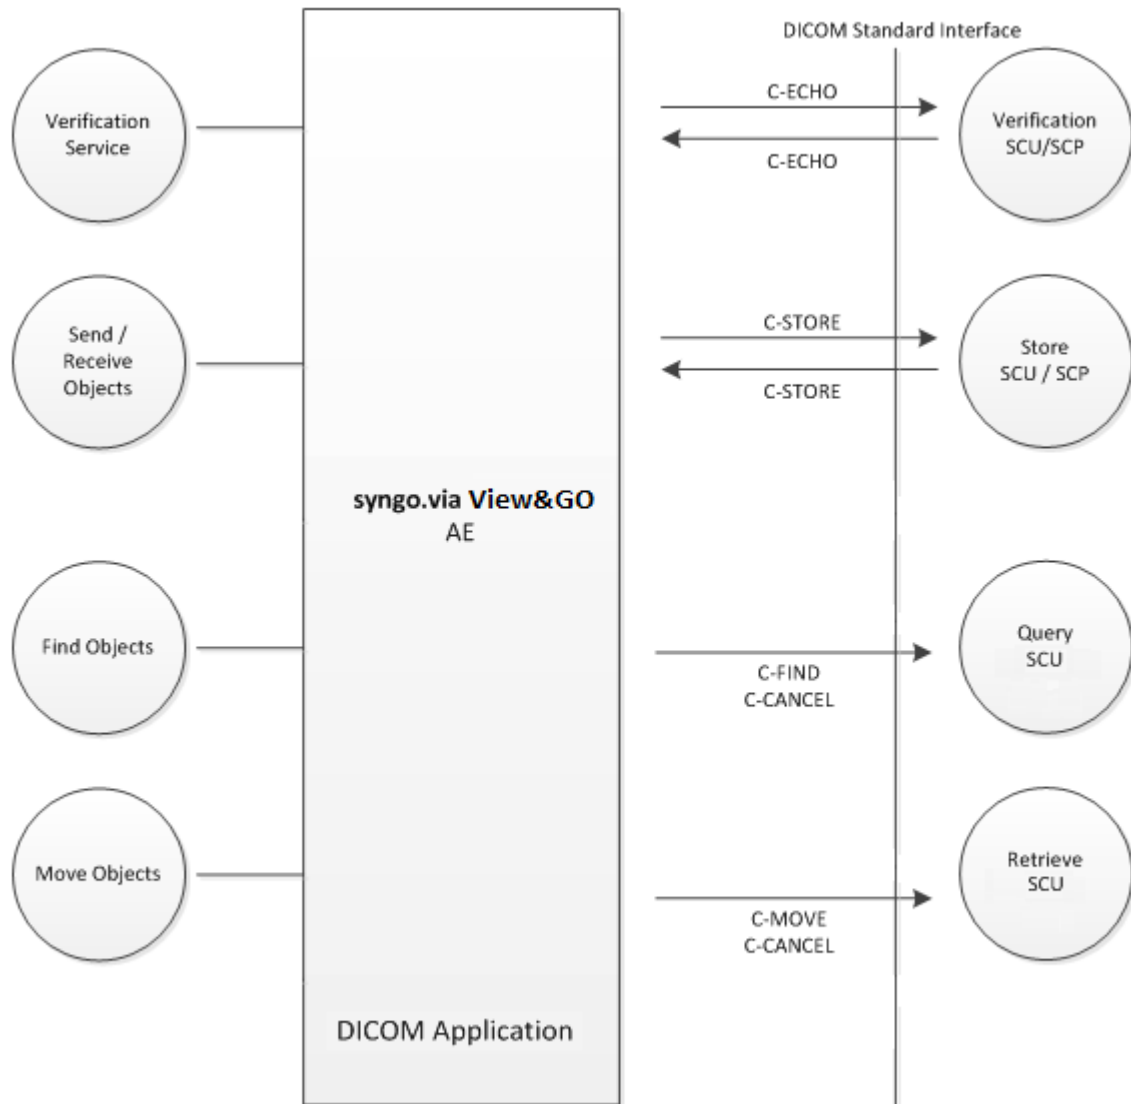


Figure 2.1-1: Application Data Flow Diagram

2.1.2 Functional Definition of AE's

The SCP components of the Application Entities of the **syngo.via View&GO** operate as background server processes. They exist as soon as the application starts and wait for association requests. Upon accepting an association with a negotiated Presentation Context they start to receive and process the requests described in the following sections.

The SCU components of the Application Entity are invoked upon requests from the user interface or indirectly triggered from internal processes.

2.1.2.1 Verification

Verification requests (SCP) will be processed and responded by the **syngo.via View&GO** AE. The **syngo.via View&GO** AE can also initiate an association and request verification to a remote AE (SCU).

2.1.2.2 Storage

The **syngo.via View&GO** Storage SCU is invoked directly by the user, or by the Query/Retrieve Application Entity that is responsible for processing retrieve requests. The request consists of data describing the composite objects selected for storage and the destination AET. An association is negotiated with the destination AE and the image data is transferred using the DIMSE C-STORE-Service.

The **syngo.via View&GO** Storage SCP starts to receive the Composite Image Objects and import them into the database after accepting an association with a negotiated Presentation Context. The system responses to the Storage Request immediately after reception of the Data.

2.1.2.3 Storage Commitment

The **syngo.via View&GO** does not support Storage Commitment.

2.1.2.4 Query

The C-FIND request to the remote SCP is invoked directly by the user. The remote SCP returns a list of responses with matching the request which are displayed to the user. The user can decide to start retrieving any of the responses or to issue another query.

As an SCU **syngo.via View&GO** supports

- Study Root Query/Retrieve Information Model (FIND)
- Patient Root Query/Retrieve Information Model (FIND)
- Patient/Study Only Query/Retrieve Information Model (FIND)
- Furthermore the SCU services may issue relational queries, if supported by the SCP node and required by the querying Application.

2.1.2.5 Retrieve

The **syngo.via View&GO** initiates a C-MOVE request to the remote Retrieve SCP. The remote Retrieve SCP in turn starts C-STORE sub operations to the **syngo.via View&GO** Storage SCP.

As an SCP **syngo.via View&GO** supports

- Study Root Query/Retrieve Information Model (MOVE,GET)
- Patient Root Query/Retrieve Information Model (MOVE,GET)
- Patient/Study Only Query/Retrieve Information Model (MOVE,GET)

2.1.3 Sequencing of Real-World Activities

Verify:

The communication between **syngo.via View&GO** and an external DICOM node in case of Verify is depicted in Figure 2.1-2 in more detail.

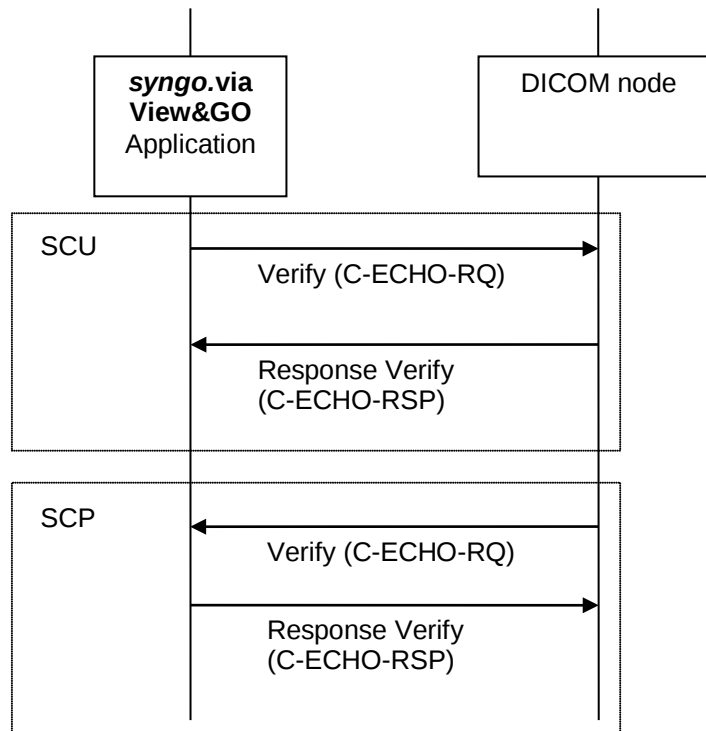


Figure 2.1-2: Sequence diagram – Verify

Storage:

The communication between **syngo.via View&GO** and an external DICOM node in case of triggering the transfer or accepting storage requests is depicted in more detail.

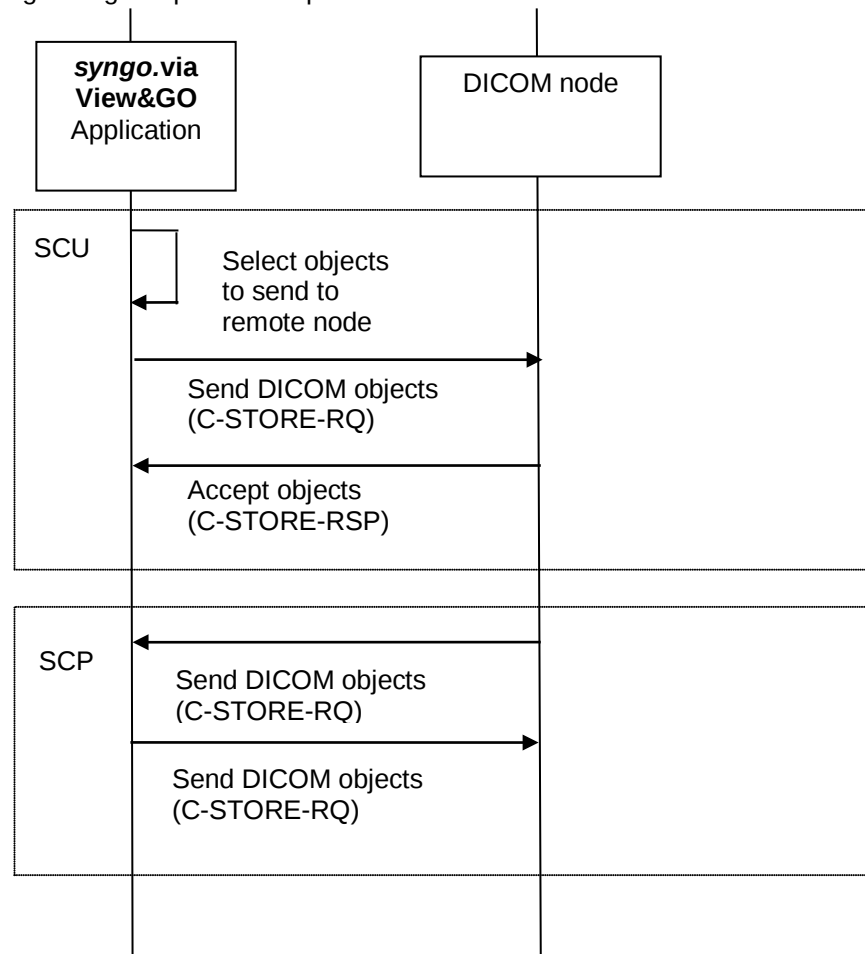


Figure 2.1-3: Sequence diagram – Storage

Query and Retrieval:

The communication between **syngo.via View&GO** and an external DICOM node in case of querying of objects from a remote DICOM node and retrieval to **syngo.via View&GO** is depicted in Figure 2.1-4 in more detail.

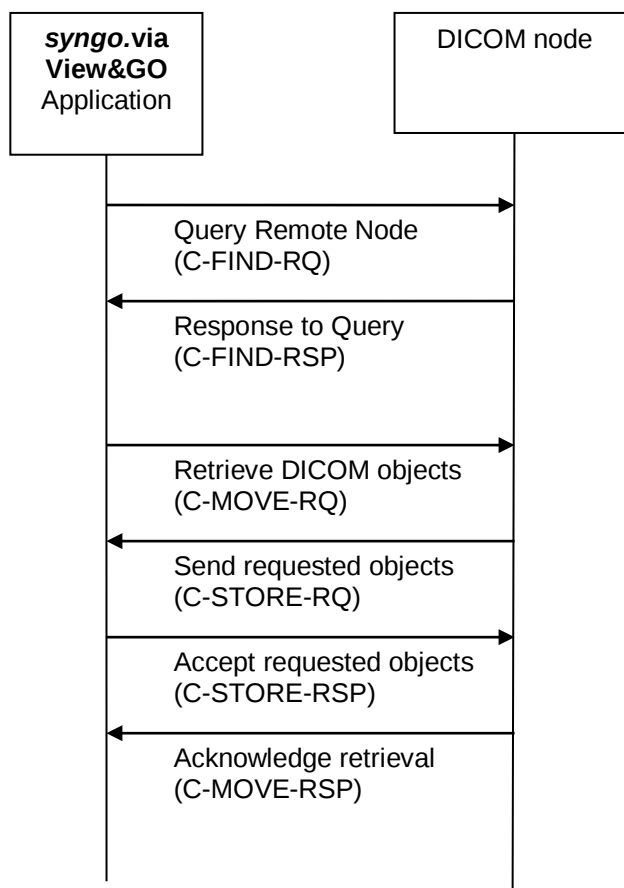


Figure 2.1-4: Sequence diagram – Query/Retrieve

2.2 AE SPECIFICATIONS

This section outlines the specifications for each of the Application Entities that are part of the **syngo.via View&GO** solution.

2.2.1 syngo.via View&GO AE

2.2.1.1 SOP Classes supported

This Application Entity provides Standard Conformance to the SOP Classes listed in Table 6-1 SOP CLASSES and

Table 6-2: Supported Non-Storage SOP Classes.

2.2.1.2 Association Establishment Policies

Table 2-1: Association Policies

Application Context Name	1.2.840.10008.3.1.1.1
PDU size	32 kB ¹
Maximum number of simultaneous associations as an association acceptor	12 ¹
Maximum number of simultaneous associations as an association initiator	unlimited

The **syngo.via View&GO** AE contains a limitation of 512 kB for the maximum PDU size. By default, the maximum PDU size is set to 32kB.

The maximum number of simultaneous receiving associations (SCP) is configurable at run time, based on the system resources available. By default, the maximum number of associations is set to 12.

There is no inherent limit to the number of outgoing associations (SCU), other than limits imposed by the computer operating system. Nevertheless, transfer jobs to one distinct remote system (Send, Retrieve) will be run sequentially one after the other.

2.2.1.2.1 Asynchronous Nature

The **syngo.via View&GO** supports asynchronous communication (multiple outstanding transactions over a single association). On the SCU side the Window size proposed is infinite. On the SCP Side any non-infinite maximum size will be accepted.

Table 2-2: Asynchronous Nature as an Association Initiator

Maximum number of outstanding asynchronous transactions	Infinite
---	----------

2.2.1.2.2 Implementation Identifying Information

Table 2-3: DICOM Implementation Class and Version

Implementation Class UID	1.3.12.2.1107.5.8.15.10.20090701
Implementation Version Name	syngo.ViewAndGO

2.2.1.3 Association Initiation Policy

syngo.via View&GO initiates associations while processing the service operations and internal messages as shown below:

Table 2-4: Association initiation policies

Operation or Real-World Activity	Association for
Verification	C-ECHO
Send / Receive Instance	C-STORE
Querying a remote node	C-FIND
Retrieval of Instances	C-MOVE

¹ Default, the value is configurable

2.2.1.3.1

2.2.1.3.2 Activity "Verification"

2.2.1.3.2.1 Description and Sequencing of Activities

The **syngo.via View&GO** verification process will accept an association, send ECHO request and receive reply.

2.2.1.3.2.2 Accepted Presentation Contexts

Table 2-5: Acceptable Presentation Contexts for Verification Activity

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

2.2.1.3.2.3 SOP specific Conformance for SOP classes

syngo.via View&GO provides standard conformance to the Verification service SCU.

2.2.1.3.3 Activity "Send To"

2.2.1.3.3.1 Description and Sequencing of Activities

Storage of DICOM object is triggered internally in the **syngo.via View&GO**.

If an association to a remote Application Entity could successfully be established, each image will be transferred one after another via the same open association.

In case the transfer fails for a permanent reason (rejection permanent reported by SCP, all Presentation Contexts refused, ...) the transfer will not be retried.

2.2.1.3.3.2 Proposed Presentation Contexts

For all supported Transfer objects (see SOP Classes in Table 6-1) the following Transfer Syntaxes are supported:

Table 2-6: Proposed Presentation Contexts for Storage

UID value	Transfer Syntax	Type
1.2.840.10008.1.2.1	Explicit Value Representation Little Endian native	Image / non-image
1.2.840.10008.1.2	Implicit Value Representation Little Endian native	Image / non-image
1.2.840.10008.1.2.4.70	JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14) lossless compressed	Image
1.2.840.10008.1.2.4.90	JPEG 2000 Image Compression (Lossless Only) compressed	Image
1.2.840.10008.1.2.5	RLE Lossless compressed	Image
1.2.840.10008.1.2.4.51	JPEG Extended (Process 2 & 4) lossy compressed	Image
1.2.840.10008.1.2.4.50	JPEG Baseline (Process 1) lossy compressed	Image
1.2.840.10008.1.2.4.91	JPEG 2000 Image Compression lossy compressed	Image

Storage SCU Service will choose a compressed or uncompressed Transfer Syntax among those accepted by the SCP for images.

An instance will be JPEG lossless compressed only if it fulfills the following criteria:

- is an image and not already compressed
- Photometric Interpretation (0028,0004) is MONOCHROME or RGB or YBR_FULL or YBR_FULL_422
- Bits Allocated (0028,0100) equal to 16'D or 8'D
- Bits Stored (0028,0101) is >8
- High Bit (0028,0102) equal to Bits Stored (0028,0101) - 1
- Pixel Representation (0028,0103) equal to 0'D

An instance will be JPEG lossy compressed only if it fulfills the following criteria:

- is an image and not already compressed
- photometric interpretation (0028,0004) is MONOCHROME or RGB
- Bits Allocated (0028,0100) equal to 16'D or 8'D
- Bits Stored (0028,0101) equal to 12'D or 8'D
- High Bit (0028,0102) equal to Bits Stored (0028,0101) - 1
- Pixel Representation (0028,0103) equal to 0'D

An instance will be JPEG 2000 lossless compressed only if it fulfills the following criteria:

- is an image and not already compressed
- Photometric interpretation (0028,0004) not MONOCHROME or RGB or YBR_FULL or YBR_FULL_422
- Bits Allocated (0028,0100) not 16'D or 8'D

An instance will be JPEG 2000 lossy compressed only if it fulfills the following criteria:

- is an image and not already compressed
- Photometric interpretation (0028,0004) is MONOCHROME or RGB
- Bits Stored (0028,0101) equal to 12'D or 8'D

There is no extended negotiation as an SCU.

2.2.1.3.3.3 SOP specific Conformance for SOP classes

The **syngo.via View&GO** will not add or change private attributes by default, even in case objects are compressed or image header is updated according to IHE [2] Patient Information Reconciliation. The behavior of **syngo.via View&GO** when encountering status codes in a C-STORE response is summarized in Table 2-7:

Table 2-7: DICOM Command Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Error	Duplicate SOP Instance UID: some of the instances sent to the SCP were already available there.	0111	Job is continued till the end.
Error	Out-Of-Resources: The remote node has run out of resources (storage resources for example)	A7XX	Job is continued till the end. The result can be checked by checking the availability of the data on the target node.
Error	Any other DIMSE Error Status	XXXX	Job is continued till the end. Error is logged in the system log.
Error	Sending partially or completely failed	Any none null Code	User does not get notified. The result can be checked by checking the availability of the data on the target node.
Success	Image is successfully stored on file system.	0000	User does not get notified. The result can be checked by checking the availability of the data on the target node.

Table 2-8: DICOM Command Communication Failure Behavior

Exception	Behavior
Timeout	User does not get notified. The result can be checked by checking the availability of the data on the target node.
Association Aborted	User does not get notified. The result can be checked by checking the availability of the data on the target node.

2.2.1.3.3.4 CT Derived object for LungCAD findings generated by **syngo.via View&GO**

Attribute	Tag	Type	Description
Specific Character Set	(0008, 0005)	1C	Copied from Input Image
Image Type	(0008,0008)	1	Value 1: DERIVED Value 2: SECONDARY Value 3: AXIAL Value 4: AlgorithmName_AlgorithmVersion_DO

Attribute	Tag	Type	Description
Instance Creation Date	(0008,0012)	3	DO ¹ instance creation date
Instance Creation Time	(0008,0013)	3	DO ¹ instance creation time
SOP Class UID	(0008,0016)	1	Copied from Input Image
SOP Instance UID	(0008,0018)	1	1.3.12.2.1107.5.99.3.99.UID ²
Study Date	(0008,0020)	2	Copied from Input Image
Series Date	(0008,0021)	3	Creation Date of the DO ¹ in <YYYYMMDD> format
Acquisition Date	(0008,0022)	3	Copied from Input Image
Study Time	(0008,0030)	2	Copied from Input Image
Series Time	(0008,0031)	3	Creation Time of the DO ¹ in <HHMMSS> format
Acquisition Time	(0008,0032)	3	Copied from Input Image
Accession Number	(0008,0050)	2	Copied from Input Image
Modality	(0008,0060)	1	Copied from Input Image
Manufacturer	(0008,0070)	2	Copied from Input Image
Institution Name	(0008,0080)	3	Copied from Input Image
Referring Physician's Name	(0008,0090)	2	Copied from Input Image
Study Description	(0008,1030)	3	Copied from Input Image
Series Description	(0008,103E)	3	Series description as configured by the application
Name Of Physician(s) Reading Study	(0008,1060)	3	Copied from Input Image
Manufacturer's Model Name	(0008,1090)	3	Copied from Input Image
Derivation description	(0008,2111)	3	Set AlgorithmName_AlgorithmVersion_DO value. For example: LUNGCAD_VD10C_DO)
Source Image Sequence	(0008,2112)	3	Set input image SOP class UID and input image SOP instance UID from original image
>Reference SOP Class UID	(0008,1150)		From original image's SOP Class UID
>Reference SOP Instance UID	(0008,1155)		From original image's SOP Instance UID
Patient Name	(0010,0010)	2	Copied from Input Image
Patient ID	(0010,0020)	2	Copied from Input Image
Patient's Birth Date	(0010,0030)	2	Copied from Input Image
Patient's Sex	(0010,0040)	2	Copied from Input Image
Patient's Size	(0010,1020)	3	Copied from Input Image
Patient's Weight	(0010,1030)	3	Copied from Input Image
Pregnancy Status	(0010,21C0)	3	Copied from Input Image
Imager Pixel Spacing	(0018,1164)	3	Copied from Input Image
Patient Position	(0018,5100)	2C	Copied from Input Image
View Position	(0018,5101)	3	Copied from Input Image
Detector Element Physical Size	(0018,7020)	3	Copied from Input Image
Detector Element Spacing	(0018,7022)	3	Copied from Input Image
Study Instance UID	(0020,000D)	1	Copied from Input Image
Series Instance UID	(0020,000E)	1	1.3.12.2.1107.5.99.3.99.UID ²
Study ID	(0020,0010)	2	Copied from Input Image
Series Number	(0020,0011)	2	Series Number as configured by the user

Attribute	Tag	Type	Description
Patient Orientation	(0020,0020)	2	Copied from Input Image
Image Laterality	(0020,0062)	1	Copied from Input Image
Samples PerPixel	(0028,0002)	1	Copied from input image
Photometric Interpretation	(0028,0004)	1	Copied from input image
Rows	(0028,0010)	1	Copied from input image
Columns	(0028,0011)	1	Copied from input image
Pixel Spacing	(0028,0030)	1	Copied from input image
Bits Allocated	(0028,0100)	1	Copied from input image
Bits Stored	(0028,0101)	1	Copied from input image
High Bit	(0028,0102)	1	Copied from input image
Pixel Representation	(0028,0103)	1	Copied from input image
Window Center	(0028,1050)	1	Copied from Input Image
Window Width	(0028,1051)	1	Copied from Input Image
Rescale Intercept	(0028,1052)	1	Copied from input image
Rescale Slope	(0028,1053)	1	Copied from input image
Rescale Type	(0028,1054)	1	Copied from input image
Presentation Creator's Name	(0070,0084)	2	Algorithm Name_Version_DO ¹
Study Comments	(0032,4000)	3	Copied from input image
Pixel Data	(7FE0,0010)	1	Sets the Derived Pixel data

1 – Derived Object

2 – UID generated by syngo.via
View@GO

2.2.1.3.4 Activity “Querying a Remote Node” for Instances

2.2.1.3.4.1 Description and Sequencing of Activities

The associated Real-World activity is a C-Find request initiated by the user (see also Figure 2.1-4). The user specifies some attributes and will send a C-Find request (according to the query model) and will then return the results to the initiating application.

2.2.1.3.4.2 Proposed Presentation Contexts

The **syngo.via View&GO** will propose Presentation Contexts as shown in the following table:

Table 2-9: Proposed Presentation Contexts for Query

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	Yes
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/	1.2.840.10008.5.1.4.1.	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	Yes

Retrieve Information Model – FIND	2.2.1	Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only Query/ Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	No
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 2-10: Extended Negotiation as an SCU

Name	UID	Extended Negotiation
Patient Root Query/Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Relational Query will be negotiated as defined in DICOM PS3.4 2016a.
Study Root Query/ Retrieve Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Relational Query will be negotiated as defined in DICOM PS3.4 2016a.

2.2.1.3.4.3 SOP Specific Conformance Statement to Query SOP classes

The **syngo.via View&GO** checks for the following status codes in the Query SCP's C-FIND-Response:

Table 2-11: DICOM Command Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Failure	e.g. Out of Resources; Cancellation; Identifier does not match SOP Class; Unable to process	Any none null Code	Failure reported to user
Pending	All optional keys are supported the same manner as Required Keys.	FF00	Pending state is indicated to user
	Matching Operation continues; some of the optional keys were not supported the same way as the required keys	FF01	Pending state is indicated to user
Success	Query has been performed successfully.	0000	Success reported to user

Table 2-12: DICOM Command Communication Failure Behavior

exception	Behavior
Timeout	Failure reported to user (Timeout configurable; default 30s)
Association Aborted	Failure reported to user

The **syngo.via View&GO** supports the following query levels:

- Study
- Series

Matching Keys on Instance Level is not supported by **syngo.via View&GO** as SCU.

The following table lists the various attributes at Study and Series levels, which can be used for **hierarchical** queries as well as return values for display. The display capabilities are highly configurable and “yes” indicates that it is possible to configure display of the data:
A “yes” in the **UI** column will indicate that the attribute may be visualized when browsing the Query results with the Browser. The Browser display is additionally influenced by the related Browser configuration

Table 2-13: Attributes supported for instance Query - SCU

Attribute Name	Tag	Type	User input	UI
Study Level				
Patient's Name	(0010,0010)	O	enter value	yes
Patient ID	(0010,0020)	O	enter value	yes
Issuer of Patient ID	(0010,0021)	O	enter value	yes
Patient's Birth Date	(0010,0030)	O	enter value	yes
Patient's Birth Time	(0010,0032)	O	enter value	yes
Patient's Sex	(0010,0040)	O	enter value	yes
Accession Number	(0008,0050)	O	enter value	yes
Study ID	(0020,0010)	O	enter value	yes
Study Instance UID	(0020,000D)	U	enter value	yes
Study Date	(0008,0020)	O	enter value	yes
Study Time	(0008,0030)	O	enter value	yes
Referring Physician' s Name	(0008,0090)	O	enter value	yes
Study Description	(0008,1030)	O	enter value	yes
Number of Study related Instances	(0020,1208)	O	-	yes
Modalities in Study	(0008,0061)	O	enter value	yes
Number of Study Related Series	(0020,1206)	O	-	yes
Series Level				
Modality	(0008,0060)	O	enter value	yes
Series Date	(0008,0021)	O	enter value	yes
Series Time	(0008,0031)	O	enter value	yes
Number of Series related Instances	(0020,1209)	O	-	yes
Series Number	(0020,0011)	O	enter value	yes
Series Description	(0008,103E)	O	enter value	yes
Request Attributes Sequence \ Requested Procedure ID	(0040,0275) \ (0040,1001)	O	enter value	yes
Request Attributes Sequence \ Scheduled Procedure Step ID	(0040,0275) \ (0040,0009)	O	enter value	yes
Performed Procedure Step Start Date	(0040,0244)	O	enter value	yes
Performed Procedure Step Start Time	(0040,0245)	O	enter value	yes

Attribute Name	Tag	Type	User input	UI
Series Instance UID	(0020,000E)	U	-	yes

2.2.1.3.5 Activity Retrieving Instances from a remote node

2.2.1.3.5.1 Description and Sequencing of Activities

The C-MOVE-RQs are used to retrieve the referenced images. The Retrieve AE supports the query model Study Root.

2.2.1.3.5.2 Accepted Presentation Contexts

Table 2-14: Proposed Presentation Contexts for Retrieve and Activity “MOVE SCU”

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	No
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	No
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	No
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

2.2.1.3.5.3 SOP Specific Conformance Statement for Move SCU Classes

At association establishment time the C-MOVE presentation context shall be negotiated. When the C-MOVE-RQ is processed, the Move Destination attribute (receiver of images) is ignored. However the Move Destination AE must conform to the DICOM conventions (value representation AE).

The behavior of **syngo.via View&GO** when encountering status codes in a C-MOVE response is summarized in Table 2-15:

Table 2-15: DICOM Command Response Status Handling Behavior

Service Status	Further Meaning	Error Code	Behavior
Error	e.g. Out of Resources; Cancellation; Identifier does not match SOP Class; Unable to process; Move destination unknown	Any non null Code	Failure reported to user
Pending	Move Operation continues	FF00	Operation continues in

			background
Success	Move has been performed successfully.	0000	Success reported to user

Table 2-16: DICOM Command Communication Failure Behavior

exception	Behavior
Timeout	Failure reported to user (Timeout configurable; default 30s)
Association Aborted	Failure reported to user

2.2.1.4 Association Acceptance Policy

The **syngo.via View&GO** attempts to accept a new association for

- DIMSE C-STORE
service operations.

Generally associations are accepted if all of the following conditions are true:

- The "called AET" matches one of the configured Application Entity Titles of the **syngo.via View&GO**.
- The "calling AET" is known (configured) at **syngo.via View&GO**.
- The maximum number of incoming associations is not reached.
- At least one Presentation Context with a minimum of one suitable transfer syntax has been proposed as defined by the "Presentation Context Tables" in the following subsections.
- The system has enough available resources to perform the service requested (e.g. enough free disk space, less than the max. number of associations are already in use)

2.2.1.4.1 Activity "Verification"

2.2.1.4.1.1 Description and Sequencing of Activities

The **syngo.via View&GO** verification process will accept an association, receive ECHO request and send reply.

2.2.1.4.1.2 Accepted Presentation Contexts

Table 2-17: Acceptable Presentation Contexts for Verification Activity

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

2.2.1.4.1.3 SOP specific Conformance for SOP classes

syngo.via View&GO provides standard conformance to the Verification service SCP.

2.2.1.4.2 Activity “Receive Instances”

2.2.1.4.2.1 Description and Sequencing of Activities

The **syngo.via View&GO** receiving process will accept C-STORE association requests, receive any objects transmitted on that association and store the objects on disk.

2.2.1.4.2.2 Accepted Presentation Contexts

For all supported Transfer objects (see SOP Classes in Table 6-1) the Transfer Syntaxes described in Table 2-6 are supported.

Generally all Presentation Contexts are accepted as long as they contain at least one suitable Transfer Syntax. All other Presentation Contexts are rejected.

There is no Extended Negotiation as an SCP

2.2.1.4.2.3 SOP-specific Conformance Statement for Storage SOP classes

The **syngo.via View&GO** conforms to the Full Storage Class at Level 2.

In case of a successful C-STORE operation, the image has successfully been written on disk either in Explicit Little Endian format or in the compression format received.

syngo.via View&GO AE returns the status “success” when the data is stored to disk and a minimal image header validation has been performed.

The following header attributes must be available and filled:

- SOP Class UID,
- Study Instance UID,
- Series Instance UID and
- SOP Instance UID.

Table 2-18: Storage C-STORE Response Status

Service Status	Further Meaning	Error Code	Reason
Success	success	0000	Image received correctly
Failure	Out-of-resource	A700	No resource left in the Short Term Storage
Failure	Unable to Process	Cxxx	Error during instance reception

Failure	Data set does not match SOP Class	A9xx	The data set is not conform to the SOP Class contained in the resource.
---------	-----------------------------------	------	---

Restriction: successful operation does not guarantee storage of header data in the database.

2.2.1.4.2.4 Other SOP specific behavior

- If an image is received that is already stored in the database - identified by the SOP Instance UID - the new image will be ignored. The existing instance is not superseded.

2.3 NETWORK INTERFACES

2.3.1 Physical Network Interface

The **syngo.via View&GO** provides DICOM 3.0 TCP/IP network communication support as defined in Part 8 of DICOM [1]. The network communication is independent from the physical medium over which TCP/IP executes; it inherits this from the Windows OS system upon which it executes.

2.3.2 Additional Protocols

none

2.3.3 IPv4 and IPv6 Support

IPv4 and IPv6 are supported. Regarding IPv6 please note, that the complete networking infrastructure in the hospital (firewalls, DNS-Servers, ...) must support IPv6 in order to get a functioning communication.

2.4 CONFIGURATION

2.4.1 AE Title/Presentation Address Mapping

AE Titles shall be unique within the hospital. A common way to achieve that is to use the hostname as part of the AE Titles. The string can be up to 16 characters and must not contain any extended characters. Only 7-bit ASCII characters (excluding Control Characters) are allowed according to DICOM [1].

2.4.1.1 Local AE Titles

The **syngo.via View&GO** allows to configure AETitles, Ports any way. Default delivery is that all services are using the same AE title and only one port number.

Parameter	Configurable	Default Value
Default AE title	Yes	hostname in uppercase characters; limited to 16 characters
Default Port	Yes	104

2.4.1.2 Remote AE Title/Presentation Address Mapping

2.4.1.2.1 Remote Association Initiators

All relevant remote applications that may setup DICOM associations towards **syngo.via View&GO** need to be configured in **syngo.via View&GO**, before the association can be established. This behavior is configurable but it is recommended, not to change this behavior.

The mapping of external AE Titles to TCP/IP addresses and ports is configurable. The Application Entity Titles and supported transfer syntaxes need to be known for configuration.

To enable a fast and efficient configuration possibility Siemens will deliver templates for known configuration examples, so that the behavior (usage of one AE title, default port numbers, supported services) is determined already through the template.

Remote Application Entities can be configured without restarting the process.

2.4.1.2.2 Remote SCP's

For remote applications that shall be able to accept DICOM associations from **syngo.via View&GO**, the following information needs to be available:

- Application Entity Title
- Host Name / IP address on which the remote application service runs
- Port number on which the remote application accepts association requests.

The remote system will be indicated in the UI of **syngo.via View&GO** with a logical name that is also entered when configuring the node in the configuration UI.

To enable a fast and efficient configuration possibility Siemens will deliver templates for known configuration examples, so that the behavior (usage of one AE title, default port numbers, supported services) is determined already through the template.

Remote Application Entities can be configured without restarting the process.

3 MEDIA INTERCHANGE

3.1 IMPLEMENTATION MODELS

3.1.1 Application Data Flow Diagram

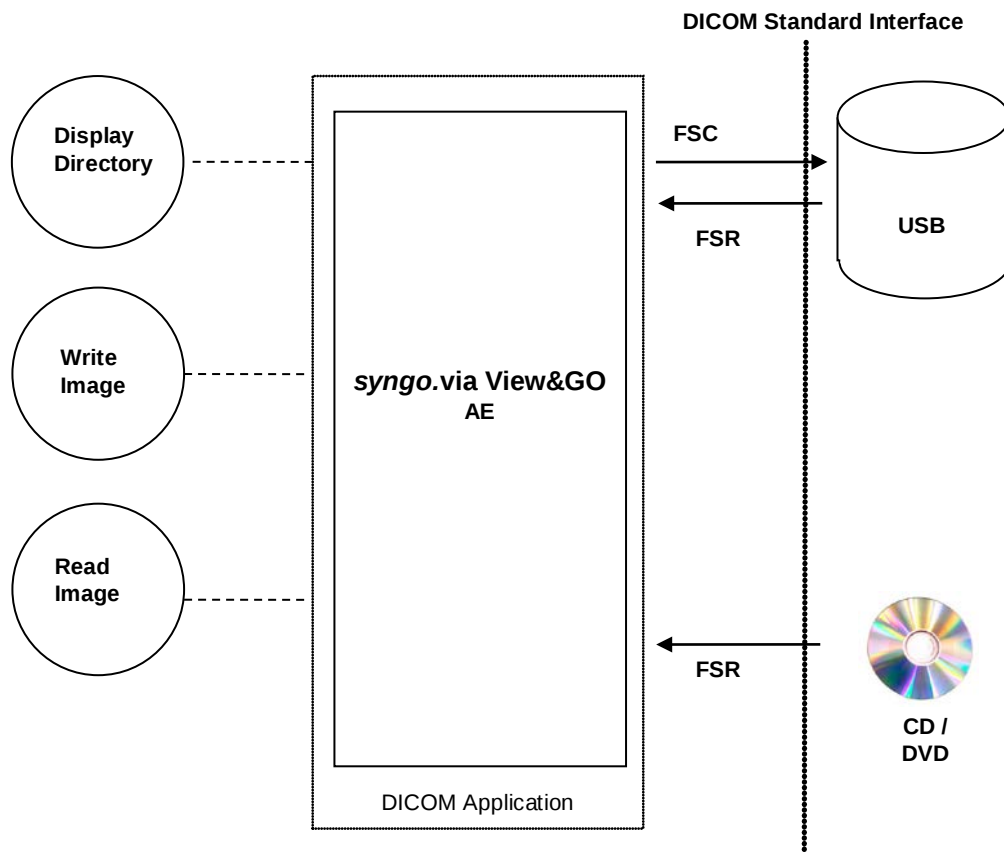


Figure 3.1-1: Media Interchange Application Data Flow Diagram

The **syngo.via View&GO** provides the functionality to Import or Export DICOM Instances from and to the File System. During export, a DICOMDIR may also be generated (user selection). All SOP Classes defined in Table 3-3 and Table 3-4 are supported for the Import/Export functionality.

3.1.2 Functional definitions of AEs

The **syngo.via View&GO** application is capable of

- creating a new File-set in the File System (Export to ...)
- importing SOP Instances from the medium onto local storage
- writing the File-sets DICOMDIR information into the file system

3.1.3 Sequencing of Real-World Activities

Whenever data is written to an external media, **syngo.via View&GO** a DICOMDIR may be created for the selected data.

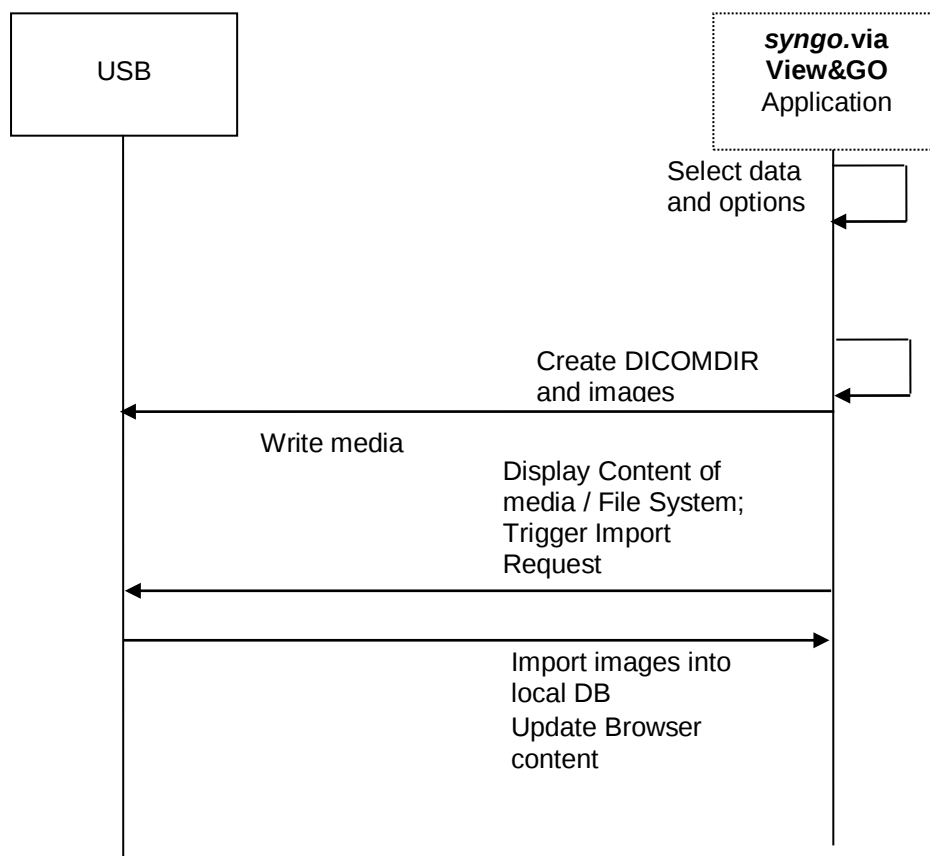


Figure 3.1-2: Sequence diagram – Media creation on USB

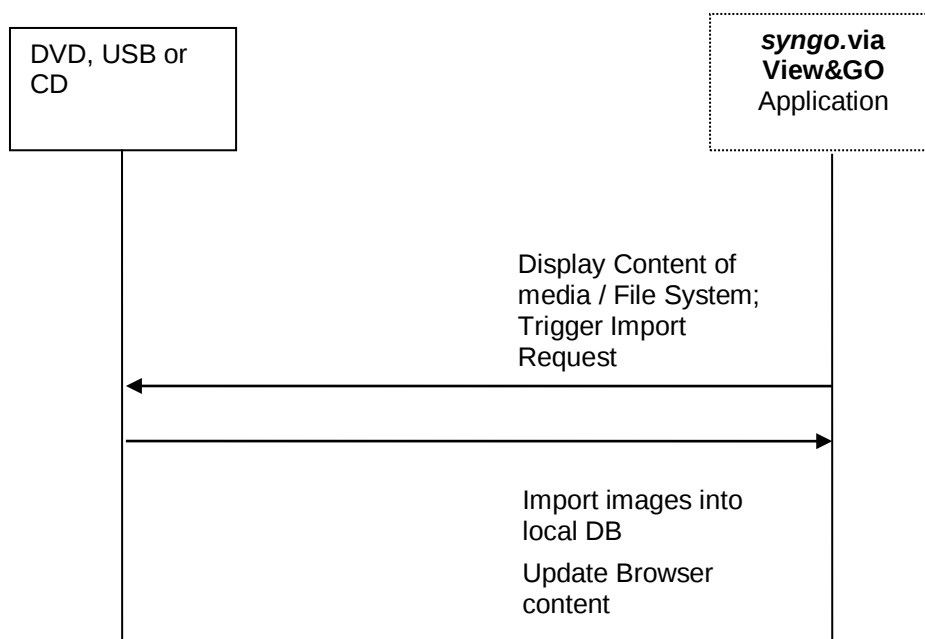


Figure 5.1-3: Sequence diagram – Media import

3.1.4 File Meta Information for Implementation Class and Version

This section describes the values assigned to the File Meta Information attributes (see DICOM [1] part PS 3.10) that pertain to the Implementation Class and Version. The implementation Class UID and the Implementation Version name in the File Meta Header are the same as the values specified for networking.

Table 3-1: Implementation Class/Version Name - Media Interchange

File Meta Information Version	0001
Implementation Class UID	1.3.12.2.1107.5.8.15.10.20090701
Implementation Version Name	syngo.ViewAndGO

3.2 AE SPECIFICATIONS

3.2.1 Media Storage AE – Specification

The **syngo.via View&GO** provides conformance to the following Application Profiles as an FSR. FSC and FSU are supported only on a non-optical storage device (e.g. USB stick).

In addition augmented conformance is provided to store extra data attributes important for the full feature support of the **syngo®**-based products. Details are listed below:

Table 3-2: Media - Application Profiles and Real-World Activities

Application Profiles Supported	Real-World Activity	Role	Service Class Option
--------------------------------	---------------------	------	----------------------

Application Profiles Supported	Real-World Activity	Role	Service Class Option
AUG-GEN-CD	Browse Directory Information Import into Application	FSR	Interchange
AUG-GEN-DVD			
AUG- GEN-DVD-J2K			
AUG- GEN-USB-J2K	Browse Directory Information Import into Application Export to local Archive Media	FSR , FSC , FSU	
STD-GEN-CD	Browse Directory Information Import into Application	FSR	Interchange
STD-GEN-DVD			
STD-GEN-DVD-J2K			
STD-GEN-USB-J2K	Browse Directory Information Import into Application Export to local Archive Media	FSR , FSC , FSU	

3.2.1.1 Real-World Activities

3.2.1.1.1 Activity “Browse Directory Information”

The **syngo.via View&GO** acts as FSR using the interchange option when requested to read the media directory.

The **syngo.via View&GO** will read the DICOMDIR and insert those directory entries that are valid for the application profiles supported, into a local database. The database then is used for browsing media contents.

Note: The “Icon Image Sequence” is also supported in DICOMDIR. But only those Icon Images with “Bits Allocated” (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

3.2.1.1.1.1 Media Storage Application Profiles

See Table 3-2 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information

3.2.1.1.2 Activity “Import into Application”

The **syngo.via View&GO** application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the application.

The SOP Instance selected from the media directory will be copied into the running Application. Only SOP Instances, that are valid for the application profile supported and supported by **syngo.via View&GO** (see Table 6-1), can be retrieved from media.

3.2.1.1.3 Media Storage Application Profiles

See Table 3-2 for the Application Profiles listed that invoke this Application Entity for the local Archive Media Real-World Activity.

3.2.1.2 SOP Classes and Transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option. In the table below (Table 3-3) the Transfer Syntax UID “RLE Lossless” only applies for decompression.

Table 3-3: SOP Classes and Transfer Syntaxes for STD-GEN-DVD-J2K and STD-GEN-USB-J2K

Information Object Definition	SOP Class UID	Transfer Syntax UID
Basic Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Color Softcopy Presentation State Storage (store & forward only)	1.2.840.10008.5.1.4.1.1.11.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CR Image Storage	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91

Information Object Definition	SOP Class UID	Transfer Syntax UID
Digital X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Digital Mammography X-Ray Image Storage- For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
Digital Mammography X-Ray Image Storage- For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Enhanced MR Color Image Storage	1.2.840.10008.5.1.4.1.1.4.3	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90

Information Object Definition	SOP Class UID	Transfer Syntax UID
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced XA Image Storage	1.2.840.10008.5.1.4.1.1.12.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Enhanced XRF Image Storage	1.2.840.10008.5.1.4.1.1.12.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
General ECG Waveform	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Grayscale Softcopy Presentation State	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Multi-frame Grayscale Byte SC Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Multi-frame Grayscale Word SC Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1)

Information Object Definition	SOP Class UID	Transfer Syntax UID
		1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended)
		1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless
		1.2.840.10008.1.2.5
Multi-frame Single Bit SC Image Storage	1.2.840.10008.5.1.4.1.1.7.1	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed
		1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1)
		1.2.840.10008.1.2.4.70
Multi-frame True Color SC Image Storage	1.2.840.10008.5.1.4.1.1.7.4	JPEG Lossy (baseline or extended)
		1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless
		1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed
		1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1)
		1.2.840.10008.1.2.4.70
		RLE Lossless
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	1.2.840.10008.1.2.1
		Explicit VR Little Endian Uncompressed
		1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1)
Pseudo-Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	1.2.840.10008.1.2.4.70
		RLE Lossless
		1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Raw DataStorage	1.2.840.10008.5.1.4.1.1.66	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed
		1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1)
		1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended)
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless
		1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91

Information Object Definition	SOP Class UID	Transfer Syntax UID
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50
		1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70

Information Object Definition	SOP Class UID	Transfer Syntax UID
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51

Information Object Definition	SOP Class UID	Transfer Syntax UID
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Ultrasound Multi-frame Storage (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
Ultrasound Multi-frame Image storage	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91
X-Ray Radiation Dose Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70
		Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
		JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51
		RLE Lossless 1.2.840.10008.1.2.5
		JPEG 2000 Lossless 1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy 1.2.840.10008.1.2.4.91

Table 3-4: SOP Classes and Transfer Syntaxes for STD-GEN-CD and STD-GEN-DVD Profile

Information Object Definition	SOP Class UID	Transfer Syntax UID
Basic Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definition	SOP Class UID	Transfer Syntax UID
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Color Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Digital X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Digital X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Digital Mammography X-Ray Image Storage- For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Digital Mammography X-Ray Image Storage- For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced MR Color Image Storage	1.2.840.10008.5.1.4.1.1.4.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced XA Image Storage	1.2.840.10008.5.1.4.1.1.12.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced XRF Image Storage	1.2.840.10008.5.1.4.1.1.12.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Grayscale Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definition	SOP Class UID	Transfer Syntax UID
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Pseudo-Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Raw DataStorage	1.2.840.10008.5.1.4.1.1.66	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ultrasound Multi-frame Storage Image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiation Dose Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

3.3 AUGMENTED AND PRIVATE APPLICATION PROFILES

3.3.1 Augmented Application Profiles

The standard application profiles are augmented with private object Siemens CSA Non-Image.

Table 3-5: Private SOP Classes and Transfer Syntaxes for Augmented Media Profiles

Information Object Definition	SOP Class UID	Transfer Syntax UID	FSC	FSR
CSA Non-Image Storage	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M

The Siemens non-image is typically used for raw data and 3D private data.

3.4 MEDIA CONFIGURATION

none

3.5 Attribute confidentiality profiles

3.5.1 De-identification

The **syngo.via View&GO** application can de-identify attributes. During export to file system it is the user responsibility to select anonymization.

For anonymization private attributes are not included in anonymized Studies.

The following table contains the attributes that are anonymized:

Table 3-6: Application Level Confidentiality Profile Attributes (standard tags)

DICOM Tag	Attribute Name
(0000,1001)	Requested SOP Instance UID
(0002,0003)	Media Storage SOP Instance UID
(0004,1511)	Referenced SOP Instance UID in File
(0008,0014)	Instance Creator UID
(0008,0015)	Instance Coercion DateTime
(0008,0018)	SOP Instance UID
(0008,0020)	Study Date
(0008,0021)	Series Date
(0008,0022)	Acquisition Date
(0008,0023)	Content Date
(0008,0024)	Overlay Date
(0008,0025)	Curve Date
(0008,002A)	Acquisition DateTime
(0008,0030)	Study Time
(0008,0031)	Series Time
(0008,0032)	Acquisition Time
(0008,0033)	Content Time
(0008,0034)	Overlay Time
(0008,0035)	Curve Time
(0008,0050)	Accession Number
(0008,0058)	Failed SOP Instance UID List
(0008,0080)	Institution Name
(0008,0081)	Institution Address
(0008,0082)	Institution Code Sequence
(0008,0090)	Referring Physician's Name
(0008,0092)	Referring Physician's Address
(0008,0094)	Referring Physician's Telephone Numbers
(0008,0096)	Referring Physician's Identification Sequence
(0008,010D)	Context Group Extension Creator UID
(0008,0201)	Timezone Offset From UTC
(0008,1010)	Station Name
(0008,1030)	Study Description
(0008,103E)	Series Description
(0008,1040)	Institutional Department Name
(0008,1048)	Physician(s) of Record
(0008,1049)	Physician(s) of Record Identification Sequence

DICOM Tag	Attribute Name
(0008,1050)	Performing Physicians' Name
(0008,1052)	Performing Physicians' Identification Sequence
(0008,1060)	Name of Physician(s) Reading Study
(0008,1062)	Physician Reading Study Identification Sequence
(0008,1070)	Operators' Name
(0008,1072)	Operators' Identification Sequence
(0008,1080)	Admitting Diagnoses Description
(0008,1084)	Admitting Diagnoses Code Sequence
(0008,1110)	Referenced Study Sequence
(0008,1111)	Referenced Performed Procedure Step Sequence
(0008,1120)	Referenced Patient Sequence
(0008,1140)	Referenced Image Sequence
(0008,1155)	Referenced SOP Instance UID
(0008,1195)	Transaction UID
(0008,2111)	Derivation Description
(0008,2112)	Source Image Sequence
(0008,3010)	Irradiation Event UID
(0008,4000)	Identifying Comments
(0008,9123)	Creator Version UID
(0010,0010)	Patient's Name
(0010,0020)	Patient ID
(0010,0021)	Issuer of Patient ID
(0010,0030)	Patient's Birth Date
(0010,0032)	Patient's Birth Time
(0010,0040)	Patient's Sex
(0010,0050)	Patient's Insurance Plan Code Sequence
(0010,0101)	Patient's Primary Language Code Sequence
(0010,0102)	Patient's Primary Language Modifier Code Sequence
(0010,1000)	Other Patient IDs
(0010,1001)	Other Patient Names
(0010,1002)	Other Patient IDs Sequence
(0010,1005)	Patient's Birth Name
(0010,1010)	Patient's Age
(0010,1020)	Patient's Size
(0010,1030)	Patient's Weight
(0010,1040)	Patient Address
(0010,1050)	Insurance Plan Identification
(0010,1060)	Patient's Mother's Birth Name
(0010,1080)	Military Rank
(0010,1081)	Branch of Service
(0010,1090)	Medical Record Locator
(0010,1100)	Referenced Patient Photo Sequence
(0010,2000)	Medical Alerts
(0010,2110)	Allergies
(0010,2150)	Country of Residence
(0010,2152)	Region of Residence
(0010,2154)	Patient's Telephone Number
(0010,2160)	Ethnic Group
(0010,2180)	Occupation
(0010,21A0)	Smoking Status
(0010,21B0)	Additional Patient's History
(0010,21C0)	Pregnancy Status
(0010,21D0)	Last Menstrual Date
(0010,21F0)	Patient's Religious Preference
(0010,2203)	Patient Sex Neutered
(0010,2297)	Responsible Person
(0010,2299)	Responsible Organization
(0010,4000)	Patient Comments
(0018,0010)	Contrast Bolus Agent
(0018,1000)	Device Serial Number
(0018,1002)	Device UID
(0018,1004)	Plate ID
(0018,1005)	Generator ID
(0018,1007)	Cassette ID
(0018,1008)	Gantry ID
(0018,1030)	Protocol Name
(0018,1400)	Acquisition Device Processing Description
(0018,2042)	Target UID
(0018,4000)	Acquisition Comments
(0018,700A)	Detector ID

DICOM Tag	Attribute Name
(0018,9424)	Acquisition Protocol Description
(0018,9516)	Start Acquisition DateTime
(0018,9517)	End Acquisition DateTime
(0018,A003)	Contribution Description
(0020,000D)	Study Instance UID
(0020,000E)	Series Instance UID
(0020,0010)	Study ID
(0020,0052)	Frame of Reference UID
(0020,0200)	Synchronization Frame of Reference UID
(0020,3401)	Modifying Device ID
(0020,3404)	Modifying Device Manufacturer
(0020,3406)	Modified Image Description
(0020,4000)	Image Comments
(0020,9158)	Frame Comments
(0020,9161)	Concatenation UID
(0020,9164)	Dimension Organization UID
(0028,1199)	Palette Color Lookup Table UID
(0028,1214)	Large Palette Color Lookup Table UID
(0028,4000)	Image Presentation Comments
(0032,0012)	Study ID Issuer
(0032,1020)	Scheduled Study Location
(0032,1021)	Scheduled Study Location AE Title
(0032,1030)	Reason for Study
(0032,1032)	Requesting Physician
(0032,1033)	Requesting Service
(0032,1060)	Requested Procedure Description
(0032,1070)	Requested Contrast Agent
(0032,4000)	Study Comments
(0038,0004)	Referenced Patient Alias Sequence
(0038,0010)	Admission ID
(0038,0011)	Issuer of Admission ID
(0038,001E)	Scheduled Patient Institution Residence
(0038,0020)	Admitting Date
(0038,0021)	Admitting Time
(0038,0040)	Discharge Diagnosis Description
(0038,0050)	Special Needs
(0038,0060)	Service Episode ID
(0038,0061)	Issuer of Service Episode ID
(0038,0062)	Service Episode Description
(0038,0300)	Current Patient Location
(0038,0400)	Patient's Institution Residence
(0038,0500)	Patient State
(0038,4000)	Visit Comments
(0040,0001)	Scheduled Station AE Title
(0040,0002)	Scheduled Procedure Step Start Date
(0040,0003)	Scheduled Procedure Step Start Time
(0040,0004)	Scheduled Procedure Step End Date
(0040,0005)	Scheduled Procedure Step End Time
(0040,0006)	Scheduled Performing Physician Name
(0040,0007)	Scheduled Procedure Step Description
(0040,000B)	Scheduled Performing Physician Identification Sequence
(0040,0010)	Scheduled Station Name
(0040,0011)	Scheduled Procedure Step Location
(0040,0012)	Pre-Medication
(0040,0241)	Performed Station AE Title
(0040,0242)	Performed Station Name
(0040,0243)	Performed Location
(0040,0244)	Performed Procedure Step Start Date
(0040,0245)	Performed Procedure Step Start Time
(0040,0248)	Performed Station Name Code Sequence
(0040,0250)	Performed Procedure Step End Date
(0040,0251)	Performed Procedure Step End Time
(0040,0253)	Performed Procedure Step ID
(0040,0254)	Performed Procedure Step Description
(0040,0275)	Request Attributes Sequence
(0040,0280)	Comments on Performed Procedure Step
(0040,0555)	Acquisition Context Sequence
(0040,1001)	Requested Procedure ID
(0040,1004)	Patient Transport Arrangements
(0040,1005)	Requested Procedure Location

DICOM Tag	Attribute Name
(0040,1010)	Names of Intended Recipient of Results
(0040,1011)	Intended Recipients of Results Identification Sequence
(0040,1101)	Person Identification Code Sequence
(0040,1102)	Person Address
(0040,1103)	Person Telephone Numbers
(0040,1400)	Requested Procedure Comments
(0040,2001)	Reason for Imaging Service Request
(0040,2008)	Order Entered By
(0040,2009)	Order Enterer Location
(0040,2010)	Order Callback Phone Number
(0040,2016)	Placer Order Number of Imaging Service Request
(0040,2017)	Filler Order Number of Imaging Service Request
(0040,2400)	Imaging Service Request Comments
(0040,3001)	Confidentiality Constraint on Patient Data Description
(0040,4005)	Scheduled Procedure Step Start DateTime
(0040,4010)	Scheduled Procedure Step Modification DateTime
(0040,4011)	Expected Completion Date Time
(0040,4023)	Referenced General Purpose Scheduled Procedure Step Transaction UID
(0040,4025)	Scheduled Station Name Code Sequence
(0040,4027)	Scheduled Station Geographic Location Code Sequence
(0040,4030)	Performed Station Geographic Location Code Sequence
(0040,4034)	Scheduled Human Performers Sequence
(0040,4035)	Actual Human Performers Sequence
(0040,4036)	Human Performers Organization
(0040,4037)	Human Performers Name
(0040,4050)	Performed Procedure Step Start DateTime
(0040,4051)	Performed Procedure Step End DateTime
(0040,4052)	Procedure Step Cancellation DateTime
(0040,A027)	Verifying Organization
(0040,A073)	Verifying Observer Sequence
(0040,A075)	Verifying Observer Name
(0040,A078)	Author Observer Sequence
(0040,A07A)	Participant Sequence
(0040,A07C)	Custodial Organization Sequence
(0040,A088)	Verifying Observer Identification Code Sequence
(0040,A123)	Person Name
(0040,A124)	UID
(0040,A171)	Observation UID
(0040,A172)	Referenced Observation UID (Trial)
(0040,A192)	Observation Date (Trial)
(0040,A193)	Observation Time (Trial)
(0040,A307)	Current Observer (Trial)
(0040,A352)	Verbal Source (Trial)
(0040,A353)	Address (Trial)
(0040,A354)	Telephone Number (Trial)
(0040,A358)	Verbal Source Identifier Code Sequence (Trial)
(0040,A402)	Observation Subject UID (Trial)
(0040,A730)	Content Sequence
(0040,DB0C)	Template Extension Organization UID
(0040,DB0D)	Template Extension Creator UID
(0070,0001)	Graphic Annotation Sequence
(0070,0084)	Content Creator's Name
(0070,0086)	Content Creator's Identification Code Sequence
(0070,031A)	Fiducial UID
(0088,0140)	Storage Media Fileset UID
(0088,0200)	Icon Image Sequence
(0088,0904)	Topic Title
(0088,0906)	Topic Subject
(0088,0910)	Topic Author
(0088,0912)	Topic Keywords
(0400,0100)	Digital Signature UID
(0400,0402)	Referenced Digital Signature Sequence
(0400,0403)	Referenced SOP Instance MAC Sequence
(0400,0404)	MAC
(0400,0550)	Modified Attributes Sequence
(0400,0561)	Original Attributes Sequence
(2030,0020)	Text String
(3006,0024)	Referenced Frame of Reference UID
(3006,00C2)	Related Frame of Reference UID

DICOM Tag	Attribute Name
(3008,0105)	Source Serial Number
(300A,0013)	Dose Reference UID
(300E,0008)	Reviewer Name
(4000,0010)	Arbitrary
(4000,4000)	Text Comments
(4008,0042)	Results ID Issuer
(4008,0102)	Interpretation Recorder
(4008,010A)	Interpretation Transcriber
(4008,010B)	Interpretation Text
(4008,010C)	Interpretation Author
(4008,0111)	Interpretation Approver Sequence
(4008,0114)	Physician Approving Interpretation
(4008,0115)	Interpretation Diagnosis Description
(4008,0118)	Results Distribution List Sequence
(4008,0119)	Distribution Name
(4008,011A)	Distribution Address
(4008,0202)	Interpretation ID Issuer
(4008,0300)	Impressions
(4008,4000)	Results Comments
(50xx,xxxx)	Curve Data
(60xx,0100)	Overlay Bits Allocated
(60xx,0102)	Overlay Bit Position
(60xx,3000)	Overlay Data
(60xx,4000)	Overlay Comments
(FFFA,FFFA)	Digital Signatures Sequence
(FFFC,FFFC)	Data Set Trailing Padding

4 SUPPORT OF CHARACTER SETS

4.1 CHARACTER SETS FOR *syngo.via* View&GO

The ***syngo.via* View&GO** DICOM application supports the following character sets as defined in the three tables below.

Table 4-1: Single-Byte Character Sets without Code Extension

Character Set Description	Defined Term	ISO registration number	Character Set
Default repertoire	none	ISO_IR 6	ISO 646:
Latin alphabet No. 1	ISO_IR 100	ISO_IR 100	Supplementary set
		ISO_IR 6	ISO 646:
Latin alphabet No. 2	ISO_IR 101	ISO_IR 101	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 3	ISO_IR 109	ISO_IR 109	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 4	ISO_IR 110	ISO_IR 110	Supplementary set
		ISO_IR 6	ISO 646
Cyrillic	ISO_IR 144	ISO_IR 144	Supplementary set
		ISO_IR 6	ISO 646
Arabic	ISO_IR 127	ISO_IR 127	Supplementary set
		ISO_IR 6	ISO 646
Greek	ISO_IR 126	ISO_IR 126	Supplementary set
		ISO_IR 6	ISO 646
Hebrew	ISO_IR 138	ISO_IR 138	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 5	ISO_IR 148	ISO_IR 148	Supplementary set
		ISO_IR 6	ISO 646
Japanese	ISO_IR 13	ISO_IR 13	JIS X 0201: Katakana
		ISO_IR 14	JIS X 0201: Romaji
Thai	ISO_IR166	ISO_IR166	TIS 620-253 (1990)
		ISO_IR 6	ISO 646

Table 4-2: Single-Byte Characters Sets with Code Extension

Character Set Description	Defined Term	Standard for Code Extension	ESC sequence	ISO registration number	Character Set
Default repertoire	ISO 2022 IR 6	ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.1	ISO 2022 IR 100	ISO 2022	ESC 02/13 04/01	ISO-IR 100	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.2	ISO 2022 IR 101	ISO 2022	ESC 02/13 04/02	ISO-IR 101	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.3	ISO 2022 IR 109	ISO 2022	ESC 02/13 04/03	ISO-IR 109	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.4	ISO 2022 IR 110	ISO 2022	ESC 02/13 04/04	ISO-IR 110	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646

Multi-Byte Character Sets without Code Extension

Table 4-3: Multi-Byte Character Sets without Code Extension

Character Set Description	Defined Term	ISO registration number	Character Set
Unicode	ISO_IR 192	ISO 10646	Unicode in UTF-8
Chinese	GB18030	GB18030	GB 18030-2000 (China Association for Standardization)

Table 4-4: Multi-Byte Character Sets with Code Extension

Character Set Description	Defined Term	Standard for Code Extension	ESC sequence	ISO registration number	Character Set
Japanese	ISO 2022 IR 159	ISO 2022	ESC 02/04 02/08 04/04	ISO-IR 159	JIS X 0212: Supplementary Kanji set
Korean	ISO 2022 IR 149	ISO 2022	ESC 02/04 02/09 04/03	ISO-IR 149	KS X 1001: Hangul and Hanja

All Specific Character Set listed above are supported for incoming Data. When creating new Instances, the system will use the default SCS (or SCS List) configured on the machine.

When there is a mismatch between the given character set in attribute (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Convert each illegal character to a '?'.

There are now three categories of character sets which have to be differentiated because of their different encoding formats:

- Conventional ISO character sets: ISO_IR 6, ISO 2022 IR 6, ISO_IR 100, etc.
→ encoded in ISO 2022
- ISO_IR 192 → encoded in UTF-8
- GB18030 → encoded in GB18030

It is not possible to recognize the following mismatches automatically on receiving or importing:

- An attribute value is encoded in ISO_IR 192 ↔ (0008,0005) contains a conventional ISO character set as primary character set
- An attribute value is encoded in GB18030 ↔ (0008,0005) contains a conventional ISO character set as primary character set
- An attribute value is encoded in ISO 2022 ↔ (0008,0005) contains ISO_IR 192
- An attribute value is encoded in ISO 2022 ↔ (0008,0005) contains GB18030

An IOD that contains one of the above mentioned inconsistencies is not DICOM conform. As these kinds of inconsistencies cannot be recognized by the system, the IOD will not be rejected but the character data might be corrupted.

The **syngo.via View&GO** supports Kanji characters in the byte zones after 74 (79, 7A, 7B and 7C).

5 SECURITY

5.1 SECURITY PROFILES

Time Synchronization Profiles: **syngo.via View&GO** acts as an NTP Client in the Maintain Time Transaction.

5.2 ASSOCIATION LEVEL SECURITY

The Echo SCP will answer to AETs.

6 Annexes

6.1 SOP Classes supported

Table 6-1 SOP CLASSES for Storage

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)	Visualization
Supported Storage SOP Classes				
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	Yes	No
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	Yes	No
Basic Text SR Storage	1.2.840.10008.5.1.4.1.1.88.11	Yes	Yes	No
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Yes	Yes	No
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	Yes	Yes
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	Yes	No
Color Softcopy Presentation State Storage SOP Class	1.2.840.10008.5.1.4.1.1.11.2	Yes	Yes	No
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes	No
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes	Yes
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Yes	Yes	No
Digital Mammography X-Ray Image Storage- For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	Yes	Yes
Digital Mammography X-Ray Image Storage- For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	Yes	No
Digital X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes	Yes
Digital X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes	No
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes	No
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Yes	Yes	Yes
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	Yes	Yes
Enhanced MR Color Image Storage	1.2.840.10008.5.1.4.1.1.4.3	Yes	Yes	Yes
Enhanced Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	Yes	No
Enhanced XA Image Storage	1.2.840.10008.5.1.4.1.1.12.1.1	Yes	Yes	Yes
Enhanced XRF Image Storage	1.2.840.10008.5.1.4.1.1.12.2.1	Yes	Yes	No
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	Yes	No
Grayscale Softcopy Presentation State Storage (store & forward only)	1.2.840.10008.5.1.4.1.1.11.1	Yes	Yes	Yes
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	Yes	No
Key Object Selection Document Storage	1.2.840.10008.5.1.4.1.1.88.59	Yes	Yes	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	Yes	Yes

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)	Visualization
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Yes	Yes	No
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	Yes	Yes
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	Yes	Yes
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	Yes	Yes
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	Yes	Yes
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	Yes	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	Yes	Yes
Pseudo-Color Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	Yes	Yes	No
PET Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	Yes	Yes
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	Yes	No
Raw DataStorage	1.2.840.10008.5.1.4.1.1.66	Yes	Yes	No
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	Yes	Yes	No
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Yes	Yes	No
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	Yes	Yes	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	Yes	Yes
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	Yes	No
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	Yes	No
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Yes	Yes	Yes
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Yes	Yes	Yes
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	Yes	Yes	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes	Yes
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Yes	Yes	No
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Yes	Yes	No
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	Yes	No
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Yes	Yes	No
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes	Yes
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes	Yes
Ultrasound Multi-frame Image Storage (Retired)	1.2.840.10008.5.1.4.1.1.3	Yes	Yes	Yes
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Yes	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes	Yes
X-Ray Radiation Dose Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes	No
X-Ray Radio-Fluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes	Yes
Supported private Storage SOP Classes				
CSA Non-Image Storage	1.3.12.2.1107.5.9.1	No	Yes	No

Table 6-2: Supported Non-Storage SOP Classes

SOP Class Name	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Supported Verification SOP Classes			
Verification	1.2.840.10008.1.1	Yes	Yes
Supported Storage Commitment SOP Classes			
Storage Commitment Push Model	1.2.840.10008.1.20.1	No	No
Storage Commitment Push Model well known SOP Instance	1.2.840.10008.1.20.1.1	No	No
Supported Query/Retrieve-FIND SOP Classes			
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Patient /Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Yes	Yes
Supported Query/Retrieve-MOVE SOP Classes			
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	Yes	Yes
Modality Worklist Information SOP Class			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Yes	No
Grayscale Print Management META SOP classes			
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Yes	No
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
- Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Yes	No
- Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No
Print Job SOP Class	1.2.840.10008.5.1.1.14	Yes	No
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23	Yes	No
Color Print Management META SOP classes			
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Yes	No
- Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Yes	No
- Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Yes	No
- Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Yes	No
- Printer SOP Class	1.2.840.10008.5.1.1.16	Yes	No
Print Job SOP Class	1.2.840.10008.5.1.1.14	Yes	No

6.2 IOD CONTENTS

6.2.1 Created SOP Instance(s)

The applications from **syngo.via View&GO** create objects of the following SOP Classes during Transferring, Post-Processing and Reading:

Table 6-3: List of created SOP Classes

SOP Class Name	SOP Class UID	Internally used (neither SCU nor SCP is applicable)
Basic Text Structured Report	1.2.840.10008.5.1.4.1.1.88.11	No
Comprehensive Structured Report Storage	1.2.840.10008.5.1.4.1.1.88.33	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	No
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	No
Enhanced Structured Report	1.2.840.10008.5.1.4.1.1.88.22	No
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	No
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	No
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	No
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	No
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	No
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	No
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	No

6.2.2 Data Dictionary of Private Attributes

The following table Table 6-4: Private Data Element Dictionary lists all private attributes created by **syngo.via View&GO**, which may be included in the generated instances. These private attributes may be deprecated or replaced with standard attributes in the future.

Table 6-4: Private Data Element Dictionary

DICOM Tag	Name	VR	VM
(0027,SIEMENS SYNGO ENHANCED IDATASET API,01)	Business Unit Code	CS	1
(0027,SIEMENS SYNGO ENHANCED IDATASET API,02)	Application Type	LO	1
(0027,SIEMENS SYNGO ENHANCED IDATASET API,03)	Application Attributes Sequence	SQ	1

DICOM Tag	Name	VR	VM
(0029,SIEMENS SYNGO FUNCTION ASSIGNMENT,01)	Data Reference	LO	1
(0009,SIEMENS SYNGO INDEX SERVICE,20)	Object Insertion Date	DA	1
(0009,SIEMENS SYNGO INDEX SERVICE,A0)	Sender System Device Name	LO	1
(0029,SIEMENS SYNGO VOLUME,12)	Slices	US	1
(0029,SIEMENS SYNGO VOLUME,14)	Volume Histogram	OB	1
(0029,SIEMENS SYNGO VOLUME,18)	Volume Level	IS	1
(0029,SIEMENS SYNGO VOLUME,30)	Voxel Spacing	DS	3
(0029,SIEMENS SYNGO VOLUME,32)	Volume Position (Patient)	DS	3
(0029,SIEMENS SYNGO VOLUME,37)	Volume Orientation (Patient)	DS	9
(0029,SIEMENS SYNGO VOLUME,40)	Resampling Flag	CS	1
(0029,SIEMENS SYNGO VOLUME,42)	Normalization Flag	CS	1
(0029,SIEMENS SYNGO VOLUME,44)	SubVolume Sequence	SQ	1-n
(0071,SIEMENS SYNGO REGISTRATION,20)	Registered Image Sequence	SQ	1
(0071,SIEMENS SYNGO REGISTRATION,21)	Registration Is Validated Flag	CS	1
(0071,SIEMENS SYNGO REGISTRATION,20)	Registered Image Sequence	SQ	1
(0071,SIEMENS SYNGO REGISTRATION,21)	Registration Is Validated Flag	CS	1
(7FDF,SIEMENS SYNGO DATA PADDING,FC)	Pixel Data Leading Padding	OB	1

Interpretation of the Dicom Tags from the above table:

(gggg, pp,ee) -> (gggg, ppee)

gggg - odd group number

pp - private creator identification code

ee - private element

6.2.3 Usage of Attributes from received IODs

N/A

6.2.4 Coerced / Modified fields

N/A

6.3 CODED TERMINOLOGY AND TEMPLATES

See application specific annexes.

6.3.1 Context Groups

See application specific annexes.

6.3.2 Template Specifications

See application specific annexes.

6.3.3 Private Code definitions

See application specific annexes.

6.4 GRAYSCALE IMAGE CONSISTENCY

N/A

6.5 STANDARD EXTENDED / SPECIALIZED / PRIVATE SOP CLASSES

N/A

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice.

Some/All of the features and products described herein may not be available in the United States or other countries.

The information in this document contains general technical descriptions of specifications and options as well as standard and optional features that do not always have to be present in individual cases.

Siemens reserves the right to modify the design, packaging, specifications and options described herein without prior notice. Please contact your local Siemens sales representative for the most current information.

In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we recycle certain components. Using the same extensive quality assurance measures as for factory- new components, we guarantee the quality of these recycled components.

Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Caution: Federal law restricts this device to sale by or on the order of a physician.

Legal Manufacturer
Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany

Siemens Healthcare Headquarters
Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany
Telephone +49 9131 84-0
siemens.com/healthcare