

# **MAX systems VF10**

**Multi-platform imaging system used by:**

**Multitom Rax VF10**

**Luminos dRF Max VF10**

**Luminos Agile Max VF10**

**Uroskop Omnia Max VF10**

**Ysio Max VF10**

**Mobilett Mira Max VF10**

**MOBILETT Elara Max VF10**

**Multix Fusion Max VF10**

## Table of Contents

|   |           |
|---|-----------|
| <b>Network Conformance Statement .....</b>                                | <b>8</b>  |
| <b>1        <i>Introduction</i>.....</b>                                  | <b>8</b>  |
| 1.1    Overview .....   | 8         |
| 1.2    Scope and Field.....   | 8         |
| 1.3    Audience .....   | 8         |
| 1.4    Remarks .....  | 9         |
| 1.5    Definitions, Terms and Abbreviations.....                          | 10        |
| 1.6    References .....   | 10        |
| 1.7    Structure .....  | 10        |
| <b>2        <i>Implementation Model Verification</i> .....</b>            | <b>12</b> |
| 2.1    Application Data Flow Diagram .....                                | 12        |
| 2.2    Functional Definitions of Applications.....                        | 12        |
| 2.3    Sequencing of Real-World Activities.....                           | 12        |
| <b>3        <i>Application Entity Specification Verification</i>.....</b> | <b>13</b> |
| 3.1    Verification AE Specification .....                                | 13        |
| 3.1.1    Association Establishment Policies .....                         | 13        |
| 3.1.1.1    General.....   | 13        |
| 3.1.1.2    Number of Associations.....                                    | 13        |
| 3.1.1.3    Asynchronous Nature .....                                      | 13        |
| 3.1.1.4    Implementation Identifying Information .....                   | 13        |
| 3.1.2    Association Initiation Policy .....                              | 13        |
| 3.1.2.1    Associated Real-World Activity.....                            | 13        |
| 3.1.3    Association Acceptance Policy .....                              | 14        |
| <b>4        <i>Implementation Model Storage</i>.....</b>                  | <b>15</b> |
| 4.1    Application Data Flow Diagram .....                                | 15        |
| 4.2    Functional Definitions of Application Entities.....                | 15        |
| 4.3    Sequencing of Real-World Activities.....                           | 16        |
| <b>5        <i>Application Entity Specification Storage</i>.....</b>      | <b>17</b> |
| 5.1    Storage AES Specification .....                                    | 17        |
| 5.1.1    Association Establishment Policies .....                         | 18        |
| 5.1.1.1    General.....   | 18        |
| 5.1.1.2    Number of Associations.....                                    | 18        |
| 5.1.1.3    Asynchronous Nature .....                                      | 18        |
| 5.1.1.4    Implementation Identifying Information .....                   | 18        |
| 5.1.2    Association Initiation Policy .....                              | 18        |
| 5.1.2.1    Associated Real-World Activity – Storage SCU .....             | 18        |
| 5.1.3    Association Acceptance Policy .....                              | 22        |
| 5.1.3.1    Associated Real-World Activity – Storage SCP .....             | 22        |
| <b>6        <i>Implementation Model Storage Commitment</i>.....</b>       | <b>26</b> |

|          |  |           |
|----------|--|-----------|
| 6.1      | Application Data Flow Diagram .....  | 26        |
| 6.2      | Functional Definitions of Application Entities.....                        | 26        |
| 6.3      | Sequencing of Real-World Activities.....                                   | 27        |
| 7        | <b><i>AE Specification Storage Commitment</i></b> .....                    | <b>28</b> |
| 7.1      | Storage Commitment AE Specification.....                                   | 28        |
| 7.1.1    | Association Establishment Policies .....                                   | 28        |
| 7.1.1.1  | General.....   | 28        |
| 7.1.1.2  | Number of Associations.....  | 28        |
| 7.1.1.3  | Asynchronous Nature.....   | 28        |
| 7.1.1.4  | Implementation Identifying Information .....                               | 28        |
| 7.1.2    | Association Initiation Policy .....  | 28        |
| 7.1.2.1  | Real World Activity – Storage Commitment SCU.....                          | 29        |
| 7.1.3    | Association Acceptance Policy .....  | 29        |
| 7.1.3.1  | Real World Activity – Storage Commitment SCU.....                          | 30        |
| 8        | <b><i>Implementation Model Query / Retrieve</i></b> .....                  | <b>31</b> |
| 8.1      | Application Data Flow Diagram .....  | 31        |
| 8.2      | Functional Definitions of Application Entities.....                        | 31        |
| 8.3      | Sequencing of Real-World Activities.....                                   | 31        |
| 9        | <b><i>AE Specification Query/Retrieve</i></b> .....                        | <b>32</b> |
| 9.1      | Query/Retrieve Service Aes Specification.....                              | 32        |
| 9.1.1    | Association Establishment Policies .....                                   | 32        |
| 9.1.1.1  | General.....   | 32        |
| 9.1.1.2  | Number of Associations.....  | 32        |
| 9.1.1.3  | Asynchronous Nature .....  | 32        |
| 9.1.1.4  | Implementation Identifying Information .....                               | 32        |
| 9.1.2    | Association Initiation Policy .....  | 32        |
| 9.1.2.1  | Real World Activity – Find SCU.....  | 33        |
| 9.1.2.2  | Real-World Activity – Move SCU.....  | 35        |
| 9.1.3    | Association Acceptance Policy .....  | 37        |
| 10       | <b><i>Implementation Model Modality Worklist</i></b> .....                 | <b>38</b> |
| 10.1     | Application Data Flow Diagram .....  | 38        |
| 10.2     | Functional Definitions of Application Entities .....                       | 38        |
| 10.3     | Sequencing of Real-World Activities .....                                  | 38        |
| 11       | <b><i>AE Specification Modality Worklist</i></b> .....                     | <b>39</b> |
| 11.1     | Modality Worklist Service Aes Specification .....                          | 39        |
| 11.1.1   | Association Establishment Policies .....                                   | 39        |
| 11.1.1.1 | General.....   | 39        |
| 11.1.1.2 | Number of Associations.....  | 39        |
| 11.1.1.3 | Asynchronous Nature .....  | 39        |
| 11.1.1.4 | Implementation Identifying Information .....                               | 39        |
| 11.1.2   | Association Initiation Policy .....  | 39        |
| 11.1.2.1 | Real-World Activity .....  | 39        |
| 11.1.3   | Association Acceptance Policy .....  | 41        |
| 12       | <b><i>Implementation Model Modality Performed Procedure Step</i></b> ..... | <b>42</b> |
| 12.1     | Application Data Flow Diagram .....  | 42        |
| 12.2     | Functional Definitions of Application Entities .....                       | 42        |

|             |  |           |
|-------------|--|-----------|
| <b>12.3</b> | <b>Sequencing of Real-World Activities .....</b>                         | <b>42</b> |
| <b>13</b>   | <b>AE Specification Modality Performed Procedure Step.....</b>           | <b>43</b> |
| <b>13.1</b> | <b>Modality Performed Procedure Step Service Aes Specification .....</b> | <b>43</b> |
| 13.1.1      | Association Establishment Policies .....                                 | 43        |
| 13.1.1.1    | General .....  | 43        |
| 13.1.1.2    | Number of Associations.....  | 43        |
| 13.1.1.3    | Asynchronous Nature .....  | 43        |
| 13.1.1.4    | Implementation Identifying Information .....                             | 43        |
| 13.1.2      | Association Initiation Policy .....                                      | 43        |
| 13.1.2.1    | Real-World Activity .....  | 44        |
| 13.1.3      | Association Acceptance Policy .....                                      | 45        |
| <b>14</b>   | <b>Implementation Model Print.....</b>                                   | <b>46</b> |
| <b>14.1</b> | <b>Application Data Flow Diagram .....</b>                               | <b>46</b> |
| <b>14.2</b> | <b>Functional Definition of Application Entities .....</b>               | <b>46</b> |
| <b>14.3</b> | <b>Sequencing of Real-World Activities .....</b>                         | <b>46</b> |
| <b>15</b>   | <b>Application Entity Specification Print.....</b>                       | <b>47</b> |
| <b>15.1</b> | <b>Print Management AE Specification .....</b>                           | <b>47</b> |
| 15.1.1      | Association Establishment Policies .....                                 | 47        |
| 15.1.1.1    | General .....  | 47        |
| 15.1.1.2    | Number of Associations.....  | 47        |
| 15.1.1.3    | Asynchronous Nature .....  | 47        |
| 15.1.1.4    | Implementation Identifying Information .....                             | 47        |
| 15.1.2      | Association Initiation Policy .....                                      | 47        |
| 15.1.2.1    | Associated Real-World Activity.....                                      | 48        |
| 15.1.3      | Association Acceptance Policy .....                                      | 52        |
| <b>16</b>   | <b>Communication Profiles .....</b>                                      | <b>53</b> |
| <b>16.1</b> | <b>Supported Communication Stacks .....</b>                              | <b>53</b> |
| 16.1.1      | TCP/IP Stack .....   | 53        |
| 16.1.1.1    | API.....   | 53        |
| 16.1.1.2    | Physical Media Support.....  | 53        |
| <b>17</b>   | <b>Extensions / Specializations / Privatizations .....</b>               | <b>54</b> |
| 17.1.1      | Standard Extended / Specialized / Private SOPs.....                      | 54        |
| 17.1.2      | Private Transfer Syntaxes .....  | 54        |
| <b>18</b>   | <b>Configuration .....</b>   | <b>55</b> |
| <b>18.1</b> | <b>AE Title/Presentation Address Mapping.....</b>                        | <b>55</b> |
| 18.1.1      | DICOM Verification .....   | 55        |
| 18.1.2      | DICOM Storage SCP AE Title .....   | 55        |
| 18.1.3      | DICOM Storage SCU AE Title .....   | 55        |
| 18.1.4      | DICOM Query/Retrieve AE Title .....                                      | 55        |
| 18.1.5      | DICOM Storage Commitment AE Title .....                                  | 55        |
| 18.1.6      | DICOM Worklist AE Title .....  | 56        |
| 18.1.7      | DICOM MPPS AE Title .....  | 56        |
| 18.1.8      | DICOM Print AE Title .....   | 56        |
| <b>18.2</b> | <b>Configurable Parameters .....</b>                                     | <b>56</b> |
| 18.2.1      | Storage and Query/Retrieve .....   | 56        |
| 18.2.2      | Storage Commitment.....  | 57        |
| 18.2.3      | Modality Worklist.....   | 57        |
| 18.2.4      | Modality Performed Procedure Step .....                                  | 57        |
| 18.2.5      | Print.....   | 57        |

|         |   |           |
|---------|---|-----------|
| 18.3    | Default Parameters .....  | 57        |
| 19      | Support of Extended Character Sets .....  | 59        |
| 20      | Security .....  | 60        |
| 20.1    | Security Profiles .....   | 60        |
| 20.1.1  | Secure Transport Connection Profiles .....  | 60        |
|         | <b>Application Profile Conformance Statement.....</b>                                     | <b>61</b> |
| 1       | Introduction.....   | 62        |
| 1.1     | Purpose .....   | 62        |
| 1.2     | Scope .....   | 62        |
| 1.3     | Definitions, Terms and Abbreviations.....   | 62        |
| 1.4     | References .....  | 62        |
| 1.5     | Remarks .....   | 62        |
| 2       | Implementation Model.....   | 64        |
| 2.1     | Application Data Flow Diagram .....   | 64        |
| 2.2     | Functional Definitions of Aes.....  | 64        |
| 2.3     | Sequencing of Real-World Activities.....  | 64        |
| 2.4     | File Meta Information Options.....  | 65        |
| 3       | AE Specifications .....   | 65        |
| 3.1     | DICOM Archive Specification.....  | 65        |
| 3.1.1   | File Meta Information for the Application Entity .....                                    | 65        |
| 3.1.2   | Real-World Activities for this Application Entity .....                                   | 65        |
| 3.1.2.1 | Real-World Activity: Browse Directory Information.....                                    | 65        |
| 3.1.2.2 | Real-World Activity: Import into local Storage .....                                      | 66        |
| 3.1.2.3 | Real-World Activity: Export to local Archive Media .....                                  | 66        |
| 4       | Augmented and Private Profiles.....   | 68        |
| 4.1     | Augmented Application Profiles.....   | 68        |
| 4.2     | Private Application Profiles.....   | 68        |
| 5       | Extensions, Specializations and Privatizations of SOP Classes and Transfer Syntaxes ..... | 69        |
| 5.1     | SOP Specific Conformance Statement for Basic Directory .....                              | 70        |
| 5.1.1   | Extension, Specialization for "Packed CD" .....   | 70        |
| 5.1.2   | DICOMDIR Attributes .....   | 70        |
| 6       | Configuration .....   | 72        |
| 6.1     | AE Title Mapping .....  | 72        |
| 6.1.1   | DICOM Media Storage AE Title .....  | 72        |
| 7       | Support of Extended Character Sets .....  | 73        |
| A       | APPENDIX .....  | 74        |
| A.1     | Common attributes in image and structured report IODs.....                                | 74        |
| A.2     | Multiframe True Color SC Storage Standard Extended SOP Class.....                         | 76        |
| A.3     | XRF Standard Extended SOP Class .....   | 77        |

|             |   |           |
|-------------|---|-----------|
| A.3.1       | configuration "XRF – Full" .....                          | 77        |
| A.3.2       | configuration "XRF – Ready Processed" .....               | 79        |
| <b>A.4</b>  | <b>CR,DX Standard Extended SOP Class .....</b>            | <b>81</b> |
| <b>A.5</b>  | <b>X-Ray Radiation Dose SR SOP Class.....</b>             | <b>83</b> |
| A.5.1       | Projection X-Ray Radiation Dose (TID 10001).....          | 83        |
| A.5.2       | Accumulated X-Ray Dose (TID 10002) .....                  | 84        |
| A.5.3       | Irradiation Event X-Ray Data (TID 10003).....             | 85        |
| A.6         | <b>EXAM Protocol as Secondary Capture Image .....</b>     | <b>87</b> |
| <b>A.7</b>  | <b>XA Standard Extended SOP Class .....</b>               | <b>88</b> |
| <b>A.8</b>  | <b>SOP Common Module – Image Type Extensions.....</b>     | <b>89</b> |
| <b>A.9</b>  | <b>Private Data .....</b>                                 | <b>89</b> |
| A.9.1       | General Private Data .....                                | 89        |
| <b>A.10</b> | <b>syngo FLC Worklist Identifier .....</b>                | <b>93</b> |
| <b>A.11</b> | <b>Modality Performed Procedure Step Identifiers.....</b> | <b>96</b> |
| <b>A.12</b> | <b>Grayscale Image Consistency .....</b>                  | <b>98</b> |

# Network Conformance Statement

## 1 Introduction

### 1.1 Overview

This Conformance Statement describes the DICOM network interface for Siemens X-Ray acquisition modalities based on the syngo FLC imaging system according to part PS 3.2 of [DICOM].

This introduction describes the application's implemented DICOM functionality in general terms.

### 1.2 Scope and Field

The Siemens product syngo FLC is a multifunctional imaging system for fluoroscopic, urologic and radiographic procedures. This DICOM Conformance Statement is valid for the following products:

- Luminos dRF Max VF10
- Luminos Agile Max VF10
- Uroskop Omnia Max VF10
- Ysio Max VF10
- Multitom Rax VF10
- Mobilett Mira Max VF10
- MOBILETT Elara Max VF10
- Multix Fusion Max VF10

The supported DICOM Services allow a smooth integration into the clinical network. Depending on system type images can be stored utilizing the DICOM XRF, XA, CR or DX IOD. The DICOM service 'Storage Commitment (Push Model) Service Class' indicates established image storage in the DICOM image archive. Images, acquired at the syngo FLC, can be retrieved from another network node by using the DICOM service 'DICOM Query/Retrieve'. With 'DICOM Basic Worklist Management Service Class' the worklist containing patient data can be retrieved from the information system and afterwards examination data can be send back to the information by using 'Modality Performed Procedure Step Service Class'. syngo FLC supports the "Print Management Service Class" and the 'Media Storage Service Class' (General Purpose CDR Application Profile) and is able to encrypt the DICOM communication according to the 'Basic TLS Secure Transport Connection Profile'.

This DICOM Conformance Statement refers to syngo FLC based products only.

### 1.3 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

## 1.4      **Remarks**

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [DICOM]. It is, however, by itself not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the user's future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

## 1.5 Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Abbreviations and terms are as follows:

|       |  |
|-------|--|
| AE    | DICOM Application Entity                           |
| AET   | DICOM Application Entity Title                     |
| ASCII | American Standard Code for Information Interchange |
| CR    | Computed Radiography                               |
| CSE   | Customer Service Engineer                          |
| DCS   | DICOM Conformance Statement                        |
| EXI   | Exposure Index                                     |
| FD    | Flat panel detector                                |
| IOD   | DICOM Information Object Definition                |
| ISO   | International Standard Organization                |
| MPPS  | Modality Performed Procedure Step                  |
| NEMA  | National Electrical Manufacturers Association      |
| NL    | Nesting Level                                      |
| R     | Required Key Attribute                             |
| O     | Optional Key Attribute                             |
| OPG   | Organ Program                                      |
| RIS   | Radiology Information System                       |
| PDU   | DICOM Protocol Data Unit                           |
| SC    | Secondary Capture                                  |
| SCU   | DICOM Service Class User (DICOM client)            |
| SCP   | DICOM Service Class Provider (DICOM server)        |
| SID   | Source Image Receptor Distance                     |
| SOD   | Source Object Distance                             |
| SOP   | DICOM Service-Object Pair                          |
| U     | Unique Key Attribute                               |
| UI    | User Interface                                     |
| UID   | Unique Identifier                                  |
| US    | Ultrasound   |
| XA    | X-Ray Angiography                                  |
| XRF   | X-Ray Radiofluoroscopy                             |

## 1.6 References

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-3.20, 2017b.

[XWP] DICOM Conformance Statement VD20, *syngo* X Workplace with *syngo* Application Software, Siemens Healthineers.

The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>.

## 1.7 Structure

The *syngo* FLC Conformance Statement is subdivided into three Parts which relate to individual documents needed to declare Conformance according to the requirements of "Part 2 – Conformance" of the DICOM Standard.

Those parts are:

- “DICOM Conformance Statement” for Network related Services
- “Offline Media Conformance Statement” to support local archive media.
- A general Appendix.

## 2 Implementation Model Verification

The syngo FLC DICOM application requests Verification to verify the ability of another DICOM application on a remote node to respond to DICOM messages.

Responding to Verification requests from remote nodes is handled by the Storage SCP application.

### 2.1 Application Data Flow Diagram

The syngo FLC DICOM application acts as SCU for the C-ECHO DICOM network service.

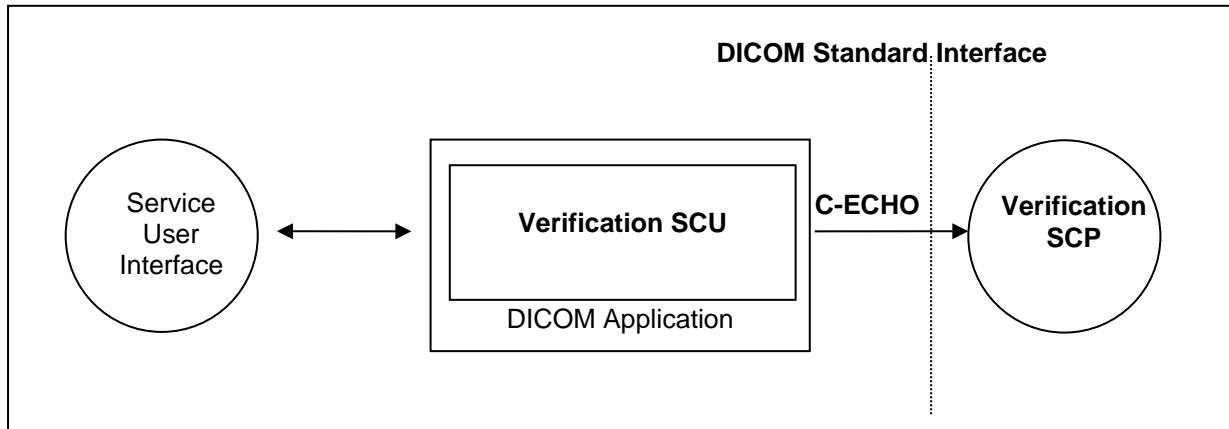


Figure 1: FLUOROSPOT Compact Application Flow Diagram – Verification SCU

### 2.2 Functional Definitions of Applications

The Siemens syngo FLC DICOM application opens an association when a “C-ECHO” of a remote application is requested from the Service User Interface. This can be done to verify the correct setup of a remote destinations configuration data.

### 2.3 Sequencing of Real-World Activities

Not applicable

### 3 Application Entity Specification Verification

#### 3.1 Verification AE Specification

##### 3.1.1 Association Establishment Policies

###### 3.1.1.1 General

The Siemens syngo FLC DICOM application attempts to open an association for verification request whenever the “C-Echo” function is activated.

###### 3.1.1.2 Number of Associations

The Siemens syngo FLC DICOM application initiates one association at a time to request verification.

###### 3.1.1.3 Asynchronous Nature

The Siemens syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

###### 3.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 3.1.2 Association Initiation Policy

The Siemens syngo FLC DICOM application attempts to initiate a new association for

- DIMSE C-ECHO  
service operations.

##### 3.1.2.1 Associated Real-World Activity

###### 3.1.2.1.1 Associated Real-World Activity – C-Echo

The associated Real-World activity is a C-ECHO request initiated by Service User Interface environment whenever a verification of a destination configuration is requested. If an association to a remote Application Entity is successfully established, verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application is received, a message will be displayed indicating that the C-Echo was successful, and the association is closed.

### 3.1.2.1.2 Proposed Presentation Contexts

The Siemens syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table – Verification SCU |                   |   |   |      |           |
|---|-------------------|---|---|------|-----------|
| Abstract Syntax                               |                   | Transfer Syntax   |   | Role | Ext. Neg. |
| Name  | UID               | Name List   | UID List  |      |           |
| Verification                                  | 1.2.840.10008.1.1 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

### 3.1.2.1.3 SOP Specific Conformance – Verification SCU

None.

## 3.1.3 Association Acceptance Policy

The Verification SCP is part of the Storage SCP – see section 5.1.3.

## 4 Implementation Model Storage

The Siemens syngo FLC DICOM Application Entity originates associations for Storage of DICOM Composite Information Objects in Remote Application Entities and receives association requests for Storage from Remote Application Entities.

“Send to...” is performed on the user’s request for each study completed or for specific images selected.

“Send to...” can also be performed for images, which are deleted (copy to Recycle Bin) but have not been archived yet.

### 4.1 Application Data Flow Diagram

The syngo FLC DICOM application acts as SCU and SCP for the C-STORE DICOM network service and as SCP for the C-ECHO DICOM network service.

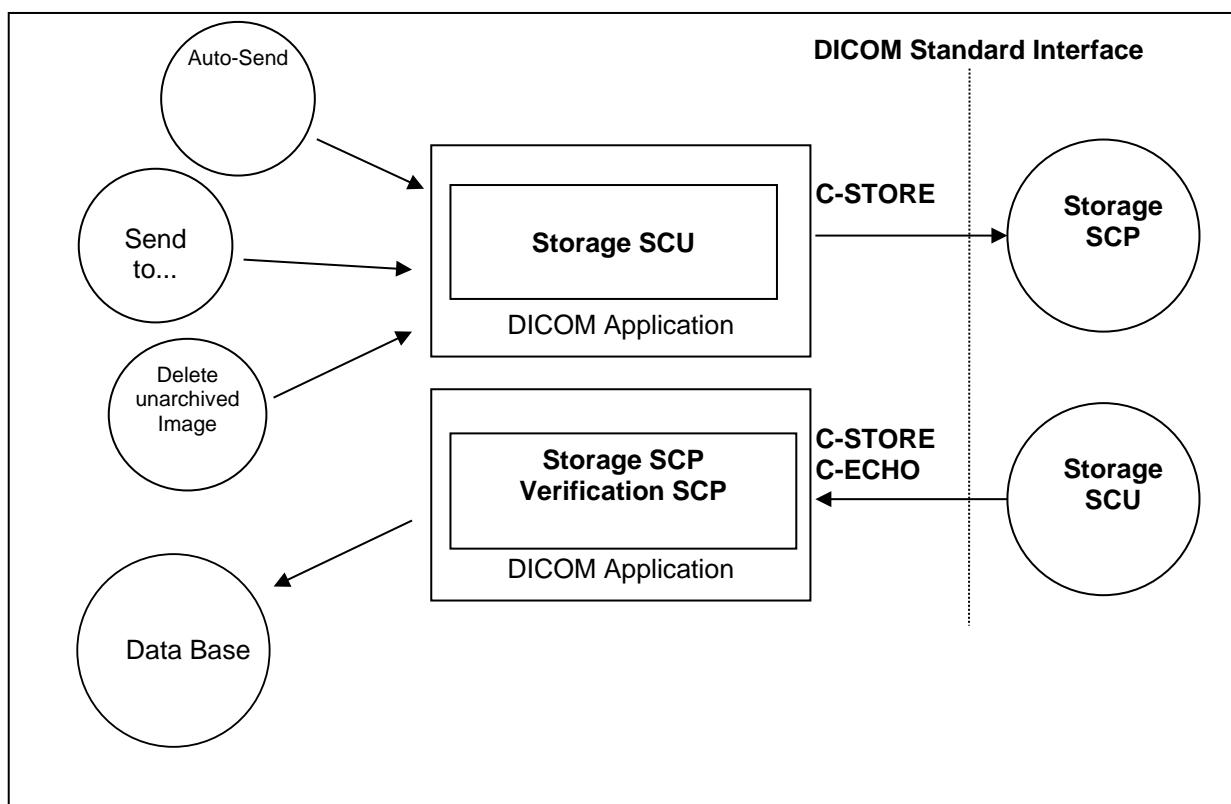


Figure 2: FLUOROSPOT Compact Application Data Flow Diagram – Storage SCU/SCP, Verification SCP

### 4.2 Functional Definitions of Application Entities

With “Send to...” the marked images can be sent automatically to multiple destinations (up to 3). Each request is forwarded to the job queue and processed individually. For each destination it can be configured during Service session, which IOD type (selection depending on system type) has to be used when sending images. For multiple destinations it is required, that all of the desired destination will support the same IOD type. If this is not the case, then only one target at a time can be addressed.

With “Send to...” initiated on user’s request in patient mode selected studies can be exported to a DICOM node chosen from a list of configured destinations.

With "Send to..." also the "Exam Protocol as Secondary Captured Image" and the DICOM Dose Structured Report can be send to defined network destinations.

With "Auto Send" the "Send To..." mechanism is invoked automatically for a set of predefined or marked images. The rules and destinations for "Auto Send" can be configured in the OGP editor and can be specified for each OGP.

With "Delete unarchived image" an image will be copied into the local Recycle Bin. Additionally for this image a "Send To..." could be invoked to a selected DICOM node.

The Storage SCU is invoked by the job control interface that is responsible for processing network archival tasks. The job consists of data describing the composite image objects marked for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported through the job control interface. Only one job will be active at a time.

The Storage SCP component of the Siemens syngo FLC DICOM application is operating as background server process. It is running when the system is triggered to import images and waits then for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database.

Verification requests will be processed and responded by the Storage SCP.

#### **4.3 Sequencing of Real-World Activities**

not applicable

## 5 Application Entity Specification Storage

### 5.1 Storage AES Specification

The syngo FLC Storage SCU/SCP applications use two different AETs when initiating/receiving associations to/from remote DICOM nodes.

The syngo FLC imaging system supports several SIEMENS X-Ray acquisition modalities. SOP Classes used for storage depend on the acquisition system. syngo FLC provides Standard Conformance to the following DICOM SOP Classes as SCU:

| SOP Class Name  | SOP Class UID                 |
|---|-------------------------------|
| Secondary Capture Image Storage                                     | 1.2.840.10008.5.1.4.1.1.7     |
| X-Ray Radiation Dose SR   | 1.2.840.10008.5.1.4.1.1.88.67 |
| X-Ray Angiographic Image Storage <sup>1</sup>                       | 1.2.840.10008.5.1.4.1.1.12.1  |
| X-Ray Radiofluoroscopic Image Storage <sup>2</sup>                  | 1.2.840.10008.5.1.4.1.1.12.2  |
| Computed Radiography Image Storage <sup>3</sup>                     | 1.2.840.10008.5.1.4.1.1.1     |
| Digital X-Ray Image Storage – For Presentation <sup>3</sup>         | 1.2.840.10008.5.1.4.1.1.1.1   |
| Multi-frame True Color Secondary Capture Image Storage <sup>4</sup> | 1.2.840.10008.5.1.4.1.1.7.4   |

SIEMENS syngo FLC imaging system provides Standard Conformance to the following DICOM SOP Classes as SCP:

| SOP Class Name   | SOP Class UID                |
|--|------------------------------|
| Secondary Capture Image Storage                        | 1.2.840.10008.5.1.4.1.1.7    |
| X-Ray Angiographic Image Storage                       | 1.2.840.10008.5.1.4.1.1.12.1 |
| X-Ray Radiofluoroscopic Image Storage                  | 1.2.840.10008.5.1.4.1.1.12.2 |
| Computed Radiography Image Storage                     | 1.2.840.10008.5.1.4.1.1.1    |
| Digital X-Ray Image Storage – For Presentation         | 1.2.840.10008.5.1.4.1.1.1.1  |
| Multi-frame True Color Secondary Capture Image Storage | 1.2.840.10008.5.1.4.1.1.7.4  |
| CT Image Storage                                       | 1.2.840.10008.5.1.4.1.1.2    |
| MR Image Storage                                       | 1.2.840.10008.5.1.4.1.1.4    |
| Ultrasound Image Storage                               | 1.2.840.10008.5.1.4.1.1.6.1  |

<sup>1</sup> Only for Multitom Rax

<sup>2</sup> Only for Fluorosystems

<sup>3</sup> Only for Radsystems

<sup>4</sup> Only for UROSKOP Omnia

|                                     |                             |
|-------------------------------------|-----------------------------|
| Ultrasound Multiframe Image Storage | 1.2.840.10008.5.1.4.1.1.3.1 |
| Verification                        | 1.2.840.10008.1.1           |

## 5.1.1 Association Establishment Policies

### 5.1.1.1 General

The existence of a job queue entry with network destination will activate the DICOM Storage Application. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the transfer is started. If the association cannot be opened, the related job is set to an error state and can be restarted by user job control interface. It is configurable by the CSE if a retry for failed jobs is initiated automatically.

The default PDU size used will be 64 KB.

### 5.1.1.2 Number of Associations

The syngo FLC DICOM application initiates one association at a time, subsequently for each destination to which a transfer request is being processed in the active job queue list. Only one job will be active at a time, the others remain pending until the active job is completed or failed.

### 5.1.1.3 Asynchronous Nature

The syngo FLC software does not support asynchronous communication (multiple outstanding transactions over a single association).

### 5.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

## 5.1.2 Association Initiation Policy

If a job with network destination gets active in the job list the syngo FLC DICOM application attempts to initiate a new association for

- DIMSE C-STORE service operations.

### 5.1.2.1 Associated Real-World Activity – Storage SCU

#### 5.1.2.1.1 Associated Real-World Activity –Send to ...

The associated Real-World activity is a C-STORE request initiated by an internal daemon process triggered by a job with network destination. If the process successfully establishes an association to a remote Application Entity, it will transfer each marked image one after another via the open association. The used storage IOD is depending on the system type and on the destination's configuration. If the C-STORE Response from the remote Application contains a status other than Success or Warning, the association is aborted. The related job is switched to a failed state. It can be restarted any time by user interaction. An automatic retry can be configured by the CSE.

Processing of images of a send job and sending of processed images is done in parallel. That means, as soon as the first image of a job is processed an association is initiated and the sending of the processed image is started.

An established association is closed as soon as no processed image is available to be sent.

**Due to different speeds of sending and processing the syngo FLC might initiate more than one association for each send job!**

### 5.1.2.1.2 Proposed Presentation Context –Send to...

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table  |                               |   |   |      |           |
|---|-------------------------------|---|---|------|-----------|
| Abstract Syntax   |                               | Transfer Syntax   |   | Role | Ext. Neg. |
| Name  | UID                           | Name List   | UID List  |      |           |
| Computed Radiography Image Storage Service Class <sup>1</sup>       | 1.2.840.10008.5.1.4.1.1.1     | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| Digital X-Ray Image Storage – For Presentation <sup>1</sup>         | 1.2.840.10008.5.1.4.1.1.1     | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| Secondary Capture Image Storage Service Class                       | 1.2.840.10008.5.1.4.1.1.7     | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| X-Ray Radiation Dose SR   | 1.2.840.10008.5.1.4.1.1.88.67 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| X-Ray Angiographic Image Storage Service Class <sup>2</sup>         | 1.2.840.10008.5.1.4.1.1.12.1  | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| X-Ray Radiofluoroscopic Image Storage Service Class <sup>3</sup>    | 1.2.840.10008.5.1.4.1.1.12.2  | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |
| Multi-frame True Color Secondary Capture Image Storage <sup>4</sup> | 1.2.840.10008.5.1.4.1.1.7.4   | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

If multiple destinations are addressed within one network job, then all of those are required to support the same IOD.

### 5.1.2.1.3 SOP specific Conformance Statement –Send to...

The DICOM images created by the DICOM interface of the syngo FLC conform to the DICOM CR, XRF, XA, DX or Multi-frame True Color Secondary Capture IOD definitions. Private elements are contained in the objects. The IODs will be a Standard Extended Image Storage SOP Classes.

The DICOM Dose Structured Report created by the DICOM interface of the syngo FLC conforms to the X-Ray Radiation Dose SR IOD definitions. Private elements are contained in the objects.

Image Laterality (0020,0062) and Patient Orientation (0020,0020) might not be included in Images sent in DX IOD.

For the projection images that are used for 3D reconstruction Multitom Rax uses the X-Ray Angiographic Image Storage Service Class. The reconstruction is carried out on a different workstation. The resulting 3D images will be encoded as CT Image Storage SOP Class. Details can be found in [XWP]. Please refer to A.7 for the definition of the attributes that are specific for XA objects used for the projection images.

Imported DICOM images cannot be exported again.

#### 5.1.2.1.3.1 Optional Attributes

<sup>1</sup> Only for radsystems

<sup>2</sup> Only for Multitom Rax

<sup>3</sup> Only for Fluorosystems

<sup>4</sup> Only for Uroskop Omnia

A list of all DICOM IOD attributes of type 2 and 3 which are encoded by the syngo FLC applications can be found in the APPENDIX (page 74 ff).

### 5.1.2.1.3.2 Image Pixel Attribute Description for Grayscale Images

The Siemens syngo FLC DICOM application supports the “MONOCHROME 2” Photometric Interpretation with the unsigned integer 16-bit (8 bit for downsized images) gray scale pixel format:

### 5.1.3 Association Acceptance Policy

The syngo FLC DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

service operations. Any Information Objects transmitted on that association will be checked on conformance and stored in database if check was successful.

#### 5.1.3.1 Associated Real-World Activity – Storage SCP

##### 5.1.3.1.1 Associated Real-World Activity – Receiving Images from a Remote Node (with Retrieve)

Receiving is possible whenever an import request (C-MOVE) is sent to a remote destination. As long as it is active, the receiver process will accept an association and will receive images transmitted on that association and will store the images on disk in the own data base if the conformance check is performed successfully.

The syngo FLC DICOM application is designed for retrieving images that were acquired by the system itself.

The syngo FLC DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table                                   |                              |  |   |      |           |
|--|------------------------------|--|---|------|-----------|
| Abstract Syntax  |                              | Transfer Syntax  |   | Role | Ext. Neg. |
| Name   | UID                          | Name List  | UID List  |      |           |
| Computed Radiography Image Storage Service Class             | 1.2.840.10008.5.1.4.1.1.1    | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| Digital X-Ray Image Storage – For Presentation               | 1.2.840.10008.5.1.4.1.1.1.1  | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| Secondary Capture Image Storage Service Class                | 1.2.840.10008.5.1.4.1.1.7    | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| X-Ray Radiofluoroscopic Image Storage Service Class          | 1.2.840.10008.5.1.4.1.1.12.2 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| X-Ray Angiographic Image Storage Service Class               | 1.2.840.10008.5.1.4.1.1.12.1 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.  | SCP  | None      |
| Multi-frame True Color Secondary Capture Image Storage Class | 1.2.840.10008.5.1.4.1.1.7.4  | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| CT Image Storage   | 1.2.840.10008.5.1.4.1.1.2    | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| MR Image Storage   | 1.2.840.10008.5.1.4.1.1.4    | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| Ultrasound Image Storage                                     | 1.2.840.10008.5.1.4.1.1.6.1  | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |
| Ultrasound Multi-frame Image Storage                         | 1.2.840.10008.5.1.4.1.1.3.1  | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP  | None      |

| Presentation Context Table |                   |   |   |     |      |
|----------------------------|-------------------|---|---|-----|------|
| Abstract Syntax            |                   | Transfer Syntax   |   |     | Ext. |
| Verification               | 1.2.840.10008.1.1 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCP | None |

### 5.1.3.1.2 SOP-specific Conformance Statement – Receiving Images from a Remote Node (with Retrieve)

The syngo FLC DICOM application conforms to the Full Storage Class at Level 1. In the event of a successful C-STORE operation, the image has successfully been written on disk.

The syngo FLC DICOM receiver returns the status Success upon successful operation otherwise one of the following status codes is returned and the association is aborted:

- **Refused (A700):**  
This error status indicates a lack of Resources (e.g. not enough disk space) on the syngo FLC modality.
- **Error (A900 or C000):**  
An error occurred while processing the image that makes it impossible to proceed. The image will not be stored and the association aborted.  
If an image instance is received that is identified by a SOP Instance UID that is already used by an Instance stored in database then the actual received image will be refused. The existing Instance is not superseded.

#### 5.1.3.1.2.1 Image Pixel Attribute Description for Receiving of Images

The syngo FLC DICOM receiver accepts pixel data with unsigned integer and 8 or 16 bits allocated.

Accepted values:

##### Pixel plane

- Samples per Pixel (0028,0002) = 1
- Photometric Interpretation (0028,0004) = "MONOCHROME2" + "RGB"
- Only Pixel Aspect Ratio (0028,0034) 1:1 is supported
- Pixel Representation (attribute 0028,0103) = 0
- Bits Allocated (0028,0100) = 8, 16
- Bits Stored (0028,0101) = 8, 10, 12, 16
- High Bit (0028,0102) = 7, 9, 11, 15

Furthermore following restrictions are valid:

- For VOI LUT, only the linear LUT (Window Center/Width) and not the VOI LUT Sequence is supported.
- Display of overlay planes is not supported.
- No manipulations except windowing are allowed on imported images not generated by a syngo FLC imaging system.
- Multiframe objects with identical image type are expected to be separated in series level.

#### 5.1.3.1.3 Presentation Context Acceptance Criterion

The syngo FLC DICOM application will accept any number of verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to the maximum of

127 (DICOM limit). In the event that the syngo FLC DICOM application runs out of resources, it will reject the association request.

#### **5.1.3.1.4 Transfer Syntax Selection Policies**

The syngo FLC DICOM application currently supports the Implicit VR LittleEndian, the Explicit VR LittleEndian and Explicit VR BigEndian Transfer Syntaxes

Any proposed presentation context including one of these transfer syntaxes will be accepted. Any proposed presentation context that does not include one of these transfer syntaxes will be rejected. Explicit LittleEndian Transfer Syntax will be preferred over the implicit Default Transfer Syntax.

The syngo FLC DICOM application will remove any Private Attributes not known to the application.

## 6 Implementation Model Storage Commitment

The Storage Commitment Service Class defines an application-level class-of-service that facilitates commitment of storage. The Storage Commitment Service Class enables an Application Entity (AE) acting as SCU to request another Application Entity (AE) acting as an SCP to make the commitment for the safekeeping of the SOP Instances (i.e. that the SOP Instances will be kept for an implementation specific period of time and can be retrieved).

The syngo FLC DICOM application will support the Storage Commitment Push Model SOP Class as SCU.

### 6.1 Application Data Flow Diagram

“Send Image complete” is performed as a result of a completed Storage request. Successful completion of a Send to... request will result in automated initiation of a Storage Commitment Service. Each request results in an initiation for an association. The association will be closed after a maximum of 10 seconds (configurable in Service) of waiting for the response. After that receiving the Storage Commitment status is expected on a different association.

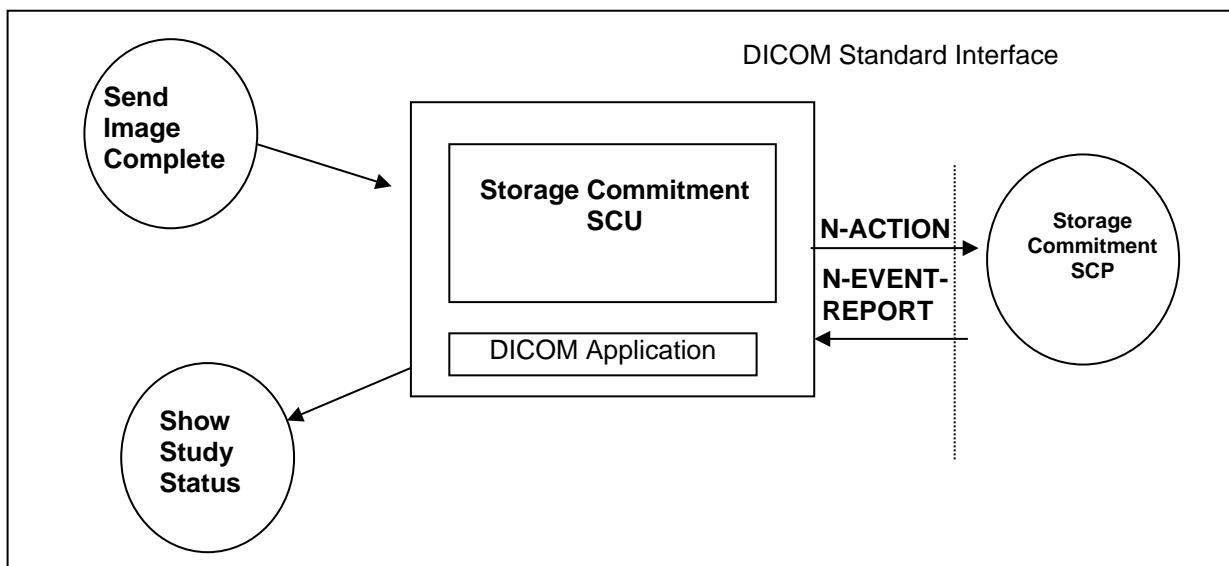


Figure 3: FLUOROSPOT Compact Application Data Flow Diagram – Storage Commitment

### 6.2 Functional Definitions of Application Entities

With each successfully completed send operation the syngo FLC DICOM Application will create a Storage Commitment Push Model Identifier from the SOP Instances sent. Then a Storage Commit Request is triggered. The syngo FLC will wait up to 10 seconds for responses, after that it expects the related response-trigger on a different association.

The commitment status derived from the related trigger response will be indicated in the Study list. Additionally the status will be evaluated previously to delete operations to inform the user about possible loss of information due to incomplete send operations and/or commit failures.

In any case, commitment will only be requested for previously and successfully sent images.

Storage Commitment is possible to different configured network nodes. Each Storage SCP can have its own Storage Commitment Server associated.

## 6.3 Sequencing of Real-World Activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send operation.

## 7 AE Specification Storage Commitment

### 7.1 Storage Commitment AE Specification

The syngo FLC DICOM application will use one AE when performing Storage Commitment request and when awaiting notification from the Storage Commitment Provider.

SIEMENS syngo FLC DICOM products provide Standard Conformance to the following DICOM SOP Classes as SCU:

| SOP Class Name                | SOP Class UID        |
|-------------------------------|----------------------|
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 |

#### 7.1.1 Association Establishment Policies

##### 7.1.1.1 General

The DICOM application will generate a Storage Commitment Identifier which references to all Instances of a selected study in the scope of the syngo FLC application. The request is then sent over a single opened association. The syngo FLC will wait for status responses to the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success status, the generated Transaction UID, together with study identification data and a time-stamp, is kept in a Pending Request Queue. The association is then closed. Multiple Storage Commitment Requests can be held in the Pending Request Queue.

The default PDU size used will be 64 KB.

##### 7.1.1.2 Number of Associations

The syngo FLC will initiate one association to send Storage Commitment requests to a configured Archive destination.

##### 7.1.1.3 Asynchronous Nature

The syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

##### 7.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 7.1.2 Association Initiation Policy

If a Storage Commitment Request needs to be sent to an Archive destination the syngo FLC DICOM application attempts to initiate a new association for

- DIMSE N-ACTION service operations.

### 7.1.2.1 Real World Activity – Storage Commitment SCU

#### 7.1.2.1.1 Associated Real-World Activity – Send Image Complete

Whenever a Store Request to a Storage SCP with associated Storage Commitment SCP is completed in the job queue, a Storage Commitment Identifier is generated for the same scope of Instances as transferred through the successful Storage Request. The identifier is then sent with the N-ACTION service to the Storage Commitment SCP. The association will wait up to 10 seconds for responses after the Storage Commitment Provider accepted the request. Storage Commitment SCP nodes can be configured by the CSE.

A number of retries for failed commit requests and a Storage Commitment timeout can be configured in User Settings.

#### 7.1.2.1.2 Proposed Presentation Contexts –Send Image Complete

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table    |                      |  |   |      |           |
|-------------------------------|----------------------|--|---|------|-----------|
| Abstract Syntax               |                      | Transfer Syntax  |   |      | Ext. Neg. |
| Name                          | UID                  | Name List  | UID List  | Role |           |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

#### 7.1.2.1.3 SOP-specific Conformance Statement – Send Image Complete

The syngo FLC DICOM application will NOT support the Storage Media File Set ID attributes.

SIEMENS syngo FLC DICOM application will request Storage commitment for the following SOP Classes as SCU:

| SOP Class Name  | SOP Class UID                |
|---|------------------------------|
| Computed Radiography Image Storage <sup>1</sup>             | 1.2.840.10008.5.1.4.1.1.1    |
| Secondary Capture Image Storage                             | 1.2.840.10008.5.1.4.1.1.7    |
| X-Ray Radiofluoroscopic Image Storage <sup>2</sup>          | 1.2.840.10008.5.1.4.1.1.12.2 |
| Digital X-Ray Image Storage – For Presentation <sup>1</sup> | 1.2.840.10008.5.1.4.1.1.1.1  |

### 7.1.3 Association Acceptance Policy

The syngo FLC Storage Commitment DICOM application attempts to accept a new association for

- DIMSE N-EVENT-REPORT service operations.

<sup>1</sup> Only for Radsystems

<sup>2</sup> Only for Fluorosystems

### 7.1.3.1 Real World Activity – Storage Commitment SCU

#### 7.1.3.1.1 Associated Real-World Activity – Show Study Status

Consecutive to start-up, the syngo FLC DICOM application will await Storage commitment Notification triggers. Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue. If not, the related Notification trigger is rejected with an “Unable to process” error. The related study is already set to commit failed due to time-out on notification.

If the Notification is valid, the Notification Identifier is evaluated and the related Instances are marked with the related status. The over-all Commit Status of the study is derived from propagation of the States of all instances included by a study.

The Study Status indicated in the Study list can be one of

- <no Status> (-) [not sent or send failed]
- Sent (S) [all images successfully sent to DICOM Send node, commitment successful for the complete study]
- Partially Sent (s) [some or all instances of the Study successfully sent to DICOM Send node, commitment outstanding for at least 1 image of the study]
- Archived (A) [all images successfully sent to Archive node, commitment successful for the complete study]
- Partially Archived (a) [some or all instances of the Study successfully sent to Archive node, commitment outstanding for at least 1 image of the study]

The syngo FLC delete function will be sensitive on the Study Status and will protect Studies. The user can override the protection by confirming the respective delete dialogues.

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

#### 7.1.3.1.2 Accepted Presentation Contexts –Show Study Status

The syngo FLC DICOM application will accept Presentation Contexts as shown in the following table:

| Presentation Context Table    |                      |  |   |        |           |
|-------------------------------|----------------------|--|---|--------|-----------|
| Abstract Syntax               |                      | Transfer Syntax  |   | Role   | Ext. Neg. |
| Name                          | UID                  | Name List  | UID List  |        |           |
| Storage Commitment Push Model | 1.2.840.10008.1.20.1 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU *1 | None      |

\*1 according to the rules defined for Storage Commitment N-EVENT-REPORT, the syngo FLC itself assumes the SCU role and therefore accepts the SCP role negotiation of the Storage Commitment Provider, even if initiator of the association negotiation.

#### 7.1.3.1.3 SOP-specific Conformance Statement – Show Study Status

The syngo FLC DICOM application will NOT support the Storage Media File Set ID attributes.

## 8 Implementation Model Query / Retrieve

The query/retrieve service class defines an application-level class of services that facilitates the management of images and patient data against the well-defined information model of DICOM and allows a DICOM AE to retrieve images from a remote DICOM node. The syngo FLC DICOM query/retrieve application supports the query/retrieve services to act as SCU.

### 8.1 Application Data Flow Diagram

The syngo FLC DICOM application acts as SCU for the query/retrieve network service.

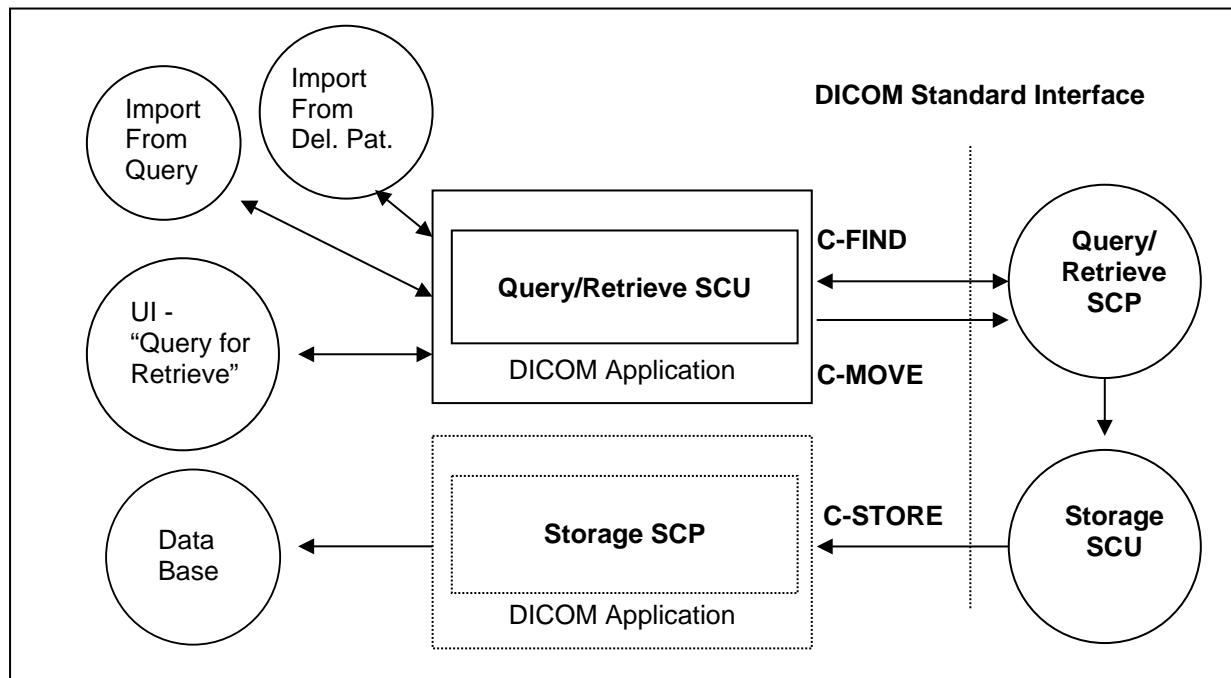


Figure 4: FLUOROSPOT Compact Application Data Flow Diagram – Query/Retrieve SCU

### 8.2 Functional Definitions of Application Entities

The syngo FLC DICOM query/retrieve SCU requests the remote query/retrieve SCP to perform a search (C-FIND) and match to the keys specified in the request in order to display the results in the syngo FLC user interface. If the defined limit of Query results is reached, the syngo FLC will cancel the running query and discard any further incoming query result responses. Queries can be operated in parallel to one running import (C-MOVE) activity.

Depending on user action (Import) the syngo FLC DICOM query/retrieve SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the syngo FLC Storage SCP. The user has the possibility to cancel a running import by an "Import Cancel" function. The syngo FLC DICOM application will perform only one running import operation at a time.

### 8.3 Sequencing of Real-World Activities

Import operation has to be completed or successfully canceled before a new import can be initiated at the user interface.

## 9 AE Specification Query/Retrieve

### 9.1 Query/Retrieve Service Aes Specification

The Query/Retrieve SCU requests that the remote SCP performs a match of all keys specified in the request, against the information in its database.

SIEMENS syngo FLC DICOM products provide Standard Conformance to the following DICOM SOP Classes as SCU:

| SOP Class Name                                     | SOP Class UID               |
|--|-----------------------------|
| Study Root Query/Retrieve Information Model – FIND | 1.2.840.10008.5.1.4.1.2.2.1 |
| Study Root Query/Retrieve Information Model – MOVE | 1.2.840.10008.5.1.4.1.2.2.2 |

#### 9.1.1 Association Establishment Policies

##### 9.1.1.1 General

With the “Query for Retrieve” function the query data are input and the DICOM query/retrieve application is started. A query request will be sent out to the selected remote node and the response data will be displayed for the user. Upon request (Import), the retrieval of selected items is initiated.

Running Query requests will be automatically canceled whenever the defined limit has been reached. A running import can be canceled upon user's request.

The default PDU size used will be 64 KB.

##### 9.1.1.2 Number of Associations

The syngo FLC DICOM application initiates one association for each query request being processed to a remote node. Only one Import (C-MOVE) request can be active at a time.

##### 9.1.1.3 Asynchronous Nature

The syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

##### 9.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 9.1.2 Association Initiation Policy

The query user interface will request the query-data (combined input of patient- and study-related data) from user and triggers one or more C-FIND request to the selected remote node. The response data will be displayed in the query UI as a combined Patient/Study list. Navigation (further queries) to Series-Level is supported by the syngo FLC, navigation to Image-Level is not

supported. A running Query will be canceled (C-CANCEL) by the DICOM Application if the response limit has been reached.

When requesting Import of a related item, the browser requests the DICOM retrieve application to send a C-MOVE request to the related remote node. SOP Instances will then be received by the Storage SCP as described in the related section. An import can be terminated by user request (C-CANCEL).

### 9.1.2.1 Real World Activity – Find SCU

#### 9.1.2.1.1 Associated Real-World Activity – Query for Retrieve

The associated Real-World activity is to fill out a query form with search data and pass it as a query request to the network application that issues one or more C-FIND requests over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. When data transfer is finished, the association is closed.

In case of error, the list is built up to the point where the error occurred. The user is informed about incomplete processing of the query results.

#### 9.1.2.1.2 Proposed Presentation Contexts – Query for Retrieve

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                   |                             |   |   |      |           |
|--|-----------------------------|---|---|------|-----------|
| Abstract Syntax                              |                             | Transfer Syntax   |   | Role | Ext. Neg. |
| Name   | UID                         | Name List   | UID List  |      |           |
| Study Root<br>Query/Retrieve Model –<br>FIND | 1.2.840.10008.5.1.4.1.2.2.1 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

Extended Negotiation to request “relational query” is not supported by the syngo FLC DICOM application.

### 9.1.2.1.3 SOP Specific Conformance Statement – Query for Retrieve

The syngo FLC DICOM Query/Retrieve SCU supports hierarchical queries with the search keys listed below. The Query SCU does not support the interactive querying of attributes on IMAGE level. The following table describes the matching keys/ return keys that the SCU supports:

| Attribute Name                     | Tag         | Type  | Matching                        | User Input            | Return Value Display |
|------------------------------------|-------------|-------|---------------------------------|-----------------------|----------------------|
| <b>Patient Level</b>               |             |       |                                 |                       |                      |
| Patient's Name <sup>1</sup>        | (0010,0010) | R     | Wildcard                        | Enter value           | Yes                  |
| Patient ID                         | (0010,0020) | U / R | Wildcard                        | Enter value           | Yes                  |
| Patient's Birth Date               | (0010,0030) | O     | Universal (Null)                | Enter value           | Yes                  |
| Patient's Sex                      | (0010,0040) | O     | Universal (Null)                | Select value          | Yes                  |
| <b>Study Level</b>                 |             |       |                                 |                       |                      |
| Study Instance UID                 | (0020,000D) | U     | Universal (Null) / Single Value | -- / Select from List | -- / Yes             |
| Study ID                           | (0020,0010) | R     | Universal (Null)                | Enter value           | No                   |
| Study Date                         | (0008,0020) | R     | Universal (Null)                | --                    | Yes                  |
| Study Time                         | (0008,0030) | R     | Universal (Null)                | --                    | Yes                  |
| Accession Number                   | (0008,0050) | R     | Universal (Null)                | Enter value           | Yes                  |
| Study Description                  | (0008,1030) | O     | Universal (Null)                | --                    | Yes                  |
| Number of Study Related Series     | (0020,1206) | O     | Universal (Null)                | --                    | Yes                  |
| Number of Study Related Instances  | (0020,1208) | O     | Universal (Null)                | --                    | Yes                  |
| <b>Series Level</b>                |             |       |                                 |                       |                      |
| Series Instance UID                | (0020,000e) | U     | Single Value                    | Select from List      | Yes                  |
| Series Number                      | (0020,0011) | R     | Universal (Null)                | --                    | Yes                  |
| Modality                           | (0008,0060) | R     | Universal (Null)                | --                    | Yes                  |
| Number of Series Related Instances | (0020,1209) | O     | Universal (Null)                | --                    | Yes                  |
| Series Description                 | (0008,103e) | O     | Universal (Null)                | --                    | Yes                  |

The Find SCU interprets following status codes:

| Service Status | Meaning  | Error Codes | Related Fields             |
|----------------|--|-------------|----------------------------|
| Refused        | Out of Resources   | A700        | (0000,0902)                |
| Failed         | Identifier does not match SOP Class  | A900        | (0000,0901)<br>(0000,0902) |
|                | Unable to process  | Cxxx        | (0000,0901)<br>(0000,0902) |
| Cancel         | Matching terminated due to Cancel request  | FE00        | None                       |
| Success        | Matching is complete – No final Identifier is supplied   | 0000        | None                       |
| Pending        | Matches are continuing – Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys          | FF00        | Identifier                 |
|                | Matches are continuing – Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier | FF01        | Identifier                 |

<sup>1</sup> In the Patient Name always a "\*" is added

## 9.1.2.2 Real-World Activity – Move SCU

### 9.1.2.2.1 Associated Real-World Activity – Import from Query

When selecting a data entry in the Query UI and activating the “Import” function, a retrieval request is passed to the archival application that issues a C-MOVE service according to the Study Root query model. (The Storage Service Class Conformance Statement SCP section describes the response behavior to the C-STORE request sub-operation that is generated by the SCP when processing the C-MOVE request.)

The transferred image data are processed as described in the Storage Class SCP descriptions.

The possibility to request the remote C-MOVE SCP to move data to an application entity other than the syngo FLC DICOM application is NOT USED.

### 9.1.2.2.2 Proposed Presentation Contexts – Import from Query

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                   |                             |   |   |      |           |
|--|-----------------------------|---|---|------|-----------|
| Abstract Syntax                              |                             | Transfer Syntax   |   | Role | Ext. Neg. |
| Name   | UID                         | Name List   | UID List  |      |           |
| Study Root<br>Query/Retrieve Model –<br>MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

### 9.1.2.2.3 SOP Specific Conformance Statement – Import from Query

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The syngo FLC will make use of the “list of UID” mechanism when specifying the Instances to be retrieved.

The Move SCU interprets following status codes:

| Service Status | Meaning  | Error Codes | Related Fields   |
|----------------|--|-------------|--|
| Refused        | Out of Resources – Unable to calculate number of matches   | A701        | (0000,0902)  |
|                | Out of Resources – Unable to perform sub operations        | A702        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Failed         | Identifier does not match SOP Class                        | A900        | (0000,0901)<br>(0000,0902)                               |
|                | Unable to process  | CXXX        | (0000,0901)<br>(0000,0902)                               |
| Cancel         | Sub-operations terminated due to Cancel Indication         | FE00        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Warning        | Sub-operations Complete – One or more Failures or Warnings | B000        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Success        | Sub-operations Complete – No Failures or Warning           | 0000        | (0000,1020)  |

| Service Status | Meaning                       | Error Codes | Related Fields   |
|----------------|-------------------------------|-------------|--|
|                |                               |             | (0000,1021)<br>(0000,1022)<br>(0000,1023)                |
| Pending        | Sub-operations are continuing | FF00        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |

#### 9.1.2.2.4 Associated Real-World Activity – Import from “Deleted Patients”

When selecting a data entry in the “Deleted Patients” UI and activate the “Import” function, a retrieval request is passed to the archival application which issues a C-MOVE service according to the Study Root query model. (The Storage Service Class Conformance Statement SCP section describes the response behavior to the C-STORE request sub-operation that is generated by the SCP when processing the C-MOVE request.). Instances can only be transferred to the system that originated the Import request.

The transferred image data are processed as described in the Storage Class SCP descriptions.

#### 9.1.2.2.5 Proposed Presentation Contexts – Import from “Deleted Patients”

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                   |                             |   |   |      |           |
|--|-----------------------------|---|---|------|-----------|
| Abstract Syntax                              |                             | Transfer Syntax   |   | Role | Ext. Neg. |
| Name   | UID                         | Name List   | UID List  |      |           |
| Study Root<br>Query/Retrieve Model –<br>MOVE | 1.2.840.10008.5.1.4.1.2.2.2 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

#### 9.1.2.2.6 SOP Specific Conformance Statement – Import from “Deleted Patients”

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The Move SCU interprets following status codes:

| Service Status | Meaning  | Error Codes | Related Fields   |
|----------------|--|-------------|--|
| Refused        | Out of Resources – Unable to calculate number of matches   | A701        | (0000,0902)  |
|                | Out of Resources – Unable to perform sub operations        | A702        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Failed         | Identifier does not match SOP Class                        | A900        | (0000,0901)<br>(0000,0902)                               |
|                | Unable to process  | CXXX        | (0000,0901)<br>(0000,0902)                               |
| Cancel         | Sub-operations terminated due to Cancel Indication         | FE00        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Warning        | Sub-operations Complete – One or more Failures of Warnings | B000        | (0000,1020)<br>(0000,1021)<br>(0000,1022)                |

| Service Status | Meaning  | Error Codes | Related Fields   |
|----------------|--|-------------|--|
|                |  |             | (0000,1023)  |
| Success        | Sub-operations Complete – No Failures or Warning | 0000        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |
| Pending        | Sub-operations are continuing                    | FF00        | (0000,1020)<br>(0000,1021)<br>(0000,1022)<br>(0000,1023) |

### 9.1.3 Association Acceptance Policy

Not applicable.

## 10 Implementation Model Modality Worklist

The Basic Worklist Management Service Class defines an application-level class-of-service that facilitates access to worklists. The worklist is queried by the AE (modality) and supplies the SCU with the tasks scheduled and which have to be performed on the modality. The syngo FLC DICOM application will support the Modality Worklist SOP class as SCU.

### 10.1 Application Data Flow Diagram

Worklist Update is performed as a result of an operator request. Each request results in an initiation for an association. Under normal condition the association will be closed after receiving a "Success" response from the Information System.

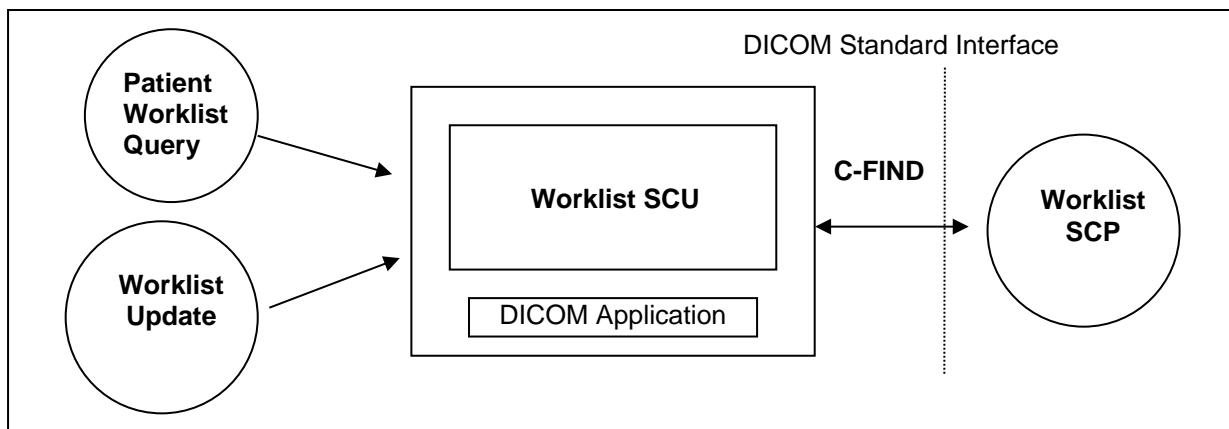


Figure 5: FLUOROSPOT Compact Application Data Flow Diagram – Modality Worklist

### 10.2 Functional Definitions of Application Entities

The request for a Worklist Update is initiated either by user interaction, i.e. pressing the button "Worklist Update" or automatically at configurable time intervals and at the switch from Patient Mode to Examination Mode. With "Worklist Update" the automated Query mechanism is performed immediately on request, while with "Patient Worklist Query" a dialog to enter search criteria is opened and an interactive query can be performed.

Upon initiation of the request, the syngo FLC will build an Identifier for the C-FIND request, will initiate an association to send the request and will wait for Worklist responses. After retrieval of all responses, syngo FLC will access the local database to add or update patient demographic data. To protect the system from overflow, the syngo FLC will limit the number of processed Worklist responses to a configurable maximum.

With automated worklist queries (including "Worklist Update") the syngo FLC always requests all items for a configured Scheduled Procedure Step Start Date, Modality Type and the Scheduled Station AE Title.

If any other SCP response status than "Success" or "Pending" is received by syngo FLC, a message "update failed" will appear on the user interface.

The syngo FLC Worklist Request Identifier is described in Annex A.10.

### 10.3 Sequencing of Real-World Activities

Not applicable.

## 11 AE Specification Modality Worklist

### 11.1 Modality Worklist Service Aes Specification

SIEMENS syngo FLC DICOM products provide Standard Conformance to the following DICOM SOP Classes as SCU:

| SOP Class Name                             | SOP Class UID          |
|--|------------------------|
| Modality Worklist Information Model – FIND | 1.2.840.10008.5.1.4.31 |

#### 11.1.1 Association Establishment Policies

##### 11.1.1.1 General

Worklist can be queried in automated mode – either cyclic or with “Update” – or with an interactive query with search criteria entered by application.

The default PDU size used will be 64 KB.

##### 11.1.1.2 Number of Associations

The syngo FLC DICOM application initiates one association at a time for a Worklist request.

##### 11.1.1.3 Asynchronous Nature

The syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

##### 11.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 11.1.2 Association Initiation Policy

The syngo FLC DICOM Application Entity acts as a Service Class User (SCU) for the Modality Worklist Service Class (to request a Worklist from a RIS).

To do so, the syngo FLC will issue a

- C-FIND DIMSE according to the Modality Worklist Information Model or a
- C-FIND-CANCEL DIMSE to stop processing of running worklist query.

##### 11.1.2.1 Real-World Activity

###### 11.1.2.1.1 Associated Real-World Activity – Patient Worklist Query

Patient Worklist Query will display a dialog for entering data as search criteria. When the Query is started on user request, only the data from the dialog will be inserted as matching keys into the query. An association is established and the query is sent. During receiving the worklist response items are counted and the query processing is canceled if the configurable limit of items (maximum **999**) is reached. The results will be displayed in a separate list. All worklist data from previous queries will be deleted when new data is received.

### 11.1.2.1.2 Proposed Presentation Contexts – Patient Worklist Query

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                 |                        |  |   |      |           |
|--|------------------------|--|---|------|-----------|
| Abstract Syntax                            |                        | Transfer Syntax  |   | Role | Ext. Neg. |
| Name                                       | UID                    | Name List  | UID List  |      |           |
| Modality Worklist Information Model – FIND | 1.2.840.10008.5.1.4.31 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

### 11.1.2.1.3 SOP Specific Conformance Statement – Patient Worklist Query

Please refer to Annex A.10 for the description of the syngo FLC Worklist Request Identifier.

If any other SCP response status than “Success” or “Pending” is received by syngo FLC, a message “query failed” will appear on the user interface.

### 11.1.2.1.4 Associated Real-World Activity –Worklist Update

Worklist Update attempts to download a Worklist from a remote node. If the syngo FLC AE establishes an association to a remote AE, it will transfer all worklist items via the open association. Also here the incoming worklist response items are counted and the query processing is canceled if the configurable limit of items (maximum **999**) is reached. The results will be displayed in a separate list. All worklist data from previous queries will be deleted when new data is received.

### 11.1.2.1.5 Proposed Presentation Contexts –Worklist Update

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                 |                        |  |   |      |           |
|--|------------------------|--|---|------|-----------|
| Abstract Syntax                            |                        | Transfer Syntax  |   | Role | Ext. Neg. |
| Name                                       | UID                    | Name List  | UID List  |      |           |
| Modality Worklist Information Model – FIND | 1.2.840.10008.5.1.4.31 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

### 11.1.2.1.6 SOP Specific Conformance Statement –Worklist Update

Please refer to Annex A.10 for the description of the syngo FLC Worklist Request Identifier.

If any other SCP response status than “Success” or “Pending” is received by syngo FLC, a message “update failed” will appear on the user interface.

### 11.1.3 Association Acceptance Policy

Not applicable.

## 12 Implementation Model Modality Performed Procedure Step

The syngo FLC DICOM application will support the Modality Performed Procedure Step (MPPS) SOP class as SCU.

### 12.1 Application Data Flow Diagram

MPPS Update is performed as a result of an operator request. Applying dose through acquisition of images or fluoroscopy mode will result in automated creation on a MPPS Instance. Each request results in an initiation for an association. The association will be closed after receiving a "Success" response from the Information System.

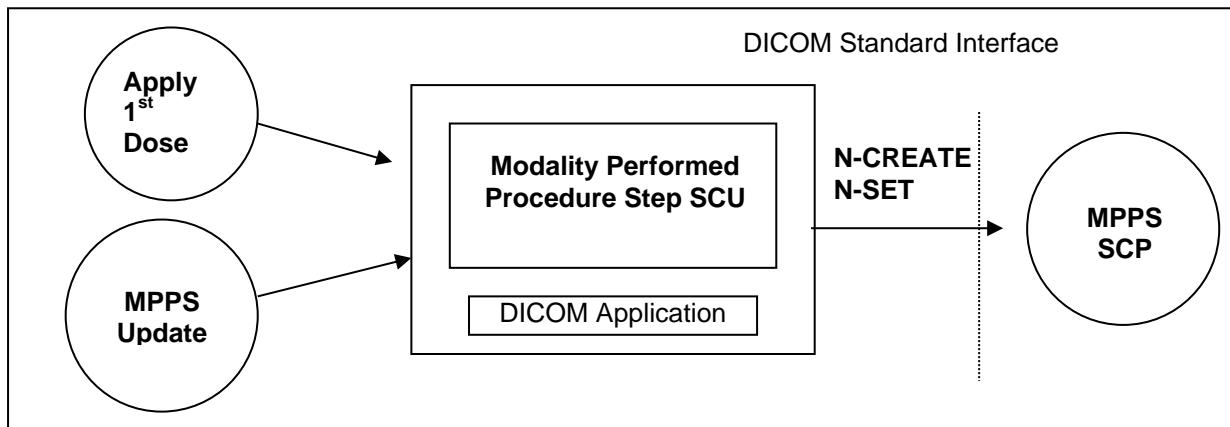


Figure 6: FLUOROSPOT Compact Application Data Flow Diagram – MPPS

### 12.2 Functional Definitions of Application Entities

With the 1<sup>st</sup> Dose applied consecutive to registering a Patient (Scheduled Procedure Step from Worklist), the syngo FLC DICOM application will create a MPPS Instance and communicate it to the MPPS SCP.

To inform the MPPS SCP about the progress or the completion of an MPPS instance, an update can be performed. It is configurable for the user how the update is performed:

- Automatic (status "COMPLETED" is sent after a patient gets inactive)
- Automatic with MPPS Dialog ("COMPLETED", "IN PROGRESS" or "DISCONTINUED" can be selected. Dialog is displayed after a patient gets inactive)
- Manual with MPPS Dialog ("COMPLETED", "IN PROGRESS" or "DISCONTINUED" can be selected.)

After a state of "COMPLETED" or "DISCONTINUED", the syngo FLC DICOM application will no longer allow updates on the related MPPS Instance.

The syngo FLC will support creation of "unscheduled cases" by allowing MPPS Instances to be communicated for locally registered Patients.

### 12.3 Sequencing of Real-World Activities

Not applicable.

## 13 AE Specification Modality Performed Procedure Step

### 13.1 Modality Performed Procedure Step Service Aes Specification

SIEMENS syngo FLC DICOM products provide Standard Conformance to the following DICOM SOP Classes as SCU:

| SOP Class Name                    | SOP Class UID           |
|-----------------------------------|-------------------------|
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 |

#### 13.1.1 Association Establishment Policies

##### 13.1.1.1 General

The creation of a MPPS Instance is done automatically by syngo FLC after the first application of radiation ("1<sup>st</sup> dose applied"). For emergency patients (patient data incomplete) the creation will be delayed until completion of the procedure step.

If the 1<sup>st</sup> dose is applied, while a worklist update is in progress, the MPPS N-Create is delayed until the next update of the Procedure Step.

Further updates on the MPPS data can either be done interactively from the related MPPS user interface or will automatically be performed if configured by the user.

The default PDU size used will be 64 KB.

##### 13.1.1.2 Number of Associations

The syngo FLC DICOM application initiates one association at a time for a communication of MPPS information.

##### 13.1.1.3 Asynchronous Nature

The syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

##### 13.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 13.1.2 Association Initiation Policy

The syngo FLC DICOM Application Entity acts as a Service Class User (SCU) for the Modality Performed Procedure Step Service Class (to notify a RIS about status of a procedure while it is performed).

To do so, the syngo FLC will issue a

- N-CREATE DIMSE according to the CREATE Modality Performed Procedure Step SOP Instance operation or a
- N-SET DIMSE to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

### 13.1.2.1 Real-World Activity

#### 13.1.2.1.1 Associated Real-World Activity – Apply 1<sup>st</sup> Dose

Consecutive to registration of Patient, the syngo FLC is awaiting the 1<sup>st</sup> application of radiation to the patient (“1<sup>st</sup> dose applied”). For emergency patients (patient data incomplete) the creation will be delayed until completion of the procedure step. From this event the trigger to create a MPPS Instance is derived. The related Instance is then immediately communicated to the configured RIS system. An association is established and the MPPS Instance is sent.

#### 13.1.2.1.2 Proposed Presentation Contexts – Apply 1<sup>st</sup> Dose

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table        |                         |   |   |      |           |
|-----------------------------------|-------------------------|---|---|------|-----------|
| Abstract Syntax                   |                         | Transfer Syntax   |   | Role | Ext. Neg. |
| Name                              | UID                     | Name List   | UID List  |      |           |
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 | Implicit VR LittleEndian<br>Explicit VR BigEndian<br>Explicit VR LittleEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

#### 13.1.2.1.3 SOP Specific Conformance Statement – Apply 1<sup>st</sup> Dose

Please refer to Annex A.11 for the description of the syngo FLC Modality Performed Procedure Step CREATE Request Identifier.

### 13.1.2.1.4 Associated Real-World Activity – MPPS Update

With a dedicated MPPS UI it is possible to set additional information and set the state to finalize the MPPS. Sending updates of the MPPS Instance can be interactively triggered. A MPPS Instance that has been sent with a state of “COMPLETED” or “DISCONTINUED” can no longer be updated.

A MPPS state of “COMPLETED” can also be sent automatically after a patient gets inactive. This automatic update without any user input is configurable for the user.

### 13.1.2.1.5 Proposed Presentation Contexts – MPPS Update

The syngo FLC DICOM application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table        |                         |  |   |      |           |
|-----------------------------------|-------------------------|--|---|------|-----------|
| Abstract Syntax                   |                         | Transfer Syntax  |   | Role | Ext. Neg. |
| Name                              | UID                     | Name List  | UID List  |      |           |
| Modality Performed Procedure Step | 1.2.840.10008.3.1.2.3.3 | Implicit VR Little Endian<br>Explicit VR Big Endian<br>Explicit VR Little Endian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.2<br>1.2.840.10008.1.2.1 | SCU  | None      |

### 13.1.2.1.6 SOP Specific Conformance Statement – MPPS Update

Please refer to Annex A.11 for the description of the syngo FLC Modality Performed Procedure Step SET Information Request Identifier.

The MPPS Set SCU interprets the following additional status code:

| Service Status     | Meaning  | Error Codes |
|--------------------|--|-------------|
| Processing Failure | Performed Procedure Step Object may no longer be updated | A710        |

If any other SCP response status than “Success” or “Pending” is received by syngo FLC, a message “MPPS update failed” will appear on the user interface.

### 13.1.3 Association Acceptance Policy

Not applicable.

## 14 Implementation Model Print

The Print Management Service Classes define an application-level class of services that facilitate the printing of images on a hardcopy medium. The print management SCU and the print management SCP are peer DICOM print management application entities. The syngo FLC DICOM print application supports the print management DIMSE services to act as SCU.

### 14.1 Application Data Flow Diagram

The syngo FLC DICOM application acts as SCU for the print management network service.

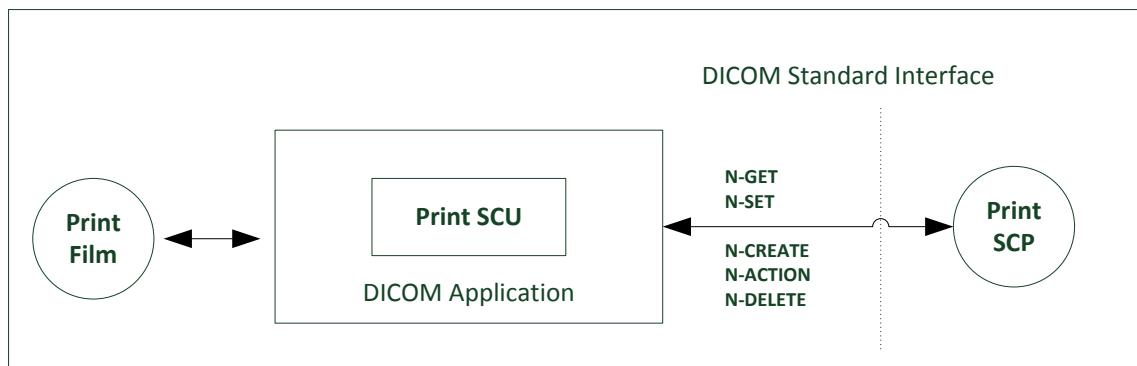


Figure 7: FLUOROSPOT Compact DICOM Application Data Flow Diagram – Print SCU

### 14.2 Functional Definition of Application Entities

The "Print Film" could either be invoked by the user interface whenever an image is ready to be printed on film, or automatically for a predefined set of images when study is completed.

The Print SCU will hold and maintain all data needed to compile a complete film-sheet from the data (images, layout, configuration) received. Whenever a film-sheet is ready to print, the related data is used to supply the information to the SOP Classes of the Basic Grayscale Print Management Meta SOP Class. A queue is maintained, in order to intermediately store up to 10 film-sheets in case of resource problems on printer. The SCU will only supply and require the mandatory SOP Classes of the Basic Grayscale Print Management Meta SOP Class.

It is configurable by the CSE to automatically initiate a retry for failed jobs.

### 14.3 Sequencing of Real-World Activities

Not applicable

## 15 Application Entity Specification Print

### 15.1 Print Management AE Specification

The syngo FLC print management SCU invokes print management DIMSE services to transfer images from the local AE to the remote SCP AE to print images with defined layout on a selected network-based DICOM hardcopy printer.

SIEMENS syngo FLC DICOM products provide Standard Conformance to the following DICOM Print Management Meta SOP Classes as SCU:

| SOP Class Name                                  | SOP Class UID         |
|---|-----------------------|
| Basic Grayscale Print Management Meta SOP Class | 1.2.840.10008.5.1.1.9 |

#### 15.1.1 Association Establishment Policies

##### 15.1.1.1 General

Whenever a film is completely set up, either automatically or by command, the job is prepared for processing. As soon as the queue is ready for processing the job, it is activated and encoded according the processing data. The related Print application will initiate an association to the print destination and process the printing of the related information.

The default PDU size used will be 64 KB.

##### 15.1.1.2 Number of Associations

The syngo FLC DICOM application initiates one association at a time for each different print device configured.

##### 15.1.1.3 Asynchronous Nature

The syngo FLC DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

##### 15.1.1.4 Implementation Identifying Information

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

#### 15.1.2 Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. With the help of the N-GET request for the Printer SOP Class the Status is determined before printing.

### 15.1.2.1 Associated Real-World Activity

#### 15.1.2.1.1 Associated Real-World Activity – Print Film

Whenever a film-sheet is prepared by the user, it is forwarded to the Printer Job queue. As soon as the associated Printer device is available the job is activated and association is set up.

The film sheet is set up with the related Film Session and Film Box services. The images are internally processed and then sent as image boxes as needed. Status is controlled by awaiting any N-EVENT message all through the transfer until the last image or film-sheet is sent.

If the response from the remote application contains a status other than “Success” or “Warning” the association is aborted. It can be restarted any time by user interaction. An automatic retry can be configured by a CSE. The syngo FLC displays all warning and failure messages in the DICOM Film job list and writes them also into a log file.

#### 15.1.2.1.2 Proposed Presentation Context – Print Film

The syngo FLC DICOM print application will propose Presentation Contexts as shown in the following table:

| Presentation Context Table                      |                        |   |   |      |           |
|---|------------------------|---|---|------|-----------|
| Abstract Syntax                                 |                        | Transfer Syntax   |   | Role | Ext. Neg. |
| Name  | UID                    | Name List   | UID List  |      |           |
| Basic Grayscale Print Management Meta SOP class | 1.2.840.10008.5.1.1.9  | Implicit VR LittleEndian<br>Explicit VR LittleEndian<br>Explicit VR BigEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU  | None      |
| Presentation LUT SOP class                      | 1.2.840.10008.5.1.1.23 | Implicit VR LittleEndian<br>Explicit VR LittleEndian<br>Explicit VR BigEndian | 1.2.840.10008.1.2<br>1.2.840.10008.1.2.1<br>1.2.840.10008.1.2.2 | SCU  | None      |

#### 15.1.2.1.3 SOP specific Conformance Statement – Meta SOP Classes

The syngo FLC DICOM print management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM Print SCP, e.g.:

- maximum number of print copies: **9**
- supported film sizes of the connected DICOM Print SCP
- supported film formats of the DICOM Print SCP

The printing is only suspended in the case of a failure return status of the Print SCP.

##### 15.1.2.1.3.1 Basic Film Session SOP class

The Basic Film Session information object definition describes all the user-defined parameters that are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes that are printed on one hardcopy printer.

The syngo FLC DICOM print management SCU supports the following DIMSE Service elements for the Basic Film Session SOP Class as SCU:

- N-CREATE
- N-DELETE

The Basic Film Session SOP Class N-CREATE-RQ (SCU) uses the following attributes:

| Attribute Name   | Tag         | Usage SCU | Supported Values |
|------------------|-------------|-----------|------------------|
| Number of Copies | (2000,0010) | U         | Set by user      |
| Print Priority   | (2000,0020) | U         | MED              |

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session – see below:

| Attribute Name             | Tag                           | Source of Information   |
|----------------------------|-------------------------------|---|
| Requested SOP Instance UID | (0000,1000)<br>-> (0000,1001) | Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session |

The N-DELETE-RQ on the Basic Film Session SOP Class is used to remove the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

| Service Status | Meaning  | Error Codes |
|----------------|--|-------------|
| Failed         | Film session SOP instances hierarchy does not contain film box SOP instances | C600        |
|                | Unable to create print job, print queue is full                              | C601        |
|                | Image size is larger than images box size                                    | C603        |
| Warning        | Memory allocation not supported  | B600        |
|                | Film session printing is not supported                                       | B601        |
|                | Film box does not contain image box (empty page)                             | B602        |
| Success        | Film box belonging to the film session is accepted for printing              | 0000        |

### 15.1.2.1.3.2 Basic Film Box SOP class

The Basic Film Box information object definition describes all the user-defined parameter of one film of the film session. The Basic Film Box information description defines the presentation parameters that are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported Service Elements as SCU are:

- N-CREATE
- N-ACTION

The Basic Film Box SOP class N-CREATE-RQ message uses the following attributes (the actual values for each attribute depend on DICOM printer configuration within the syngo FLC DICOM print management SCU):

| Attribute Name                   | Tag         | Usage SCU | Supported Values                                     |
|----------------------------------|-------------|-----------|--|
| Image Display Format             | (2010,0010) | M         | 1*1  |
| Referenced Film Session Sequence | (2010,0500) | M         |  |
| > Referenced SOP Class UID       | (0008,1150) | M         | 1.2.840.10008.5.1.1.1                                |
| > Referenced SOP Instance UID    | (0008,1155) | M         |  |
| Film Orientation                 | (2010,0040) | U         | (from Camera Configuration)<br>PORTRAIT or LANDSCAPE |

| Attribute Name                       | Tag         | Usage SCU | Supported Values   |
|--------------------------------------|-------------|-----------|--|
| Film Size ID                         | (2010,0050) | U         | (from Camera Configuration)<br>8INX10IN, 10INX12IN,<br>11INX14IN,, 14INX14IN,<br>14INX17IN |
| Referenced Presentation LUT Sequence | (2050,0500) | MC        | Only if Print Presentation LUT is configured for the DICOM Print SCP                       |
| > Referenced SOP Class UID           | (0008,1150) | M         | 1.2.840.10008.5.1.1.23   |
| > Referenced SOP Instance UID        | (0008,1155) | M         | Instance UID of presentation LUT object  |

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with SOP Class/Instance UID pairs that will be kept internally to be further used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film-sheet have been set, the syngo FLC DICOM print manager will issue an N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-ACTION-RQ) on the Basic Film Box – see below:

| Attribute Name             | Tag                           | Source of Information                                       |
|----------------------------|-------------------------------|---|
| Requested SOP Instance UID | (0000,1000)<br>-> (0000,1001) | Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box |

The Basic Film Box SOP class interprets the following status codes:

| Service Status | Meaning   | Error Codes |
|----------------|---|-------------|
| Failure        | Unable to create print job, print queue is full                         | C601        |
|                | Image size is larger than images box size                               | C603        |
| Warning        | Film box does not contain image box (empty page)                        | B603        |
|                | Requested MinDensity or MaxDensity outside of Printer's operating range | B605        |
| Success        | Film accepted for printing  | 0000        |

### 15.1.2.1.3.3 Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data that apply to a single image of a sheet of film.

The Grayscale Image Box SOP Class uses only the N-SET-RQ with the following attributes:

| Attribute Name                 | Tag         | Usage SCU | Supported Values            |
|--------------------------------|-------------|-----------|-----------------------------|
| Image Position                 | (2020,0010) | M         | Depending on display format |
| Basic Grayscale Image Sequence | (2020,0110) | M         |                             |
| > Samples per Pixel            | (0028,0002) | M         | 1                           |
| > Photometric Interpretation   | (0028,0004) | M         | MONOCHROME2                 |
| > Rows                         | (0028,0010) | M         |                             |
| > Columns                      | (0028,0011) | M         |                             |
| > Pixel Aspect Ratio           | (0028,0034) | M         | 1\1                         |
| > Bits Allocated               | (0028,0100) | M         | 8                           |
| > Bits Stored                  | (0028,0101) | M         | 8                           |
| > High Bit                     | (0028,0102) | M         | 7                           |
| > Pixel Representation         | (0028,0103) | M         | 0                           |

| Attribute Name | Tag         | Usage SCU | Supported Values |
|----------------|-------------|-----------|------------------|
| > Pixel Data   | (7FE0,0010) | M         |                  |

The Grayscale Image Box SOP class interprets the following status codes:

| Service Status | Meaning   | Error Codes |
|----------------|---|-------------|
| Failure        | Image contains more pixel than printer can print in Image Box             | C603        |
|                | Insufficient memory in printer to store the image                         | C605        |
| Warning        | Requested Min Density or Max Density outside of Printer's operating range | B605        |
| Success        |   | 0000        |

#### 15.1.2.1.3.4 Printer SOP Class

The Printer SOP Class is the possibility to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The syngo FLC DICOM print manager can directly ask the Printer (SCP) for its status or receive events from the Printer asynchronously:

- N-GET as SCU
- N-EVENT-REPORT as SCU

In both cases the following information is supported:

*Used Printer N-EVENT Report attributes*

| Event-type Name | Event | Attributes          | Tag         | Usage SCU |
|-----------------|-------|---------------------|-------------|-----------|
| Normal          | 1     |                     |             |           |
| Warning         | 2     | Printer Status Info | (2110,0020) | U         |
| Failure         | 3     | Printer Status Info | (2110,0020) | U         |

*Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes*

| Attribute Name      | Tag         | Usage SCP | Supported Values         |
|---------------------|-------------|-----------|--------------------------|
| Printer Status      | (2110,0010) | M         | NORMAL, FAILURE, WARNING |
| Printer Status Info | (2110,0020) | M         |                          |

#### 15.1.2.1.4 SOP specific Conformance Statement – Print Presentation LUT SOP class

The objective of the Presentation LUT is to realize image hardcopy printing tailored for specific modalities, applications and user preferences.

The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

The syngo FLC DICOM print management SCU supports the following DIMSE Service elements for the Print Presentation LUT SOP Class as SCU:

- N-CREATE
- N-DELETE

The Print Presentation LUT SOP Class N-CREATE-RQ (SCU) uses the following attributes:

| Attribute Name         | Tag         | Usage SCU | Supported Values |
|------------------------|-------------|-----------|------------------|
| Presentation LUT Shape | (2050,0020) | U         | IDENTITY         |

### 15.1.3 Association Acceptance Policy

Not applicable

## **16 Communication Profiles**

### **16.1 Supported Communication Stacks**

The syngo FLC DICOM application provides DICOM TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

#### **16.1.1 TCP/IP Stack**

The syngo FLC DICOM application uses the TCP/IP stack from the underlying Operating System upon which it executes. It uses the MergeCOM-3 subroutine library from Merge Technologies Inc. that is based on a Berkeley socket interface.

##### **16.1.1.1 API**

The syngo FLC DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

##### **16.1.1.2 Physical Media Support**

The syngo FLC DICOM application is indifferent to the physical medium over which TCP/IP executes; it inherits this from the underlying operating system upon which it executes.

## **17      Extensions / Specializations / Privatizations**

### **17.1.1    Standard Extended / Specialized / Private SOPs**

Please refer to Appendix A.1 and A.3 for all information on these topics. A detailed overview is given there.

### **17.1.2    Private Transfer Syntaxes**

Not applicable

## 18 Configuration

### 18.1 AE Title/Presentation Address Mapping

To ensure unique identification within the network the hostname could be used as part of the AE Titles (see examples below, hostname = FLC1). The string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters) are allowed according to DICOM Standard.

#### 18.1.1 DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. E.g. Verification will use the Storage SCU AE, if initiated to check the configuration of a remote DICOM storage provider.

#### 18.1.2 DICOM Storage SCP AE Title

The DICOM Storage Provider application provides an application entity title that can be configured via Service UI; this AE Title must be different from the Storage SCU AE Title:

e.g. FLC\_STORE\_SCP

There are 2 fixed listening port numbers used:

- 104 for unencrypted communication
- 2762 for TLS-based encrypted communication.

#### 18.1.3 DICOM Storage SCU AE Title

The DICOM Storage User application provides an application entity title that can be configured via Service UI:

e.g. FLC\_STORE\_SCU

For each Storage destination the AET, Port and IP-Address can be configured.

#### 18.1.4 DICOM Query/Retrieve AE Title

The DICOM Query/Retrieve application provides an own application entity title that can be configured via Service UI:

e.g. FLC\_QR\_SCU

For each Query/Retrieve provider the AET, Port and IP-Address can be configured.

#### 18.1.5 DICOM Storage Commitment AE Title

The DICOM Storage Commitment application provides the application entity title that can be configured via Service UI:

e.g. FLC\_STC\_SCU

There are 2 fixed listening port numbers used:

- 104 for unencrypted communication

- 2762 for TLS-based encrypted communication.

For each Storage Commitment provider the AET, Port and IP-Address can be configured.

### 18.1.6 DICOM Worklist AE Title

The DICOM Worklist application provides an application entity title that can be configured via Service UI:

e.g. FLC\_WK\_SCU

For **one** Worklist provider the AET, Port and IP-Address can be configured.

### 18.1.7 DICOM MPPS AE Title

The DICOM Modality Performed Procedure Step application uses the same application entity title as configured for the DICOM Worklist application 18.1.6.

For **one** MPPS provider the AET, Port and IP-Address can be configured.

### 18.1.8 DICOM Print AE Title

The DICOM Print application provides the application entity title:

e.g. FLC\_PRINT\_SCU

For each Print provider the AET, Port and IP-Address can be configured

## 18.2 Configurable Parameters

The Application Entity Titles, host names and port numbers are configured using the Siemens syngo FLC Service/Installation Tool. For each AET the list of services supported can be configured.

### 18.2.1 Storage and Query/Retrieve

The Siemens syngo FLC Service/Installation Tool can be used to set the AETs, port-numbers, host-names, IP-addresses and capabilities for the remote nodes (SCPs).

Storage:  
(General Settings)

- Retry delay for failed jobs (range: 5 to 180 minutes, 0 means no retry). Maximum 5 retries will occur (per AE target).
- Usage of Pixel Spacing in addition to Imager Pixel Spacing
- **1 image per series** (default data model of syngo FLC) or **n images per series / Singleframe per series** (all single frame images, belonging to the same procedure step, are in the same series)
- Downscaling of Fluoroloops

(Node specific settings)

- Usage of Ready Window. Ready Window means, that windowing is calculated into the pixel data. Bit depth is not changed.
- Ready Processing (burn in of shutter, overlay, zoom and pan) for XRF IODs
- Archive flag
- Associated Storage Commitment Server

### 18.2.2 Storage Commitment

One destination (AET, Port and IP) can be configured for Storage Commitment requests.

- A timeout (1-10s) for a Storage Commitment result within the same association can be defined.
- A Storage Commitment timeout and the number of retries could be configured in User Settings.

### 18.2.3 Modality Worklist

One destination (AET, Port and IP) can be configured for Worklist requests.

- Time-out waiting for a response from the worklist provider (Query waiting time: maximum 999 s).
- Maximum of worklist entries received (Max. Query Match: maximum 999).
- Time between automated worklist queries (0 .. 1440 min.; 0 min means no automatic query) and used modality (0008,0060) in worklist query.
- Usage of own AET in worklist query (Query by AET)
- Time range used in worklist query

### 18.2.4 Modality Performed Procedure Step

One destination (AET, Port and IP) can be configured for MPPS data.

The “MPPS Complete” method can be selected in the user configuration.

### 18.2.5 Print

The Siemens syngo FLC Service/Installation Tool can be used to configure the SCPs (DICOM-Printers). The AET, host-name, IP-address and port-number can be set.

Print: Retry delay for failed jobs (range: 5 to 180 minutes, 0 means no retry). Maximum 5 retries will occur.

- Usage of Print Presentation LUT

## 18.3 Default Parameters

This installation tool also uses some default parameters:

- max. PDU size set to 65536 Bytes (64 KB)
- time-out for accepting/rejecting an association request: 60 s
- time-out for responding to an association open/close request: 60 s
- time-out for accepting a message over network: 60 s
- time-out for waiting for data between TCP/IP-packets: 60 s
- timeout for a network connect: 15s

The time-outs for waiting for a Service Request/Response message from the remote node are as follows:

- for Storage SCU: 30 s for single frame images, 600 s for multiframe
- for Storage SCP: 600 s
- for Query/Retrieve SCP/SCU: 600 s
- for Print Management SCU:
  - time-out for Response to N-SET-RQ: 25 s
  - time-out for Response to other Requests: 25 s

## 19 Support of Extended Character Sets

The Siemens syngo FLC DICOM application supports the

- ISO\_IR 100 (ISO 8859-1:1987 Latin Alphabet No. 1 supplementary set)
- GB18030 (used when Chinese patient data input is configured)
- ISO 2022 IR 13, ISO 2022 IR 87 and ISO 2022 IR 159 (used when Japanese patient data input is configured)
- ISO\_IR 144 (used when Russian patient data input is configured)

## **20 Security**

### **20.1 Security Profiles**

#### **20.1.1 Secure Transport Connection Profiles**

FLC supports the “Basic TLS Secure Transport Connection Profile” as specified in [DICOM].

The following TLS versions are supported: 1.0, 1.1, 1.2.

The cypher suites that are provided by the underlying Operating System are used.

The private key and certificate used by an FLC based system and Certificate Authorities (CA) to validate certificates received from remote nodes are stored in the local Certificate Store of the underlying Operating System.

The listening port used for the DICOM services is 2762.

# Application Profile Conformance Statement

This chapter contains the Conformance Statement to all "Offline Media Application Profiles (incl. private extensions)" supported by the syngo FLC archive options.

Those application profiles supported shall be:

- General Purpose CDR
- General Purpose DVD
- General Purpose USB

## 1 Introduction

### 1.1 Purpose

This DICOM Conformance Statement describes the DICOM offline interface for Siemens X-ray acquisition modalities based on the syngo FLC imaging system according to part PS 3.2 of [DICOM].

### 1.2 Scope

The syngo FLC DICOM offline media storage service implementation acts as FSC, FSU and/or FSR for the specified application profiles and the related SOP Class instances.

### 1.3 Definitions, Terms and Abbreviations

|         |  |
|---------|--|
| ACR     | American College of Radiology                                    |
| AE      | DICOM Application Entity   |
| ASCII   | American Standard Code for Information Interchange               |
| CR      | Computed Radiography   |
| DCS     | DICOM Conformance Statement                                      |
| DICOM   | Digital Imaging and Communications in Medicine                   |
| DIMSE   | DICOM Message Service Element                                    |
| DIMSE-C | DICOM Message Service Element with Composite information objects |
| FSC     | File Set Creator   |
| FSR     | File Set Reader  |
| FSU     | File Set Updater   |
| GSDF    | Grayscale Standard Display Function                              |
| IOD     | DICOM Information Object Definition                              |
| FD      | Flat panel detector  |
| ISO     | International Standard Organization                              |
| MOD     | Magneto-optical Disk   |
| NEMA    | National Electrical Manufacturers Association                    |
| O       | Optional Key Attribute   |
| PDU     | DICOM Protocol Data Unit   |
| R       | Required Key Attribute   |
| RWA     | Real-World Activity  |
| U       | Unique Key Attribute   |
| XA      | X-Ray Angiography  |
| XRF     | X-Ray Radiofluoroscopy   |

### 1.4 References

[DICOM] Digital Imaging and Communications in Medicine (DICOM), NEMA PS 3.1-20, 2014.

### 1.5 Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' Medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [DICOM]. It is, however, by itself not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens and non-Siemens equipment.
- Test procedures should be defined and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the users' future requirements. Siemens is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.
- Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

## 2 Implementation Model

### 2.1 Application Data Flow Diagram

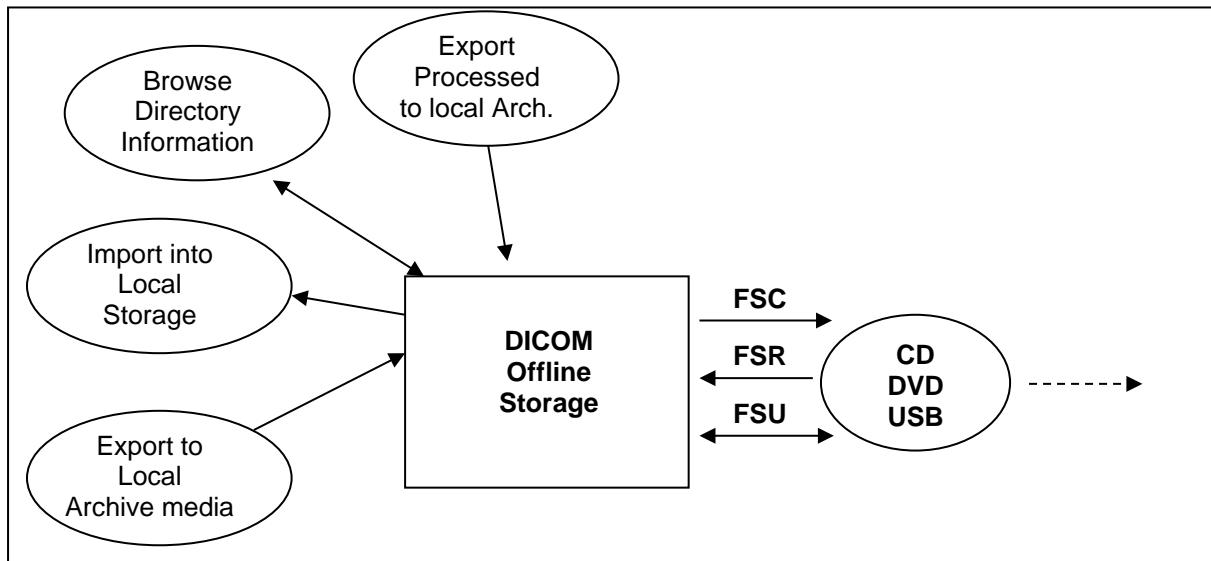


Figure 8: FLUOROSPOT Compact DICOM Media Storage Implementation Model

The DICOM Offline Storage application will serve as an interface to the CD, DVD and USB offline medium device. It serves interfaces to include the offline media directory into the browser and to copy SOP instances to a medium or retrieve SOP Instances from medium into local storage.

The DICOM Offline Storage application will support the 120 mm CD-R/DVD-R/DVD+R medium and USB connected removable storage devices.

The FSU role will update new SOP Instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will be temporarily stored in a local Archive-Database.

### 2.2 Functional Definitions of Aes

The syngo FLC DICOM offline media storage application consists of the DICOM application entity serving all interfaces to access offline media. The DICOM Offline Storage application is capable of

1. creating a new File-set onto an unwritten medium (Export to...),
2. updating an existing File-set by writing new SOP Instances onto the medium (Export to...),
3. importing SOP Instances from the medium onto local storage,
4. reading the File-sets DICOMDIR information into temporary database and pass it to display applications,
5. writing/updating File-Sets with processed image export.

### 2.3 Sequencing of Real-World Activities

Not applicable.

## 2.4 File Meta Information Options

|                             |                     |
|-----------------------------|---------------------|
| Implementation Class UID    | 1.3.12.2.1107.5.3.4 |
| Implementation Version Name | Siemens_FLC_80      |

## 3 AE Specifications

### 3.1 DICOM Archive Specification

The DICOM Offline Storage provides Standard conformance to Media Storage Service Class (Interchange Option). Details are listed in following Table:

| Application Profiles Supported | Real-World Activity           | Role     | SC Option   |
|--------------------------------|-------------------------------|----------|-------------|
| STD-GEN-CD                     | Browse Directory Information  | FSR      | Interchange |
|                                | Import into local Storage     | FSR      | Interchange |
|                                | Export to local Archive Media | FSC, FSU | Interchange |
| STD-GEN-DVD <sup>1</sup>       | Browse Directory Information  | FSR      | Interchange |
|                                | Import into local Storage     | FSR      | Interchange |
|                                | Export to local Archive Media | FSC, FSU | Interchange |
| STD-GEN-USB <sup>1</sup>       | Browse Directory Information  | FSR      | Interchange |
|                                | Import into local Storage     | FSR      | Interchange |
|                                | Export to local Archive Media | FSC, FSU | Interchange |

#### 3.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See Chapter “Configuration” for details.

#### 3.1.2 Real-World Activities for this Application Entity

##### 3.1.2.1 Real-World Activity: Browse Directory Information

The DICOM Offline Storage application acts as FSR using the interchange option when requested to read the media directory.

The DICOM Offline Storage application will read the DICOMDIR and insert those directory entries valid for the application profiles supported into a local database. The database can then be used for browsing media contents.

*During operation no “Attribute Value Precedence” is applied to the SOP Instances. Detached Patient Management is not supported.*

##### 3.1.2.1.1 Application Profiles for the RWA: Browse Directory Information

See Table in section 3.1 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

<sup>1</sup> No support for compressed Transfer Syntaxes

### 3.1.2.2 Real-World Activity: Import into local Storage

The DICOM Offline Storage application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the local storage.

The SOP Instance selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported, can be retrieved from media storage. This is due to the fact that the Browse Directory Information will filter all SOP Instances not matching the Application profiles supported.

*During operation no “Attribute Value Precedence” is applied to the SOP Instances. Detached Patient Management is not supported.*

*Compressed Transfer Syntaxes are not supported by the DICOM Offline Storage application neither as FSR/FSC or FSU.*

For media conforming to the STD-GEN-CD, STD-GEN-DVD and STD-GEN-USB profiles the following SOP classes will be supported as an FSR:

| Information Object Definition  | SOP Class UID                 | Transfer Syntax UID                             |
|--|-------------------------------|---|
| Secondary Capture Image Storage  | 1.2.840.10008.5.1.4.1.1.7     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Radiation Dose SR  | 1.2.840.10008.5.1.4.1.1.88.67 | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Angiographic Image Storage   | 1.2.840.10008.5.1.4.1.1.12.1  | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Radiofluoroscopic Image Storage<br>(only for Fluorosystems)                  | 1.2.840.10008.5.1.4.1.1.12.2  | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Computed Radiography Image Storage<br>(only for Radsystems)                        | 1.2.840.10008.5.1.4.1.1.1     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Digital X-Ray Image Storage – For Presentation                                     | 1.2.840.10008.5.1.4.1.1.1.1   | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Multi-frame True Color Secondary Capture Image Storage<br>(only for Uroskop Omnia) | 1.2.840.10008.5.1.4.1.1.7.4   | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| CT Image Storage   | 1.2.840.10008.5.1.4.1.1.2     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| MR Image Storage   | 1.2.840.10008.5.1.4.1.1.4     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Ultrasound Image Storage   | 1.2.840.10008.5.1.4.1.1.6.1   | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Ultrasound Multi-frame Image Storage   | 1.2.840.10008.5.1.4.1.1.3.1   | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |

#### 3.1.2.2.1 Application Profiles for the RWA: Import into local Storage

See Table in section 3.1 for the Application Profiles listed that invoke this Application Entity for the Import into Local Storage RWA.

### 3.1.2.3 Real-World Activity: Export to local Archive Media

The DICOM Offline Storage application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium.

The DICOM Archive application will receive a list of marked SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted. The user can select if “all” images are marked or the marks from image acquisition will be retained.

The user can choose the IOD format of the instances (CR or DX for RAD images). For XRF it can be configured to store images “ready processed”.

The DICOM archive application will not close the medium in case of CD-R/DVD-R or DVD+R.

Conforming to the STD-GEN-CD, STD-GEN-DVD and STD-GEN-USB profiles the following SOP classes will be supported as an FSC and FSU:

| Information Object Definition  | SOP Class UID                 | Transfer Syntax UID                             |
|--|-------------------------------|---|
| Secondary Capture Image Storage  | 1.2.840.10008.5.1.4.1.1.7     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Radiation Dose SR  | 1.2.840.10008.5.1.4.1.1.88.67 | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Radiofluoroscopic Image Storage<br>(only for Fluorosystems)                  | 1.2.840.10008.5.1.4.1.1.12.2  | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| X-Ray Angiographic Image Storage<br>(only for Multitom Rax)                        | 1.2.840.10008.5.1.4.1.1.12.1  | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Computed Radiography Image Storage<br>(only for Radsystems)                        | 1.2.840.10008.5.1.4.1.1.1     | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Digital X-Ray Image Storage For Presentation<br>(only for Radsystems)              | 1.2.840.10008.5.1.4.1.1.1.1.  | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |
| Multi-frame True Color Secondary Capture Image Storage<br>(only for Uroskop Omnia) | 1.2.840.10008.5.1.4.1.1.7.4   | Explicit VR LittleEndian<br>1.2.840.10008.1.2.1 |

### 3.1.2.3.1 Application Profiles for the RWA: Export to local Archive Media

See Table in section 3.1 for the Application Profiles listed that invoke this Application Entity for the Export to local Archive Media RWA.

## **4 Augmented and Private Profiles**

### **4.1 Augmented Application Profiles**

Not applicable.

### **4.2 Private Application Profiles**

Not applicable.

## 5 Extensions, Specializations and Privatizations of SOP Classes and Transfer Syntaxes

The SOP Classes listed refer in majority to those created by the equipment to which this Conformance Statement is related to. For SOP classes not listed in this section, please refer to the Storage section of the DICOM Conformance Statement of the product. This will include all SOP Instances that can be received and displayed and therefore will be included into offline media storage even though these SOP Instances are not created by the equipment serving the Media Storage Service.

Restrictions and Extensions<sup>1</sup>:

1. It is possible to store images on offline media in a “packed” manner. This will result in a DICOMDIR containing “PRIVATE” records instead of “IMAGE” records. This functionality is not intended as exchange media with other systems.
2. The user can choose the IOD format of the instances. RAD images can be stored in CR or DX IOD. For XRF it can be configured to store images “ready processed”.
3. It is possible to update an offline media containing unpacked images with packed images and vice versa.

---

<sup>1</sup> Not valid for Mobilett Mira Max / MOBILETT Elara Max, as they do not store images in a “packed” manner.

## 5.1 SOP Specific Conformance Statement for Max / Basic Directory

### 5.1.1 Extension, Specialization for “Packed CD”

The PRIVATE directory records will be identified according to the information in the following table:<sup>1</sup>

| Attribute          | Tag         | Value used            |
|--------------------|-------------|-----------------------|
| Private Record UID | (0004,1432) | 1.3.12.2.1107.5.3.4.1 |

### 5.1.2 DICOMDIR Attributes

The DICOMDIR file will contain the following attributes for the levels Patient – Study – Series – Image –Private

| Attribute Name   | Tag         | Type  | Notes   |
|--|-------------|-------|---|
| File Set Identification  |             |       |   |
| File-set ID  | (0004,1130) | 2     | Volume label of media                               |
| Directory Information  |             |       |   |
| Offset of the First Directory Record of the Root Directory Entry | (0004,1200) | 1     |   |
| Offset of the Last Directory Record of the Root Directory Entry  | (0004,1202) | 1     |   |
| File-set Consistency Flag  | (0004,1212) | 1     | 0000h   |
| Directory Record Sequence  | (0004,1220) | 2     |   |
| > Offset of Next Directory Record                                | (0004,1400) | 1C    |   |
| > Record In-use Flag   | (0004,1410) | 1C    | FFFFh   |
| > Offset of Referenced Lower-Level Directory Entity              | (0004,1420) | 1C    |   |
| > Directory Record Type  | (0004,1430) | 1C    | PATIENT, STUDY, SERIES, IMAGE, PRIVATE              |
| > Private Record UID   | (0004,1432) | 1C    | For PRIVATE Directory Record                        |
| > Referenced File ID   | (0004,1500) | 1C    | Filename and path, only for IMAGE Directory Records |
| > Referenced SOP Class UID in File                               | (0004,1510) | 1C    | For IMAGE Directory Records                         |
| > Referenced SOP Instance UID in File                            | (0004,1511) | 1C    | For IMAGE Directory Records                         |
| > Referenced Transfer Syntax UID in File                         | (0004,1512) | 1C    | For IMAGE Directory Records                         |
| > Record Selection Keys  | See below   | n. a. |   |
| Patient Keys   |             |       | Directory Record Type PATIENT                       |
| Specific Character Set   | (0008,0005) | 1C    |   |
| Patient's Name   | (0010,0010) | 2     |   |
| Patient ID   | (0010,0020) | 1     |   |
| Date of Birth  | (0010,0030) | 3     |   |
| Patient's Sex  | (0010,0040) | 3     |   |
| Study Keys   |             |       | Directory Record Type STUDY                         |
| Specific Character Set   | (0008,0005) | 1C    |   |
| Study Date   | (0008,0020) | 1     |   |
| Study Time   | (0008,0030) | 1     |   |
| Accession Number   | (0008,0050) | 2     |   |
| Study Description  | (0008,1030) | 2     |   |
| Study Instance UID   | (0020,000D) | 1C    |   |
| Study ID   | (0020,0010) | 1     |   |
| Series Keys  |             |       | Directory Record Type SERIES                        |

<sup>1</sup> Not valid for Mobilett Mira Max / MOBILETT Elara Max.

| Attribute Name              | Tag         | Type | Notes                         |
|-----------------------------|-------------|------|-------------------------------|
| Specific Character Set      | (0008,0005) | 1C   |                               |
| Series Date                 | (0008,0021) | 3    |                               |
| Series Time                 | (0008,0031) | 3    |                               |
| Modality                    | (0008,0060) | 1    |                               |
| Institution Name            | (0008,0080) | 3    |                               |
| Institution Address         | (0008,0081) | 3    | Zero length                   |
| Series Description          | (0008,103E) | 3    |                               |
| Performing Physician        | (0008,1050) | 3    |                               |
| Series Instance UID         | (0020,000E) | 1    |                               |
| Series Number               | (0020,0011) | 1    |                               |
| Image Keys                  |             |      | Directory Record Type IMAGE   |
| Image Type                  | (0008,0008) |      |                               |
| Instance Number             | (0020,0013) | 1    |                               |
| Number of Frames            | (0028,0008) | 3    |                               |
| Icon Image Sequence         | (0088,0200) | 3    |                               |
| >Samples per Pixel          | (0028,0002) | 1C   | 1                             |
| >Photometric Interpretation | (0028,0004) | 1C   | MONOCHROME2                   |
| >Rows                       | (0028,0010) | 1C   | 128                           |
| >Columns                    | (0028,0011) | 1C   | 128                           |
| >Bits Allocated             | (0028,0100) | 1C   | 8                             |
| >Bits Stored                | (0028,0101) | 1C   | 8                             |
| >High Bit                   | (0028,0102) | 1C   | 7                             |
| >Pixel Representation       | (0028,0103) | 1C   | 0000H                         |
| >Pixel Data                 | (7FE0,0010) | 1C   | Icon Image                    |
| Private Keys                |             |      | Directory Record Type PRIVATE |
| Private Record UID          | (0004,1432) | 1    |                               |
| Instance Number             | (0020,0013) | 1    |                               |

## **6 Configuration**

### **6.1 AE Title Mapping**

#### **6.1.1 DICOM Media Storage AE Title**

The DICOM Storage application provides the application entity title:

Not applicable.

## 7 Support of Extended Character Sets

The Siemens syngo FLC DICOM application supports the

- ISO\_IR 100 (ISO 8859-1:1987 Latin Alphabet No. 1 supplementary set)
- ISO\_IR 144 (Cyrillic, supplementary set of ISO 8859, used when Russian patient data input is configured)
- GB18030 (used when Chinese patient data input is configured)
- ISO 2022 IR 13, ISO 2022 IR 87 and ISO 2022 IR 159 (used when Japanese patient data input is configured)

## A APPENDIX

### A.1 Common attributes in image and structured report IODs

Overview of supplied attributes – all type of images and structured report

| Attribute Name                               | Tag         | Value   |
|--|-------------|---|
| Specific Character Set                       | (0008,0005) | dependent on system configuration   |
| Image Type                                   | (0008,0008) | see A.7   |
| SOP Class UID                                | (0008,0016) | dependent on the SOP Class (see chapter 5.1)  |
| SOP Instance UID                             | (0008,0018) | System generated  |
| Study Date                                   | (0008,0020) | <yyyymmdd>  |
| Series Date                                  | (0008,0021) | <yyyymmdd>  |
| Acquisition Date                             | (0008,0022) | <yyyymmdd>  |
| Content Date                                 | (0008,0023) | <yyyymmdd>  |
| Study Time                                   | (0008,0030) | <hhmmss>  |
| Series Time                                  | (0008,0031) | <hhmmss>  |
| Acquisition Time                             | (0008,0032) | <hhmmss>  |
| Image Time                                   | (0008,0033) | <hhmmss>  |
| Accession Number                             | (0008,0050) | From Modality Worklist or user input  |
| Manufacturer                                 | (0008,0070) | SIEMENS   |
| Institution Name                             | (0008,0080) | From Configuration or value from Worklist   |
| Referring Physician's Name                   | (0008,0090) | From Modality Worklist or user input  |
| Station Name                                 | (0008,1010) | From Configuration (hostname)   |
| Study Description                            | (0008,1030) | Requested Procedure Description (0032,1060) from Modality Worklist or first Exam Name of the study    |
| Procedure Code Sequence                      | (0008,1032) | (0032,1064) from Modality Worklist  |
| > Code Value                                 | (0008,0100) | (0032,1064) from Modality Worklist  |
| > Coding Scheme Designator                   | (0008,0102) | (0032,1064) from Modality Worklist  |
| > Coding Scheme Version                      | (0008,0103) | (0032,1064) from Modality Worklist  |
| > Code Meaning                               | (0008,0104) | (0032,1064) from Modality Worklist  |
| Series Description                           | (0008,103E) | Organ program name  |
| Institutional Department Name                | (0008,1040) |   |
| Performing Physician's Name                  | (0008,1050) | Physician field in Study list, default (0040,0006) from Modality Worklist or user input               |
| Operator's Name                              | (0008,1070) | User input  |
| Admitting Diagnoses Description              | (0008,1080) | From Modality Worklist or user input  |
| Manufacturer's Model Name                    | (0008,1090) | For Dose Reports: the name of the system (e.g. "Multitom_Rax").<br>Otherwise: "Fluorospot Compact FD" |
| Referenced Study Sequence                    | (0008,1110) | From Modality Worklist  |
| > Referenced SOP Class UID                   | (0008,1150) | From Modality Worklist  |
| > Referenced SOP Instance UID                | (0008,1155) | From Modality Worklist  |
| Referenced Patient Sequence                  | (0008,1120) | From Modality Worklist  |
| > Referenced SOP Class UID                   | (0008,1150) | From Modality Worklist  |
| > Referenced SOP Instance UID                | (0008,1155) | From Modality Worklist  |
| Referenced Performed Procedure Step Sequence | (0008,1111) | Only with MPPS  |
| > Referenced SOP Class UID                   | (0008,1150) | 1.2.840.10008.3.1.2.3.3 (MPPS)  |
| > Referenced SOP Instance UID                | (0008,1155) | Reference to MPPS   |
| Derivation Description 1)                    | (0008,2111) |   |
| Irradiation Event UID 1) 2)                  | (0008,3010) |   |
| Patient's Name                               | (0010,0010) | From Modality Worklist or user input (all 5 components)   |
| Patient ID                                   | (0010,0020) | From Modality Worklist or user input  |
| Patient's Birth Date                         | (0010,0030) | From Modality Worklist or user input  |
| Patient's Sex                                | (0010,0040) | From Modality Worklist or user input  |

| Attribute Name                                  | Tag         | Value  |
|---|-------------|--|
| Other Patient IDs                               | (0010,1000) | From Modality Worklist   |
| Other Patient Names                             | (0010,1001) | From Modality Worklist   |
| Patient's Age                                   | (0010,1010) |  |
| Patient's Size                                  | (0010,1020) | From Modality Worklist or user input   |
| Patient's Weight                                | (0010,1030) | From Modality Worklist or user input   |
| Ethnic Group                                    | (0010,2160) | From Modality Worklist   |
| Additional Patient History                      | (0010,21B0) | From Modality Worklist   |
| Patient Comments                                | (0010,4000) | From Modality Worklist   |
| Device Serial Number                            | (0018,1000) | From Configuration   |
| Software Version                                | (0018,1020) | From Configuration   |
| Protocol Name <sup>1</sup>                      | (0018,1030) | Organ program name   |
| Date of Last Calibration <sup>1,2</sup>         | (0018,1200) |  |
| Study Instance UID                              | (0020,000D) | From Modality Worklist or generated by FLC                                     |
| Series Instance UID                             | (0020,000E) | System generated   |
| Study ID  | (0020,0010) | User Input, default (0040,1001) from Modality Worklist                         |
| Series Number                                   | (0020,0011) | System generated   |
| Acquisition Number <sup>1,2</sup>               | (0020,0012) | System generated   |
| Instance Number                                 | (0020,0013) | System generated   |
| Patient Orientation <sup>1,2</sup>              | (0020,0020) | not available  |
| Laterality <sup>1,2</sup>                       | (0020,0060) | Zero length if not available, not sent when Laterality is "both" or "unpaired" |
| Image Comments <sup>1,2</sup>                   | (0020,4000) | From user input  |
| Burned in Annotations 1)                        | (0028,0301) | "NO"   |
| Window Center <sup>1</sup>                      | (0028,1050) | Dependent on user input and bit depth  |
| Window Width <sup>1</sup>                       | (0028,1051) | Dependent on user input and bit depth  |
| Lossy Image Compression <sup>1</sup>            | (0028,2110) | "00"   |
| Study Comments                                  | (0032,4000) | User Input   |
| Current Patient Location                        | (0038,0300) | From Modality Worklist   |
| Performed Procedure Step Start Date             | (0040,0244) | = (0008,0020)  |
| Performed Procedure Step Start Time             | (0040,0245) | = (0008,0030)  |
| Performed Procedure Step ID                     | (0040,0253) | Internally created   |
| Performed Procedure Step Description            | (0040,0254) | = (0008,1030)  |
| Performed Protocol Code Sequence <sup>1,2</sup> | (0040,0260) | Only present, if usage of protocol codes is configured in user settings        |
| > Code Value                                    | (0008,0100) |  |
| > Coding Scheme Designator                      | (0008,0102) |  |
| > Coding Scheme Version                         | (0008,0103) |  |
| > Code Meaning                                  | (0008,0104) |  |
| Request Attributes Sequence                     | (0040,0275) |  |
| >Scheduled Procedure Step Description           | (0040,0007) | From Modality Worklist   |
| > Scheduled Protocol Code Sequence              | (0040,0008) | From Modality Worklist   |
| >> Code Value                                   | (0008,0100) | From Modality Worklist   |
| >> Coding Scheme Designator                     | (0008,0102) | From Modality Worklist   |
| >> Coding Scheme Version                        | (0008,0103) | From Modality Worklist   |
| >> Code Meaning                                 | (0008,0104) | From Modality Worklist   |
| >Scheduled Procedure Step ID                    | (0040,0009) | From Modality Worklist   |
| >Requested Procedure ID                         | (0040,1001) | From Modality Worklist or user input   |
| Presentation LUT Shape <sup>1</sup>             | (2050,0020) | "IDENTITY"   |
| Pixel Data <sup>1</sup>                         | (7FE0,0010) | System generated   |

<sup>1</sup> Not used for X-Ray Radiation Dose SR SOP Class<sup>2</sup> Not used for EXAM Protocol as Secondary Capture Image

## A.2 Multiframe True Color SC Storage Standard Extended SOP Class

*Overview of specific attributes – Multiframe True Color SC image*

| Attribute Name               | Tag         | Value                                     |
|------------------------------|-------------|---|
| Modality                     | (0008,0060) | "OT"                                      |
| Conversion Type              | (0008,0064) | "WSD"                                     |
| Series Description           | (0008,103E) | not present                               |
| Derivation Description       | (0008,2111) | not present                               |
| Body Part Examined           | (0018,0015) |   |
| Protocol Name                | (0018,1030) | not present                               |
| Samples per Pixel            | (0028,0002) | 3   |
| Photometric Interpretation   | (0028,0004) | RGB                                       |
| Planar Configuration         | (0028,0006) | 0   |
| Number of Frames             | (0028,0008) | 1 for CAP images<br>≥1 for Medical Report |
| Frame Increment Pointer      | (0028,0009) | (0018,1063)                               |
| Rows                         | (0028,0010) |   |
| Columns                      | (0028,0011) |   |
| Bits Allocated               | (0028,0100) | 8   |
| Bits Stored                  | (0028,0101) | 8   |
| High Bit                     | (0028,0102) | 7   |
| Pixel Representation         | (0028,0103) | 0000H                                     |
| Pixel Intensity Relationship | (0028,1040) | "LIN"                                     |
| Window Center                | (0028,1050) | not present                               |
| Window Width                 | (0028,1051) | not present                               |

## A.3 XRF Standard Extended SOP Class

### A.3.1 configuration “XRF – Full”

Overview of specific attributes – XRF image (Full)

| Attribute Name                              | Tag          | Value   |
|---|--------------|---|
| Modality                                    | (0008,0060)  | “RF”  |
| Recommended Display Frame Rate              | (0008,2144)  | Only for multi-frame  |
| Body Part Examined                          | (0018,0015)  | -value from OGP<br>-Zero length if not available  |
| KVP   | (0018,0060)  | From Acquisition  |
| Device Serial Number                        | (0018,1000)  | From Configuration  |
| Frame Time                                  | (0018,1063)  | Only if multi-frame   |
| Distance Source to Detector                 | (0018,1110)  | SID from Acquisition (not available for all devices)  |
| Distance Source to Patient                  | (0018,1111)  | SOD (only if table object distance, image receptor table distance and SID are available)                            |
| Estimated Radiographic Magnification Factor | (0018,1114)  | only if SID and SOD are available (=SID/SOD)  |
| Table Motion                                | (0018,1134)  | “STATIC” (not available for all devices)  |
| Table Angle                                 | (0018,1138)  | From Acquisition (not available for all devices)  |
| Table Type                                  | (0018,113A)  | “TILTING” (not available for all devices)   |
| Field of View Shape                         | (0018,1147)  | “RECTANGLE”   |
| Field of View Dimension(s)                  | (0018, 1149) | rows\columns in mm  |
| Exposure Time                               | (0018,1150)  | From Acquisition, not available for all devices (e.g. Mobilett Mira Max / MOBILETT Elara Max)                       |
| Exposure                                    | (0018,1152)  | From Acquisition  |
| Exposure in $\mu$ As                        | (0018,1153)  | From Acquisition  |
| X-Ray Tube Current                          | (0018,1151)  | From Acquisition, not available for all devices   |
| Filter Type                                 | (0018,1160)  | Defined Terms:<br>"NONE", "CU_0.1_MM", "CU_0.2_MM", "CU_0.3_MM"   |
| Average Pulse Width                         | (0018,1154)  | From Acquisition  |
| Radiation Setting                           | (0018,1155)  | GR or SC  |
| Radiation Mode                              | (0018,115A)  | PULSED  |
| Image Area Dose Product                     | (0018,115E)  | If dose measurement is available, in $\text{dGy cm}^2$ .<br>Only present for acquisitions, not for fluoro.          |
| Imager Pixel Spacing                        | (0018,1164)  | For detector images:<br>"0.148\0.148" or "0.296\0. 296" or "0.444\0.444"<br>For I.I: images: zoomed image size/1024 |
| Grid  | (0018,1166)  | “NONE”, “FOCUSED”, “UNIVERSAL”  |
| Date of Last Calibration                    | (0018,1200)  |   |
| Acquisition Device Processing Description   | (0018,1400)  | Description of processing parameter set   |
| Acquisition Device Processing Code          | (0018,1401)  | Code to identify processing parameter set   |
| Relative X-Ray Exposure                     | (0018,1405)  | Exposure Index (EXI)  |
| Column Angulation                           | (0018,1450)  | From Acquisition  |
| Tomo Layer Height                           | (0018,1460)  | only for tomo acquisitions  |
| Tomo Angle                                  | (0018,1470)  | only for tomo acquisitions  |
| Tomo Time                                   | (0018,1480)  | only for tomo acquisitions  |
| Positioner Type                             | (0018,1508)  | device dependent  |
| Shutter Shape                               | (0018,1600)  | RECTANGULAR for detector images<br>CIRCULAR for I.I images  |
| Shutter Left Vertical Edge                  | (0018,1602)  | From Acquisition / Post-processing  |
| Shutter Right Vertical Edge                 | (0018,1604)  | From Acquisition / Post-processing  |
| Shutter Upper Horizontal Edge               | (0018,1606)  | From Acquisition / Post-processing  |
| Shutter Lower Horizontal Edge               | (0018,1608)  | From Acquisition / Post-processing  |
| Center of Circular Shutter                  | (0018,1610)  | for I.I images  |
| Radius of Circular Shutter                  | (0018,1612)  | for I.I images  |
| View Position                               | (0018,5101)  | Only if information is available  |
| Sensitivity                                 | (0018,6000)  |   |
| Detector Conditions Nominal Flag            | (0018,7000)  | Set to "NO" if user was notified about possible image quality   |

| Attribute Name                    | Tag         | Value  |
|-----------------------------------|-------------|--|
|                                   |             | compromise, e.g. because detector temperature is out of range  |
| Detector Temperature              | (0018,7001) | the last received detector temperature   |
| Detector Type                     | (0018,7004) | "SCINTILLATOR"   |
| Detector Description              | (0018,7006) | only for detector images<br>Detector data:<br>- Factory Serial Number<br>- Factory Date Code<br>- Configuration Version<br>- Factory Part Number |
| Detector ID                       | (0018,700A) | Factory Serial Number  |
| Date of Last Detector Calibration | (0018,700C) | <yyyymmdd>   |
| Time of Last Detector Calibration | (0018,700E) | <hhmmss>   |
| Field of View Origin              | (0018,7030) |  |
| Field of View Rotation            | (0018,7032) | Enumerated Values: "0", "90", "180", "270"   |
| Field of View Horizontal Flip     | (0018,7034) | Enumerated Values: "NO", "YES"   |
| Grid Focal Distance               | (0018,704C) | "1150", "1250", "1500", "1800", "3000"<br>only if Grid (0018,1166) = FOCUSED"  |
| X-Ray Tube Current in $\mu$ A     | (0018,8151) | From Acquisition, not available for all devices  |
| Samples per Pixel                 | (0028,0002) | 1  |
| Photometric Interpretation        | (0028,0004) | MONOCHROME2  |
| Number of Frames                  | (0028,0008) |  |
| Frame Increment Pointer           | (0028,0009) | <0018,1063> only if multi-frame  |
| Rows                              | (0028,0010) | Depending on detector and acquisition mode   |
| Columns                           | (0028,0011) | Depending on detector and acquisition mode   |
| Pixel Spacing                     | (0028,0030) | only if configured in service<br>value = 0018,1164 if no SOD is present<br>otherwise: value = (0018,1164) * SOD / SID                            |
| Bits Allocated                    | (0028,0100) | 8, 16 depending on user selection  |
| Bits Stored                       | (0028,0101) | 8, 16 depending on user selection  |
| High Bit                          | (0028,0102) | 7, 15 depending on user selection  |
| Pixel Representation              | (0028,0103) | 0  |
| Pixel Intensity Relationship      | (0028,1040) | LIN or LOG   |
| Recommended Viewing Mode          | (0028,1090) | NAT, SUB, only if multi-frame and (0028,1040) = LOG  |
| Window Center & Width Explanation | (0028,1055) | only if (0028,1040) = LOG  |
| Modality LUT Sequence             | (0028,3000) | No Modality LUT is written even in case the Pixel Intensity Relationship is set to "LOG"   |
| > LUT Descriptor                  | (0028,3002) |  |
| > Modality LUT Type               | (0028,3004) |  |
| > LUT Data                        | (0028,3006) |  |
| Representative Frame Number       | (0028,6010) | Only if multi-frame  |
| Mask Subtraction Sequence         | (0028,6100) | Only if multi-frame and (0028,1040) = LOG  |
| > Mask Operation                  | (0028,6101) | "AVG_SUB"  |
| > Mask Frame Numbers              | (0028,6110) | Mask Frame Number (always only one mask)   |
| > Mask Sub-pixel Shift            | (0028,6114) | From Post-processing   |

### A.3.2 configuration “XRF – Ready Processed”

Overview of specific attributes – XRF image (Ready Processed)

| Attribute Name                              | Tag          | Value   |
|---|--------------|---|
| Modality                                    | (0008,0060)  | “RF”  |
| Recommended Display Frame Rate              | (0008,2144)  | Only for multi-frame  |
| Body Part Examined                          | (0018,0015)  | -value from OGP<br>-Zero length if not available  |
| KVP   | (0018,0060)  | From Acquisition  |
| Device Serial Number                        | (0018,1000)  | From Configuration  |
| Frame Time                                  | (0018,1063)  | Only if multi-frame   |
| Distance Source to Detector                 | (0018,1110)  | SID from Acquisition (not available for all devices)  |
| Distance Source to Patient                  | (0018,1111)  | SOD (only if table object distance, image receptor table distance and SID are available)                                    |
| Estimated Radiographic Magnification Factor | (0018,1114)  | only if SID and SOD are available (=SID/SOD)  |
| Table Motion                                | (0018,1134)  | “STATIC”  |
| Table Angle                                 | (0018,1138)  | From Acquisition  |
| Table Type                                  | (0018,113A)  | “TILTING”   |
| Field of View Shape                         | (0018,1147)  | “RECTANGLE”   |
| Field of View Dimension(s)                  | (0018, 1149) | rows\columns in mm  |
| Exposure Time                               | (0018,1150)  | From Acquisition, not available for all devices (e.g. Mobillett Mira Max / MOBILETT Elara Max)                              |
| Exposure                                    | (0018,1152)  | From Acquisition  |
| Exposure in $\mu$ As                        | (0018,1153)  | From Acquisition  |
| X-Ray Tube Current                          | (0018,1151)  | From Acquisition, not available for all devices   |
| Filter Type                                 | (0018,1160)  | Defined Terms:<br>"NONE", "CU_0.1_MM", "CU_0.2_MM", "CU_0.3_MM"   |
| Average Pulse Width                         | (0018,1154)  | From Acquisition  |
| Radiation Setting                           | (0018,1155)  | GR or SC  |
| Radiation Mode                              | (0018,115A)  | PULSED  |
| Image Area Dose Product                     | (0018,115E)  | If dose measurement is available, in $\text{dGy cm}^2$ .<br>Only present for acquisitions, not for fluoro.                  |
| Imager Pixel Spacing                        | (0018,1164)  | For detector images:<br>"0.148\0.148" or "0.296\0. 296" or "0.444\0.444" For I.I: images: zoomed image size/1024            |
| Grid  | (0018,1166)  | “NONE”, “FOCUSSED”, “UNIVERSAL”   |
| Date of Last Calibration                    | (0018,1200)  |   |
| Acquisition Device Processing Description   | (0018,1400)  | Description of processing parameter set   |
| Acquisition Device Processing Code          | (0018,1401)  | Code to identify processing parameter set   |
| Relative X-Ray Exposure                     | (0018,1405)  | Exposure Index (EXI)  |
| Column Angulation                           | (0018,1450)  | From Acquisition  |
| Tomo Layer Height                           | (0018,1460)  | only for tomo acquisitions  |
| Tomo Angle                                  | (0018,1470)  | only for tomo acquisitions  |
| Tomo Time                                   | (0018,1480)  | only for tomo acquisitions  |
| Positioner Type                             | (0018,1508)  | device dependent  |
| Shutter Shape                               | (0018,1600)  | RECTANGULAR for detector images<br>CIRCULAR for I.I images  |
| Shutter Left Vertical Edge                  | (0018,1602)  | From Acquisition / Post-processing  |
| Shutter Right Vertical Edge                 | (0018,1604)  | From Acquisition / Post-processing  |
| Shutter Upper Horizontal Edge               | (0018,1606)  | From Acquisition / Post-processing  |
| Shutter Lower Horizontal Edge               | (0018,1608)  | From Acquisition / Post-processing  |
| Center of Circular Shutter                  | (0018,1610)  | for I.I images  |
| Radius of Circular Shutter                  | (0018,1612)  | for I.I images  |
| View Position                               | (0018,5101)  | Only if information is available  |
| Sensitivity                                 | (0018,6000)  |   |
| Detector Conditions Nominal Flag            | (0018,7000)  | Set to "NO" if user was notified about possible image quality compromise, e.g. because detector temperature is out of range |

| Attribute Name                    | Tag         | Value  |
|-----------------------------------|-------------|--|
| Detector Temperature              | (0018,7001) | the last received detector temperature   |
| Detector Type                     | (0018,7004) | "SCINTILLATOR"   |
| Detector Description              | (0018,7006) | only for detector images<br>Detector data:<br>- Factory Serial Number<br>- Factory Date Code<br>- Configuration Version<br>- Factory Part Number |
| Detector ID                       | (0018,700A) | Factory Serial Number  |
| Date of Last Detector Calibration | (0018,700C) | <yyyymmdd>   |
| Time of Last Detector Calibration | (0018,700E) | <hhmmss>   |
| Field of View Origin              | (0018,7030) |  |
| Field of View Rotation            | (0018,7032) | Enumerated Values: "0", "90", "180", "270"   |
| Field of View Horizontal Flip     | (0018,7034) | Enumerated Values: "NO", "YES"   |
| Grid Focal Distance               | (0018,704C) | "1150", "1250", "1500", "1800", "3000"<br>only if Grid (0018,1166) = FOCUSED"  |
| X-Ray Tube Current in $\mu$ A     | (0018,8151) | From Acquisition, not available for all devices  |
| Samples per Pixel                 | (0028,0002) | 1  |
| Photometric Interpretation        | (0028,0004) |  |
| Number of Frames                  | (0028,0008) |  |
| Frame Increment Pointer           | (0028,0009) | <0018,1063> only if multi-frame  |
| Rows                              | (0028,0010) | Depending on detector and acquisition mode   |
| Columns                           | (0028,0011) | Depending on detector and acquisition mode   |
| Pixel Spacing                     | (0028,0030) | only if configured in service<br>value = 0018,1164 if no SOD is present<br>otherwise: value = (0018,1164) * SOD / SID                            |
| Bits Allocated                    | (0028,0100) | 8, 16 depending on user selection  |
| Bits Stored                       | (0028,0101) | 8, 16 depending on user selection  |
| High Bit                          | (0028,0102) | 7, 15 depending on user selection  |
| Pixel Representation              | (0028,0103) | 0  |
| Pixel Intensity Relationship      | (0028,1040) | LIN  |
| Representative Frame Number       | (0028,6010) | Only if multi-frame  |

## A.4 CR,DX Standard Extended SOP Class


### Overview of supplied attributes –CR/DX image

| Attribute Name                            | Tag          | Value  |
|---|--------------|--|
| Modality                                  | (0008,0060)  | “CR” or “DX”   |
| Presentation Intent Type                  | (0008,0068)  | “FOR PRESENTATION” (DX only)   |
| Anatomic Region Sequence                  | (0008,2218)  | Empty (DX only)  |
| Body Part Examined                        | (0018,0015)  | -value from OGP<br>-Zero length if not available   |
| KVP                                       | (0018,0060)  | From Acquisition   |
| Device Serial Number                      | (0018,1000)  | From Configuration   |
| Software Version                          | (0018,1020)  | From Configuration   |
| Protocol Name                             | (0018,1030)  | Organ Program Name   |
| Distance Source to Detector               | (0018,1110)  | SID from Acquisition (not available for all devices)   |
| Distance Source to Patient                | (0018,1111)  | - SOD (only if table object distance, image receptor table distance and SID are available)<br>- not available for free exposures |
| Table Angle                               | (0018,1138)  | From Acquisition   |
| Table Type                                | (0018,113A)  | “TILTING”  |
| Field of View Shape                       | (0018,1147)  | “RECTANGLE”  |
| Field of View Dimension(s)                | (0018, 1149) | rows\columns in mm   |
| Exposure Time                             | (0018,1150)  | From Acquisition, not available for all devices (e.g. Mobilett Mira Max / MOBILETT Elara Max)                                    |
| Exposure                                  | (0018,1152)  | From Acquisition   |
| Exposure in $\mu$ As                      | (0018,1153)  | From Acquisition   |
| X-Ray Tube Current                        | (0018,1151)  | From Acquisition, not available for all devices  |
| Filter Type                               | (0018,1160)  | Defined Terms:<br>“NONE”, “CU_0.1_MM”, “CU_0.2_MM”, “CU_0.3_MM”  |
| Radiation Setting                         | (0018,1155)  | GR   |
| Radiation Mode                            | (0018,115A)  | PULSED   |
| Image Area Dose Product                   | (0018,115E)  | Only if dose measurement is available, in $\text{dGy cm}^2$ .  |
| Imager Pixel Spacing                      | (0018,1164)  | detector dependent   |
| Grid                                      | (0018,1166)  | “NONE”, “FOCUSED”, “UNIVERSAL”<br>Always “NONE” for Multix Fusion Max  |
| Acquisition Device Processing Description | (0018,1400)  | Description of processing parameter set  |
| Acquisition Device Processing Code        | (0018,1401)  | Code to identify processing parameter set  |
| Relative X-Ray Exposure                   | (0018,1405)  | Exposure Index (EXI)   |
| Exposure Index                            | (0018,1411)  | Clinical Exi value, (in units of 100. $\mu$ Gy)  |
| Target Exposure Index                     | (0018,1412)  | From OGP, (in units of 100. $\mu$ Gy)  |
| Deviation Index                           | (0018,1413)  |  |
| Column Angulation                         | (0018,1450)  | From Acquisition   |
| Tomo Layer Height                         | (0018,1460)  | only for tomo acquisitions   |
| Tomo Angle                                | (0018,1470)  | only for tomo acquisitions   |
| Tomo Time                                 | (0018,1480)  | only for tomo acquisitions   |
| Positioner Type                           | (0018,1508)  | device dependent   |
| Patient Position                          | (0018,5100)  | not available  |
| View Position                             | (0018,5101)  | Only if information is available   |
| Sensitivity                               | (0018,6000)  |  |
| Detector Conditions Nominal Flag          | (0018,7000)  | Set to “NO” if user was notified about possible image quality compromise, e.g. because detector temperature is out of range      |
| Detector Temperature                      | (0018,7001)  | the last received detector temperature   |
| Detector Type                             | (0018,7004)  | “SCINTILLATOR”   |
| Detector Description                      | (0018,7006)  | only for detector images<br>Detector data:<br>- Factory Serial Number<br>- Factory Date Code<br>- Configuration Version          |

| Attribute Name                    | Tag         | Value   |
|-----------------------------------|-------------|---|
|                                   |             | - Factory Part Number   |
| Detector ID                       | (0018,700A) | Factory Serial Number   |
| Date of Last Detector Calibration | (0018,700C) | <yyyymmdd>  |
| Time of Last Detector Calibration | (0018,700E) | <hhmmss>  |
| Field of View Origin              | (0018,7030) |   |
| Field of View Rotation            | (0018,7032) | Enumerated Values: "0", "90", "180", "270"  |
| Field of View Horizontal Flip     | (0018,7034) | Enumerated Values: "NO", "YES"  |
| Grid Focal Distance               | (0018,704C) | "1150", "1250", "1500", "1800", "3000"<br>only if Grid (0018,1166) = FOCUSED<br>not available for Multix Fusion Max   |
| X-Ray Tube Current in $\mu$ A     | (0018,8151) | From Acquisition, not available for all devices   |
| Image Laterality                  | (0020,0062) | User Input / Organ Program /empty (DX only)   |
| Samples per Pixel                 | (0028,0002) | 1   |
| Photometric Interpretation        | (0028,0004) | MONOCHROME2   |
| Rows                              | (0028,0010) | Depending on detector and acquisition mode  |
| Columns                           | (0028,0011) | Depending on detector and acquisition mode  |
| Pixel Spacing                     | (0028,0030) | only if configured in service<br>value = 0018,1164 if no SOD is present<br>otherwise: value = (0018,1164) * SOD / SID |
| Bits Allocated                    | (0028,0100) | 16  |
| Bits Stored                       | (0028,0101) | 16  |
| High Bit                          | (0028,0102) | 15  |
| Pixel Representation              | (0028,0103) | 0   |
| Pixel Intensity Relationship      | (0028,1040) | DISP or LIN for DX  |
| Rescale Intercept                 | (0028,1052) | 0 (DXonly)  |
| Rescale Slope                     | (0028,1053) | 1 (DXonly)  |
| Rescale Type                      | (0028,1054) | US (DXonly)   |
| Pixel Intensity Relationship Sign | (0028,1041) | "-1" for "Bones White"<br>"1" for "Bones Black"<br>Remark: DX only, uncertainty of LUT handling                       |

## A.5 X-Ray Radiation Dose SR SOP Class

The syngo FLC will create X-Ray Radiation Dose SRs implementing TID 10001 Projection X-Ray Radiation Dose as indicated in Figure 9.

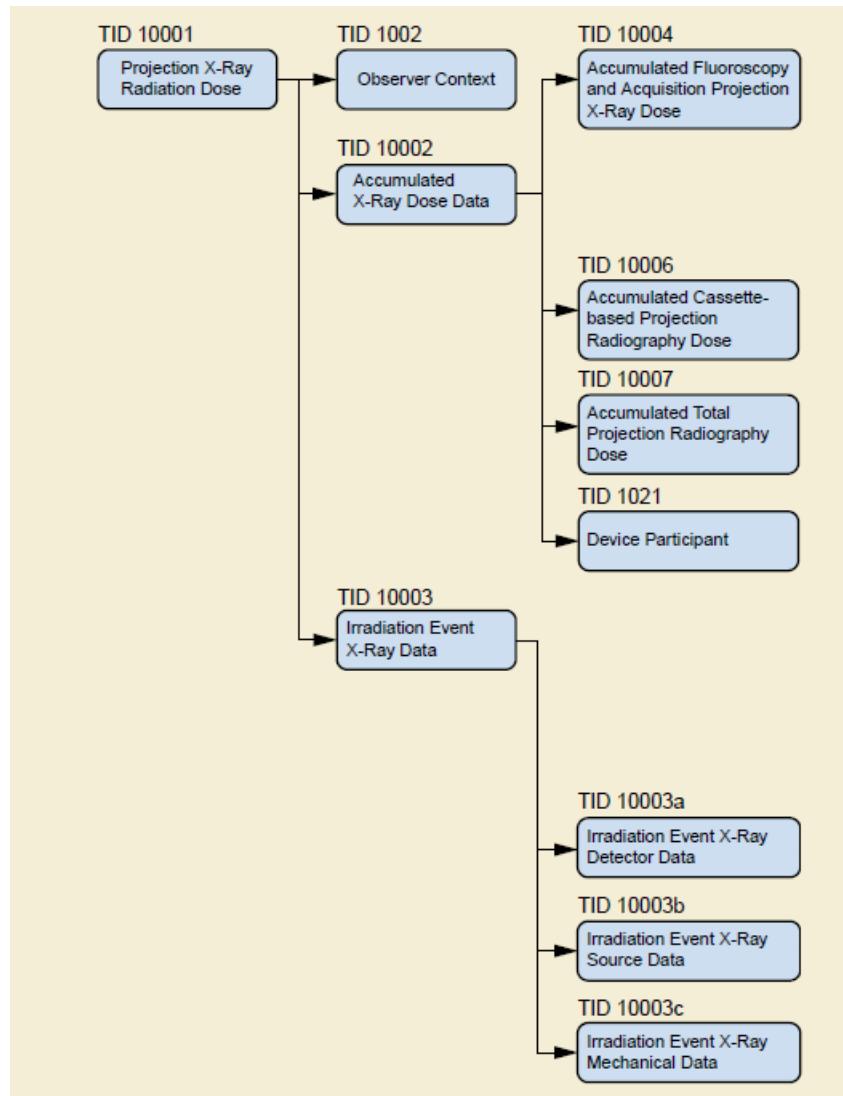

**Figure 9: X-Ray Radiation Dose SR IOD Template Structure**

The scope of accumulation is "Study" or "Performed Procedure Step" if MPPS is configured.

The report is kept open (Completion Flag (0040,A491) = "PARTIAL") to support continuation of the study. Closing a study will set the Completion Flag (0040,A491) to "COMPLETED". Updating of a SR will not change the SOP Instance UID.

All patient level, study level and equipment information is taken from the acquired images. The related attribute mapping from Modality Worklist to X-Ray Radiation Dose SR is equal to the mapping into acquired images. Please refer to A.10 syngo FLC Worklist Identifier for mapping of worklist information.

### A.5.1 Projection X-Ray Radiation Dose (TID 10001)

| NL                           | Relation with Parent | VT        | Concept Name  | Value  |
|------------------------------|----------------------|-----------|---|--|
|                              |                      | CONTAINER | EV (113701, DCM, "X-Ray Radiation Dose Report")   | Root node.   |
| >                            | HAS CONCEPT MOD      | CODE      | EV (121058, DCM, "Procedure reported")  | DT (113704, DCM, "Projection X-Ray")   |
| >>                           | HAS CONCEPT MOD      | CODE      | EV (G-C0E8, SRT, "Has Intent")  | EV (R-408C3, SRT, "Diagnostic Intent")                                       |
| DTID 1002 "Observer Context" |                      |           |   |  |
| >                            | HAS OBS CONTEXT      | CODE      | EV (121005, DCM, "Observer Type")   | EV (121007, DCM, "Device")   |
| >                            | HAS OBS CONTEXT      | UIDREF    | EV (121012, DCM, "Device Observer UID")   | Root UID including serial number   |
| >                            | HAS OBS CONTEXT      | TEXT      | EV (121013, DCM, "Device Observer Name")  | Value from Station Name (0008,1010)  |
| >                            | HAS OBS CONTEXT      | TEXT      | EV (121014, DCM, "Device Observer Manufacturer")  | Value from Manufacturer (0008,0070)  |
| >                            | HAS OBS CONTEXT      | TEXT      | EV (121015, DCM, "Device Observer Model Name")  | Value from Manufacturer's Model Name (0008,1090)                             |
| >                            | HAS OBS CONTEXT      | TEXT      | EV (121016, DCM, "Device Observer Serial Number")   | Value from Device Serial Number (0018,1000)                                  |
| >                            | HAS OBS CONTEXT      | CODE      | EV (113705, DCM, "Scope of Accumulation")   | EV (113016, DCM, "Performed Procedure Step") or<br>EV (113014, DCM, "Study") |
| >>                           | HAS PROPERTIES       | UIDREF    | EV (121126, DCM, "Performed Procedure Step SOP Instance UID")<br>or<br>EV (110180, DCM, "Study Instance UID") | Study Instance UID or MPPS UID   |
| >                            | CONTAINS             | INCLUDE   | DTID 1002 "Accumulated X-Ray Dose"  | See A.5.2  |
| >                            | CONTAINS             | INCLUDE   | DTID 10003 "Irradiation Event X-Ray Data"   | For each Irradiation Event. See A.5.3  |
| >                            | CONTAINS             | CODE      | EV (113854, DCM, "Source of Dose Information")  | EV ("A-2C090", SRT, "Dosimeter")   |
| >                            | CONTAINS             | TEXT      | EV (121106, DCM, "Comment")   | Formatted report.  |

## A.5.2 Accumulated X-Ray Dose (TID 10002)

| NL | Relation with Parent | VT        | Concept Name  | Value  |
|----|----------------------|-----------|---|--|
|    |                      | CONTAINER | EV (113702, DCM, "Accumulated X-Ray Dose Data")                 |  |
| >  | HAS CONCEPT MOD      | CODE      | EV (113764, DCM, "Acquisition Plane")                           | EV (113622, DCM, "Single Plane")                           |
| >  | CONTAINS             | CONTAINER | EV (122505, DCM, "Calibration")                                 |  |
| >> | HAS CONCEPT MOD      | CODE      | EV (113794, DCM, "Dose Measurement Device")                     | EV (A-2C090, SRT, "Dosimeter")                             |
| >> | CONTAINS             | DATETIME  | EV (113723, DCM, "Calibration Date")                            | Date and time of dosimeter calibration                     |
| >> | CONTAINS             | NUM       | EV (122322, DCM, "Calibration Factor")                          | 1  |
| >> | CONTAINS             | NUM       | EV (113763, DCM, "Calibration Uncertainty")                     | Read from local file.                                      |
| >> | CONTAINS             | TEXT      | EV (113724, DCM, "Calibration Responsible Party")               | Read from local file.                                      |
| >  | CONTAINS             | NUM       | EV (113722, DCM, "Dose Area Product Total") <sup>1</sup>        | Accumulated dose area product from FLUORO and acquisition. |
| >  | CONTAINS             | NUM       | EV (113725, DCM, "Dose (RP) Total")                             | Accumulated entrance dose from FLUORO and acquisition.     |
| >  | CONTAINS             | NUM       | EV (113726, DCM, "Fluoro Dose Area Product Total") <sup>1</sup> | Accumulated dose area product from FLUORO only.            |
| >  | CONTAINS             | NUM       | EV (113728, DCM, "Fluoro Dose (RP) Total") <sup>1</sup>         | Accumulated entrance dose from FLUORO only.                |
| >  | CONTAINS             | NUM       | EV (113730, DCM, "Total Fluoro Time") <sup>1</sup>              | The time the FLUORO switch was pressed.                    |
| >  | CONTAINS             | NUM       | EV (113727, DCM, "Acquisition Dose Area Product Total")         | Accumulated dose area product from acquisition only.       |
| >  | CONTAINS             | NUM       | EV (113729, DCM, "Acquisition Dose (RP) Total")                 | Accumulated entrance dose from acquisition only.           |

<sup>1</sup> Only present in case of at least one FLUORO event.

| NL | Relation with Parent | VT   | Concept Name                                   | Value   |
|----|----------------------|------|--|---|
| >  | CONTAINS             | CODE | EV (113780, DCM, "Reference Point Definition") | <b>Luminos dRF and Uroskop Omnia:</b><br>EV (113863, DCM, "30cm above table")<br><b>Luminos Agile:</b><br>EV (113862, DCM, "1cm above table")<br><b>Ysio:</b><br>EV (1000, SMS_XP, "Skin Focus Distance Configuration") |
| >  | CONTAINS             | NUM  | EV (113855, DCM, "Total Acquisition Time")     | Accumulated acquisition time.   |

### A.5.3 Irradiation Event X-Ray Data (TID 10003)

| NL  | Relation with Parent | VT        | Concept Name  | Value  |
|-----|----------------------|-----------|---|--|
| >   | CONTAINS             | CONTAINER | EV (113706, DCM, "Irradiation Event X-Ray Data")                |  |
| >>  | HAS CONCEPT MOD      | CODE      | EV (113764, DCM, "Acquisition Plane")                           | EV (113662, DCM, "Single Plane")   |
| >>  | CONTAINS             | DATETIME  | DT (111526, DCM, "DateTime Started")                            | Date/Time the irradiation event started  |
| >>  | CONTAINS             | CODE      | EV (113721, DCM, "Irradiation Event Type")                      | EV (113611, DCM, "Stationary Acquisition") or<br>EV (P5-06000, SRT, "Fluoroscopy") or<br>EV (113612, DCM, "Stepping Acquisition") or<br>EV (113613, DCM, "Rotational Acquisition") |
| >>  | CONTAINS             | TEXT      | EV (125203, DCM, "Acquisition Protocol")                        | Name of used OGP or FLUORO program   |
| >>  | CONTAINS             | CODE      | EV (113780, DCM, "Reference Point Definition")                  | See A.5.2  |
| >>  | CONTAINS             | UIDREF    | EV (113769, DCM, "Irradiation Event UID")                       | Value from Irradiation Event UID (0008,3010)   |
| >>  | CONTAINS             | NUM       | EV (122130, DCM, "Dose Area Product")                           | Dose Area Product for this irradiation event.  |
| >>  | CONTAINS             | NUM       | EV (113845, DCM, "Exposure Index")                              |  |
| >>  | CONTAINS             | NUM       | EV (113846, DCM, "Target Exposure Index")                       |  |
| >>  | CONTAINS             | NUM       | EV (113847, DCM, "Deviation Index")                             |  |
| >>  | CONTAINS             | NUM       | EV (113738, DCM, "Dose (RP)")                                   | Entrance Dose for this irradiation event.  |
| >>  | CONTAINS             | NUM       | EV (113770, DCM, "Column Angulation")                           | Value from Column Angulation (0018,1450)   |
| >>  | CONTAINS             | CONTAINER | EV (113771, DCM, "X-Ray Filters")                               |  |
| >>> | CONTAINS             | CODE      | EV (113772, DCM, "X-Ray Filter Type")                           | EV (111609, DCM, "No Filter") or<br>EV (113650, DCM, "Strip filter")   |
| >>> | CONTAINS             | CODE      | EV (113757, DCM, "X-Ray Filter Material") <sup>1</sup>          | EV (C-127F9, SRT, "Copper or Copper compound")   |
| >>> | CONTAINS             | NUM       | EV (113758, DCM, "X-Ray Filter Thickness Minimum") <sup>1</sup> | Thickness of copper filter.  |
| >>> | CONTAINS             | NUM       | EV (113773, DCM, "X-Ray Filter Thickness Maximum") <sup>1</sup> | Thickness of copper filter.  |
| >>  | CONTAINS             | CODE      | EV (113732, DCM, "Fluoro Mode") <sup>2</sup>                    | EV (113631, DCM, "Pulsed")   |
| >>  | CONTAINS             | NUM       | EV (113791, DCM, "Pulse Rate") <sup>2</sup>                     | FLUORO frame rate.   |
| >>  | CONTAINS             | NUM       | EV (113768, DCM, "Number of Pulses")                            |  |
| >>  | CONTAINS             | NUM       | EV (113733, DCM, "KVP")   |  |
| >>  | CONTAINS             | NUM       | EV (113734, DCM, "X-Ray Tube Current")                          |  |
| >>  | CONTAINS             | NUM       | EV (113824, DCM, "Exposure Time")                               |  |
| >>  | CONTAINS             | NUM       | EV (113793, DCM, "Pulse Width")                                 |  |
| >>  | CONTAINS             | NUM       | EV (113736, DCM, "Exposure")                                    |  |
| >>  | CONTAINS             | NUM       | EV (113742, DCM, "Irradiation Duration")                        |  |

<sup>1</sup> Only if filter was used.

<sup>2</sup> Only for FLUORO irradiation events.

| NL  | Relation with Parent | VT     | Concept Name  | Value   |
|-----|----------------------|--------|---|---|
| >>  | CONTAINS             | NUM    | EV (113750,DCM, "Distance Source to Detector") <sup>1</sup> |   |
| >>  | CONTAINS             | CODE   | EV (123014,DCM, "Target Region")                            | Filled with entry from CID 4031 "Common Anatomic Regions" - part 16 of [DICOM]                          |
| >>  | CONTAINS             | CODE   | EV (113876, DCM, "Device Role in Procedure")                | EV (113859, DCM, "Irradiating Device")  |
| >>> | HAS PROPERTIES       | TEXT   | EV (113878, DCM, "Device Manufacturer")                     | SIEMENS   |
| >>> | HAS PROPERTIES       | TEXT   | EV (113879, DCM, "Device Model Name")                       | Fluorospot Compact FD   |
| >>> | HAS PROPERTIES       | TEXT   | EV (113880, DCM, "Device Serial Number")                    | Value from Device Serial Number (0018,1000).  |
| >>> | HAS PROPERTIES       | UIDREF | EV (121012, DCM, "Device Observer UID")                     | Root UID including serial number  |
| >>  | CONTAINS             | IMAGE  | EV (113795, DCM, "Acquired Image")                          | Reference to the image (but only in case an image was created for this event). Not present for FLUOROS. |

---

<sup>1</sup> Only in case distance is known.

## A.6 EXAM Protocol as Secondary Capture Image

The syngo FLC will create a secondary capture image containing the "Exam Protocol" as image. The Secondary Capture Image Storage Service Class (1.2.840.10008.5.1.4.1.1.7) is used for this.

The value for Modality (0008,0060) depends on the images, acquired for this procedure step. If **only** RAD images are present, "CR" is used. If DFR images are present "RF" is used.

*Overview of supplied attributes –SC image*

| Attribute Name  | Tag         | Value        |
|-----------------|-------------|--------------|
| Modality        | (0008,0060) | "CR" or "RF" |
| Conversion Type | (0008,0064) | "DI"         |
| Rows            | (0028,0010) | 2100         |
| Columns         | (0028,0011) | 2970         |
| Bits Allocated  | (0028,0100) | 16           |
| Bits Stored     | (0028,0101) | 12           |
| High Bit        | (0028,0102) | 11           |

Additionally the following private attributes are used for documentation of accumulated dose values:

| Tag         | Private Owner Code           | Name                          | VR | VM |
|-------------|------------------------------|-------------------------------|----|----|
| (0017,xxD0) | SIEMENS_FLCOMPACT_VA01A_PROC | Accumulated fluorotime in sec | US | 1  |
| (0017,xxD1) | SIEMENS_FLCOMPACT_VA01A_PROC | Accumulated DAP in dGy*cm*cm  | LO | 1  |
| (0017,xxD2) | SIEMENS_FLCOMPACT_VA01A_PROC | Accumulated Skin Dose in mGy  | LO | 1  |

The scope of accumulation is the Procedure Step.

## A.7 XA Standard Extended SOP Class

*Overview of specific attributes – XA image*

| Attribute Name                                  | Tag         | Value  |
|---|-------------|--|
| Image Type                                      | (0008,0008) | ORIGINAL\PRIMARY\ SINGLE PLANE\3DSCAN\3DRAX  |
| Distance Source to Detector                     | (0018,1110) | Contains the SID.  |
| Distance Source to Patient                      | (0018,1111) | Contains the SOD.  |
| Estimated Radiographic Magnification Factor     | (0018,1114) | Ratio of SID over SOD.   |
| Intensifier Size                                | (0018,1162) | 480  |
| Positioner Motion                               | (0018,1500) | STATIC if the imaging table moves during a multi-frame acquisition, but the X-Ray positioner does not move. Otherwise DYNAMIC. |
| Positioner Primary Angle                        | (0018,1510) | 0  |
| Positioner Secondary Angle                      | (0018,1511) | 0  |
| Positioner Primary Angle Increment              | (0018,1520) | (0,...,0) for each frame   |
| Positioner Secondary Angle Increment            | (0018,1521) | (0,...,0) for each frame   |
| Detector Primary Angle                          | (0018,1530) | Not contained  |
| Detector Secondary Angle                        | (0018,1531) | Not contained  |
| Collimator Left Vertical Edge                   | (0018,1702) | According to initial collimator settings.  |
| Collimator Right Vertical Edge                  | (0018,1704) | According to initial collimator settings.  |
| Collimator Upper Horizontal Edge                | (0018,1706) | According to initial collimator settings.  |
| Collimator Lower Horizontal Edge                | (0018,1708) | According to initial collimator settings.  |
| Patient Position                                | (0018,5100) | Always set as the Patient Position is needed for reconstruction to set the Patient Orientation.                                |
| <b>Private Creator “SIEMENS SMS-AX ACQ 1.0”</b> |             |  |
| Please refer to A.9.1                           |             |  |

## A.8 SOP Common Module – Image Type Extensions

*Overview of settings in tag Image Type (0008,0008)*

| Type of Scene / Image                             | Image Type   |
|---|--|
| Standard DFR Acquisition Image (Single and Scene) | ORIGINAL\PRIMARY\SINGLE PLANE                      |
| Fluoro Single Image                               | ORIGINAL\PRIMARY\SINGLE PLANE\FLUORO\SINGLE        |
| Fluoro Scene                                      | ORIGINAL\PRIMARY\SINGLE PLANE\FLUORO\LOOP          |
| DSA Single Image                                  | ORIGINAL\PRIMARY\SINGLE PLANE\STORE MONITOR\DSA    |
| DSA Peak Opacification                            | ORIGINAL\PRIMARY\SINGLE PLANE\STORE MONITOR\PEAKOP |
| DSA Series  | ORIGINAL\PRIMARY\SINGLE PLANE\DSA                  |
| Store Monitor Average                             | DERIVED\SECONDARY\SINGLE PLANE\SUM                 |
| Standard Roadmap Series                           | ORIGINAL\PRIMARY\SINGLE PLANE\ROADMAP\LOOP         |
| Roadmap Single Image                              | ORIGINAL\PRIMARY\SINGLE PLANE\ROADMAP\SINGLE       |
| Fluoro Image Last Image Hold                      | ORIGINAL\PRIMARY\SINGLE PLANE\FLUORO\LIH           |
| Twinview/Quadview Image                           | DERIVED\SECONDARY\SINGLE PLANE\COMBI               |
| Tomography Image                                  | ORIGINAL\PRIMARY\TOMO                              |
| Tomography Image (Image Intensifier)              | ORIGINAL\PRIMARY\SINGLE PLANE\TOMO                 |
| Scan Mode Image                                   | ORIGINAL\PRIMARY\SINGLE PLANE\SCAN                 |
| Radiography Image                                 | ORIGINAL\PRIMARY\RAD                               |
| Tilting Ortho Mode Image                          | ORIGINAL\PRIMARY\ORTHO\TILTING                     |
| Exam Protocol as Secondary Capture                | DERIVED\SECONDARY\SINGLE PLANE\EXAM PROTOCOL       |
| Composed Image                                    | DERIVED\SECONDARY\"algorithm"\\"version"           |
| Videomanager Image                                | ORIGINAL\PRIMARY\SINGLE PLANE\CAP                  |
| Store Monitor of Standard Single Image            | DERIVED\SECONDARY\SINGLE PLANE\STORE MONITOR       |
| Multitom Rax Projection Images                    | ORIGINAL\PRIMARY\SINGLE PLANE\3DSCAN\3DRAX         |

## A.9 Private Data

### A.9.1 General Private Data

The following tables describe private data that may be used for the FLC generated IODs.

*Private Creator "SIEMENS\_FLCOMPACT\_VA01A\_PROC"*

| Tag         | Name                                 | VR | VM |
|-------------|--------------------------------------|----|----|
| (0017,xx0A) | Blackening Correction                | SS | 1  |
| (0017,xx0B) | Dose Level                           | SS | 1  |
| (0017,xx0C) | SDM                                  | SS | 1  |
| (0017,xx0D) | Frame Rate                           | FL | 1  |
| (0017,xx0E) | Characteristic Curve                 | LO | 1  |
| (0017,xx0F) | Acquisition Filter                   | LO | 1  |
| (0017,xx10) | Skin Dose                            | SS | 1  |
| (0017,xx11) | Focus                                | SS | 1  |
| (0017,xx14) | Native Edge Enhancement Percent Gain | US | 1  |
| (0017,xx16) | Bone Level Black White               | US | 1  |
| (0017,xx17) | Contrast Native                      | US | 1  |
| (0017,xx18) | Brightness Native                    | US | 1  |
| (0017,xx19) | ShutterX                             | US | 1  |
| (0017,xx1A) | ShutterXY                            | US | 1  |
| (0017,xx1B) | FlipH                                | US | 1  |

| Tag         | Name  | VR | VM |
|-------------|---|----|----|
| (0017,xx1C) | FlipV   | US | 1  |
| (0017,xx1E) | Zoom  | US | 1  |
| (0017,xx1F) | PanX  | SS | 1  |
| (0017,xx20) | PanY  | SS | 1  |
| (0017,xx21) | Harmonization                                 | US | 1  |
| (0017,xx22) | Mask Frame Number                             | US | 1  |
| (0017,xx23) | DSA Viewing Mode                              | US | 1  |
| (0017,xx24) | DSA Contrast Subtracted                       | US | 1  |
| (0017,xx25) | DSA Brightness Subtracted                     | US | 1  |
| (0017,xx26) | Subtracted Edge Enhancement Percent Gain      | US | 1  |
| (0017,xx27) | Anatomical Background Percent                 | US | 1  |
| (0017,xx28) | Pixel Shift X                                 | FL | 1  |
| (0017,xx29) | Pixel Shift Y                                 | FL | 1  |
| (0017,xx48) | Series Number                                 | SS | 1  |
| (0017,xx49) | Label   | SS | 1  |
| (0017,xx4A) | Label Position                                | SS | 1  |
| (0017,xx4B) | Acquisition Number String                     | SS | 1  |
| (0017,xx4C) | Modification Number String                    | LO | 1  |
| (0017,xx4D) | Single Series Flag                            | SS | 1  |
| (0017,xx4E) | FlcSeriesDate                                 | LO | 1  |
| (0017,xx4F) | FlcSeriesTime                                 | LO | 1  |
| (0017,xx50) | Image Type                                    | SS | 1  |
| (0017,xx51) | Calibration Factor                            | FL | 1  |
| (0017,xx52) | Edge Enhancement Kernel Native                | SS | 1  |
| (0017,xx53) | Edge Enhancement Kernel Subtracted            | SS | 1  |
| (0017,xx54) | Harmonization Kernel                          | SS | 1  |
| (0017,xx55) | DSA Flag                                      | SS | 1  |
| (0017,xx5A) | Overlay List V1                               | OW | 1  |
| (0017,xx5B) | Overlay List V2                               | OW | 1  |
| (0017,xx5C) | Overlay List V3                               | OW | 1  |
| (0017,xx64) | Native Edge Enhancement Percent Gain Acq.     | FL | 1  |
| (0017,xx66) | Bone Level Black White Acq.                   | US | 1  |
| (0017,xx67) | Contrast Native Acq.                          | US | 1  |
| (0017,xx68) | Brightness Native Acq.                        | US | 1  |
| (0017,xx85) | Harmonization Acq.                            | US | 1  |
| (0017,xx86) | Mask Frame Number Acq.                        | US | 1  |
| (0017,xx87) | DSA Viewing Mode Acq.                         | US | 1  |
| (0017,xx88) | DSA Contrast Subtracted Acq.                  | US | 1  |
| (0017,xx89) | DSA Brightness Subtracted Acq.                | US | 1  |
| (0017,xx8A) | Subtracted Edge Enhancement Percent Gain Acq. | US | 1  |
| (0017,xx8B) | Anatomical Background Percent Acq.            | US | 1  |
| (0017,xx8C) | Pixel Shift X Acq.                            | FL | 1  |
| (0017,xx8D) | Pixel Shift Y Acq.                            | FL | 1  |
| (0017,xx8E) | Shutter X Acq.                                | US | 1  |
| (0017,xx8F) | Shutter Y Acq.                                | US | 1  |
| (0017,xx90) | Internal Data                                 | US | 1  |
| (0017,xx91) | Internal Data                                 | US | 1  |
| (0017,xx92) | Internal Data                                 | US | 1  |
| (0017,xx93) | Internal Data                                 | US | 1  |
| (0017,xxA0) | Laterality                                    | US | 1  |
| (0017,xxA1) | Label1 Flag                                   | US | 1  |
| (0017,xxA2) | Position Label 1                              | LO | 1  |
| (0017,xxAA) | System Type                                   | US | 1  |

| Tag         | Name                                 | VR | VM |
|-------------|--------------------------------------|----|----|
| (0017,xxAB) | Internal Data                        | US | 1  |
| (0017,xxB0) | Detector Calibration Temperature     | DS | 1  |
| (0017,xxBF) | name of the performed OGP            | LO | 1  |
| (0017,xxC0) | name of the performed Exam           | LO | 1  |
| (0017,xxC1) | Internal Data                        | US | 1  |
| (0017,xxC2) | Internal Data                        | US | 1  |
| (0017,xxC3) | Stored marking number                | US | 1  |
| (0017,xxC4) | "Name for RIS" of the performed exam | LO | 1  |

*Private Creator "Thorax/Multix FD Lab Settings"*

| Tag         | Name                    | VR | VM  |
|-------------|-------------------------|----|-----|
| (0019,xx06) | Table Object Distance   | FD | 1   |
| (0019,xx07) | Table Detector Distance | FD | 1   |
| (0019,xx08) | Ortho Step Distance     | US | 1-n |
| (0019,xx09) | Asymmetric Collimation  | LO | 1   |

*Private Creator "Thorax/Multix FD Post Processing"*

| Tag         | Name                    | VR | VM |
|-------------|-------------------------|----|----|
| (0021,xx08) | Auto Window Flag        | US | 1  |
| (0021,xx09) | Auto Window Center      | SL | 1  |
| (0021,xx0A) | Auto Window Width       | SL | 1  |
| (0021,xx0B) | Filter ID               | SS | 1  |
| (0021,xx13) | Internal Value          | US | 1  |
| (0021,xx14) | Anatomic Correct View   | US | 1  |
| (0021,xx15) | Auto Window Shift       | SS | 1  |
| (0021,xx16) | Auto Window Expansion   | DS | 1  |
| (0021,xx17) | System Type             | LO | 1  |
| (0021,xx18) | Detector Type           | LO | 1  |
| (0021,xx30) | Anatomic Sort Number    | SH | 1  |
| (0021,xx31) | Acquisition Sort Number | SH | 1  |

*Private Creator "Siemens: Thorax/Multix FD Raw Image Settings"*

| Tag         | Name                    | VR | VM |
|-------------|-------------------------|----|----|
| (0025,xx00) | Raw Image Amplification | SS | 1  |
| (0025,xx0C) | Harmonization Kernel    | SS | 1  |
| (0025,xx0D) | Harmonization Gain      | FL | 1  |
| (0025,xx0E) | Edge Enhancement Kernel | SS | 1  |
| (0025,xx0F) | Edge Enhancement Gain   | FL | 1  |
| (0025,xx10) | Internal Value          | LT | 1  |
| (0025,xx18) | Auto Gain               | US | 1  |
| (0025,xx19) | Ortho Subsampling       | US | 1  |
| (0025,xx1A) | Image Crop Upper Left   | US | 2  |
| (0025,xx1B) | Image Crop Upper Right  | US | 2  |
| (0025,xx1C) | Image Crop Lower Left   | US | 2  |
| (0025,xx1D) | Image Crop Lower Right  | US | 2  |
| (0025,xx30) | Manual Cropping         | US | 1  |
| (0025,xx31) | Gamma LUT Parameter 1   | SS | 1  |
| (0025,xx32) | Gamma LUT Parameter 2   | DS | 1  |
| (0025,xx33) | Gamma LUT Parameter 3   | SS | 1  |

| Tag         | Name                  | VR | VM |
|-------------|-----------------------|----|----|
| (0025,xx34) | Gamma LUT Parameter 4 | SS | 1  |
| (0025,xx35) | Gamma LUT Name        | LO | 1  |
| (0025,xx36) | Physical EXI          | DS | 1  |
| (0025,xx37) | Clinical EXI          | DS | 1  |

*Private Creator "SIEMENS SMS-AX ACQ 1.0"*

| Tag         | Name                            | VR | VM  | Comment   |
|-------------|---------------------------------|----|-----|---|
| (0021,xx0F) | Xray Quadruples                 | SL | 1-n | (voltage, current in $\mu$ A, pulse time in $\mu$ s, $\mu$ As) per projection                         |
| (0021,xx62) | Reconstruction Preset           | US | 1   | 1973  |
| (0021,xxF0) | FlcXmlParams3D                  | UT | 1   | Contains XML structure with reconstruction parameters and parameters for Geometry and I0-Calibration. |
| (0021,xxF1) | Automatic Gain Correction (AGC) | FL | 1-n | Contains the AGC value for each frame.  |

## A.10 syngo FLC Worklist Identifier

| Module Name<br>Attribute Name               | Tag         | M | R | Q | UI | IOD            |
|---|-------------|---|---|---|----|----------------|
| <b>SOP Common</b><br>Specific Character Set | (0008,0005) |   | x |   |    | x              |
| <b>Scheduled Procedure Step</b>             |             |   |   |   |    |                |
| Scheduled Procedure Step Sequence           | (0040,0100) |   | x |   |    |                |
| > Scheduled Station AET                     | (0040,0001) | S |   |   |    |                |
| > Scheduled Procedure Step Start Date       | (0040,0002) | S |   |   |    |                |
| > Scheduled Procedure Step Start Time       | (0040,0003) | S |   |   |    |                |
| > Modality                                  | (0008,0060) | S |   |   |    |                |
| > Scheduled Performing Physician's Name     | (0040,0006) | S | x | x | x  | x <sup>1</sup> |
| > Scheduled Procedure Step Description      | (0040,0007) | S | x |   |    | x              |
| > Scheduled Protocol Code Sequence          | (0040,0008) | S | x |   |    | x              |
| >> Code Value                               | (0008,0100) | S | x |   |    | x              |
| >> Coding Scheme Designator                 | (0008,0102) | S | x |   |    | x              |
| >> Coding Scheme Version                    | (0008,0103) | S | x |   |    | x              |
| >> Code Meaning                             | (0008,0104) | S | x |   |    | x              |
| > Scheduled Procedure Step Location         | (0040,0011) | S | x |   |    |                |
| > Pre-Medication                            | (0040,0012) | S | x |   |    |                |
| > Scheduled Procedure Step ID               | (0040,0009) | S | x |   |    |                |
| > Scheduled Procedure Step Status           | (0040,0020) | S | x |   |    | x              |
| > Requested Contrast Agent                  | (0032,1070) | S | x |   |    |                |
| <b>Requested Procedure</b>                  |             |   |   |   |    |                |
| Requested Procedure ID                      | (0040,1001) | P | x | x | x  | x <sup>2</sup> |
| Requested Procedure Description             | (0032,1060) | P | x | x | x  | x <sup>3</sup> |
| Requested Procedure Code Sequence           | (0032,1064) | P | x | x | x  | x <sup>4</sup> |
| > Code Value                                | (0008,0100) | P | x | x | x  | x <sup>4</sup> |
| > Coding Scheme Designator                  | (0008,0102) | P | x | x | x  | x <sup>4</sup> |
| > Coding Scheme Version                     | (0008,0103) | P | x | x | x  | x <sup>4</sup> |
| > Code Meaning                              | (0008,0104) | P | x | x | x  | x <sup>4</sup> |
| Study Instance UID                          | (0020,000D) | P | x | x | x  | x              |
| Referenced Study Sequence                   | (0008,1110) | P | x | x | x  | x              |
| > Referenced SOP Class UID                  | (0008,1150) | P | x | x | x  | x              |
| > Referenced SOP Instance UID               | (0008,1155) | P | x | x | x  | x              |
| Requested Procedure Priority                | (0040,1003) | P | x | x | x  | x              |
| Names of Intended Recipients of Results     | (0040,1010) | P | x | x | x  | x              |
| Requested Procedure Comments                | (0040,1400) | P | x | x | x  | x              |
| <b>Imaging Service Request</b>              |             |   |   |   |    |                |
| Accession Number                            | (0008,0050) | P | x | x | x  | x              |
| Requesting Physician                        | (0032,1032) | P | x | x | x  | x              |
| Referring Physician's Name                  | (0008,0090) | P | x | x | x  | x              |
| Requesting Service                          | (0032,1033) | P | x | x | x  | x              |
| Imaging Service Request Comments            | (0040,2400) | P | x | x | x  | x              |
| <b>Visit Identification</b>                 |             |   |   |   |    |                |
| Institution Name                            | (0008,0080) |   | x |   | x  | x              |
| Admission ID                                | (0038,0010) |   | x |   | x  | x              |
| <b>Visit Status</b>                         |             |   |   |   |    |                |
| Current Patient Location                    | (0038,0300) |   | x | x |    | x              |
| <b>Visit Admission</b>                      |             |   |   |   |    |                |
| Admitting Diagnoses Description             | (0008,1080) |   | x |   |    | x              |
| <b>Visit Relationship</b>                   |             |   |   |   |    |                |
| Referenced Patient Sequence                 | (0008,1120) |   | x | x | x  | x              |
| > Referenced SOP Class UID                  | (0008,1150) |   | x | x | x  | x              |
| > Referenced SOP Instance UID               | (0008,1155) |   | x | x | x  | x              |

| Module Name<br>Attribute Name               | Tag         | M | R              | Q | UI | IOD            |
|---|-------------|---|----------------|---|----|----------------|
| <b>Patient Identification</b>               |             |   |                |   |    |                |
| Patient Name                                | (0010,0010) | P | x              | x | x  | x              |
| Patient ID                                  | (0010,0020) | P | x              | x | x  | x              |
| Other Patient IDs                           | (0010,1000) |   | x              |   |    | x              |
| Other Patient Names                         | (0010,1001) |   | x              |   |    | x              |
| <b>Patient Demographic</b>                  |             |   |                |   |    |                |
| Patient's Birth Date                        | (0010,0030) |   | x              |   | x  | <sup>5</sup> x |
| Patient's Sex                               | (0010,0040) |   | x              |   | x  | x              |
| Patient's Weight                            | (0010,1030) |   | x              |   | x  | x              |
| Patient's Size                              | (0010,1020) |   | x              |   | x  | x              |
| Patient's Address                           | (0010,1040) |   | x              |   |    |                |
| Military Rank                               | (0010,1080) |   | x              |   | x  | x              |
| Ethnic Group                                | (0010,2160) |   | x              |   |    | x              |
| Patient Comments                            | (0010,4000) |   | x              |   |    | x              |
| Confidentiality Constraints on Patient Data | (0040,3001) |   | x              |   |    | x              |
| <b>Patient Medical</b>                      |             |   |                |   |    |                |
| Patient State                               | (0038,0500) |   | x              |   |    |                |
| Patient Weight                              | (0010,1030) |   | x              |   |    | x              |
| Pregnancy Status                            | (0010,21C0) |   | x              |   |    |                |
| Medical Alerts                              | (0010,2000) |   | <sup>6</sup> x |   |    |                |
| Contrast Allergies                          | (0010,2110) |   | x              |   |    |                |
| Special Needs                               | (0038,0050) |   | x              |   |    |                |
| Smoking Status                              | (0010,21A0) |   | x              |   |    |                |
| Additional Patient History                  | (0010,21B0) |   | x              |   |    | x              |
| Last Menstrual Date                         | (0010,21D0) |   | x              |   |    |                |

Table 1: Basic Worklist C-FIND-RSP Return Key Attributes

The table should be read as follows:

**Attribute Name:** Attributes supported to build a syngo FLC Worklist Request Identifier.

**Tag:** Appropriate DICOM tag for this attribute.

**M:** Matching keys for Worklist Update. A "S" will indicate that syngo FLC will supply an attribute value for Single Value Matching. It can be configured that the attribute is used as Return Key only. A "P" indicated, that the user can enter a single value for a Patient based worklist query.

**R:** Return keys. A "x" will indicate that syngo FLC will supply this attribute as Return Key with zero length for Universal Matching.

**Q:** Interactive Query Key. A "x" will indicate that syngo FLC will supply this attribute as matching key, if entered in the Query Patient Worklist dialog. The other keys will then be Return Keys only.

**IOD:** An "x" indicates that this Worklist attribute is included into all Object Instances created during performance of the related Procedure Step.

The default Query Configuration is set to "Modality" and "Date". Optionally, matching for the own "AE Title" and "Date" is configurable. For "Date" one of the following settings could be configured: "Today", "Yesterday – Today", "Today +/- 12 hours", "Today +/- 24 hours", and "Use no Date".

In Patient based worklist update the usage of date and time can be deactivated! The Scheduled AE Title is used as Return Key only.

x<sup>1</sup> : "Scheduled Performing Physician's Name (0040,0006)" is not directly included in the header. However its value is stored in the header as "Performing Physician's Name (0008,1050)". It can be modified by user during Patient Registration.

x<sup>2</sup> : Requested Procedure ID (0040,1001) is directly included in the header. Additionally its value is stored in the header as Study ID (0020,0010). Study ID can be modified by the user during Patient Registration.

x<sup>3</sup>: Requested Procedure Description (0032,1060) is not directly included in the header. However its value is stored in the header as "Study Description (0008,1030)". It can be modified by user during Patient Registration.

x<sup>4</sup>: Requested Procedure Code Sequence (0032,1064) is not directly included in the header. However its value is stored in the header as "Procedure Code Sequence (0008,1032)". It is not sent, when the scheduled protocol codes differ from the performed protocol codes.

x<sup>5</sup>: If a date of birth (0010,0030) with zero\_length value is received via worklist, the date of birth will internally set to 1850/01/01.

The value 1850/01/01 for the date of birth is not used in a DICOM header (DICOM Send, MPPS, CD/DVD Export), but again replaced by zero\_length.

x<sup>6</sup>: Medical Alerts (0010,2000) has a VM of 1-n. Only 20 entries are accepted.

## A.11 Modality Performed Procedure Step Identifiers

| Attribute Name                                | Tag         | N-CREATE<br>no value                                     | N-CREATE<br>with value                                  | N-SET<br>Final                                 |
|---|-------------|--|---|--|
| Specific Character Set                        | (0008,0005) |  | value depends on regional settings                      | ./.  |
| Modality                                      | (0008,0060) |  | "CR", "RF"  | ./.  |
| Procedure Code Sequence                       | (0008,1032) | - If not received via worklist<br>- for unscheduled case | If received via worklist                                | ./.  |
| > Code Value                                  | (0008,0100) |  | From Modality Worklist (0032,1064)                      |  |
| > Coding Scheme Designator                    | (0008,0102) |  | From Modality Worklist (0032,1064)                      |  |
| > Coding Scheme Version                       | (0008,0103) |  | From Modality Worklist (0032,1064)                      |  |
| > Code Meaning                                | (0008,0104) |  | From Modality Worklist (0032,1064)                      |  |
| Referenced Patient Sequence                   | (0008,1120) | Y if not received via worklist                           | From Modality Worklist (0008,1120)                      | ./.  |
| Patient's Name                                | (0010,0010) |  | From Modality Worklist or user input (all 5 components) | ./.  |
| Patient ID                                    | (0010,0020) |  | From Modality Worklist or user input                    | ./.  |
| Patient's Birth Date                          | (0010,0030) |  | From Modality Worklist or user input                    | ./.  |
| Patient's Sex                                 | (0010,0040) |  | From Modality Worklist or user input                    | ./.  |
| Distance Source to Detector (SID)             | (0018,1110) | Y  |   | minimum value                                  |
| Image Area Dose Product                       | (0018,115E) | Y  |   | includes fluoro and cassette images            |
| Study ID                                      | (0020,0010) |  | From Modality Worklist (0040,1001) or user input        | ./.  |
| Performed Station AE Title                    | (0040,0241) |  | AE Title of MPPS SCU                                    | ./.  |
| Performed Station Name                        | (0040,0242) |  | Hostname  | ./.  |
| Performed Location                            | (0040,0243) | Y  |   | ./.  |
| Performed Procedure Step Start Date           | (0040,0244) |  | Y   | ./.  |
| Performed Procedure Step Start Time           | (0040,0245) |  | Y   | ./.  |
| Performed Procedure Step End Date             | (0040,0250) | Y  |   | ./. (if IN PROGRESS)<br>Actual end date (ELSE) |
| Performed Procedure Step End Time             | (0040,0251) | Y  |   | ./. (if IN PROGRESS)<br>Actual end time (ELSE) |
| Performed Procedure Step Status               | (0040,0252) |  | IN PROGRESS   | IN PROGRESS<br>DISCONTINUED<br>COMPLETED       |
| Performed Procedure Step ID                   | (0040,0253) |  | Internally created                                      | ./.  |
| Performed Procedure Step Description          | (0040,0254) |  | From Modality Worklist (0040,0007)                      | (0040,0007) or user input                      |
| Performed Procedure Type Description          | (0040,0255) | Y  |   | zero Length                                    |
| Performed Protocol Code Sequence <sup>1</sup> | (0040,0260) |  |   | ./.  |
| > Code Value                                  | (0008,0100) |  | From performed Exam                                     | From performed Exam                            |
| > Coding Scheme Designator                    | (0008,0102) |  | From performed Exam                                     | From performed Exam                            |
| > Coding Scheme Version                       | (0008,0103) |  | From performed Exam                                     | From performed Exam                            |

<sup>1</sup> items only present if system is configured to use protocol codes, otherwise zero length

| Attribute Name  | Tag         | N-CREATE<br>no value | N-CREATE<br>with value                                 | N-SET<br>Final   |
|---|-------------|----------------------|--|--|
| > Code Meaning  | (0008,0104) |                      | From performed Exam                                    | From performed Exam  |
| Scheduled Step Attributes Sequence                            | (0040,0270) |                      | If 1 <sup>st</sup> dose applied results in an Instance | ./.  |
| > Accession Number  | (0008,0050) |                      | From Modality Worklist                                 | ./.  |
| > Referenced Study Sequence                                   | (0008,1110) |                      |  | ./.  |
| >> Referenced SOP Class UID                                   | (0008,1150) |                      | From Modality Worklist                                 | ./.  |
| >> Referenced SOP Instance UID                                | (0008,1155) |                      | From Modality Worklist                                 | ./.  |
| > Study Instance UID  | (0020,000D) |                      | From Modality Worklist                                 | ./.  |
| > Requested Procedure Description                             | (0032,1060) |                      | From Modality Worklist                                 | ./.  |
| > Scheduled Procedure Step Description                        | (0040,0007) |                      | From Modality Worklist                                 | ./.  |
| > Scheduled Protocol Code Sequence                            | (0040,0008) |                      |  | ./.  |
| >> Code Value   | (0008,0100) |                      | From Modality Worklist (0040,0008)                     | ./.  |
| >> Coding Scheme Designator                                   | (0008,0102) |                      | From Modality Worklist (0040,0008)                     | ./.  |
| >> Coding Scheme Version                                      | (0008,0103) |                      | From Modality Worklist (0040,0008)                     | ./.  |
| >> Code Meaning   | (0008,0104) |                      | From Modality Worklist (0040,0008)                     | ./.  |
| > Scheduled Procedure Step ID                                 | (0040,0009) |                      | From Modality Worklist                                 | ./.  |
| > Requested Procedure ID                                      | (0040,1001) |                      | From Modality Worklist                                 | ./.  |
| Performed Procedure Step Discontinuation Reason Code Sequence | (0040,0281) | Y                    |  | only if (0040,0252) = "DISCONTINUED"   |
| > Code Value  |             |                      |  | See Context ID 9300 DICOM 3.16   |
| > Coding Scheme Designator                                    | (0008,0102) |                      |  | DCM  |
| > Code Meaning  | (0008,0104) |                      |  | See Context ID 9300  |
| Total Time of Fluoroscopy                                     | (0040,0300) | Y                    |  | Total time   |
| Total Number of Exposures                                     | (0040,0301) | Y                    |  | Number of exposures  |
| Distance Source to Entrance                                   | (0040,0306) | Y                    |  | Minimum value  |
| Exposure Dose Sequence  | (0040,030E) | Y                    |  | Zero or more items   |
| > KVP   | (0018,0060) |                      |  | Current value  |
| > Protocol Name   | (0018,1030) |                      |  | Current value, if extended MPPS is configured  |
| > X-Ray Tube Current in $\mu$ A                               | (0018,8151) |                      |  | Current value  |
| > Exposure Time   | (0018,1150) |                      |  | Current value  |
| > Filter Type   | (0018,1160) |                      |  | Current value  |
| > Image Area Dose Product                                     | (0018,115E) |                      |  | Current value, if Extended MPPS is configured  |
| > Entrance Dose in mGy  | (0040,8302) |                      |  | Current value, if Extended MPPS is configured  |
| Comments on Radiation Dose                                    | (0018,0310) | Y                    |  | Formatted table of dose information for all acquisition events format:<br><OPG  dGy*cm <sup>2</sup>   kV  mAs  Filter  Physical EXI>\r\n |
| Billing Procedure Sequence                                    | (0040,0320) | Y                    |  | Zero or more items   |
| Film Consumption Sequence                                     | (0040,0321) | Y                    |  | Zero or more items   |
| > Film Size ID  | (2010,0050) |                      |  | Y if Seq. present  |

| Attribute Name   | Tag         | N-CREATE<br>no value | N-CREATE<br>with value | N-SET<br>Final   |
|--|-------------|----------------------|------------------------|--|
| > Number of Films  | (2100,0170) |                      |                        | Y if Seq. present  |
| Performed Series Sequence                                    | (0040,0340) | Y                    |                        | One or more items  |
| > Retrieve AE Title  | (0008,0054) |                      |                        | AE Title of archive  |
| > Series Description   | (0008,103E) | --                   |                        | Organ Program<br>Name  |
| > Performing Physician's Name                                | (0008,1050) | --                   |                        | from Modality<br>Worklist (0040,0006)<br>or user input       |
| > Operator's Name  | (0008,1070) | --                   |                        | user input   |
| > Referenced Image Sequence                                  | (0008,1140) | --                   |                        | One or more items  |
| >> Referenced SOP Class UID                                  | (0008,1150) | --                   |                        | System dependent   |
| >> Referenced SOP Instance UID                               | (0008,1155) | --                   |                        | Y  |
| > Protocol Name  | (0018,1030) | --                   |                        | Organ Program  |
| > Series Instance UID  | (0020,000E) | --                   |                        | Y  |
| > Referenced Non-Image<br>Composite SOP Instance<br>Sequence | (0040,0220) |                      |                        | Zero length  |
| Entrance Dose in mGy   | (0040,8302) | Y                    |                        | Accumulated value,<br>includes fluoro and<br>cassette images |

## A.12 Grayscale Image Consistency

The used monitors come with a DICOM Grayscale Standard Display Function (GSDF) compliant factory pre-setting. A typical working environment setup is assumed for ambient light.

MAX systems VF10 is not commercially available in all countries. Due to regulatory reasons its future availability cannot be guaranteed. Please contact your local Siemens organization for further details.

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products/services/features included in this brochure are available through the Siemens sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice.

The information in this document contains general descriptions of the technical options available and may not always apply in individual cases.

Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens sales representative for the most current information.

In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we may recycle certain components where legally permissible.

For recycled components we use the same extensive quality assurance measures as for factory-new components.

Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

---

**Siemens Healthineers Headquarters**

Siemens Healthcare GmbH

Henkestr. 127

91052 Erlangen

Germany

Phone +49 9131 84-0

[siemens.com/healthineers](http://siemens.com/healthineers)