

syngo CT VB10

DICOM Conformance Statement



Overview

This DICOM Conformance Statement is written according to part PS 3.2 of DICOM® Standards Publication Part(s) 3, 4, ©NEMA.

Date of issue

The date of issue of this DICOM Conformance Statement document is 2018-04.

Applicability

The applications described in this conformance statement are implemented in the Siemens SOMATOM CT products using the Somaris/7 *syngo* CT VB10 software.



Table of Contents

Table of Contents	3
List of Figures	8
List of Tables	9
1 Introduction	12
1.1 Overview	12
1.2 Audience	12
1.3 Scope	13
1.4 Definitions, Acronyms and Abbreviations	14
1.4.1 Definitions	14
1.4.2 Acronyms and Abbreviations	14
1.5 References	15
1.6 Connectivity and Interoperability	15
Part I - Network	16
2 Implementation Models	17
2.1 Verification	17
2.1.1 Application Data Flow Diagram	17
2.1.2 Functional Definitions of Application	17
2.1.3 Sequencing of Real-World Activities	17
2.2 Storage	17
2.2.1 Application Data Flow Diagram	18
2.2.2 Functional Definitions of Application Entities	18
2.2.3 Sequencing of Real-World Activities	18
2.3 Storage Commitment	19
2.3.1 Application Data Flow Diagram	19
2.3.2 Functional Definitions of Application Entities	20
2.3.3 Sequencing of real-world activities	20
2.4 Query/Retrieve	21
2.4.1 Application Data Flow Diagram	21
2.4.2 Functional Definitions of Application Entities	22
2.4.3 Sequencing of Real-World Activities	22
2.5 Print	23
2.5.1 Application Data Flow Diagram	23
2.5.2 Functional Definitions of Application Entities	23
2.5.3 Sequencing of Real-World Activities	23
2.6 Model Worklist	24
2.6.1 Application Data Flow Diagram	24
2.6.2 Functional Definitions of Application Entities	25
2.6.3 Sequencing of Real-World Activities	25
2.7 Modality Performed Procedure Step	26
2.7.1 Application Data Flow Diagram	26
2.7.2 Functional Definitions of Application Entities	27
2.7.3 Sequencing of real World Activities	27

3	AE Specifications	28
3.1	Verification AE Specification	28
3.1.1	Association Establishment Policies	28
3.1.1.1	General	28
3.1.1.2	Number of Associations	28
3.1.1.3	Asynchronous Nature	28
3.1.1.4	Implementation Identifying Information	28
3.1.2	Association Initiation by Real-World Activity	28
3.1.2.1	Associated Real-World Activity - Verification	29
3.1.3	Association Acceptance Policy	29
3.2	Storage AE Specification	30
3.2.1	Association Establishment Policies	32
3.2.1.1	General	32
3.2.1.2	Number of Associations	32
3.2.1.3	Asynchronous Nature	32
3.2.1.4	Implementation Identifying Information	32
3.2.2	Association Initiation Policy	33
3.2.2.1	Associated Real-World Activity - Send (Storage SCU)	33
3.2.3	Association Acceptance Policy	46
3.2.3.1	Real-World Activity - Receive (Storage SCP)	47
3.3	Storage Commitment AE Specification	69
3.3.1	Association Establishment Policies	69
3.3.1.1	General	69
3.3.1.2	Number of Associations	69
3.3.1.3	Asynchronous Nature	69
3.3.1.4	Implementation Identifying Information	69
3.3.2	Association Initiation Policy	70
3.3.2.1	Real-World Activity - Send Storage Commitment Request	70
3.3.3	Association Acceptance Policy	71
3.3.3.1	Associated Real-World Activity - Receive Storage Commit SCU	71
3.4	Query/Retrieve AE Specification	74
3.4.1	Association Establishment Policies	75
3.4.1.1	General	75
3.4.1.2	Number of Associations	76
3.4.1.3	Asynchronous Nature	76
3.4.1.4	Implementation Identifying Information	76
3.4.2	Association Initiation Policy	76
3.4.2.1	Real-World Activity - Find SCU	76
3.4.2.2	Real-World Activity - Move SCU	82
3.4.3	Association Acceptance Policy	85
3.4.3.1	Real-World Activity - Find SCP	85
3.4.3.2	Real-World Activity - Get SCP	97
3.4.3.3	Real-World Activity - Move SCP	99
3.5	Print AE Specification	102
3.5.1	Association Establishment Policies	102
3.5.1.1	General	102
3.5.1.2	Number of Associations	103

3.5.1.3	Asynchronous Nature.....	103
3.5.1.4	Implementation Identifying Information	103
3.5.2	Association Initiation Policy.....	103
3.5.2.1	Real-World Activity	103
3.6	Modality Worklist AE Specification	123
3.6.1	Association Establishment Policies.....	123
3.6.1.1	General.....	123
3.6.1.2	Number of Associations	123
3.6.1.3	Asynchronous Nature.....	123
3.6.1.4	Implementation Identifying Information	123
3.6.2	Association Initiation Policy.....	124
3.6.2.1	Real-World Activity	124
3.7	Modality Performed Procedure Step AE Specification	135
3.7.1	Association Establishment Policies.....	135
3.7.1.1	General.....	135
3.7.1.2	Number of Associations	135
3.7.1.3	Asynchronous Nature.....	135
3.7.1.4	Implementation Identifying Information	135
3.7.2	Association Initiation Policy.....	135
3.7.2.1	Real-World Activity	136
4	Extensions/Specifications/Privatizations	145
4.1	Standard Extensions	145
4.1.1	Standard Extensions of all SOP Classes	145
4.1.1.1	Image Type	146
4.1.1.2	Body Part Examined.....	151
4.1.1.3	RGB color images	152
4.1.1.4	CT Images with Color Lookup Table	157
4.1.2	Specializations	158
4.1.2.1	Images created by Somaris/7.....	158
4.1.2.2	Structured Reports created by Somaris/7	164
4.1.2.3	Somaris/7 Attribute Interpretation.....	165
4.1.2.4	OOG, Overlays, High Bits	172
4.2	Privatizations.....	173
4.2.1	Private Elements for Storage SOP Classes.....	173
4.2.1.1	Registry of DICOM Data Elements.....	173
4.2.1.2	All syngo-Supported Image SOP Classes.....	175
4.2.2	Private Elements for CT Image Storage SOP Class.....	182
4.2.2.1	Registry of DICOM Data Elements.....	182
4.2.3	Private SOP class CSA Non-Image	185
4.2.3.1	CSA Non-Image IOD Entity Relationship Model	185
4.2.3.2	CSA Non-Image IOD Module Table	186
4.2.3.3	CSA Non-Image Module	187
4.2.3.4	CT Extensions of the Non-Image Object.....	189
4.2.4	Private SOP Classes.....	190
4.2.5	Private Transfer Syntaxes.....	190
5	Communication Profiles	191

5.1	Supported Communication Stacks	191
5.1.1	OSI Stack	191
5.1.2	TCP/IP Stack	191
5.1.2.1	API	191
5.1.2.2	Physical Media Support	191
5.1.3	Point-to-Point Stack	191
6	Configuration	192
6.1	AE Title / Presentation Address Mapping	192
6.1.1	DICOM Verification	193
6.1.2	DICOM Storage/StorageCommitment/QR AE Title	193
6.1.3	DICOM Modality Worklist and MPPS AE Title	193
6.1.4	DICOM Print AE Title	193
6.1.5	Remote AE Titles and Presentation Addresses	193
6.2	Configurable Parameters	193
6.2.1	Storage, Storage Commitment and Query/Retrieve	194
6.2.2	Print	194
6.2.3	Modality Worklist	195
6.2.4	Modality Performed Procedure Step	195
6.3	Default Parameters	196
7	Support of Extended Character Sets	197
8	Security	201
8.1	Security Profile	201
8.1.1	Security Transport Connection Profiles	201
Part II - Media Storage		204
9	Implementation Models	205
9.1	Application Data Flow Diagram	205
9.2	Functional definitions of AEs	205
9.3	Sequencing of Real-World Activities	206
9.4	File Meta Information Options	206
10	AE Specifications	207
10.1	DICOM Archive Specification	207
10.1.1	File Meta Information for the Application Entity	207
10.1.2	Real-World Activities for this Application Entity	208
10.1.2.1	Real-World Activity: Browse Directory Information	208
10.1.2.2	Real-World Activity: Import into local Storage	208
10.1.2.3	Real-World Activity: Export to local Archive Media	212
11	Augmented and Private Profiles	213
11.1	Augmented Application Profiles	213
11.1.1	AUG-GEN-CD	213
11.1.2	AUG-CTMR-xxxx	213
11.1.3	AUG-XA1K-CD	213
11.2	syngo® private offline Media Application Profile	214
11.2.1	Class and Profile Identification	214
11.2.2	Clinical Context	215
11.2.2.1	Roles and Service Class Options	215

11.2.3PRI-SYNGO Profiles	217
11.2.3.1 SOP Classes and Transfer Syntaxes	217
11.2.3.2 Physical Media and Formats	232
11.2.3.3 Directory Information in DICOMDIR	233
11.2.3.4 Other Parameters	235
12 Extensions, Specializations and Privatizations of SOP Classes and Transfer Syntaxes	236
12.1 SOP-Specific Conformance Statement for Basic Directory	236
12.1.1 Extension, Specialization for SIEMENS Non-Image Objects	236
13 Configuration	237
13.1 AE Title Mapping	237
13.1.1 DICOM Media Storage AE Title	237
14 Support of Extended Character Sets	238
A Annex	242
A.1 Siemens Private Non-Image IOD	242
A.2 Siemens Standard Extended Modules	242
A.3 Siemens Standard Extended Modules	242
A.4 Standard Extensions of all SOP Classes	242
A.5 DICOM Print SCU - detailed status displays	242
Index	243

List of Figures

Fig. 1: Application Data Flow Diagram Verification SCU	17
Fig. 2: Application Data Flow Diagram C-STORE SCU	18
Fig. 3: Application Data Flow Diagram C-STORE SCP	18
Fig. 4: Application Data Flow Diagram Storage Commitment SCU/SCP	19
Fig. 5: Application Data Flow Diagram QUERY/RETRIEVE SCU	21
Fig. 6: Application Data Flow Diagram QUERY/RETRIEVE SCP	21
Fig. 7: Application Data Flow Diagram PRINT SCU	23
Fig. 8: Application Data Flow Diagram BASIC WORKLIST SCU	24
Fig. 9: Application Data Flow Diagram MODALITY PERFORMED PROCEDURE STEP SCU	26
Fig. 10: Interconnection of CT Radiation Dose Templates	164
Fig. 11: DICOM Information Model	186
Fig. 12: TLS Handshake Message Protocol	203

List of Tables

Table 1:	Siemens SOMATOM DICOM products	13
Table 2:	Initiation presentation context Verification	29
Table 3:	Standard SOP Classes as a Storage SCU and an SCP	30
Table 4:	Private SOP Classes as a Storage SCU and an SCP	31
Table 5:	Initiation presentation context Storage	34
Table 6:	Acceptable presentation contexts Storage	47
Table 7:	Standard SOP Classes as Storage Commitment Push Model	69
Table 8:	Initiation presentation context Storage Commitment Request	71
Table 9:	Presentation context accepted for Storage Commitment	72
Table 10:	SOP Classes as a Query/Retrieve SCU	74
Table 11:	SOP Classes as a Query/Retrieve SCP	75
Table 12:	Proposed Presentation Contexts - Find SCU:	77
Table 13:	Query attributes	78
Table 14:	C-FIND response status	82
Table 15:	Proposed Presentation Contexts - Move SCU	83
Table 16:	C-MOVE response status	84
Table 17:	Accepted Presentation Contexts - Find SCP	85
Table 18:	Patient level attributes, Patient Root Information Model, Patient level attributes	87
Table 19:	Study level attributes, Patient Root Information Model	88
Table 20:	Series level attributes, Patient Root Information Model	88
Table 21:	Image level attributes, Patient Root Information Model	89
Table 22:	Study level attributes, Study Root Information Model	91
Table 23:	Series level attributes, Study Root Information Model	92
Table 24:	Image level attributes, Study Root Information Model	93
Table 25:	Patient instance level, Patient Study Only Information Model	95
Table 26:	Study level attributes, Patient Study Only Information Model	95
Table 27:	C-FIND return status	97
Table 28:	Proposed Presentation Contexts -- Get SCP	98
Table 29:	C-GET return status	99
Table 30:	Proposed Presentation Contexts - Move SCP	100
Table 31:	C-MOVE return status	101
Table 32:	Basic Grayscale Print Management Meta SOP-Classes	102
Table 33:	Basic Color Print Management Meta SOP-Classes	102
Table 34:	Presentation contexts - Print SCU	104
Table 35:	Used Basic Film Session N-CREATE_RQ attributes	105
Table 36:	Attributes of the N-DELETE-RQ on the Basic Film Session SOP Class	105
Table 37:	Basic Film Session SOP status	106
Table 38:	Used Film Box N-CREATE_RQ attributes	106
Table 39:	Attributes of the N_DELETE_RQ on the Basic Film Session SOP Class	108
Table 40:	Basic Film Box SOP status	108
Table 41:	Used Basic Grayscale Image Box N-SET attributes	108
Table 42:	Basic Grayscale Image Box SOP status	109
Table 43:	Used Basic Color Image Box N-SET attributes	109
Table 44:	Basic Color Image Box SOP status	110
Table 45:	Attributes of the N_CREATE_RQ on the Presentation LUT SOP Class	110
Table 46:	Attributes of the N_DELETE_RQ on the Presentation LUT SOP Class	110
Table 47:	Presentation LUT SOP status	111
Table 48:	Used Printer N-EVENT report	111

Table 49:	Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes	111
Table 50:	Used Print Job N-EVENT report	112
Table 51:	Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class	113
Table 52:	Printer Status Infos: Additional Agfa printer status infos	119
Table 53:	Printer Status Infos: Additional Kodak infos for Pacs Link (formerly Imation cameras) ..	119
Table 54:	Printer Status Infos: Additional Kodak infos for Kodak 190	119
Table 55:	Printer Status Infos: Additional Kodak infos for 2180/1120	120
Table 56:	Printer Status Infos: Additional Codonics infos	120
Table 57:	Additional DICOM Execution Status Information - evaluation	122
Table 58:	SOP Classes as an SCU	123
Table 59:	Proposed presentation contexts	124
Table 60:	Search Key Attributes in a broad worklist query	125
Table 61:	Basic Worklist C_FIND_RSP Return Key Attributes	127
Table 62:	Search Key Attributes in a patient-based worklist query	133
Table 63:	C-FIND Response Status	134
Table 64:	SOP Classes as an SCU	135
Table 65:	Proposed presentation contexts	136
Table 66:	Performed Procedure Step N-CREATE Attributes	137
Table 67:	N-SET Response Status	140
Table 68:	Performed Procedure Step N-SET Attributes	141
Table 69:	N-SET Response Status	144
Table 70:	Standard Extensions of all SOP Classes	145
Table 71:	Somaris/7 Image Type (0008,0008) for objects created by Somaris/7	152
Table 72:	Somaris/7 Image Type (0008,0008) for objects created by Somaris/7	157
Table 73:	Somaris/7 Image Type (0008,0008) for objects created by Somaris/7	158
Table 74:	Somaris/7 Image Type (0008,0008) for objects created by Somaris/7	164
Table 75:	Somaris/7 Attribute Interpretation	165
Table 76:	CSA Image IOD Modules	175
Table 77:	CSA Image Header Module	175
Table 78:	CSA Series Header Module	176
Table 79:	MEDCOM Header Module	176
Table 80:	MEDCOM History Information	180
Table 81:	MEDCOM OOG Module	180
Table 82:	syngo Report Data	181
Table 83:	3CSA Non-Image IOD Modules	186
Table 84:	CSA Non-Image Module	187
Table 85:	(Non-)Image Type (0008,0008) for private Somaris/7 Non-image Objects	190
Table 86:	SOP Classes	190
Table 87:	Default AET Characteristics	192
Table 88:	Single-Byte Character Sets without Code Extension	197
Table 89:	Single-Byte Character Sets with Code Extension	198
Table 90:	Multi-Byte Character Sets without Code Extension	199
Table 91:	Multi-Byte Character Sets with Code Extension	199
Table 92:	Application profiles, Activities, and Roles for the DICOM Archive application	207
Table 93:	SOP Classes and Transfer Syntax	217
Table 94:	DICOMDIR keys	233
Table 95:	DICOMDIR keys for CsaNonImage	235
Table 96:	Single-Byte Character Sets without Code Extension	238
Table 97:	Single-Byte Character Sets with Code Extension	239

Table 98: Multi-Byte Character Sets without Code Extension240

Table 99: Multi-Byte Character Sets with Code Extension240

1 Introduction

1.1 Overview

This DICOM Conformance Statement is written according to part PS 3.2 of [1].

The applications described in this conformance statement are implemented in the Siemens SOMATOM products using the Somaris/7 *syngo* CT VB10 software (internal designation: VB10A).

The Somaris/7 DICOM network implementation acts both as an SCU and an SCP for the DICOM Verification, Storage, Storage Commitment Push Model, and Query/Retrieve Services. It acts as an SCU for the DICOM Print Management Service, the Modality Worklist Service, and the Performed Procedure Step Service.

These services are described in "Part I".

The DICOM Media Storage Service implementation acts as the FSC, FSU, and FSR for the specified application profiles and the related SOP Class instances. These services are described in "Part II".

Somaris/7 is based on a Siemens common medical platform. This platform is shared with other Siemens modalities in order to provide a common look and feel, as well as common interoperability features.

In this document, the different parts of the Siemens common medical platform are referred to by the terms "*syngo*"¹, "MedCom", and "CSA".

As Somaris/7 is a *syngo*-based product, this DICOM Conformance Statement is based on the corresponding *syngo* template [2].

1.2 Audience

This document is intended to be used by hospital staff, health system integrators, hospital IT managers, and software designers or implementors. It is assumed that the reader has a working understanding of DICOM.

¹ '*syngo*' is a registered trademark of Siemens Healthcare GmbH

1.3 Scope

This DICOM Conformance Statement refers to Siemens SOMATOM products using the Somaris/7 software. The following table relates software names to Siemens products.

Table 1: Siemens SOMATOM DICOM products

Software name	Siemens product
Somaris/7 syngo CT VB10 (internal: VB10A)	SOMATOM Definition Edge
	SOMATOM Definition Flash
	SOMATOM Definition AS
	SOMATOM Drive
	SOMATOM Confidence
	SOMATOM Edge Plus
	SOMATOM Force

1.4 Definitions, Acronyms and Abbreviations

1.4.1 Definitions

DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite information objects

1.4.2 Acronyms and Abbreviations

ACR	American College of Radiology
AE	DICOM Application Entity
AET	Application Entity Title
ASCII	American Standard Code for Information Interchange
CAD	Computer Aided Detection
DX	Digital Radiography
FSC	File Set Creator
FSR	File Set Reader
FSU	File Set Updater
HIS	Hospital Information System
IHE	Integrating the Healthcare Enterprise
IOD	DICOM Information Object Definition
ISO	International Standard Organization
LUT	Lookup Table
M	Mandatory Key Attribute
MPPS	Modality Performed Procedure Step
MWL	Modality Worklist
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
R	Required Key Attribute
RP	Requested Procedure
RIS	Radiology Information System
RWA	Real-World Activity
PDU	DICOM Protocol Data Unit
SCU	DICOM Service Class User (DICOM client)

SCP	DICOM Service Class Provider (DICOM server)
SOP	DICOM Service-Object Pair
SPS	Scheduled Procedure Step
SR	Structured Report
TLS	Transport Layer Security
U	Unique Key Attribute
UID	Unique Identifier
UTF-8	Unicode Transformation Format-8
VOI	Value of Interest
VR	Value Representation

1.5 References

- [1] DICOM® Standards Publication Part(s) 3, 4, ©NEMA
Standard is under continuous maintenance, the current official version is available at: <http://dicom.nema.org>
- [2] *syngo* VI20A DICOM Conformance Statement

1.6 Connectivity and Interoperability

The implementation of the Somaris/7 DICOM interface has been carefully tested to ensure correspondence with this Conformance Statement. However, the Conformance Statement and the DICOM standard do not guarantee interoperability of Siemens modalities and modalities of other vendors. The user must compare the relevant Conformance Statements and, if a successful interconnection is in theory possible, the user is responsible for specifying an appropriate test suite and for validating the interoperability, which is required. A network environment may need additional functions beyond the scope of DICOM.

Part I - Network

2 Implementation Models

2.1 Verification


The Verification service class defines an application-level class of service which allows the operator to verify the ability of an application on a remote node, in order to respond to DICOM messages. The DICOM Service Tool application supports the Verification service in acting as an SCU.

The other direction - responding to Verification requests from remote applications - is handled by the Storage SCP application.

2.1.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as the SCU for the C-ECHO DICOM network service. The product target operating system is Windows 10.

Fig. 1: Application Data Flow Diagram Verification SCU

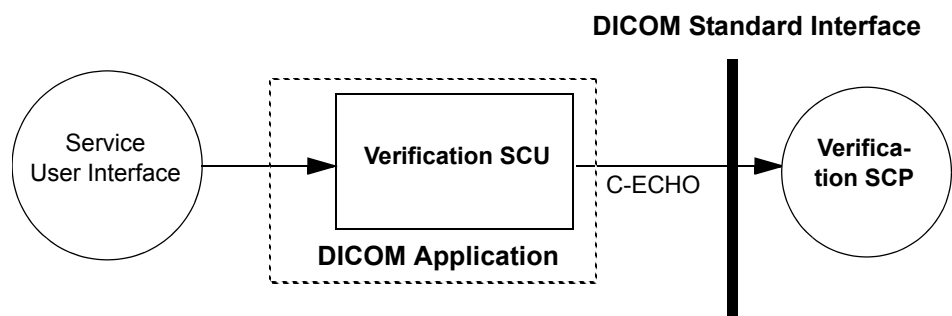

2.1.2 Functional Definitions of Application

The DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

2.1.3 Sequencing of Real-World Activities

Newly configured data of a remote AE has to be first saved before a "verification" of this data is possible.

2.2 Storage

The Somaris/7 DICOM Application Entity both originates associations for the Storage of DICOM Composite Information Objects in Remote Application Entities and accepts association requests for Storage from Remote Application Entities.

2.2.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as both an SCU and an SCP for the C-STORE DICOM network service, and as the SCP for the C-ECHO DICOM network service. The product target operating system is Windows 10.

Fig. 2: Application Data Flow Diagram C-STORE SCU


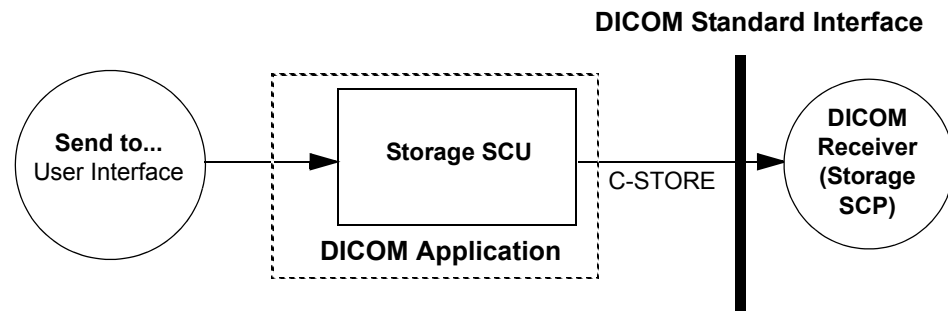


Fig. 3: Application Data Flow Diagram C-STORE SCP

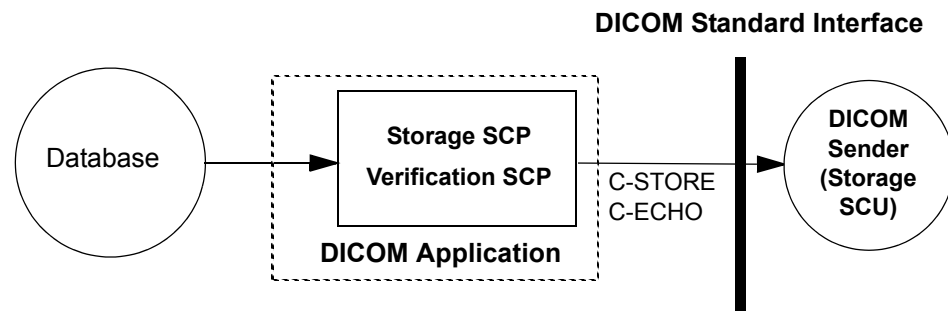

2.2.2 Functional Definitions of Application Entities

The Storage SCU is invoked by the job control interface that is responsible for processing network archiving tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE service. The status of the transfer is reported to the job control interface.

The Storage SCP component of the Siemens Somaris/7 DICOM application operates as a background server process. It already exists when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context, it starts to receive the Composite Image Objects and imports them into the local database. Verification requests will also be processed and responded to by the Storage SCP component.

2.2.3 Sequencing of Real-World Activities

Not applicable.


2.3 Storage Commitment

The Storage Commitment service class defines an application-level class of service which facilitates the commitment to storage. It performs an additional task for the commitment of composite objects apart from the network-based storage of images as defined by the Storage Service class. The Somaris/7 DICOM implementation supports the Storage Commitment Push Model both as an SCU and as an SCP.

2.3.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as the SCU for the Storage Commitment Push Model Service using the Storage Commitment Service Class. The product target operating system is Windows 10.

Fig. 4: Application Data Flow Diagram Storage Commitment SCU/SCP

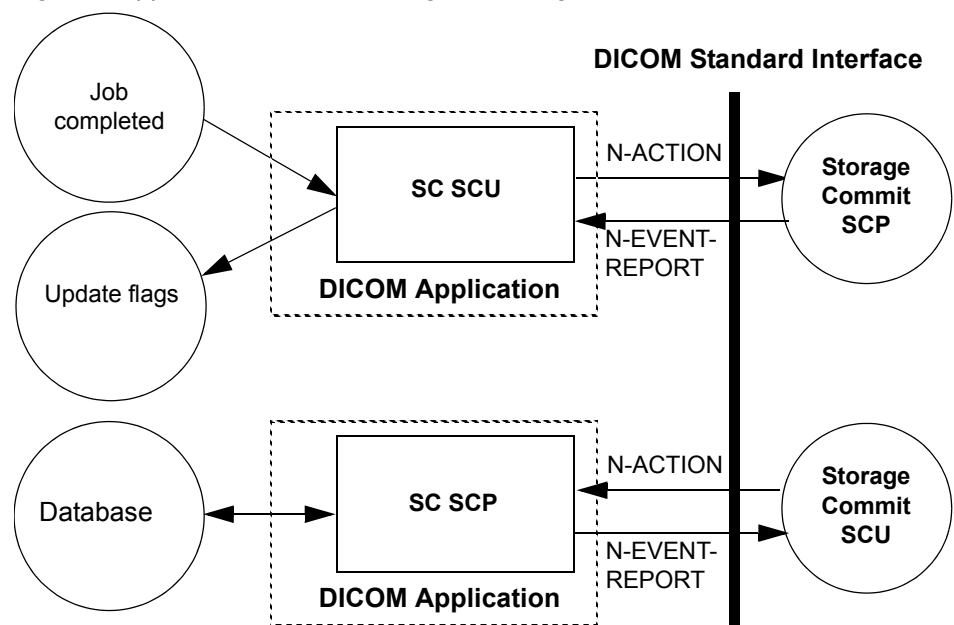

2.3.2 Functional Definitions of Application Entities

With each successfully completed send job, the Somaris/7 DICOM application creates a Storage Commitment Push Model Identifier from the SOP Instances sent. Then, a Storage Commit Request is triggered. Depending on the configuration, the Somaris/7 DICOM application keeps the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response is indicated by the Status Flags of the related entry. It is possible to create triggers ("auto rules") from this event.

The Transaction UUIDs of the pending commitment request are kept "open" for a configurable amount of time (default: 1h). If the "open time" for a pending commitment request has elapsed without a related response from the provider, the Transaction UUID is removed and the related entities are indicated as "commit failed".

In any case, a commitment will only be requested for previously and successfully sent images.

2.3.3 Sequencing of real-world activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

2.4 Query/Retrieve

The Query/Retrieve service class defines an application-level class of services which facilitates the management of images and patient data against the well-defined DICOM information model. It allows a DICOM AE to retrieve images from a remote DICOM node or to request a remote DICOM AE to initiate a transfer of images to another DICOM AE. The DICOM Query/Retrieve application supports the Query/Retrieve services to act as both an SCU and an SCP.

2.4.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as both the SCU and an SCP for the Query/Retrieve network service. The product target operating system is Windows 10.

Fig. 5: Application Data Flow Diagram QUERY/RETRIEVE SCU


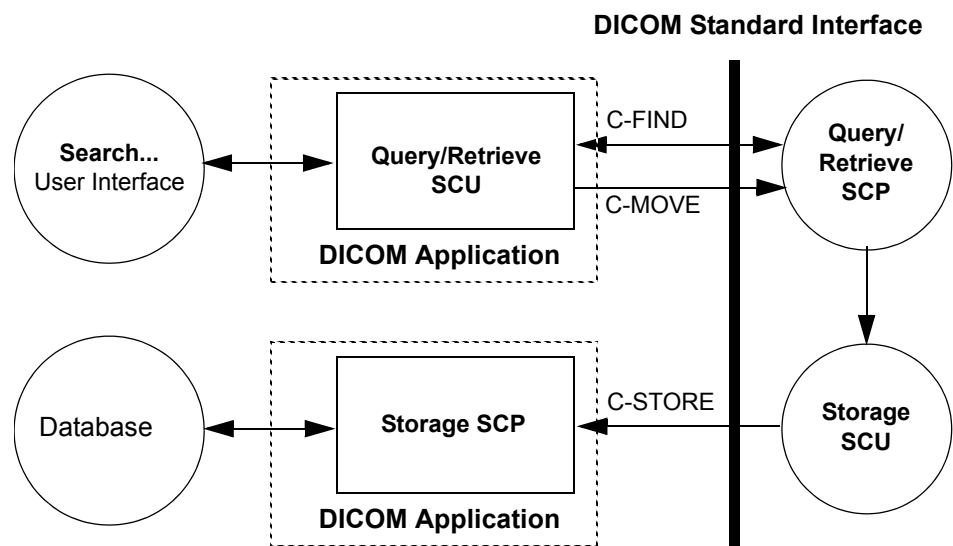


Fig. 6: Application Data Flow Diagram QUERY/RETRIEVE SCP

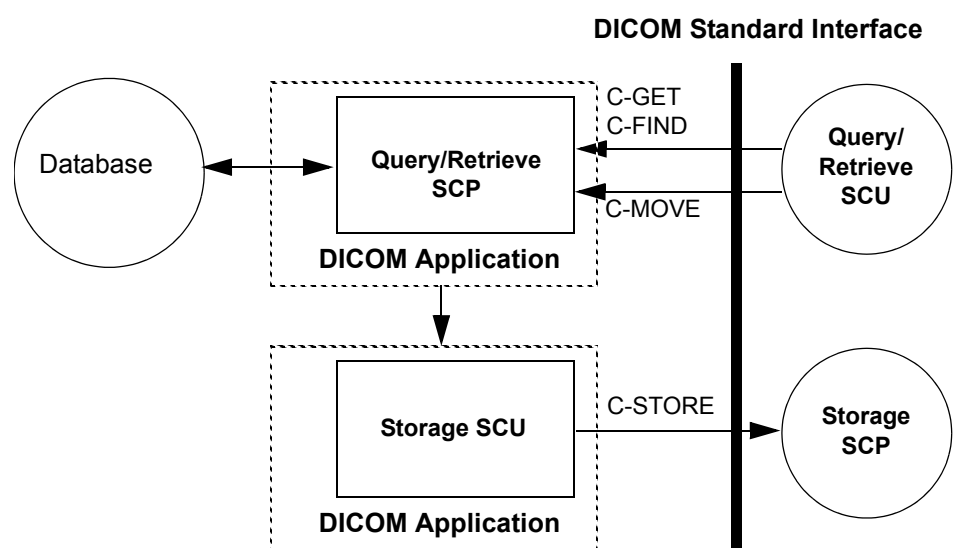

2.4.2 Functional Definitions of Application Entities

The Query/Retrieve SCU requests the remote Query/Retrieve SCP to perform a search and match to the keys specified in the request, in order to display the results in the user interface. Depending on the user action (Import), the Somaris/7 DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP and to start an image transfer from the remote Storage SCU to the Somaris/7 DICOM Storage SCP.

The Query/Retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote requests, a C-GET or a C-MOVE involves the Somaris/7 DICOM Query/Retrieve SCP application initiating a C-STORE association (by triggering and parameterizing its own Storage SCU) to send image objects to a remote Storage SCP.

All components of the Somaris/7 DICOM Query/Retrieve SCP application operate as background server processes. They already exist when the machine is powered on and respond to queries based on the records stored in its database.

Note

The Somaris/7 DICOM Query/Retrieve SCU application executes new queries based on the data found in the higher-level query. For details, see 3.4.2.1.3 *SOP-Specific Conformance Statement - Find SCU* on page 78.

2.4.3 Sequencing of Real-World Activities

The retrieval of images is only possible if results from a previous "Search..." operation exist and these entities can be selected for "Import".


2.5 Print

The Print Management Service Classes define an application-level class of services which facilitates the printing of images on a hardcopy medium. The print management SCU and print management SCP are peer DICOM print management application entities. The DICOM print application supports the print management DIMSE services to act as an SCU.

2.5.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as the SCU for the print management network service. The product target operating system is Windows 10.

Fig. 7: Application Data Flow Diagram PRINT SCU

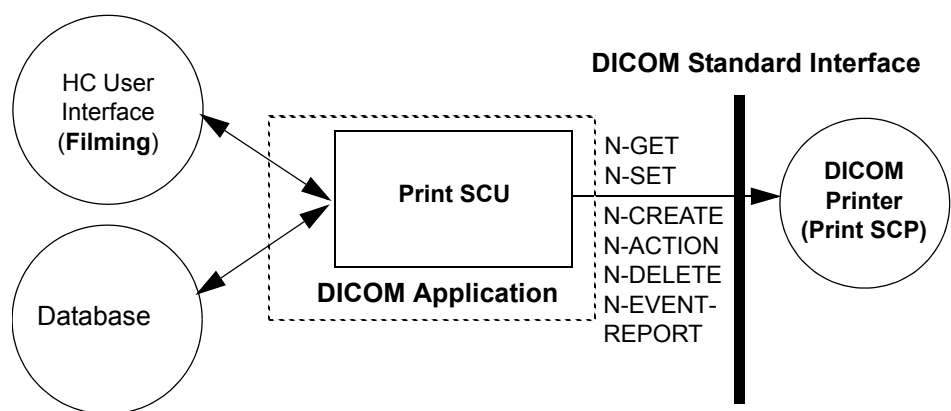

2.5.2 Functional Definitions of Application Entities

The Print SCU is invoked by the user interface to set up a film sheet layout and whenever an image is ready to be printed on film. The print SCU holds and maintains all the data needed to compile a complete film sheet from the data (images, layout, configuration) received. Whenever a film sheet is ready to print, the related data is used to supply the information to the SOP Classes of the Print Management Service Class. A queue is maintained in order to intermediately store several film sheets in case of resource problems on the printer. The SCU only supplies and requires the mandatory SOP Classes of the Print Management Service Class.

2.5.3 Sequencing of Real-World Activities

Not applicable.


2.6 Model Worklist

The Basic Worklist Service Class defines an application-level class of service, which facilitates the transfer of worklists from the information system to the imaging modality. The worklist is queried by the AE and supplies the SCU with the scheduled tasks that have to be performed on the modality. The DICOM worklist application supports the worklist service as an SCU.

2.6.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as the SCU for the Basic Worklist Service using the Modality Worklist SOP Class. The product target Operating System is Windows 10.

Fig. 8: Application Data Flow Diagram BASIC WORKLIST SCU

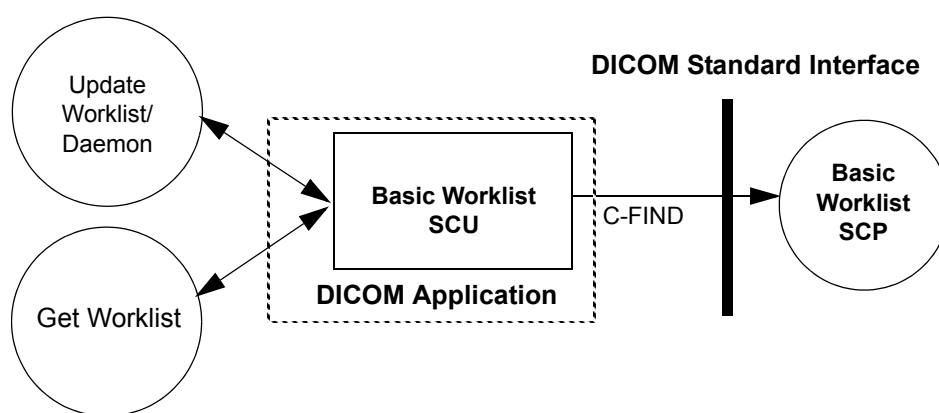

Note: Worklist updates can be configured to be received either automatically (in a configurable time interval) or manually (initiated by the user). Users can either initiate a broad worklist query (all jobs for their own modality or application entity) or a patient-based worklist query (where more search keys can be given, including Patient Name and Patient ID).

2.6.2 Functional Definitions of Application Entities

The worklist SCU ("broad query") is invoked from the patient browser user interface or by timer to request the worklist from a remote Information System (Modality Worklist SCP). This is done to match against the internal worklist query keys specified in the C-FIND DIMSE service issued for the Modality Worklist Model.

The Worklist SCP responds to the C-FIND query and scheduled imaging service requests (scheduled procedure steps). Patient demographic information is downloaded from the information system to the Somaris/7 modality. All information retrieved is held in the scheduling database for use during the patient registration procedure.

Furthermore, the patient-based query dialog from the patient browser allows you to enter specific matching criteria ("narrow query") for the issue worklist query. The Patient Registration dialog can be populated with the response data according to availability in the worklist response identifier.

2.6.3 Sequencing of Real-World Activities

The "narrow" (patient-based) Worklist Query requires that sufficient matching keys or a unique matching key are/is entered before the query is issued. Only then can a single response be expected to complete the registration dialog.


2.7 Modality Performed Procedure Step

The Modality Performed Procedure Step (MPPS) service class defines an application-level class of service which facilitates the transfer of billing and radiation dose information from the imaging modality to the information system. The performed procedure step is created and set by the AE and supplies the SCP with the information about a real-world procedure that is performed on the modality. The DICOM Modality Performed Procedure Step application supports the MPPS service as an SCU.

2.7.1 Application Data Flow Diagram

The Somaris/7 DICOM network implementation acts as the SCU for the performed procedure step network service. The target operating system is Windows 10.

Fig. 9: Application Data Flow Diagram MODALITY PERFORMED PROCEDURE STEP SCU

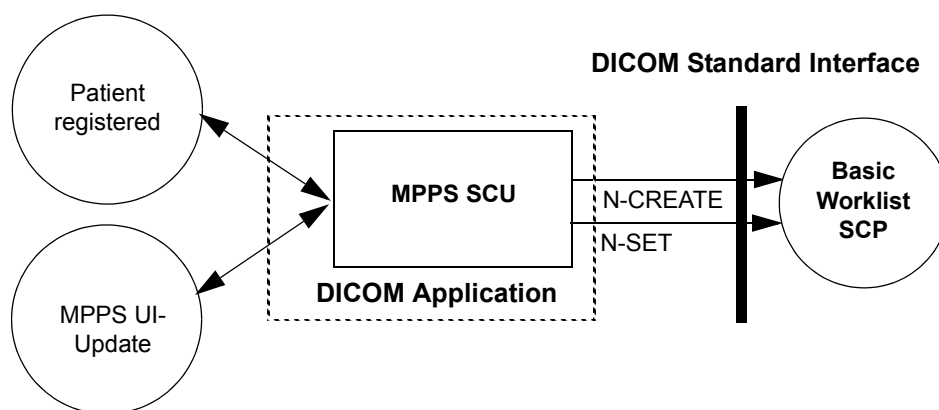

2.7.2 Functional Definitions of Application Entities

When a patient is registered (for example, via a Scheduled Procedure Step from the Worklist), the Somaris/7 DICOM application creates an MPPS instance and communicates it to the MPPS SCP.

Furthermore, a manual update can be performed using the Somaris/7 MPPS user interface. It is only possible to set the state of the MPPS to "Completed" or "Discontinued" there. If this is done, the DICOM application will no longer allow updates on the related MPPS instance.

Multiple requested procedures scheduled for a CT examination will result in multiple studies and MPPS, where each RP is related to one study.

Somaris/7 supports the creation of "unscheduled cases" by allowing MPPS instances to be communicated for locally registered patients.

2.7.3 Sequencing of real World Activities

Not applicable.

3AE Specifications

3.1 Verification AE Specification

3.1.1 Association Establishment Policies

3.1.1.1 General

The Somaris/7 DICOM Service Tool application attempts to open an association for verification request whenever the "verification" function is activated during the network configuration of a remote DICOM application.

3.1.1.2 Number of Associations

The Somaris/7 DICOM Service Tool application initiates one association at a time to request verification.

3.1.1.3 Asynchronous Nature

The Somaris/7 DICOM Service Tool application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.1.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.1.2 Association Initiation by Real-World Activity

The Somaris/7 DICOM Service Tool application attempts to initiate a new association for

- DIMSE C-ECHO

service operations.

3.1.2.1 Associated Real-World Activity - Verification

3.1.2.1.1 Associated Real-World Activity - Verification SCU

The associated Real-World activity is a C-ECHO request initiated by the Service and Configuration SW environment whenever a "verification" is requested. If an association with a remote Application Entity is successfully established, Verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application contains a status other than "Success", this will be indicated in the service environment and the association is closed.

3.1.2.1.2 Proposed Presentation Contexts - Verification SCU

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 2: Initiation presentation context Verification

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1

3.1.2.1.3 SOP-Specific Conformance Statement - Verification SCU

The Application conforms to the definition of a Verification SCU in accordance with the DICOM Standard.

3.1.3 Association Acceptance Policy

The Verification SCP is part of the Storage SCP - see 3.2.3 *Association Acceptance Policy* on page 46.

3.2 Storage AE Specification

The Somaris/7 Storage service class user applications and service class provider applications use one AE when initiating/receiving associations to/from remote DICOM nodes.

The SIEMENS Somaris/7 DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Classes as both an SCU and an SCP:

Table 3: Standard SOP Classes as a Storage SCU and an SCP

SOP Class Name	SOP Class UID
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1
Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2
Enhanced Computed Tomography Image Storage	1.2.840.10008.5.1.4.1.1.2.1
Digital X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.1
Digital X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1
Digital MammoGraphy Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.2
Digital MammoGraphy Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1
Digital Intra-oral X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.1.3
Digital Intra-oral X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1
Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4
Enhanced Magnetic Resonance Image Storage	1.2.840.10008.5.1.4.1.1.4.1
Magnetic Resonance Spectroscopy Image Storage	1.2.840.10008.5.1.4.1.1.4.2
Enhanced Magnetic Resonance Colored Storage	1.2.840.10008.5.1.4.1.1.4.3
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20
PET Image Storage	1.2.840.10008.5.1.4.1.1.128
Radio Therapy Image Storage	1.2.840.10008.5.1.4.1.1.481.1
Radio Therapy Dose Storage	1.2.840.10008.5.1.4.1.1.481.2
Radio Therapy Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3
Radio Therapy Plan Storage	1.2.840.10008.5.1.4.1.1.481.5
Radio Therapy Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8
Radio Therapy Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9
Radio Therapy Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6
Radio Therapy Ion Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1
Multi-frame Grayscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2

Table 3: Standard SOP Classes as a Storage SCU and an SCP

SOP Class Name	SOP Class UID
Multi-frame Grayscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3
Multi-frame True Color Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4
UltraSound Image Storage	1.2.840.10008.5.1.4.1.1.6.1
UltraSound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
X-Ray RadioFluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1
Spatial Fiducial Storage	1.2.840.10008.5.1.4.1.1.66.2
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1
Verification (only SCP)	1.2.840.10008.1.1

The SIEMENS Somaris/7 DICOM implementation provides Private Conformance to the following DICOM V3.0-conform Private SOP Classes as both an SCU and an SCP:

Table 4: Private SOP Classes as a Storage SCU and an SCP

SOP Class Name	SOP Class UID
CSA Non-Image Storage	1.3.12.2.1107.5.9.1

3.2.1 Association Establishment Policies

3.2.1.1 General

The existence of a job queue with a network destination, or an internal trigger after processing a retrieve request, activates the DICOM Storage Application. An association request is sent to the destination AE and, upon successful negotiation of a Presentation Context, the transfer starts.

The default PDU size is of 32 kB.

3.2.1.2 Number of Associations

The Somaris/7 DICOM application initiates several associations at the same time, one for each destination to which a transfer request is being processed in the active job queue list.

The Somaris/7 DICOM application is able to accept multiple associations at the same time. It can handle up to 10 associations in parallel.

The number of Simultaneous DICOM associations can be configured via the Service UI. The dialog can be found via Configuration / DICOM / General.

3.2.1.3 Asynchronous Nature

The Somaris/7 DICOM application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.2.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.2.2 Association Initiation Policy

If a job with a network destination becomes active in the job list, or a retrieve sub-operation is processed, the Somaris/7 DICOM application attempts to initiate a new association for

- DIMSE C-STORE

service operations.

3.2.2.1 Associated Real-World Activity - Send (Storage SCU)

3.2.2.1.1 Associated Real-World Activity - Send Image Objects to a Network Destination

The associated Real-World activity is a C-STORE request initiated by an internal daemon process. This is triggered by a job with a network destination or by the processing of an external C-MOVE retrieve request. If the process successfully establishes an association to a remote Application Entity, it transfers each image one after another via the open association. If the C-STORE Response from the remote Application contains a status other than "Success" or "Warning", the association is aborted.

3.2.2.1.2 Proposed Presentation Contexts - Send Images (Storage SCU)

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Enhanced Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Digital X-Ray Image for pre- sentation	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Digital X-Ray Image for pro- cessing	1.2.840.10008.5.1.4.1.1.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
MammoGra- phy Image for presentation	1.2.840.10008.5.1.4.1.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
MammoGra- phy Image for processing	1.2.840.10008.5.1.4.1.1.1.2.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Digital Intra- oral X-Ray Image for pre- sentation	1.2.840.10008.5.1.4.1.1.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Digital Intra- oral X-Ray Image for pro- cessing	1.2.840.10008.5.1.4.1.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Enhanced Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Magnetic Resonance Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.1
		Implicit VR Little Endian	1.2.840.10008.1.2.2
Enhanced Magnetic Resonance Colored Storage	1.2.840.10008.5.1.4.1.1.4.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.1
		Implicit VR Little Endian	1.2.840.10008.1.2.2

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Breast Tomo- synthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Nuclear Medi- cine Image	1.2.840.10008.5.1.4.1.1.20	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
PET Image	1.2.840.10008.5.1.4.1.1.128	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Multi-frame Grayscale Byte Second- ary Capture Image	1.2.840.10008.5.1.4.1.1.7.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Multi-frame Grayscale Word Second- ary Capture Image	1.2.840.10008.5.1.4.1.1.7.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
UltraSound Multi-Frame Image	1.2.840.10008.5.1.4.1.1.3.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
UltraSound Image	1.2.840.10008.5.1.4.1.1.6.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
X-Ray Angio-graphic Image	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
X-Ray RadioFluoro- scopic Image	1.2.840.10008.5.1.4.1.1.12.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Waveform	1.2.840.10008.5.1.4.1.1.9.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform 12-lead ECG Object	1.2.840.10008.5.1.4.1.1.9.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform General ECG Object	1.2.840.10008.5.1.4.1.1.9.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Ambulatory ECG Object	1.2.840.10008.5.1.4.1.1.9.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Hemody- namic Object	1.2.840.10008.5.1.4.1.1.9.2.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Cardiac Elec- trophysiology Object	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Basic Audio Object	1.2.840.10008.5.1.4.1.1.9.4.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Raw Data Storage Object	1.2.840.10008.5.1.4.1.1.66	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Spatial Registration Object	1.2.840.10008.5.1.4.1.1.66.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Spatial Fiducials Object	1.2.840.10008.5.1.4.1.1.66.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1) ^a	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4) ^a	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Table 5: Initiation presentation context Storage

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Mammo- graphy CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Key Object Selection Doc- ument	1.2.840.10008.5.1.4.1.1.88.59	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
X-Ray Radia- tion Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
CSA Non-Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

^a. The Transfer Syntax used is strongly influenced by the accepted Transfer Syntax at the time when the instance was received. For example, instances received with JPEG Lossy Transfer Syntaxes are not converted and can only be sent out with the same Transfer Syntax.

Note

1. The proposed Transfer Syntax is highly restricted for images stored internally in a lossy compression format. For example, instances received with JPEG Lossy Transfer Syntaxes are not converted and can only be sent out with the same Transfer Syntax.

2. The compression is only supported for images with pixel representation (0028, 0103) equal to 0 (=unsigned).

The "MOVE" destinations must be configured as Storage destinations. This includes the configuration of Transfer Syntax capabilities.

Not all the listed transfer syntaxes are proposed every time. For some abstract syntaxes, only a list of uncompressed (UC) transfer syntaxes (one or more) is proposed, while for other abstract syntaxes, the JPEG Loss-Less (LL) syntax and/or a list of JPEG Lossy (LY) transfer syntaxes are also proposed. The contents of this lists are configurable, for example, UC could be configured to contain only Implicit Little Endian. For further configuration details, see 6.2.1 *Storage, Storage Commitment and Query/Retrieve* on page 194.

It is not possible to send an image that is locally stored in a lossy compressed format using an uncompressed or lossless transfer syntax.

Depending on the real-world activity initiating the C-STORE, the following behavior is observed:

- If the C-STORE is initiated by a user, a configuration parameter called QualityFactor(Q) is used to decide which transfer syntax lists will be proposed. Q can take values between 0 and 100. If Q = 0, only UC is proposed. If Q = 100, UC and LL are proposed. Otherwise, UC and LY are proposed.
- If the C-STORE is initiated by the C-MOVE SCP, another configuration parameter called Compression Types Supported (CTS) is used to decide which transfer syntaxes are proposed. CTS can take integer values. If CTS = 0 or CTS > 3, UC is proposed. If CTS = 1, UC and LY are proposed. If CTS = 2, UC and LL are proposed. If CTS >= 3, UC, LL and LY are proposed.

The JPEG lossy and JPEG lossless compression types are parameters that are part of the Application Entity Properties configuration (storage checked). The configuration can be reached via the Service UI: Configuration / DICOM / Network nodes.

3.2.2.1.3 SOP-Specific Conformance Statement - Storage SCU

The DICOM images created by the Somaris/7 DICOM application conform to the DICOM IOD definitions (Standard Extended IODs). However, they also contain additional private elements that have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed after modification.

Somaris/7 does not change private attributes if no modification is done. However, during a *Save as* operation, all non-*syngo* defined private attributes are removed. For association and DIMSE level time-outs, refer to 6.2 *Configurable Parameters* on page 193.

3.2.3 Association Acceptance Policy

The Somaris/7 DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

service operations. Any Information Object transmitted on this association is checked for conformance and stored in the database if the check is successful.

3.2.3.1 Real-World Activity - Receive (Storage SCP)

3.2.3.1.1 Associated Real-World Activity - Receiving Images from a Remote Node (Storage SCP)

The daemon receiving process accepts an association and receives any images transmitted on this association. It stores the images on disk in its own database if the conformance check is successful.

3.2.3.1.2 Proposed Presentation Contexts - Receiving Images (Storage SCP)

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Computed Radiography Image	1.2.840.10008.5.1.4.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Enhanced Computed Tomography Image	1.2.840.10008.5.1.4.1.1.2.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Digital X-Ray Image for pre- sentation	1.2.840.10008.5.1.4.1.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Digital X-Ray Image for pro- cessing	1.2.840.10008.5.1.4.1.1.1.1.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Digital MammoGraphy X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Digital MammoGraphy X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.2.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Digital Intra-oral X-Ray Image for presentation	1.2.840.10008.5.1.4.1.1.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Digital Intra-oral X-Ray Image for processing	1.2.840.10008.5.1.4.1.1.1.3.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Enhanced Magnetic Resonance Image	1.2.840.10008.5.1.4.1.1.4.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
Magnetic Resonance Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
		Explicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.1
		Implicit VR Little Endian	1.2.840.10008.1.2.2

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Enhanced Magnetic Resonance Colored Storage	1.2.840.10008.5.1.4.1.1.4.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
Grayscale Soft-copy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.1
		Implicit VR Little Endian	1.2.840.10008.1.2.2
X-Ray 3D Angiographic Image	1.2.840.10008.5.1.4.1.1.13.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Breast Tomo-synthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Nuclear Medicine Image	1.2.840.10008.5.1.4.1.1.20	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
PET Image	1.2.840.10008.5.1.4.1.1.128	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Big Endian	1.2.840.10008.1.2.2
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
Multi-frame Single Bit Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.1	RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Multi-frame Grayscale Byte Secondary Cap- ture Image	1.2.840.10008.5.1.4.1.1.7.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
		Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Multi-frame True Color Secondary Capture Image	1.2.840.10008.5.1.4.1.1.7.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
UltraSound Multi-Frame Image	1.2.840.10008.5.1.4.1.1.3.1 1.2.840.10008.5.1.4.1.1.3 (retired) *1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
UltraSound Image	1.2.840.10008.5.1.4.1.1.6.1 1.2.840.10008.5.1.4.1.1.6 (retired) *1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
X-Ray Angio-graphic Image	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
X-Ray RadioF-luoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
Waveform	1.2.840.10008.5.1.4.1.1.9.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform General ECG Object	1.2.840.10008.5.1.4.1.1.9.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Ambulatory ECG Object	1.2.840.10008.5.1.4.1.1.9.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Hemodynamic Object	1.2.840.10008.5.1.4.1.1.9.2.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Cardiac Electrophysiology Object	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Waveform Basic Audio Object	1.2.840.10008.5.1.4.1.1.9.4.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Raw Data Storage Object	1.2.840.10008.5.1.4.1.1.66	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Spatial Registration Object	1.2.840.10008.5.1.4.1.1.66.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Spatial Fiducials Object	1.2.840.10008.5.1.4.1.1.66.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50
		JPEG Lossy Extended (2 & 4)	1.2.840.10008.1.2.4.51
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70
		JPEG Lossless, Process 14 Non-HIER	1.2.840.10008.1.2.4.57
		JPEG 2000 Lossless	1.2.840.10008.1.2.4.90
		JPEG 2000 Lossy	1.2.840.10008.1.2.4.91
		RLE Lossless	1.2.840.10008.1.2.5
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Table 6: Acceptable presentation contexts Storage

Presentation Context Table		Role	Extended Negotiation
		SCP	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Encapsulated PDF	1.2.840.10008.5.1.4.1.1.104.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
CSA Non-Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

*1: US Retired and US Multi-Frame Retired images are converted to US images/ US Multi-Frame images before being stored in the local database. The conversion creates new images, which implies new UUIDs.

Note

With the RLE Lossless Transfer Syntax and the JPEG Lossless, Process14, Non_HIER Transfer Syntax the DICOM application decompresses the image before storing it in the database.

Note

JPEG 2000 decompression is supported only for import in connection with the COSMOS / *syngo* Imaging workplace.

Note

Private attributes in sequence items are removed during import to *syngo*.

Note

After receiving images of types Multi-frame Single-Bit Secondary Capture Image, Multi-frame Grayscale Byte Secondary Capture Image, Multi-frame Grayscale Word Secondary Capture Image and Multi-frame True Color Secondary Capture Image, the SOP class UID of the received image is changed to that of a Secondary Capture Image (1.2.840.10008.5.1.4.1.1.7) and stored.

3.2.3.1.3 SOP-Specific Conformance Statement - Receiving Images

The Somaris/7 DICOM application conforms to the Full Storage Service Class at Level 2.

When a C-STORE-RQ is successfully received, the SIEMENS Somaris/7 DICOM receiver performs a quick plausibility test on the received image and available system resources. If this test succeeds, it returns the status SUCCESS, otherwise one of the following status codes is returned and the association is aborted:

- Refused (A700):
This error status indicates a lack of Resources (for example, not enough disk space) on the Somaris/7 modality.
- Invalid Dataset (A900):
The data set does not contain one of the attributes "Study Instance UID", "Series UID" or "SOP Instance UID", or one of these has an invalid value.
- Processing Error (0110):
An error occurred while processing the image, making it impossible to proceed.

Attention! The image is saved in the database only after the response is sent. If an error occurs during this operation, the association is aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored in the database.

In order to confirm that the images sent were successfully stored in the database, the sending application should use the Storage Commitment Service.

If an image instance is received having an SOP Instance UID that is already used by an Instance stored in the database, then the received image is discarded. The existing image is not superseded by the received image. Therefore, if a remote node sends the same image twice (as identified by the SOP Instance UID), only one image (the first) is kept in the database of the DICOM receiver.

The following sections differentiate between the attribute contents required for image viewing. The Somaris/7 DICOM application supports more formats for the storage of images than it does for viewing.

3.2.3.1.3.1 Image Pixel Attribute Acceptance Criterion for Grayscale Images - Viewing

The Siemens Somaris/7 Multi-Modality application accepts the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay - with unsigned integers and 8 or 16 bits allocated. The following values are accepted:

Pixel plane

- Samples per pixel (attribute 0028, 0002) = 1
- Photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- Photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- Pixel representation (attribute 0028, 0103) = 0 (unsigned)
- Bits allocated (attribute 0028, 0100) = 8, 16
- Bits stored (attribute 0028,0101) = 8, 10, 12, 14,15, 16
- High bit (attribute 0028,0102) = 7,9,11
- Only the aspect ratio (attribute 0028,0034) 1:1 is supported

Overlay plane

- Overlay type (attribute 60xx, 0040) = "G"
- Overlay bits allocated (attribute 60xx, 0100) = 16
- Overlay bit position (attribute 60xx, 0102) = 12, 13, 14, 15 (only bits above high bit permitted)
- The graphic overlay is shifted to fill overlay planes from bit 12 and consecutive bits.

Overlay plane

- Overlay type (attribute 60xx, 0040) = "G"
- Overlay bits allocated (attribute 60xx, 0100) = 1
- Overlay bit position (attribute 60xx, 0102) = 0
- Overlay data (attribute 60xx, 3000) = supported.

The Somaris/7 DICOM Viewing application also accepts the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integers and 16 bits allocated. The following values are accepted:

Pixel plane

- Samples per pixel (attribute 0028, 0002) = 1
- Photometric interpretation (attribute 0028,0004) = "MONOCHROME1"
- Photometric interpretation (attribute 0028,0004) = "MONOCHROME2"
- Pixel representation (attribute 0028, 0103) = 1 (signed)
- Bits allocated (attribute 0028, 0100) = 16
- Bits stored (attribute 0028,0101) = 16
- High bit (attribute 0028,0102) = 15
- Only the aspect ratio (attribute 0028,0034) 1:1 is supported

Overlay plane

- Overlay type (attribute 60xx, 0040) = "G"
- Overlay bits allocated (attribute 60xx, 0100) = 1
- Overlay bit position (attribute 60xx, 0102) = 0
- Overlay data (attribute 60xx, 3000) = supported.

For the MOD LUT, both the linear LUT (Rescale Slope/Intercept) and the MOD LUT SQ are supported and considered when pixel data is displayed. However, there are two limitations. The MOD LUT SQ is ignored in the following cases:

- 8-bit signed pixels
- The pixel format is changed by the MOD LUT (for example, 8 bits -> 16 bits).

If the MOD LUT SQ contains multiple LUTs, then only the first one is used.

For the VOI LUT, both the linear LUT (Window Center/Width) and the VOI LUT SQ are also supported (VOI LUT SQ with 8-bit or 16-bit LUT data).

However, if both a VOI LUT SQ and a linear MOD LUT are specified within one image, then the value of Rescale Slope is restricted to 1.

If the VOI LUT SQ contains multiple LUTs, then only the first one is used by default. The other VOI LUTs are selectable.

In this version, the Display application supports only rectangular and circular shutters. Images with other shutter types are displayed without a shutter.

3.2.3.1.3.2 Image Pixel Attribute Acceptance Criterion for Color Images - Viewing

The Siemens Somaris/7 Multi-Modality Viewing application supports the RGB color image description with the unsigned integer, 24-bit color image plane pixel format. The following values are accepted:

- Samples per pixel (attribute 0028, 0002) = 3
- Photometric interpretation (attribute 0028,0004) = "RGB"
- Pixel representation (attribute 0028, 0103) = 0
- Bits allocated (attribute 0028, 0100) = 8
- Bits stored (attribute 0028,0101) = 8
- High bit (attribute 0028,0102) = 7
- Planar configuration (attribute 0028,0006) = 0 (pixel interleave) or 1 (plane interleave)

The Siemens Somaris/7 Multi-Modality Viewing application supports the "Palette Color" color image description with the unsigned integer and 2's complement pixel format:

- Samples per pixel (attribute 0028, 0002) = 1
- Photometric interpretation (attribute 0028,0004) = "PALETTE COLOR"
- Pixel representation (attribute 0028, 0103) = 0
- Bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- Bits allocated (attribute 0028, 0100) = 16 and bits stored (attribute 0028,0101) = 16
- High bit (attribute 0028,0102) = 7, 15

Both 8-bit and 16-bit palettes are supported, but no Segmented Palette Color LUTs.

The Siemens Somaris/7 Multi-Modality Viewing application supports the YBR color image description with the unsigned integer pixel format. The following values are accepted:

- Samples per pixel (attribute 0028, 0002) = 3
- Photometric interpretation (attribute 0028,0004) = "YBR_FULL" or "YBR_FULL_422"
- Pixel representation (attribute 0028, 0103) = 0
- Bits allocated (attribute 0028, 0100) = 8 and bits stored (attribute 0028,0101) = 8
- High bit (attribute 0028,0102) = 7

If Somaris/7 software does any persistent changes on a YBR image, the resulting new image is saved with the Photometric Interpretation "RGB".

3.2.3.1.4 Presentation Context Acceptance Criterion - Storage SCP

The Somaris/7 DICOM application accepts any number of Verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to a maximum of 127 (DICOM limit). In case the Siemens Somaris/7 DICOM application runs out of resources, it will reject the association request.

3.2.3.1.5 Transfer Syntax Selection Policies - Storage SCP

The Somaris/7 DICOM application supports the following transfer syntaxes:

- Implicit VR Little Endian, Explicit VR Little Endian and Explicit VR Big Endian transfer syntaxes
- JPEG Baseline and JPEG Extended transfer syntaxes (JPEG lossy)
- JPEG Lossless Non-Hierarchical transfer syntax
- RLE Lossless Transfer Syntax
- JPEG 2000 Lossless and Lossy Transfer Syntax

Any proposed presentation context including one of these transfer syntaxes is accepted. Any proposed presentation context that does not include one of these Transfer Syntaxes is rejected.

The order of preference for accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is as follows:

1. JPEG Lossy Extended
2. JPEG Lossless Non-hierarchical
3. JPEG Lossy Baseline
4. RLE Lossless
5. Explicit VR Little Endian
6. Explicit VR Big Endian
7. Implicit VR Little Endian
8. JPEG 2000 Lossy
9. JPEG 2000 Lossless

With the RLE Lossless Transfer Syntax, the Somaris/7 application decompresses the image before storing it in the database.

With the Implicit VR Little Endian Transfer Syntax, the Somaris/7 DICOM application removes any private attributes not known to the application. A decision on the removal of a Private Element is done if there are NO entries in the attribute dictionary of the Somaris/7 DICOM application.

Therefore, any of the Explicit VR Transfer Syntaxes shall preferably be used by the Storage SCUs when sending Composite Image Instances to the Somaris/7 application.

3.3 Storage Commitment AE Specification

The Somaris/7 DICOM application provides Standard Conformance to the following DICOM V3.0 SOP Classes as an SCU

Table 7: Standard SOP Classes as Storage Commitment Push Model

SOP Class Name	SOP Class UID
Storage Commitment Push Model	1.2.840.10008.1.20.1

3.3.1 Association Establishment Policies

3.3.1.1 General

When a Send Job is successfully completed, the DICOM application generates a Storage Commitment Identifier which references all instances of the processed job. The Commit Request is then sent over a single open association. Somaris/7 waits for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with the Success Status, the generated Transaction UID is kept, together with study identification data and a time stamp. Depending on the configuration, the association is closed when the configured time-out has elapsed or after a response is received. If the association is closed before a response was received, the response is then expected on a different association. Multiple Storage Commitment Requests can be pending.

The default PDU size is of 32 kB.

3.3.1.2 Number of Associations

The Somaris/7 DICOM application initiates several associations at the same time, one for each destination to which a transfer request is being processed in the active job queue list.

The Somaris/7 DICOM application is able to accept multiple associations at the same time. It can handle up to 10 associations in parallel.

3.3.1.3 Asynchronous Nature

The Somaris/7 DICOM application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.3.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.3.2 Association Initiation Policy

The Somaris/7 Storage Commitment Application Entity acts as a Service Class User (SCU) for the

- Storage Commitment Push Model Service Class (to request commitment for the storage of instances previously sent)

To do so, Somaris/7 issues one of the following:

- N-ACTION DIMSE to request commitment
- N-EVENT-REPORT DIMSE to respond to a received storage commitment request if the association was closed by the remote system prior to response

3.3.2.1 Real-World Activity - Send Storage Commitment Request

3.3.2.1.1 Associated Real-World Activity - Job Completed

The Somaris/7 Storage Commitment application sends the commit request (N-ACTION_RQ) message and waits for acceptance of this request (N_ACTION-RSP). After receiving this, the transaction is marked as "waiting".

Depending on a particular configuration value, the association is then closed or kept open. In the first case, another configurable time-out gives the time in hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N_EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association. For both cases, if the commit response (N-EVENT-REPORT) does not arrive during the configured time, the transaction is marked as having failed. Somaris/7 does not re-send objects because of a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as having failed, otherwise the transaction is marked as "completed". In both cases, a message is given to the user.

3.3.2.1.2 Proposed Presentation Contexts - Job Completed

The Somaris/7 Storage Commitment AE will propose Presentation Contexts as shown in the following table:

Table 8: Initiation presentation context Storage Commitment Request

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

3.3.2.1.3 SOP-Specific Conformance Statement - Job Completed

Storage Commitment is supported for all the SOP class UIDs mentioned in *Table 6: Acceptable presentation contexts Storage* on page 47.

The Referenced Study Component Sequence is not supported.

The Storage Media File Set ID and UID Attributes are not supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

3.3.3 Association Acceptance Policy

The Somaris/7 Storage Commitment AE accepts an association in this case: When it is acting as an SCU and is configured to receive N-EVENT-REPORT on a separate association.

3.3.3.1 Associated Real-World Activity - Receive Storage Commit SCU

3.3.3.1.1 Associated Real-World Activity - Update Flags

Consider the case when the Somaris/7 Storage Commitment AE has sent a Storage Commitment Request and, being configured to receive responses on a separate association, has closed the association. It now gets an association request from the Storage Commitment SCP that wants to send the results. The application waits for Storage Commitment Notification triggers. Any incoming notification is checked for validity, that is, whether the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid, the Notification Identifier is evaluated and the related Instances marked with the related status. The overall Commit Status of the higher Information Entities is derived by propagation of all Image entities included in a study.

The status flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of the following (English UI assumed):

- "AC" or "SC" - Successful Commitment. A means archived to the configured archive destination, whereas S means sent to any other destination.
- "Af" or "Sf" - Commitment failed
- "A?" or "S?" - Commitment request is sent, response is pending

In case of failure, the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment is performed after sending is completed successfully.

Note: The flags A (Archived) and S (Sent) only indicate the reception of the images by the remote AE. They do not indicate the successful storage in the intended archive. The data may be lost if it is deleted by the sender, for example, by an auto-delete mechanism, and cannot be stored by the receiver.

Advise the service technician to always use 'storage commitment' if this is supported by the sender and receiver of data.

Source of danger: Misleading/misinterpretation of the flags AC/SC

The flags "AC" and "SC" indicate the reception and storage on the hard disk on the receiver side, which may be not sufficient to fulfill the regulatory requirements of long-term archiving.

Consequence: Loss of data before the required period of retention expires.

Remedy: Sending data with the attributes AC or SC over the network indicates a safe data transfer but does not fulfill the regulatory requirements of long-term archiving. Objects with the "committed" flag may be deleted by the user. Observe the regulatory requirements regarding the archiving procedure.

3.3.3.1.2 Accepted Presentation Contexts - Update Flags

The Somaris/7 Storage Commitment AE accepts Presentation Contexts as shown in the following table:

Table 9: Presentation context accepted for Storage Commitment

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

3.3.3.1.3 SOP-Specific Conformance Statement - Update Flags

If the Commitment Response (N_EVENT_REPORT) received has the status "complete - failure exists", the transaction is marked as having failed, otherwise the transaction is marked as "completed". In both cases, a message is given to the user.

The related status flags are set for the committed images in the local database.

The Somaris/7 DICOM application does NOT support the Storage Media File Set ID attributes.

3.4 Query/Retrieve AE Specification

The Query/Retrieve SCU requests that the remote SCP matches all keys specified in the request against the information in its database, and that the identified images are moved over a different (C-MOVE) storage association.

The Query/Retrieve SCP responds to queries based on the records of its database and images are sent to the requesting SCU or to a different storage destination.

The Somaris/7 DICOM application provides Standard Conformance to the following DICOM V3.0 SOP Classes as an SCU:

Table 10: SOP Classes as a Query/Retrieve SCU

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2

The Somaris/7 DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

Table 11: SOP Classes as a Query/Retrieve SCP

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Patient Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.1.3
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Study Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.2.3
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2
Patient/Study Only Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.3.3

Note

See also the Storage DICOM Conformance Statement (3.2.3 *Association Acceptance Policy* on page 46) to compare for conformance of the C-STORE sub-operation generated by the C-MOVE and C-GET DIMSE services. Furthermore, compare the supported Storage Service SOP classes described in the Storage DICOM Conformance Statement of the Modality to which the images shall be transferred.

3.4.1 Association Establishment Policies

3.4.1.1 General

With the "Search..." function, the query data is entered and the DICOM Query/Retrieve application is started. A query request is sent out to one remote node that can be selected from a list of configured Query Providers, and the response data is displayed to the user. In order to provide detailed information, early additional queries are sent for the more detailed levels not yet covered by the first results. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used is of 32 kB.

3.4.1.2 Number of Associations

The Somaris/7 DICOM Query/Retrieve application initiates several associations at a time, one for each query/retrieve request being processed.

The Somaris/7 DICOM Query/Retrieve application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

3.4.1.3 Asynchronous Nature

The Somaris/7 DICOM Query/Retrieve application does not support asynchronous communication (multiple outstanding transactions over a single association).

3.4.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.4.2 Association Initiation Policy

The Query user interface requests the query data from the user and triggers C-FIND requests to the selected remote node. The response data is displayed in the query UI for further data navigation.

When requesting an import of related items, the browser requests the retrieve application to send a C_MOVE request to the related remote node. Images are then received by the Storage SCP as described in the related section.

The following DIMSE-C operations are supported as an SCU:

- C-FIND
- C-MOVE

3.4.2.1 Real-World Activity - Find SCU

3.4.2.1.1 Associated Real-World Activity - Find SCU "Search"

The associated Real-World activity is to fill out a query form with search data and pass it as queries to the network application, which issues a C-FIND over a previously built association. The remote SCP responds with related data entries that are passed to a browser application. When the data transfer has finished, the association is closed.

3.4.2.1.2 Proposed Presentation Contexts - Find SCU

The Somaris/7 DICOM Query application proposes Presentation Contexts as shown in the following table:

Table 12: Proposed Presentation Contexts - Find SCU:

Presentation Context Table		Role	Extended Negotiation
		SCU	See Note
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2
Patient Study only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2

Note

Which of the three query models is to be used by the Somaris/7 Query SCU application can be configured. If the Patient and Study Root Abstract Syntaxes are configured, the C_FIND SCU uses the Patient Root Model only for C-FIND requests on the PATIENT level. For all other levels, it uses the STUDY Root Model.

It is highly recommended that you only configure the Study Root Model if the corresponding Query SCP supports this Model. If the Query SCP does not support queries on the Series Level, the Patient Study Only Model should be used.

3.4.2.1.3 SOP-Specific Conformance Statement - Find SCU

The Somaris/7 DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. On each level, the unique attributes of all previous levels are also sent (values are provided by the user by selection from a list). For instance, for a query using the patient root model on the Series level, the Patient ID of the currently selected patient and the Study Instance UID of the currently selected study are included in the message. The interactive querying of attributes on the IMAGE level is not supported by the Query SCU. Nevertheless, the retrieval of individual Objects is possible.

The Query dialog in Somaris/7 offers search keys on different levels (Patient, Study, Series). Depending on the used Query Model (Patient Root, Study Root, Patient Study Only), the Somaris/7 DICOM Query/Retrieve SCU executes multiple queries sequentially.

Example using the Patient Root Model:

The first query is performed on patient level with the entered patient level query keys. For each query result, a new query is performed on study level with the entered study level query keys. Finally, for each result on study level, a query is performed on series level with the entered series level keys.

The *Query attributes* describe the search keys for the three query models (Patient Root, Study Root, Patient Study Only) that the Somaris/7 Query/Retrieve application supports as an SCU. Matchings are either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is returned no matter what value it has.

Table 13: Query attributes

Attribute name	Tag	Type	Matching	user input	return value displayed
Patient level^a					
Patient name	(0010,0010)	R	wildcard ^d	enter value	yes
Patient ID	(0010,0020)	U	wildcard ^d	enter value	yes
Patient's birth date	(0010,0030)	O	universal (NULL)	enter value	yes
Patient's sex	(0010,0040)	O	universal (NULL)	enter value	yes
Number of Patient related studies	(0020,1200)	O	universal (NULL)	-	yes ^b
Number of Patient relates series	(0020,1202)	O	universal (NULL)	-	no
Number of Patient related instances	(0020,1204)	O	universal (NULL)	-	no
Study level					
Patient Name ^c	(0010,0010)	R	wildcard ^d	enter value	yes
Patient ID	(0010,0020)	R	wildcard ^d	enter value	yes
Patient's Birth date ^c	(0010,0030)	O	universal (NULL)	enter value	yes

Attribute name	Tag	Type	Matching	user input	return value displayed
Patient's Sex ^c	(0010,0040)	O	universal (NULL)	enter value	yes
Study Instance UID	(0020,000D)	U	single value	-	no
Study ID	(0020,0010)	R	universal (NULL)	enter value ^d	yes
Study Date	(0008,0020)	R	universal (NULL)	enter value ^e	yes
Study Time	(0008,0030)	R	universal (NULL)	-	yes
Accession Number	(0008,0050)	R	universal (NULL)	enter value ^d	yes
Study Description	(0008,1030)	O	universal (NULL)	enter value ^d	yes
Referring Physician's Name	(0008,0090)	O	universal (NULL)	enter value ^d	yes
Name of Physician Reading Study	(0008,1060)	O	universal (NULL)	enter value ^d	yes
Modalities in Study	(0008,0061)	O	universal (NULL)	enter value ^d	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	no
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	no
Number of Study related Series	(0020,1206)	O	universal (NULL)	-	yes ^f
Number of Study related Instances	(0020,1208)	O	universal (NULL)	-	no
Series level					
Series Instance UID	(0020,000E)	U	single value	-	no
Series Number	(0020,0011)	R	universal (NULL)	-	yes
Modality	(0008,0060)	R	universal (NULL)	enter value	yes
Series Date	(0008,0021)	O	universal (NULL)	-	yes
Series Time	(0008,0031)	O	universal (NULL)	-	yes
Study ID	(0020,0010)	O	universal (NULL)	-	yes
Series Description	(0008,103E)	O	universal (NULL)	enter value ^d	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	yes
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	yes
Body Part Examined	(0018,0015)	O	universal (NULL)	enter value ^d	yes
Scan Options	(0018,0022)	O	universal (NULL)	_d	yes

Attribute name	Tag	Type	Matching	user input	return value displayed
Protocol name	(0018,1030)	O	universal (NULL)	-	no
Performing Physician	(0018,1050)	O	universal (NULL)	enter value ^d	yes
Performed procedure step start date	(0040,0244)	O	universal (NULL)	-	yes
Performed procedure step start time	(0040,0245)	O	universal (NULL)	-	yes
Request Attribute Sequence	(0040,0275)	O	universal (NULL)	-	yes
>Requested Procedure ID	(0040,1001)	O	universal (NULL)	-	yes
>Scheduled Procedure ID	(0040,0009)	O	universal (NULL)	-	yes
Number of series related instances	(0020,1209)	O	universal (NULL)	-	yes
Image Level					
SOP Instance UID	(0008,0018)	U	single value	-	no
Image Number	(0020,0013)	R	universal (NULL)	-	yes
Storage Media File Set ID	(0008,0130)	O	universal (NULL)	-	no
Retrieve AE Title	(0008,0054)	O	universal (NULL)	-	no
Instance Date	(0008,0023)	O	universal (NULL)	-	no
Instance Time	(0008,0033)	O	universal (NULL)	-	no
Number of Frames	(0028,0008)	O	universal (NULL)	-	yes
Content Date	(0008,0023)	O	single value, range matching, universal	enter value	yes
Content Time	(0008,0033)	O	single value, range matching, universal	enter value	yes
Image comments	(0020,4000)	O	universal (NULL)	-	no
Referenced Request Sequence	(0040,A370)	O	sequence matching	-	yes
> Accession Number	(0008,0050)	O	single value, universal	-	yes
> Requested Procedure ID	(0040,1000)	O	single value, universal	-	yes
Concept Name Code Sequence	(0040,A043)	O	sequence matching	enter value	yes
> Code Value	(0008,0100)	O	single value, universal, wildcard	enter value	yes
> Coding Scheme Designator	(0008,0102)	O	single value, universal, wildcard	-	yes

Attribute name	Tag	Type	Matching	user input	return value displayed
> Coding Scheme Version	(0008,0103)	O	single value, universal, wildcard	-	yes
> Code Meaning	(0008,0104)	O	single value, universal, wildcard	-	yes
Template Identifier	(0040,DB00)	O	single value, universal, wildcard	-	yes
Completion Flag	(0040,A491)	O	single value, universal, wildcard	enter value	yes
Verification Flag	(0040,A493)	O	single value, universal, wildcard	enter value	yes
Verifying Observer Sequence	(0040,A073)	O	sequence matching	enter value	yes
> Verifying Organization	(0008,A072)	O	single value, universal, wildcard	-	yes
> Verifying DateTime	(0008,A030)	O	single value, range matching, universal	enter value	yes
> Verifying Observer Name	(0008,A075)	O	single value, universal, wildcard	enter value	yes
> Verifying Observer Identification Code Sequence	(0040,A088)	O	sequence matching		yes
>> Code Value	(0008,0100)	O	single value, universal, wildcard	-	yes
>> Coding Scheme Designator	(0008,0102)	O	single value, universal, wildcard	-	yes
>> Coding Scheme Version	(0008,0103)	O	single value, universal, wildcard	-	yes
>> Code Meaning	(0008,0104)	O	single value, universal, wildcard	-	yes

^a. Only for the Patient Root or Patient Study Only information model

^b. Implicitly visualized in the UI if no study and series search attributes have been entered

^c. Only for the Study Root information model

^d. A "*" is always added to the user supplied string

^e. Date range possible

^f. Implicitly visualized in the UI if no series search attributes have been entered

The Find SCU interprets the following status codes:

Table 14: C-FIND response status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - the Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.4.2.2 Real-World Activity - Move SCU

3.4.2.2.1 Associated Real-World Activity - Move SCU "Import"

The operator selects a data entry in the Query UI and activates the "Import" function.

This generates a retrieval request to the archival application, which issues a C-MOVE service according to the Patient Root or Study Root query model. The Storage Service Class Conformance Statement of the SCP describes the C-STORE service, which is generated by processing the C-MOVE service.

The transferred image data is processed as described in the storage class SCP descriptions.

The possibility to request the remote C-MOVE provider to move data to an application entity other than the C-MOVE SCU (the Somaris/7 DICOM application) is NOT used.

3.4.2.2.2 Proposed Presentation Contexts - Move SCU "Import"

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 15: Proposed Presentation Contexts - Move SCU

Presentation Context Table		Role	Extended Negotiation
		SCU	See Note
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1 (1)
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1 (1)
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2
Patient Study Only Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	DICOM Implicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2
		DICOM Explicit VR Little Endian Transfer Syntax	1.2.840.10008.1.2.1 (2)
		DICOM Explicit VR Big Endian Transfer Syntax	1.2.840.10008.1.2.2

Note

(1) C-MOVE extended negotiation is not supported by the SCU

(2) The Study Transfer supports C-MOVE on Patient level

3.4.2.2.3 SOP-Specific Conformance Statement - Move SCU "Import"

The C-MOVE presentation context is negotiated at the time of establishment of the association. The C-STORE sub-operations must be done on a different association to transfer images to their own Storage Service Class SCP.

The Move SCU interprets the following status codes:

Table 16: C-MOVE response status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub-operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
Failed	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.4.3 Association Acceptance Policy

The Query/Retrieve SCU and SCP establish an association by using the DICOM association services. During association establishment, the Query/Retrieve application entities negotiate the supported SOP classes to exchange the capabilities of the SCU and the SCP.

The following DIMSE-C operations are supported as an SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

3.4.3.1 Real-World Activity - Find SCP

3.4.3.1.1 Associated Real-World Activity - Find SCP

The associated Real-World activity is to respond to query requests to an SCU with the Patient Root, Study Root and Patient/Study Only query models. Relational retrieve operations are NOT supported. Using a C-FIND-CANCEL request, the running query can be cancelled at any time.

The SCP supports multiple C-FIND-requests over the same association, but not multiple C-MOVE requests.

3.4.3.1.2 Accepted Presentation Contexts - Find SCP

The Somaris/7 Query/Retrieve AE accepts Presentation Contexts as shown in the following table:

Table 17: Accepted Presentation Contexts - Find SCP

Presentation Context Table		Role	Extended Negotiation
		SCP	See Note
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Patient/Study Only Query/ Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Note

C-FIND Extended Negotiation is NOT supported by the SCP.

The order of preference in accepting a Transfer syntax is the following:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.1.3 SOP-Specific Conformance Statement - Find SCP

The Somaris/7 DICOM Query/Retrieve SCP supports hierarchical queries with all mandatory and optional search keys.

The following six notes apply to the handling of the Patient's Name attribute (0010,0010) as a Query/Retrieve SCP. The syntactical structure of the Patient's Name (0010,0010) attribute is as follows:

<single byte group>=<ideographic group>=<phonetic group>

Each group may have up to five components, which are separated by carets "^".

1. The matching of the Patient's Name attribute (0010,0010) is case-insensitive.
2. If a search string matches the complete value of a database object's Patient's Name, a match is returned.
3. If a search string matches an individual group (single byte, ideographic or phonetic) of a database object's Patient's Name, a match is returned.
4. If a search string matches two consecutive groups of a database object's Patient's Name, a match will be returned.
5. Redundant group separators "=" or component separators "^" are treated as insignificant for matching.
6. Leading and trailing blanks within a component or a group of Patient's Name (0010,0010) are treated as insignificant for matching.

Except for the Patient's Name attribute (0010,0010), any other query attribute contents are treated as Case Sensitive.

In wildcard queries, the symbol "?" is treated as "*" by the C-FIND-SCP application. As a consequence, the query string "?abc*" is processed as "**abc*".

If the value of the patient level unique key "Patient ID" is not known, it may be returned with zero length. The "Image Comments" attribute is not included in the C-FIND-RSP, if this is not set in the DB, even if it was requested as the return key in the related C-FIND-RQ.

Use of the Storage Media File Set ID and Retrieve AE Title attributes with the C-FIND-RSP message:

- The C-FIND SCP may return the Storage Media File Set ID (0088,0130) and Storage Media File Set UID (0088,0140) DICOM attributes empty or not at all. The Storage Media File Set ID - if existent - can be returned at Study/Series/Image Level. Only on Image Level, the values ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related instance.
- The C-FIND SCP may return the Retrieve AE Title (0008,0054) DICOM attribute as empty or not at all. The Retrieve AE Title - if existent - can only be returned at Image Level (for the Patient Root and Study Root models) or at Study Level (for the Patient/Study Only model).

Relational Queries are NOT supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. It is possible that matches continue (more C-FIND responses with status PENDING) until the cancel operation has completed.

The attributes supported on the various levels of the three information models are listed in the tables of the following sections.

3.4.3.1.3.1 Patient Root Information Model

Table 18: Patient level attributes, Patient Root Information Model, Patient level attributes

Attribute name	Tag	Type	Matching
Patient Name	(0010,0010)	R	single value, wildcard, universal
Patient ID	(0010,0020)	U	single value, wildcard, universal
Patient's Birth Date	(0010,0030)	O	single value, range, universal
Patient's Birth Time	(0010,0032)	O	single value, range, universal
Patient's Sex	(0010,0040)	O	single value, wildcard, universal
Ethnic Group	(0010,2160)	O	single value, wildcard, universal
Patient Comments	(0010,4000)	O	wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal

Table 19: Study level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Study Instance UID	(0020,000D)	U	single value, list of UIDs
Study ID	(0020,0010)	R	single value, wildcard, universal
Study Date	(0008,0020)	R	single value, range, universal
Study Time	(0008,0030)	R	single value, range, universal
Accession Number	(0008,0050)	R	single value, wildcard, universal
Referring Physi- cian's Name	(0008,0090)	O	single value, wildcard, universal
Study Description	(0008,1030)	O	single value, wildcard, universal
Admitting Diag- noses Description	(0008,1080)	O	single value, wildcard, universal
Patient's Age	(0010,1010)	O	single value, wildcard, universal
Patient's Size	(0010,1020)	O	single value, universal
Patient's Weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal
Additional Patient History	(0010,21B0)	O	wildcard, universal
Name of Physician reading Study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of Study related Series	(0020,1206)	O	universal
Number of study related Instances	(0020,1208)	O	universal

Table 20: Series level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Series Instance UID	(0020,000E)	U	single value, list of UID
Series Number	(0020,0011)	R	single value, universal

Table 20: Series level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body Part Examined	(0018,0015)	O	single value, wildcard, universal
Patient Position	(0018,5100)	O	single value, wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	single value, universal
Largest Pixel Value in Series	(0028,0109)	O	single value, universal
Protocol Name	(0018,1030)	O	single value, wildcard, universal
Series Date	(0008,0021)	O	single value, range, universal
Series Time	(0008,0031)	O	single value, range, universal
Series Description	(0008,103E)	O	single value, wildcard, universal
Operator's Name	(0008,1070)	O	single value, wildcard, universal
Performing Physi- cian's Name	(0008,1050)	O	single value, wildcard, universal
Performed Proce- dure Step Start Date	(0040,0244)	O	universal
Performed Proce- dure Step Start Time	(0040,0245)	O	universal
Number of series related Instances	(0020,1209)	O	universal
Referenced Request Sequence	(0040,A370)	O	sequence matching
>Requested Proce- dure ID	(0040,1001)	O	single value, universal

Table 21: Image level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
SOP Instance UID	(0008,0018)	U	single value, list of UID
SOP Class UID	(0008,0016)	U	single value
Instance Number	(0020,0013)	R	single value, universal

Table 21: Image level attributes, Patient Root Information Model

Attribute name	Tag	Usage SCU	Matching
Content Date	(0008,0023)	O	single value, range, universal
Content Time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image comments	(0020,4000)	O	universal
Concept Name Code Sequence	(0040,A043)	O	sequence matching
> Code Value	(0008,0100)	O	single value, universal, wild- card
> Coding Scheme Designator	(0008,0102)	O	single value, universal, wild- card
> Coding Scheme Version	(0008,0103)	O	single value, universal, wild- card
> Code Meaning	(0008,0104)	O	single value, universal, wild- card
Template Identifier	(0040,DB00)	O	single value, universal, wild- card
Completion Flag	(0040,A491)	O	single value, universal, wild- card
Verification Flag	(0040,A493)	O	single value, universal, wild- card
Verifying Observer Sequence	(0040,A073)	O	sequence matching
> Verifying Organization	(0008,A072)	O	single value, universal, wild- card
> Verifying DateTime	(0008,A030)	O	single value, range matching, universal
> Verifying Observer Name	(0008,A075)	O	single value, universal, wild- card
> Verifying Observer Identification Code Sequence	(0040,A088)	O	sequence matching
>> Code Value	(0008,0100)	O	single value, universal, wild- card
>> Coding Scheme Designator	(0008,0102)	O	single value, universal, wild- card
>> Coding Scheme Version	(0008,0103)	O	single value, universal, wild- card
>> Code Meaning	(0008,0104)	O	single value, universal, wild- card

3.4.3.1.3.2 Study Root Information Model

Table 22: Study level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Patient Name	(0010,0010)	R	single value, wildcard, universal
Patient ID	(0010,0020)	R	single value, wildcard, universal
Patient's Birth Date	(0010,0030)	O	single value, range, universal
Patient's Birth Time	(0010,0032)	O	single value, range, universal
Patient's Sex	(0010,0040)	O	single value, wildcard, universal
Patient Comments	(0010,4000)	O	wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient relates Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Instance UID	(0020,000D)	U	single value, list of UIDs
Study ID	(0020,0010)	R	single value, wildcard, universal
Study Date	(0008,0020)	R	single value, range, universal
Study Time	(0008,0030)	R	single value, range, universal
Accession Number	(0008,0050)	R	single value, wildcard, universal
Referring Physician's Name	(0008,0090)	O	single value, wildcard, universal
Study Description	(0008,1030)	O	single value, wildcard, universal
Admitting Diagnoses Description	(0008,1080)	O	single value, wildcard, universal
Patient's Age	(0010,1010)	O	single value, wildcard, universal
Patient's Size	(0010,1020)	O	single value, universal
Patient's Weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal
Additional Patient History	(0010,21B0)	O	wildcard, universal

Table 22: Study level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Name of Physician reading Study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of Study related Series	(0020,1206)	O	universal
Number of Study related Instances	(0020,1208)	O	universal

Table 23: Series level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Series Instance UID	(0020,000E)	U	single value, list of UID
Series Number	(0020,0011)	R	single value, universal
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body Part Examined	(0018,0015)	O	single value, wildcard, universal
Patient Position	(0018,5100)	O	single value, wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	single value, universal
Largest Pixel Value in Series	(0028,0109)	O	single value, universal
Protocol Name	(0018,1030)	O	single value, wildcard, universal
Series Date	(0008,0021)	O	single value, range, universal
Series Time	(0008,0031)	O	single value, range, universal
Series Description	(0008,103E)	O	single value, wildcard, universal
Operators Name	(0008,1070)	O	single value, wildcard, universal
Performing Physician's Name	(0008,1050)	O	single value, wildcard, universal
Performed Procedure Step Start Date	(0040,0244)	O	universal

Table 23: Series level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Performed Procedure Step Start Time	(0040,0245)	O	universal
Number of Series related Instances	(0020,1209)	O	universal

Table 24: Image level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
SOP Instance UID	(0008,0018)	U	single value, list of UID
SOP Class UID	(0008,0016)	U	single value,
Instance Number	(0020,0013)	R	single value, universal
Content Date	(0008,0023)	O	single value, range, universal
Content Time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image Comments	(0020,4000)	O	universal
Referenced Request Sequence	(0040,A370)	O	sequence matching
> Accession Number	(0008,0050)	O	single value, universal
> Requested Procedure ID	(0040,1000)	O	single value, universal
Concept Name Code Sequence	(0040,A043)	O	sequence matching
> Code Value	(0008,0100)	O	single value, universal, wildcard
> Coding Scheme Designator	(0008,0102)	O	single value, universal, wildcard
> Coding Scheme Version	(0008,0103)	O	single value, universal, wildcard
> Code Meaning	(0008,0104)	O	single value, universal, wildcard
Template Identifier	(0040,DB00)	O	single value, universal, wildcard
Completion Flag	(0040,A491)	O	single value, universal, wildcard
Verification Flag	(0040,A493)	O	single value, universal, wildcard

Table 24: Image level attributes, Study Root Information Model

Attribute name	Tag	Usage SCU	Matching
Verifying Observer Sequence	(0040,A073)	O	sequence matching
> Verifying Organization	(0008,A072)	O	single value, universal, wild-card
> Verifying DateTime	(0008,A030)	O	single value, range matching, universal
> Verifying Observer Name	(0008,A075)	O	single value, universal, wild-card
> Verifying Observer Identification Code Sequence	(0040,A088)	O	sequence matching
>> Code Value	(0008,0100)	O	single value, universal, wild-card
>> Coding Scheme Designator	(0008,0102)	O	single value, universal, wild-card
>> Coding Scheme Version	(0008,0103)	O	single value, universal, wild-card
>> Code Meaning	(0008,0104)	O	single value, universal, wild-card

3.4.3.1.3.3 Patient Study Only Information Models

Table 25: Patient instance level, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Patient Name	(0010,0010)	R	single value, wildcard, universal
Patient ID	(0010,0020)	U	single value, wildcard, universal
Patient's Birth Date	(0010,0030)	O	single value, range, universal
Patient's Birth Time	(0010,0032)	O	single value, range, universal
Patient's Sex	(0010,0040)	O	single value, wildcard, universal
Ethnic Group	(0010,2160)	O	single value, wildcard, universal
Patient comments	(0010,4000)	O	wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient relates Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal

Table 26: Study level attributes, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Study Instance UID	(0020,000D)	U	single value, list of UIDs
Study ID	(0020,0010)	R	single value, wildcard, universal
Study Date	(0008,0020)	R	single value, range, universal
Study Time	(0008,0030)	R	single value, range, universal
Accession Number	(0008,0050)	R	single value, wildcard, universal
Referring Physi- cian's Name	(0008,0090)	O	single value, wildcard, universal
Study Description	(0008,1030)	O	single value, wildcard, universal
Admitting Diag- noses Description	(0008,1080)	O	single value, wildcard, universal
Patient's Age	(0010,1010)	O	single value, wildcard, universal
Patient's Size	(0010,1020)	O	single value, universal

Table 26: Study level attributes, Patient Study Only Information Model

Attribute name	Tag	Usage SCU	Matching
Patient's Weight	(0010,1030)	○	single value, universal
Occupation	(0010,2180)	○	single value, wildcard, universal
Additional Patient History	(0010,21B0)	○	wildcard, universal
Name of Physician reading Study	(0008,1060)	○	single value, wildcard, universal
Modalities in Study	(0008,0061)	○	multiple values, universal
Number of Study related Series	(0020,1206)	○	universal
Number of Study related Instances	(0020,1208)	○	universal

Note

The C-FIND-RSP message contains the following attributes:

- Specific Character Set (0008,0005), if there is a specific character set in use
- Query/Retrieve Level (0008,0052) from the C_FIND_RQ
- Retrieve AE Title (0008,0054) at study, series and image level.
This value is a list of AE titles from which the images can be retrieved. It is always NULL except for at the lowest level of the query model (Image level for the the Patient Root or Study Root models, and Study level for the Patient/ Study Only model).
- Storage Media File set ID (0088,0130) at the study, series and image levels.
If Storage Media File set ID is not present, a NULL value is returned.
- Attributes requested by C_FIND_RQ and supported by the SCP

Note

See also 3.4.3.1.3 SOP-Specific Conformance Statement - Find SCP on page 86

The Find SCP returns the following status codes:

Table 27: C-FIND return status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - the Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.4.3.2 Real-World Activity - Get SCP

3.4.3.2.1 Associated Real-World Activity - Get SCP

The associated Real-World activity is to respond to retrieve requests initiated by a foreign SCU. The SCP supports the Patient Root, Study Root and Patient/Study Only query models. The Storage Service Class Conformance Statement describes the C-STORE service which is generated by the C-GET service. Relational retrieve operations are NOT supported.

Multiple C-GET requests over the same association are NOT supported.

3.4.3.2.2 Proposed Presentation Contexts - Get SCP

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 28: Proposed Presentation Contexts -- Get SCP

Presentation Context Table		Role	Extended Negotiation
		SCP	See Note
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Patient Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.1.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Study Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.2.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Patient/Study Only Query/ Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Note

C-GET Extended Negotiation is NOT supported by the SCP.

The order of preference in accepting a Transfer syntax is as follows:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.2.3 SOP-Specific Conformance Statement - Get SCP

The C-GET presentation context must be negotiated at the time of establishment of the association, along with the C-STORE sub-operations that must be carried out on the same association as the C-GET operation. Relational retrieve operations are NOT supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section give information about "U" marked key attributes.

Note

In DICOM wildcard queries, the symbol '?' is treated as '*' by the Find SCP. Therefore, a wildcard query using "?abc*" is actually treated as "*abc*".

The Get SCP returns the following status codes:

Table 29: C-GET return status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub-operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.4.3.3 Real-World Activity - Move SCP

3.4.3.3.1 Associated Real-World Activity - Move SCP

The associated Real-World activity is to respond to retrieve requests to an SCU. The SCP supports the Patient Root, Study Root and Patient/Study Only query models. The Storage Service Class Conformance Statement describes the C-STORE service that is generated by the C-MOVE service. Relational retrieve operations are NOT supported.

Multiple C-MOVE requests over the same association are NOT supported.

3.4.3.3.2 Accepted Presentation Contexts - Move SCP

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 30: Proposed Presentation Contexts - Move SCP

Presentation Context Table		Role	Extended Negotiation
		SCP	See Note
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Patient Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Patient/Study Only Query/ Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

Note

C-MOVE Extended Negotiation is NOT supported by the SCP.

The order of preference in accepting a Transfer syntax is as follows:

1. Explicit VR Little Endian
2. Explicit VR Big Endian
3. Implicit VR Little Endian

3.4.3.3.3 SOP-Specific Conformance Statement - Move SCP

The C-MOVE presentation context is negotiated at the time of establishment of the association. The C-STORE sub-operations are done on a different association, specified in the C-MOVE request, to transfer images to another SCP of the Storage Service Class. Relational retrieve operations are NOT supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section give information about "U" marked key attributes.

Note

In DICOM wildcard queries, the symbol '?' is treated as '*' by Find SCP. Therefore, a wildcard query with "?abc*" is actually treated as "*abc*".

The Move SCP returns the following status codes:

Table 31: C-MOVE return status

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub-operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

3.5 Print AE Specification

The print management SCU (HCS) invokes print management DIMSE services to transfer images from the local AE to the remote SCP AE, in order to print the images with the defined film format and size on a selected network DICOM hard-copy printer (see DICOM part 4 annex H). This is done in a "full-page" print mode.

The Somaris/7 DICOM implementation provides Standard Conformance to the following DICOM V3.0 Basic Grayscale Print Management Meta SOP Classes as an SCU:

Table 32: Basic Grayscale Print Management Meta SOP-Classes

SOP Class Name	SOP Class UID
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9
▪ Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
▪ Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
▪ Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4
▪ Printer SOP Class	1.2.840.10008.5.1.1.16
▪ Print Job SOP Class	1.2.840.10008.5.1.1.14
▪ Presentation LUT SOP Class	1.2.840.10008.5.1.1.23

Table 33: Basic Color Print Management Meta SOP-Classes

SOP Class Name	SOP Class UID
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18
▪ Basic Film Session SOP Class	1.2.840.10008.5.1.1.1
▪ Basic Film Box SOP Class	1.2.840.10008.5.1.1.2
▪ Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1
▪ Printer SOP Class	1.2.840.10008.5.1.1.16
▪ Print Job SOP Class	1.2.840.10008.5.1.1.14

3.5.1 Association Establishment Policies

3.5.1.1 General

Whenever a film is completely set up and printed by command or automatism, the job is prepared for processing. As soon as the queue is ready to process, the job is activated and carried out according to the processing data. The related Print application initiates an association to the print destination and processes the printing of the related information.

The default PDU size is of 32 kB.

3.5.1.2 Number of Associations

The Somaris/7 DICOM Print application initiates one association at a time for the print device configured.

3.5.1.3 Asynchronous Nature

The Somaris/7 DICOM implementation does not support asynchronous communication (multiple outstanding transactions over a single association).

3.5.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.5.2 Association Initiation Policy

When triggered by the Print job queue, the Print Management SCU establishes an association by using the DICOM association services. With the help of the N-GET request for the printer SOP Class, the Status is determined before printing.

In case no problems are encountered with the N-CREATE/N-SET Services for the related Basic Print SOP Classes, the film sheet is set up for printing and the image(s) is(are) transferred to the printer device.

After the last film has been printed from the queue, the Print application leaves the association open for another 60 seconds. If a new film job is ready for printing within this time limit, the job will be processed immediately over the still open association. If there is no new job, the association is closed after the time-out has elapsed. This is done to optimize automatic printing.

During the "idle time" (no open association to printer) the Print application issues a cyclic camera status request (using N-GET of the Printer SOP Class) every 5 minutes.

3.5.2.1 Real-World Activity

3.5.2.1.1 Associated Real-World Activity - Printing a Printer Job Queue Entry

Whenever a film sheet is prepared by the user, it is forwarded to the Printer Job queue. As soon as the associated Printer device is available, the job is activated and an association is set up.

The film sheet is internally processed, converted to a Standard/1-1 page and the page image is sent. The status is controlled by waiting for an N-EVENT message throughout the transfer until the last image or film sheet has been sent.

If the response from the remote application contains a status other than Success or Warning, the association is aborted.

3.5.2.1.2 Proposed Presentation Contexts (Presentation Context Table)

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 34: Presentation contexts - Print SCU

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Basic Grayscale Print Management Meta SOP class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic Color Print Management Meta SOP class	1.2.840.10008.5.1.1.18	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic film session SOP class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic film box SOP class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic grayscale image box SOP class	1.2.840.10008.5.1.1.4	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Basic color image box SOP class	1.2.840.10008.5.1.1.4.1	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Printer SOP class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Print Job SOP class	1.2.840.10008.5.1.1.14	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2
Presentation LUT SOP class	1.2.840.10008.5.1.1.23	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

3.5.2.1.3 SOP-Specific Conformance Statement - Meta SOP Classes

The Somaris/7 DICOM Print Management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class and Basic Color Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM SCP, for example:

- Maximum number of print jobs in the queue
- Maximum number of print copies
- Supported film sizes of the connected DICOM SCP
- Supported film formats of the DICOM SCP
- Lookup table definition

The printing is only suspended in the case of a failure return status of the SCP.

3.5.2.1.3.1 Basic Film Session SOP Class

The Basic Film Session information object definition describes all the user defined parameters that are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes that are printed on one hardcopy printer.

The Somaris/7 DICOM Print application supports the following DIMSE Service Elements for the Basic Film Session SOP class as an SCU:

- N-CREATE
- N-DELETE

The Basic Film Session SOP class N-CREATE-RQ (SCU) uses the following attributes:

Table 35: Used Basic Film Session N-CREATE_RQ attributes

Attribute name	Tag	Usage SCU	Supported Values
Number of Copies	(2000,0010)	U	1
Medium Type	(2000,0030)	U	BLUE FILM CLEAR FILM PAPER
Film Destination	(2000,0040)	U	MAGAZINE PROCESSOR

The number of copies sent to the DICOM printer is always 1. The job is sent n times for n copies.

The affected SOP Instance UID received with the N-CREATE-RSP message from the SCP is kept internally and used for later requests (for example, using N-DELETE-RQ) on the Basic Film Session SOP Class. Refer to the table below:

Table 36: Attributes of the N-DELETE-RQ on the Basic Film Session SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session

The N-DELETE-RQ on the Basic Film Session SOP Class is used to delete the entire Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP class interprets the following status codes (from the N-CREATE-RSP, N-DELETE-RSP messages):

Table 37: Basic Film Session SOP status

Service Status	Meaning	Protocol Codes
Failure	Film session SOP instance hierarchy does not contain film box SOP instances	C600
	Unable to create print job, print queue is full	C601
	Image size is larger than the image box size	C603
Warning	Memory allocation not supported	B600
	Film session printing is not supported	B601
	Film box does not contain image box (empty page)	B602
Success	Films belonging to the film session are accepted for printing	0000

3.5.2.1.3.2 Basic Film Box SOP Class

The Basic Film Box information object definition describes all the user-defined parameters of one film of the film session. The Basic Film Box information description defines the presentation parameters that are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

The following are supported as an SCU:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP class N-CREATE-RQ message uses the following attributes (the values used for each attribute depend on the DICOM Printer configuration within the Somaris/7 DICOM print management SCU):

Table 38: Used Film Box N-CREATE_RQ attributes

Attribute name	Tag	Usage SCU	Supported Values
Image Display Format	(2010,0010)	M	STANDARD\C-R
Referenced Film Session Sequence	(2010,0500)	M	
>Referenced SOP Class UID	(0008,1150)	M	1.2.840.10008.5.1.1.1

Table 38: Used Film Box N-CREATE_RQ attributes

Attribute name	Tag	Usage SCU	Supported Values
>Referenced SOP Instance UID	(0008,1155)	M	
Film Orientation	(2010,0040)	M	PORTRAIT LANDSCAPE
Film Size ID	(2010,0050)	M	8INX10IN 10INX12IN 10INX14IN 11INX14IN 14INX14IN 14INX17IN 24CMX24CM 24CMX30CM
Magnification Type	(2010,0060)	M	BILINEAR CUBIC NONE REPLICATE
Border Density	(2010,0100)	U	BLACK WHITE
Max Density	(2010,0130)	U	0 < Value
Min Density	(2010,0120)	U	0 < Value < 50
Illumination	(2010,015E)	U	0 < Value Required if Presentation LUT is present
Reflective Ambient Light	(2010,0160)	U	0 < Value Required if Presentation LUT is present
Referenced Presentation LUT Sequence	(2050,0500)	U	

For Page Mode printing, the Image Display format used is Standard\1,1. For Image Mode Printing, the Image Display format used is Standard\C,R where C is the number of Columns and R is the number of Rows as specified in the Hard-copy Layout.

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with its SOP Class / Instance UID pairs, which are stored internally to be further used by the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film sheet have been set, the Somaris/7 DICOM print manager issues an N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box (returned in N-CREATE-RSP of the Basic Film Box SOP class) and the Action Type ID 1.

The affected SOP Instance UID received with the N-CREATE-RSP message is kept internally and used for later requests (for example, using N-DELETE-RQ) on the Basic Film Box SOP Class. Refer to the table below:

Table 39: Attributes of the N_DELETE_RQ on the Basic Film Session SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box

The Basic Film Box SOP class interprets the following status codes:

Table 40: Basic Film Box SOP status

Service Status	Meaning	Protocol Codes
Failure	Unable to create print job; print queue is full	C602
	Image size is larger than the image box size	C603
	Film box does not contain image box (empty page)	B603
Warning	Requested MinDensity or MaxDensity outside of printer's operating range	B605
Success	Film accepted for printing	0000

3.5.2.1.3.3 Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image-related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data that apply to a single image of a sheet of film.

The Grayscale Image Box SOP class uses only the N-SET-RQ with the following attributes:

Table 41: Used Basic Grayscale Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
Basic Grayscale Image Sequence	(2020,0110)	M	
>Samples Per Pixel	(0028,0002)	M	1
>Photometric Interpretation	(0028,0004)	M	MONOCH- ROME2
>Rows	(0028,0010)	M	
>Columns	(0028,0011)	M	
>Pixel Aspect Ratio	(0028,0034)	M	
>Bits Allocated	(0028,0100)	M	8,16

Table 41: Used Basic Grayscale Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
>Bits Stored	(0028,0101)	M	8,12
>High Bit	(0028,0102)	M	7,11
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

The Grayscale Image Box SOP class interprets the following status codes:

Table 42: Basic Grayscale Image Box SOP status

Service Status	Meaning	Protocol Codes
Failure	Image contains more pixels than the printer can print in the Image box	C603
	Insufficient memory in printer to store the image	C605
Warning	Requested MinDensity or MaxDensity outside of printer's operating range	B605
Success		0000

3.5.2.1.3.4 Basic Color Image Box SOP Class

The Basic Color Image Box information object definition is the presentation of an image and image-related data in the image area of a film. The Basic Image Box information describes the presentation parameters and image pixel data that apply to a single image of a sheet of film.

The Color Image Box SOP class uses only the N-SET-RQ with the following attributes:

Table 43: Used Basic Color Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
Basic Color Image Sequence	(2020,0111)	M	
>Samples Per Pixel	(0028,0002)	M	3
>Photometric Interpretation	(0028,0004)	M	RGB
>Planar Configuration	(0028,0006)	M	0
>Rows	(0028,0010)	M	
>Columns	(0028,0011)	M	
>Pixel Aspect Ratio	(0028,0034)	M	
>Bits Allocated	(0028,0100)	M	8
>Bits Stored	(0028,0101)	M	8
>High Bit	(0028,0102)	M	7

Table 43: Used Basic Color Image Box N-SET attributes

Attribute name	Tag	Usage SCU	Supported Values
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

The Color Image Box SOP class interprets the following status codes:

Table 44: Basic Color Image Box SOP status

Service Status	Meaning	Protocol Codes
Failure	Image contains more pixels than the printer can print in the Image box	C603
	Insufficient memory in printer to store the image	C605
Warning	Image size larger than the image box size	B604
Success		0000

3.5.2.1.3.5 Presentation LUT SOP Class

The objective of the Presentation LUT is to realize image hardcopy printing tailored for specific modalities, applications, and user preferences.

The output of the Presentation LUT consists of Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

Table 45: Attributes of the N_CREATE_RQ on the Presentation LUT SOP Class

Attribute name	Tag	Usage SCU	Supported Values
Presentation LUT Shape	(2050,0020)	U	IDENTITY

The affected SOP Instance UID received with the N-CREATE-RSP message is stored internally and used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ). Refer to the table below:

Table 46: Attributes of the N_DELETE_RQ on the Presentation LUT SOP Class

Attribute name	Tag	Source of information
Requested SOP Instance UID	(0000,1000) -> (0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Presentation LUT

The Presentation LUT SOP class interprets the following status codes:

Table 47: Presentation LUT SOP status

Service Status	Meaning	Protocol Codes
Warning	Requested Min Density or Max Density outside the HCD's operating range. HCD uses its minimum or maximum density value instead.	B605
Success	Presentation LUT was successfully created	0000

3.5.2.1.3.6 Printer SOP Class

The Printer SOP Class provides the possibility to monitor the status of the hard-copy printer in a synchronous and an asynchronous way.

The SCU uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way.

It can directly ask the Printer (SCP) for its status or can receive Events from the Print SCP asynchronously:

- N_GET as SCU
- N_EVENT_REPORT as SCU

In both cases, the following information is supported:

Table 48: Used Printer N-EVENT report

Event type name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

Table 49: Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

Attribute name	Tag	Usage SCP	Supported values
Printer Status	(2110,0010)	M	NORMAL FAILURE WARNING
Printer Status Info	(2110,0020)	M	See 3.5.2.1.3.8 DICOM Print SCU - detailed status displays on page 112

For a detailed description of how Somaris/7 reacts to the various messages, please refer to 3.5.2.1.3.8 DICOM Print SCU - detailed status displays on page 112.

3.5.2.1.3.7 Print Job SOP Class

The Print Job SOP Class provides the possibility to monitor the execution of the print process.

The Somaris/7 DICOM Print application supports the optional N-EVENT-REPORT DIMSE service to receive the changes of the print job status in an asynchronous way.

It can receive events from the Print SCP asynchronously:

- N-EVENT-REPORT

Note

Somaris/7 does not support receiving N-EVENT from the camera during print sessions; normally this is configurable in the camera.

The following information is supported:

Table 50: Used Print Job N-EVENT report

Event type name	Event	Attributes	Tag	Usage SCU
Pending	1	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
Printing	2	Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
Done	3	Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
		Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
Failure	4	Printer Name	(2110,0030)	U
		Print Job ID	(2100,0010)	- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U

For a detailed description of how Somaris/7 reacts to the various messages, please refer to 3.5.2.1.3.8 DICOM Print SCU - detailed status displays on page 112.

3.5.2.1.3.8 DICOM Print SCU - detailed status displays

The following tables document the behavior of the Somaris/7 DICOM Print AE in response to messages received for the printer SOP class and the print job SOP class.

Definitions of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed
- Interact: The user has to react in the near future, but not immediately.
Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by N-EVENT-REPORT.
- Queue Stopped: The user has to react immediately. Either the camera needs immediate interaction or a job has been aborted.
Example: A camera is out of 8x10 clear sheets, or is down, or a film job has been aborted.

Note

Different camera symbols are displayed according to the Printer Status Info.

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visi- ble in the Status Bar	Other action for UI/ camera symbol
NORMAL	Camera is ready.	Camera is ready.	<None>/idle
BAD RECEIVE MGZ	There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine.	Problem with receive magazine.	<None>/interact
BAD SUPPLY MGZ	There is a problem with a film supply magazine. Films from this magazine cannot be transported into the printer.	Problem with supply magazine.	<None>/interact
CALIBRATING	The printer is self-calibrating and is expected to be available for normal operation shortly.	Self calibration. Please wait.	<None>/idle
CALIBRATION ERR	An error in the printer calibration has been detected; the quality of processed films may not be optimal.	Problem in calibration. Film quality may not be optimal.	<None>/interact
CHECK CHEMIS- TRY	A problem with the processor chemicals has been detected; the quality of processed films may not be optimal.	Problem with chemis-try. Film quality may not be optimal.	<None>/interact
CHECK SORTER	There is an error in the film sorter.	Error in film sorter.	<None>/interact
CHEMICALS EMPTY	There are no processing chemi-cals in the processor; films will not be printed and processed until the processor is back to normal.	Camera chemistry empty. Please check.	<None>/interact
CHEMICALS LOW	The chemical level in the proces-sor is low; if not corrected, it will probably shut down soon.	Camera chemistry low. Please check.	<None>/interact
COVER OPEN	One or more printer or processor covers, drawers, doors are open.	Camera cover, drawer or door open.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
ELEC CONFIG ERR	Printer configured improperly for this job.	Camera configured improperly for this job. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
ELEC DOWN	Printer is not operating due to some unspecified electrical hardware problem.	Camera electrical hardware problem.	<None>/interact
ELEC SW ERROR	Printer is not operating due to some unspecified software error.	Camera software problem. Queue stopped.	Queue for this camera will be STOPPED/ queue stopped
EMPTY 8x10	The 8x10 inch film supply magazine is empty.	8x10 film supply empty.	<None>/interact
EMPTY 8x10 BLUE	The 8x10 inch blue film supply magazine is empty.	8x10 blue film supply empty.	<None>/interact
EMPTY 8x10 CLR	The 8x10 inch clear film supply magazine is empty.	8x10 clear film supply empty.	<None>/interact
EMPTY 8x10 PAPR	The 8x10 inch paper supply magazine is empty.	8x10 paper supply empty.	<None>/interact
EMPTY 10x12	The 10x12 inch film supply magazine is empty.	10x12 film supply empty.	<None>/interact
EMPTY 10x12 BLUE	The 10x12 inch blue film supply magazine is empty.	10x12 blue film supply empty.	<None>/interact
EMPTY 10x12 CLR	The 10x12 inch clear film supply magazine is empty.	10x12 clear film supply empty.	<None>/interact
EMPTY 10x12 PAPR	The 10x12 inch paper supply magazine is empty.	10x12 paper supply empty.	<None>/interact
EMPTY 10x14	The 10x14 inch film supply magazine is empty.	10x14 film supply empty.	<None>/interact
EMPTY 10x14 BLUE	The 10x14 inch blue film supply magazine is empty.	10x14 blue film supply empty.	<None>/interact
EMPTY 10x14 CLR	The 10x14 inch clear film supply magazine is empty.	10x14 clear film supply empty.	<None>/interact
EMPTY 10x14 PAPR	The 10x14 inch paper supply magazine is empty.	10x14 paper supply empty.	<None>/interact
EMPTY 11x14	The 11x14 inch film supply magazine is empty.	11x14 film supply empty.	<None>/interact
EMPTY 11x14 BLUE	The 11x14 inch blue film supply magazine is empty.	11x14 blue film supply empty.	<None>/interact
EMPTY 11x14 CLR	The 11x14 inch clear film supply magazine is empty.	11x14 clear film supply empty.	<None>/interact
EMPTY 11x14 PAPR	The 11x14 inch paper supply magazine is empty.	11x14 paper supply empty.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
EMPTY 14x14	The 14x14 inch film supply magazine is empty.	14x14 film supply empty.	<None>/interact
EMPTY 14x14 BLUE	The 14x14 inch blue film supply magazine is empty.	14x14 blue film supply empty.	<None>/interact
EMPTY 14x14 CLR	The 14x14 inch clear film supply magazine is empty.	14x14 clear film supply empty.	<None>/interact
EMPTY 14x14 PAPR	The 14x14 inch paper supply magazine is empty.	14x14 paper supply empty.	<None>/interact
EMPTY 14x17	The 14x17 inch film supply magazine is empty.	14x17 film supply empty.	<None>/interact
EMPTY 14x17 BLUE	The 14x17 inch blue film supply magazine is empty.	14x17 blue film supply empty.	<None>/interact
EMPTY 14x17 CLR	The 14x17 inch clear film supply magazine is empty.	14x17 clear film supply empty.	<None>/interact
EMPTY 14x17 PAPR	The 14x17 inch paper supply magazine is empty.	14x17 paper supply empty.	<None>/interact
EMPTY 24x24	The 24x24 inch film supply magazine is empty.	24x24 film supply empty.	<None>/interact
EMPTY 24x24 BLUE	The 24x24 inch blue film supply magazine is empty.	24x24 blue film supply empty.	<None>/interact
EMPTY 24x24 CLR	The 24x24 inch clear film supply magazine is empty.	24x24 clear film supply empty.	<None>/interact
EMPTY 24x24 PAPR	The 24x24 inch paper supply magazine is empty.	24x24 paper supply empty.	<None>/interact
EMPTY 24x30	The 24x30 inch film supply magazine is empty.	24x30 film supply empty.	<None>/interact
EMPTY 24x30 BLUE	The 24x30 inch blue film supply magazine is empty.	24x30 blue film supply empty.	<None>/interact
EMPTY 24x30 CLR	The 24x30 inch clear film supply magazine is empty.	24x30 clear film supply empty.	<None>/interact
EMPTY 24x30 PAPR	The 24x30 inch paper supply magazine is empty.	24x30 paper supply empty.	<None>/interact
EMPTY A4 PAPR	The A4 paper supply magazine is empty.	A4 paper supply empty.	<None>/interact
EMPTY A4 TRANS	The A4 transparency supply magazine is empty.	A4 transparency supply empty.	<None>/interact
EXPOSURE FAILURE	The exposure device has failed due to some unspecified reason.	Exposure device has failed.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visi- ble in the Status Bar	Other action for UI/ camera symbol
FILM JAM	A film transport error has occurred and a film is jammed in the printer or processor.	Film jam.	<None>/interact
FILM TRANSP ERR	There is a malfunction with the film transport; there may or may not be a film jam.	Film transport problem.	<None>/interact
FINISHER EMPTY	The finisher is empty.	Finisher is empty.	<None>/interact
FINISHER ERROR	The finisher is not operating due to some unspecified reason.	Finisher problem.	<None>/interact
FINISHER LOW	The finisher is low on supplies	Finisher low.	<None>/interact
LOW 8x10	The 8x10 inch film supply magazine is low.	8x10 film supply low.	<None>/interact
LOW 8x10 BLUE	The 8x10 inch blue film supply magazine is low.	8x10 blue film supply low.	<None>/interact
LOW 8x10 CLR	The 8x10 inch clear film supply magazine is low.	8x10 clear film supply low.	<None>/interact
LOW 8x10 PAPR	The 8x10 inch paper supply magazine is low.	8x10 paper supply low.	<None>/interact
LOW 10x12	The 10x12 inch film supply magazine is low.	10x12 film supply low.	<None>/interact
LOW 10x12 BLUE	The 10x12 inch blue film supply magazine is low.	10x12 blue film supply low.	<None>/interact
LOW 10x12 CLR	The 10x12 inch clear film supply magazine is low.	10x12 clear film supply low.	<None>/interact
LOW 10x12 PAPR	The 10x12 inch paper supply magazine is low.	10x12 paper supply low.	<None>/interact
LOW 10x14	The 10x14 inch film supply magazine is low.	10x14 film supply low.	<None>/interact
LOW 10x14 BLUE	The 10x14 inch blue film supply magazine is low.	10x14 blue film supply low.	<None>/interact
LOW 10x14 CLR	The 10x14 inch clear film supply magazine is low.	10x14 clear film supply low.	<None>/interact
LOW 10x14 PAPR	The 10x14 inch paper supply magazine is low.	10x14 paper supply low.	<None>/interact
LOW 11x14	The 11x14 inch film supply magazine is low.	11x14 film supply low.	<None>/interact
LOW 11x14 BLUE	The 11x14 inch blue film supply magazine is low.	11x14 blue film supply low.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
LOW 11x14 CLR	The 11x14 inch clear film supply magazine is low.	11x14 clear film supply low.	<None>/interact
LOW 11x14 PAPR	The 11x14 inch paper supply magazine is low.	11x14 paper supply low.	<None>/interact
LOW 14x14	The 14x14 inch film supply magazine is low.	14x14 film supply low.	<None>/interact
LOW 14x14 BLUE	The 14x14 inch blue film supply magazine is low.	14x14 blue film supply low.	<None>/interact
LOW 14x14 CLR	The 14x14 inch clear film supply magazine is low.	14x14 clear film supply low.	<None>/interact
LOW 14x14 PAPR	The 14x14 inch paper supply magazine is low.	14x14 paper supply low.	<None>/interact
LOW 14x17	The 14x17 inch film supply magazine is low.	14x17 film supply low.	<None>/interact
LOW 14x17 BLUE	The 14x17 inch blue film supply magazine is low.	14x17 blue film supply low.	<None>/interact
LOW 14x17 CLR	The 14x17 inch clear film supply magazine is low.	14x17 clear film supply low.	<None>/interact
LOW 14x17 PAPR	The 14x17 inch paper supply magazine is low.	14x17 paper supply low.	<None>/interact
LOW 24x24	The 24x24 inch film supply magazine is low.	24x24 film supply low.	<None>/interact
LOW 24x24 BLUE	The 24x24 inch blue film supply magazine is low.	24x24 blue film supply low.	<None>/interact
LOW 24x24 CLR	The 24x24 inch clear film supply magazine is low.	24x24 clear film supply low.	<None>/interact
LOW 24x24 PAPR	The 24x24 inch paper supply magazine is low.	24x24 paper supply low.	<None>/interact
LOW 24x30	The 24x30 inch film supply magazine is low.	24x30 film supply low.	<None>/interact
LOW 24x30 BLUE	The 24x30 inch blue film supply magazine is low.	24x30 blue film supply low.	<None>/interact
LOW 24x30 CLR	The 24x30 inch clear film supply magazine is low.	24x30 clear film supply low.	<None>/interact
LOW 24x30 PAPR	The 24x30 inch paper supply magazine is low.	24x30 paper supply low.	<None>/interact
LOW A4 PAPR	The A4 paper supply magazine is low.	A4 paper supply low.	<None>/interact
LOW A4 TRANS	The A4 transparency supply magazine is low.	A4 transparency supply low.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
NO RECEIVE MGZ	The film receive magazine is not available.	Film receiver not available.	<None>/interact
NO RIBBON	The ribbon cartridge needs to be replaced.	Replace ribbon cartridge.	<None>/interact
NO SUPPLY MGZ	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
CHECK PRINTER	The printer is not ready at this time; operator intervention is required to make the printer available.	Check camera.	<None>/interact
CHECK PROC	The processor is not ready at this time; operator intervention is required to make the printer available.	Check processor.	<None>/interact
PRINTER DOWN	The printer is not operating due to some unspecified reason.	Camera down.	<None>/interact
PRINTER INIT	The printer is not ready at this time; it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Camera initializing.	<None>/idle
PRINTER OFFLINE	The printer has been disabled by an operator or service person.	Camera off-line.	<None>/interact
PROC DOWN	The processor is not operating due to some unspecified reason.	Processor down.	<None>/interact
PROC INIT	The processor is not ready at this time; it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Processor initializing.	<None>/idle
PROC OVERFLOW FL	Processor chemicals are approaching the overflow full mark.	Processor chemicals overflow.	<None>/interact
PROC OVERFLOW HI	Processor chemicals have reached the overflow full mark.	Processor chemicals near overflow.	<None>/interact
QUEUED	Print job in Queue	-	<None>/idle
RECEIVER FULL	The Film receive magazine is full.	Receiver full.	<None>/interact
REQ MED NOT INST	The requested film, paper, or other media supply magazine is installed in the printer, but may be available with operator intervention.	Install media supply.	<None>/interact

Table 51: Printer Status Infos in the Printer SOP Class/Execution Status Infos in the Print Job SOP Class

Printer Status info/ Execution Status info	Description	Message string visible in the Status Bar	Other action for UI/ camera symbol
REQ MED NOT AVAI	The requested film, paper, or other media requested are not available on this printer.	Media supply not available on this camera. Queue stopped. Change camera.	Queue for this camera will be STOPPED/ queue stopped
RIBBON ERROR	There is an unspecified problem with the print ribbon.	Error with print ribbon.	<None>/interact
SUPPLY EMPTY	The printer is out of film.	Camera out of film.	<None>/interact
SUPPLY LOW	The film supply is low.	Film supply low.	<None>/interact
UNKNOWN	There is an unspecified problem.	Unspecified problem with camera.	<None>/interact

Table 52: Printer Status Infos: Additional Agfa printer status infos

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
WARMING UP	Printer is in the warm-up stage. Spooling of print jobs to disk is still possible.	Camera is warming up.	<None>idle
OFFLINE	Printer is switched off-line. Spooling of print jobs to disk is still possible.	Camera is switched off-line.	<None>/interact
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	-	<None>/idle

Table 53: Printer Status Infos: Additional Kodak infos for Pacs Link (formerly Imation cameras)

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
SUPPLY MGZ ERR	The supply magazine has an error.	Film supply has an error.	<None>/interact

Table 54: Printer Status Infos: Additional Kodak infos for Kodak 190

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
PRINTER STOPPED	The printer has stopped.	Camera has stopped.	<None>/interact
FATAL ERROR	Fatal error.	Fatal error. Queue stopped.	Queue for this camera will be STOPPED/ queue stopped

Table 55: Printer Status Infos: Additional Kodak infos for 2180/1120

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
PRINTER NOT RDY	Printer not ready.	Camera not ready.	<None>/interact
CHECK PROCESSOR	Check processor.	Check processor.	<None>/interact
NO TONER	No toner.	No toner.	<None>/interact
FATAL	Fatal error.	Fatal error. Queue stopped.	Queue for this camera will be STOPPED/ queue stopped

Table 56: Printer Status Infos: Additional Codonics infos

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
STANDARD	Printer is ready.	Camera is ready.	<None>/Normal
LOAD A-SIZE	Load A-size media.	Load A-size media.	<None>/interact
LOAD A-DVPAPER	Load A-size black and white paper.	Load A-size black and white paper.	<None>/interact
LOAD A-CVPAPER	Load A-size color paper.	Load A-size color paper.	<None>/interact
LOAD A-CVTRANS	Load A-size transparencies.	Load A-size transparencies.	<None>/interact
LOAD A4-SIZE	Load A4-size media.	Load A4-size media.	<None>/interact
LOAD A4-DVPAPER	Load A4-size black and white paper.	Load A4-size black and white paper.	<None>/interact
LOAD A4-CVPAPER	Load A4-size color paper.	Load A4-size color paper.	<None>/interact
LOAD A4-CVTRANS	Load A4-size transparencies.	Load A4-size transparencies.	<None>/interact
LOAD LA-SIZE	Load LA-size media.	Load LA-size media.	<None>/interact
LOAD LA-DVPAPER	Load LA-size black and white paper.	Load LA-size black and white paper.	<None>/interact
LOAD LA-CVPAPER	Load LA-size color paper.	Load LA-size color paper.	<None>/interact
LOAD LA-CVTRANS	Load LA-size transparencies.	Load LA-size transparencies.	<None>/interact
LOAD LA4-SIZE	Load LA4-size media.	Load LA4-size media.	<None>/interact
LOAD LA4-DVPA-PER	Load LA4-size black and white paper.	Load LA4-size black and white paper.	<None>/interact
LOAD LA4-CVPA-PER	Load LA4-size color paper.	Load LA4-size color paper.	<None>/interact

Table 56: Printer Status Infos: Additional Codonics infos

Printer Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
LOAD LA4-CVTRANS	Load LA4-size transparencies.	Load LA4-size transparencies.	<None>/interact
LOAD XLA-SIZE	Load XLA-size media.	Load XLA-size media.	<None>/interact
LOAD XLA-DVPA-PER	Load XLA-size black and white paper.	Load XLA-size black and white paper.	<None>/interact
LOAD XLA-CVPA-PER	Load XLA-size color paper.	Load XLA-size color paper.	<None>/interact
LOAD XLA-CVTRANS	Load XLA-size transparencies.	Load XLA-size transparencies.	<None>/interact
LOAD XLA4-SIZE	Load XLA4-size media.	Load XLA4-size media.	<None>/interact
LOAD XLA4-DVPAPE	Load XLA4-size black and white paper.	Load XLA4-size black and white paper.	<None>/interact
LOAD XLA4-CVPAPE	Load XLA4-size color paper.	Load XLA4-size color paper.	<None>/interact
LOAD XLA4-CVT-RAN	Load XLA4-size transparencies.	Load XLA4-size transparencies.	<None>/interact
LOAD XLW-SIZE	Load XLW-size media.	Load XLW-size media.	<None>/interact
LOAD XLW-DVPA-PER	Load XLW-size black and white paper.	Load XLW-size black and white paper.	<None>/interact
LOAD XLW-CVPA-PER	Load XLW-size color paper.	Load XLW-size color paper.	<None>/interact
LOAD 8X10-SIZE	Load 8x10 media.	Load 8x10 media.	<None>/interact
LOAD 8X10-DVFILM	Load 8x10 black and white film.	Load 8x10 black and white film.	<None>/interact
SUPPLY MISSING	The film supply magazine specified for this job is not available.	Film supply not available.	<None>/interact
RIBBON MISSING	Ribbon is missing.	Ribbon is missing.	<None>/interact
RIBBON EMPTY	Ribbon is empty.	Ribbon is empty.	<None>/interact
TOP COVER OPEN	Top cover of printer is open.	Top cover of camera is open.	<None>/interact

Table 57: Additional DICOM Execution Status Information - evaluation

Execution Status info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
INVALID PAGE DES	The specified page layout cannot be printed or other page description errors have been detected.	Film Job cannot be printed on this camera. Queue stopped. Please redirect film job.	Queue for this camera will be STOPPED/ Queue stopped
INSUFFICIENT MEMORY	There is not enough memory available to complete this job.	Not enough memory available in camera. Queue stopped. Please continue queue or change camera.	Queue for this camera will be STOPPED/ Queue stopped
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	-	<None>/idle

Additional DICOM Execution Status Information

Printer Status Info and Execution Status Info are defined terms and can therefore be extended or reduced by camera manufacturers. In this way, *syngo* remains flexible.

If any other printer status info or execution status info is received, *syngo* will react as shown in the following table:

Printer Status / Execution	Printer/Execution Status Info	Description	Message string visible in the Status Bar	Other action for syngo/camera symbol
WARNING	<any other>	<not defined status info>	Camera info: <status info>	<None>/interact
FAILURE	<any other>	<not defined status info>	Camera info: <status info> Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped

3.6 Modality Worklist AE Specification

The Modality Worklist SCU (patient registration in conjunction with the network application) requests that the remote SCP matches all keys specified in the query against the information in its worklist database.

The SIEMENS Somaris/7 DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

Table 58: SOP Classes as an SCU

SOP Class Name	SOP Class UID
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31

3.6.1 Association Establishment Policies

3.6.1.1 General

It is possible to configure a cyclic update of the modality scheduler database through a background worklist request with date/time and modality information.

In addition, you can request a worklist update with "Update Worklist". No duplicate entries are added in the Scheduler DB. Entries are uniquely identified by the Study Instance UID (0020,000D) for the Requested Procedure and the SPS ID (0040,0009) in the SPS Sequence (0040,0100).

An interactive worklist query can be issued with search criteria entered in the patient-based Query dialog from the patient browser.

The default PDU size used is of 32 kB.

3.6.1.2 Number of Associations

The Somaris/7 DICOM application initiates one association at a time to query worklist entry data.

3.6.1.3 Asynchronous Nature

The Somaris/7 DICOM implementation does not support asynchronous communication (multiple outstanding transactions over a single association).

3.6.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.6.2 Association Initiation Policy

The network application (if configured) queries the worklist periodically or by user request. Ever then it establishes an association by using the DICOM association services. During association establishment, the negotiation of SOP classes to exchange the capabilities of the SCU and the SCP is not supported.

The following DIMSE-C operation is supported as an SCU:

- C-FIND

3.6.2.1 Real-World Activity

3.6.2.1.1 Associated Real-World Activity - Query (Update) Worklist

A network application performs worklist queries with the C-FIND request at regular intervals. In addition, it can be triggered by immediate request. The received worklist items are compared with the contents of the local scheduler database. New items are inserted into the scheduler database.

After each broad query, all RP/SPS that were cancelled or rescheduled to another modality at the RIS will be automatically removed from the scheduler DB, if the following applies:

1. The Examination of this procedure has not been started or finished yet.
2. The corresponding configuration item "Automatic removal of cancelled/rescheduled Request" was checked in the Service UI under the DICOM/HIS/RIS Node.

No automatic clean-up of the scheduler DB is performed after a Patient-based Query, since the worklist received does not give the complete list of all currently scheduled procedures for the modality.

3.6.2.1.2 Proposed Presentation Contexts - Query (Update) Worklist

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 59: Proposed presentation contexts

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Modality Worklist Information Model- FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

3.6.2.1.3 SOP-Specific Conformance Statement - Update Worklist

3.6.2.1.3.1 Search Key Attributes of the Worklist C-FIND

The Somaris/7 DICOM worklist SCU supports "broad worklist queries" with all the required search keys.

The following tables describe the "broad query" search keys that the SCU supports. A broad query is a query for all tasks scheduled for the SCU's own modality or own modality application entity defined with the following search keys:

Table 60: Search Key Attributes in a broad worklist query

Attribute name ^a	Tag	Matching Key Type	query value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	
>Scheduled Station AE Title	(0040,0001)	R	Configurable ^b : own AET or "*"
>Scheduled Procedure Step Start Date	(0040,0002)	R	Configurable ^c : <act. Date>-<act Date> or range from UI
>Scheduled Procedure Step Start Time	(0040,0003)	R	Configurable ^c : <zero length> or range from UI
>Modality	(0008,0060)	R	Configurable ^b : own modality or "*"

^a No other attributes of the Register Dialog used for C-FIND

^b It depends on the users' configuration (Options -> Configuration -> Patient Registration) whether their "own AET" is provided or not. Use the HIS/RIS tabcard for configuration.

^c It depends on the user configuration (Options -> Configuration -> Patient Registration) if the actual date with a full time range or an interactive input dialog for date/time specification is used (<start-Date>-<endDate>).

Note

Since various SCP implementations depend on the Specific Character Set attribute to be sent with C-FIND in order to deliver the attribute filled with C-FIND-RSP (see below), as a default the attribute will be sent even if it is empty. In case this turns out to be a problem for a specific SCP, this can be configured in cooperation with Siemens so as not to include this attribute.

3.6.2.1.3.2 Return Key Attributes of the Worklist C-FIND-RSP

The Somaris/7 DICOM worklist SCU supports worklist queries with return key attributes of all types. The following tables describe the return keys that the SCU supports.

An "x" in the UI column indicates that the attribute is visualized when browsing the Worklist results with the Patient Browser and/or during Patient Registration. The Patient Browser display is additionally influenced by the related Browser configuration.

A tag in the IOD column indicates that the related attribute is included in the SOP Instances of the IODs created during processing of this worklist request.

A tag in the MPPS column indicates that the related attribute is included in the SOP Instances of the MPPS objects created during processing of this worklist request. See also the tables *Table 66: Performed Procedure Step N-CREATE Attributes* on page 137 and *Table 68: Performed Procedure Step N-SET Attributes* on page 141.

Table 61: Basic Worklist C_FIND_RSP Return Key Attributes

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
SOP Common					
Specific Character Set ^a	(0008,0005)	1C	-	(0008,0005)	(0008,0005)
Scheduled Procedure Step					
Scheduled Procedure Step Sequence	(0040,0100)	1			
>Modality	(0008,0060)	1	x	(0008,0060)	(0008,0060)
>Requested Contrast Agent	(0032,1070)	2C	x	(0032,1070)	
>Scheduled Station AE Title	(0040,0001)	1	x		(0040,0241) ^b
>Scheduled Procedure Step Start Date	(0040,0002)	1	x		
>Scheduled Procedure Step Start Time	(0040,0003)	1	x		
>Scheduled Procedure Step End Date	(0040,0004)	3	-		
>Scheduled Procedure Step End Time	(0040,0005)	3	-		
>Scheduled Performing Physician's Name	(0040,0006)	1	x	(0008,1050)	(0008,1050) ^c
>Scheduled Procedure Step Description ^d	(0040,0007)	1C	x	(0040,0007) (0040,0254)	(0040,0007) (0040,0254)
>Scheduled Protocol Code Sequence ^e	(0040,0008)	1C	-	(0040,0008) (0040,0260) ^f	(0040,0008) (0040,0260) ^f
>>Code Value	(0008,0100)	1C	x		
>>Coding Scheme Designator	(0008,0102)	1C	x		
>>Coding Scheme Version	(0008,0103)	3	x		
>>Code Meaning	(0008,0104)	3	x		
>Scheduled Procedure Step ID ^g	(0040,0009)	1	x	(0040,0009) (0040,0253)	(0040,0009) (0040,0253)
>Scheduled Station Name	(0040,0010)	2	x		

^a. The Specific Character Set distributed via the Modality Worklist by the hospital network reflects the global hospital context, for example a hospital with a German context shall not restrict the worklist entries to ISO_IR 6 but will supply a character set adequate for holding all German language text input.

^b. "Scheduled Station AE Title" is taken as the default for "Performed Station AE Title"

^c. "Scheduled Performing Physician's Name" is taken as the default for "Performing Physician's Name"

^d. "Scheduled Procedure Step Description" is taken as the default for "Performed Procedure Step Description"

^e. Uses universal sequence match

^f. "Scheduled Protocol Code Sequence" is taken as the default for "Performed Protocol Code Sequence"

^g. "Scheduled Procedure Step ID" is taken as the default for "Performed Procedure Step ID"

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
>Scheduled Procedure Step Location	(0040,0011)	2	x		(0040,0242) ^a
>Pre-Medication	(0040,0012)	2C	x		
>Scheduled Procedure Step Status	(0040,0020)	3	x		
>Comments on the Scheduled Procedure Step	(0040,0400)	3	-		
Requested Procedure					
Referenced Study Sequence ^b	(0008,1110)	2	-	(0008,1110)	(0008,1110)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Study Instance UID	(0020,000D)	1	-	(0020,000D)	(0020,000D)
Requested Procedure Description	(0032,1060)	1C	x	(0032,1060)	(0032,1060)
Requested Procedure Code Sequence ^b	(0032,1064)	1C	-	(0032,1032) ^c (0032,1064)	(0032,1032) ^c
>Code Value	(0008,0100)	1C	x		
>Code Scheme Designator	(0008,0102)	1C	x		
>Code Scheme Version	(0008,0103)	3	x		
>Code Meaning	(0008,0104)	3	x		
Requested Procedure ID	(0040,1001)	1	x	(0040,1001) (0020,0010) ^d	(0040,1001) (0020,0010) ^d
Reason for the Requested Procedure	(0040,1002)	3	-		
Requested Procedure Priority	(0040,1003)	2	x		
Patient Transport Arrangements	(0040,1004)	2	-		
Requested Procedure Location	(0040,1005)	3	-		
Confidentiality Code	(0040,1008)	3	-		
Reporting Priority	(0040,1009)	3	-		
Names of Intended Recipients of results	(0040,1010)	3	-	(0008,1048)	
Requested Procedure Comments	(0040,1400)	3	x		

^a. "Scheduled Procedure Step Location" is taken as the default for "Performed Procedure Step Location"

^b. Uses universal sequence match

^c. "Requested Procedure Code Sequence" is taken as the default for "Procedure Code Sequence"

^d. "Requested Procedure ID" is taken as the default for "Study ID"

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Reason for the Requested Procedure Code Sequence	(0040,100A)	3	-		
Imaging Service Request					
Accession Number	(0008,0050)	2	x	(0008,0050)	(0008,0050)
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Requesting Physician	(0032,1032)	2	x	(0032,1032)	(0032,1032)
Requesting Service	(0032,1033)	3	x	(0032,1033)	
Reason for the Imaging Service Request	(0040,2001)	3	-		
Issuing Date of Imaging Service Request	(0040,2004)	3	-		
Issuing Time of Imaging Service Request	(0040,2005)	3	-		
Placer Order Number / Imaging Service Request ^a	(0040,2016)	3	-		(0040,2016)
Filler Order Number / Imaging Service Request ^b	(0040,2017)	3	-		(0040,2017)
Order entered by...	(0040,2008)	3	-		
Order Enterer's Location	(0040,2009)	3	-		
Order Callback Phone Number	(0040,2010)	3	-		
Imaging Service Request Comments	(0040,2400)	3	x		
Visit Identification					
Institution Name	(0008,0080)	3	x	(0008,0080)	
Institution Address	(0008,0081)	3	-	(0008,0081)	
Institution Code Sequence ^c	(0008,0082)	3	-		
>Code Value	(0008,0100)	1C			
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Admission ID	(0038,0010)	2	x		
Issuer of Admission ID	(0038,0011)	3	-		

^a. Old tag (0040,2006) is retired and not used

^b. Old tag (0040,2007) is retired and not used

^c. Uses universal sequence match

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Visit Status					
Visit Status ID	(0038,0008)	3	-		
Current Patient Location	(0038,0300)	2	x		
Patient's Institution Residence	(0038,0400)	3	-		
Visit Comments	(0038,4000)	3	-		
Visit Relationship					
Referenced Study Sequence ^a	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Sequence ^a	(0008,1120)	2	-		(0008,1120)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Visit Admission					
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Referring Physician's Address	(0008,0092)	3	-		
Referring Physician's Phone Numbers	(0008,0094)	3	-		
Admitting Diagnoses Description	(0008,1080)	3	x	(0008,1080)	
Admitting Diagnosis Code Sequence ^a	(0008,1084)	3			
>Code Value	(0008,0100)	1C			
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Route of Admissions	(0038,0016)	3	-		
Admitting Date	(0038,0020)	3	-		
Admitting Time	(0038,0021)	3	-		

^a. Uses universal sequence match

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Patient Identification					
Patient's Name	(0010,0010)	1	x	(0010,0010)	(0010,0010)
Patient ID	(0010,0020)	1	x	(0010,0020)	(0010,0020)
Issuer of Patient ID	(0010,0021)	3	-	(0010,0021)	
Other Patient IDs	(0010,1000)	3	x	(0010,1000)	
Other Patient IDs Sequence	(0010,1002)	3	x	(0010,1002)	
>Patient ID	(0010,0020)	3	x	(0010,0020)	
>Issuer of Patient ID	(0010,0021)	3	x	(0010,0021)	
>Type of Patient ID	(0010,0022)	3	x	(0010,0022)	
Other Patient Names	(0010,1001)	3	x	(0010,1001)	
Patient's Birth Name	(0010,1005)	3	-	(0010,1005)	
Patient's Mother's Birth Name	(0010,1060)	3	-	(0010,1060)	
Medical Record Locator	(0010,1090)	3	-	(0010,1090)	
Patient Demographic					
Patients Birth Date	(0010,0030)	2	x	(0010,0030)	(0010,0030)
Patients Birth Time	(0010,0032)	3	-	(0010,0032)	
Patient's Sex	(0010,0040)	2	x	(0010,0040)	(0010,0040)
Patient's Insurance Plan Code Sequence ^a	(0010,1050)	3	-	(0010,1050)	
>Code Value	(0008,0100)	1C			
>Code Scheme Designator	(0008,0102)	1C			
>Code Scheme Version	(0008,0103)	3			
>Code Meaning	(0008,0104)	3			
Patient's Age	(0010,1010)	3	x	(0010,1010)	
Patient's Size	(0010,1020)	3	x	(0010,1020)	
Patient's Weight	(0010,1030)	2	x	(0010,1030)	
Patient's Address	(0010,1040)	3	x	(0010,1040)	
Military Rank	(0010,1080)	3	x	(0010,1080)	
Branch of Service	(0010,1081)	3	-	(0010,1081)	
Country of Residence	(0010,2150)	3	-	(0010,2150)	
Region of Residence	(0010,2152)	3	-	(0010,2152)	
Patient's Telephone Numbers	(0010,2154)	3	-	(0010,2154)	
Ethnic Group	(0010,2160)	3	x	(0010,2160)	
Occupation	(0010,2180)	3	-	(0010,2180)	

^a. Uses universal sequence match

Attribute name	Tag	Return Key Type	UI	IOD	MPPS
Patient's Religious Preference	(0010,21F0)	3	-	(0010,21F0)	
Patient Comments	(0010,4000)	3	x	(0010,4000)	
Patient Data Confidentiality Constraint Description	(0040,3001)	2	x	(0040,3001)	
Patient Medical					
Medical Alerts	(0010,2000)	2	x	(0010,2000)	
Contrast Allergies	(0010,2110)	2	x	(0010,2110)	
Pregnancy Status	(0010,21C0)	2	x	(0010,21C0)	
Smoking Status	(0010,21A0)	3	x	(0010,21A0)	
Last Menstrual Date	(0010,21D0)	3	x	(0010,21D0)	
Additional Patient History	(0010,21B0)	3	x	(0010,21B0)	
Special Needs	(0038,0050)	2	x	(0038,0050)	
Patient State	(0038,0500)	2	x	(0038,0500)	
Patient Relationship					
Referenced Study Sequence ^a	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Visit Sequence ^a	(0008,1125)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Alias Sequence ^a	(0038,0004)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		

^a Uses universal sequence match

3.6.2.1.4 Associated Real-World Activity - Get Worklist

Using "Get Worklist" in the patient-based Worklist Query dialog, the entered attributes are used to form a worklist request identifier. The Patient Registration dialog is updated with the response data to perform an examination in advance. The response data is additionally placed in the scheduler database.

3.6.2.1.5 Proposed Presentation Contexts - Get Worklist

The same Presentation contexts are proposed as with "Update Worklist". Refer to table *Table 59: Proposed presentation contexts* on page 124.

3.6.2.1.6 SOP-Specific Conformance - Get Worklist

3.6.2.1.6.1 Search Key Attributes of the Worklist C-FIND

The Somaris/7 DICOM worklist SCU supports "narrow worklist queries" with all the required search keys.

The following table describes the search keys that the SCU supports for a patient based worklist query, which is defined by the following search keys:

Table 62: Search Key Attributes in a patient-based worklist query

Attribute name	Tag	Matching Key Type	Query value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	
>Scheduled Performing Physician's Name	(0040,0006)	R	inserted in UI or zero length
Requested Procedure			
Requested Procedure ID	(0040,1001)	O	inserted in UI or zero length
Imaging Service Request			
Accession Number	(0008,0050)	O	inserted in UI or zero length
Referring Physician's Name	(0008,0090)	O	inserted in UI or zero length
Visit Status			
Current Patient Location	(0038,0300)	O	inserted in UI or zero length
Patient Identification			
Patient's Name ^a	(0010,0010)	R	inserted in UI or zero length
Patient ID	(0010,0020)	R	inserted in UI or zero length

^a Please be aware that, although in the UI there are different entries for First Name and Last Name of a patient, these are combined into one query attribute. Querying just for the Last Name (without wildcards) or not providing a first letter for the First Name may prevent expected matches.

3.6.2.1.6.2 Return Key Attributes used from the Worklist C-FIND-RSP

Refer to *Table 61: Basic Worklist C_FIND_RSP Return Key Attributes* on page 127.

3.6.2.1.6.3 Status Codes of the Worklist C-FIND

The worklist SCU interprets the following status codes:

Table 63: C-FIND Response Status

Service Status	Meaning	Status Codes (0000,0900)	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match the SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - the Current Match is supplied and any Optional Keys are supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

3.7 Modality Performed Procedure Step AE Specification

The Modality Performed Procedure Step SCU (Patient Registration and MPPS UI) provides information about a performed real-world Procedure to a remote SCP (Information System).

The SIEMENS Somaris/7 DICOM implementation provides Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

Table 64: SOP Classes as an SCU

SOP Class Name	SOP Class UID
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3

3.7.1 Association Establishment Policies

3.7.1.1 General

The creation of an MPPS Instance is done automatically by the Somaris/7 DICOM application whenever a patient is registered for image acquisition through the Patient Registration dialog. Exception: In case of Emergency Patients, the MPPS is created only when the user explicitly sends a corresponding message from the MPPS user interface.

Further updates on the MPPS data can be done interactively from the related MPPS user interface. The MPPS "Complete" or "Discontinued" states can only be set from the user interface.

The default PDU size used is of 32 kB.

3.7.1.2 Number of Associations

The Siemens DICOM application initiates one association at a time, to create or set MPPS instances.

3.7.1.3 Asynchronous Nature

The Siemens DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

3.7.1.4 Implementation Identifying Information

- Implementation Class UID 1.3.12.2.1107.5.1.4
- Implementation Version Name SIEMENS_S7VB10A

3.7.2 Association Initiation Policy

The Somaris/7 DICOM Application Entity acts as a Service Class User (SCU) for the

Modality Performed Procedure Step Service Class (to notify an RIS about the status of a procedure while it is performed).

To do so, it will issue one of the following:

- N-CREATE DIMSE according to the CREATE Modality Performed Procedure Step SOP Instance operation
- N-SET DIMSE to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation

3.7.2.1 Real-World Activity

3.7.2.1.1 Associated Real-World Activity - Patient Registered

A patient is registered by the Patient Registration "Exam" action. The trigger to create a MPPS Instance is derived from this event. The related Instance is then immediately communicated to the configured RIS system. An association is established and the MPPS Instance is sent.

3.7.2.1.2 Proposed Presentation Contexts - Patient Registered

The Somaris/7 DICOM application proposes Presentation Contexts as shown in the following table:

Table 65: Proposed presentation contexts

Presentation Context Table		Role	Extended Negotiation
		SCU	None
Abstract Syntax		Transfer Syntax	
Name	UID	Name List	UID List
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2
		Explicit VR Little Endian	1.2.840.10008.1.2.1
		Explicit VR Big Endian	1.2.840.10008.1.2.2

3.7.2.1.3 SOP-Specific Conformance Statement - Patient Registered

3.7.2.1.3.1 Attributes used for the Performed Procedure Step N-CREATE

The Siemens DICOM Modality Performed Procedure Step SCU informs the remote SCP of when the examination of a scheduled procedure step will be performed (that is, the patient is registered). The N-CREATE message is sent when the examination starts after the successful registration of patient data. The following table describes the supported attributes for an N-CREATE message.

Table 66: Performed Procedure Step N-CREATE Attributes

Attribute name	Tag	Required Type	Value
SOP Common			
Specific Character Set	(0008,0005)	1C	from MWL or created
Performed Procedure Step Relationship			
Scheduled Step Attribute Sequence	(0040,0270)	1	
>Study Instance UID	(0020,000D)	1	from MWL or created
>Referenced Study Sequence	(0008,1110)	2	from MWL or zero length
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Accession Number	(0008,0050)	2	from MWL or user input
>Placer Order Number / Imaging Service Request	(0040,2016)	3	from MWL or zero length
>Filler Order Number / Imaging Service Request	(0040,2017)	3	from MWL or zero length
>Requested Procedure ID	(0040,1001)	2	from MWL or user input
>Requested Procedure Description	(0032,1060)	2	from MWL or zero length
>Scheduled Procedure Step ID	(0040,0009)	2	from MWL or zero length
>Scheduled Procedure Step Description	(0040,0007)	2	from MWL or zero length
>Scheduled Protocol Code Sequence	(0040,0008)	2	from MWL or zero length
>>Code Value	(0008,0100)	1C	
>>Coding Scheme Designator	(0008,0102)	1C	
>>Code Scheme Version	(0008,0103)	3	
>>Code Meaning	(0008,0104)	3	
Patient's Name	(0010,0010)	2	from MWL or user input
Patient ID	(0010,0020)	2	from MWL or user input or created
Patients Birth Date	(0010,0030)	2	from MWL or user input
Patient's Sex	(0010,0040)	2	from MWL or user input
Referenced Patient Sequence	(0008,1120)	2	from MWL or zero length
>Referenced SOP Class UID	(0008,1150)	1C	
>Referenced SOP Instance UID	(0008,1155)	1C	
Performed Procedure Step Information			
Performed Procedure Step ID	(0040,0253)	1	from SPS ID or created
Performed Station AE Title	(0040,0241)	1	own AE Title
Performed Station Name	(0040,0242)	2	own hostname

Attribute name	Tag	Required Type	Value
Performed Location	(0040,0243)	2	from SPS Location or zero length
Performed Procedure Step Start Date	(0040,0244)	1	created
Performed Procedure Step Start Time	(0040,0245)	1	created
Performed Procedure Step Status	(0040,0252)	1	IN PROGRESS
Performed Procedure Step Description	(0040,0254)	2	from SPS Description or zero length
Performed Procedure Type Description	(0040,0255)	2	zero length
Procedure Code Sequence	(0008,1032)	2	from Requested Procedure Code or zero length
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Procedure Step End Date	(0040,0250)	2	zero length
Performed Procedure Step End Time	(0040,0251)	2	zero length
Exposure Dose Sequence ^a	(0040,030E)	3	
>Radiation Mode	(0018,115A)	3	
>KVp	(0018,0060)	3	
>XrayTubeCurrentInuA	(0018,8151)	3	
>Exposure Time	(0018,1150)	3	
>FilterType	(0018,1160)	3	
>FilterMaterial	(0018,7050)	3	
>CTDIVol ^b	(0018,9345)	2C	
>CTDI PhantomTypeCodeSequence ^b	(0018,9346)	3	
>>Code Value	(0008,0100)	1	
>>Coding Scheme Designator	(0008,0102)	1	
>>Code Meaning ^b	(0008,0104)	1	
>Private Creator ^b	(0019,00xx)		Value: SIEMENS CT DOSE
>DoseLengthProduct ^b	(0019,xx10)		
>CommentsOnRadiationDose ^b	(0040,0310)	3	
>OrganDose ^b	(0040,0316)	3	
Image Acquisition Results			
Modality	(0008,0060)	1	CT

Attribute name	Tag	Required Type	Value
Study ID	(0020,0010)	2	from Requested Procedure ID or created
Performed Protocol Code Sequence	(0040,0260)	2	from Scheduled Protocol Code SQ or zero length
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Series Sequence	(0040,0340)	2	
>Performing Physicians's Name	(0008,1050)	2C	from MWL or user input
>Protocol Name	(0018,1030)	n/a	User-defined description of the conditions under which the Series was performed
>Operator's Name	(0008,1070)	2C	user input
>Series Instance UID	(0020,000E)	1C	created
>Series Description	(0008,103E)	2C	zero length
>Retrieve AE Title	(0008,0054)	2C	zero length
>Referenced Image Sequence	(0008,1140)	2C	zero length
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	zero length
Radiation Dose Module			
DistanceSourceToDetector	(0018,1110)	3	created
DistanceSourceToEntrance	(0040,0306)	3	zero length
TotalNumberOfExposures	(0040,0301)	3	created
CommentsOnRadiationDose	(0040,0310)	3	created
Exposure Dose Sequence	(0040,030E)	3	created
Billing And Material Management Code Module			
Billing Supplies and Devices Sequence	(0040,0324)	3	created
Quantity Sequence	(0040,0293)	3	created

^a. This sequence added is not part of this module as per DICOM standard. Support for this sequence in this module is additional and does not conform to the DICOM standard.

^b. As per the DICOM standard, this attribute is not part of the Exposure Dose Sequence.

3.7.2.1.3.2 Status Codes of the Performed Procedure Step N-CREATE

The Performed Procedure Step SCU interprets the following status values:

Table 67: N-SET Response Status

Service Status	Meaning	Status Codes (0000,0900)
Failure	Processing Failure	0110
	No such attribute	0105
	Invalid attribute value	0106
	Duplicate SOP Instance	0111
	No such SOP Instance	0112
	No such SOP class	0118
	Class instance conflict	0119
	Missing attribute	0120
	Missing attribute value	0121
	Resource limitation	0213
	Successful Operation	0000
Success		

3.7.2.1.4 Associated Real-World Activity - UI Update

The associated Real-World activity is to send examination information to an SCP by using the DICOM Modality Performed Procedure Step Service, either implicitly (examination) or explicitly (MPPS UI).

3.7.2.1.5 Proposed Presentation Contexts - UI Update

The same Presentation Contexts as in *Table 65: Proposed presentation contexts* on page 136 are proposed.

3.7.2.1.6 SOP-Specific Conformance Statement - UI Update

3.7.2.1.6.1 Attributes used for the Performed Procedure Step N-SET

The Somaris/7 DICOM Performed Procedure Step SCU informs the remote SCP about the performed examination and its status. The N-SET message is sent once for each reconstruction of acquisition data with the status "IN_PROGRESS". The N-SET message is sent after user input with the status "COMPLETED" or "DISCONTINUED". This is intended to be used when the examination is finished with status "COMPLETED", or when the examination could not be completed with status "DISCONTINUED" (already sent automatically when the examination is ended via End Exam and no acquisition was done). The following table describes the attributes supported for an N-SET message.

Table 68: Performed Procedure Step N-SET Attributes

Attribute name	Tag	Required Type	Value
Performed Procedure Step Information			
Performed Procedure Step Status	(0040,0252)	3	IN_PROGRESS or COMPLETED or DISCONTINUED (see above)
Performed Procedure Step Description	(0040,0254)	3	from SPS Description or user input
Performed Procedure Type Description	(0040,0255)	3	zero length
Procedure Code Sequence	(0008,1032)	3	from Requested Procedure Code or empty on user change (see IHE Technical Framework Y3, App. C Note 6)
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Procedure Step End Date	(0040,0250)	1	created
Performed Procedure Step End Time	(0040,0251)	1	created
Exposure Dose Sequence ^a	(0040,030E)	3	
>Radiation Mode	(0018,115A)	3	
>KVp	(0018,0060)	3	
>XrayTubeCurrentInuA	(0018,8151)	3	
>Exposure Time	(0018,1150)	3	
>FilterType	(0018,1160)	3	
>FilterMaterial	(0018,7050)	3	
>CommentsOnRadiationDose	(0040,0310)	3	
>OrganDose ^b	(0040,0316)	3	
Image Acquisition Results			
Performed Protocol Code Sequence	(0040,0260)	3	from Scheduled Protocol Code SQ or user input
>Code Value	(0008,0100)	1C	
>Code Scheme Designator	(0008,0102)	1C	
>Code Scheme Version	(0008,0103)	1C	
>Code Meaning	(0008,0104)	1C	
Performed Series Sequence	(0040,0340)	1	

Attribute name	Tag	Required Type	Value
>Performing Physicians's Name	(0008,1050)	2C	from MWL or user input [empty if Study Split is used]
>Protocol Name	(0018,1030)	1C	name of Scan Protocol (Siemens standard or user defined) [dummy if Study Split is used]
>Operator's Name	(0008,1070)	2C	user input [empty if Study Split is used]
>Series Instance UID	(0020,000E)	1C	created [dummy if Study Split is used]
>Series Description	(0008,103E)	2C	range name with generated reconstruction information or user input [empty if Study Split is used]
>Retrieve AE Title	(0008,0054)	2C	from Storage Commitment RSP or zero length
>Referenced Image Sequence	(0008,1140)	2C	created [empty if Study Split is used]
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	zero length
Radiation Dose			
Total Number of Exposures	(0040,0301)	3	created (number of scans)
Distance Source to Detector (SID)	(0018,1110)	3	created
Distance Source to Entrance	(0040,0306)	3	created
Comments on Radiation Dose	(0040,0310)	3	created (one line per scan) ^c
Exposure Dose Sequence	(0040,030E)	3	created
>Radiation Mode	(0018,115A)	3	created
>KVP	(0018,0060)	3	created
>X-ray Tube Current in uA	(0018,8151)	3	created
>Exposure Time	(0018,1150)	3	created
>Filter Type	(0018,1160)	3	"WEDGE_2" "WEDGE_3" "WEDGE_2_3" "SN_DE" "FLAT", "AU_DESF", "SN_DESF", "AUSN_DESF" or combinations of "WEDGE_*" and "SN_DE"
>CTDIvol ^b	(0018,9345)	3	created

Attribute name	Tag	Required Type	Value
>CTDI Phantom Type Code Sequence ^b	(0018,9346)	3	created
>>Code Value ^b	(0008,0100)	1	
>>Coding Scheme Designator ^b	(0008,0102)	1	
>>Code Meaning ^b	(0008,0104)	1	
>Private ^b	(0019,00xx)		"SIEMENS CT DOSE"
>Dose Length Product ^b	(0019,xx10)		
>Comments on Radiation Dose	(0040,0310)	3	e.g.: Topogram: kV=120 mAs=95 CTDIvol=0.13 DLP=3 Phantom- Type=32cm
Billing and Material Management Code			
Film Consumption Sequence	(0040,0321)	3	created or zero length
>Number of Films	(2100,0170)	3	
>Medium Type	(2000,0030)	3	
>Film Size ID	(2010,0050)	3	
Billing Supplies and Devices Sequence	(0040,0324)	3	user input in Examination Card (example values below) or MPPS window
>Billing Item Sequence	(0040,0296)	3	
>>Code Value	(0008,0100)	1C	for example contrast media code
>>Code Scheme Designator	(0008,0102)	1C	for example contrast media catalog
>>Code Meaning	(0008,0104)	1C	for example contrast media name
>Quantity Sequence	(0040,0293)	1C	
>>Quantity	(0040,0294)	3	for example volume of contrast media
>>Measuring Units Sequence	(0040,0295)	3	
>>>Code Value	(0008,0100)	1C	for example cm ³
>>>Code Scheme Designator	(0008,0102)	1C	for example UCUM
>>>Code Scheme Version	(0008,0103)	1C	for example 1.4
>>>Code Meaning	(0008,0104)	1C	for example cm ³

^a. This sequence added is not part of this module as per DICOM standard. Support for this sequence in this module is additional and does not conform to the DICOM Standard.

^b. As per the DICOM standard, this attribute is not part of the Exposure Dose Sequence.

^c. The following format is used:

RangeName: kV = xxx, mAs = xxx, CTDI_{vol} = xx, DLP = xxx

DualTube: kV = xxx/yyy, mAs = xxx, CTDI_{vol} = xxx, DLP = xxx

CTDI_{vol} and DLP is not provided for Topogram scans.

3.7.2.1.6.2 Status Codes of the Performed Procedure Step N-SET

The Performed Procedure Step SCU interprets the following status values:

Table 69: N-SET Response Status

Service Status	Meaning	Status Codes (0000,0900)
Failure	Processing Failure: Performed Procedure Step Object may no longer be updated	0110
	No such attribute	0105
	Invalid attribute value	0106
	No such SOP Instance	0112
	Invalid object instance	0117
	No such SOP class	0118
	Class instance conflict	0119
	Missing attribute value	0121
	Resource limitation	0213
Success	MPPS instance set	0000

4 Extensions/Specifications/Privatizations

4.1 Standard Extensions

4.1.1 Standard Extensions of all SOP Classes

The following tables list the data dictionary of all the DICOM IOD attributes for which the DICOM standard definitions are extended:

Table 70: Standard Extensions of all SOP Classes

Attribute Name	Tag	Private Creator	Type	Notes
Image Type	(0008,0008)	-	1	See 4.1.1.1 <i>Image Type</i> on page 146 for further explanation.
				Additional Defined Terms:
				Defined Terms for value 3: OTHER, MPR, PROJECTION IMAGE, UNDEFINED
				Defined Terms for value 4: CSA ^{*a} , CT_SOM4 *, CT_SOM5 ^{*b} , CT_SOM6 *, CT_SOM7 *, ECAT *, SHS *
				Somaris/7-based SOMATOM products provide a value 5 with the Defined Terms: ADD, CTL, FINISHED, IN_WORK, MRTD, OTOM, OTOP, PBF, PBV, PKET, PMON, STD, TTP, TTS, AVG, MIP, CBF, CBF1,CBFA, PEAK, CBV, CBVP,CBVA, BV, BVP, TTSA, MTTA, PMBP, RSQP,CSQP, RSDP,CSDP, ALP
				Somaris/7-based SOMATOM products provide a value 6 with the Defined Terms: DNRG, SNRG
				Somaris/7-based SOMATOM products provide a value 7 with the Defined Terms: DET_A, DET_B, DET_AB
				Somaris/7-based SOMATOM products provide a value 8 with the Defined Terms: IREC_PREVIEW
				Additional Defined Terms for the Magnetom Open: HLS, HLP, FLS, FLP, HLDL, HLDR, FLDL, FLDR
Patient Position	(0018,5100)	-	2C	

Table 70: Standard Extensions of all SOP Classes

Attribute Name	Tag	Private Creator	Type	Notes
Body Part Examined	(0018,0015)		3	Additional Defined Terms for the Somaris/7 based SOMATOM products: SPINE, SPECIAL, UNKNOWN, SERVICE See 4.1.1.2 <i>Body Part Examined</i> on page 151 for further explanation.

^a. For terms beginning with the stated prefix, for example, "CSA", and ending with "*", see 4.1.1.1 *Image Type* on page 146.

^b. For private extensions, see 4.2.1 *Private Elements for Storage SOP Classes* on page 173.

All SOP classes may contain additional type 3 attributes which the DICOM standard defines in a different DICOM IOD or DICOM SOP class (attributes from Normalized SOP classes).

This is the case, for example, for:

- Rescale Slope (0028,1053)
- Rescale Intercept (0028,1052)

which are also used in the MR IOD.

4.1.1.1 Image Type

The Image Type (0008,0008) attribute identifies important image identification characteristics. These characteristics are:

1. Pixel Data Characteristics:
 - Is the image an ORIGINAL Image: an image whose pixel values are based on original or source data, or
 - Is the image a DERIVED Image: an image whose pixel values have been derived in some manner from the pixel value of one or more other images.
2. Patient Examination Characteristics:
 - Is the image a PRIMARY Image: an image created as a direct result of the Patient examination, or
 - Is the image a SECONDARY Image: an image created after the initial Patient examination.
3. Modality Specific Characteristics (SOP Specific Characteristics).
4. Implementation-specific identifiers; other implementation-specific identifiers are documented in the implementation's conformance claim.

The Image Type attribute is multi-valued and is provided as follows:

- **Value 1** identifies the Pixel Data Characteristics; Enumerated Values for the Pixel Data Characteristics are:
 - ORIGINAL = Identifies an Original Image
 - DERIVED = Identifies a Derived Image
- **Value 2** identifies the Patient Examination Characteristics; Enumerated Values for the Patient Examination Characteristics are:
 - PRIMARY = Identifies a Primary Image
 - SECONDARY = Identifies a Secondary Image
- **Value 3** identifies any Image IOD-specific specialization. The following terms are defined in addition to the DICOM standard definitions:
 - OTHER = Converted non-Axial and non-Localizer CT images; images of no special type (new syntax)
 - UNDEFINED = Images of no special type (old syntax)
- **Value 4** is implementation-specific. The following terms are defined:
 - Original *syngo*-generated data set types:
 - CSA 3D EDITOR = Object created by 3D Editor
 - CSA 3D FLY PATH = Object created by Fly Through Path
 - CSA 3D FLY VRT = Object created by Fly Through Volume Rendering Technique
 - CSA 3D FUSION = Object created by Fusion
 - CSA AVERAGE = Image created by Average
 - CSA BLACK IMAGE = SC Image with black pixels; only graphics information is of interest
 - CSA BOOKMARK = InSpace-generated SC image containing bookmark information
 - CSA RESAMPLED = Derived image created by zooming or panning the original image
 - CSA REPORT = *syngo* Reporting (documentation of diagnosis)
 - CSA RESULT = *syngo* Reporting (post-processing results)
 - CSA MIP = Image created by Maximum Intensity Projection
 - CSA MIP THIN = Image created by Maximum Intensity Projection
 - CSA MIP THIN CV = Image created by Maximum Intensity Projection (curved cut)
 - CSA MPR = Image created by Multi-Planar Reconstruction
 - CSA MPR CV = Image created by Multi-Planar Reconstruction (curved cut)
 - CSA MPR THICK = Image created by Multi-Planar Reconstruction
 - CSA MPR THICK CV = Image created by Multi-Planar Reconstruction (curved cut)
 - CSA MPR THIN = Image created by Multi-Planar Reconstruction
 - CSA PSSD = SC Image as Perspective Shaded Surface Display
 - CSA SSD = SC Image as Shaded Surface Display
 - CSA SUBTRACT = Image created by Subtraction
 - CSA VRT = SC Image created by Volume Rendering Technique
 - ECAT ACF = CTI PET Attenuation Correction
 - ECAT NORMAL = CTI PET Normalization

ECAT 3D SINO = CTI PET 3D Sinogram Short

ECAT 3D SINO FLT = CTI PET 3D Sinogram Float

- Additional image types generated by Somaris/7- or Somaris/5-based SOMATOM products

CT_SOM7 PCT = PerfusionCT Image

CT_SOM5 AVE = Averaged Image

CT_SOM5 ICD = Interventional Cine Display Image

CT_SOM5 MON = Monitoring or Premonitoring Image

CT_SOM5 MUL = Multiscan Image

CT_SOM5 PAR = Parameter Image

CT_SOM5 PROT = Protocol Image

CT_SOM5 ROT = ROT Image

CT_SOM5 RTD = Real Time Display Image

CT_SOM5 RTD DUAL = Common Somaris/7 Dual Tube Real-Time Display Image

CT_SOM7 RTD DUAL = Specific Somaris/7 Dual Tube Real-Time Display Image

CT_SOM5 SEQ = Sequence Image

CT_SOM5 SEQ DUAL = Somaris/7 Dual Tube Sequence Image

CT_SOM5 SPI = Spiral Image

CT_SOM5 SPI DUAL = Somaris/7 Dual Tube Spiral Image

CT_SOM7 SPI DUAL = Specific Somaris/7 Dual Tube Spiral Image

CT_SOM5 SPO = Spiral Oblique Image

CT_SOM5 STA = Static Image

CT_SOM5 SUB = Subtracted Image

CT_SOM5 TOP = Topogram

CT_SOM5 DPAN = Dental Panorama Rebuilt Tomogram

CT_SOM5 DPAR = Dental Paraxial Rebuilt Tomogram

CT_SOM5 DFLM = Dental Filming Image

CT_SOM5 DYB = Dynamic Evaluation Averaged Baseline Image

CT_SOM5 DYF = Dynamic Evaluation Fused Multislice Image

CT_SOM5 PEVI = Pulmo Evaluation Image

CT_SOM5 OEVA = Osteo Evaluated Tomogram

CT_SOM5 MIP = Maximum Intensity Projection image created by a CT application

CT_SOM5 MPR = Multi Planar Reconstruction image created by a CT application

CT_SOM5 REP = Lung Care Report Image

CT_SOM7 VPCT = Volume Perfusion CT

CT_SOM7 FLU = Fluoroscopic

- Converted images

CT_SOM4 NONE = Converted SOMARIS image

CT_SOM4 CONV = Converted SOMARIS Convolution Kernel file

CT_SOM4 DART = Converted SOMARIS Dental Artificial image

CT_SOM4 DEVA = Converted SOMARIS Dental Evaluation image

CT_SOM4 DGRA = Converted SOMARIS Dental Graphics image
CT_SOM4 DMEA = Converted SOMARIS Dynamic Measurement image
CT_SOM4 DPAN = Converted SOMARIS Dental Panorama image
CT_SOM4 DPAR = Converted SOMARIS Dental Paraxial image
CT_SOM4 EBT = Converted SOMARIS Evolution image
CT_SOM4 HIS = Converted SOMARIS Histogram Graphics image
CT_SOM4 HISC = Converted SOMARIS Histogram Graphics image
CT_SOM4 MUL = Converted SOMARIS Multiscan image
CT_SOM4 OEVA = Converted SOMARIS Osteo Evaluation image
CT_SOM4 OTOM = Converted SOMARIS Osteo Tomogram image
CT_SOM4 OTOP = Converted SOMARIS Osteo Topogram image
CT_SOM4 PLOT = Converted SOMARIS Plot image
CT_SOM4 QUAL = Converted SOMARIS Quality image
CT_SOM4 R2D = Converted SOMARIS 2D Rebuild image
CT_SOM4 R3D = Converted SOMARIS 3D Rebuild image
CT_SOM4 R3DE = Converted SOMARIS 3D Rebuild image
CT_SOM4 RMAX = Converted SOMARIS Maximum Intensity Projection image
CT_SOM4 RMIN = Converted SOMARIS Minimum Intensity Projection image
CT_SOM4 ROT = Converted SOMARIS Rotation Mode image
CT_SOM4 RRAD = Converted SOMARIS Radiographic Projection image
CT_SOM4 RVIT = Converted SOMARIS Vessel Image Tool image
CT_SOM4 RVRT = Converted SOMARIS Volumetric Rendering image
CT_SOM4 SAVE = Converted SOMARIS Evolution Screen Save image
CT_SOM4 SCAN = Converted SOMARIS Standard Mode image
CT_SOM4 SEQ = Converted SOMARIS Sequence Mode image
CT_SOM4 SER = Converted SOMARIS Serial Mode image
CT_SOM4 SIN = Converted SOMARIS Sinogram image
CT_SOM4 SINC = Converted SOMARIS Sinogram image
CT_SOM4 SPI = Converted SOMARIS Spiral Mode image
CT_SOM4 STA = Converted SOMARIS Static Mode image
CT_SOM4 TAB = Converted SOMARIS Correction Table image
CT_SOM4 TOP = Converted SOMARIS Topogram image
CT_SOM4 GTOP = Converted SOMARIS Topo Graphics image
CT_SOM4 PEVG = Converted SOMARIS Pulmo Evaluation image
CT_SOM4 PEVI = Converted SOMARIS Pulmo Evaluation image
CT_SOM4 PUL = Converted SOMARIS Pulmo Respiration curve
CT_SOM4 PROT = Converted SOMARIS Protocol image
CT_SOM4 TEXT = Converted SOMARIS Text image
CT_SOM4 ICD = Converted SOMARIS Interventional Cine image

SHS DENT = Converted MagicView Dental Tomogram image
SHS DPAN = Converted MagicView Dental Panorama image
SHS DPAR = Converted MagicView Dental Paraxial image

SHS 3D_CURVED = Converted MagicView image

SHS 3D_MIP = Converted MagicView Maximum Intensity Projection image

SHS 3D_MPR = Converted MagicView Multi Planar Reconstruction image

SHS 3D_SSD = Converted MagicView Shaded Surface Display image

SHS 3D_VRT = Converted MagicView Volumetric Rendering image

- **Value 5** is specific to the Somaris/7- or Somaris/5-based SOMATOM products. In special cases (3D post-processing), values mentioned for a lower index may appear for value 5 or higher. This refers to 3D post-processing base image types.

The following terms are defined:

- ADD = Additional Scan
- ALP = Arterial Liver Perfusion
- AVG = Average
- BF = NeuroVPCT Blood Flow
- BFI = NeuroVPCT Blood Flow - IncGamma
- BV = NeuroVPCT Blood Volume
- BVP = NeuroVPCT Blood Volume - Patlak
- CBF = NeuroVPCT Blood Flow
- CBFA = NeuroVPCT Blood Flow - Alternate
- CBFi = NeuroVPCT Blood Flow - IncGamma
- CBV = NeuroVPCT Blood Volume
- CBVA = NeuroVPCT Blood Volume - Alternate
- CBVP = NeuroVPCT Blood Volume - Patlak
- CSQP = Patlak ChiSquare
- CTL = Control Scan
- HPI = Hepatic Perfusion Index
- FINISHED = Lung Care Report Image (finished)
- IN_WORK = Lung Care Report Image (not finished)
- MIP = Maximum Intensity Projection
- MRTD = Multiscan Real Time Display Image
- MTTA = Mean Transit Time - Alternate
- OTOM = Osteo Scanned Tomogram
- OTOP = Osteo Scanned Topogram
- PBF = Perfusion Blood Flow Image
- PBV = Perfusion Blood Volume Image
- PKET = Peak Enhancement Parameter Image
- PMBA = Permeability - Alternate
- PMBP = Permeability
- PMON = Premonitoring Scan
- PEAK = NeuroVPCT Peak Enhancement
- PVP = Portal Venous Liver Perfusion
- RSDP = Patlak Residual
- RSQP = Patlak RSquare
- RT3D CONFIG = InSpace Configuration Image
- STD = Standard image of corresponding Type 4

- TTDA = Time-to-Drain - Alternate
- TTP = Time-to-Peak Parameter Image
- TTS = Time-to-Start Parameter Image
- TTSA = NeuroVPCT Time-to-Start Parameter Image
- VPCT MCnFn = Motion Corrected, Filtered
- **Value 6** is specific to the Somaris/7-based SOMATOM products. Dual Tube scans require a more detailed distinction. The following terms are defined:
 - DNRG = Dual Energy
 - SNRG = Single Energy
- **Value 7** is specific to the Somaris/7-based SOMATOM products. Dual Energy scans require a more detailed distinction. The following terms are defined:
 - DET_A = Only data of detector A used
 - DET_B = Only data of detector B used
 - DET_AB = Data is derived from detector A and detector B
- **Value 8** is specific to the Somaris/7-based SOMATOM products. Preview images of SAFIRE/ADMIRE Reconstructions require the following term to be defined:
 - IREC_PREVIEW

4.1.1.2 Body Part Examined

The Body Part Examined (0018,0015) attribute provides a textual description of the part of the body that is being examined. The Somaris/7-based SOMATOM products extend the Defined Terms:

- SPINE = Summary term used instead of the Defined Terms CSPINE, TSPINE, LSPINE, and SSPINE
- SPECIAL = Image was acquired using acquisition modes that are not mapped to a certain part of the body
- SERVICE = Image was acquired for maintenance purposes
- UNKNOWN = No information about the body part is available

See 4.1.2 *Specializations* on page 158 for a mapping of the organ characteristics used for the examination to the Body Part Examined terms.

In addition, the user interface allows the user to define new terms. Therefore, any syntactically correct value may be present as a value of this attribute. However, it is recommended to use the DICOM defined terms when appropriate.

4.1.1.3 RGB color images

The Somaris/7 DICOM application extends the CT Image IOD by using the RGB color image description with the unsigned integer, 24-bit color image plane pixel format:

- Samples per pixel (attribute 0028, 0002) = 3
- Photometric interpretation (attribute 0028,0004) = "RGB"
- Pixel representation (attribute 0028, 0103) = 0
- Bits allocated (attribute 0028, 0100) = 8
- Bits stored (attribute 0028,0101) = 8
- High bit (attribute 0028,0102) = 7
- Planar configuration (attribute 0028,0006) = 0.

This format is used for Functional Imaging, that is, images that meaningfully use all common CT Image attributes. However, the pixel values do not represent a scaled Hounsfield value but a different value (depending on the type of image). Thus, window-related attributes must not be used to interpret the pixel values as scaled HU values. The values used by Somaris/7 are:

- Window center (attribute 0028, 1050) = 128
- Window width (attribute 0028,1051) = 256
- Rescale intercept (attribute 0028, 1050) = 0
- Rescale slope (attribute 0028,1051) = 1

The following types of images may use this format:

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
Averaged Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 AVE	None	AVE
Parameter Image (Patlak Blood Volume)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKBV	PAR
Parameter Image (Peak enhancement)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKET	PAR
Parameter Image (Perfusion Blood Flow)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBF	PAR
Parameter Image (Perfusion Blood Volume)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBV	PAR
Parameter Image (Permeability)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PMB	PAR
Parameter Image (Time to Peak)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTP	PAR

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
Parameter Image (Time to Start)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTS	PAR
Parameter Image (Patlak Residual)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKER	PAR
Parameter Image (Patlak RSquare)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKR2	PAR
Parameter Image (Arterial Liver Perfusion)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	ALP	PAR
Parameter Image (Portal Venous Liver Perfusion)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PVP	PAR
Parameter Image (Hepatic Perfusion Index)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	HPI	PAR
PerfusionCT Image (Maximum Intensity Projection)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	MIP	VPCT
PerfusionCT Image (Average)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	AVG	VPCT
PerfusionCT Image (NeuroVPCT Blood Flow)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBF	VPCT
PerfusionCT Image (NeuroVPCT Blood Flow - IncGamma)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBFI	VPCT
PerfusionCT Image (NeuroVPCT Blood Flow - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBFA	VPCT
PerfusionCT Image (NeuroVPCT Not Motion Corrected, No Filter)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI, CT_SOM5 SEQ, CT_SOM5 MUL	VPCT MC0F0	SPI, SEQ, MUL

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
PerfusionCT Image (NeuroVPCT, Motion Corrected, No Filter)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,		SPI,
					CT_SOM5 SEQ,	VPCT MC1F0	SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (NeuroVPCT Not Motion Corrected, Filtered)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,		SPI,
					CT_SOM5 SEQ,	VPCT MC0F1	SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (NeuroVPCT Motion Corrected, Filtered)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,		SPI,
					CT_SOM5 SEQ,	VPCT MC1F1	SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (BodyVPCT Blood Flow)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BF	VPCT
PerfusionCT Image (BodyVPCT Blood Flow - IncGamma)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BFI	VPCT
PerfusionCT Image (BodyVPCT Blood Flow - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BFA	VPCT
PerfusionCT Image (Peak enhancement)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	PEAK	VPCT
PerfusionCT Image (NeuroVPCT Blood Volume)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBV	VPCT
PerfusionCT Image (NeuroVPCT Blood Volume - Patlak)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBVP	VPCT

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
PerfusionCT Image (NeuroVPCT Blood Volume - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CBVA	VPCT
PerfusionCT Image (BodyVPCT Blood Volume)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BV	VPCT
PerfusionCT Image (BodyVPCT Blood Volume - Patlak)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BVP	VPCT
PerfusionCT Image (BodyVPCT Blood Volume - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	BVA	VPCT
PerfusionCT Image (BodyVPCT Not Motion Corrected, No Filter)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,	VPCT MC0F0	SPI,
					CT_SOM5 SEQ,		SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (BodyVPCT, Motion Corrected, No Filter)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,	VPCT MC1F0	SPI,
					CT_SOM5 SEQ,		SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (BodyVPCT Not Motion Corrected, Filtered)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,	VPCT MC0F1	SPI,
					CT_SOM5 SEQ,		SEQ,
					CT_SOM5 MUL		MUL
PerfusionCT Image (BodyVPCT Motion Corrected, Filtered)	CT	DERIVED	PRIMARY	AXIAL	CT_SOM5 SPI,	VPCT MC1F1	SPI,
					CT_SOM5 SEQ,		SEQ,
					CT_SOM5 MUL		MUL

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
PerfusionCT Image (Time to Start)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	TTS	VPCT
PerfusionCT Image (Time to Start - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	TTSA	VPCT
PerfusionCT Image (Time to Peak)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	TTP	VPCT
PerfusionCT Image (Time To Drain Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	TTDA	VPCT
PerfusionCT Image (Mean Transit Time - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	MTTA	VPCT
PerfusionCT Image (Permeability)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	PMBP	VPCT
PerfusionCT Image (Permeability - Alternate)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	PMBA	VPCT
PerfusionCT Image (Patlak RSquare)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	RSQP	VPCT
PerfusionCT Image (Patlak ChiSquare)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	CSQP	VPCT
PerfusionCT Image (Patlak Residual)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	RSDP	VPCT
PerfusionCT Image (Arterial Liver Perfusion)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	ALP	VPCT
PerfusionCT Image (Portal Venous Liver Perfusion)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	PVP	VPCT
PerfusionCT Image (Hepatic Perfusion Index)	CT	DERIVED	SECONDARY	AXIAL, SAGITTAL, CORONAL	CT_SOM7 VPCT	HPI	VPCT
Screenshot Image	SC	DERIVED	SECONDARY	OTHER	VPCT	None	VPCT

Table 71: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text
Max Intensity Projection Image (Perfusion)	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MIP		MIP
LungCARE send-to-Filming images	CT	DERIVED	SECONDARY	OTHER	CSA MIP THIN	LC VALID WINDOW	MIP
LungCARE send-to-Filming images	CT	DERIVED	SECONDARY	OTHER	CSA MPR THICK	LC VALID WINDOW	MPR
LungCARE send-to-Filming images	CT	DERIVED	SECONDARY	OTHER	CSA VRT THIN	LC VALID WINDOW	VRT
LungCARE send-to-Filming images	CT	DERIVED	SECONDARY	OTHER	CSA PRVT	LC VALID WINDOW	PVRT
LungCARE send-to-Filming images	CT	DERIVED	SECONDARY	OTHER	CSA MPR	LC VALID WINDOW	MPR

4.1.1.4 CT Images with Color Lookup Table

Images derived from the Application Neuro PBV are created as CT Images with the Photometric Interpretation (0028,0004) set to "MONOCHROME2". Additionally, a Color Lookup Table is stored in the Private Header.

Table 72: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
[known creating applications]							
Neuro PBV (Perfused Blood Volume)	CT	DERIVED	SECONDARY	AXIAL	NEU-ROPBV	None	None
Neuro PBV (Perfusion Weighted Map)	CT	DERIVED	SECONDARY	AXIAL	NEUOPM	None	None

4.1.2 Specializations

4.1.2.1 Images created by Somaris/7

The following table lists the Somaris/7 image types and the corresponding combinations of the Image Type Attribute values.

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description [known creating applications]	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
3D MPR	SC	DERIVED	SECONDARY	LOCAL- IZER	CSA MPR	None	MPR
3D MPR THICK	SC	DERIVED	SECONDARY	LOCAL- IZER	CSA MPR THICK	None	MPR THICK
3D MIP	SC	DERIVED	SECONDARY	LOCAL- IZER	CSA MIP	None	MIP
3D MIP THIN	SC	DERIVED	SECONDARY	LOCAL- IZER	CSA MIP THIN	None	MIP THIN
Averaged Image [Average, DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 AVE	None	AVE
Interventional Cine Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 ICD	None	ICD
Monitoring Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MON	None	MON
Premonitoring Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MON	PMON	MON
Multiscan Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 MUL	None	MUL
Parameter Image (Arterial Liver Per- fusion) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	ALP	PAR
Parameter Image (Hepatic Perfusion Index) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	HPI	PAR
Parameter Image (Portal Venous Liver Perfusion) [BodyPerfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PVP	PAR
Protocol Image, Time Density Curve Image [BodyPerfusion] ^a	SC	DERIVED	SECONDARY	OTHER	None	None	AC

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
[known creating applications]							
Parameter Image (Patlak Blood Volume) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKBV	PAR
Parameter Image (Patlak Residual) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKER	PAR
Parameter Image (Patlak RSquare) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKR2	PAR
Parameter Image (Peak enhance- ment) [DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PKET	PAR
Parameter Image (Perfusion Blood Flow) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBF	PAR
Parameter Image (Perfusion Blood Volume) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PBV	PAR
Parameter Image (Permeability) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	PMB	PAR
Parameter Image (Time to Peak) [DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTP	PAR
Parameter Image (Time to Start) [Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PAR	TTS	PAR
Protocol Image	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 PROT	None	PROT (List only)
Report Image (not finished)	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 REP	IN_WORK	REP
Report Image (finished)	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 REP	FINISHED	REP
ROT Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 ROT	None	ROT

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
[known creating applications]							
Real Time Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 RTD	None	RTD
Real Time Display Image (Dual Tube), Som5-com- patible	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 RTD DUAL	STD	RTD DUAL
Real Time Display Image (Cardio)	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM7 RTD DUAL	STD	RTD DUAL
Multiscan Real Time Display Image	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 RTD	MRTD	RTD
Sequence Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	None	SEQ
Sequence Image (Dual Tube)	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ DUAL	STD	SEQ DUAL
Additional Scan Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	ADD	SEQ
Control Scan Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SEQ	CTL	SEQ
Spiral Image	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SPI	None	SPI
Spiral Image (Dual Tube)	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SPI DUAL	STD	SPI DUAL
Spiral Image (Cardio)	CT	ORIGINAL	PRIMARY / SECONDARY	AXIAL	CT_SOM7 SPI DUAL	STD	SPI DUAL
Spiral Oblique Image	CT	DERIVED	PRIMARY / SECONDARY	AXIAL	CT_SOM5 SPO	None	SPO
Static Image	CT	ORIGINAL	PRIMARY	OTHER	CT_SOM5 STA	None	STA
Subtracted Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 SUB	None	SUB
Topogram	CT	ORIGINAL	PRIMARY	LOCAL- IZER	CT_SOM5 TOP	None	TOP
Osteo Scanned Tomogram	CT	ORIGINAL	PRIMARY	AXIAL	CT_SOM5 SEQ	OTOM	SEQ
Osteo Scanned Topogram	CT	ORIGINAL	PRIMARY	LOCAL- IZER	CT_SOM5 TOP	OTOP	TOP
Osteo Evaluated Tomogram	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 OEVA	None	OEVA

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description [known creating applications]	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
Pulmo Evaluated Tomogram	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 PEVI	None	PEVI
Calcium Scoring Table [Calcium Scoring]	SC	DERIVED	SECONDARY	OTHER	CT_SOM5 TAB	None	TAB
Dental Filming Image	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DFLM	None	DFLM
Dental Panorama Rebuild Tomogram	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DPAN	None	DPAN
Dental Paraxial Rebuild Tomogram	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 DPAR	None	DPAR
Dental/Volume Maximum Inten- sity Projection Image [Dental, Vol- ume, DynEva, Perfusion]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MIP	None	MIP
Dental Panorama Reference Image [Dental, Volume]	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	None	MPR
Dental Paraxial Reference Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	None	MPR
Dental Reference Image	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 MPR	None	MPR
Dynamic Evalua- tion Averaged Baseline	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 DYB	None	DYB
Dynamic Evalua- tion Fused Multi- slice	CT	DERIVED	SECONDARY	AXIAL	CT_SOM5 DYF	None	DYF
Volume reformat- ted images (sagit- tal and coronal)	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 MPR	None	MPR
Various result images [CalciumScoring, Colon]	CT	DERIVED	SECONDARY	AXIAL	CSA MPR	None	MPR
Various result images	CT	DERIVED	SECONDARY	AXIAL	CSA MPR THICK	None	MPR

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
[known creating applications]							
Various result images	CT	DERIVED	SECONDARY	AXIAL	CSA MIP	None	MIP
Various result images [CalciumScoring]	CT	DERIVED	SECONDARY	AXIAL	CSA MIP THIN	None	MIP
Various result images [Colon]	SC	DERIVED	SECONDARY	OTHER	CSA PSSD	None	PSSD
Various result images	CT	DERIVED	SECONDARY	AXIAL	CSA VRT	None	VRT
Various result images [Colon]	SC	DERIVED	SECONDARY	OTHER	CSA VRT	None	VRT
InSpace bookmark [InSpace]	SC	DERIVED	SECONDARY	OTHER	CSA BOOK- MARK	RT3D CONFIG	BOOK
InSpace result images [InSpace]	SC	DERIVED	SECONDARY	OTHER	CSA 3DPROJEC TION	None	3DPR
LungCARE save images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	MIP	LC VALID WINDOW	MIP
LungCARE save images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	MPR	LC VALID WINDOW	MPR
LungCARE save images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	VRT	LC VALID WINDOW	VRT
LungCARE save images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	PVRT	LC VALID WINDOW	PVRT
LungCARE save images [LungCARE]	CT	DERIVED	SECONDARY	OTHER	MPR	LC VALID WINDOW	MPR
LungCARE save images [LungCARE]	CT	DERIVED	SECONDARY	OTHER	CT_SOM5 SPI	LC VALID WINDOW	SPI

Table 73: Somaris/7 Image Type (0008,0008) for objects **created** by Somaris/7

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somaris/7 Image Text or Lists
[known creating applications]							
LungCARE report images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	MIP	LC VALID WINDOW	None
LungCARE report images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	MPR	LC VALID WINDOW	None
LungCARE report images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	VRT	LC VALID WINDOW	None
LungCARE report images [LungCARE]	SC	DERIVED	SECONDARY	OTHER	PVRT	LC VALID WINDOW	None
Various Graphics [DynEva, Osteo, Pulmo, Volume, Perfusion, Argus]	SC	DERIVED	SECONDARY	OTHER	CSA BLACK IMAGE	None	None
Dual Energy Mixed Series [Dual Energy]	SC	ORIGINAL	SECONDARY	AXIAL	CT_SOM5 SPI DUAL	STD	None

^a. More detailed attribute information will be provided in a future version.

Note

Structured Reports

Some applications creates Structured Reports. However, when running in specific (service configured) settings outside of the system, they appear as an SC image, labeled as Type 3 "OTHER" and Type 4 "CSA REPORT". This private extension is not published in detail here, as the intended use is real DICOM SR.

Note

CT Perfusion Maps

The following CT Perfusion maps contain a blow-up factor in a private section of the DICOM header. This should taken in consideration in quantitative evaluations on systems other than those based on *syngo.classic* (e.g. PACs, *syngo.via*).

- All blood volume maps: CBV, CBV(A), CBV(P), Extravascular Volume (MDC), BV (MDC)

- All maps containing time information: TTS, TTS(A), TTP, TTP(MDC), TTD, MTT, Tissue Transit Time

- Patlak Residuals

4.1.2.2 **Structured Reports created by Somaris/7**

The following table lists the Somaris/7 image types and the corresponding combinations of the Image Type Attribute values.

Table 74: *Somarisl7 Image Type (0008,0008) for objects created by Somaris/7*

Image Type Description	IOD	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5	Somarisl7 Image Text or Lists
[known creating applications]							
LungCARE SR reports							
[LungCARE, Calcium Scoring, Circulation]	SR	ORIGINAL	PRIMARY	OTHER	CSA REPORT	None	None
CT Dose SR reports	SR	ORIGINAL	PRIMARY	OTHER	CSA REPORT	None	None

The LungCARE, Calcium Scoring and Circulation applications create Comprehensive Structured Reports.


The following is valid for Structured Reports created by Calcium Scoring:

The CaScoring application creates structured reports generally following the templates defined in the DICOM supplement 97 “CT/MR Cardiovascular Analysis Report” (Version: 0.11; Working Draft). There may be some changes when the document is released in its final version and which could not be considered. The following is valid for Structured Reports created by Circulation: The Circulation application creates structured reports generally following the DICOM template TID 3900.

Note

CT Dose Report
The CT Dose Report generally follows the templates defined in the DICOM Standard 2014b “CT Radiation Dose” (TID 10011), “CT Accumulated Dose Data” (TID 10012 , TID10013) and supports all mandatory elements.

Fig. 10: Interconnection of CT Radiation Dose Templates

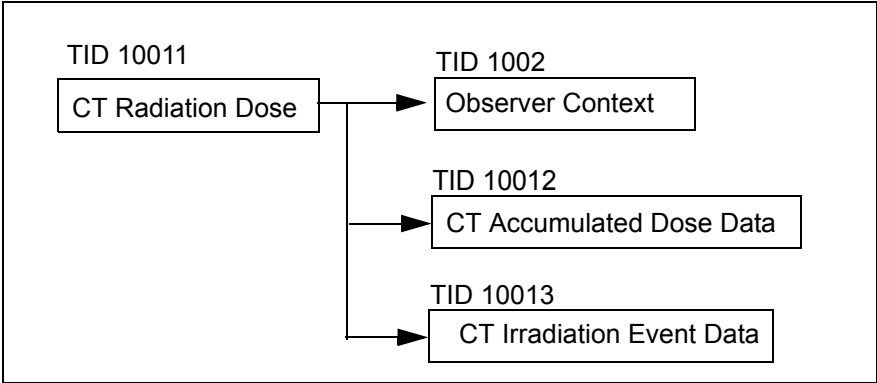

4.1.2.3 Somaris/7 Attribute Interpretation

For an overview of selected attribute filling for different Image Types, please refer to the *Annex*.

The table below explains how common attributes of created and uncompressed ORIGINAL and AXIAL images are set by Somaris/7 image reconstruction. This table does not intend to be a substitute for DICOM 3.0 attribute definitions. However, in addition to these definitions, it provides an impression of which attributes are in common use - and how these are related to Somaris/7 examinations:

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
0002,0012	Implementation Class UID	Value: 1.3.12.2.1107.5.1.4
0002,0013	Implementation Version Name	Value: SIEMENS_S7VB10A
0008,0005	Specific Character Set	
0008,0008	Image Type	see 4.1.2.1 Images created by Somaris/7 on page 158
0008,0016	SOP Class UID	Value: 1.2.840.10008.5.1.4.1.1.2
0008,0018	SOP Instance UID	Created
0008,0020	Study Date	The date and time entries of existing studies are copied into the corresponding entries in the header of a new image.
0008,0030	Study Time	If a new study is created, the date and time entries from the first series of this new study will be used.
0008,0021	Series Date	The date and time entries of existing series are copied into the corresponding entries in the header of a new image.
0008,0031	Series Time	If a new series is created, the current real-world date and time will be used.
0008,0022	Acquisition Date	Acquisition Date and Time are defined as the real-world start of the accumulation of data contributing to a particular image. As a result of multi-slice technology, several images may have the same Acquisition Date and Time.
0008,0032	Acquisition Time	
0008,0023	Image (Content) Date	
0008,0033	Image (Content) Time	For all images that result from the reconstruction of acquired data, the time stamp is the same as the Acquisition Date and Time. This is true for images that were reconstructed immediately after data acquisition, as well as for images that were reconstructed at any time later.
		For all other images created by any other means, the time stamp is derived from a point in time during the creation process of these images.
0008,0050	Accession Number	Input is entered from MWL or during patient registration, and may have null length. Note: When Study Split is used, the value corresponding to the Requested Procedure Description selected in the Exam UI is sent.
0008,0060	Modality	Value: CT
0008,0070	Manufacturer	Value: SIEMENS

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
0008,0080	Institution Name	Hospital name read from configuration data or user input entered during patient registration or examination setup
0008,0081	Institution Address	Hospital address read from configuration data. The default format is 4 lines consisting of Street, City, District and Country.
0008,0090	Referring Physician's Name	Input from MWL or entered during patient registration or examination setup; may have null length.
0008,1010	Station Name	Name of the computer controlling the examination
0008,1030	Study Description	Derived from information entered during patient registration or examination setup as the concatenation of the Body Region and the selected Scan Protocol name, separated by a "^" Note: When Study Split is used, the Requested Procedure Description selected in the Exam UI will be sent.
0008,1032	ProcedureCodeSequence	Used for taskflow IDs received from syngo.via
>0008,0100	CodeValue	TaskflowId Code received from syngo.via
>0008,0104	CodeMeaning	TaskflowId Meaning received from syngo.via
>0008,0102	MeaningCoding Scheme Designator	Fixed value: "99CT_VIA"
0008,1050	Performing Physician's Name	Input entered from MWL or during patient registration
0008,1070	Operator's Name	According to user input
0008,1080	Admitting Diagnoses Description	Input entered from MWL or during patient registration.
0008,103E	Series Description	According to user input (system proposes <Range Name> <Slice Thickness> <Kernel>)
0008,1090	Manufacturer's Model Name	The Siemens product name
0008,1140	Referenced Image Sequence	
>0008,1150	Referenced SOP Class UID	SOP Class UID of Topogram used for planning
>0008,1155	Referenced SOP Instance UID	SOP Instance UID of Topogram used for planning
0008,2112	Source Image Sequence	
>0008,1150	Referenced SOP Class UID	SOP Class UID of Raw data used for reconstruction
>0008,1155	Referenced SOP Instance UID	SOP Instance UID of Raw data used for reconstruction

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation																								
0008,2111	Derivation Description	Lossy Image Compression will be set to 01 for the Extended Field of View because of low image quality. Derivation Description: "Reconstruction field larger than scan field".																								
0009,00xx	Private Creator	Value: SIEMENS CT VA1 DUMMY																								
0010,0010	Patient's Name	Input from MWL or entered during patient registration or examination setup																								
0010,0020	Patient ID	Input from MWL or entered or generated during patient registration or examination setup																								
0010,0030	Patient's Birth Date	Input from MWL or entered during patient registration or examination setup; may be calculated from age																								
0010,0040	Patient's Sex	Input from MWL or entered during patient registration or examination setup																								
0010,1010	Patient's Age	Input from MWL or entered during patient registration or examination setup; may be calculated from Patient's Birth Date																								
0018,0010	Contrast/Bolus Agent	<p>If present:</p> <p>The attribute is filled with the value entered in the contrast card. If nothing was entered, the attribute is filled with the fixed term "APPLIED".</p>																								
0018,0015	Body Part Examined	<p>The Body Part Examined attribute is derived from the organ characteristic of the scan or directly entered by the operator, overriding this default.</p> <p>The organ characteristic parameter is contained in the scan protocol selected for examination during patient registration or examination setup, and may vary for different scans within one protocol (use System/Run/List Scan Protocols column "OrgChar" for a list of values for specific scan protocols).</p> <table><tr><th>Organ Characteristic</th><th>Body Part Examined</th></tr><tr><td>Head</td><td>HEAD</td></tr><tr><td>Neck</td><td>NECK</td></tr><tr><td>Shoulder</td><td>SHOULDER</td></tr><tr><td>Thorax</td><td>CHEST</td></tr><tr><td>Abdomen</td><td>ABDOMEN</td></tr><tr><td>Spine</td><td>SPINE</td></tr><tr><td>Pelvis</td><td>PELVIS</td></tr><tr><td>Extremities</td><td>EXTREMITY</td></tr><tr><td>Cardio</td><td>HEART</td></tr><tr><td>Service</td><td>SERVICE</td></tr><tr><td>n. a.</td><td>UNKNOWN</td></tr></table>	Organ Characteristic	Body Part Examined	Head	HEAD	Neck	NECK	Shoulder	SHOULDER	Thorax	CHEST	Abdomen	ABDOMEN	Spine	SPINE	Pelvis	PELVIS	Extremities	EXTREMITY	Cardio	HEART	Service	SERVICE	n. a.	UNKNOWN
		Organ Characteristic	Body Part Examined																							
		Head	HEAD																							
		Neck	NECK																							
		Shoulder	SHOULDER																							
		Thorax	CHEST																							
		Abdomen	ABDOMEN																							
		Spine	SPINE																							
		Pelvis	PELVIS																							
		Extremities	EXTREMITY																							
		Cardio	HEART																							
		Service	SERVICE																							
n. a.	UNKNOWN																									
0018,0022	Scan Options	This field is used to store cardiac information.																								
0018,0050	Slice Thickness	Resulting slice thickness; not necessarily equal to collimated slice																								
0018,0060	KVP	Voltage selected for scan																								
0018,0090	Data Collection Diameter	The diameter in mm of the region over which data was collected																								

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
0018,1000	Device Serial Number	Serial number of the CT system's gantry
0018,1020	Software Version(s)	Software version of Somaris/7; only one value is used
0018,1030	Protocol Name	Name of Scan Protocol selected during patient registration or examination setup
0018,1100	Reconstruction Diameter	Field of View selected for reconstruction
0018,1110	Distance Source to Detector	
0018,1111	Distance Source to Patient	
0018,1120	Gantry/Detector Tilt	
0018,1130	Table Height	Table height as entered for scan
0018,1140	Rotation Direction	
0018,1150	Exposure Time	The exposure time for the respective image. For a spiral scan or multiscan, this corresponds to the rotation time.
0018,1151	X-ray Tube Current	Tube current used for scanning
0018,1152	Exposure	(Effective) mAs. For spiral images, the product of exposure time and x-ray tube current is corrected with Table Feed per Rotation. This attribute is expressed in mAs.
0018,1160	Filter Type	"WEDGE_2","WEDGE_3","WEDGE_2_3", "SN_DE","FLAT","AU_DESF","SN_DESF","AUSN_DESF" or combinations of "WEDGE_*", "SN_DE"
0018,1170	Generator Power	
0018,1190	Focal Spots	Size of the focal spot actually used to generate x-ray radiation for a particular image. This is a single value expressed in mm.
0018,1200	Date of Last Calibration	Date of last Base Calibration
0018,1201	Time of Last Calibration	Time of last Base Calibration
0018,1210	Convolution Kernel	5-character code of convolution kernel. In case SAFIRE/ADMIRE was used, the strength is written to the second value of this attribute.
0018,5100	Patient Position	As entered for scan
0018,9306	Single Collimation Width	As entered for scan
0018,9307	Total Collimation Width	As entered for scan
0018,9309	Table Speed	The distance in mm that the table moves in one second during the gathering of data that resulted in this image
0018,9310	Table Feed per Rotation	As entered for scan
0018,9311	CT Pitch Factor	As entered for scan
0018,9313	Data Collection Center (Patient)	Only filled when data is available or defined
0018,9318	Reconstruction Target Center (Patient)	Only filled when data is available

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
0018,9323	Exposure Modulation Type	A label describing the type of exposure modulation used for the purpose of limiting the dose:
		Defined Terms:
		DoseModulationType DICOM Entry (string)
		ZAxisExposureControl Z_EC
		OnlineControl XY_EC
		mAControl FIX_EC
		AutomaticExposureControl XYZ_EC
		DvModulation PULS_EC
		DvAdvanced PULS_MINDOSE_EC
		DvModulationZEC PULS_EC
		DvAdvancedZEC PULS_MINDOSE_EC
		DvModulationMAC PULS_EC
		DvAdvancedMAC PULS_MINDOSE_EC
		AngularTrigger X_CARE_EC
		AngularTriggerZEC X_CARE_Z_EC
		AngularTriggerMAC X_CARE_FIX_EC
		NoModulation OFF
0018,9324	Estimated Dose Saving	Calculated by the system
0018,9345	CTDIvol	Calculated by the system
0018,9346	CTDIPhantomType-CodeSequence	Calculated by the system
>0008,0100	Code Value	Calculated by the system
>0008,0102	Code Scheme Designator	Calculated by the system
>0008,0104	Code Meaning	Calculated by the system
0018,9351	Calcium Scoring Mass Factor Patient	Calculated by the system
0018,9352	Calcium Scoring Mass Factor Device	Calculated by the system
0018,9353	Energy Weighting Factor	Weighting factor for primary system; only set if additional X-ray sources are used. The value is as entered for the scan.
0018,9360	CT Additional X-Ray Source Sequence	Filled if a second X-ray source was used
>0018,0060	> kVP	Voltage selected for scan
>0018,9330	>X-Ray Tube Current in mA	Tube current used for scanning in milliamperes
>0018,0090	>Data Collection Diameter	The diameter in mm of the region over which data was collected
>0018,1190	>Focal Spot(s)	Size of the focal spot actually used to generate x-ray radiation for a particular image. This is a single value expressed in mm.
>0018,1160	>Filter Type(s)	"WEDGE_2","WEDGE_3","WEDGE_2_3", "SN_DE","FLAT","AU_DESF","SN_DESF","AUSN_DESF" or combinations of "WEDGE_*" and "SN_DE"

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
>0018,7050	>Filter Material	Values: "TITANIUM", "TIN" or combinations
>0018,9332	>Exposure in mAs	(Effective) mAs. For spiral images, the product of exposure time and x-ray tube current is corrected with Table Feed per Rotation. This attribute is expressed in mAs.
>0018,9353	>Energy Weighting Factor	Weighting factor for secondary system. If the weighting factor is the weighting as entered for the scan, this value is 1-wf.
0019,00xx	Private Creator	Value: SIEMENS CT VA0 COAD
0019,xxB0	Feed per Rotation	Movement of table during one rotation in mm
		From MWL or created
0020,000D	Study Instance UID	Note: When Study Split is used, the value corresponding to the Requested Procedure Description selected in the Exam UI will be sent.
0020,000E	Series Instance UID	From MWL or created
		From MWL or created
0020,0010	Study ID	Note: When Study Split is used, the value corresponding to the Requested Procedure Description selected in the Exam UI will be sent.
0020,0011	Series Number	Created
0020,0012	Acquisition Number	Scan number within this examination
0020,0013	Instance Number	Created; direction within range selectable by user
0020,0032	Image Position (Patient)	The x, y, and z coordinates of the center of the first pixel, in mm
0020,0037	Image Orientation (Patient)	Calculated by the system
0020,0052	Frame of Reference UID	Created
0020,1040	Position Reference Indicator	Null length
		Topogram: Slice Location is defined as the relative table position of the start of the Topogram image expressed in mm.
0020,1041	Slice Location	Tomogram: Slice Location is defined as the relative position of the intersection of the image slice with the z-axis expressed in mm. This position is relative to the current reference point and corresponds to the table position.
0020,4000	Image Comments	According to user input; 2 lines supported
0021,00xx	Private Creator	Value: SIEMENS MED
0021,xx11	Target	Center x/y as entered for reconstruction
0028,0002	Samples per Pixel	Value: 1
0028,0004	Photometric Interpretation	Value: MONOCHROME2

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
0028,0010	Rows	Image Rows
0028,0011	Columns	Image Columns
0028,0030	Pixel Spacing	Calculated from FOV and Rows/Columns
0028,0100	Bits Allocated	Value: 16
0028,0101	Bits Stored	Value: 12
0028,0102	High Bit	Value: 11
0028,0103	Pixel Representation	Value: 0
0028,0106	Smallest Image Pixel Value	Calculated by examination
0028,0107	Largest Image Pixel Value	Calculated by examination
0028,1050	Window Center	Last windowing center saved; first window followed by second window
0028,1051	Window Width	Last windowing width saved; first window followed by second window
0028,1052	Rescale Intercept	Value -1024 for images without extended CT scale
0028,1053	Rescale Slope	Value 1 for images without extended CT scale
0028,1055	Window Center & Width Explanation	Value: "WINDOW1", "WINDOW2"
0028,2110	Lossy Image Compression	Lossy Image Compression will be set to 01 for the Extended Field of View because of low image quality. Derivation Description: "Reconstruction field larger than scan field".
0029,xxxx	(private data)	See 4.2 Privatizations on page 173
0029,xx40	Application Header Sequence	See 4.2 Privatizations on page 173
>0029,00xx	Private Creator	"SIEMENS MEDCOM HEADER"
>0029,xx41	Application Header Type	"SOM 5 TPOS"
>0029,xx42	Application Header ID	"SOM 5 NULLPOSITION"
>0029,xx43	Application Header Version	"VB10 20030626"
>0029,xx44	Application Header Info	Table Null Position coded as a null terminated character buffer
0032,1060	Requested Procedure Description	Input entered during patient registration or examination setup. Note: When Study Split is used, the value corresponding to the Requested Procedure Description selected in the Exam UI will be sent
0040,0260	PerformedProtocol-CodeSequence	Used for DataRoles received from <i>syngo.via</i>
>0040,0100	CodeValue	DataRoleCode received from <i>syngo.via</i>
>0040,0104	CodeMeaning	DataRole Meaning received from <i>syngo.via</i>

Table 75: Somaris/7 Attribute Interpretation

Tag	Name	Explanation
>0040,0102	MeaningCoding Scheme Designator	Fixed value: "99CT_VIA"
7FE0,0010	Pixel Data	

4.1.2.4 OOG, Overlays, High Bits

Graphics in Somaris/7 images are stored as Object Oriented Graphics (OOG) in private attributes (see 4.2.1.2.5 *MEDCOM OOG Module* on page 180). Non-syngo based systems are not expected to interpret this information.

In order to allow display access to graphic information for DICOM-based systems, private OOG information is converted on export into DICOM Overlay information stored in group 6000. This is the recommended way for a DICOM-based system to access overlay graphics information.

The following attributes are generated:

Overlay Rows (6000,0010)

Overlay Columns (6000,0011)

Number of Frames in Overlay (6000,0015)

Overlay Description (6000,0022) = "Siemens MedCom Object Graphics"

Overlay Type (6000,0040) = "G"

Origin (6000,0050) = 1, 1

Image Frame Origin (6000,0051)

Overlay Bits Allocated (6000,0100)

Bit Position (6000,0102)

Overlay Data (6000,3000)

However, DICOM Overlay information stored in group 6000 is not supported by all systems that might be used to store Somaris/7 images. These systems may not be able to display Somaris/7-generated overlays. For a special group of these systems, there is another way to provide graphical overlay information. A remote node can be configured to convert overlay graphics into unused pixel data above the High Bit (0028,0102) for images that fulfil the following conditions:

- Bits allocated (attribute 0028, 0100) = 16
- Bits stored (attribute 0028,0101) = 12
- High bit (attribute 0028,0102) = 11

Some systems are known to support this coding and are able to display this information with the images. Please note, however, that the proper and recommended way to store overlays with DICOM is using the group 6000.

4.2 Privatizations

4.2.1 Private Elements for Storage SOP Classes

The following private attributes are defined for all Siemens *syngo*-based applications.

4.2.1.1 Registry of DICOM Data Elements

Tag	Private Owner Code	Name	VR	VM
(0029,xx08)	SIEMENS CSA HEADER	CSA Image Header Type	CS	1
(0029,xx09)	SIEMENS CSA HEADER	CSA Image Header Version	LO	1
(0029,xx10)	SIEMENS CSA HEADER	CSA Image Header Info	OB	1
(0029,xx18)	SIEMENS CSA HEADER	CSA Series Header Type	CS	1
(0029,xx19)	SIEMENS CSA HEADER	CSA Series Header Version	LO	1
(0029,xx20)	SIEMENS CSA HEADER	CSA Series Header Info	OB	1
(0029,xx08)	SIEMENS CSA NON-IMAGE	CSA Data Type	CS	1
(0029,xx09)	SIEMENS CSA NON-IMAGE	CSA Data Version	LO	1
(0029,xx10)	SIEMENS CSA NON-IMAGE	CSA Data Info	OB	1
(0029,xx08)	SIEMENS CSA REPORT	<i>syngo</i> Report Type	CS	1
(0029,xx09)	SIEMENS CSA REPORT	<i>syngo</i> Report	LO	1
(0029,xx15)	SIEMENS CSA REPORT	SR Variant	US	1
(0029,xx17)	SIEMENS CSA REPORT	SC SOP Instance UID	UI	1
(0029,xx10)	SIEMENS CSA ENVELOPE	<i>syngo</i> Report Data	OB	1
(0029,xx11)	SIEMENS CSA ENVELOPE	<i>syngo</i> Report Presentation	OB	1
(0029,xx08)	SIEMENS MEDCOM HEADER	MedCom Header Type	CS	1
(0029,xx09)	SIEMENS MEDCOM HEADER	MedCom Header Version	LO	1
(0029,xx10)	SIEMENS MEDCOM HEADER	MedCom Header Info	OB	1
(0029,xx20)	SIEMENS MEDCOM HEADER	MedCom History Information	OB	1
(0029,xx31)	SIEMENS MEDCOM HEADER	PMTF Information 1	LO	1
(0029,xx32)	SIEMENS MEDCOM HEADER	PMTF Information 2	UL	1
(0029,xx33)	SIEMENS MEDCOM HEADER	PMTF Information 3	UL	1
(0029,xx34)	SIEMENS MEDCOM HEADER	PMTF Information 4	CS	1
(0029,xx35)	SIEMENS MEDCOM HEADER	PMTF Information 5	UL	1
(0029,xx40)	SIEMENS MEDCOM HEADER	Application Header Sequence	SQ	1
(0029,xx41)	SIEMENS MEDCOM HEADER	Application Header Type	CS	1

Tag	Private Owner Code	Name	VR	VM
(0029,xx42)	SIEMENS MEDCOM HEADER	Application Header ID	LO	1
(0029,xx43)	SIEMENS MEDCOM HEADER	Application Header Version	LO	1
(0029,xx44)	SIEMENS MEDCOM HEADER	Application Header Info	OB	1
(0029,xx50)	SIEMENS MEDCOM HEADER	Workflow Control Flags	LO	8
(0029,xx51)	SIEMENS MEDCOM HEADER	Archive Management Flag Keep Online	CS	1
(0029,xx52)	SIEMENS MEDCOM HEAD	Archive Management Flag Do Not Archive	CS	1
(0029,xx53)	SIEMENS MEDCOM HEADER	Image Location Status	CS	1
(0029,xx54)	SIEMENS MEDCOM HEADER	Estimated Retrieve Time	DS	1
(0029,xx55)	SIEMENS MEDCOM HEADER	Data Size of Retrieved Images	DS	1
(0029,xx70)	SIEMENS MEDCOM HEADER	Siemens Link Sequence	SQ	1
(0029,xx71)	SIEMENS MEDCOM HEADER	Referenced Tag	AT	1
(0029,xx72)	SIEMENS MEDCOM HEADER	Referenced Tag Type	CS	1
(0029,xx73)	SIEMENS MEDCOM HEADER	Referenced Value Length	UL	1
(0029,xx74)	SIEMENS MEDCOM HEADER	Referenced Object Device Type	CS	1
(0029,xx75)	SIEMENS MEDCOM HEADER	Referenced Object Device Location	OB	1
(0029,xx76)	SIEMENS MEDCOM HEADER	Referenced Object ID	OB	1
(0029,xx60)	SIEMENS MEDCOM HEADER2	Series Work Flow Status	LO	1
(0029,xx08)	SIEMENS MEDCOM OOG	MEDCOM OOG Type	CS	1
(0029,xx09)	SIEMENS MEDCOM OOG	MEDCOM OOG Version	LO	1
(0029,xx10)	SIEMENS MEDCOM OOG	MEDCOM OOG Info	OB	1
(7FE1,xx10)	SIEMENS CSA NON-IMAGE	CSA Data	OB	1

The following sub-sections explain in which IODs these private data elements are used.

4.2.1.2 All syngo-Supported Image SOP Classes

4.2.1.2.1 Extended Image IOD Module Table

Table 76: CSA Image IOD Modules

IE	Module	Reference	Usage	Note
Patient	Patient	[1] PS 3.3 C.7.1.1	M	
Study	General Study	[1] PS 3.3 C.7.2.1	M	
	Patient Study	[1] PS 3.3 C.7.2.2	U	
Series	General Series	[1] PS 3.3 C.7.3.1	M	
Equipment	General Equipment	[1] PS 3.3 C.7.5.1	U	
	General Image	[1] PS 3.3 C.7.6.1	M	
	Image Pixel	[1] PS 3.3 C.7.6.3	M	
	IOD specific modules	[1] PS 3.3 C.8.2.1	M/U	Depends on the IOD
Image	CSA Image Header	4.2.1.2.2 CSA Image Header Module on page 175	U	
	CSA Series Header	4.2.1.2.3 CSA Series Header Module on page 176	U	
	MEDCOM Header	4.2.1.2.4 MEDCOM Header Module on page 176	U	Private syngo information
	MEDCOM OOG	4.2.1.2.5 MEDCOM OOG Module on page 180	U	If object graphics are attached to image
	SOP Common	[1] PS 3.3 C.12.1	M	

4.2.1.2.2 CSA Image Header Module

The table in this section contains private IOD Attributes that describe the CSA Image Header.

Table 77: CSA Image Header Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Image Header Type	(0029,xx08)	SIEMENS CSA HEADER	1	CSA Image Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = Somaris/5 or Somaris/7

Table 77: CSA Image Header Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Image Header Version	(0029,xx09)	SIEMENS CSA HEADER	3	Version of CSA Image Header Info (0029,xx10) format.
CSA Image Header Info	(0029,xx10)	SIEMENS CSA HEADER	3	Manufacturer model-dependent information.

4.2.1.2.3 CSA Series Header Module

The table in this section contains private IOD Attributes that describe the CSA Series Header.

Table 78: CSA Series Header Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Series Header Type	(0029,xx18)	SIEMENS CSA HEADER	1	CSA Series Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = Somaris/5
CSA Series Header Version	(0029,xx19)	SIEMENS CSA HEADER	3	Version of CSA Series Header Info (0029,xx20) format.
CSA Series Header Info	(0029,xx20)	SIEMENS CSA HEADER	3	Manufacturer model-dependent information.

4.2.1.2.4 MEDCOM Header Module

The table in this section contains private IOD Attributes that describe the MEDCOM Header.

Table 79: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MED-COM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 Required if MedCom Header Info (0029,xx10) is present.
MedCom Header Version	(0029,xx09)	SIEMENS MED-COM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. Required if MEDCOM Header Info (0029,xx10) is present.

Table 79: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
MedCom Header Info	(0029,xx10)	SIEMENS MED-COM HEADER	3	Manufacturer model-dependent information. The value of the MedCom Header Info attribute (0029,xx10) can be built up in each user-defined format.
MedCom History Information	(0029,xx20)	SIEMENS MED-COM HEADER	3	MedCom-defined Patient Registration history information. See <i>4.2.1.2.4.1 MEDCOM History Information</i> on page 180.
PMTF Information 1	(0029,xx31)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 2	(0029,xx32)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 3	(0029,xx33)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 4	(0029,xx34)	SIEMENS MED-COM HEADER	3	Transformation Information
Application Header Sequence	(0029,xx40)	SIEMENS MED-COM HEADER	3	Sequence of Application Header Items. Zero or more Items are included in this sequence. Encoded as a sequence of items.
>Application Header Type	(0029,xx41)	SIEMENS MED-COM HEADER	1C	Application Header identification characteristics. Required if a sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MED-COM HEADER	3	Identification of an application header.
>Application Header Version	(0029,xx43)	SIEMENS MED-COM HEADER	3	Version of Application Header Info (0029,xx43) format.
>Application Header Info	(0029,xx44)	SIEMENS MED-COM HEADER	3	Application-dependent information.
Workflow Control Flags	(0029,xx50)	SIEMENS MED-COM HEADER	3	Eight freely definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS MED-COM HEADER	3	Flag to control a remote archive management system to keep the image always online (also when already archived). Enumerated values: 00 = remote control not required, 01 = keep image online.

Table 79: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS MED-COM HEADER	3	Flag to control a remote archive management system not to archive the related image. Enumerated values: 00 = remote control not required, 01 = do not archive image.
Image Location Status	(0029,xx53)	SIEMENS MED-COM HEADER	3	Image location status to control retrieving. Defined Terms: ONLINE = retrieving has to be done as usual, NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54), OFFLINE = invoking a retrieve operation initiates an operator request, INVALID = invoking a retrieve operation will always result in an error.
Estimated Retrieve Time	(0029,xx54)	SIEMENS MED-COM HEADER	3	Estimated retrieve time in seconds. A value less than zero (< 0) indicates that the location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS MED-COM HEADER	3	Data size of images in MByte.
Siemens Link Sequence	(0029,xx70)	SIEMENS MED-COM HEADER	3	Sequence of Link items. Each item identifies the location of one missing tag. One or more items can be located in this sequence.
Referenced Tag	(0029,xx71)	SIEMENS MED-COM HEADER	1	The referenced tag. The value of this tag is in the Child Data Object (CDO). Currently it is always Pixel Data (7FE0,0010).
Referenced Tag Type	(0029,xx72)	SIEMENS MED-COM HEADER	1	The value representation (type) of the missing tag (e.g. OW). Enumerated values are all DICOM-defined Value Representations.
Referenced Value Length	(0029,xx73)	SIEMENS MED-COM HEADER	1	The length of the referenced tag value in bytes.

Table 79: MEDCOM Header Module

Attribute Name	Tag	Private Creator	Type	Notes
Referenced Object Device Type	(0029,xx74)	SIEMENS MED-COM HEADER	1	<p>The Device Type that stores the Child Data Object (CDO) with the referenced tag value. Currently, it should be "SHMEM". In future, "SDM", "LOID" or "FILE" will also be possible.</p> <p>Defined Terms are</p> <p>SHMEM = Shared Memory</p> <p>SDM = Series Data Management</p> <p>LOID = Database</p> <p>FILE</p>
Referenced Object Device Location	(0029,xx75)	SIEMENS MED-COM HEADER	2	<p>The Location of the device that stores the Child Data Object (CDO) with the referenced tag value. For the "SHMEM" case, this is the shared memory directory.</p> <p>This can be empty, in which case the default directory is taken. In future, for "SDM" this will be the SDM_ID, for FILE it will be the directory name, and for "LOID" it will be the database name.</p>
Referenced Object ID	(0029,xx76)	SIEMENS MED-COM HEADER	1	<p>The ID of the object that contains the Child Data Object (CDO) with the referenced tag value. In case of "SHMEM", this is the shared memory ID.</p> <p>In future, for "SDM" this will be a Sirius OID, for "FILE" the file name, for "DB" the LOID.</p>
Series Work Flow Status	(0029,xx60)	SIEMENS MED-COM HEADER2	3	<p>syngo Patient Browser-specific flags used for clinical work:</p> <ul style="list-style-type: none"> - com = completed - rea = read - ver = verified

4.2.1.2.4.1 MEDCOM History Information

The value of the MEDCOM History Information attribute (0029,xx20) is defined as follows:

Table 80: MEDCOM History Information

Part	Name	Type	Bytes	Notes
header	Identifier	String	32	Always "CSA HISTORY"
	Version	String	32	For example "V1.10"
n items	Class Name	String	64	
	Modification String	String	1024	

4.2.1.2.5 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used when object graphics are drawn on the image and need to be stored as graphic object properties (Line, Circle, Rectangle, Arrow, and so on). Given the condition that the module contents were not removed by other modalities, the graphic objects remain re-animatable if such an image is transferred and is then retrieved back.

Table 81: MEDCOM OOG Module

Attribute Name	Tag	Private Creator	Type	Notes
MedCom OOG Type	(0029,xx08)	SIEMENS MEDCOM OOG	1	MEDCOM Object-Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1
MedCom OOG Version	(0029,xx09)	SIEMENS MEDCOM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format
MedCom OOG Info	(0029,xx10)	SIEMENS MEDCOM OOG	3	MEDCOM Object-Oriented Graphics (OOG) data

The graphics objects are also stored in one Image overlay plane for compatibility with other products that do not support the MedCom OOG module. Any system which does not support this MedCom OOG module has to remove these private attributes when modifying the image overlay plane content.

4.2.1.2.6 syngo Report Data

The module contains private IOD Attributes that describe *syngo* reports. This module is used when *syngo* report data is added to DICOM SR and DICOM SC objects.

Table 82: *syngo Report Data*

Attribute Name	Tag	Private Creator	Type	Notes
<i>syngo</i> Report Type	(0029,xx08)	SIEMENS CSA REPORT	1	<p><i>syngo</i> report characteristics, e.g. report creating application.</p> <p>Defined Terms:</p> <p>CT_CASCORING</p> <p>CT_CIRCULATION</p> <p>CT_LUNGCARE</p> <p>INSPACE</p> <p>MR_ARGUS</p> <p>This attribute value is used to identify the corresponding application during generic extension dll management. A restricted character set is used:</p> <p>Only A-Z and underscore are supported.</p>
<i>syngo</i> Report Version	(0029,xx09)	SIEMENS CSA REPORT	3	Version of <i>syngo</i> Report Data (0029,xx10) format
<i>syngo</i> Report Data	(0029,xx10)	SIEMENS CSA ENVELOPE	3	Application-specific report related data
<i>syngo</i> Report Presentation	(0029,xx11)	SIEMENS CSA ENVELOPE	3	Application-specific report related data

Table 82: syngo Report Data

Attribute Name	Tag	Private Creator	Type	Notes
SR Variant	(0029,xx15)	SIEMENS CSA REPORT		DICOM SR Variant. Enumerated Values: 0 = Basic Text SR (1.2.840.1008.5.1.4.1.1.88.11) 1 = Enhanced SR (1.2.840.1008.5.1.4.1.1.88.22) 2 = Comprehensive SR (1.2.840.1008.5.1.4.1.1.88.33) 3 = Mammography CAD SR (1.2.840.1008.5.1.4.1.1.88.50) 4 = Key Object Selection Document (1.2.840.1008.5.1.4.1.1.88.59) 5 = Chest CAD SR (1.2.840.1008.5.1.4.1.1.88.65)
SC SOP Instance UID	(0029,xx17)	SIEMENS CSA REPORT	3	DICOM SOP Instance UID of syngo- based SC image representing the syngo report object. This UID is used to identify the Resulting SC object after SR to SC conversion.

4.2.2 Private Elements for CT Image Storage SOP Class

The following private attributes are defined for Somaris/7.

4.2.2.1 Registry of DICOM Data Elements

Tag	Private Owner Code	Name	VR	VM	Notes
(0019,xx90)	SIEMENS CT VA0 COAD	Osteo Offset	DS	1	Offset of the water-equivalent material of the Siemens Osteo phantom to real water
(0019,xx92)	SIEMENS CT VA0 COAD	Osteo Regression Line Slope	DS	1	Slope of the regression line for the ESP (European Spine Phantom) standardization. If a scalefactor is defined for the in-scan reference phantom, this value contains the product of the scalefactor and the slope of the regression line for the ESP standardization.
(0019,xx93)	SIEMENS CT VA0 COAD	Osteo Regression Line Intercept	DS	1	Intercept of the regression line for the ESP (European Spine Phantom) standardization
(0019,xx96)	SIEMENS CT VA0 COAD	Osteo Phantom Number	IS	1	Number of the Siemens Osteo phantom
(0019,xxB0)	SIEMENS CT VA0 COAD	Feed per Rotation	DS	1	Som/4-style Feed per Rotation (Backwards Compatibility)
(0019,xxBD)	SIEMENS CT VA0 COAD	Pulmo Trigger Level	IS	1	Spirometer trigger level used for the scan, given in percent of VC (Vital Capacity) of the patient
(0019,xxBE)	SIEMENS CT VA0 COAD	Expiratoric Reserve Volume	DS	1	ERV (Expiratoric Reserve Volume) achieved by the patient
(0019,xxBF)	SIEMENS CT VA0 COAD	Vital Capacity	DS	1	VC (Vital Capacity) achieved by the patient
(0019,xxC0)	SIEMENS CT VA0 COAD	Pulmo Water	DS	1	Density of the water insert of the Siemens Pulmo phantom
(0019,xxC1)	SIEMENS CT VA0 COAD	Pulmo Air	DS	1	Density of the air holes of the Siemens Pulmo phantom
(0019,xxC2)	SIEMENS CT VA0 COAD	Pulmo Date	DA	1	Date of the evaluation of the Siemens Pulmo phantom

Tag	Private Owner Code	Name	VR	VM	Notes
(0019,xxC3)	SIEMENS CT VA0 COAD	Pulmo Time	TM	1	Time of the evaluation of the Siemens Pulmo phantom
(0021xx11)	SIEMENS MED	Target	DS	2	Som/4-style Target (Backwards Compatibility)
0009,00xx	SIEMENS CT VA1 DUMMY	Private Creator Data Element	LO	1	1

4.2.3 Private SOP class CSA Non-Image

This chapter includes the definition of the Siemens AG B Med CSA-defined private Non-Image Object (called CsaNonImage IOD). The focus of this private Non-Image Object is to address the requirement for non-image data sets found in *syngo*-based applications.

The MedCom Non-Image Information Object Definition specifies data sets that are converted from a non-DICOM format to a modality-independent DICOM format.

Examples of such manufacturer model-dependent data sets are:

- Raw Data
- CT Admin Data
- MR Spectroscopy Data
- Etc.

4.2.3.1 CSA Non-Image IOD Entity Relationship Model

The E-R model in [DICOM] A.1.2 depicts those components of the DICOM Information Model that directly refer to the CSA Non-Image IOD. The frame of reference IE, overlay IE, modality lookup table IE, VOI lookup table IE and curve IE are not components of the CSA Non-Image IOD.

```

classDiagram
    class PatientIOD["Patient IOD"]
    class VisitIOD["Visit IOD"]
    class StudyIOD["Study IOD"]
    class StudyComponentIOD["Study Component IOD"]
    class ImageIOD["Image IOD"]
    class ImageOverlayBoxIOD["Image Overlay Box IOD"]
    class ImageBoxIOD["Image Box IOD"]
    class FilmBoxIOD["Film Box IOD"]
    class FilmSessionIOD["Film Session IOD"]
    class PrinterIOD["Printer IOD"]
    class PrintJobIOD["Print Job IOD"]
    class CSANonImageIOD["CSA Non-Image IOD"]
    class StandaloneModLUTIOD["Stand-alone Mod. LUT IOD"]
    class StandaloneVOILUTIOD["Stand-alone VOI LUT IOD"]
    class StandaloneOverlayIOD["Stand-alone Overlay IOD"]
    class StandaloneCurveIOD["Stand-alone Curve IOD"]
    class BasicStudyDescriptorIOD["Basic Study Descriptor IOD"]
    class ResultsIOD["Results IOD"]
    class InterpretationIOD["Interpretation IOD"]
    class VOILUTBoxIOD["VOI LUT Box IOD"]
    class AnnotationIOD["Annotation IOD"]

    PatientIOD --> VisitIOD : references (1 to 1-n)
    VisitIOD --> StudyIOD : references (1 to 1-n)
    StudyIOD --> StudyComponentIOD : comprised of (1 to 1-n)
    StudyIOD --> ImageIOD : references (1 to 0-n)
    StudyIOD --> ResultsIOD : see note (1 to 0-n)
    StudyIOD --> InterpretationIOD : references (1 to 0-1)
    StudyIOD --> CSANonImageIOD : 0-n
    StudyIOD --> StandaloneModLUTIOD : 0-n
    StudyIOD --> StandaloneVOILUTIOD : 0-n
    StudyIOD --> StandaloneOverlayIOD : 0-n
    StudyIOD --> StandaloneCurveIOD : 0-n
    StudyIOD --> ImageOverlayBoxIOD : 1-n
    StudyIOD --> ImageBoxIOD : 1-n
    StudyIOD --> FilmBoxIOD : 1-n
    StudyIOD --> FilmSessionIOD : 1-n
    StudyIOD --> AnnotationIOD : 0-n

    ImageIOD --> ImageOverlayBoxIOD : references (1 to 1-n)
    ImageIOD --> ImageBoxIOD : references (1 to 1-n)
    ImageIOD --> FilmBoxIOD : references (1 to 1-n)
    ImageIOD --> FilmSessionIOD : references (1 to 1-n)
    ImageIOD --> AnnotationIOD : 0-n

    ImageOverlayBoxIOD --> ImageBoxIOD : references (1 to 1-n)
    ImageBoxIOD --> FilmBoxIOD : references (1 to 1-n)
    FilmBoxIOD --> FilmSessionIOD : references (1 to 1-n)
    FilmSessionIOD --> AnnotationIOD : contains (1 to 0-n)

    PrinterIOD --> PrintJobIOD : prints (1 to 0-1)
    PrintJobIOD --> FilmSessionIOD : is tracked by (1 to 1-n)
  
```

Table 83: 3CSA Non-Image IOD Modules

IE	Module	Reference	Usage
Patient	Patient	[1] PS3.3 C.7.1.1	M
Study	General Study	[1] PS3.3 C.7.2.1	M
	Patient Study	[1] PS3.3 C.7.2.2	U
Series	General Series	[1] PS3.3 C.7.3.1	M
Equipment	General Equipment	[1] PS3.3 C.7.5.1	U

Table 83: 3CSA Non-Image IOD Modules

IE	Module	Reference	Usage
CSA	CSA Image Header	4.2.1.2.2 CSA Image Header Module on page 175	U
	CSA Series Header	4.2.1.2.3 CSA Series Header Module on page 176	U
	MEDCOM Header	4.2.1.2.4 MEDCOM Header Module on page 176	U
	CSA Non-Image	4.2.3.3 CSA Non-Image Module on page 187	M
	SOP Common	[1] PS3.3 C.12.1	M

4.2.3.3 CSA Non-Image Module

The table in this section contains private IOD Attributes that describe CSA Non-Images.

Table 84: CSA Non-Image Module

Attribute Name	Tag	Private Creator	Type	Notes
Image Type	(0008,0008)	-	3	Image-identification characteristics. See 4.2.3.4 CT Extensions of the Non-Image Object on page 189.
Acquisition Date	(0008,0022)	-	3	The start date for acquisition of data that resulted in this data set
Acquisition Time	(0008,0032)	-	3	The start time for acquisition of data that resulted in this data set
Conversion Type	(0008,0064)	-	3	Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation.
Referenced Image Sequence	(0008,1140)	-	3	A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as a sequence of items: (0008,1150) and (0008,1155).
Derivation Description	(0008,2111)	-	3	A text description of how this data set was derived

Table 84: CSA Non-Image Module

Attribute Name	Tag	Private Creator	Type	Notes
Source Image Sequence	(0008,2112)	-	3	<p>A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to derive this data set.</p> <p>Zero or more Items may be included in this Sequence.</p> <p>Encoded as a sequence of items: (0008,1150) and (0008,1155).</p>
Patient Position	(0018,5100)	-	3	Patient position descriptor relative to the equipment
Acquisition Number	(0020,0012)	-	3	A number identifying the gathering of data over a period of time which resulted in this data set
Instance Number	(0020,0013)	-	3	A number that identifies this data set
Frame of Reference UID	(0020,0052)	-	3	Uniquely identifies the frame of reference for a Series
Image Comments	(0020,4000)	-	3	User-defined comments about the image
Quality Control Image	(0028,0300)	-	3	<p>Indicates whether or not this image is a quality control or a phantom image.</p> <p>If this Attribute is not available, then the image may or may not be a quality control or a phantom image.</p> <p>Enumerated Values: YES, NO.</p>
Burned In Annotation	(0028,0301)	-	3	<p>Indicates whether or not the image contains sufficient burned-in annotation to identify the patient and date the image was acquired.</p> <p>If this Attribute is not available, then the image may or may not contain burned-in annotation.</p> <p>Enumerated Values: YES, NO.</p>
Lossy Image Compression	(0028,2110)	-	3	<p>Specifies whether an Image has been subjected to lossy compression.</p> <p>Enumerated Values: 00 = Image has NOT been subjected to lossy compression, 01 = Image has been subjected to lossy compression.</p>
Lossy Image Compression Ratio	(0028,2112)	-	3	<p>Describes the approximate lossy compression ratio(s) that have been applied to this image.</p> <p>May be multi-valued if successive lossy compression steps have been applied.</p>

Table 84: CSA Non-Image Module

Attribute Name	Tag	Private Creator	Type	Notes
CSA Data Type	(0029,xx08)	SIEMENS CSA NON-IMAGE	1	CSA Data identification characteristics. Defined Terms: RAW DATA NUM 4 = NUMARIS/4 Raw Data SPEC NUM 4 = NUMARIS/4 Spectroscopy RAW DATA SOM 5 = Somaris/5 Raw Data RAW DATA SOM 7 = Somaris/7 Raw Data BSR REPORT = BSR Study Report Data COL REPORT SOM5 = syngo Colonography Report Data
CSA Data Version	(0029,xx09)	SIEMENS CSA NON-IMAGE	3	Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format.
CSA Data Info	(0029,xx10)	SIEMENS CSA NON-IMAGE	3	Information describing the CSA Data (7FE1,xx10). The value of the CSA Data Info attribute (0029,xx10) can be built up in each user-defined format.
CSA Data	(7FE1,xx10)	SIEMENS CSA NON-IMAGE	1	Binary data as a byte stream

4.2.3.4 CT Extensions of the Non-Image Object

Somaris/7 uses the following defined terms for the Image Type (0008,0008):

- Value 1: ORIGINAL
- Value 2: PRIMARY
- Value 3: AXIAL, LOCALIZER, OTHER
- Value4: a CT_SOM5 * enumeration
- Value5: Somaris/7-specific enumeration

The following table lists the Somaris/7 non-image types and the corresponding combinations of the Image Type Attribute values:

Table 85: (Non-)Image Type (0008,0008) for private Somaris/7 Non-image Objects

Description	0008,0008 Value 1	0008,0008 Value 2	0008,0008 Value 3	0008,0008 Value 4	0008,0008 Value 5
CAD Results	DERIVED	SECONDARY	OTHER	CAD MARKS	None
Colonography Data	DERIVED	SECONDARY	OTHER	CT_SOM5 COL	None
Coronary Tree	DERIVED	SECONDARY	OTHER	CT_CIRCULATION	None
Raw Data	Same entries as for images				

4.2.4 Private SOP Classes

Table 86: SOP Classes

SOP Class Name	SOP Class UID
CSA Non-Image	1.3.12.2.1107.5.9.1

4.2.5 Private Transfer Syntaxes

Not applicable

5 Communication Profiles

5.1 Supported Communication Stacks

The Somaris/7 DICOM application provides DICOM V3.0 TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.

The product target operating system is Windows 10.

5.1.1 OSI Stack

Not supported.

5.1.2 TCP/IP Stack

The Somaris/7 DICOM application uses the TCP/IP stack from the Windows 10 system. It uses the MergeCOM-3 sub-routine library from Merge Technologies Inc., which is based on a Berkeley socket interface.

5.1.2.1 API

The Somaris/7 DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

5.1.2.2 Physical Media Support

The Somaris/7 DICOM application is indifferent to the physical medium over which TCP/IP executes. It inherits this from the target operating system upon which it executes.

5.1.3 Point-to-Point Stack

Not supported.

6 Configuration

6.1 AE Title / Presentation Address Mapping

According to the DICOM Standard, the AET string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters).

Note

The current implementation does not support the full DICOM standard syntax. Spaces and special characters (such as &<>) in the AE title string are not supported.

Change of the default AE Titles chosen by the system can be performed in the Service UI under

“Configuration / DICOM / General” item - first page.

Table 87: Default AET Characteristics

Appication Entity	Default AET	TCI/IP Port
Verification SCU	RANDOM_STR_SEC RANDOM_STR	-
Verification SCP		2762 (fixed) 104 (fixed)
Storage SCU		-
Storage SCP		2762 (fixed) 104 (fixed)
Query/Retrieve SCU		-
Query/Retrieve SCP		2762 (fixed) 104 (fixed)
Print SCU	RANDOM_STR	-
Worklist SCU	RANDOM_STR	-
MPPS SCU		-

Port 2762 is used for Secure DICOM Communication and Port 104 is used for Unsecure DICOM Communication.

There are two AET for Storage SCP, Verification SCP and Query/Retrieve SCP. RANDOM_STR and RANDOM_STR_SEC denote the randomly generated AE Titles. RANDOM_STR_SEC denotes the AET value for Secure DICOM communication.

6.1.1 DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. For example, Verification uses the Storage AE, if initiated to check the configuration of a remote DICOM node.

6.1.2 DICOM Storage/StorageCommitment/QR AE Title

There is a common AE Title for the Storage, Storage Commitment and Query/Retrieve services. This can be configured via the Service UI in Configuration/DICOM/General.

The port is set to the fixed value of 104.

6.1.3 DICOM Modality Worklist and MPPS AE Title

There is a common AE Title for the Modality Worklist and MPPS services. This can be configured via the Service UI in Configuration/DICOM/General.

6.1.4 DICOM Print AE Title

There is a separate AE Title for the Print application. This can be configured via the Service UI in Configuration/DICOM/General.

Input of AETs starting with a numeric character is not possible.

6.1.5 Remote AE Titles and Presentation Addresses

Remote AETs, host names, IP addresses and port numbers can be configured using the Service application. For each AET, a list of supported services can be configured.

6.2 Configurable Parameters

The Application Entity Titles, host names and port numbers for remote AE are configured using the Somaris/7 Service/Installation Tool. For each AET, the list of services supported can be configured.

6.2.1 Storage, Storage Commitment and Query/Retrieve

- "a quality factor which determines the proposed transfer syntax in case that a user has initiated C-STORE. By convention, 0 means that only Uncompressed Transfer Syntax(es) are proposed, 100 means that the Lossless Transfer Syntax is proposed, and any other value between 1 and 99 means that a JPEG Lossy Transfer Syntax is proposed. One Uncompressed Transfer Syntax will be proposed in any case. This parameter is a general one for all destination nodes.
- "a "compression type supported" which determines the proposed transfer syntax in case the C-STORE was initiated as a sub-operation of an incoming C-MOVE-RQ. By convention, 0 means that only Uncompressed Transfer Syntax(es) are proposed, 1 means that the Lossless Transfer Syntax is proposed, and 2 means that a JPEG Lossy Transfer Syntax is proposed. One uncompressed transfer syntax will be proposed in any case. This parameter can be set for each configured destination node.

Note

By default, association requests are accepted by the SCP regardless of the value of the DICOM Application Context Name set in the requests.

This behavior can be changed by modifying the value of the `ACCEPT_ANY_CONTEXT_NAME` entry in the `mergecom.pro` configuration file of the MergeCOM-3 toolkit. If the value is `FALSE`, association requests are accepted only when the DICOM Application Context Name is set to "1.2.840.10008.3.1.1.1" (see DICOM specification PS 3.7-2003, A.2.1).

Additional configurable parameters for the Storage Commitment service:

When acting as an SCU:

- Flag to indicate whether the association will be kept open to receive the response, or to close the association and be prepared to receive the response on another association
- Time-out which defines how long the association of N-ACTION is kept to receive an N-EVENT-REPORT on the same association. The same value is used to wait for an N-EVENT-REPORT on another association (applicability of transaction UID).
(default 1 h)

When acting as an SCP:

- Flag to indicate whether an archive system is installed

6.2.2 Print

The Service application can be used to configure the SCP (DICOM printer).

It is mandatory to set these parameters:

- AET
- Host name
- IP address
- Port number

These parameters have defaults as per configuration file and can be changed:

- Default camera
- Pixel size
- Additional or changed film sheet formats (for example, inch 14x14, inch 14x17, ...)
- List mapping pixel size to each film sheet format
- Minimum density
- Stored printed film jobs
- Media type
- Film destination

6.2.3 Modality Worklist

The Service application can be used to set the AETs, port numbers, host names, IP addresses, capabilities, and time-outs for the remote nodes (SCPs).

Additional configurable parameters for the Basic Worklist Query:

- Query Waiting time - the time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default 20 s)
- Max. Query Match Number - the maximum number of entries accepted in one worklist (default is 200)
- Query Interval - the time between two C-FIND-RQs to the Hospital Information System (default is 60 min.)
 - Broad Worklist Query behaviour; two values are defined:
 - Set the AE Title search attribute to the own AE Title, and the Modality search attribute to "**".
 - Set the Modality search attribute to the own modality and the AE Title search attribute to "**".

The sending of an empty Specific Character Set in a C-FIND-RQ can be omitted by configuration. However, this is not available in the Service application but must be set by a Siemens service technician.

6.2.4 Modality Performed Procedure Step

The Service application can be used to configure the Modality Worklist SCP to also be a Modality Performed Procedure Step SCP.

Additional configurable parameters for the Modality Performed Procedure Step:

- Default Catalog Name - (0008,0102) used for items entered in the MPPS UI
- Default Catalog Version - (0008,0103) used for items entered in the MPPS UI

6.3 Default Parameters

This configuration tool also uses some default parameters:

- Maximum PDU size set to 262144 Bytes
 - Time-out for accepting/rejecting an association request: 60 s
 - Time-out for responding to an association open/close request: 60 s
 - Time-out for accepting a message over the network: 60 s
 - Time-out for waiting for data between TCP/IP packets: 60 s

The Time-outs for waiting for a Service Request/Response message from the remote node are as follows:

- For Storage SCP/SCU: 600 s
 - For the Storage Commitment SCU:
 - Time-out for Response to N-ACTION: 600 s
 - Time-out for N-EVENT-REPORT: configurable, see *6.2 Configurable Parameters* on page 193
- For Query/Retrieve SCP/SCU: 600 s
- For Modality Worklist SCU: configurable, see *6.2 Configurable Parameters* on page 193.
- For Print Management SCU:
 - Time-out for Response to N-SET-RQ: 240 s
 - Time-out for Response to other Requests: 60 s

7 Support of Extended Character Sets

The Somaris/7 DICOM application supports the following character sets as defined in the four tables below:

Table 88: Single-Byte Character Sets without Code Extension

Character Set Description	Defined Term	ISO Registration Number	Character Set
Default repertoire	None	ISO_IR 6	ISO 646
Latin alphabet no. 1	ISO_IR 100	ISO_IR 100 ISO_IR 6	Supplementary set ISO 646
Latin alphabet no. 2	ISO_IR 101	ISO_IR 101 ISO_IR 6	Supplementary set ISO 646
Latin alphabet no. 3	ISO_IR 109	ISO_IR 109 ISO_IR 6	Supplementary set ISO 646
Latin alphabet no. 4	ISO_IR 110	ISO_IR 110 ISO_IR 6	Supplementary set ISO 646
Cyrillic	ISO_IR 144	ISO_IR 144 ISO_IR 6	Supplementary set ISO 646
Arabic	ISO_IR 127	ISO_IR 127 ISO_IR 6	Supplementary set ISO 646
Greek	ISO_IR 126	ISO_IR 126 ISO_IR 6	Supplementary set ISO 646
Hebrew	ISO_IR 138	ISO_IR 138 ISO_IR 6	Supplementary set ISO 646
Latin alphabet no. 5	ISO_IR 148	ISO_IR 148 ISO_IR 6	Supplementary set ISO 646
Japanese	ISO_IR 13	ISO_IR 13 ISO_IR 14	JIS X 0201:Katakana JIS X 0201:Romaji

Table 89: Single-Byte Character Sets with Code Extension

Character Set Description	Defined Term	Standart for Code Extension	ESC Sequence	ISO Registration Number	Character Set
Default repertoire	ISO 2022 IR 6	ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet no.1	ISO 2022 IR 100	ISO 2022	ESC 02/13 04/01	ISO_IR 100	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet no.2	ISO 2022 IR 101	ISO 2022	ESC 02/13 04/02	ISO_IR 101	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet no.3	ISO 2022 IR 109	ISO 2022	ESC 02/13 04/03	ISO_IR 109	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet no.4	ISO 2022 IR 110	ISO 2022	ESC 02/13 04/04	ISO_IR 110	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Cyrillic	ISO 2022 IR 144	ISO 2022	ESC 02/13 04/12	ISO_IR 144	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Arabic	ISO 2022 IR 127	ISO 2022	ESC 02/13 04/07	ISO_IR 127	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Greek	ISO 2022 IR 126	ISO 2022	ESC 02/13 04/06	ISO_IR 126	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Hebrew	ISO 2022 IR 138	ISO 2022	ESC 02/13 04/08	ISO_IR 138	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet no.5	ISO 2022 IR 148	ISO 2022	ESC 02/13 04/13	ISO_IR 148	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Japanese	ISO 2022 IR 13	ISO 2022	ESC 02/13 04/09	ISO_IR 13	JIS X 0201:Katakana
		ISO 2022	ESC 02/08 04/02	ISO_IR 14	JIS X 0201-1976:Romaji

Table 90: Multi-Byte Character Sets without Code Extension

Character Set Description	Defined Term	ISO Registration Number	Character Set
Unicode	ISO_IR 192	ISO 10646	Unicode in UTF-8
Chinese	GB18030	GB18030	GB 18030-2000 (China Association for Standardization)

Table 91: Multi-Byte Character Sets with Code Extension

Character Set Description	Defined Term	Standard for Code Extension	ESC Sequence	ISO Registration Number	Character Set
Japanese	ISO 2022 IR 87	ISO 2022	ESC 02/04 04/02	ISO_IR 87	JIS X 0208: Kanji
	ISO 2022 IR 159	ISO 2022	ESC 02/04 02/08 04/04	ISO_IR 159	JIS X 2012: Supplementary Kanji set
Chinese ^a	ISO 2022 IR 58	ISO 2022	ESC 02/04 04/01	ISO_IR 58	GB2312-80 (China Association for Standardization)

^a. This Character Set is an extension of DICOM for the Chinese language.

When a mismatch exists between the SCS tags (0008,0005) and the characters in an IOD coming into the system, then the following measures are taken to make the characters DICOM-conform:

- Try to import with ISO-IR 100. If ISO-IR 100 also fails, convert each illegal character to '?'.

There are now 3 categories of character sets which have to be differentiated because of their different encoding formats:

- Conventional ISO character sets: ISO_IR 6, ISO 2022 IR 6, ISO_IR 100, etc. =>Encoded in ISO 2022
- ISO_IR 192: Encoded in UTF-8
- GB18030: Encoded in GB18030

It is not possible to recognize the following mismatches automatically on receiving or importing:

- An attribute value is encoded in ISO_IR 192 <=> (0008,0005) contains a conventional ISO character set as the primary character set
- An attribute value is encoded in GB18030 <=> (0008,0005) contains a conventional ISO character set as the primary character set
- An attribute value is encoded in ISO 2022 <=> (0008,0005) contains ISO_IR 192
- An attribute value is encoded in ISO 2022 <=> (0008,0005) contains GB18030

An IOD that contains one of the above mentioned inconsistencies is not DICOM-conform. As these kinds of inconsistencies cannot be recognized by the system, the IOD is not rejected, but the character data might be corrupted.

Older versions of syngo do not support the newly introduced character sets ISO_IR 192 and GB18030, and their special encodings. This means that an IOD which contains one of these new character sets in (0008,0005) will be rejected by an older syngo system.

8 Security

8.1 Security Profile

The Somaris/7 DICOM application conforms to the IHE Basic Security Integration Profile that is used for the DICOM Communication.

Syngo allows the use of either a conventional (non-secure) DICOM communication or a secure DICOM communication. For secure DICOM communication syngo application uses Transport Layer Protocol (TLS v1.1 and TLS v1.2). Following features are supported for the secure DICOM communication.

The port in which syngo acts as SCP for secure DICOM communication is 2762 (fixed). The port in which syngo acts as SCP for unsecure DICOM communication is 104 (fixed). The following security profile are done in syngo using TLS 1.1 and TLS v1.2 protocol

- Secure authentication of node
- Integrity and confidentiality of transmitted data.
- Generation of audit trail records access control and user authentication.

8.1.1 Security Transport Connection Profiles

Somaris/7 conforms to the Basic TLS Transport Connection Profile. Somaris/7 initiates the TLS connections and accepts TLS connections with Storage commitment.

Somaris/7 provides a configuration panel by which local systems can configure the certificate that needs to bind for DICOM communication. Secure communication is a “mode of operation” of syngo supported by the implementation of the DICOM Basic TLS Secure Transport Connection Profile. This functionality will be used by the nodes that can authenticate each other before they exchange DICOM information. For secure communication the TLS protocol is used which provides message authentication, integrity and confidentiality.

Somaris/7 supports X.509 certificates. The type of X.509 certificates that are supported in this Somaris/7 are

1. Self Signed certificate
2. Certificate for which chain building (Trusted chain building, Trusted CA) is possible.

The following TLS certification checks will be done (TLS Handshake). The machine (either server or client) that will send its certificate will:

- Choose the certificate according to Common Name (CN), if the syngo self signed is used. If customer specific certificate needs to be used then Serial Number of the certificate is used for choosing the certificate.

The server verifies

- that the client certificate is X.509 certificate which is not tampered with
- that the client certificate is in the list of trusted certificates (Trust Chain Building)
- that the client certificate is not in the revoked list.
- that the client certificate is not expired (present time is between "Valid From" and "Valid To" fields of X.509 certificate)
- that the client certificate has the correct purpose (at least the client authentication purpose).

The client verifies:

- that the server certificate is a X.509 certificate which is not tampered with
- that the server certificate is in the list of trusted certificates (Trust Chain Building)
- that the server certificate is not in the revoked list.
- that the server certificate is not expired (present time is between "Valid From" and "Valid To" fields of X.509 certificate)
- that the server certificate has the correct purpose (at least the server authentication purpose).

No verification is done on certificate for

1. Direct certificate validation
2. Certificate received from peer have multiple X.509 certificates within the TLS Handshake.

The X.509 certificate imported and used for DICOM communication

1. must have purpose set for Client and Server Authentication.
2. must be exportable to generate the certificate file and private key file.

If intermediate and root X.509 certificates are present then the intermediate certificate must be imported to Intermediate Certificate Authorities -> Certificates. The root certificate must be imported to the Trusted Root Certificates -> Certificates.

Somaris/7 communicates with either of the following Cipher suites for encrypting the data send across the network:


TLS_RSA_WITH_AES_128_CBC_SHA

TLS_RSA_WITH_3DES_EDE_CBC_SHA

Note

There is no support for NULL Cipher(TLS_RSA_WITH_NULL_SHA).

Fig. 12: TLS Handshake Message Protocol

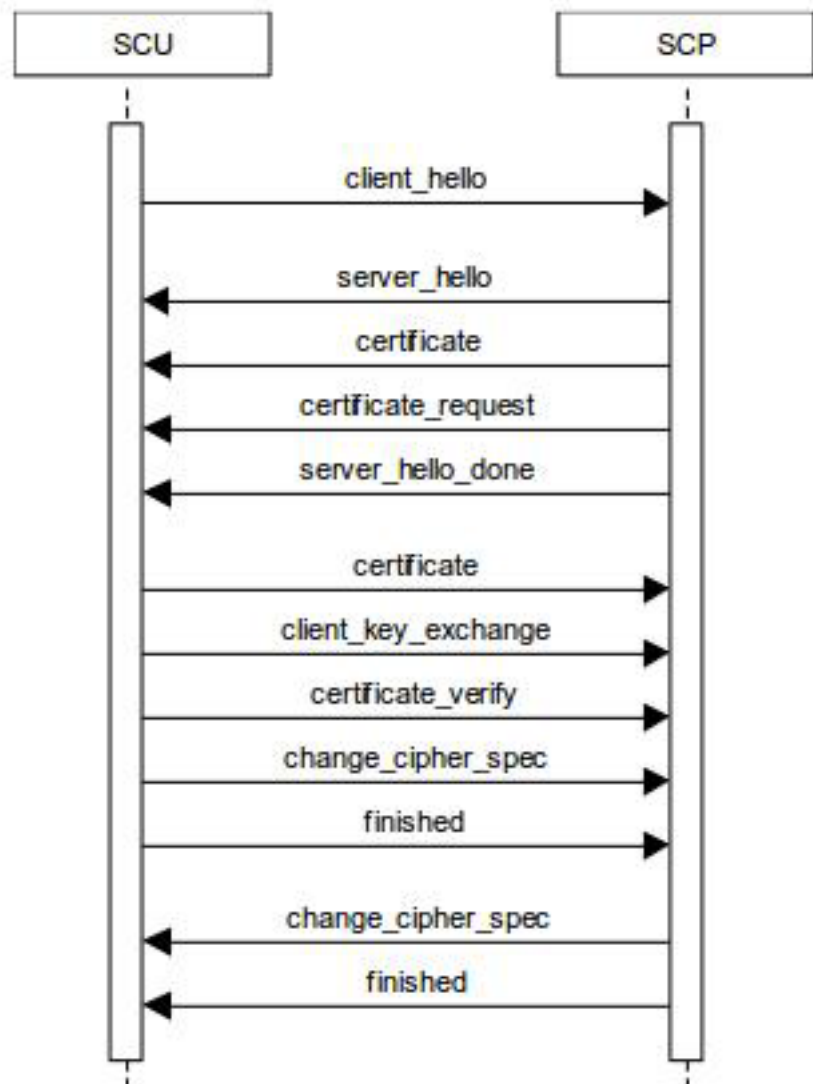

Part II - Media Storage

This part contains the Conformance Statement to all "Offline Media Application Profiles (incl. private extensions)" supported by the Somaris/7 archive options.


The application profiles supported are:

- Standard Application Profiles
- Augmented Application Profiles
- syngo private Application Profiles

For general introductory topics, see [1] *DICOM® Standards Publication Part(s) 3, 4, ©NEMA Standard is under continuous maintenance, the current official version is available at: <http://dicom.nema.org> on page 15.*

9 Implementation Models

9.1 Application Data Flow Diagram

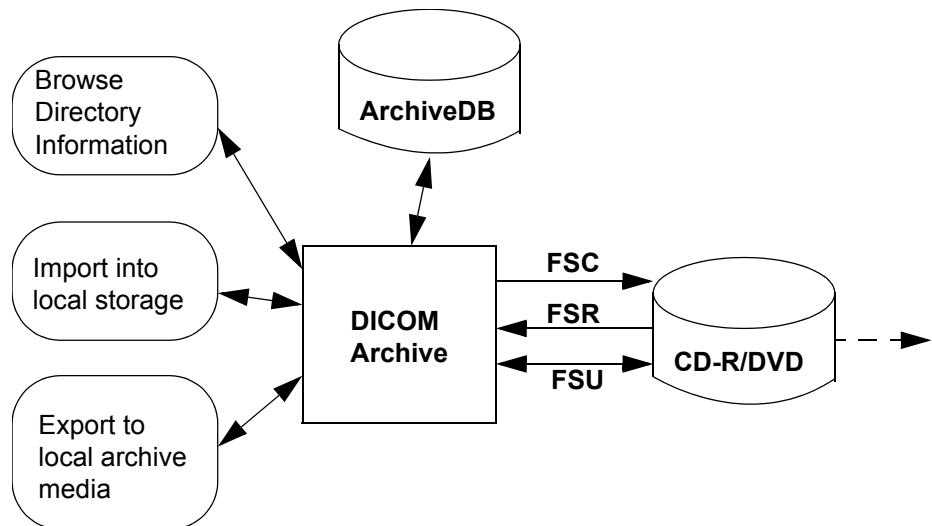

The DICOM archive application serves as an interface to the CD-R/DVD off-line medium device. It provides interfaces to include the off-line media directory into the browser and to copy SOP instances to a medium or retrieve SOP instances from the medium into local storage.

The DICOM Archive application supports 120 mm CD-R and DVD-R (see *Table 92: Application profiles, Activities, and Roles for the DICOM Archive application* on page 207).

The FSU role updates new SOP instances only to media with pre-existing File sets conforming to the Application Profiles supported.

The contents of the DICOMDIR are temporarily stored in the Archive-Database.

9.2 Functional definitions of AEs

The Somaris/7 DICOM off-line media storage application consists of the DICOM Archive application entity serving all interfaces to access off-line media. The DICOM Archive application is capable of the following:

1. Creating a new File set on an unwritten medium (Export to...)
2. Updating an existing File set by writing new SOP instances on the medium (Export to...)
3. Importing SOP instances from the medium to local storage
4. Reading the File set's DICOMDIR information temporarily into the database and passing it to display applications

9.3 Sequencing of Real-World Activities

The DICOM Archive application does not perform updates before the Directory information of the DICOMDIR has been completely read.

When performing updates, the existence of SOP instances is checked before updating. Duplicate instances are avoided.

9.4 File Meta Information Options

Implementation Class UID	1.3.12.2.1107.5.1.4
Implementation Version Name	SIEMENS_S7VB10A

10 AE Specifications

10.1 DICOM Archive Specification

The DICOM Archive application provides Standard conformance to the Media Storage Service Class (Interchange Option).

Table 92: Application profiles, Activities, and Roles for the DICOM Archive application

Application Profiles Supported	Real-World Activity	Role	SC Option
PRI-SYNGO-CD	Browse Directory Information	FSR	Interchange
PRI-SYNGO-DVD	Import into local Storage	FSR	Interchange
AUG-GEN-CD			
AUG-CTMR-CD ^a	Export to local archive media	FSC,FSU	Interchange
STD-XA1K-CD ^a			
STD-GEN-CD	Browse Directory Information	FSR	Interchange
STD-CTMR-CD			
STD-XABC-CD			
STD-XA1K-CD	Import into local Storage	FSR	Interchange
TD-US-zz-yF-xxxxxx ^b			

^a. With no private SOP Class used, the PRI-SYNGO-CD profile definitions are appropriate to describe the augmentation of the related STD Profiles.

^b. All combinations of the following values for zz, yF and xxxxxx are supported:

'yF' can take two values: SF for Single Frame and MF for Multi-Frame.

'zz' can take three values: ID (Image Display), SC (Spatial Calibration) or CC (Combined Calibration)

xxxxxx can take 2 values: CDR and DVD

On syngo-based products, the Private Extended syngo Profile (for example, PRI-SYNGO-CD) is preferred for use by the system. The General Purpose Interchange Profile (STD-GEN-CD), Ultrasound Profile (STD-US-xxx), CT and MR Image Profile (STD-CTMR-xxx), Waveform Interchange (STD-WVFM-xxx), Basic Cardiac Profile (STD-XABC-CD) and 1024 X-Ray Angiographic Profile (STD-XA1K-CD) are supported with read capability of the related media.

10.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See 6 *Configuration* on page 192 for details.

10.1.2 Real-World Activities for this Application Entity

10.1.2.1 Real-World Activity: Browse Directory Information

The DICOM Archive application acts as an FSR using the interchange option when requested to read the media directory.

The DICOM archive application reads the DICOMDIR and inserts the directory entries that are valid for the application profiles supported into a local database. The database can then be used to browse media contents.

Note

Icon Image SQ is also supported in DICOMDIR. However, only those Icon Images with Bits Allocated (0028,0100) equal to 8 and a size of 64 x 64 or 128 x 128 pixels are imported into the database and are visible in the Patient Browser.

10.1.2.1.1 Application Profiles for the RWA: Browse Directory Information

See *Table 92: Application profiles, Activities, and Roles for the DICOM Archive application* on page 207 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

10.1.2.2 Real-World Activity: Import into local Storage

The DICOM Archive application acts as an FSR using the interchange option when requested to read SOP Instances from the medium to the local storage.

The SOP Instance selected from the media directory is copied into the local storage. Only SOP Instances that are valid for the application profile supported and that are listed as supported by the Storage SCP Conformance section (see *3.2 Storage AE Specification* on page 30), can be retrieved from media storage. This is due to the fact that the Browse Directory Information filters all SOP Instances not matching the Application profiles supported.

During operation, no "Attribute Value Precedence" is applied to the SOP Instances. Detached Patient Management is not supported (please refer to DICOM part 11, Media Storage Application Profiles).

For media conforming to the STD-GEN-CD Profile, the following SOP classes are supported as an FSR:

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Breast Tomosynthesis Image	1.2.840.10008.5.1.4.1.1.13.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
MR Spectroscopy Image	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
SC Image	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiofluoroscopic-Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Information Object Definitions	SOP Class UID	Transfer Syntax and UID
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Csa Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Spatial Fiducial Storage	1.2.840.10008.5.1.4.1.1.66.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Note

Importing of Enhanced CT and Enhanced MR images with concatenated data is not supported. This is realized by checking the Concatenation UID (Tag ID: 0020, 9161) of the Multi-Frame Functional Group, which is set for Concatenated data.

Note

After receiving an image of type Multi-frame Single Bit Secondary Capture Image, Multi-frame Grayscale Byte Secondary Capture Image, Multi-frame Grayscale Word Secondary Capture Image and Multi-frame True Color Secondary Capture Image, the SOP class UID of the received image is changed and stored as a Secondary Capture Image (1.2.840.10008.5.1.4.1.1.7).

10.1.2.2.1 Application Profiles for the RWA: Import into local Storage

See Table 92: Application profiles, Activities, and Roles for the DICOM Archive application on page 207 for the Application Profiles listed that invoke this Application Entity for the Import to Local Storage RWA.

10.1.2.3 Real-World Activity: Export to local Archive Media

The DICOM Archive application acts as an FSU (for media with an existing DICOM file-set) or an FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to the local Archive medium.

The DICOM Archive application receives a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM fileset), the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

When the DICOM archive application is requested to copy SOP Instances, the preferred application profile according to the configuration will be used to validate and copy the referred SOP Instances. When creating a new file-set, no Descriptor File is allocated and the related ID is not used.

The DICOM archive application does not close the medium.

10.1.2.3.1 Application Profiles for the RWA: Export to local Archive Media

See *Table 92: Application profiles, Activities, and Roles for the DICOM Archive application* on page 207 for the Application Profiles listed that invoke this Application Entity for export to local Archive Media RWA.

11 Augmented and Private Profiles

11.1 Augmented Application Profiles

11.1.1 AUG-GEN-CD

With no private Siemens Non-Images stored on the Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the SUCD Standard Profile.

The storage of Private Information Objects is only supported with reference to a Private Application Profile (see next section).

The Siemens non-image is typically used for raw data and 3D private data.

11.1.2 AUG-CTMR-xxxx

With no private Siemens Non-Images stored on the Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the and STD-CTMR-CD Standard Profiles.

The storage of Private Information Objects is only supported with reference to a Private Application Profile (see next section).

11.1.3 AUG-XA1K-CD

With no private Siemens Non-Images stored on the Medium, the definitions of the PRI-SYNGO-CD Profile are applicable to denote the augmentations for the STD-XA1K-CD Standard Profile.

The storage of Private Information Objects is only supported with reference to a Private Application Profile (see next section).

11.2 *syngo*® private offline Media Application Profile

This section contains a *syngo*-specific Application Profile.

The Structure of this Application Profile is defined in Part 11 of the 2000 DICOM Standard.

It is needed to describe the requirements for Offline Media Storage of the private IOD (Non-Image IOD).

11.2.1 Class and Profile Identification

This document defines an Application Profile class for "*syngo*® speaking"¹ modalities or applications.

The identifier for this class shall be PRI-SYNGO. This class is intended to be used for the interchange of extended and private Information Objects via CD-R offline media between dedicated acquisition or workstation modalities built from a common *syngo* architecture.

The specific application profiles in this class are shown in the table below:

Application Profile	Identifier	Description
" <i>syngo</i> speaking" System on CD-R	PRI-SYNGO-CD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)
" <i>syngo</i> speaking" System on DVD R	PRI-SYNGO-DVD	Handles interchange of Composite SOP Instances and privately defined SOP Instances (Siemens Non-Image IOD)

Equipment claiming conformance with this *syngo* Application Profile Class shall make a clear statement on the handling of the private defined SOP Instances.

¹ *syngo* is a registered trademark of Siemens AG

11.2.2 Clinical Context

This application profile facilitates the interchange of original acquired and derived images and private data related to them. A typical media interchange would be from in-lab acquisition equipment to dedicated workstations and archive systems with specific extensions to handle the private data objects (in both directions).

Additionally, images used to prepare procedures, multi-modality images (for example, integrated US) and images derived from primary diagnostic images, such as annotations, quantitative analysis images, reference images, and screen capture images, may be interchanged via this profile.

11.2.2.1 Roles and Service Class Options

This Application Profile uses the Media Storage Service Class defined in PS 3.4 with the Interchange Option.

The Application Entity supports one or more of the roles of File Set Creator (FSC), File Set Reader (FSR), and File Set Updater (FSU), defined in PS3.10.

11.2.2.1.1 File Set Creator

The Application Entity acting as File Set Creator generates a File Set under the PRI-SYNGO Application Profiles.

File Set Creators are able to generate the Basic Directory SOP Class in the DICOMDIR file with all the subsidiary Directory Records related to the Image SOP Classes and Private SOP Classes stored in the File Set.

In the case of the PRI-SYNGO-CD and PRI-SYNGO-DVD profile, the FSC offers the ability to allow multi-session (additional information may be subsequently added to the disc). For both profiles, multi-session media can be finalized.

Note

A multiple volume (a logical volume that can cross multiple physical media) is not supported by this Application Profile Class. If a set of Files, for example, a Study, cannot be written entirely on one CD-R, the FSC creates multiple independent DICOM File Sets such that each File Set can reside on a single CD-R medium controlled by its individual DICOMDIR file. The user of the FSC can opt to use written labels on the discs to reflect that there is more than one disc for this set of files (for example, a study).

11.2.2.1.2 File Set Reader

The role of the File Set Reader is used by Application Entities that receive the transferred File Set.

File Set Readers are able to read all the defined SOP Instance file defined for the specific Application Profiles to which a conformance claim is made, using all the defined Transfer Syntaxes.

11.2.2.1.3 File Set Updater

The role of the File Set Updater is used by Application Entities, that receive a transferred File Set and update it by adding processed information.

File Set Updaters are able to read and update the DICOMDIR file. File Set Updaters do not have to read the image/private information objects. File Set Updaters are able to generate any of the SOP Instance files defined for the specific Application Profiles to which a conformance claim is made, and to read and update the DICOMDIR file.

In the case of the PRI-SYNGO-CD and PRI-SYNGO-DVD profile, the FSU offers the ability to allow multi-session (additional information can be subsequently added to the disc).

Note**(for CD-R and DVD-R)**

If the disc has not been finalized, the File Set Updater is able to update information assuming there is enough space on the disc to write a new DICOMDIR file, the information, and the fundamental CD-R/DVD-R control structures. CD-R/DVD-R control structures are the structures inherent to CD-R/DVD-R standards, see PS 3.12.

11.2.3 PRI-SYNGO Profiles

11.2.3.1 SOP Classes and Transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option. In the table below, the Transfer Syntax UID "RLE Lossless" applies only for decompression.

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
Basic Directory	1.2.840.10008.1.3.10	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	M
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
CR Image	1.2.840.10008.5.1.4.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
CR Image	1.2.840.10008.5.1.4.1.1.1	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
DX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.1	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
DX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossless 1.2.840.10008.1.2.90	O	O	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	JPEG Lossy 1.2.840.10008.1.2.91	O	O	O
MG Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
MG Image - For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossless 1.2.840.10008.1.2.90	O	O	O
IOX Image - For Presentation	1.2.840.10008.5.1.4.1.1.1.3	JPEG Lossy 1.2.840.10008.1.2.91	O	O	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
IOX Image - For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
CT Image	1.2.840.10008.5.1.4.1.1.2	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
Enhanced CT Image	1.2.840.10008.5.1.4.1.1.2.1				
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG 2000 Lossless 1.2.840.10008.1.2.90	-	M	-
US-MF image (retired)	1.2.840.10008.5.1.4.1.1.3	JPEG 2000 Lossy 1.2.840.10008.1.2.91	-	M	-
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
US-MF image	1.2.840.10008.5.1.4.1.1.3.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Little Endian Uncompressed	M	M	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.1			
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossless Process 14 (selection value 1)	O	M	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.4.70			
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossless Process 14 NON-HIER	-	M	-
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.4.57			
MR Image	1.2.840.10008.5.1.4.1.1.4	Explicit VR Big Endian Uncompressed	O	M	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.2			
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG Lossy (baseline or extended)	O	O	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51			
MR Image	1.2.840.10008.5.1.4.1.1.4	RLE Lossless	O	O	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.5			
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG 2000 Lossless	O	O	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.90			
MR Image	1.2.840.10008.5.1.4.1.1.4	JPEG 2000 Lossy	O	O	O
Enhanced MR Image	1.2.840.10008.5.1.4.1.1.4.1	1.2.840.10008.1.2.90			
MR Spectroscopy Image	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed	M	M	O
		1.2.840.10008.1.2.1			
MR Spectroscopy Image	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Big Endian Uncompressed	O	M	O
		1.2.840.10008.1.2.2			
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Little Endian Uncompressed	M	M	O
		1.2.840.10008.1.2.1			
Grayscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.4.2	Explicit VR Big Endian Uncompressed	O	M	O
		1.2.840.10008.1.2.2			
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Little Endian Uncompressed	M	M	O
		1.2.840.10008.1.2.1			
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless Process 14 (selection value 1)	O	M	O
		1.2.840.10008.1.2.4.70			

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.7	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	RLE Lossless 1.2.840.10008.1.2.5	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG 2000 Lossless 1.2.840.10008.1.2.90	-	M	-
US Image (retired)	1.2.840.10008.5.1.4.1.1.6	JPEG 2000 Lossy 1.2.840.10008.1.2.91	-	M	-
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
US Image	1.2.840.10008.5.1.4.1.1.6.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	M	O
US Image	1.2.840.10008.5.1.4.1.1.6.1	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	M	O
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
Multi-frame Grayscale Worde SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Multi-frame Grayscale Worde SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
Multi-frame Grayscale Worde SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
SC Image	1.2.840.10008.5.1.4.1.1.7	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2				
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2				
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				
SC Image	1.2.840.10008.5.1.4.1.1.7				
Multi-frame Single Bit SC Image	1.2.840.10008.5.1.4.1.1.7.1				
Multi-frame Grayscale Byte SC Image	1.2.840.10008.5.1.4.1.1.7.2	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
Multi-frame Grayscale Word SC Image	1.2.840.10008.5.1.4.1.1.7.3				
Multi-frame True Color SC Image	1.2.840.10008.5.1.4.1.1.7.4				
SC Image	1.2.840.10008.5.1.4.1.1.7				

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
	1.2.840.10008.5.1.4.1.1.9.1.2				
	1.2.840.10008.5.1.4.1.1.9.1.3				
	1.2.840.10008.5.1.4.1.1.9.2.1				
	1.2.840.10008.5.1.4.1.1.9.3.1				
	1.2.840.10008.5.1.4.1.1.9.4.1				
Waveform Storage SOP Classes	1.2.840.10008.5.1.4.1.1.9.1.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
	1.2.840.10008.5.1.4.1.1.9.1.2				
	1.2.840.10008.5.1.4.1.1.9.1.3				
	1.2.840.10008.5.1.4.1.1.9.2.1				
	1.2.840.10008.5.1.4.1.1.9.3.1				
	1.2.840.10008.5.1.4.1.1.9.4.1				
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	M	O
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	RLE Lossless 1.2.840.10008.1.2.5	O	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	M	O
X-Ray Radio-fluoroscopic Image	1.2.840.10008.5.1.4.1.1.12.2	JPEG 2000 Lossless 1.2.840.10008.1.2.91	O	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
NM Image	1.2.840.10008.5.1.4.1.1.20	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
NM Image	1.2.840.10008.5.1.4.1.1.20	JPEG 2000 Lossless 1.2.840.10008.1.2.91	O	O	O
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Mammography CAD SR	1.2.840.10008.5.1.4.1.1.88.50	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
Chest CAD SR	1.2.840.10008.5.1.4.1.1.88.65	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
Procedure Log	1.2.840.10008.5.1.4.1.1.88.40	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
X-Ray Radiation Dose SR	1.2.840.10008.5.1.4.1.1.88.67	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
PET Image	1.2.840.10008.5.1.4.1.1.128	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
PET Image	1.2.840.10008.5.1.4.1.1.128	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossless Process 14 (selection value 1) 1.2.840.10008.1.2.4.70	O	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossless Process 14 NON-HIER 1.2.840.10008.1.2.4.57	-	M	-
RT Image	1.2.840.10008.5.1.4.1.1.481.1	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG Lossy (baseline or extended) 1.2.840.10008.1.2.4.50 1.2.840.10008.1.2.4.51	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	RLE Lossless 1.2.840.10008.1.2.5	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG 2000 Lossless 1.2.840.10008.1.2.90	O	O	O
RT Image	1.2.840.10008.5.1.4.1.1.481.1	JPEG 2000 Lossy 1.2.840.10008.1.2.91	O	O	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Dose	1.2.840.10008.5.1.4.1.1.481.2	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Structure Set	1.2.840.10008.5.1.4.1.1.481.3	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.4	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Plan	1.2.840.10008.5.1.4.1.1.481.5	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O

Table 93: SOP Classes and Transfer Syntax

Information Object Definitions	SOP Class UID	Transfer Syntax and UID	FSC	FSR	FSU
RT Brachy Treatment Record	1.2.840.10008.5.1.4.1.1.481.6	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Treatment Summary Record	1.2.840.10008.5.1.4.1.1.481.7	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Ion Plan	1.2.840.10008.5.1.4.1.1.481.8	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	M	M	O
RT Ion Beams Treatment Record	1.2.840.10008.5.1.4.1.1.481.9	Explicit VR Big Endian Uncompressed 1.2.840.10008.1.2.2	O	M	O
Csa Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1	O	M	O

FSC, FSR, FSU - denote the requirements for these roles

O - Optional

M - Mandatory

11.2.3.2 Physical Media and Formats

The PRI-SYNGO-CD Profile requires the use of 120 mm CD-R physical media with the ISO/IEC 9660 Media Format, as defined in PS3.12.

The PRI-SYNGO-DVD Profile requires the use of 120 mm DVD-R physical media with the UDF 2.01 Media Format, as defined in PS3.12.

11.2.3.3 Directory Information in DICOMDIR

Conforming Application Entities include in the DICOMDIR File the Basic Directory IOD, containing Directory Records at the Patient and subsidiary levels appropriate to the SOP Classes in the File Set. All DICOM files in the File Set incorporating SOP instances defined for the specific Application Profile are referenced by Directory Records.

Note

DICOMDIRs with no directory information are not allowed by this Application Profile.

Privately defined IODs are referenced by "PRIVATE" Directory Records.

11.2.3.3.1 Basic Directory IOD Specification

This Application Profile makes use of optional attributes of the Basic Directory IOD to support recognition of the Patient's Storage Service request results in spanning multiple volumes (file sets). Therefore, the File Set Descriptor File can be used and is then referenced by optional Basic Directory IOD attributes. If this exists, the specified Descriptor File may be used by FSR applications. Any FSU or FSC shall make a clear statement if the Descriptor File mechanism is used according to the specialization defined in this Application Profile.

The Descriptor Files has the following contents:

One single line without any control characters and according to the Basic Character Set having the following defined text:

"MULTIVOLUME: xx of yy"

xx, yy are replaced by the actual number of the volume (xx) and the total number of volumes in the set (yy).

If used, the Descriptor File has "README" as its File ID and resides in the same directory level as the DICOMDIR. It is referenced by the attribute [0004,1141] File Set Descriptor File ID having the defined contents of "README".

11.2.3.3.2 Additional Keys

File Set Creators and Updaters are required to generate the mandatory elements specified in PS 3.3, Annex F of the DICOM Standard. Table below: PRI-SYNGO-CD Additional DICOMDIR Keys specifies the additional associated keys. Other additional data elements can be added at each directory record level, but it is not required that File Set Readers be able to use them as keys. Refer to the Basic Directory IOD in PS 3.3.

Table 94: DICOMDIR keys

Attribute Name	Tag	Directory Record Level	Type	Notes
Date Of Birth	(0010,0030)	PATIENT	2C	Required, if present in SOP Instance
Patient's Sex	(0010,0040)	PATIENT	2C	Required, if present in SOP Instance
Series Date	(0008,0021)	SERIES	3	
Series Time	(0008,0031)	SERIES	3	

Table 94: DICOMDIR keys

Attribute Name	Tag	Directory Record Level	Type	Notes
Institution Name	(0008,0080)	SERIES	2C	Required, if present in SOP Instance
Institution Address	(0008,0081)	SERIES	2C	Required, if present in SOP Instance
Series Description	(0008,103E)	SERIES	3	
Performing Physician's Name	(0008,1050)	SERIES	2C	Required, if present in SOP Instance
Image Type	(0008,0008)	IMAGE	1C	Required, if present in SOP Instance
SOP Class UID	(0008,0016)	IMAGE	3	
SOP Instance UID	(0008,0018)	IMAGE	3	
Image Date	(0008,0023)	IMAGE	3	
Image Time	(0008,0033)	IMAGE	3	
Referenced Image Sequence	(0008,1140)	IMAGE	1C	Required, if present in SOP Instance
> Referenced SOP Class UID	(0008,1150)			
> Referenced SOP Instance UID	(0008,1155)			
Image Position (Patient)	(0020,0032)	IMAGE	2C	Required, if present in SOP Instance
Image Orientation (Patient)	(0020,0037)	IMAGE	2C	Required, if present in SOP Instance
Frame Of Reference UID	(0020,0052)	IMAGE	2C	Required, if present in SOP Instance
Rows	(0028,0010)	IMAGE	3	
Columns	(0028,0011)	IMAGE	3	
Pixel Spacing	(0028,0030)	IMAGE	1C	C
Calibration Image	(0050,0004)	IMAGE	2C	Required, if present in SOP Instance
Icon Image Sequence	(0088,0200)	IMAGE	3	Required for Image SOP Classes
> Samples per Pixel	(0028,0002)			1
> Photometric Interpretation	(0028,0004)			MONOCHROME2
> Rows	(0028,0010)			128 for XA IOD, 64 otherwise
> Columns	(0028,0011)			128 for XA IOD, 64 otherwise
> Bits Allocated	(0028,0100)			8
> Bits Stored	(0028,0101)			8
> High Bit	(0028,0102)			7
> Pixel Representation	(0028,0103)			0 (unsigned)
> Pixel Data	(7FE0,0010)			Icon Image pixel data
Curve Number	(0020,0024)	CURVE	1C	required, if present in SOP Instance

11.2.3.3.3 Private Directory Record Keys

Private Directory Records are supported by this Application Profile Class at the following level:

IMAGE

The PRIVATE Directory Records have other required elements in addition to the mandatory elements specified in PS 3.3.

The following table lists the additionally required keys for PRIVATE Directory Records.

Table 95: DICOMDIR keys for CsaNonImage

Attribute Name	Tag	Directory Record Level	Type	Notes
Private Record UID	(0004,1432)	PRIVATE	1	See Conformance Statement
SOP Class UID	(0008,0016)	PRIVATE	1C	Required, if present in SOP Instance
SOP Instance UID	(0008,0018)	PRIVATE	1C	Required, if present in SOP Instance
Image Type	(0008,0008)	PRIVATE	3	Identification characteristics
Acquisition Date	(0008,0022)	PRIVATE	3	
Acquisition Time	(0008,0032)	PRIVATE	3	
Acquisition Number	(0020,0012)	PRIVATE	3	
CSA Data Type	(0029,xx08)	PRIVATE	1	Private owner code = SIEMENS CSA NON-IMAGE
CSA Data Version	(0029,xx09)	PRIVATE	3	Private owner code = SIEMENS CSA NON-IMAGE

11.2.3.3.4 Icon Images

Directory Records of type SERIES or IMAGE may include Icon Images. The Icon Image Pixel data is as specified in PS 3.3 "Icon Image Key Definition", and restricted such that Bits Allocated (0028,0100) and Bits Stored (0028,0101) are equal to 8, and Rows (0028,0010) and Columns (0028, 0011) are equal to 128 for XA Images and 64 for all other images. The Photometric interpretation (0028,0004) is always restricted to "MONOCHROME2".

PRIVATE Directory Records will not contain Icon Image information.

11.2.3.4 Other Parameters

This section defines other parameters common to all specific Application Profiles in the PRI-SYNGO class that need to be specified in order to ensure interoperable media interchange.

11.2.3.4.1 Multiframe JPEG Format

The JPEG encoding of pixel data uses the Interchange Format (with table specification) for all frames.

12 Extentions, Spicializations and Privatizations of SOP Classes and Transfer Syntaxes

The SOP Classes listed mainly refer to those created by the equipment to which this Conformance Statement is related. For SOP classes not listed in this section, please refer to the Storage section of the DICOM Conformance Statement of the product. This includes all SOP Instances that can be received and displayed, and therefore will be included in offline media storage even though these SOP Instances are not created by the equipment serving the Media Storage Service.

12.1 SOP-Specific Conformance Statement for Basic Directory

12.1.1 Extension, Specialization for SIEMENS Non-Image Objects

According to the PRI-SYNGO Application Profile Class, the use of the Private Creator UIDs and further optional keys for the Directory Records referring to SIEMENS Non-Image Objects is given in the following table.

Attribute	Tag	Value used
Private Record UID	(0004,1432)	1.3.12.2.1107.5.9.1
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1

For the Non-Images no Icon Image Sequence is generated.

13 Configuration

13.1 AE Title Mapping

13.1.1 DICOM Media Storage AE Title

The DICOM Storage application (Image Manager) provides the application entity title:

- CsalmageManager

14 Support of Extended Character Sets

The Somaris/7 DICOM application supports the following character sets as defined in the four tables below:

Table 96: *Single-Byte Character Sets without Code Extension*

Character Set Description	Defined Term	ISO Registration Number	Character Set
Default repertoire	NoneNone	ISO_IR 6	ISO 646
Latin alphabet No. 1	ISO_IR 100	ISO_IR 100	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 2	ISO_IR 101	ISO_IR 101	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 3	ISO_IR 109	ISO_IR 109	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 4	ISO_IR 110	ISO_IR 110	Supplementary set
		ISO_IR 6	ISO 646
Cyrillic	ISO_IR 144	ISO_IR 144	Supplementary set
		ISO_IR 6	ISO 646
Arabic	ISO_IR 127	ISO_IR 127	Supplementary set
		ISO_IR 6	ISO 646
Greek	ISO_IR 126	ISO_IR 126	Supplementary set
		ISO_IR 6	ISO 646
Hebrew	ISO_IR 138	ISO_IR 138	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 5	ISO_IR 148	ISO_IR 148	Supplementary set
		ISO_IR 6	ISO 646
Japanese	ISO_IR 13	ISO_IR 13	JIS X 0201:Katakana
		ISO_IR 14	JIS X 0201:Romaji

Table 97: Single-Byte Character Sets with Code Extension

Character Set Description	Defined Term	Standart for Code Extension	ESC Sequence	ISO Regis- tration Number	Character Set
Default repertoire	ISO 2022 IR 6	ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet No.1	ISO 2022 IR 100	ISO 2022	ESC 02/13 04/01	ISO_IR 100	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet No.2	ISO 2022 IR 101	ISO 2022	ESC 02/13 04/02	ISO_IR 101	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet No.3	ISO 2022 IR 109	ISO 2022	ESC 02/13 04/03	ISO_IR 109	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet No.4	ISO 2022 IR 110	ISO 2022	ESC 02/13 04/04	ISO_IR 110	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Cyrillic	ISO 2022 IR 144	ISO 2022	ESC 02/13 04/12	ISO_IR 144	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Arabic	ISO 2022 IR 127	ISO 2022	ESC 02/13 04/07	ISO_IR 127	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Greek	ISO 2022 IR 126	ISO 2022	ESC 02/13 04/06	ISO_IR 126	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Hebrew	ISO 2022 IR 138	ISO 2022	ESC 02/13 04/08	ISO_IR 138	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Latin alphabet No.5	ISO 2022 IR 148	ISO 2022	ESC 02/13 04/13	ISO_IR 148	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO_IR 6	ISO 646
Japanese	ISO 2022 IR 13	ISO 2022	ESC 02/13 04/09	ISO_IR 13	JIS X 0201:Kata- kana
		ISO 2022	ESC 02/08 04/02	ISO_IR 14	JIS X 0201- 1976:Romaji

Table 98: Multi-Byte Character Sets without Code Extension

Character Set Description	Defined Term	ISO Registration Number	Character Set
Unicode	ISO_IR 192	ISO 10646	Unicode in UTF-8
Chinese	GB18030	GB18030	GB 18030-2000 (China Association for Standardization)

Table 99: Multi-Byte Character Sets with Code Extension

Character Set Description	Defined Term	Standart for Code Extension	ESC Sequence	ISO Registration Number	Character Set
Japanese	ISO 2022 IR 87	ISO 2022	ESC 02/04 04/02	ISO_IR 87	JIS X 0208: Kanji
	ISO 2022 IR 159	ISO 2022	ESC 02/04 02/08 04/04	ISO_IR 159	JIS X 0212: Supplementary Kanji set
Chinese ^a	ISO 2022 IR 58	ISO 2022	ESC 02/04 04/01	ISO_IR 58	GB2312-80 (China Association for Standardization)

^a This Character Set is an extension of DICOM for the Chinese language.

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD coming into the system, then the following measures are taken to make the characters DICOM-conform:

- Try to import with ISO-IR 100. If ISO-IR 100 also fails, convert each illegal character to '?'.

There are now 3 categories of character sets which have to be differentiated because of their different encoding formats:

- Conventional ISO character sets: ISO_IR 6, ISO 2022 IR 6, ISO_IR 100, etc. =>Encoded in ISO 2022
- ISO_IR 192: Encoded in UTF-8
- GB18030: Encoded in GB18030

It is not possible to recognize the following mismatches automatically on receiving or importing:

- An attribute value is encoded in ISO_IR 192 <=> (0008,0005) contains a conventional ISO character set as the primary character set
- An attribute value is encoded in GB18030 <=> (0008,0005) contains a conventional ISO character set as the primary character set
- An attribute value is encoded in ISO 2022 <=> (0008,0005) contains ISO_IR 192
- An attribute value is encoded in ISO 2022 <=> (0008,0005) contains GB18030

An IOD that contains one of the above mentioned inconsistencies is not DICOM-conform. As these kinds of inconsistencies cannot be recognized by the system, the IOD is not rejected, but the character data might be corrupted.

Older versions of syngo do not support the newly introduced character sets ISO_IR 192 and GB18030, and their special encodings. This means that an IOD which contains one of these new character sets in (0008,0005) will be rejected by an older syngo system.

A Annex

A.1 Siemens Private Non-Image IOD

Please see 4.2.3 *Private SOP class CSA Non-Image* on page 185.

A.2 Siemens Standard Extended Modules

Please see 4.2.1.2 *All syngo-Supported Image SOP Classes* on page 175.

A.3 Siemens Standard Extended Modules

Please see 4.2.1.1 *Registry of DICOM Data Elements* on page 173 and 4.2.2.1 *Registry of DICOM Data Elements* on page 182.

A.4 Standard Extensions of all SOP Classes

Please see 4.1.1 *Standard Extensions of all SOP Classes* on page 145.

A.5 DICOM Print SCU - detailed status displays

Please see 3.5.2.1.3.8 *DICOM Print SCU - detailed status displays* on page 112.

Index

B

Basic Color Print Management 105
Basic Worklist 123
Body Part Examined 151, 167

C

Case Sensitive 86
C-ECHO 18, 28, 29, 46
Certificate 202
C-FIND 22, 25, 76, 85, 86, 124, 125, 133, 134
C-FIND-CANCEL 85
C-FIND-RQ 195
C-FIND-RSP 195
C-GET 22, 75, 85, 97, 98
C-GET-CANCEL 85
C-MOVE 22, 75, 76, 82, 83, 85, 99, 100
C-MOVE-CANCEL 85
Color Images 66
Color Print Management 102
Configuration 237
C-STORE 18, 22, 33, 46, 82, 83, 97, 98, 99, 100
C-STORE-RQ 64

D

Data Flow 17, 19, 205
Dose Report 164

E

Extended Character Sets 197, 201, 238
Extended Negotiation 86, 98, 100

F

Film Box 102, 105, 106, 107, 108
Film Session 102, 105, 106

G

Graphic overlay 65
Grayscale Images 65
Grayscale Print Management 102, 105

I

Image Box 102, 106, 107, 108, 109
Implementation models 17

M

Match 74
MOD LUT SQ 66
Modality Worklist 195
MONOCHROME1 65, 66
MONOCHROME2 65, 66, 234

N

N_EVENT_REPORT 111
N-ACTION 106
N-CREATE 105, 106, 136
N-DELETE 105, 106
N-SET 136

O

Organ Characteristic 167
Overlay plane 65, 66, 180

P

PALETTE COLOR 67
Performed Procedure Step 26
Pixel plane 66
Presentation LUT 102
Print Job SOP Class 102
Printer SOP Class 102

R

RGB 66, 152

S

Secure DICOM 201
SOP Classes 69
Structured Reports 163

T

TLS 201

V

Verification 17, 28, 63, 67
VOI LUT SQ 66

X

X.509 certificates 201

Y

YBR_FULL 67

The original language of this document is English.

Caution: Federal law restricts this device to sale by or on the order of a physician, dentist, or veterinarian (21 CFR 801.109(b)(1)).

.....
Siemens Healthineers Headquarters
Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany
Phone: +49 9131 84-0
siemens-healthineers.com

Legal Manufacturer
Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen
Germany