



DICOM Conformance Statement Sensis Vibe VD1

[siemens-healthineers.com](https://www.siemens-healthineers.com)

1 Conformance Statement Overview

The Sensis is a syngo®-based vital signs recording system. It supports storage and transfer of medical information utilizing the DICOM "Storage Service Class", the display of data and retrieval of information from DICOM Archives utilizing the DICOM "Query/Retrieve Service Class". Workflow Management is supported by querying worklists from RIS and returning information about the procedure performed. Furthermore, the import from and export to DICOM CD media is supported. Printing of viewing results is provided with Print Management Services.

The Sensis conforms to the DICOM Standard and supports the network services as described in Table 1 Network Services and the media services as described in Table 2 Media Services.

SOP Classes	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Verification			
Verification	1.2.840.10008.1.1	Yes	Yes
SOP Classes created and managed by Sensis			
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	Yes
Transfer (Private SOP Class)			
Syngo Non-Image Storage	1.3.12.2.1107.5.9.1	Yes	Yes
Storage Commitment			
Storage Commitment Push Model SOP Class	1.2.840.10008.1.20.1	Yes	No
Worklist Management			
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Yes	No
Modality Performed Procedure Step SOP Class	1.2.840.10008.3.1.2.3.3	Yes	No
Query/Retrieve			
Patient Root Q/R - Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Patient Root Q/R - Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Patient Root Q/R - Information Model - GET	1.2.840.10008.5.1.4.1.2.1.3	No	Yes
Study Root Q/R - Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Study Root Q/R - Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Study Root Q/R - Information Model - GET	1.2.840.10008.5.1.4.1.2.2.3	No	Yes
Patient/Study Only Q/R - Information Model FIND	1.2.840.10008.5.1.4.1.2.2.3	No	Yes

SOP Classes	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Patient/Study Only Q/R - Information Model MOVE	1.2.840.10008.5.1.4.1.2.3.2	No	Yes
Patient/Study Only Q/R - Information Model GET	1.2.840.10008.5.1.4.1.2.3.3	No	Yes

Table 1 Network Services

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
Compact Disk – Recordable / Digital Versatile Disk – Recordable		
STD-GEN-CD	No	Yes
STD-XABC-CD	No	Yes
STD-XA1K-CD	No	Yes
PRI-XAMAS-CD	Yes	Yes
AUG-XA1K-CD	Yes	Yes
STD-GEN-DVD	No	Yes
STD-XABC-DVD	No	Yes
STD-XA1K-DVD	No	Yes
PRI-XAMAS-DVD	Yes	Yes
AUG-XA1K-DVD	Yes	Yes

Table 2 Media Services

Name	Value
Application Context Name	1.2.840.100008.3.1.1.1
Implementation Class UID	1.3.12.2.1107.5. 9.20000101
Implementation Version Name	SIEMENS_SWFVE31F

Table 3 Implementation Identifying Information

2 Table of Contents

1	<i>Conformance Statement Overview</i>	2
2	<i>Table of Contents</i>	4
3	<i>Introduction</i>	7
3.1	Revision History	7
3.2	Overview.....	7
3.3	Scope and Field.....	7
3.4	Audience.....	7
3.5	Remarks	7
3.6	Definitions, Terms and Abbreviations	8
3.7	References	9
3.8	Structure	9
4	<i>Implementation Model Verification</i>	10
4.1	Application Data Flow Diagram	10
4.2	Functional Definitions of Applications.....	10
4.3	Sequencing of Real-World Activities.....	10
5	<i>Application Entity Specification Verification</i>	11
5.1	Verification AE Specification.....	11
5.1.1	Association Establishment Policies	11
5.1.2	Association Initiation Policy	11
5.1.3	Association Acceptance Policy	12
6	<i>Implementation Model Storage</i>	13
6.1	Application Data Flow Diagram	13
6.2	Functional Definitions of Application Entities	13
6.3	Sequencing of Real-World Activities.....	13
7	<i>Application Entity Specification Storage</i>	14
7.1	Storage AE Specification.....	14
7.1.1	Association Establishment Policies	15
7.1.2	Association Initiation Policy	15
7.1.3	Association Acceptance Policy	18
8	<i>Implementation Model Storage Commitment</i>	21
8.1	Application Data Flow Diagram	21
8.2	Functional Definitions of Application Entities	21

8.3	Sequencing of Real-World Activities	21
9	<i>AE Specification Storage Commitment</i>	22
9.1	Storage Commitment AE Specification	22
9.1.1	Association Establishment Policies	22
9.1.2	Association Initiation Policy	22
10	<i>Implementation Model Query / Retrieve</i>	25
10.1	Application Data Flow Diagram	25
10.2	Functional Definitions of Application Entities	26
10.3	Sequencing of Real-World Activities	26
11	<i>Application Entity Specification Query/Retrieve</i>	27
11.1	Query/Retrieve Service AE Specification	27
11.1.1	Association Establishment Policies	28
11.1.2	Association Initiation Policy	28
11.1.3	Association Acceptance Policy	33
12	<i>Implementation Model Worklist</i>	42
12.1	Application Data Flow Diagram	42
12.2	Functional Definitions of Application Entities	42
12.3	Sequencing of Real-World Activities	42
13	<i>Application Entity Specification Worklist</i>	43
13.1	Modality Worklist Service AE Specification	43
13.1.1	Association Establishment Policies	43
13.1.2	Association Initiation Policy	43
14	<i>Implementation Model MPPS</i>	52
14.1	Application Data Flow Diagram	52
14.2	Functional Definitions of Application Entities	52
14.3	Sequencing of Real-World Activities	52
15	<i>AE Specification MPPS</i>	53
15.1	Modality Performed Procedure Step AE Specification	53
15.1.1	Association Establishment Policies	53
15.1.2	Association Initiation Policy	53
16	<i>Communication Profiles</i>	60
16.1	Supported Communication Stacks	60
16.1.1	TCP/IP Stack	60
17	<i>Extensions / Specializations / Privatizations</i>	61
17.1.1	Standard Extended / Specialized / Private SOPs	61

17.1.2	Private Transfer Syntaxes.....	61
18	<i>Configuration</i>	62
18.1	AE Title/Presentation Address Mapping.....	62
18.1.1	DICOM Verification.....	62
18.1.2	DICOM AE Titles	62
18.2	Configurable Parameters	62
18.2.1	Storage, Storage Commitment and Query/Retrieve	62
18.2.2	Modality Worklist	63
18.3	Default Parameters	63
19	<i>Support of Extended Character Sets</i>	64
20	<i>Offline Media Conformance Statement</i>	65
20.1	Implementation Model	65
20.1.1	Application Data Flow Diagram.....	65
20.1.2	Functional Definitions of AEs	65
20.1.3	Sequencing of Real-World Activities	66
20.1.4	Implementation Identifying Information	66
20.2	AE Specifications.....	66
20.2.1	DICOM Archive Specification.....	66
20.3	Augmented and Private Profiles	68
20.3.1	Augmented Application Profiles.....	68
20.3.2	Private Application Profiles	68
20.4	Extensions, Specialization and Privatization of SOP Classes.....	68
20.4.1	SOP Specific Conformance Statement for Basic Directory	68
20.5	Configuration.....	69
20.5.1	AE Title Mapping.....	69
20.6	Support of Extended Character Sets	69
	<i>Annex A: Additional Information</i>	70
	<i>Annex B: Index of Tables</i>	84

3 Introduction

3.1 Revision History

Product	Product Version	Document Version	Date
Sensis Vibe	VD12A	6656990-ESK-200-02	12/2013
Sensis Vibe	VD15A	6656990-ESK-200-03	03/2022
Sensis Vibe	VD15B	6656990-ESK-200-04	07/2022

3.2 Overview

The Conformance Statement describes the DICOM interface for the Siemens Healthineers Sensis in terms of part 2 of the DICOM standard.

This introduction describes the application's implemented DICOM functionality in general terms.

3.3 Scope and Field

The Sensis is a “syngo®-speaking¹” Cardiac Interventional System for Acquisition and Viewing of Waveform data during a catheterization procedure. The Sensis is designed to be integrated into an environment of medical DICOM-based devices. The Sensis DICOM network implementation acts as SCU and SCP for the DICOM Storage and Query/Retrieve services and as SCU for the DICOM Basic Worklist and Storage Commitment Services. The primary purpose for supporting DICOM image storage in Sensis is for the ability to include images in the reports. Clinical reports can also be converted to DICOM XA multiframe images or DICOM Encapsulated PDF to be sent over the network or stored on media. Neither image viewing, nor viewing of foreign DICOM waveform objects is supported in this release. Verification is supported in SCU (only via Service environment) and SCP role. Furthermore, the handling of CD offline media is supported as a FSC, FSU and FSR.

Software Name	SIEMENS Healthineers Product
Sensis Vibe	Sensis product family

Table 4 List of products applicable to this Conformance Statement

3.4 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

3.5 Remarks

DICOM, by itself, does not guarantee interoperability. However, the Conformance Statement facilitates a first-level validation for interoperability between different applications supporting the same DICOM functionality as SCU and SCP, respectively.

¹ syngo® is a registered trademark of Siemens Healthcare GmbH

© Siemens Healthcare GmbH. 2022. All rights reserved.

This Conformance Statement is not intended to replace validation with other DICOM equipment to ensure proper exchange of information intended.

The scope of this Conformance Statement is to facilitate communication with Siemens and other vendors' medical equipment. The Conformance Statement should be read and understood in conjunction with the DICOM 3.0 Standard [DICOM]. However, by itself it is not guaranteed to ensure the desired interoperability and a successful interconnectivity.

The user should be aware of the following important issues:

- The comparison of different conformance statements is the first step towards assessing interconnectivity between Siemens Healthineers and non-Siemens Healthineers equipment.
- Test procedures should be defined, and tests should be performed by the user to validate the connectivity desired. DICOM itself and the conformance parts do not specify this.
- The standard will evolve to meet the users' future requirements. Siemens Healthineers is actively involved in developing the standard further and therefore reserves the right to make changes to its products or to discontinue its delivery.

Siemens Healthineers reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens Healthineers representative for the most recent product information.

3.6 Definitions, Terms and Abbreviations

Definitions, terms, and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

ACR	American College of Radiology
AE	DICOM Application Entity
ASCII	American Standard Code for Information Interchange
DB	Database
DCS	DICOM Conformance Statement
DICOM	Digital Imaging and Communications in Medicine
DIMSE	DICOM Message Service Element
DIMSE-C	DICOM Message Service Element with Composite Information Objects
DIMSE-N	DICOM Message Service Element with Normalized Information Objects
IOD	DICOM Information Object Definition
ISO	International Standard Organization
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
RIS	Radiology Information System
RWA	Real-World Activity
SCP	DICOM Service Class Provider (DICOM server)
SCU	DICOM Service Class User (DICOM client)
SOP	DICOM Service-Object Pair
U	Unique Key Attribute

3.7 References

NEMA PS3 Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>

Integrating the Healthcare Enterprise – IHE Radiology Technical Framework – <http://www.ihe.net>

3.8 Structure

This Conformance Statement is subdivided into multiple Parts, which relate to individual documents need-ed to declare Conformance according to the requirements of “Part 2 – Conformance” of the DICOM Standard.

Those parts are:

- “Network Conformance Statement” for Network related Services
 - Verification – User/Provider
 - Storage – User/Provider
 - Storage Commitment – User
 - Query/Retrieve – User/Provider
 - Basic Worklist – User
- “Offline Media Conformance Statement” to support local archive media.
- A general Appendix.

4 Implementation Model Verification

The Sensis DICOM Service Tool application requests Verification to verify the ability of a foreign DICOM application on a remote node to respond to DICOM messages.

Responding to Verification requests from remote nodes is handled by the Storage SCP application.

4.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU and via the Storage SCP application as SCP for the C-ECHO DICOM network service. The product target Operating System is Microsoft Windows.

The following figures provide a functional overview of the Sensis Application Entities (AE). Relationships are shown between user-invoked activities (in the circles at the left of the AEs) and the associated real-world activities provided by DICOM service providers (in the circles at the right of the AEs)

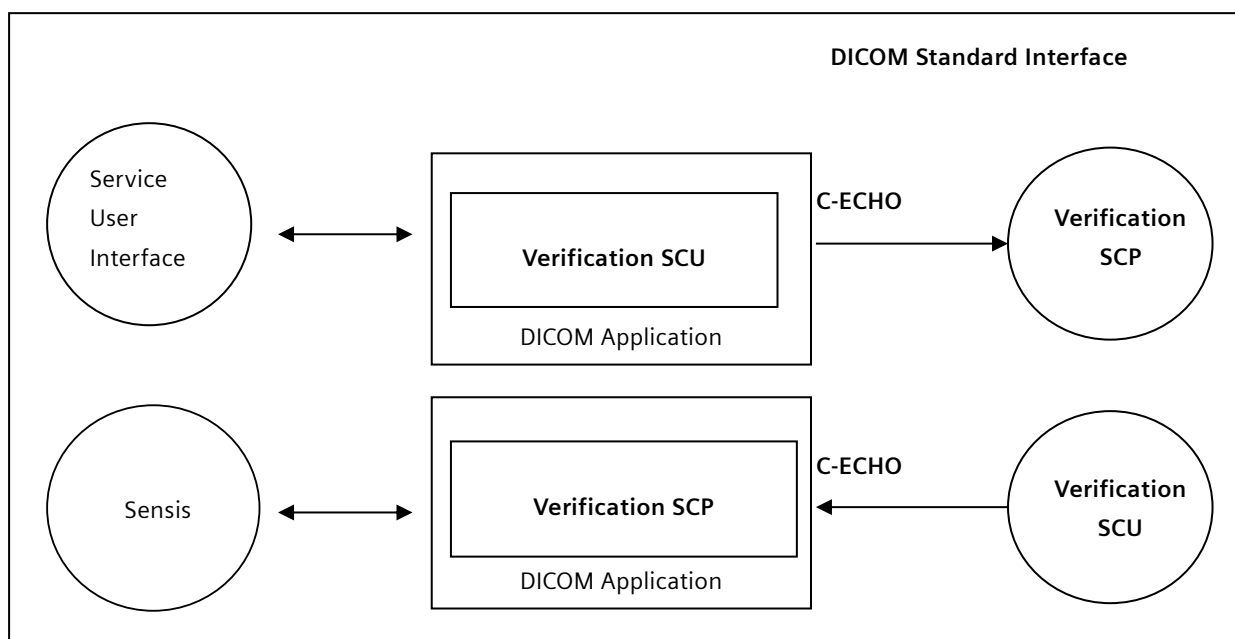


Figure 1 Application Data Flow Diagram - Verification SCU/SCP

4.2 Functional Definitions of Applications

The Sensis DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

4.3 Sequencing of Real-World Activities

Newly entered data must be saved first, before a "verification" of these data is possible.

5 Application Entity Specification Verification

5.1 Verification AE Specification

5.1.1 Association Establishment Policies

5.1.1.1 General

The Sensis DICOM Service Tool application attempts to open an association for verification request whenever the “verification” function is activated during network configuration of a remote DICOM application.

The Sensis DICOM application will accept association requests for verification.

5.1.1.2 Number of Associations

The Sensis DICOM Service Tool application initiates one association at a time to request verification.

The Sensis DICOM application can accept multiple associations at a time. It can handle up to 10 associations in parallel.

5.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

5.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

5.1.2 Association Initiation Policy

The Sensis DICOM Service Tool application attempts to initiate a new association for

- DIMSE C-ECHO

service operations.

5.1.2.1 Associated Real-World Activity – Verification

5.1.2.1.1 Associated Real-World Activity – Request Verification

The associated Real-World activity is a C-ECHO request initiated by Service and Configuration SW environment whenever a “verification” is requested. If an association to a remote Application Entity is successfully established, Verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application contains a status other than “Success” this will be indicated in the service environment and the association is closed.

5.1.2.1.2 **Proposed Presentation Contexts**

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table – Verification SCU					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

Table 5 Proposed Presentation Contexts

5.1.2.1.3 **SOP Specific Conformance – Verification SCU**

The Application conforms to the definitions of the Verification SCU in accordance with the DICOM Standard.

5.1.3 **Association Acceptance Policy**

The Verification SCP is part of the Storage SCP – see Section 7.1.3.

6 Implementation Model Storage

The Sensis DICOM Application Entity both originates associations for Storage of DICOM Composite Information Objects in Remote Application Entities and accepts association requests for Storage from Remote Application Entities.

6.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU and SCP for the C-STORE DICOM network service and as SCP for the C-ECHO DICOM network service. The product target Operating System is Microsoft Windows.

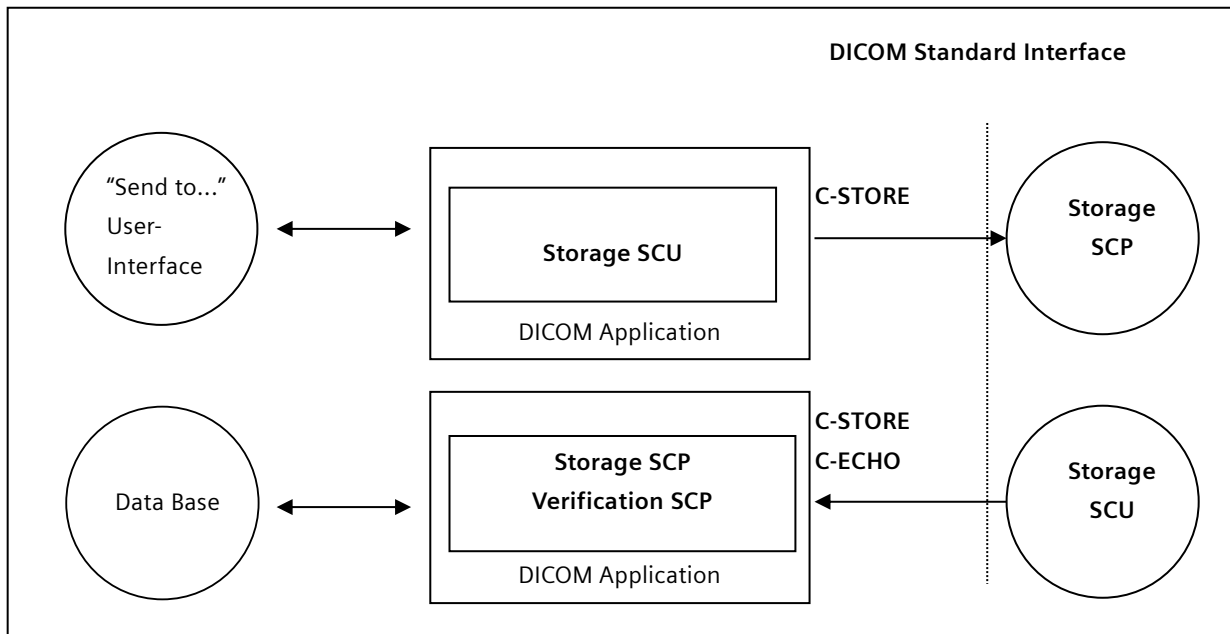


Figure 2 Application Data Flow Diagram - Storage SCU/SCP

6.2 Functional Definitions of Application Entities

The Storage SCU is invoked by the job control interface that is responsible for processing network archival tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

The Storage SCP component of the Sensis DICOM application is operating as background server process. It is running when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context it starts to receive the Composite Image Objects and imports them to local database. Verification requests will be processed and responded by Storage SCP component, too.

6.3 Sequencing of Real-World Activities

Not applicable.

7 Application Entity Specification Storage

7.1 Storage AE Specification

The Sensis Storage service class user/service class provider applications use one AE when initiating/receiving associations to/from remote DICOM nodes.

Siemens Healthineers Sensis products provide Standard Conformance to the following DICOM SOP Classes as an SCU:

SOP Class Name	SOP Class UID
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

Table 6 Supported SOP Classes as an SCU

Siemens Healthineers Sensis products provide Private Conformance to the following DICOM V3.0 conform private SOP Classes as an SCU:

SOP Class Name	SOP Class UID
CSA Non-Image Storage	1.3.12.2.1107.5.9.1

Table 7 Supported private SOP Classes as an SCU

Siemens Healthineers Sensis products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

SOP Class Name	SOP Class UID
Verification	1.2.840.10008.1.1
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1

Table 8 Supported SOP Classes as an SCP

Siemens Healthineers Sensis products provide Private Conformance to the following DICOM-conform private SOP Classes as an SCP:

SOP Class Name	SOP Class UID
CSA Non-Image Storage	1.3.12.2.1107.5.9.1

Table 9 Supported private SOP Classes as an SCP

7.1.1 Association Establishment Policies

7.1.1.1 General

The existence of a job queue entry with network destination or an internal trigger from processing a retrieve request will activate the DICOM Storage Application. An association request is sent to the destination AE and upon successful negotiation of a Presentation Context the transfer is started.

The default PDU size used will be 256 KB.

7.1.1.2 Number of Associations

The Sensis DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The Sensis DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of Simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in Configuration / DICOM / General.

7.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

7.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

7.1.2 Association Initiation Policy

If a job with network destination gets active in the job list or a retrieve sub-operation is processed the Sensis DICOM application attempts to initiate a new association for

- DIMSE C-STORE

service operations.

7.1.2.1 Associated Real-World Activity – Send

7.1.2.1.1 Associated Real-World Activity – Send Image Objects to a Network Destination

The associated Real-World activity is a C-STORE request initiated by an internal daemon process triggered by a job with network destination or the processing of an external C-MOVE retrieve request. If the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. If the C-STORE Response from the remote Application contains a status other than "Success" or "Warning", the association is aborted.

7.1.2.1.2 Proposed Presentation Context – Send Objects

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50		
		JPEG Lossy Extended (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Cardiac Electro-physiology Wave-form Storage SOP Class	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
CSA Non-Image	1.3.12.2.1107.5.9.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 10 Proposed Presentation Context – Send Images

7.1.2.1.3 SOP specific Conformance to Storage SOP classes

The Sensis application will create XA IOD type images or Encapsulated PDF IOD from the reporting application. Furthermore, a private "Non-Image IOD" will be used to store presentation data and textual report data (Examination Log). The XA IOD will be a "Standard Extended XA Storage" SOP Class. The XA IOD will be a "Standard Extended XA Storage" SOP Class.

For association and DIMSE level time-outs, please refer to Section 20.5 of this document.

7.1.2.1.3.1 Specialized Information Object Definitions

The DICOM images created by Sensis DICOM application conform to the DICOM IOD definitions (Standard extended IODs). But they will contain additional private elements, which must be discarded by a DICOM system when modifying the object.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification!

7.1.2.1.3.2 Data Dictionary of applied private IOD Attributes

Please see Annex A.4 for a list of possible private IOD attributes.

7.1.2.1.3.3 Image Pixel Attribute Description for Grayscale Images

The Siemens Healthineers Sensis DICOM application supports the Monochrome2 Photometric Interpretation with the unsigned integer 16-bit grayscale pixel and graphic overlay format. The lower 12 bits are used for pixel and the higher 4 bits are used for the graphic overlay:

Pixel plane

- Samples Per Pixel (attribute 0028, 0002) = 1
- Photometric Interpretation (attribute 0028,0004) = "MONOCHROME2"
- Pixel Representation (attribute 0028, 0103) = 0
- Bits Allocated (attribute 0028, 0100) = 8, 16
- Bits Stored (attribute 0028,0101) = 8, 10, 12
- High Bit (attribute 0028,0102) = 7, 9, 11 (Bits Stored - 1)

Overlay plane

- Overlay Type (attribute 60xx, 0040) = "G"
- Bits Allocated (attribute 60xx, 0100) = 1
- Bit Position (attribute 60xx, 0102) = 0
- Overlay Data (attribute 60xx, 3000) = supported (with "bits allocated = 8")

7.1.2.1.3.4 Attribute Description for Waveforms

Waveform Sequence

- Sampling Frequency (attribute 003A,001A) = 2000
- Waveform Bits Allocated (attribute 5400,1004) = 16
- Waveform Bits Stored (attribute 003A,021A) = 16
- Modality (attribute 0008,0060) = "EPS". This applies to both the Hemodynamic and Electrophysiology applications in Sensis, because of the same sampling rate of 2000 Hz.

7.1.2.1.3.5 Private Information Object Definitions

To fulfill all application requirements, the Sensis DICOM implementation will use private IOD's to store Data currently not defined in the DICOM Standard according the DICOM information model. The privately defined IOD will contain all references to identify the Patient/Study/Series/Instances to which the related information belongs.

Currently this format is used for the proprietary "Event Log", "Presentation Log objects", "Ablation Graph" and "Mapping system images".

All IOD used to store this private Information will be based on various Instances of the SIEMENS Non-Image IOD.

Please see "SIEMENS Private Non-Image IOD" and "Private Non-Image IOD" in the Appendix for a detailed overview of the private IOD definition and the IOD tables for value encoding.

Note: The private Non-Image IODs are necessary for opening and viewing a Sensis study. So, it is mandatory that any DICOM node handling the Sensis study also supports these IODs.

7.1.2.1.3.6 **Attribute Description for Encapsulated PDF Reports**

- BurnedInAnnotation (attribute 0028,0301) = Yes
- MIMETypeOfEncapsulatedDocument (attribute 0042,0012) = application/pdf

7.1.3 **Association Acceptance Policy**

The Sensis DICOM application attempts to accept a new association for

- DIMSE C-ECHO
- DIMSE C-STORE

service operations. Any Information Objects transmitted on that association will be checked on conformance and stored in database if check was successful.

7.1.3.1 **Associated Real-World Activity - Receive**

7.1.3.1.1 **Associated Real-World Activity – Receiving Images or Encapsulated PDFs from a Remote Node**

The daemon receiving process will accept an association and will receive any images or Encapsulated PDF transmitted on that association and will store the images or Encapsulated PDF on disk in the own database if the conformance check is performed successfully.

7.1.3.1.2 **Accepted Presentation Context – Receiving Images or Encapsulated PDFs**

The Sensis DICOM storage provider will only accept MONOCHROME encoded images or Encapsulated PDFs.

Color encoded images (RGB or Palette Color) are not supported. Encapsulated PDF report can have colored exported waveform images.

The Sensis DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
		JPEG Lossy Baseline (Process 1) *1	1.2.840.10008.1.2.4.50		
		JPEG Lossy Extended *1 (Process 2 & 4)	1.2.840.10008.1.2.4.51		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Cardiac Electrophysiology Waveform Storage SOP Class	1.2.840.10008.5.1.4.1.1.9.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
CSA Non-Image Storage	1.3.12.2.1107.5.9.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Table 11 Proposed Presentation Context – Receiving Images

7.1.3.1.3 SOP-specific Conformance Statement – Receiving Images or Encapsulated PDFs

Upon successfully receiving a C-STORE-RQ, the Siemens Healthineers Sensis DICOM receiver performs a plausibility test on the received object and checks the availability of system resources. In the event of a successful C-STORE operation, the image object or Encapsulated PDF object has successfully been written on disk in the Siemens Healthineers Sensis image format or Encapsulated PDF object respectively. For Private Attributes of VR=SQ only a nesting level of one is supported. This means that Private Sequences containing another Sequence will be removed from the image header during Storage.

The Sensis DICOM application returns the status SUCCESS upon successful operation, otherwise one of the following status codes is returned and the association is aborted:

- Refused (A700):
This error status indicates a lack of Resources (e.g. not enough disk space) on the Sensis modality.
- Invalid Dataset (0xA900 or 0xC000):
An error occurred while processing the object which makes it impossible to proceed. The object will not be stored, and the association is aborted. The dataset may not contain one of the Attributes "Study Instance UID", "Series Instance UID" or "SOP Instance UID", or one of them might have an invalid value.
- Processing Error (0110):
An error occurred while processing the object, which makes it impossible to proceed.

Attention! Only after sending the response, the image will be saved into the database. If during this operation an error occurs, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

If an image instance is received that is identified by a SOP Instance UID which is already used by an Instance stored in database, then the actual received image will be discarded. The existing Instance is not superseded.

7.1.3.1.3.1 **Restrictions for Waveforms**

In Sensis only Waveforms generated by Sensis can be displayed and only if the corresponding NonImage objects are present in the same study.

The maximum size for Waveform objects is 600 MB to make them fit one CD for export and long-term storage.

7.1.3.1.4 **Presentation Context Acceptance Criterion**

The Sensis DICOM application will accept any number of verification or storage SOP classes that are listed above. The number of presentation contexts accepted is limited to the maximum of 127 (DICOM limit). If the Sensis DICOM application runs out of resources, it will reject the association request.

7.1.3.1.5 **Transfer Syntax Selection Policies**

The Sensis DICOM application currently supports

- the Implicit VR Little Endian, the Explicit VR Little Endian and Explicit VR Big Endian Transfer Syntaxes
- the JPEG Lossless Non-hierarchical Transfer Syntax
- the JPEG Baseline and JPEG Extended Transfer Syntaxes (JPEG Lossy).

Any proposed presentation context including one of these Transfer Syntaxes will be accepted. Any proposed presentation context that does not include one of these Transfer Syntaxes will be rejected.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

- 1) JPEG Lossy Extended
- 2) JPEG Lossless non-hierarchical
- 3) JPEG Lossy Baseline
- 4) Explicit VR Little Endian
- 5) Explicit VR Big Endian
- 6) Implicit VR Little Endian

With Implicit VR Little Endian Transfer Syntax, the Sensis DICOM application will remove any Private Attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute-dictionary of the Sensis DICOM application.

Therefore, any Explicit VR Transfer Syntax shall preferably be used by the Storage SCUs when sending Composite Image Instances to the Sensis DICOM application.

8 Implementation Model Storage Commitment

The Storage Commitment service class defines an application-level class of service which facilitates the commitment to storage. It performs an additional task of commitment of composite objects apart from the network-based storage of images as defined by the Storage Service class. The Sensis DICOM implementation supports the Storage Commitment Push Model as SCU.

8.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU for the Storage Commitment Push Model Service using the Storage Commitment Service Class. The product target Operating System is Microsoft Windows.

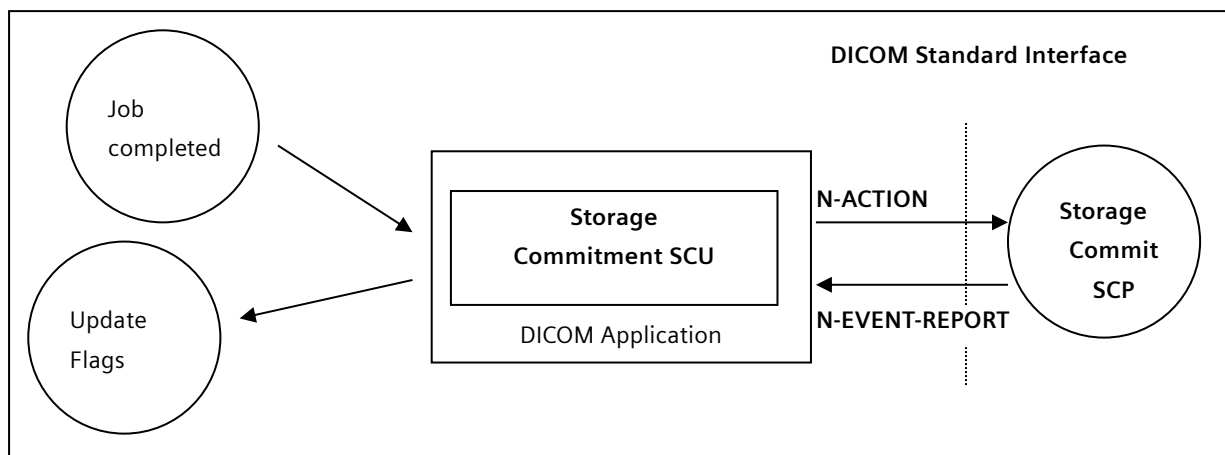


Figure 3 Application Data Flow Diagram - Storage Commitment SCU

8.2 Functional Definitions of Application Entities

With each successfully completed send job, the Sensis DICOM Application will create a Storage Commitment Push Model Identifier from the SOP Instances sent. Then a Storage Commit Request is triggered. Depending on configuration, the Sensis DICOM application will keep the association open for responses with a configurable time-out or closes the association and expects responses on a different association that must be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the related Status Flags of the related entity. It is possible to create triggers ("auto rules") from this event.

The Transaction UIDs of the pending commitment request are kept "open" for a configurable amount in time (default: 1h). If the "open time" for a pending commitment request has elapsed w/o a related response from the provider, the Transaction UID is removed, and the related entities are indicated as "commit failed".

In any case, commitment will only be requested for previously and successfully sent images.

8.3 Sequencing of Real-World Activities

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

9 AE Specification Storage Commitment

9.1 Storage Commitment AE Specification

SIEMENS HEALTHINEERS Sensis DICOM application provides Standard Conformance to the following DICOMV3.0 SOP Class as an SCU:

SOP Class Name	SOP Class UID
Storage Commitment Push Model	1.2.840.10008.1.20.1

Table 12 Storage Commitment SOP Class supported

9.1.1 Association Establishment Policies

9.1.1.1 General

With a Send Job successfully completed, the DICOM application will generate a Storage Commitment Identifier which references to all Instances of the processed job. The Commit Request is then sent over a single opened association. The Sensis will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and a timestamp, is kept. Depending on configuration, the association is closed when the configured time-out has elapsed, or a response was received before. If the association is closed before a response was received, the response is then expected on a different association. Multiple Storage Commitment Requests can be pending.

The default PDU size used will be 256 KB.

9.1.1.2 Number of Associations

The Sensis DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The Sensis DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

9.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

9.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

9.1.2 Association Initiation Policy

The Sensis DICOM Application Entity acts as a Service Class User (SCU) for the

- Storage Commitment Push Model Service Class (to request commitment for storage of instances previously sent).
To do so, the Sensis will issue a
- N-ACTION DIMSE to request commitment

© Siemens Healthcare GmbH. 2022. All rights reserved.

9.1.2.1 Real World Activity – Storage Commitment

9.1.2.1.1 Associated Real-World Activity - Job Completed

The Sensis Storage Commitment application sends the commit request (N-ACTION-RQ) message and waits for acceptance of this request (N-ACTION-RSP). After receiving this, the transaction is marked as “waiting”.

Depending on a configuration value, the association will then be closed or kept open. In the first case, there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N-EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association. For both cases, if the commit response (N-EVENT-REPORT) does not arrive during the configured time, the transaction will be marked as failed. The Sensis does not resend objects from a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of “complete - failure exists”, the transaction is marked as failed, else the transaction is marked as “completed”; In both cases, a message is shown to the user.

9.1.2.1.2 Proposed Presentation Contexts - Job Completed

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 13 Proposed Presentation contents – request Storage Commitment

9.1.2.1.3 SOP Specific Conformance Statement- Job Completed

Storage Commitment is supported for all the SOP class UIDs mentioned in Section 7.1.3.1.2.

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes will not be supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

9.1.2.1.4 Associated Real-World Activity - Update Flags

The Sensis Storage Commitment DICOM Application has sent a Storage Commitment Request and, being configured to receive response on a separate association, has closed the association, and now it gets an association request from the Storage Commitment SCP that want to send the results. The Sensis DICOM application will await Storage commitment Notification triggers. Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid, the Notification Event Information is evaluated, and the related Instances marked with the related status. The over-all Commit Status of the higher Information Entities is derived from propagation of the States of all Image entities included in a study.

The Status Flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of

- “AC” or “SC” - Successful Commitment, A means archived to configured Archive destination, whereas S means sent to any other destination

- "Af" of "Sf" - Commitment failed.
- "A?" or "S?" - Commitment request is sent, response is pending.

In case of failure the user has to repeat the transfer of images or Encapsulated PDFs to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

9.1.2.1.5 Accepted Presentation Contexts - Update Flags

The Siemens Healthineers Sensis DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Storage Commitment Push Model	1.2.840.10008.1.20.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 14 Accepted Presentation contents – request Storage Commitment

9.1.2.1.6 SOP-specific Conformance Statement - Update Flags

If the Commitment response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as failed, else the transaction is marked as "completed"; In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

The Sensis DICOM application will NOT support the Storage Media File Set ID attributes.

10 Implementation Model Query / Retrieve

The query/retrieve service class defines an application-level class of services which facilitates the management of images and patient data against the well-defined information model of DICOM and allows a DICOM AE to retrieve images from a remote DICOM node or to request a remote DICOM AE to initiate a transfer of images to another DICOM AE. The Sensis DICOM query/retrieve application supports the query/retrieve services to act as SCU and SCP.

10.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU and SCP for the query/retrieve network service. The product target Operating System is Microsoft Windows.

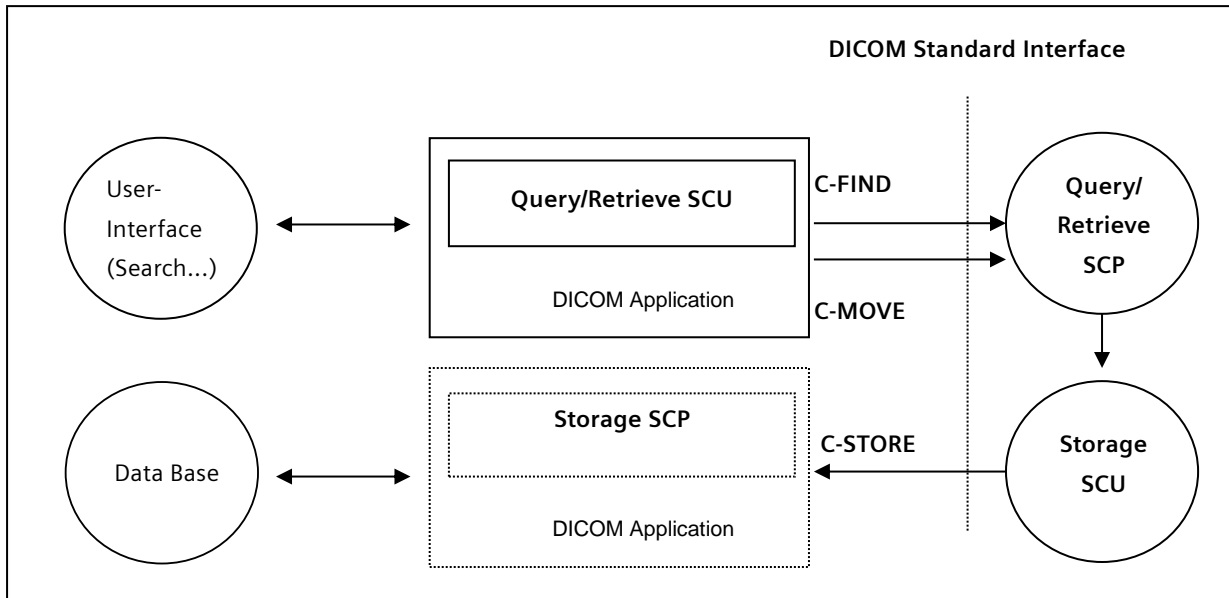


Figure 4 Application Data Flow Diagram - Query/Retrieve SCU

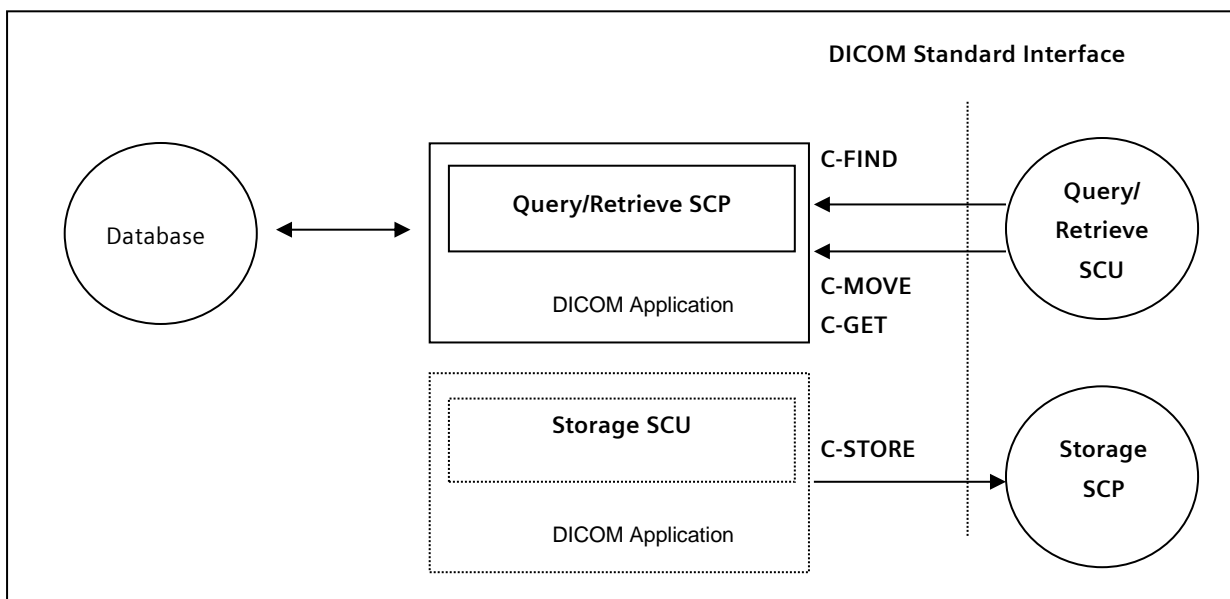


Figure 5 Application Data Flow Diagram - Query/Retrieve SCP

© Siemens Healthcare GmbH. 2022. All rights reserved.

10.2 Functional Definitions of Application Entities

The Sensis DICOM Query/Retrieve SCU requests the remote query/retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in the Sensis user interface. Depending on user action (Import) the Sensis DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the Sensis Storage SCP.

The Sensis DICOM Query/Retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote request, a C-GET or a C-MOVE involves the Sensis DICOM query/retrieve SCP application to initiate a C-STORE association (by triggering the own Storage SCU) to send image objects to a remote Storage SCP.

All components of the DICOM query/retrieve SCP application are operating as background server processes. They are running when the machine is powered on and respond to queries based on the records stored in the database.

10.3 Sequencing of Real-World Activities

Retrieve of images is only possible if results from a previous "Search..." operation are available, and those entities can be selected for "Import".

11 Application Entity Specification Query/Retrieve

11.1 Query/Retrieve Service AE Specification

The Query/Retrieve SCU requests that the remote SCP performs a match of all keys specified in the request, against the information in its database and the identified images will be moved over a different (C-MOVE) storage association.

The Query/Retrieve SCP responds to queries based on the records based on its database and images will be sent to the requesting SCU or to a different storage destination.

SIEMENS HEALTHINEERS Sensis DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as SCU:

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2

Table 15 Supported SOP Classes as SCU

SIEMENS HEALTHINEERS Sensis DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Classes as an SCP:

SOP Class Name	SOP Class UID
Patient Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1
Patient Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2
Patient Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.1.3
Study Root Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1
Study Root Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2
Study Root Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.2.3
Patient/Study Only Query/Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.3.1
Patient/Study Only Query/Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2
Patient/Study Only Query/Retrieve Information Model - GET	1.2.840.10008.5.1.4.1.2.3.3

Table 16 Supported SOP Classes as SCP

Note: See also the Storage DICOM Conformance Statement of the Sensis DICOM application to compare for conformance of the C-STORE sub-operation generated by the C-GET or C-MOVE DIMSE services. Furthermore, compare the supported Storage Service SOP classes described in the Storage DICOM Conformance Statement of the Modality to which the images shall be transferred to.

11.1.1 Association Establishment Policies

11.1.1.1 General

With the "Search..." function the query data are input and the DICOM query/retrieve application is started. A query request will be sent out to one remote node that can be selected from a list of configured Query Providers and the response data will be displayed for the user. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used will be 256 KB.

11.1.1.2 Number of Associations

The Sensis DICOM application initiates one association for each query request being processed to a remote node. The maximum number of active associations is configurable.

The Sensis DICOM application can accept multiple associations at a time. It can handle up to 10 associations in parallel.

11.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

11.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

11.1.2 Association Initiation Policy

The query user interface will request the query-data from the user and triggers one C-FIND request to the selected remote node. The response data will be displayed in the query UI for further data navigation.

When requesting Import of related items, the browser requests the retrieve application to send a C-MOVE request to the related remote node. Images will then be received by the Storage SCP as described in the related section.

The query/retrieve operation can be canceled at any time by a respective C-FIND-CANCEL or C-MOVE-CANCEL.

11.1.2.1 Real World Activity - Find SCU

11.1.2.1.1 Associated Real-World Activity - Find SCU "Search"

The associated Real-World activity is to fill out a query form with search data and pass it as query to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. When data transfer is finished the association is closed.

11.1.2.1.2 Proposed Presentation Contexts - Find SCU

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		

Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1. 1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.2. 1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 17 Proposed Presentation Contexts - Find SCU

It is configurable which of the two query models (or both) are to be used by the Sensis DICOM Query SCU application. If both Abstract Syntaxes are configured, The C-FIND SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the STUDY root model.

11.1.2.1.3 Conformance Statement - Find SCU

The Sensis DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. The interactive querying of attributes on IMAGE level is supported by the Query SCU, hence but no search criteria can be entered. So image level is always queried with a fixed list of "universal (Null)" values.

The following table describes the search keys for the different query models that the SCU supports. Matching is either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is requested as return value.

Attribute name	Tag	Type	Matching	User input	return value display
Patient Level²					
Patient Name	(0010,0010)	R	Wildcard ³	enter value	yes
Patient ID	(0010,0020)	U	Wildcard	enter value	yes
Patient's Birth date	(0010,0030)	O	universal (Null)	enter value	yes
Patient's Sex	(0010,0040)	O	universal (Null)	enter value	yes
Number of Patient related Studies	(0020,1200)	O	universal (Null)	-	yes ⁴
Number of Patient related Series	(0020,1202)	O	universal (Null)	-	no
Number of Patient related Instances	(0020,1204)	O	universal (Null)	-	no
Study Level					
Patient Name ⁵	(0010,0010)	R	Wildcard ³	enter value	yes
Patient ID	(0010,0020)	R	Wildcard ³	enter value	yes
Patient's Birth date ⁵	(0010,0030)	O	universal (Null)	enter value	yes
Patient's Sex ⁵	(0010,0040)	O	universal (Null)	enter value	yes
Study Instance UID	(0020,000D)	U	single value	-	yes

² Patient Root Information Model only

³ Always a "*" is appended to the user-supplied string

⁴ Implicitly visualized in the UI if no study and series search attributes have been entered

⁵ Study Root model only

Attribute name	Tag	Type	Matching	User input	return value display
Study ID	(0020,0010)	R	universal (Null)	enter value	yes
Study Date	(0008,0020)	R	universal (Null)	enter value	yes
Study Time	(0008,0030)	R	universal (Null)	-	yes
Accession Number	(0008,0050)	R	universal (Null)	-	yes
Study Description	(0008,1030)	O	universal (Null)	-	yes
Referring Physician's Name	(0008,0090)	O	universal (Null)	-	yes
Name of Physician Reading Study	(0008,1060)	O	universal (Null)	-	yes
Modalities in Study	(0008,0061)	O	universal (Null)	-	yes
Storage Media File-Set ID	(0008,0130)	O	universal (Null)	-	no
Retrieve AE Title	(0008,0054)	O	universal (Null)	-	no
Number of Study related Series	(0020,1206)	O	universal (Null)	-	yes
Number of Study related Instances	(0020,1208)	O	universal (Null)	-	no
Series Level					
Series Instance UID	(0020,000E)	U	single value	-	yes
Series Number	(0020,0011)	R	universal (Null)	-	yes
Modality	(0008,0060)	R	universal (Null)	enter value	yes
Series Date	(0008,0021)	O	universal (Null)	-	yes
Series Time	(0008,0031)	O	universal (Null)	-	yes
Series Description	(0008,103E)	O	universal (Null)	enter value	yes
Body Part Examined	(0018,0015)	O	universal (Null)	enter value	yes
Performing Physician	(0008,1050)	O	universal (Null)	enter value	yes
Storage Media File-Set ID	(0008,0130)	O	universal (Null)	-	yes
Retrieve AE Title	(0008,0054)	O	universal (Null)	-	yes
Protocol Name	(0018,1030)	O	universal (Null)	-	no
Perf. Procedure Step Start Date	(0040,0244)	O	universal (Null)	-	yes
Perf. Procedure Step Start Time	(0040,0245)	O	universal (Null)	-	yes
Requested Attribute Sequence	(0040,0275)	O	universal (Null)	-	yes
> Requested Procedure ID	(0040,1001)	O	universal (Null)	-	yes
> Scheduled Procedure ID	(0040,0009)	O	universal (Null)	-	yes
Number of Series related Instances	(0020,1209)	O	universal (Null)	-	yes

Attribute name	Tag	Type	Matching	User input	return value display
Instance Level					
SOP Instance UID	(0008,0018)	U	single value	-	no
Instance Number	(0020,0013)	R	universal (Null)	-	yes
Storage Media File-Set ID	(0008,0130)	O	universal (Null)	-	no
Retrieve AE Title	(0008,0054)	O	universal (Null)	-	no
Instance Date	(0008,0023)	O	universal (Null)	-	no
Instance Time	(0008,0033)	O	universal (Null)	-	no
Number of Frames	(0028,0008)	O	universal (Null)	-	yes
Image Comments	(0020,4000)	O	universal (Null)	-	no

Table 18 Search keys for Query models - Find SCU

The Find SCU interprets following status codes:

Service Status	Meaning	Protocol Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

Table 19 C-FIND response status

11.1.2.2 Real-World Activity – Move SCU

11.1.2.2.1 Associated Real-World Activity – Move SCU “Import”

When selecting a data entry in the Query UI and activate the “Import” function, a retrieval request is passed to the archival application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by processing the C-MOVE service.)

The transferred object data are processed as described in the storage class SCP descriptions.

The possibility to request the remote C-MOVE provider (remote application that responded to the C-FIND) to move data to an application entity other than the C-MOVE SCU (the Sensis DICOM application) is NOT USED.

C-MOVE operation on Patient Level is not supported by the Query UI.

11.1.2.2.2 Proposed Presentation Contexts - Move SCU “Import”

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 20 Proposed Presentation Contexts - Move SCU “Import”

Note: C-MOVE extended negotiation will not be supported by the SCU

11.1.2.2.3 SOP Specific Conformance Statement - Move SCU “Import”

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations must be done on a different association to transfer images to the own Storage Service Class SCP.

The Move SCU interprets following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	CXXX	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures or Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021)

Service Status	Meaning	Error Codes	Related Fields
			(0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Table 21 Status Codes - Move SCU "Import"

11.1.3 Association Acceptance Policy

The Sensis DICOM application will accept associations for the following DIMSE-C operations as SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

Extended negotiation - which is relational retrieve - is NOT supported for the above listed services. The Sensis DICOM application does support multiple C-FIND requests over the same association, while multiple C-MOVE or C-GET operations are not supported over the same association.

11.1.3.1 Real-World Activity - Find SCP

11.1.3.1.1 Associated Real-World Activity - Find SCP

The associated Real-World activity is to respond query requests to an SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is NOT supported. With a C-FIND-CANCEL request the running query can be canceled at any time.

Multiple C-FIND requests over the same association are supported.

11.1.3.1.2 Accepted Presentation Contexts - Find SCP

The Sensis DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Study Root Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model – FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 22 Accepted Presentation Contexts - Find SCP

Note: C-FIND Extended Negotiation will NOT be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian

11.1.3.1.3 SOP Specific Conformance Statement - Find SCP

The Sensis DICOM Query/Retrieve SCP supports hierarchical queries with all mandatory and optional search keys.

The query attribute contents will be treated case sensitive.

With wildcard queries the symbol “?” is treated as “*” by the C-FIND SCP application. As a consequence the query string of “?abc*” will be processed as “*abc*”.

If the value for the patient-level unique key “Patient ID” is not known, it may be returned with zero length. The attribute “Image Comments” will not be included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File-Set ID, Retrieve AE Title with C-FIND-RSP message:

- The Storage Media File-Set ID - if existent - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related Instance.
- The Retrieve AE Title - if existent - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are **not** supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation has completed.

The supported attributes on the various query levels of the three supported information models are list in the tables of the following sections.

11.1.3.1.3.1 Patient Root Information Model

Attribute Name	Tag	Usage SCU	Matching
Patient Level			
Patient Name	(0010,0010)	R	single value, wildcard, universal
Patient ID	(0010,0020)	U	single value, wildcard, universal
Patient’s Birth Date	(0010,0030)	O	single value, range, universal
Patient’s Birth Time	(0010,0032)	O	single value, range, universal
Patient’s Sex	(0010,0040)	O	single value, wildcard, universal
Ethnic Group	(0010,2160)	O	single value, wildcard, universal
Patient Comments	(0010,4000)	O	wildcard, universal

© Siemens Healthcare GmbH. 2022. All rights reserved.

Attribute Name	Tag	Usage SCU	Matching
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Level			
Study Instance UID	(0020,000D)	U	single value, list of UIDs
Study ID	(0020,0010)	R	single value, wildcard, universal
Study Date	(0008,0020)	R	single value, range, universal
Study Time	(0008,0030)	R	single value, range, universal
Accession Number	(0008,0050)	R	single value, wildcard, universal
Referring Physician's Name	(0008,0090)	O	single value, wildcard, universal
Study Description	(0008,1030)	O	single value, wildcard, universal
Admitting Diagnoses Description	(0008,1080)	O	single value, wildcard, universal
Patient's Age	(0010,1010)	O	single value, wildcard, universal
Patient's Size	(0010,1020)	O	single value, universal
Patient's Weight	(0010,1030)	O	single value, universal
Occupation	(0010,2180)	O	single value, wildcard, universal
Additional Patient History	(0010,21B0)	O	wildcard, universal
Name of Physician reading Study	(0008,1060)	O	single value, wildcard, universal
Modalities in Study	(0008,0061)	O	multiple values, universal
Number of Study related Series	(0020,1206)	O	universal
Number of Study related Instances	(0020,1208)	O	universal
Series Level			
Series Instance UID	(0020,000E)	U	single value, list of UID
Series Number	(0020,0011)	R	single value, universal
Modality	(0008,0060)	R	single value, wildcard, universal
Laterality	(0020,0060)	O	single value, wildcard, universal
Body Part Examined	(0018,0015)	O	single value, wildcard, universal
Patient Position	(0018,5100)	O	single value, wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	single value, universal
Largest Pixel Value in Series	(0028,0109)	O	single value, universal
Protocol Name	(0018,1030)	O	single value, wildcard, universal
Series Date	(0008,0021)	O	single value, range, universal
Series Time	(0008,0031)	O	single value, range, universal
Series Description	(0008,103E)	O	single value, wildcard, universal
Operators Name	(0008,1070)	O	single value, wildcard, universal
Performing Physician's Name	(0008,1050)	O	single value, wildcard, universal

Attribute Name	Tag	Usage SCU	Matching
Perf. Procedure Step Start Date	(0040,0244)	O	universal
Perf. Procedure Step Start Time	(0040,0245)	O	universal
Number of Series related Instances	(0020,1209)	O	universal
Instance Level			
SOP Instance UID	(0008,0018)	U	single value, list of UID
Image Number	(0020,0013)	R	single value, universal
Image Date	(0008,0023)	O	single value, range, universal
Image Time	(0008,0033)	O	single value, range, universal
Modality	(0008,0060)	O	single value, wildcard, universal
Image Comments	(0020,4000)	O	Universal

Table 23 Supported Query attributes sorted by Query Level – Patient Root Information Model

11.1.3.1.3.2 Study Root Information Model

Attribute Name	Tag	Usage SCU	Matching
Study Level			
Patient Name	(0010,0010)	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	R	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Instance UID	(0020,000D)	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	Single Value, Wildcard, universal
Study Date	(0008,0020)	R	Single Value, Range, universal
Study Time	(0008,0030)	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	Single Value, universal
Patient's Weight	(0010,1030)	O	Single Value, universal
Occupation	(0010,2180)	O	Single Value, Wildcard, universal
Additional Patient History	(0010,2180)	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	universal
Number of Study Related Instances	(0020,1208)	O	universal

© Siemens Healthcare GmbH. 2022. All rights reserved.

Attribute Name	Tag	Usage SCU	Matching
Series Level			
Series Instance UID	(0020,000E)	U	Single Value, List of UIDs
Series Number	(0020,0011)	R	Single Value, universal
Modality	(0008,0060)	R	Single Value, Wildcard, universal
Laterality	(0020,0060)	O	Single Value, Wildcard, universal
Body Part Examined	(0018,0015)	O	Single Value, Wildcard, universal
Patient Position	(0018,5100)	O	Single Value, Wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	Single Value, universal
Largest Pixel Value in Series	(0028,0109)	O	Single Value, universal
Protocol Name	(0018,1030)	O	Single Value, Wildcard, universal
Series Date	(0008,0021)	O	Single Value, Range, universal
Series Time	(0008,0031)	O	Single Value, Range, universal
Series Description	(0008,103E)	O	Single Value, Wildcard, universal
Operator's Name	(0008,1070)	O	Single Value, Wildcard, universal
Performing Physician's Name	(0008,1050)	O	Single Value, Wildcard, universal
Performed Procedure Step Start Date	(0040,0244)	O	universal
Performed Procedure Step Start Time	(0040,0245)	O	universal
Number of Series related Instances	(0020,1209)	O	universal
Instance Level			
SOP Instance UID	(0008,0018)	U	Single Value, List of UIDs
Image Number	(0020,0013)	R	Single Value, universal
Image Date	(0008,0023)	O	Single Value, Range, universal
Image Time	(0008,0033)	O	Single Value, Range, universal
Modality	(0008,0060)	O	Single Value, Wildcard, universal
Image Comments	(0020,4000)	O	universal

Table 24 Supported Query attributes sorted by Query Level – Study Root Information Model

11.1.3.1.3.3 Patient/Study Only Information Model

Attribute Name	Tag	Usage SCU	Matching
Patient Level			
Patient Name	(0010,0010)	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	U	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	Single Value, Wildcard, universal
Ethnic Group	(0010,2160)	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	universal
Number of Patient related Series	(0020,1202)	O	universal
Number of Patient related Instances	(0020,1204)	O	universal
Study Level			
Study Instance UID	(0020,000D)	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	Single Value, Wildcard, universal

© Siemens Healthcare GmbH. 2022. All rights reserved.

Attribute Name	Tag	Usage SCU	Matching
Study Date	(0008,0020)	R	Single Value, Range, universal
Study Time	(0008,0030)	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	Single Value, universal
Patient's Weight	(0010,1030)	O	Single Value, universal
Occupation	(0010,2180)	O	Single Value, Wildcard, universal
Additional Patient History	(0010,21B0)	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	universal
Number of Study Related Instances	(0020,1208)	O	universal

Table 25 Supported Query attributes sorted by Query Level – Patient/Study only Information Model

The Find SCP returns following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

Table 26 Status Codes

11.1.3.2 Real-World Activity - Get SCP

11.1.3.2.1 Associated Real-World Activity - Get SCP

The associated Real-World activity is to respond to retrieve requests initiated from a foreign SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by the C-GET service. Relational retrieve operation is NOT supported.

Multiple C-GET requests over the same association are NOT supported.

11.1.3.2.2 Accepted Presentation Contexts - Get SCP

The Sensis DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – GET	1.2.840.10008.5.1.4.1.2.1.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – GET	1.2.840.10008.5.1.4.1.2.2.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model – GET	1.2.840.10008.5.1.4.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 27 Accepted Presentation Contexts - Get SCP

Note: C-GET Extended negotiation will NOT be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

11.1.3.2.3 SOP Specific Conformance Statement - Get SCP

At association establishment time the C-GET presentation context must be negotiated along with the C-STORE sub-operations which must be accomplished on the same association as the C-GET operation. Relational retrieve operation is NOT supported.

The Get SCP returns following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020)

Service Status	Meaning	Error Codes	Related Fields
			(0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Table 28 Status Codes

11.1.3.3 Real-World Activity - Move SCP

11.1.3.3.1 Associated Real-World Activity - Move SCP

The associated Real-World activity is to respond to retrieve requests to an SCU. The SCP supports the query model Patient Root, Study Root and Patient/Study Only. The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by the C-MOVE service. Relational retrieve operation is NOT supported.

Multiple C-MOVE requests over the same association are NOT supported.

11.1.3.3.2 Accepted Presentation Contexts - Move SCP

The Sensis DICOM application will accept Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Study Root Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
Patient/Study Only Query/Retrieve Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 29 Accepted Presentation Contexts - Move SCP

Note: C-MOVE Extended negotiation will NOT be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

11.1.3.3.3 SOP Specific Conformance Statement - Move SCP

At association establishment time the C-MOVE presentation context shall be negotiated. The C-STORE sub-operations is done on a different association, specified in the C-MOVE request, to transfer images to a remote SCP of the Storage Service Class. Relational retrieve operation is NOT supported.

The Move SCP returns following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

Table 30 Status Codes

12 Implementation Model Worklist

The Basic Worklist Management Service class defines an application-level class of service that facilitates the transfer of worklists from the information system to the imaging modality. The worklist is queried by the AE and supplies the SCU with the scheduled tasks, which have to be performed on the modality. The Sensis DICOM worklist application supports the worklist service as SCU.

12.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU for the Basic Worklist Service using the Modality Worklist SOP Class. The product target Operating System is Microsoft Windows.

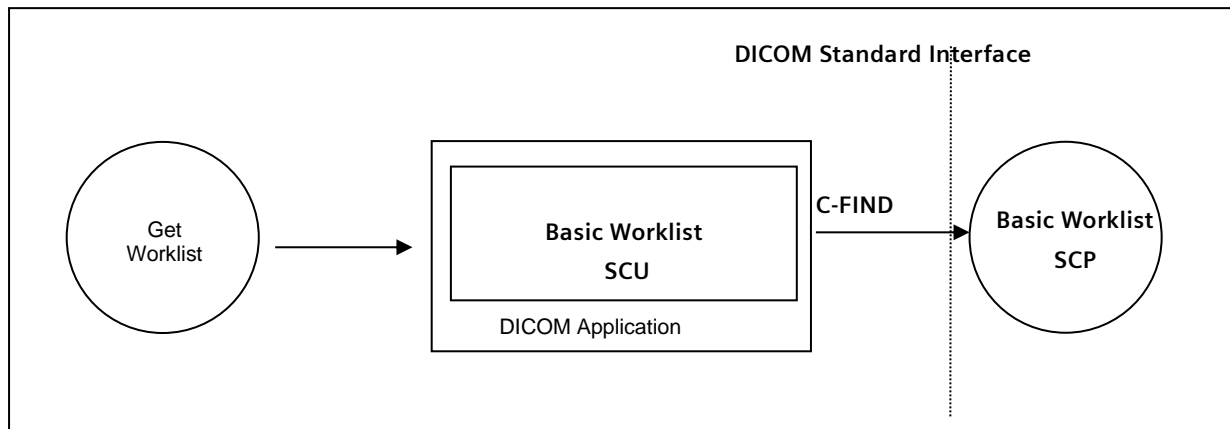


Figure 6 Application Flow Diagram – Basic Worklist SCU

12.2 Functional Definitions of Application Entities

The worklist SCU ("broad query") is invoked from the patient browser user interface or by timer to request the worklist from a remote Information System (Modality Worklist Class SCP). This is done to perform a match to the internal worklist query keys specified in the C-Find DIMSE service issued for the Modality Worklist Model.

The worklist SCP responds to the C-FIND query and scheduled imaging service requests (scheduled procedure steps) and patient demographic information will be downloaded from the information system to the Sensis modality. All information retrieved will be hold in the scheduling database for usage during patient registration procedure.

Furthermore, the patient-based Query dialog from the patient browser allows entering specific matching criteria ("narrow query") for the worklist query. With the response data the Patient Registration dialog can be populated according to availability within the worklist response identifier.

12.3 Sequencing of Real-World Activities

The "narrow" (interactive) Worklist Query requires that sufficient matching keys or a unique matching key are/is entered before the query is issued. Only then a single response can be expected to complete the registration dialog.

13 Application Entity Specification Worklist

13.1 Modality Worklist Service AE Specification

The Modality worklist SCU (patient registration in conjunction with the network application) requests that the remote SCP performs a match of all keys specified in the query against the information in its worklist database.

The Sensis DICOM network implementation acts as SCU for the Basic Worklist Service using the Modality Worklist SOP Class:

SOP Class Name	SOP Class UID
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31

Table 31 SOP Classes as a SCU

13.1.1 Association Establishment Policies

13.1.1.1 General

It is possible to configure a cyclic update of the modality scheduler database through a background worklist request with date/time and modality information.

In addition, the user can request worklist update with "Update Worklist". No duplicate entries will be added in the Scheduler DB. Entries are uniquely identified by the Study Instance UID (0020,000D) for the Requested Procedure and the SPS ID (0040,009) in the SPS Sequence (0040,0100).

An interactive worklist query can be issued with search criteria entered in the patient-based Query dialog from the patient browser.

The default PDU size used will be 256 KB.

13.1.1.2 Number of Associations

The Sensis DICOM application initiates one association at a time to query worklist entry data.

13.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

13.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

13.1.2 Association Initiation Policy

The network application will cyclically query the worklist provider and by request from the patient registration interface. It establishes an association by using the DICOM association services. During association establishment the negotiation of SOP classes to exchange the capabilities of the SCU and the SCP is not supported.

The following DIMSE-C operation is supported as SCU:

- C-FIND

13.1.2.1 Real-World Activity

13.1.2.1.1 Associated Real-World Activity - Query (Update) Worklist

A network application will perform worklist queries with the C-FIND request at regular intervals. In addition, it can be triggered by immediate request. The received worklist items will be compared with the contents of the local scheduler database. New items will be inserted into scheduler database.

After each broad-query, all RP/SPS that were canceled or rescheduled to another modality at the RIS will be automatically removed from the Scheduler DB if:

1. the Examination of this procedure has not been started or finished yet, and
2. the corresponding configuration item "Automatic removal of canceled/rescheduled Request" was checked in the Service UI under DICOM/HIS-RIS Node.

No automatic clean-up of the scheduler DB is performed after a Patient base Query since the worklist received does not give the complete list of all currently scheduled procedures for the modality.

13.1.2.1.2 Proposed Presentation Contexts

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Worklist Information Model- FIND	1.2.840.10008.5.1.4.31	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 32 Proposed Presentation Contexts

13.1.2.1.3 SOP Specific Conformance Statement

- Search Key Attributes of the Worklist C-FIND

The Sensis DICOM worklist SCU supports "broad worklist queries" with all required search keys. The following tables describe the "broad query" search keys that the SCU supports.

Attribute Name	Tag	Matching Key Type	Query Value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	N/A
>Scheduled Station AE Title <i>(This depends on user configuration (Options->Configuration->Patient Registration) if the "own AET" is provided or not. Use the "HIS/RIS" tab card for configuration.)</i>	(0040,0001)	R	<own AET> or <zero length>

Attribute Name	Tag	Matching Key Type	Query Value
>Scheduled Procedure Step Start Date <i>(It depends on user configuration (Options->Configuration->Patient Registration) if the actual Date with a full-time range or an interactive input dialog for date/time specification is used.)</i>	(0040,0002)	R	<act. Date>-<act. Date> or range from UI
>Scheduled Procedure Step Start Time <i>(It depends on user configuration (Options->Configuration->Patient Registration) if the actual Date with a full-time range or an interactive input dialog for date/time specification is used.)</i>	(0040,0003)	R	00.00-235959.00 or range from UI
>Modality <i>(This depends on user configuration (Options->Configuration->Patient Registration) if the "own Modality" is provided or not. Use the "HIS/RIS" tab card for configuration.)</i>	(0008,0060)	R	<zero length> or <own Modality>
>Scheduled Performing Physician	(0040,0006)	R	NULL

Table 33 Supported Broad Worklist Query Search Key Attributes

- Return Key Attributes of the Worklist C-FIND

The Sensis DICOM worklist SCU supports worklist queries with return key attributes of all types. The following tables describe the return keys that the SCU supports.

An "x" in the **UI** column will indicate the attribute is visualized when browsing the Worklist results with Patient Browser and/or during Patient Registration. The Patient Browser display is additionally influenced by the related Browser configuration.

A tag in the **IOD** column will indicate that the related attribute is included into the SOP Instances of the IODs created during processing of this worklist request.

A tag in the **MPPS** column will indicate that the related attribute is included into the SOP Instances of the MPPSs created during processing of this worklist request.

Note: For SIEMENS Word.Report XA image or Encapsulated PDF (see Appendix) some Worklist attributes will not be copied.

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
SOP Common					
Specific Character Set	(0008,0005)	1C	-	(0008,0005)	(0008,0005)
Scheduled Procedure Step					
Scheduled Procedure Step Sequence	(0040,0100)	1			
>Modality	(0008,0060)	1	x	(0008,0060)	(0008,0060)
>Requested Contrast Agent	(0032,1070)	2C	x	(0032,1070)	
>Scheduled Station AE Title <i>("Scheduled Station AE Title" is taken as default for "Performed Station AE Title")</i>	(0040,0001)	1	x		(0040,0241)
>Scheduled Procedure Step Start Date	(0040,0002)	1	x		

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
>Scheduled Procedure Step Start Time	(0040,0003)	1	x		
>Scheduled Procedure Step End Date	(0040,0004)	3	-		
>Scheduled Procedure Step End Time	(0040,0005)	3	-		
>Scheduled Performing Physician's Name (<i>"Scheduled Performing Physician's Name" is taken as default for "Performing Physician's Name"</i>)	(0040,0006)	1	x	(0008,1050)	(0008,1050)
>Scheduled Procedure Step Description (<i>"Scheduled Procedure Step Description" is taken as default for "Performed Procedure Step Description"</i>)	(0040,0007)	1C	x	(0040,0007) (0040,0254)	(0040,0007) (0040,0254)
>Scheduled Protocol Code Sequence (<i>universal Sequence Match</i>) (<i>"Scheduled Protocol Code Sequence" is taken as default for "Performed Protocol Code Sequence"</i>)	(0040,0008)	1C	-	(0040,0008) (0040,0260)	(0040,0008) (0040,0260)
>>Code Value	(0008,0100)	1C	x		
>>Coding Scheme Designator	(0008,0102)	1C	x		
>>Coding Scheme Version	(0008,0103)	3	x		
>>Code Meaning	(0008,0104)	3	x		
>Scheduled Procedure Step ID (<i>"Scheduled Procedure Step ID" is taken as default for "Performed Procedure Step ID"</i>)	(0040,0009)	1	x	(0040,0009) (0040,0253)	(0040,0009) (0040,0253)
>Scheduled Station Name	(0040,0010)	2	x		
>Scheduled Procedure Step Location (<i>"Scheduled Procedure Step Location" is taken as default for "Performed Location"</i>)	(0040,0011)	2	x		(0040,0242)
>Pre-Medication	(0040,0012)	2C	x		
>Scheduled Procedure Step Status	(0040,0020)	3	x		
>Comments on the Scheduled Procedure Step	(0040,0400)	3	-		
Requested Procedure					
Referenced Study Sequence (<i>universal Sequence Match</i>)	(0008,1110)	2	-	(0008,1110)	(0008,1110)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Study Instance UID	(0020,000D)	1	-	(0020,000D)	(0020,000D)
Requested Procedure Description	(0032,1060)	1C	x	(0032,1060)	(0032,1060)
Requested Procedure Code Sequence (<i>universal Sequence Match</i>) (<i>"Requested Procedure Code Sequence" is taken as default for "Procedure Code Sequence"</i>)	(0032,1064)	1C	-	(0008,1032) (0032,1064)	(0008,1032)
>Code Value	(0008,0100)	1C	x		
>Coding Scheme Designator	(0008,0102)	1C	x		
>Coding Scheme Version	(0008,0103)	3	x		
>Code Meaning	(0008,0104)	3	x		

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
Requested Procedure ID <i>("Requested Procedure ID" is taken as default for "Study ID")</i>	(0040,1001)	1	x	(0040,1001) (0020,0010)	(0040,1001) (0020,0010)
Reason for the Requested Procedure	(0040,1002)	3	-		
Requested Procedure Priority	(0040,1003)	2	x		
Patient Transport Arrangements	(0040,1004)	2	-		
Requested Procedure Location	(0040,1005)	3	-		
Confidentiality Code	(0040,1008)	3	-		
Reporting Priority	(0040,1009)	3	-		
Names of intended Recipients of Results	(0040,1010)	3	-	(0008,1048)	
Requested Procedure Comments	(0040,1400)	3	x		
Imaging Service Request					
Accession Number	(0008,0050)	2	x	(0008,0050)	(0008,0050)
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Requesting Physician	(0032,1032)	2	x	(0032,1032)	(0032,1032)
Requesting Service	(0032,1033)	3	x	(0032,1033)	
Reason for the Imaging Service Request	(0040,2001)	3	-		
Issuing Date of Imaging Service Request	(0040,2004)	3	-		
Issuing Time of Imaging Service Request	(0040,2005)	3	-		
Placer Order Number / Imaging Service Request <i>(Old tag (0040,2006) is retired and not used.)</i>	(0040,2016)	3	-		(0040,2016)
Filler Order Number / Imaging Service Request <i>(Old tag (0040,2007) is retired and not used.)</i>	(0040,2017)	3	-		(0040,2017)
Order entered by ...	(0040,2008)	3	-		
Order Enterer's location	(0040,2009)	3	-		
Order Callback Phone Number	(0040,2010)	3	-		
Imaging Service Request Comments	(0040,2400)	3	x		
Visit Identification					
Institution Name	(0008,0080)	3	x	(0008,0080)	
Institution Address	(0008,0081)	3	-	(0008,0081)	
Institution Code Sequence <i>(universal Sequence Match)</i>	(0008,0082)	3	-		
>Code Value	(0008,0100)	1C	-		
>Coding Scheme Designator	(0008,0102)	1C	-		
>Coding Scheme Version	(0008,0103)	3	-		
>Code Meaning	(0008,0104)	3	-		
Admission ID	(0038,0010)	2	x		
Issuer of Admission ID	(0038,0011)	3	-		
Visit Status					
Visit Status ID	(0038,0008)	3	-		
Current Patient Location	(0038,0300)	2	x		

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
Patient's Institution Residence	(0038,0400)	3	-		
Visit Comments	(0038,4000)	3	-		
Visit Relationship					
Referenced Study Sequence (<i>universal Sequence Match</i>)	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Sequence (<i>universal Sequence Match</i>)	(0008,1120)	2	-		(0008,1120)
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Visit Admission					
Referring Physician's Name	(0008,0090)	2	x	(0008,0090)	
Referring Physician's Address	(0008,0092)	3	-		
Referring Physician's Phone Numbers	(0008,0094)	3	-		
Admitting Diagnosis Description	(0008,1080)	3	x	(0008,1080)	
Admitting Diagnosis Code Sequence (<i>universal Sequence Match</i>)	(0008,1084)	3	-		
>Code Value	(0008,0100)	1C	-		
>Coding Scheme Designator	(0008,0102)	1C	-		
>Coding Scheme Version	(0008,0103)	3	-		
>Code Meaning	(0008,0104)	3	-		
Route of Admissions	(0038,0016)	3	-		
Admitting Date	(0038,0020)	3	-		
Admitting Time	(0038,0021)	3	-		
Patient Identification					
Patient's Name	(0010,0010)	1	x	(0010,0010)	(0010,0010)
Patient ID	(0010,0020)	1	x	(0010,0020)	(0010,0020)
Issuer of Patient ID	(0010,0021)	3	-	(0010,0021)	
Other Patient IDs	(0010,1000)	3	x	(0010,1000)	
Other Patient Names	(0010,1001)	3	x	(0010,1001)	
Patient's Birth Name	(0010,1005)	3	-	(0010,1005)	
Patient's Mother's Birth Name	(0010,1060)	3	-	(0010,1060)	
Medical Record Locator	(0010,1090)	3	-	(0010,1090)	
Patient Demographic					
Patient's Birth Date	(0010,0030)	2	x	(0010,0030)	(0010,0030)
Patient's Birth Time	(0010,0032)	3	-	(0010,0032)	
Patient's Sex	(0010,0040)	2	x	(0010,0040)	(0010,0040)
Patient's Insurance Plan Code Sequence (<i>universal Sequence Match</i>)	(0010,0050)	3	-	(0010,0050)	
>Code Value	(0008,0100)	1C	-		
>Coding Scheme Designator	(0008,0102)	1C	-		

Attribute Name	Tag	Return Key Type	UI	IOD	MPPS
>Coding Scheme Version	(0008,0103)	3	-		
>Code Meaning	(0008,0104)	3	-		
Patient's Age	(0010,1010)	3	x	(0010,1010)	
Patient's Size	(0010,1020)	3	x	(0010,1020)	
Patient's Weight	(0010,1030)	2	x	(0010,1030)	
Patient's Address	(0010,1040)	3	x	(0010,1040)	
Military Rank	(0010,1080)	3	x	(0010,1080)	
Branch of Service	(0010,1081)	3	-	(0010,1081)	
Country of Residence	(0010,2150)	3	-	(0010,2150)	
Region of Residence	(0010,2152)	3	-	(0010,2152)	
Patient's Telephone Numbers	(0010,2154)	3	-	(0010,2154)	
Ethnic Group	(0010,2160)	3	x	(0010,2160)	
Occupation	(0010,2180)	3	-	(0010,2180)	
Patient's Religious Preference	(0010,21F0)	3	-	(0010,21F0)	
Patient Comments	(0010,4000)	3	x	(0010,4000)	
Patient Data Confidentiality Constraint Description	(0040,3001)	2	x	(0040,3001)	
Patient Medical					
Medical Alerts	(0010,2000)	2	x	(0010,2000)	
Contrast Allergies	(0010,2110)	2	x	(0010,2110)	
Pregnancy Status	(0010,21C0)	2	x	(0010,21C0)	
Smoking Status	(0010,21A0)	3	x	(0010,21A0)	
Last Menstrual Date	(0010,21D0)	3	x	(0010,21D0)	
Additional Patient History	(0010,21B0)	3	x	(0010,21B0)	
Special Needs	(0038,0050)	2	x	(0038,0050)	
Patient State	(0038,0500)	2	x	(0038,0500)	
Patient Relationship					
Referenced Study Sequence (<i>universal Sequence Match</i>)	(0008,1110)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Visit Sequence (<i>universal Sequence Match</i>)	(0008,1125)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		
Referenced Patient Alias Sequence (<i>universal Sequence Match</i>)	(0038,0004)	3	-		
>Referenced SOP Class UID	(0008,1150)	1C	-		
>Referenced SOP Instance UID	(0008,1155)	1C	-		

Table 34 Basic Worklist C-FIND-RSP Return Key Attributes

Note on Specific Character Set (0008,0005)

If the C-FIND-RQ does not contain "specific characters", 0008,0005 will not be part of the C-FIND-RQ. If, however, the C-FIND-RSP contains "specific characters" in any of the Return Keys, it is expected, that (0008,0005) is part of the C-FIND-RSP from the MWL SCP.

13.1.2.1.4 Associated Real-World Activity – Get Worklist

With "Get Worklist" in the patient-based Worklist Query dialog, the entered attributes are used to form a worklist request identifier. With the response data the Patient Registration dialog can be updated to perform examination in advance. The response data are additionally placed in the scheduler database.

13.1.2.1.5 Proposed Presentation Contexts – Get Worklist

This RWA will propose the same Presentation Contexts as with "Update Worklist". Please see Table 32.

13.1.2.1.6 SOP Specific Conformance – Get Worklist

13.1.2.1.6.1 Search Key Attributes of the Worklist C-FIND

The Sensis DICOM worklist SCU supports "narrow worklist queries" with all required search keys. The following tables describe the "narrow query" search keys that the SCU supports.

Attribute Name	Tag	Matching Key Type	Query Value
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	R	input from UI or <zero length>
>Scheduled Performing Physician's Name	(0040,0006)	R	input from UI or <zero length>
Requested Procedure			
Requested Procedure ID	(0040,1001)	O	input from UI or <zero length>
Imaging Service Request			
Accession Number	(0008,0050)	O	input from UI or <zero length>
Referring Physician's Name	(0008,0090)	O	input from UI or <zero length>
Visit Status			
Current Patient Location	(0038,0300)	O	input from UI or <zero length>
Patient Identification			
Patient's Name	(0010,0010)	R	input from UI or <zero length>
Patient ID	(0010,0020)	R	input from UI or <zero length>

Table 35 Patient based "narrow query" Search Key Attributes

13.1.2.1.6.2 Return Key Attributes of the Worklist C-FIND

Please see list for "Update Worklist" RWA.

13.1.2.1.6.3 Status Codes of the Worklist C-FIND

The worklist SCU interprets following status codes:

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

Table 36 C-FIND-RSP Status

14 Implementation Model MPPS

The Modality Performed Procedure Step Service class defines an application-level class of service that facilitates the transfer of procedure, billing, and radiation dose information from the imaging modality to the information system. The Performed Procedure Step is created and set by the AE and supplies the SCP with the information about a real-world procedure which is performed on the modality. The Sensis DICOM Modality Performed Procedure Step application supports the MPPS service as SCU.

14.1 Application Data Flow Diagram

The Sensis DICOM network implementation acts as SCU for the Modality Performed Procedure Step SOP Class. The product target Operating System is Microsoft Windows.

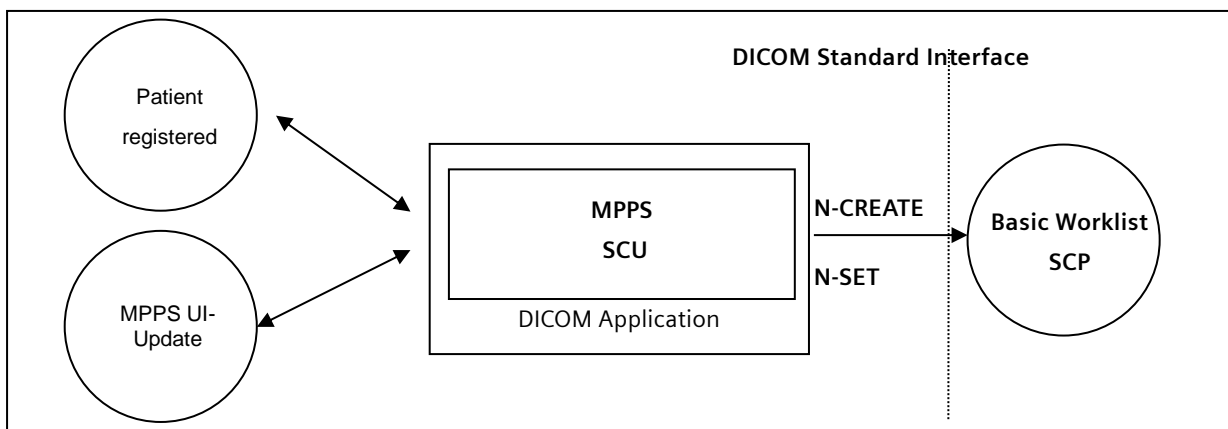


Figure 7 Application Flow Diagram – MPPS SCU

14.2 Functional Definitions of Application Entities

With registering a Patient (i.e. a Scheduled Procedure Step from Worklist), the Sensis DICOM application will create a MPPS Instance and communicate it to the MPPS SCP.

It is configurable to set the states of all related MPPS to "Completed" when a patient is closed. Furthermore, a manual update can be performed with the Sensis MPPS user interface. From the user interface it is possible to set the state of the MPPS to "Completed" or "Discontinued". After that the DICOM application will no longer allow updates on the related MPPS Instance.

The Sensis will not only allow a "1:1 -relationship" of Scheduled Procedure Steps and Performed Procedure Steps, but also supports the "simple group-case" (grouping several SPS of the same Requested Procedure), "complex group-case" (grouping several SPS from different Requested Procedures) and "append case" from the respective IHE-scenarios.

The Sensis will support creation of "unscheduled cases" by allowing MPPS Instances to be communicated for locally registered Patients.

14.3 Sequencing of Real-World Activities

An MPPS Update is only possible, if the MPPS Instance was created with Patient Registration before.

15 AE Specification MPPS

15.1 Modality Performed Procedure Step AE Specification

The Modality Performed Procedure Step SCU (Patient Registration and MPPS UI) provide information about a performed real-world Procedure to a remote SCP (Information System).

Siemens Healthineers Sensis DICOM products provide Standard Conformance to the following DICOM V3.0 SOP Class as an SCU:

SOP Class Name	SOP Class UID
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3

Table 37 SOP Classes as an SCU

15.1.1 Association Establishment Policies

15.1.1.1 General

The creation of MPPS Instance is done automatically by Sensis whenever a patient is registered for image acquisition through the Patient Registration dialog.

Further updates on the MPPS data can be done interactively from the related MPPS user interface. The MPPS “Complete” or “Discontinued” states can only be set from user interface.

The default PDU size used will be 256 KB.

15.1.1.2 Number of Associations

The Sensis DICOM application initiates one association at a time to create or set MPPS instance.

15.1.1.3 Asynchronous Nature

The Sensis DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

15.1.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

15.1.2 Association Initiation Policy

The Sensis DICOM Application Entity acts as a Service Class User (SCU) for the

- Modality Performed Procedure Step Service Class (to notify a RIS about status of a procedure while it is performed).

To do so, the Sensis will issue a

- N-CREATE DIMSE according to the CREATE Modality Performed Procedure Step SOP Instance operation or a

- N-SET DIMSE to update the contents and state of the MPPS according to the SET Modality Performed Procedure Step Information operation.

15.1.2.1 Real World Activity

15.1.2.1.1 Associated Real-World Activity - Patient registered

A patient is registered by the Patient Registration “Exam” action. From this event the trigger to create a MPPS Instance is derived. The related Instance is then immediately communicated to the configured RIS system. An association is established and the MPPS Instance is sent.

15.1.2.1.2 Proposed Presentation Contexts - Patient registered

The Sensis DICOM application will propose Presentation Contexts as shown in the following table:

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Modality Performed Procedure Step	1.2.840.10008.3.1.2.3.3	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

Table 38 Proposed Presentation Contexts – MPPS

15.1.2.1.3 SOP Specific Conformance Statement- Patient registered

15.1.2.1.3.1 Attributes used for the Performed Procedure Step N-CREATE

The Siemens Healthineers Sensis DICOM Modality Performed Procedure Step SCU informs the remote SCP when the examination of a scheduled procedure step will be performed (i.e. the patient is registered). The N-CREATE message is sent when the examination is started with successful registration of the patient data. The following table describes the supported attributes of a N-CREATE message.

Attribute Name	Tag	Type	Value
SOP Common			
Specific Character Set	(0008,0005)	1C	from MWL or created
Performed Procedure Step Relationship			
Scheduled Step Attribute Sequence	(0040,0270)	1	
>Study Instance UID	(0020,000D)	1	from MWL or created
>Referenced Study Sequence	(0008,1110)	2	from MWL or <zero length>
>>Referenced SOP Class UID	(0008,1150)	1C	
>>Referenced SOP Instance UID	(0008,1155)	1C	
>Accession Number	(0008,0050)	2	from MWL or user input
>Placer Order Number/Imaging Service Request	(0040,2016)	3	from MWL or <zero length>
>Filler Order Number/Imaging Service Request	(0040,2017)	3	from MWL or <zero length>
>Requested Procedure ID	(0040,0001)	2	from MWL or user input
>Requested Procedure Description	(0032,1060)	2	from MWL or <zero length>
>Scheduled Procedure Step ID	(0040,0009)	2	from MWL or <zero length>

Attribute Name	Tag	Type	Value
>Scheduled Procedure Step Description	(0040,0007)	2	from MWL or <zero length>
>Scheduled Protocol Code Sequence	(0040,0008)	2	from MWL or <zero length>
>>Code Value	(0008,0100)	1C	
>>Coding Scheme Designator	(0008,0102)	1C	
>>Coding Scheme Version	(0008,0103)	3	
>>Code Meaning	(0008,0104)	3	
Patient's Name	(0010,0010)	2	from MWL or user input
Patient ID	(0010,0020)	2	from MWL or user input
Patient's Birth Date	(0010,0030)	2	from MWL or user input
Patient's Sex	(0010,0040)	2	from MWL or user input
Referenced Patient Sequence	(0008,1120)	2	from MWL or <zero length>
>Referenced SOP Class UID	(0008,1150)	1C	
>Referenced SOP Instance UID	(0008,1155)	1C	
Performed Procedure Step Information			
Performed Procedure Step ID	(0040,0253)	1	From SPS ID or created
Performed Station AE Title	(0040,0241)	1	own AE Title
Performed Station Name	(0040,0242)	2	own hostname
Performed Location	(0040,0243)	2	from SPS location or <zero length>
Performed Procedure Step Start Date	(0040,0244)	1	created
Performed Procedure Step Start Time	(0040,0245)	1	created
Performed Procedure Step Status	(0040,0252)	1	"IN PROGRESS"
Performed Procedure Step Description	(0040,0254)	2	from SPS Description or <zero length>
Performed Procedure Type Description	(0040,0255)	2	<zero length>
Procedure Code Sequence	(0008,1032)	2	from Requested Procedure Code or <zero length>
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Procedure Step End Date	(0040,0250)	2	<zero length>
Performed Procedure Step End Time	(0040,0251)	2	<zero length>
Comments on the Performed Procedure Steps	(0040,0280)	3	<zero length>
Image Acquisition Results			
Modality	(0008,0060)	1	XA
Study ID	(0020,0010)	2	from Requested Procedure ID or created
Performed Protocol Code Sequence	(0040,0260)	2	from Scheduled Protocol Code Sequence or <zero length>
>Code Value	(0008,0100)	1C	
>Coding Scheme Designator	(0008,0102)	1C	
>Coding Scheme Version	(0008,0103)	3	
>Code Meaning	(0008,0104)	3	
Performed Series Sequence	(0040,0340)	2	

Attribute Name	Tag	Type	Value
>Performing Physician's Name	(0008,1050)	2C	from MWL or user input
>Operator's Name	(0008,1070)	2C	User input
>Series Instance UID	(0020,000E)	1C	created
>Series Description	(0008,103E)	2C	<zero length>
>Retrieve AE Title	(0008,0054)	2C	<zero length>
>Protocol Name	(0018,1030)	1C	from organ program
>Referenced Image Sequence	(0008,1140)	2C	<zero length>
>Referenced Non-Image Composite SOP Instance Sequence	(0040,0220)	2C	<zero length>
Radiation Dose			
Anatomic Structure, Space or Region Sequence	(0008,2229)	3	<zero length>
Total Time of Fluoroscopy	(0040,0300)	3	<zero length>
Total Number of Exposures	(0040,0301)	3	<zero length>
Distance Source to Detector	(0018,1110)	3	<zero length>
Distance Source to Entrance	(0040,0306)	3	<zero length>
Entrance Dose	(0040,0302)	3	<zero length>
Exposed Area	(0040,0303)	3	<zero length>
Image Area Dose Product	(0018,115E)	3	<zero length>
Comments on Radiation Dose	(0040,0310)	3	<zero length>
Billing and Material Management Code			
Billing Procedure Step Sequence	(0040,0320)	3	<zero length>
Film Consumption Sequence	(0040,0321)	3	
>Number of Films	(2100,0170)	3	<zero length>
>Medium Type	(2000,0030)	3	<zero length>
>Film Size ID	(2010,0050)	3	<zero length>
Billing Supplies and Devices Sequence	(0040,0324)	3	
>Billing Item Sequence	(0040,0296)	3	<zero length>
>Quantity Sequence	(0040,0293)	3	
>>Quantity	(0040,0294)	3	<zero length>
>>Measuring Units Sequence	(0040,0295)	3	<zero length>

Table 39 Performed Procedure Step N-CREATE Attributes

15.1.2.1.3.2 Status Codes of the Performed Procedure Step N-CREATE

The Performed Procedure Step SCU interprets following status codes:

Service Status	Meaning	Error Codes (0000.0900)
Failure	Processing Failure	0110
	No such attribute	0105
	Invalid attribute value	0106
	Duplicate SOP Instance	0111
	No such SOP Instance	0112
	No such SOP Class	0118
	Class Instance conflict	0119

	Missing attribute	0120
	Missing attribute value	0121
	Resource limitation	0213
Success	MPPS Instance created	0000

Table 40 MPPS N-CREATE Response Status

15.1.2.1.4 Associated Real-World Activity – MPPS UI-Update

With the MPPS UI the status of the MPPS Instance can be set to “COMPLETED” or “DISCONTINUED”. During performance of the procedure the status will remain “IN PROGRESS”.

15.1.2.1.5 Proposed Presentation Contexts – MPPS UI-Update

This RWA will propose the same Presentation Contexts as with “Patient registered”. Please see Table 38.

15.1.2.1.6 SOP Specific Conformance Statement – MPPS UI-Update

15.1.2.1.6.1 Attributes used for the Performed Procedure Step N-SET

The Siemens Healthineers Sensis DICOM Modality Performed Procedure Step SCU informs the remote SCP about the performed examination and its status. The N-SET message is sent after each acquisition (status “IN PROGRESS”) and per finished examination (finished status “COMPLETED” or incomplete status “DISCONTINUED”). The following table describes the supported attributes of a N-SET message.

Attribute Name	Tag	Type	Value
Performed Procedure Step Information			
Performed Procedure Step Status	(0040,0252)	3	“IN PROGRESS” during procedure, “COMPLETED” or “DISCONTINUED” for final N-SET
Performed Procedure Step Description	(0040,0254)	3	from SPS Description or user input
Performed Procedure Type Description	(0040,0255)	3	User input
Procedure Code Sequence	(0008,1032)	3	from Requested Procedure
>Code Value	(0008,0100)	1C	N/A
>Coding Scheme Designator	(0008,0102)	1C	N/A
>Coding Scheme Version	(0008,0103)	3	N/A
>Code Meaning	(0008,0104)	3	N/A
Performed Procedure Step End Date	(0040,0250)	1	created
Performed Procedure Step End Time	(0040,0251)	1	created
Image Acquisition Results			
Performed Protocol Code Sequence	(0040,0260)	3	from Scheduled Protocol Code Sequence
>Code Value	(0008,0100)	1C	N/A
>Coding Scheme Designator	(0008,0102)	1C	N/A
>Coding Scheme Version	(0008,0103)	3	N/A
>Code Meaning	(0008,0104)	3	N/A
Performed Series Sequence	(0040,0340)	1	N/A
>Performing Physician’s Name	(0008,1050)	2C	from MWL or user input
>Protocol Name	(0018,1030)	1C	from related SOP Instance
>Operator’s Name	(0008,1070)	2C	user input

Attribute Name	Tag	Type	Value
>Series Instance UID	(0020,000E)	1C	from related SOP Instance
>Series Description	(0008,103E)	2C	from related SOP Instance
>Retrieve AE Title	(0008,0054)	2C	N/A
>Referenced Image Sequence	(0008,1140)	2C	Series related SOP Instances as items
>>Referenced SOP Class UID	(0008,1150)	1C	N/A
>>Referenced SOP Instance UID	(0008,1155)	1C	N/A
>Referenced Standalone SOP Instance Sequence	(0040,0220)	2C	<zero length>
Radiation Dose			
Total Number of Exposures	(0040,0301)	3	N/A
Distance Source to Detector	(0018,1110)	3	N/A
Image Area Dose Product	(0018,115E)	3	N/A
Billing and Material Management Code			
Film Consumption Sequence	(0040,0321)	3	N/A
>Number of Films	(2100,0170)	3	<zero length>
>Medium Type	(2000,0030)	3	<zero length>
>Film Size ID	(2010,0050)	3	<zero length>

Table 41 Performed Procedure Step N-SET Attributes

15.1.2.1.6.2 Status Codes of the Performed Procedure Step N-SET

The Performed Procedure Step SCU interprets following status codes:

Service Status	Meaning	Error Codes (0000.0900)
Failure	Processing Failure: Performed Procedure Step Object may no longer be updated.	0110
	No such attribute	0105
	Invalid attribute value	0106
	No such SOP Instance	0112
	Invalid Object instance	0117
	No such SOP Class	0118
	Class Instance conflict	0119
	Missing attribute value	0121
	Resource limitation	0213
Success	MPPS Instance set	0000

Table 42 MPPS N-SET Response Status

15.1.2.1.6.3 Performed Procedure Step ID without MPPS

Handling of Performed Procedure Step ID in case

- MPPS is not configured or
- Unscheduled case

The attribute "Performed Procedure Step ID" (0040,0235) will be encoded based on "YYYYMMDDHHMMSS". This date and time is based on the time when the first image is acquired. The "Performed Procedure Step ID" stays the same for all acquired or derived images as long as the patient is re-registered. A re-registered patient with a new study or new series within the existing study will get a newly assigned "Performed Procedure Step ID".

16 **Communication Profiles**

16.1 **Supported Communication Stacks**

The Siemens Healthineers Sensis DICOM application provides DICOM TCP/IP Network Communication Support as defined in Part 8 of the DICOM Standard.
The product target Operating System is Microsoft Windows.

16.1.1 **TCP/IP Stack**

The Sensis DICOM application uses the TCP/IP stack from the target operating system upon which it executes. It uses the MergeCOM-3 subroutine library from Merge Technologies Inc. that is based on a Berkeley socket interface.

16.1.1.1 **API**

The Sensis DICOM application uses the MergeCOM library that is based on a TCP/IP socket interface.

16.1.1.2 **Physical Media Support**

The Sensis DICOM application is indifferent to the physical medium over which TCP/IP executes; it inherits this from the target operating system upon which it executes.

17 **Extensions / Specializations / Privatizations**

17.1.1 **Standard Extended / Specialized / Private SOPs**

Please refer to Annex A for further information on these topics. A detailed overview is given there.

17.1.2 **Private Transfer Syntaxes**

Not applicable.

18 Configuration

18.1 AE Title/Presentation Address Mapping

To ensure unique identification within the network the hostname should be used as part of the AE Titles (see examples below, hostname = NAME1). The string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters) are allowed according to DICOM Standard.

Note: the current implementation of *syngo*[®] does not support the full DICOM Standard. Spaces and special characters (like &<> ") in the AE title string are not supported.

18.1.1 DICOM Verification

The Verification Service uses the AE configuration of the DICOM Service that is checked with the C-ECHO message. e.g. Verification will use the Storage AE, if initiated to check the configuration of a remote DICOM node.

18.1.2 DICOM AE Titles

Within *syngo*[®] there are local application entity titles for HIS/RIS, Study Transfer and Print. They can be configured via Service-UI in "Configuration / DICOM / General".

18.1.2.1 DICOM Storage AE Title

The DICOM Storage application provides the application entity title which can be configured via Service UI in "Configuration/DICOM/General":

e.g. STU_NAME1

The port number is set to the fixed value of

104

18.1.2.2 DICOM Query/Retrieve AE Title

The DICOM Query/Retrieve application uses the same application entity title as the DICOM Storage AE.

18.1.2.3 DICOM Modality Worklist AE Title

The DICOM Modality Worklist application provides the application entity title which can be configured via Service UI in "Configuration/DICOM/General", e.g. HRI_NAME1.

18.2 Configurable Parameters

The Application Entity Titles, host names and port numbers for remote AE are configured using the Sensis Service/Installation Tool. For each AET the list of services supported can be configured.

18.2.1 Storage, Storage Commitment and Query/Retrieve

The Sensis Service/Installation Tool can be used to set the AETs, port-numbers, hostnames, IP-addresses and capabilities for the remote nodes (SCPs). The service user can select transfer syntaxes, compression modes and query models for each SCP separately.

The sending of the private SOP Class (Exam Protocol) can be disabled.

Additional configurable parameters for Storage Commitment are:

- flag to indicate whether the association will be kept open to receive the response or to close the association and be prepared to receive the response on another association.
- time-out which defines how long the association of N-ACTION is kept to receive a N-EVENT-REPORT on the same association. The same value is used to wait for a N-EVENT-REPORT on another association (default 1 h).

18.2.2 Modality Worklist

The Service application can be used to set the AET, port number, host name, IP address, capabilities and time-outs for the remote node (SCP)

Additional configurable parameters for Modality Worklist Query are:

- Query Waiting time - the time to wait for the C-FIND-RSP after sending the C-FIND-RQ (default 20 sec.)
- Max Query Match Number - the maximum number of entries accepted in one worklist (default is 200)
- Query Interval: the time between two C-FIND-RQ to the Hospital Information system (default is 60 min., minimum is 3 min., maximum is 1440 min. i.e. 24 hours)
- Broad Worklist Query behavior (two values are defined):
 - Set the AE Title search attribute to the own AE Title, and the Modality search attribute to <zero length>.
 - Set the Modality search attribute to the own modality and the AE Title search attribute to <zero length>.

18.3 Default Parameters

This installation tool also uses some default parameters:

- max PDU size set to 262144 Bytes (256 KB)
- time-out for accepting/rejecting an association request: 60 s
- time-out for responding to an association open/close request: 60 s
- time-out for accepting a message over network: 60 s
- time-out for waiting for data between TCP/IP-packets: 60 s

The time-outs for waiting for a Service Request/Response message from the remote node are as follows:

- for Storage SCP/SCU: 600 s
- for Storage Commitment SCU:
time-out for Response to N-ACTION: 600 s
- for Query/Retrieve SCP/SCU: 600 s

19 Support of Extended Character Sets

The Sensis DICOM application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

Also, the Japanese language character sets JIS X 0201 (ISO-IR 13 Japanese katakana and ISO-IR 14 Japanese romaji), JIS X 0208 (ISO-IR 87 Japanese kanji) and JIS X 0212 (ISO-IR 159 Supplementary Japanese kanji) are supported in the DICOM interfaces but will not be correctly represented in the generated reports.

When there is a mismatch between the "Specific Character Set" attribute (0008,0005) and the characters encoded in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?'.

20 Offline Media Conformance Statement

This chapter defines the Conformance Statement to all “Offline Media Application Profiles (incl. private extensions)” supported by the Sensis archive options. Those application profiles supported shall be:

- Basic Cardiac
- 1024 Extended Cardiac Application Profile
- General Purpose CDR Profiles
- Sensis private Application Profile

20.1 Implementation Model

20.1.1 Application Data Flow Diagram

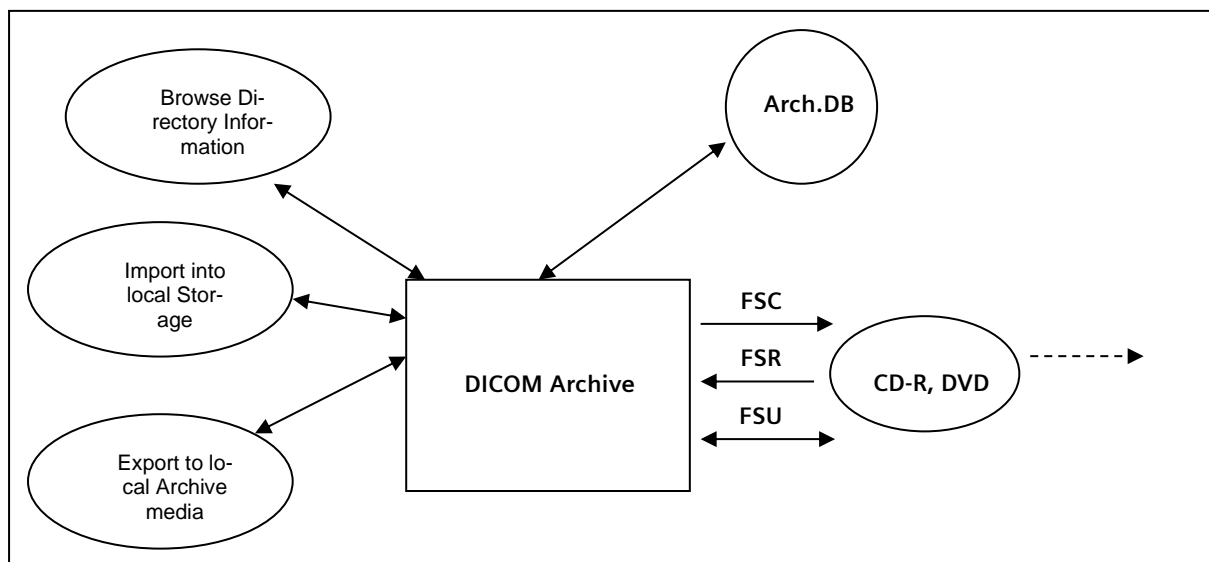


Figure 8 Application Data Flow Diagram

The DICOM archive application will serve as an interface to the CD-R offline medium device. It serves interfaces to include the offline media directory into the browser and to copy SOP instances to a medium or retrieve SOP instances from medium into local storage.

The DICOM Archive application will support the 120mm CD-R and DVD medium.

The FSU role will update new SOP instances only to media with pre-existing File-sets conforming to the Application Profiles supported.

The contents of the DICOMDIR will be temporarily stored in Archive-Database.

20.1.2 Functional Definitions of AEs

The Sensis DICOM offline media storage application consists of the DICOM Archive application entity serving all interfaces to access offline media. The DICOM Archive application is capable of

- 1) creating a new File-set onto an unwritten medium (Export to...).

- 2) updating an existing File-set by writing new SOP Instances onto the medium (Export to...).
- 3) importing SOP Instances from the medium onto local storage
- 4) reading the File-sets DICOMDIR information into temporary database and pass it to display applications.

20.1.3 Sequencing of Real-World Activities

The DICOM Archive application will not perform updates before the Directory information of the DICOMDIR is completely read.

When performing updates, the SOP instances are checked for existence before updating. Duplicate instances will be avoided.

20.1.4 Implementation Identifying Information

Please refer to Table 3 in the overview.

20.2 AE Specifications

20.2.1 DICOM Archive Specification

The DICOM Archive provides Standard conformance to Media Storage Service Class (Interchange Option). In addition, Augmented conformance is provided to store extra data attributes important for the full feature support of the Sensis product SW. Details are listed in following Table:

Application Profiles Supported	Real-World Activity	Role	SC Option
PRI-XAMAS-CD AUG-XA1K-CD *1	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange
	Export to local Archive Media	FSC, FSU	Interchange
STD-GEN-CD STD-XABC-CD STD-XA1K-CD	Browse Directory Information	FSR	Interchange
	Import into local Storage	FSR	Interchange

*1 – With no Private SOP Class used, the PRI-SYNGO-CD profile definitions are appropriate to describe the augmentation of the related -STD Profiles.

Table 43 Application profiles, Activities, and Roles for DICOM Archive

On Sensis based Systems, the Private Extended *syngo*[®] Profiles (PRI-SYNGO-CD) will be preferably used by the system. The General Purpose Interchange Profile (STD-GEN-CD), Basic Cardiac Profile (STD-XABC-CD) and 1024 X-Ray Angiographic Profile (STD-XA1K-CD) will be supported with read, write, and update capability of the related media.

For DVD profiles the same rules apply as for CD profiles.

20.2.1.1.1 File Meta Information for the Application Entity

The Source Application Entity Title is set by configuration. See Section 20.5 for details.

20.2.1.2 Real-World Activities for this Application Entity

20.2.1.2.1 Real-World Activity: Browse Directory Information

The DICOM Archive application acts as FSR using the interchange option when requested to read the media directory.

The DICOM archive application will read the DICOMDIR and insert those directory entries, that are valid for the application profiles supported, into a local database. The database can then be used for browsing media contents.

Note

Icon Image SQ is also supported in DICOMDIR. But only those Icon Images with Bits Allocated (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

20.2.1.2.1.1 Application Profiles for the RWA: Browse Directory Information

See Table 43 for the Application Profiles listed that invoke this Application Entity for the Browse Directory Information RWA.

20.2.1.2.2 Real-World Activity: Import into local Storage

The DICOM Archive application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the local storage.

The SOP Instance selected from the media directory will be copied into the local storage. Only SOP Instances, that are valid for the application profile supported and are listed as supported by the Storage SCP Conformance section (see Section 7.1.3.1.2), can be retrieved from media storage. This is because the Browse Directory Information will filter all SOP Instances not matching the Application profiles supported.

During operation no "Attribute Value Precedence" is applied to the SOP Instances. Detached Patient Management is not supported.

For media conforming to the STD-GEN-CD Profile the following SOP classes will be supported as an FSR:

Information Object Definition	SOP Class UID	Transfer Syntax UID
X-Ray Angiographic Image	1.2.840.10008.5.1.4.1.1.12.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1
Cardiac Electrophysiology Waveform Storage SOP Class	1.2.840.10008.5.1.4.1.1.9.3.1	Explicit VR Little Endian 1.2.840.10008.1.2.1
CSA Non-Image	1.3.12.2.1107.5.9.1	Explicit VR Little Endian Uncompressed 1.2.840.10008.1.2.1

Table 44 STD-GEN-CD Supported SOP Classes for FSR Role

20.2.1.2.2.1 Application Profiles for the RWA: Import into local Storage

See Table 43 for the Application Profiles listed that invoke this Application Entity for the Import into Local Storage RWA.

20.2.1.2.3 Real-World Activity: Export to local Archive Media

The DICOM Archive application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium.

The DICOM Archive application will receive a list of SOP Instances to be copied to the local archive medium. According to the state of the medium inserted (new medium, Medium with DICOM file-set) the validity of the SOP Instances according to the applicable profile is checked. Only valid SOP Instances are accepted.

When the DICOM archive application is requested to copy SOP Instances the preferred application profile according to configuration (AUG-XA1K-CD or PRI-XAMAS-CD) will be used to validate and copy the referred SOP Instances. When creating a new file-set no Descriptor File will be allocated and the related ID is not used.

The DICOM archive application will not close the medium.

20.2.1.2.3.1 **Application Profiles for the RWA: Export to local Archive Media**

See Table 43 for the Application Profiles listed that invoke this Application Entity for the Export to local Archive Media RWA.

20.3 **Augmented and Private Profiles**

20.3.1 **Augmented Application Profiles**

With no private SIEMENS Non-Images stored onto Medium, the definitions of the PRI-XAMAS-CD Profile are applicable to denote the augmentations for the STD-XA1K-CD Standard Profile.

Storage of Private Information Objects will only be supported with reference to a Private Application Profile (see next section).

20.3.2 **Private Application Profiles**

20.3.2.1 **PRI-XAMAS-CD**

The DICOM Archive application is conforming to the PRI-XAMAS-CD application profile provided in a separate document. Please refer to next section for detailed definition of SOP classes supported in accordance with this Application Profile.

20.4 **Extensions, Specialization and Privatization of SOP Classes**

The SOP Classes listed refer in majority to those created by the equipment to which this conformance Statement is related to. For SOP classes not listed in this section, please refer to the Storage section of the DICOM Conformance Statement of the product. This will include all SOP Instances that can be received and displayed and therefore will be included into offline media storage even though these SOP Instances are not created by the equipment serving the Media Storage Service.

20.4.1 **SOP Specific Conformance Statement for Basic Directory**

The Basic Directory Header will not contain Information to indicate the current medium is part of a sequence of multiple media holding the Objects of one patient/study in total.

20.4.1.1 **Extension, Specialization for SIEMENS Non-Image Objects**

According to the PRI-XAMAS Application Profile Class the usage of the Private Creator UIDs and further optional keys for the Directory Records referring to SIEMENS Non-Image Objects are listed in the following tables.

Attribute	Tag	Value used
Private Record UID	(0004,1432)	1.3.12.2.1107.5.9.1
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1

Table 45 Extension, Specialization for SIEMENS Non-Image Objects

For those “Non-Images” no Icon Image Sequence will be generated.

20.5 Configuration

20.5.1 AE Title Mapping

20.5.1.1 DICOM Media Storage AE Title

The DICOM Storage application provides the application entity title:

- CsImageManager

20.6 Support of Extended Character Sets

The Siemens Healthineers Sensis DICOM archive application supports the ISO 8859 Latin 1 (ISO-IR 100) character set.

Also, the Japanese language character sets JIS X 0201 (ISO-IR 13 Japanese katakana and ISO-IR 14 Japanese romaji), JIS X 0208 (ISO-IR 87 Japanese kanji) and JIS X 0212 (ISO-IR 159 Supplementary Japanese kanji) are supported in the DICOM interfaces but will not be correctly represented in the generated reports.

When there is a mismatch between the SCS tags (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Try to import with ISO_IR 100. If ISO_IR 100 fails, convert each illegal character to a '?'.

Annex A: Additional Information

A.1 SIEMENS Waveform IOD description

Attribute	Tag	Value
Group 0002 Length	(0002,0000)	
File Meta Information Version	(0002,0001)	==> binary data; value is 2 bytes long
Media Storage SOP Class UID	(0002,0002)	1.2.840.10008.5.1.4.1.1.9.3.1
Media Storage SOP Instance UID	(0002,0003)	1.3.12.2.1107.5.13.2.serialno.uniqueid
Transfer Syntax UID	(0002,0010)	1.2.840.10008.1.2.1
Implementation Class UID	(0002,0012)	1.3.12.2.1107.5.9.20000101
Implementation Version Name	(0002,0013)	"SIEMENS_SWFVE31F"
Source Application Entity Title	(0002,0016)	No value
Private Information Creator UID	(0002,0100)	No value
Private Information	(0002,0102)	No value
Specific Character Set	(0008,0005)	from Configuration
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.9.3.1
SOP Instance UID	(0008,0018)	1.3.12.2.1107.5.13.2.serialno.x.yyyyyyyyyyy
Study Date	(0008,0020)	<yyyymmdd>
Content Date	(0008,0023)	<hhmmss>
Acquisition Datetime	(0008,002A)	<yyyymmdd hhmmss mmmm>
Study Time	(0008,0030)	<hhmmss mmmm>
Content Time	(0008,0033)	<hhmmss mmmm>
Accession Number	(0008,0050)	RIS or "Accession Number" input
Modality	(0008,0060)	"EPS"
Manufacturer	(0008,0070)	"Siemens Healthineers"
Institution Name	(0008,0080)	From system configuration
Referring Physician's Name	(0008,0090)	RIS or "Referring Physician's name" input
Instance Creation Date	(0008,0012)	Date of report creation
Instance Creation Time	(0008,0013)	Time of report creation
Series Description	(0008,103E)	"WAVEFORM SERIES"
Manufacturer's Model Name	(0008,1090)	"Sensis Vibe"
Patient's Name	(0010,0010)	RIS or "Patient Name" input
Patient ID	(0010,0020)	RIS or "Patient ID" input
Patient's Birth Date	(0010,0030)	<yyyymmdd>
Patient's Sex	(0010,0040)	"M", "F" or "O"
Other Patient IDs	(0010,1000)	N/A
Other Patient Names	(0010,1001)	N/A
Patient's Age	(0010,1010)	calculated from "DoB" input
Patient's Address	(0010,1040)	"Address" input"
Military Rank	(0010,1080)	"Military Rank input"
Synchronization Trigger	(0018,106A)	"NO TRIGGER"
Acquisition Time Synchronized	(0018,1800)	"N"
Patient Position	(0018,5100)	From "Patient Position" input
Study Instance UID	(0020,000D)	from RIS or system generated
Series Instance UID	(0020,000E)	System generated
Study ID	(0020,0010)	RIS or "Study ID" input
Series Number	(0020,0011)	System generated

Attribute	Tag	Value
Instance Number	(0020,0013)	System generated
Synchronization Frame of Reference UID	(0020,0200)	UID System generated
Private Creator	(0029,0010)	"SIEMENS CSA HEADER"
Modality Series Header Type	(0029,1018)	"WAVEFORMSERIES"
Modality Series Header Version	(0029,1019)	From system label
Modality Series Header Info	(0029,1020)	N/A
Requesting Physician	(0032,1032)	N/A
Requested Procedure Description	(0032,1060)	From RIS
Study Completion Date	(0032,1050)	<yyyymmdd>
Study Completion Time	(0032,1051)	<hhmmss mmmm>
Acquisition Context Sequence	(0040,0555)	N/A
Annotation Sequence	(0040,B020)	N/A
> Concept-name Code Sequence	(0040,A043)	System generated
>> Code Value	(0008,0100)	System codes
>> Coding Scheme Designator	(0008,0102)	System coding scheme
>> Code Meaning	(0008,0104)	System generated depending on user action
> Referenced Waveform Channels	(0040,A0B0)	System generated depending on affected channel
> Temporal Range Type	(0040,A130)	System generated depending on user action
> Referenced Datetime	(0040,A13A)	<yyyymmdd hhmmss mmmm> See note 1
> Concept Code Sequence	(0040,A168)	N/A
>> Code Value	(0008,0100)	N/A
>> Coding Scheme Designator	(0008,0102)	N/A
>> Code Meaning	(0008,0104)	N/A
Waveform Sequence	(5400,0100)	N/A
> Waveform Originality	(003A,0004)	"ORIGINAL"
> Number of Waveform Channels	(003A,0005)	From configuration
> Number of Waveform Samples	(003A,0010)	Recording length times sampling frequency
> Sampling Frequency	(003A,001A)	"2000"
> Mux Group Label	(003A,0020)	From configuration: "ECG", "IECG", "Pressure", or "Indicator" or user defined from configuration.
> Channel Definition Sequence	(003A,0200)	N/A
>> Waveform Channel Number	(003A,0202)	System number
>> Channel Label	(003A,0203)	User configuration
>> Channel Status	(003A,0205)	"OK" or "Disconnected"
>> Channel Source Sequence	(003A,0208)	Several channels at "pullback". See note 2
>>> Code Value	(0008,0100)	System codes
>>> Coding Scheme Designator	(0008,0102)	System coding scheme
>>> Code Meaning	(0008,0104)	System meaning
>> Channel Source Modifier Sequence	(003A,0209)	Electrode positions or "pullback" sites. From configuration
>>> Code Value	(0008,0100)	System codes
>>> Coding Scheme Designator	(0008,0102)	System coding scheme
>>> Code Meaning	(0008,0104)	N/A
>> Channel Sensitivity Units Sequence	(003A,0211)	System generated. See note 2
>> Channel Sensitivity Correction Factor	(003A,0212)	System generated
>> Channel Baseline	(003A,0213)	System generated
>> Channel Time Skew	(003A,0214)	0
>> Waveform Bits Stored	(003A,021A)	16
>> Filter Low Frequency	(003A,0220)	From configuration

Attribute	Tag	Value
>> Filter High Frequency	(003A,0221)	From configuration
>> Notch Filter Frequency	(003A,0222)	From configuration
>> Channel Label	(003A,0203)	System generated. Defines channel types
> Waveform Bits Allocated	(5400,1004)	16
> Waveform Sample Interpretation	(5400,1006)	"SS"
>Waveform Padding Value	(5400,100A)	==> binary data; value is 2 bytes long
> Waveform Data	(5400,1010)	==> binary data;

Table 46 WF IOD description for instances created by Sensis

Note 1: The time in the recorded data to which the Annotation applies is denoted by the Referenced Datetime (0040, A13A) attribute. The Referenced Waveform Channel (0040, A0B0) refers to the (M, C) value pair of the same channel.

Note 2: For the objects of Channel Source Modifier Sequence and Channel Sensitivity Units Sequence, the Code Value, Code Scheme Designator and Code Meaning for Waveform IODs created by Sensis Vibe are internal codes and no standard coding scheme is used or may be empty.

A.2 SIEMENS Encapsulated PDF IOD description

Module	Attribute Name	TAG	Type	Comments
Patient	Patient's Name	0010,0010	2	RIS or "Patient Name" input
	Patient ID	0010,0020	2	RIS or "Patient ID" input
	Patient's Birth Date	0010,0030	2	RIS or "Patient Birth Date" input
	Patient's Sex	0010,0040	2	RIS or "Patient Sex" input
	Patient's Age	0010,1010	2	calculated from "DoB" input
General Study	Study Instance UID	0020,000D	1	System generated
	Study Date	0008,0020	2	System generated
	Study Time	0008,0030	2	System generated
	Referring Physician's Name	0008,0090	2	RIS or "Referring Physician's name" input
	Study ID	0020,0010	2	RIS or "Study ID" input
	Accession Number	0008,0050	2	RIS or "Accession No" input
	Study Description	0008,1030	3	RIS or "Study Description" input
	Acquisition Datetime	0008, 002A		<yyyymmdd hhmmss >
Encapsulated Document Series	Modality	0008,0060	1	"XA"
	Series Instance UID	0020,000E	1	System generated
	Series Number	0020,0011	2	System generated
	Series Date	0008,0021	3	Date of report creation
	Series Time	0008,0031	3	Time of report creation
	Series Description	0008.103E	3	"Sensis Report Series"
General Equipment	Manufacturer	0008,0070	2	"Siemens Healthineers"
	Institution Name	0008,0080	3	RIS or "Institution Name" input
	Institution Address	0008.0081	3	RIS or "Institution Address" input
	Manufacturer's Model Name	0008,1090	3	"Sensis Vibe"
	Station Name	0008,1010	3	Station Name
	Device Serial Number	0018,1000	3	Device Serial Number
SC Equipment	Conversion Type	0008,0064	1	"WSD"
Encapsulated Document	Instance Number	0020,0013	2	System generated
	MIME Type Of Encapsulated Document	0042,0012	3	application/pdf
	Encapsulated PDF Document	0042,0011	3	Encapsulated Document stream, containing a document encoded according to the MIME Type
	Document Title	0042,0010	3	Document Title
	Burned in Annotation	0028,0301	3	"YES"
	Content Date	0008,0023	2C	Date of report creation
	Content Time	0008,0033	2C	Time of report creation
	Concept name Code Sequence	0040,A043	2	System generated
	>Code Value	0008,0100	2	"4238976004"
	> Coding Scheme Designator	0008,0102	2	"SCT"
> Code Meaning	0008,0104	2	"Clinical document (record artifact)"	
SOP Common	SOP Class UID	0008,0016	1	1.2.840.10008.5.1.4.1.1.104.1
	SOP Instance UID	0008,0018	1	System generated
	Specific Character Set	0008,0005	1C	"ISO_IR 100"
	Instance Creation Date	0008,0012	3	Date of report creation
	Instance Creation Time	0008,0013	3	Time of report creation

Table 47 Encapsulated PDF IOD description for instances created by Sensis

Note: The resulting PDF size depends on the report type

Report Type	PDF Type Value	Report Size	Comments
PDF document	PDF REPORT	A4(210mm x 297mm)	If user chooses the report template of A4 size type
	PDF REPORT	Letter(215.9mm x 279.4mm)	If user chooses the report template of Letter size type

Table 48 Sensis PDF report types

A.3 SIEMENS Private Non-Image IOD

For encoding binary data-streams not representing image data, Siemens Healthineers has created a private “Non-Image IOD” according to the rules governed by the DICOM Standard. The following section will define this Private IOD. It can be communicated with Network Storage Service and Offline Media Storage Services.

The SIEMENS “Non-Image IOD” is identified by a private Non-Image Storage SOP Class UID.

Private Non-Image Object	Private Non-Image IOD
CSA Non-Image	1.3.12.2.1107.5.9.1

Table 49 SIEMENS Private Non-Image IOD

A.3.1 SIEMENS Non-Image IOD – E-R Model

The E-R model in A.3.2 depicts those components of the DICOM Information Model which directly refer to the SIEMENS Non-Image IOD. The Frame of Reference IE, Overlay IE, Modality Lookup-Table IE, VOI Lookup-Table IE and Curve IE are not components of the SIEMENS Non-Image IOD.

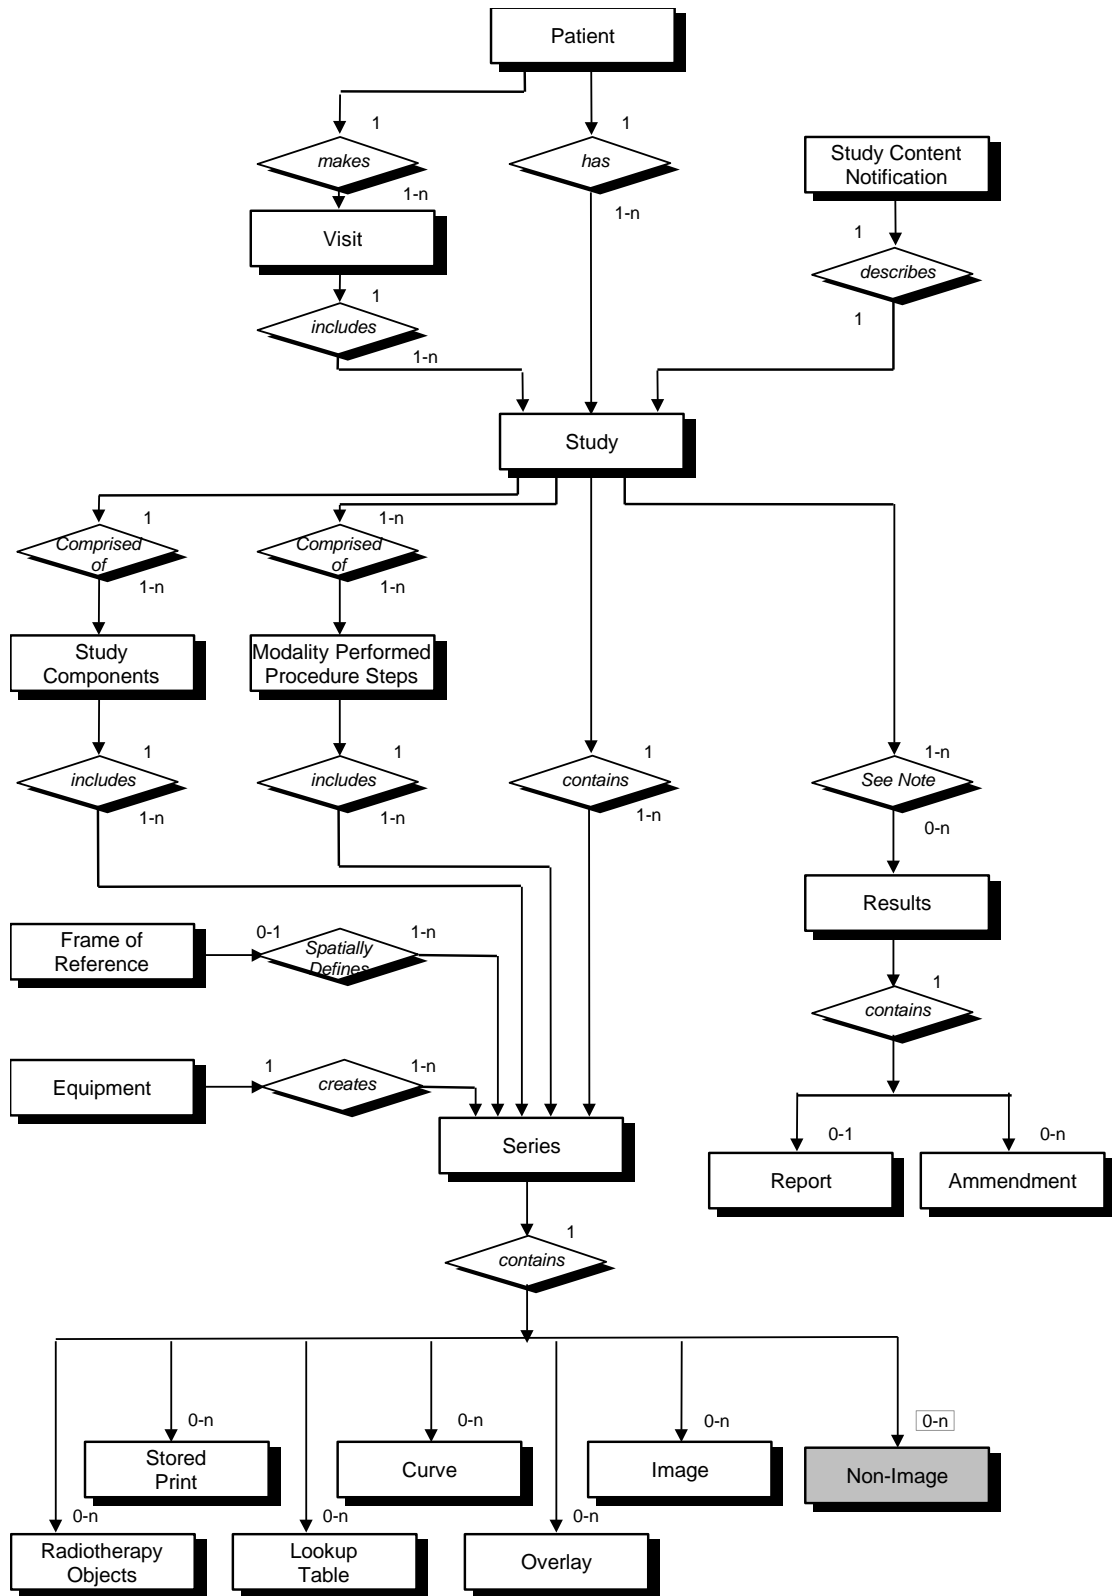


Figure 9 DICOM Information Model

A.3.2 SIEMENS Non-Image IOD - Module Table

IE	Module	Reference	Usage
Patient	Patient	[1] PS3.3 C.7.1.1	M
Study	General Study	[1] PS3.3 C.7.2.1	M
	Patient Study	[1] PS3.3 C.7.2.2	U
Series	General Series	[1] PS3.3 C.7.3.1	M
Equipment	General Equipment	[1] PS3.3 C.7.5.1	U
CSA	CSA Image Header	A.2.1	U
	CSA Series Header	A.2.2	U
	MEDCOM Header	A.2.3	U
	CSA Non-Image	A.1.3.1	M
	SOP Common	[1] PS3.3 C.12.1	M

Table 50 CSA Non-Image IOD Modules

A.3.3 SIEMENS Non-Image IOD - Modules

A.3.3.1 CSA Non-Image Attributes

The table in this section contains private IOD Attributes that describe CSA Non-Images.

Attribute Name	Tag	Owner	Type	Notes
Image Type	(0008,0008)	-	3	Image identification characteristics.
Acquisition Date	(0008,0022)	-	3	The date the acquisition of data that resulted in this data set started.
Acquisition Time	(0008,0032)	-	3	The time the acquisition of data that resulted in this data set started.
Conversion Type	(0008,0064)	-	3	Describes the kind of image conversion. Defined Terms: DV = Digitized Video, DI = Digital Interface, DF = Digitized Film, WSD = Workstation.
Referenced Image Sequence	(0008,1140)	-	3	A sequence which provides reference to a set of Image SOP Class/Instance identifying other images significantly related to this data set. Encoded as sequence of items: (0008,1150) and (0008,1155).
Derivation Description	(0008,2111)	-	3	A text description of how this data set was derived.
Source Image Sequence	(0008,2112)	-	3	A Sequence which identifies the set of Image SOP Class/Instance pairs of the Images which were used to derive this data set. Zero or more Items may be included in this Sequence. Encoded as sequence of items: (0008,1150) and (0008,1155).
Patient Position	(0018,5100)	-	3	Patient position descriptor relative to the equipment.

Acquisition Number	(0020,0012)	-	3	A number identifying the single continuous gathering of data over a period of time which resulted in this data set.
Image Number	(0020,0013)	-	3	A number that identifies this data set.
Frame of Reference UID	(0020,0052)	-	3	Uniquely identifies the frame of reference for a Series.
Image Comments	(0020,4000)	-	3	User-defined comments about the image.
Quality Control Image	(0028,0300)	-	3	Indicates whether or not this image is a quality control or phantom image. If this Attribute is absent, then the image may or may not be a quality control or phantom image. Enumerated Values: YES, NO.
Burned in Annotation	(0028,0301)	-	3	Indicates whether or not image contains sufficient burned in annotation to identify the patient and date the image was acquired. If this Attribute is absent, then the image may or may not contain burned in annotation. Enumerated Values: YES, NO.
Lossy Image Compression	(0028,2110)	-	3	Specifies whether an Image has undergone lossy compression. Enumerated Values: 00 = Image has NOT been subjected to lossy compression, 01 = Image has been subjected to lossy compression.
Lossy Image Compression Ratio	(0028,2112)	-	3	Describes the approximate lossy compression ratio(s) that have been applied to this image. May be multi valued if successive lossy compression steps have been applied.
CSA Data Type	(0029,xx08)	SIEMENS CSA NON-IMAGE	1	CSA Data identification characteristics. Defined Terms: BSR REPORT = Study Report Data 3D EDITOR 3D FLY PATH = Fly Through Data 3D FLY VRT = Fly Through Data 3D FUSION MATRIX = Fusion Data RAW DATA NUM 4 = NUMARIS/ Raw Data RAW DATA SOM 5 = SOMARIS/ Raw Data RT3D CONFIG = InSpaceIS Data SPEC NUM 4 = NUMARIS/4 Spectroscopy
CSA Data Version	(0029,xx09)	SIEMENS CSA NON-IMAGE	3	Version of CSA Data Info (0029,xx10) format and CSA Non-Image Data (7FE1,xx10) format.
CSA Data Info	(0029,xx10)	SIEMENS CSA NON-IMAGE	3	Information to describe the CSA Data (7FE1,xx10).

CSA Data	(7FE1,xx10)	SIEMENS CSA NON-IMAGE	2	Binary data as byte stream.
----------	-------------	--------------------------	---	-----------------------------

Table 51 CSA Non-Image Attributes

A.4 SIEMENS Standard Extended Modules

IE	Module	Reference	Usage	Note
Image	CSA Image Header	A.2.1	U	private GG information
	CSA Series Header	A.2.2	U	
	MEDCOM Header	A.2.3	U	private <i>syngo</i> [®] information
	MEDCOM OOG	A.2.4	U	if object graphics is attached to image
	Original Image Info	A.2.9	U	if derived image

Table 52 CSA Image IOD Modules

A.4.1 CSA Image Header Module

The table in this section contains private IOD Attributes that describe the CSA Image Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Image Header Type	(0029,xx08)	SIEMENS CSA HEADER	1	CSA Image Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4 SOM 5 = SOMARIS/5
CSA Image Header Version	(0029,xx09)	SIEMENS CSA HEADER	3	Version of CSA Image Header Info (0029,xx10) format.
CSA Image Header Info	(0029,xx10)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

A.4.2 CSA Series Header Module

The table in this section contains private IOD Attributes that describe the CSA Series Header:

Attribute Name	Tag	Owner	Type	Notes
CSA Series Header Type	(0029,xx18)	SIEMENS CSA HEADER	1	CSA Series Header identification characteristics. Defined Terms: NUM 4 = NUMARIS/4
CSA Series Header Version	(0029,xx19)	SIEMENS CSA HEADER	3	Version of CSA Series Header Info (0029,xx20) format.
CSA Series Header Info	(0029,xx20)	SIEMENS CSA HEADER	3	Manufacturer model dependent information.

A.4.3 MEDCOM Header Module

The table in this section contains private IOD Attributes that describe MEDCOM Header:

Attribute Name	Tag	Owner	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MEDCOM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 (Required if MedCom Header Info (0029,xx10) present.)
MedCom Header Version	(0029,xx09)	SIEMENS MEDCOM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. (Required if MEDCOM Header Info (0029,xx10) present.)
MedCom Header Info	(0029,xx10)	SIEMENS MEDCOM HEADER	3	Manufacturer model dependent information. The value of the attribute MedCom Header Info (0029,xx10) can be build up in each user defined format.
MedCom History Information	(0029,xx20)	SIEMENS MEDCOM HEADER	3	MedCom defined Patient Registration history information. See A.2.3.1.
Application Header Sequence	(0029,xx40)	SIEMENS MEDCOM HEADER	3	Sequence of Application Header items. Zero or more items are possible.
>Application Header Type	(0029,xx41)	SIEMENS MEDCOM HEADER	1C	Application Header identification characteristics. Required, if Sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MEDCOM HEADER	3	Identification of an application header
>Application Header Version	(0029,xx43)	SIEMENS MEDCOM HEADER	3	Version of CSA Series Header Info (0029,xx44) format.
>Application Header Info	(0029,xx44)	SIEMENS MEDCOM HEADER	3	Application dependent information.
Workflow Control Flags	(0029,xx50)	SIEMENS MEDCOM HEADER	3	Eight free definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS MEDCOM HEADER	3	Flag to control remote archive management system to keep the image always online (also when already archived). Enumerated Values: 00 = remote control not required 01 = keep image online
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS MEDCOM HEADER	3	Flag to control remote archive management system not to archive the related image. Enumerated Values: 00 = remote control not required 01 = don't archive image
Image Location Status	(0029,xx53)	SIEMENS MEDCOM HEADER	3	Image location status to control retrieving.

				<p>Defined Terms:</p> <p>ONLINE = retrieving has to be done as usual,</p> <p>NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54),</p> <p>OFFLINE = invoking a retrieve operation initiates an operator request,</p> <p>INVALID = invoking a retrieve operation would always result in an error.</p>
Estimated Retrieve Time	(0029,xx54)	SIEMENS MEDCOM HEADER	3	Estimated retrieve time in seconds. A value less than zero (< 0) indicates location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS MEDCOM HEADER	3	Data size of images in MByte.
SIEMENS Link Sequence	(0029,xx70)	SIEMENS MEDCOM HEADER	3	Sequence of link items. Each item identify the location of one missing tag. One or more items can be included in this sequence.
Referenced Tag	(0029,xx71)	SIEMENS MEDCOM HEADER	1	The referenced tag. The value of this tag is in the Child Data Object (CDO). Currently it is always Pixel Data (7FE0,0010).
Referenced Tag Type	(0029,xx72)	SIEMENS MEDCOM HEADER	1	The Value Representation (type) of the missing tag (e.g. OW). Enumerated values are all DICOM defined Value Representations.
Referenced Value Length	(0029,xx73)	SIEMENS MEDCOM HEADER	1	The length of the referenced tag value in bytes.
Referenced Object Device Type	(0029,xx74)	SIEMENS MEDCOM HEADER	1	<p>The Device Type that stores the Child Data Object (CDO) with the referenced tag value. Currently it should be "SHMEM". In future, "SDM", "LOID" or "FILE" are also imaginable.</p> <p>Defined Terms are</p> <p>SHMEM = Shared Memory</p> <p>SDM = Series Data Management</p> <p>LOID = Database</p> <p>FILE</p>
Referenced Object Device Location	(0029,xx75)	SIEMENS MEDCOM HEADER	2	The Location of the device that stores the Child Data Object (CDO) with the referenced tag value. For the "SHMEM" case, it is the shared memory directory. Can be empty, then the default directory will be taken. In future, for "SDM" this will be the SDM_ID, for FILE it will be the directory name and for "LOID" it will be the database name.
Referenced Object ID	(0029,xx76)	SIEMENS MEDCOM HEADER	1	The ID of the object that contains the Child Data Object (CDO) with the referenced tag value. In case of "SHMEM" it is the shared memory ID. In future, for "SDM" this will be

				a Sirius OID, for "FILE" the file name, for "DB" the LOID.
Series Work Flow Status	(0029,xx60)	SIEMENS MEDCOM HEADER2	3	syngo® Patient Browser specific flags used for clinical work: <ul style="list-style-type: none"> • com = completed • rea = read • ver = verified

Table 53 MEDCOM Header Modules

A.4.3.1 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined in the following way:

Part	Name	Type	Bytes	Notes
header	Identifier	string	32	Always "CSA HISTORY"
	Version	string	32	e.g. "V1.10"
n Items	Class Name	string	64	
	Modification String	string	1024	

Table 54 MEDCOM History Information

A.4.4 MEDCOM OOG Module

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used whenever object graphics is drawn on the image and need to be stored as graphic object properties. Given the condition that the module contents was not removed by other modalities, the graphic objects remain re-animatable if such an image was transferred and is then retrieved back

Attribute Name	Tag	Owner	Type	Notes
MedCom OOG Type	(0029,xx08)	SIEMENS MEDCOM OOG	1	MEDCOM Object Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1 MEDCOM OOG 2
MedCom OOG Version	(0029,xx09)	SIEMENS MEDCOM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format.
MedCom OOG Info	(0029,xx10)	SIEMENS MEDCOM OOG	3	MEDCOM Object Oriented Graphics (OOG) data.

Table 55 MEDCOM OOG Module

The graphics objects are also fully drawn in the Image Overlay Plane for compatibility with other products, which do not support the MedCom OOG module. Any system not supporting the MedCom OOG module shall remove the OOG module and its content when modifying the image overlay plane content.

A.5 Private Non-Image IOD

The Sensis system will create numerical data that cannot be correlated to an individual image or waveform instance and therefore need to be stored in separate instance(s). This is necessary to correlate the information in the right level of the DICOM data model hierarchy. Since there is no fitting DICOM SOP Class definition, Siemens Healthineers has created a private "Non-Image IOD" to contain numerical data heaps to be managed within a DICOM structure. Please see previous chapters of the Appendix for IOD definition and the following tables for detailed encoding of the different "Non-Image SOP Class Instances".

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	from Configuration
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1
SOP Instance UID	(0008,0018)	N/A
Study Date	(0008,0020)	<yyyymmdd>
Series Date	(0008,0021)	<yyyymmdd>
Study Time	(0008,0030)	<hhmmss>
Series Time	(0008,0031)	<hhmmss>
Accession Number	(0008,0050)	RIS or "Accession Number" input
Modality	(0008,0060)	EPS
Manufacturer	(0008,0070)	Siemens Healthineers
Institution Name	(0008,0080)	N/A
Performing Physician's Name	(0008,1050)	"Performing Physician 1" \ "Performing Physician 2" input
Admitting Diagnosis Description	(0018,1080)	RIS or "Admitting Diagnoses" input
Manufacturer's Model Name	(0008,1090)	Sensis Vibe
Patient's Name	(0010,0010)	RIS or "Patient Name" input
Patient ID	(0010,0020)	RIS or "Patient ID" input
Patient's Birth Date	(0010,0030)	RIS or checked input
Patient's Sex	(0010,0040)	RIS or input (M or F or O/unknown)
Patient's Age	(0010,1010)	calculated from "DoB" input
Patient's Size	(0010,1020)	(in meters)
Patient's Weight	(0010,1030)	(in kilograms)
Patient's Address	(0010,1040)	"Address" input"
Patient Comments	(0010,4000)	"Additional Info" input"
Study Instance UID	(0020,000D)	from RIS or system generated
Series Instance UID	(0020,000E)	N/A
Study ID	(0020,0010)	N/A
Series Number	(0020,0011)	N/A
Private Creator	(0029,00xx)	SIEMENS CSA NON-IMAGE
Data Type	(0029,xx08)	WF_PRES_DATA
Data Version	(0029,xx09)	1.0
Requested Procedure Description	(0032,1060)	from RIS
Study Comments	(0032,4000)	"Exam Comment" input
Private Creator	(7FE1,00xx)	SIEMENS CSA NON-IMAGE
Data	(7FE1,xx10)	binary data

Table 56 Overview of supplied attributes – Non-Image (WF PRES DATA)

Attribute Name	Tag	Value
Specific Character Set	(0008,0005)	from Configuration
SOP Class UID	(0008,0016)	1.3.12.2.1107.5.9.1
SOP Instance UID	(0008,0018)	N/A
Study Date	(0008,0020)	<yyyymmdd>
Series Date	(0008,0021)	<yyyymmdd>

Attribute Name	Tag	Value
Study Time	(0008,0030)	<hhmmss>
Series Time	(0008,0031)	<hhmmss>
Accession Number	(0008,0050)	RIS or "Accession Number" input
Modality	(0008,0060)	EPS
Manufacturer	(0008,0070)	Siemens Healthineers
Institution Name	(0008,0080)	N/A
Performing Physician´s Name	(0008,1050)	"Performing Physician 1" \ "Performing Physician 2" input
Admitting Diagnosis Description	(0018,1080)	RIS or "Admitting Diagnoses" input
Manufacturer´s Model Name	(0008,1090)	Sensis Vibe
Patient´s Name	(0010,0010)	RIS or "Patient Name" input
Patient ID	(0010,0020)	RIS or "Patient ID" input
Patient´s Birth Date	(0010,0030)	RIS or checked input
Patient´s Sex	(0010,0040)	RIS or input (M or F or O/unknown)
Patient´s Age	(0010,1010)	calculated from "DoB" input
Patient´s Size	(0010,1020)	(in meters)
Patient´s Weight	(0010,1030)	(in kilograms)
Patient´s Address	(0010,1040)	"Address" input
Patient Comments	(0010,4000)	"Additional Info" input
Device Serial Number	(0018,1000)	From Service UI
Software Version	(0018,1020)	SIEMENS Sensis Software Version (VC03A, VC10, VC11, VC12, VD11 etc.)
Study Instance UID	(0020,000D)	from RIS or system generated
Series Instance UID	(0020,000E)	N/A
Study ID	(0020,0010)	N/A
Series Number	(0020,0011)	N/A
Private Creator	(0029,00xx)	SIEMENS CSA NON-IMAGE
Data Type	(0029,xx08)	EVENT_LOG_DATA or BINARY_DATA
Data Version	(0029,xx09)	5.0
Requested Procedure Description	(0032,1060)	from RIS
Study Comments	(0032,4000)	"Exam Comment" input
Private Creator	(7FE1,00xx)	SIEMENS CSA NON-IMAGE
Data	(7FE1,xx10)	binary data

Table 57 Overview of supplied attributes – Non-Image (EVENT LOG DATA, BINARY DATA)

Annex B: Index of Tables

Table 1 Network Services	3
Table 2 Media Services.....	3
Table 3 Implementation Identifying Information.....	3
Table 4 List of products applicable to this Conformance Statement.....	7
Table 5 Proposed Presentation Contexts.....	12
Table 6 Supported SOP Classes as an SCU	14
Table 7 Supported private SOP Classes as an SCU.....	14
Table 8 Supported SOP Classes as an SCP	14
Table 9 Supported private SOP Classes as an SCP.....	14
Table 10 Proposed Presentation Context – Send Images.....	16
Table 11 Proposed Presentation Context – Receiving Images	19
Table 12 Storage Commitment SOP Class supported	22
Table 13 Proposed Presentation contents – request Storage Commitment.....	23
Table 14 Accepted Presentation contents – request Storage Commitment	24
Table 15 Supported SOP Classes as SCU	27
Table 16 Supported SOP Classes as SCP	27
Table 17 Proposed Presentation Contexts - Find SCU	29
Table 18 Search keys for Query models - Find SCU.....	31
Table 19 C-FIND response status	31
Table 20 Proposed Presentation Contexts - Move SCU “Import”	32
Table 21 Status Codes - Move SCU “Import”.....	33
Table 22 Accepted Presentation Contexts - Find SCP.....	34
Table 23 Supported Query attributes sorted by Query Level – Patient Root Information Model	36
Table 24 Supported Query attributes sorted by Query Level – Study Root Information Model	37
Table 25 Supported Query attributes sorted by Query Level – Patient/Study only Information Model	38
Table 26 Status Codes.....	38
Table 27 Accepted Presentation Contexts - Get SCP	39
Table 28 Status Codes.....	40
Table 29 Accepted Presentation Contexts - Move SCP	40
Table 30 Status Codes.....	41
Table 31 SOP Classes as a SCU.....	43
Table 32 Proposed Presentation Contexts.....	44
Table 33 Supported Broad Worklist Query Search Key Attributes	45
Table 34 Basic Worklist C-FIND-RSP Return Key Attributes	50
Table 35 Patient based "narrow query" Search Key Attributes	50
Table 36 C-FIND-RSP Status	51
Table 37 SOP Classes as an SCU.....	53
Table 38 Proposed Presentation Contexts – MPPS.....	54
Table 39 Performed Procedure Step N-CREATE Attributes	56
Table 40 MPPS N-CREATE Response Status.....	57
Table 41 Performed Procedure Step N-SET Attributes	58
Table 42 MPPS N-SET Response Status	58
Table 43 Application profiles, Activities, and Roles for DICOM Archive	66
Table 44 STD-GEN-CD Supported SOP Classes for FSR Role	67
Table 45 Extension, Specialization for SIEMENS Non-Image Objects.....	69
Table 46 WF IOD description for instances created by Sensis	72

© Siemens Healthcare GmbH. 2022. All rights reserved.

Table 47 Encapsulated PDF IOD description for instances created by Sensis	74
Table 48 Sensis PDF report types	74
Table 49 SIEMENS Private Non-Image IOD	74
Table 50 CSA Non-Image IOD Modules	76
Table 51 CSA Non-Image Attributes	78
Table 52 CSA Image IOD Modules	78
Table 53 MEDCOM Header Modules.....	81
Table 54 MEDCOM History Information	81
Table 55 MEDCOM OOG Module	81
Table 56 Overview of supplied attributes – Non-Image (WF PRES DATA).....	82
Table 57 Overview of supplied attributes – Non-Image (EVENT LOG DATA, BINARY DATA).....	83

A.6 Table of Figures

Figure 1 Application Data Flow Diagram - Verification SCU/SCP	10
Figure 2 Application Data Flow Diagram - Storage SCU/SCP	13
Figure 3 Application Data Flow Diagram - Storage Commitment SCU.....	21
Figure 4 Application Data Flow Diagram - Query/Retrieve SCU	25
Figure 5 Application Data Flow Diagram - Query/Retrieve SCP	25
Figure 6 Application Flow Diagram – Basic Worklist SCU.....	42
Figure 7 Application Flow Diagram – MPPS SCU.....	52
Figure 8 Application Data Flow Diagram	65
Figure 9 DICOM Information Model.....	75

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens Healthineers sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice.

Some/All of the features and products described herein may not be available in the United States or other countries.

The information in this document contains general technical descriptions of specifications and options as well as standard and optional features that do not always have to be present in individual cases.

Siemens Healthineers reserves the right to modify the design, packaging, specifications, and options described herein without prior notice. Please contact your local Siemens Healthineers sales representative for the most current information.

In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we recycle certain components. Using the same extensive quality assurance measures as for factory-new components, we guarantee the quality of these recycled components.

Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Caution: Federal law restricts this device to sale by or on the order of a physician.

VD15

Siemens Healthineers Headquarters

Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen, Germany
Phone: +49 9131 84-0
siemens-healthineers.com

Published by Siemens Healthcare GmbH · Doc-Ident. 6656990-ESK-200-04 · ©Siemens Healthcare GmbH, 2022