

DICOM Conformance Statement

syngo X Workplace
with *syngo* Application Software
VD3

siemens-healthineers.com

1 Conformance Statement Overview

The syngo X Workplace is a “syngo®-based¹” Multipurpose Workstation for Viewing of Images from various digital imaging procedures. The syngo X Workplace is designed to be integrated into an environment of medical, DICOM-based devices. The syngo X Workplace supports Storage and Transfer of images utilizing the DICOM “Storage Service Class”, the display of data and retrieval of images from DICOM Archives utilizing the DICOM “Query/Retrieve Service Class”. Furthermore, the Import from and export to DICOM CD/DVD media is supported. Printing of viewing results is provided with Print Management Services.

Table 1 - Network Services

SOP Classes	SOP Class UID	User of Service (SCU)	Provider of Service (SCP)
Verification			
Verification	1.2.840.10008.1.1	Yes	Yes
Transfer (Image SOP Class)			
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Enhanced CT Image Storage	1.2.840.10008.5.1.4.1.1.2.1	Yes	Yes
Digital X-Ray Image Storage - for Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	Yes
Digital X-Ray Image Storage - for Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	Yes
Enhanced MR Image Storage	1.2.840.10008.5.1.4.1.1.4.1	Yes	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	Yes
Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.4	Yes	Yes (Note 1)
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	Yes
Ultrasound Multi-Frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	Yes
X-Ray 3D Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.13.1.1	Yes	Yes
Transfer (Non-image SOP Class)			
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	Yes
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Yes	Yes
Enhanced SR Storage	1.2.840.10008.5.1.4.1.1.88.22	Yes	Yes
Comprehensive SR Storage	1.2.840.10008.5.1.4.1.1.88.33	Yes	Yes
X-Ray Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.67	Yes	Yes
Transfer (Private SOP Class)			
Syngo Non-Image Storage	1.3.12.2.1107.5.9.1	Yes	Yes
Workflow Management			
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	Yes
Query/Retrieve			
Patient Root Q/R Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	Yes
Patient Root Q/R - Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	Yes
Study Root Q/R - Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	Yes
Study Root Q/R - Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	Yes
Patient/Study Only Q/R - Information Model FIND	1.2.840.10008.5.1.4.1.2.2.3	Yes	Yes
Patient/Study Only Q/R - Information Model MOVE	1.2.840.10008.5.1.4.1.2.3.2	Yes	Yes

¹ syngo is a registered trademark of Siemens Healthcare GmbH
 © Siemens Healthcare GmbH. 2020. All rights reserved.

Print Management			
Basic Grayscale Print Management Meta	1.2.840.10008.5.1.1.9	Yes	No
Basic Color Print Management Meta	1.2.840.10008.5.1.1.1	Yes	No
Print Job	1.2.840.10008.5.1.1.14	Yes	No
Presentation LUT	1.2.840.10008.5.1.1.23	Yes (for Grayscale)	No

Note 1: current restriction: only self-created objects.

Table 2 - Media Services

Media Storage Application Profile	Write Files (FSC or FSU)	Read Files (FSR)
Compact Disk - Recordable		
General Purpose on CD-R	Yes	Yes
Basic Cardiac X-Ray on CD-R	Yes	Yes
1024 X-Ray on CD-R	Yes	Yes
DVD		
1024 X-Ray on DVD	Yes	Yes
General Purpose DVD with JPEG	Yes	Yes
BD		
General Purpose on BD	Yes	Yes

Table 3 - Implementation Identifying Information

Name	Value
Application Context Name	1.2.840.100008.3.1.1.1
Implementation Class UID	1.3.12.2.1107.5.4.7
Implementation Version Name	"SIEMENSXLEOVD3"

2	Table of Contents	
1	Conformance Statement Overview	2
2	Table of Contents	4
3	Introduction	6
3.1	Revision History	6
3.2	Audience	6
3.3	Remarks	6
3.4	Definitions, Terms and Abbreviations	6
3.5	References	7
4	Networking	8
4.1	Implementation Model	8
4.1.1	Application Data Flow	8
4.1.2	Functional Definitions of Application Entities	11
4.1.3	Sequencing of Activities	12
4.2	Application Entity Specification	12
4.2.1	Verification SCU AE Specification	12
4.2.2	Storage SCU AE Specification	14
4.2.3	Storage SCP AE Specification	16
4.2.4	Query/Retrieve SCU Specification	23
4.2.5	Query/Retrieve SCP Specification	28
4.2.6	Print SCU Specification	34
4.3	Network Interfaces	41
4.3.1	Physical Network Interface	41
4.3.2	Additional Protocols	42
4.4	Configuration	42
4.4.1	AE Title/Presentation Address Mapping	42
4.4.2	Parameters	43
5	Media Interchange	45
5.1	Implementation Model	45
5.1.1	Application Data Flow Diagram	45
5.1.2	Functional Definitions of AEs	46
5.1.3	Sequencing of Real-World Activities	46
5.1.4	File Meta Information for Implementation Class and Version	46
5.2	AE Specifications	47
5.2.1	Media Storage AE – Specification	47
5.3	Augmented and Private Application Profiles	48
5.4	Media Configuration	48
5.4.1	Single- / Multi-Session CD burning	48
5.4.2	“Viewer on CD”	48
5.4.3	Auto-Labeling	48

6	<i>Support of Extended Character Sets</i>	49
7	<i>Security</i>	50
7.1	Security Profile	50
7.1.1	Security Transport Connection Profiles	51
7.2	Application Level Confidentiality Profile	53
7.2.1	Anonymization workflow (De-identifier).....	53
8	<i>Annexes</i>	55
8.1	IOD Contents	55
8.1.1	Created SOP Instances.....	55
8.1.2	Usage of attributes from received IODs	88
8.1.3	Attribute mapping	88
8.1.4	Coerced/Modified fields.....	88
8.2	Data Dictionary of private Attributes	88
8.3	Coded Terminology and Templates	92
8.3.1	Context Groups.....	92
8.3.2	Template Specifications.....	94
8.3.3	Private Code Definitions	101
8.4	Grayscale Image Consistency	101
8.5	Standard Extended/Specialized/Private SOP Classes	101
8.5.1	Standard Extended XA.....	101
8.5.2	Standard Extended Segmentation.....	105
8.5.3	Standard Extended Surface Segmentation.....	105
8.5.4	Standard Extended for other created SOP Class.....	109
8.6	Private Transfer Syntaxes	111
8.7	DICOM Print SCU – detailed status displays	111
8.7.1	Common Status Information.....	111
8.7.2	Additional DICOM Execution Status Information	116
8.7.3	Unknown DICOM Execution Status Information	116
Annex A:	<i>Index of Tables</i>	118

3 Introduction

3.1 Revision History

Table 4 - Revision History

Product	Product Version	Document Version	Date
syngo X Workplace	VD30	11275126-ESK-001-00	11/2020

3.2 Audience

This document is intended for hospital staff, health system integrators, software designers or implementers. It is assumed that the reader has a working understanding of DICOM.

3.3 Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between syngo X Workplace and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard [1]. DICOM by itself does not guarantee interoperability.

The Conformance Statement does, however, facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement is not supposed to replace validation with other DICOM equipment to ensure proper exchange of intended information. In fact, the user should be aware of the following important issues:

- The comparison of conformance statements is the first step towards assessing interconnectivity and interoperability between syngo X Workplace and other DICOM conformant equipment.
- Test procedures should be defined and executed to validate the required level of interoperability with specific compatible DICOM equipment, as established by the healthcare facility.

Siemens reserves the right to modify the design and specifications contained herein without prior notice. Please contact your local Siemens representative for the most recent product information.

3.4 Definitions, Terms and Abbreviations

Definitions, terms and abbreviations used in this document are defined within the different parts of the DICOM standard.

Additional Abbreviations and terms are as follows:

AE	DICOM Application Entity
AET	Application Entity Title
ASCII	American Standard Code for Information Interchange
CSE	Customer Service Engineer
DCS	DICOM Conformance Statement
DICOM	Digital Imaging and Communications in Medicine
FSC	File Set Creator
FSR	File Set Reader
FSU	File Set Updater
GSDF	Grayscale Standard Display Function
IOD	DICOM Information Object Definition

ISO	International Standard Organization
MOD	Magneto-optical Disk
n.a.	not applicable
NEMA	National Electrical Manufacturers Association
O	Optional Key Attribute
PDU	DICOM Protocol Data Unit
R	Required Key Attribute
SCU	DICOM Service Class User (DICOM client)
SCP	DICOM Service Class Provider (DICOM Server)
SOP	DICOM Service-Object Pair
SPS	Scheduled Procedure Step
SR	Structured Report
TFT	Thin Film Transistor (Display)
TID	Template ID
U	Unique Key Attribute
UID	Unique Identifier
UTF-8	Unicode Transformation Format-8
VR	Value Representation
syngo X Workplace	Workstation for Angiographic/Radiographic viewing & processing

3.5 References

[NEMA PS3] Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>²

² The DICOM Standard is under continuous maintenance, the current official version is available at <http://dicom.nema.org>
 © Siemens Healthcare GmbH. 2020. All rights reserved.

4 Networking

4.1 Implementation Model

syngo X Workplace supports storing DICOM images to remote nodes like workstations or Archiving Systems. Using the Storage Commitment Service, it can request safe keeping of previously stored instances from an Archiving system. Additionally, the syngo X Workplace can query remote notes, retrieve and store selected instances from that node. Using the Modality Worklist service, the syngo X Workplace can query a HIS/RIS for scheduled procedures. Performed procedure status and other procedure data can be returned to the HIS/RIS using the Modality Performed Procedure Step (MPPS) Service. Furthermore, printing of grayscale images is supported.

4.1.1 Application Data Flow

The following figures provide a functional overview of the syngo X Workplace Application Entities (AE). Relationships are shown between user-invoked activities (in the circles at the left of the AEs) and the associated real-world activities provided by DICOM service providers (in the circles at the right of the AEs)

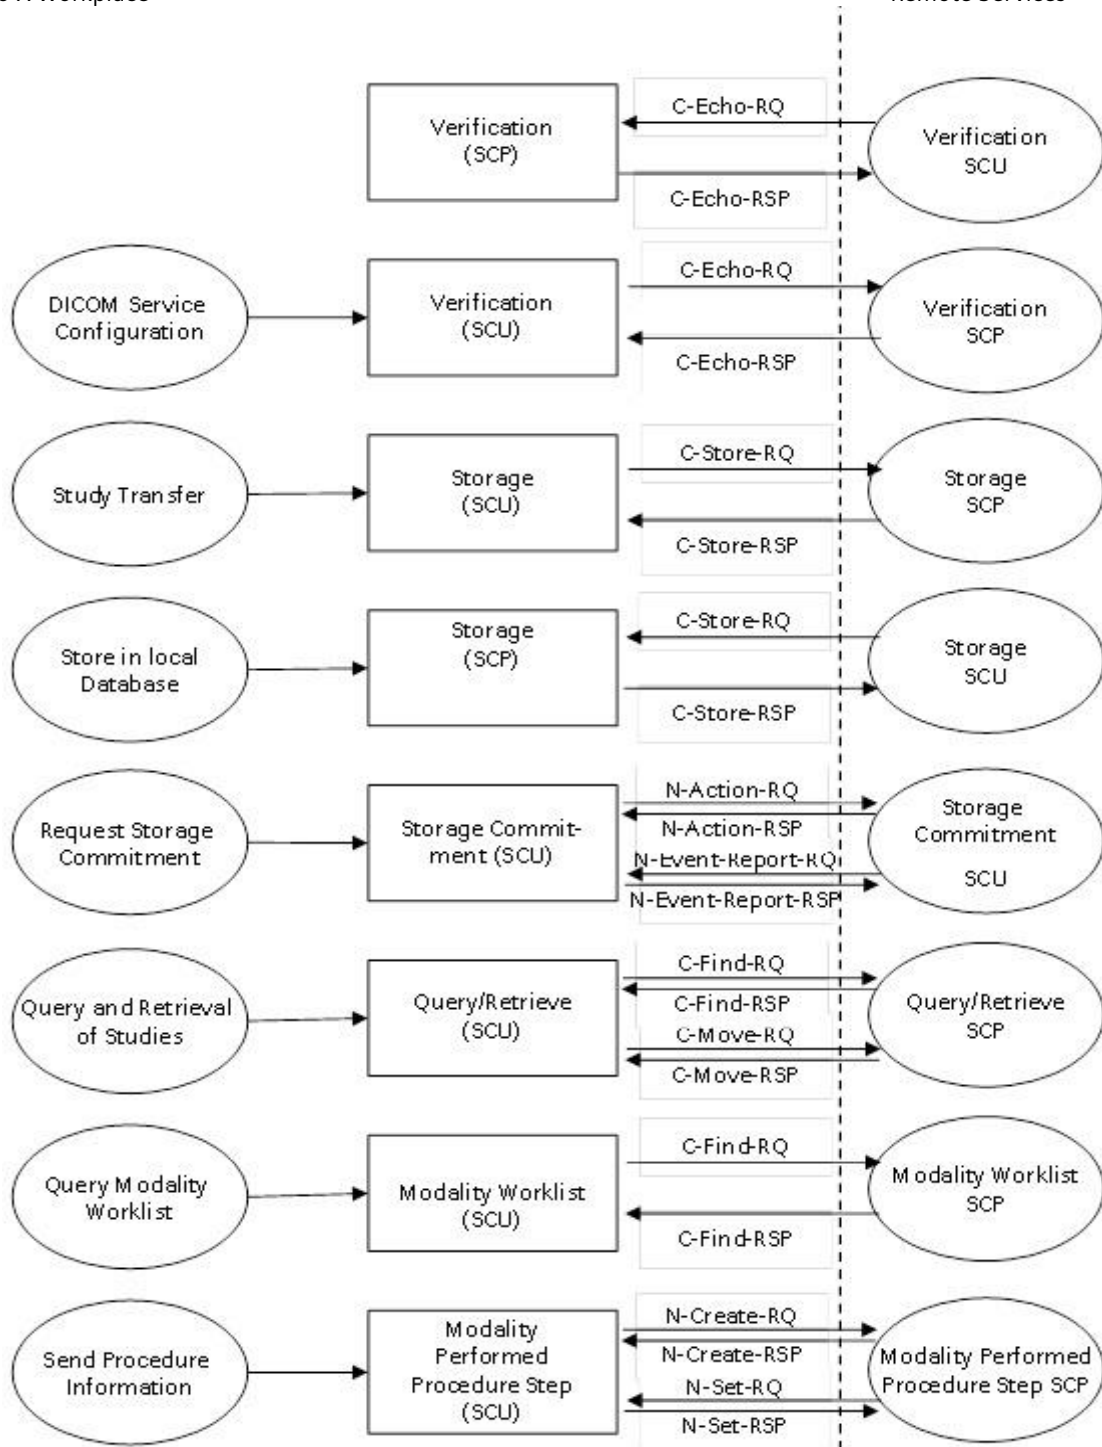


Figure 1: syngo X Workplace DICOM Data Flow diagram – Acquisition Workflow

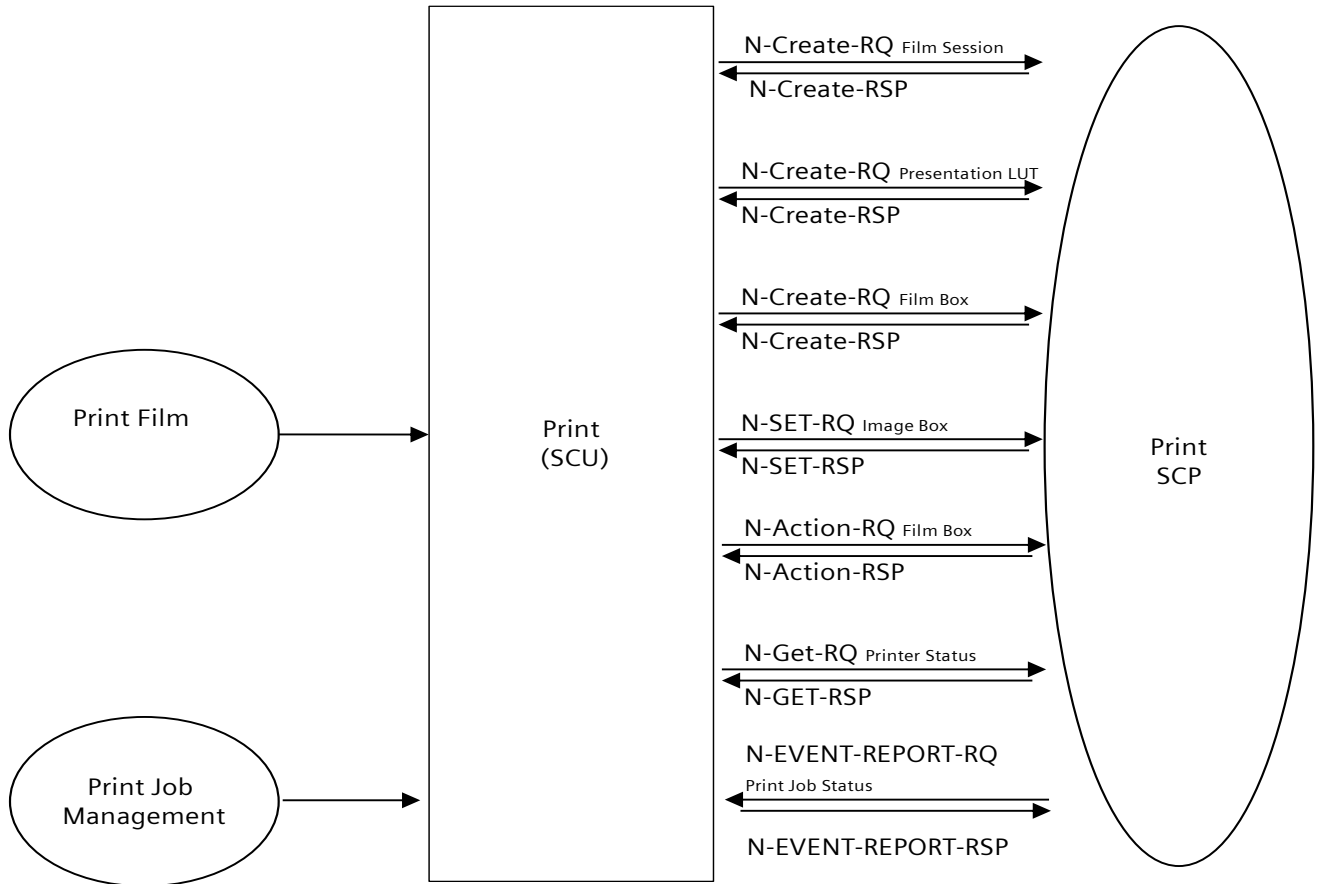


Figure 2: syngo X Workplace DICOM Data Flow diagram - Printing

4.1.2 Functional Definitions of Application Entities

4.1.2.1 Functional Definition of Verification-SCU AE

The syngo X Workplace DICOM Service Tool application opens an association when a "verification" of a remote application is requested during a configuration session. This can be done when entering new data for remote application configuration or to verify existing configuration data.

4.1.2.2 Functional Definition of Storage-SCU AE

The syngo X Workplace Storage SCU is invoked by the job control interface that is responsible for processing network archival tasks. The job consists of data describing the composite image objects selected for storage and the destination. An association is negotiated with the destination application entity and the image data is transferred using the C-STORE DIMSE-Service. Status of the transfer is reported to the job control interface.

With each successfully completed send job, the syngo X Workplace DICOM Application will populate the Storage Commitment Push Model Action Information from the SOP Instances sent. Then a Storage Commit Request is triggered, if configured. Depending on configuration, the syngo X Workplace DICOM application will keep the association open for responses with a configurable time-out, or closes the association and expects responses on a different association that has to be established by the remote Storage Commitment SCP.

The commitment status derived from the related trigger response will be indicated in the related Status Flags of the related entity. It is possible to create triggers ("auto rules") from this event.

The Transaction UIDs of the pending commitment request are kept "open" (Job-status is "waiting") for a configurable time (default: 1h). If the "open time" for a pending commitment request has elapsed w/o a related response from the provider, the Transaction UID is removed and the related entities are indicated as "commit failed".

Open Transaction UIDs of pending commitment requests are discarded after a reboot of the system. The related entities are indicated as "commit failed".

4.1.2.3 Functional Definition of Storage-SCP AE

The Storage SCP component of the syngo X Workplace DICOM application is operating as background server process. The process starts when the machine is powered on and waits for Storage association requests. Upon accepting an association with a negotiated Presentation Context, it starts to receive the Composite Image Objects and imports them to local database.

The Verification SCP is included in the Storage SCP.

The Storage Commitment SCP is running in background and is ready to receive requests when the system is started. Storage Commitment will be checked and returned against the SOP Classes received and kept in the local Storage of the syngo X Workplace. The response will either be sent "on same" (association not closed by requester) or "on separate" association (requester closed association consecutive to positive request status).

4.1.2.4 Functional Definition of Query/Retrieve-SCU AE

The syngo X Workplace DICOM Query/Retrieve SCU requests the remote Query/Retrieve SCP to perform a search and match to the keys specified in the request in order to display the results in the system's user interface. Depending on user action (Import) the syngo X Workplace Query/Retrieve DICOM SCU sends a C-MOVE DIMSE service to initiate a C-STORE sub-operation on the SCP to start an image transfer from remote Storage SCU (running on Query/Retrieve SCP) to the system's Storage SCP.

4.1.2.5 Functional Definition of Query/Retrieve-SCP AE

The syngo X Workplace DICOM Query/Retrieve SCP responds to C-FIND DIMSE services from remote SCU applications. Depending on further remote request, a C-GET or a C-MOVE involves the system's DICOM Query/Retrieve SCP application to initiate a C-STORE association (by triggering and parameterizing the own Storage SCU) to send image objects to a remote Storage SCP.

All components of the DICOM Query/Retrieve SCP application are operating as background server processes. The processes start when the machine is powered on and then respond to queries based on the records stored in its database.

4.1.2.6 Functional Definition of Print SCU AE

The Print SCU is invoked by the user interface to setup film-sheet layout and whenever an image is ready to be printed on film. The Print SCU will hold and maintain all data needed to compile a complete film-sheet from the data (images, layout, configuration) received. Whenever a film-sheet is ready to print the related data is used to supply the Information to the SOP Classes of the Print Management Service Class. A queue is maintained, in order to intermediately store several film-sheets in case of resource problems on printer. The SCU will only supply and require the mandatory SOP Classes of the Print Management Service Class.

4.1.3 Sequencing of Activities

4.1.3.1 Verification

Newly entered data have to be saved first, before a "verification" of these data is possible.

4.1.3.2 Storage

Prior to sending of SOP Instances the syngo X Workplace Storage application is capable of invoking processing and resizing features in order to prepare image pixel contents into convenient formats for certain multi-vendor environments.

The Storage Commitment trigger is automatically derived from the successful completion of a Send Job.

4.1.3.3 Query/Retrieve

Retrieve of images is only possible if a result from a previous "Search..." operation exists, and those entities can be selected for "Import".

The Query application will not "per se" request information on IMAGE level. The user can select a series and request image level information with the "Image List" function.

4.2 Application Entity Specification

4.2.1 Verification SCU AE Specification

4.2.1.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" section "Verification" in the "Conformance Statement Overview".

4.2.1.2 Association Policies

4.2.1.2.1 General

The syngo X Workplace DICOM Service Tool application attempts to open an association for verification request whenever the "verification" function is activated during network configuration of a remote DICOM application.

4.2.1.2.2 Number of Associations

The syngo X Workplace DICOM Service Tool application initiates one association at a time to request verification.

4.2.1.2.3 Asynchronous Nature

The syngo X Workplace DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.1.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information" in the "Conformance Statement Overview".

4.2.1.3 Association Initiation Policy

4.2.1.3.1 Activity – "Verification"

4.2.1.3.1.1 Description and Sequencing of Activity

The Verification SCU C-ECHO request is initiated by Service and Configuration SW whenever "Verification" is requested. If an association to a remote Application Entity is successfully established, Verification with the configured AET is requested via the open association. If the C-ECHO Response from the remote Application contains a status other than "Success" this will be indicated in the service environment and the association is closed.

4.2.1.3.1.2 Proposed Presentation Contexts

The syngo X Workplace DICOM application will propose Presentation Contexts as shown in the following table:

Table 5 - Presentation Context Table "Verification"

Presentation Context Table – "Verification"					
Abstract Syntax		Transfer Syntax		Role	Extended Negotiation
Name	UID	Name List	UID List		
Verification	1.2.840.10008.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None

4.2.1.3.1.3 SOP Specific Conformance – Verification SCU

The Application conforms to the definition of the Verification SCU in accordance to the DICOM Standard.

4.2.1.4 Association Acceptance Policy

The Verification SCP is part of the Storage SCP.

4.2.2 Storage SCU AE Specification

4.2.2.1 SOP Classes

For SOP Classes supported, please refer to “Table 1 - Network Services”, sections “Transfer” and “Workflow Management”.

4.2.2.2 Association Policies

4.2.2.2.1 General

The DICOM Storage application will be triggered by the transfer job queue or by an external retrieve request. An association request is sent to the destination AE and, upon successful negotiation of a Presentation Context, the transfer is started. Depending on configuration, processing or down-sizing can be applied to the images prior to being sent.

With a Send Job successfully completed, the DICOM application will generate the Storage Commitment Action Information which references to all Instances of the processed job. The Commit Request is sent over a single opened association. The syngo X Workplace will wait for Status responses of the Storage Commitment Request. If the Provider accepts the Storage Commitment with Success Status, the generated Transaction UID, together with study identification data and a timestamp, is kept. Depending on configuration, the association is closed or kept open for a configured time range. If the association is closed immediately, the response is expected on a different association which is the default setting. Multiple Storage Commitment Requests can be pending.

The default PDU size used will be 528378 bytes.

4.2.2.2.2 Number of Associations

The syngo X Workplace DICOM application initiates several associations at a time, one for each destination to which a transfer request is being processed in the active job queue list.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in “Configuration / DICOM / General”.

4.2.2.2.3 Asynchronous Nature

The syngo X Workplace DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.2.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to “Table 3 - Implementation Identifying Information” in the “Conformance Statement Overview”.

4.2.2.3 Association Initiation Policy

If a job with network destination gets active in the job list or a retrieve sub-operation is processed, the syngo X Workplace DICOM application attempts to initiate a new association for

- DIMSE C-STORE to send images and with successful status and
- N-ACTION DIMSE for the Storage Commitment Push Model Service Class to request commitment.

4.2.2.3.1 Activity – “Send to ...”

4.2.2.3.1.1 Description and Sequencing of Activity

The C-STORE request is triggered by a job with network destination or the processing of an external C-MOVE retrieve request. If the process successfully establishes an association to a remote Application Entity, it will transfer each image one after another via the open association. Processing features and resizing of the pixel matrix can be applied as part of

the transfer. If the C-STORE Response from the remote Application contains a status other than "Success" or "Warning", the association is aborted.

With success status for the previous transfer, the syngo X Workplace Storage application sends the commit request (N-ACTION-RQ) message and waits for acceptance of this request (N-ACTION-RSP). After receiving this, the transaction is marked as "waiting".

Depending on a configuration value, the association will then be closed or kept open. In the first case, there is another configurable timeout giving the number of hours (h) and minutes (m) (by default 1h:0m) to wait for the corresponding commit response (N-EVENT-REPORT). In the second case, this time is the (also configurable) time-out for the association being kept open. In both cases, if the commit response (N-EVENT-REPORT) does not arrive within the configured time-out, the transaction will be marked as failed. The syngo X Workplace does not re-send objects from a failed Storage Commitment result in any case.

If the commit response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as failed, else the transaction is marked as "completed". In both cases, a message is shown to the user.

4.2.2.3.1.2 Proposed Presentation Contexts

The syngo X Workplace DICOM application will propose Storage SCU Presentation Contexts as shown in the following table:

Table 6 - Presentation Context Table "Send to ..."

Presentation Context Table – "Send to ..."				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Any image SOP Class detailed in "Table 1 - Network Services" section "Transfer (Image SOP Class)".	JPEG Lossy Extended	1.2.840.10008.1.2.4.51	SCU	None
	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
	JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50		
	Explicit VR Little Endian	1.2.840.10008.1.2.1		
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
X-Ray 3D Angiographic Image Storage SOP Class "4D DSA"	JPEG-LS Lossless	1.2.840.10008.1.2.4.80	SCU	None
Any Non-image SOP Class detailed in "Table 1 - Network Services" section "Transfer (Non-image SOP Class)".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Private SOP Class as detailed in Chapter "Table 1 - Network Services" section "Transfer (Private SOP Class)".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Management SOP Class as detailed in "Table 1 - Network Services" section "Workflow Management".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCU	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.2.3.1.3 SOP specific Conformance - "Send to ..."

The syngo X Workplace can send images in different formats. In a destination specific service level configuration, it can be configured if images are sent original, resized (512x512 8 bit, 1024x1024 12 bit) and/or processed.

For association and DIMSE level time-outs, please refer to section Configuration (4.4.2 Parameters) of this document.

4.2.2.3.1.3.1 Optional Attributes

Please refer to the related Image Object definition tables in the Annex (section "Created SOP Instances") for a list of all DICOM IOD attributes of type 2 and 3, which are encoded by the syngo X Workplace applications.

4.2.2.3.1.3.2 Specialized Information Object Definitions

The DICOM images sent by syngo X Workplace DICOM application conform to the DICOM IOD definitions (Standard extended IODs). But they will contain additional private elements, which have to be discarded by a DICOM system when modifying the image.

The DICOM nodes are responsible for data consistency when modifying images. All unknown private attributes have to be removed upon modification!

4.2.2.3.1.3.3 *Data Dictionary of applied private IOD Attributes*

Please refer to "Standard Extended/Specialized/Private SOP Classes" in the Annex for a list of possible private IOD attributes.

4.2.2.3.1.4 SOP specific Conformance - Request Commitment

Storage Commitment is supported for all the SOP Classes detailed in Chapter "Table 1 - Network Services" section "Workflow Management".

The Referenced Study Component Sequence is not supported.

Storage Media File-Set ID and UID Attributes will not be supported in the commitment request (N-ACTION primitive) invoked by the Storage Commitment SCU.

4.2.2.4 Association Acceptance Policy

See next section "Storage SCP AE Specification".

4.2.3 Storage SCP AE Specification

4.2.3.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" Sections "Transfer" on page 1.

4.2.3.2 Association Policies

4.2.3.2.1 General

The syngo X Workplace DICOM application will accept any number of verification or storage SOP classes that are referred to above. There is no limit on the number of presentation contexts accepted except for the DICOM limit. In the event that the Siemens DICOM application runs out of resources, it will reject the association request.

syngo X Workplace will only accept Associations from known hosts with a known AET ("trusted hosts" concept). Hosts and AETs have to be entered in "Local Service" by a Siemens CSE.

The default PDU size used will be 528378 KB.

4.2.3.2.2 Number of Associations

The Siemens syngo X Workplace DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in "Configuration / DICOM / General".

4.2.3.2.3 Asynchronous Nature

The syngo X Workplace DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.3.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information" in the "Conformance Statement Overview".

4.2.3.3 Association Initiation Policy

If the result from a previously accepted Storage Commitment request is evaluated, the syngo X Workplace DICOM application attempts to initiate a new association for

- DIMSE N-EVENT-REPORT for sending commitment result from a previous request.

4.2.3.3.1 Activity - Return Commitment Result

When syngo X Workplace Storage SCP AE received a Storage Commitment request it tries to send the response back on the same association. When the association is not open anymore it will initiate an association to send the Storage Commitment response (N-EVENT-REPORT) to the SCU.

4.2.3.3.1.1 Proposed Presentation Context

The syngo X Workplace DICOM application will propose Storage SCP Presentation Contexts for returning Storage Commitment results as shown in the following table:

Table 7 - Presentation Context Table "Return Commitment Result"

Presentation Context Table – "Return Commitment Result"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Storage Commitment SOP Class as detailed in "Table 1 - Network Services" section "Workflow Management".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.3.3.1.2 SOP Specific Conformance

Storage Media File-Set ID and UID Attributes will not be supported in the N-EVENT-REPORT primitive invoked by the Storage SCP.

4.2.3.4 Association Acceptance Policy

The syngo X Workplace DICOM application attempts to accept a new association for

- DIMSE C-ECHO for incoming Verification requests
- DIMSE C-STORE for external image senders request storage of instances
- DIMSE N-ACTION for external systems requesting Storage Commitment
- DIMSE N-EVENT-REPORT for receiving commitment result from a previous request

4.2.3.4.1 Activity – Save to local disk

4.2.3.4.1.1 Description and Sequencing of Activity

The syngo X Workplace DICOM application will accept an association and will receive SOP Instances according to the listed presentation contexts on that association and will store the images to the local hard disk if the conformance check is performed successfully.

Upon successful receiving a C-STORE-RQ, the syngo X Workplace DICOM receiver performs a plausibility test on the received image and available system resources. If this test succeeds, it returns the Status SUCCESS, otherwise one of the following status codes is returned and the association is aborted:

Table 8 - Status codes "Save to local disk"

Code	Meaning
A700	<u>Refused</u> : This error status indicates a lack of Resources (e.g. not enough disk space) on the syngo X Workplace modality.

A900	<u>Invalid Dataset</u> : An error occurred while processing the image, which makes it impossible to proceed. The image will not be stored and the association is aborted.
0110	<u>Processing Error</u> : An error occurred while processing the image, which makes it impossible to proceed. Association is aborted.

Note: The image will be saved after sending the response. If during this operation an error occurs, the association will be aborted. This implies that a C-STORE-RSP with status SUCCESS does not mean that the image was successfully stored into the database.

4.2.3.4.1.2 Accepted Presentation Context

The syngo X Workplace DICOM application will accept Presentation Contexts as shown in the following table:

Table 9 - Presentation Context Table "Save to local disk"

Presentation Context Table – "Save to local disk"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Any image SOP Class detailed in "Table 1 - Network Services" section "Transfer (Image SOP Class)".	JPEG Lossy Extended	1.2.840.10008.1.2.4.51	SCP	None
	JPEG Lossless, Process 14 (selection value 1)	1.2.840.10008.1.2.4.70		
	JPEG Lossy Baseline (Process 1)	1.2.840.10008.1.2.4.50		
	Explicit VR Little Endian	1.2.840.10008.1.2.1		
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
X-Ray 3D Angiographic Image Storage SOP Class "4D DSA"	JPEG-LS Lossless	1.2.840.10008.1.2.4.80	SCP	None
Any non-image SOP Class detailed in "Table 1 - Network Services" section "Transfer (Non-image SOP Class)".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		
Private SOP Class as detailed in Chapter "Table 1 - Network Services" section "Transfer (Private SOP Class)".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.3.4.1.3 SOP specific Conformance

The syngo X Workplace application conforms to the Full Storage Service Class at Level 2.

With Implicit VR Little Endian Transfer Syntax, the syngo X Workplace DICOM application will remove any Private Attributes not known to the application. Decision on removal of a Private Element is done if there is NO entry in the attribute-dictionary of the DICOM application.

Therefore, any Explicit VR Transfer Syntax is preferred to be used by the Storage SCUs when sending Composite Image Instances to the syngo X Workplace DICOM application.

If an image instance is received that is identified by a SOP Instance UID which is already used by an Instance stored in database, then the actual received image will be discarded. The existing Instance is not superseded.

The order of preference in accepting Transfer Syntaxes within Presentation Contexts or Presentation Contexts with single Transfer Syntaxes is:

Table 10 - Order of Preference Transfer Syntax

Order	DICOM Transfer Syntax
1	JPEG Lossy Extended
2	JPEG Lossless Non-hierarchical
3	JPEG Lossy Baseline
4	RLE Lossless
5	Explicit VR Little Endian
6	Explicit VR Big Endian
7	Implicit VR Little Endian
8	JPEG 2000
9	JPEG 2000 (Lossless only)

With RLE Lossless Transfer Syntax, the syngo X Workplace DICOM application will decompress the image before storing it into the database.

The following sections will differentiate the attribute contents required for Image Viewing. The syngo X Workplace DICOM application supports more formats for Storage of Images than for Viewing.

The syngo X Workplace Angio Viewer supports only XA-Images for display. Only a number of pixel columns with a multiple of 4 is supported for display in Angio Viewer.

Image Pixel Attribute Acceptance Criterion for Grayscale Images

The syngo X Workplace Multi-modality Viewing application accepts MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format and graphic overlay with unsigned integer and 8 or 16 bits allocated. The Angio Viewer application accepts only square-sized matrices with 512 or 1024 pixels. Accepted values:

Pixel plane

- Samples per Pixel (attribute 0028,0002) = 1
- Photometric Interpretation (attribute 0028,0004) = "MONOCHROME1"
- Photometric Interpretation (attribute 0028,0004) = "MONOCHROME2"
- Only aspect ratio 1:1 is supported
- Pixel Representation (attribute 0028,0103) = 0
- Bits Allocated (attribute 0028,0100) = 8, 16
- Bits Stored (attribute 0028,0101) = 8, 10, 12
- High Bit (attribute 0028,0102) = 7, 9, 11
- (Angio Viewer only) Rows/Columns = 512 or 1024

Overlay plane "embedded"

- Overlay Type (attribute 60xx,0040) = "G"
- Bits Allocated (attribute 60xx,0100) = 16
- Bit Position (attribute 60xx,0102) = 12, 13, 14, 15

Graphic Overlay will be shifted to fill Overlay Planes from Bit 12 and consecutive.

Overlay plane "explicit"

- Overlay Type (attribute 60xx,0040) = "G"
- Bits Allocated (attribute 60xx,0100) = 1
- Bit Position (attribute 60xx,0102) = 0
- Overlay Data (attribute 60xx,3000) = supported

The syngo X Workplace Multi-Modality Viewing application accepts also the MONOCHROME1 and MONOCHROME2 photometric interpretation pixel format with binary 2's complement integer and 16 bits allocated. This format is not supported for Angio Viewer display. Accepted values:

Pixel plane

- Samples per Pixel (attribute 0028,0002) = 1
- Photometric Interpretation (attribute 0028,0004) = "MONOCHROME1"
- Photometric Interpretation (attribute 0028,0004) = "MONOCHROME2"
- Only aspect ratio 1:1 is supported
- Pixel Representation (attribute 0028,0103) = 1
- Bits Allocated (attribute 0028,0100) = 16
- Bits Stored (attribute 0028,0101) = 16
- High Bit (attribute 0028,0102) = 15

Overlay plane

- Overlay Type (attribute 60xx,0040) = "G"
- Bits Allocated (attribute 60xx,0100) = 1
- Bit Position (attribute 60xx,0102) = 0
- Overlay Data (attribute 60xx,3000) = supported

For Modality LUT, both the linear LUT (Rescale Slope/Intercept) and the Modality LUT Sequence are supported and considered when pixel data is displayed. However, there are two limitations. The Modality LUT Sequence will be ignored in the following cases:

- 8-Bit signed pixels
- the pixel format is changed by the Modality LUT (e.g. 8bit -> 16bit)

If the Modality LUT Sequence contains multiple LUTs, then only the first one is used.

For VOI LUT, both the linear LUT (Window Center/Width) and the VOI LUT Sequence are supported (VOI LUT Sequence with 8 or 16 bit LUT data)

But if both, a VOI LUT Sequence and a linear Modality LUT, are specified within one image, then the value for Rescale Slope is restricted to 1.

If the VOI LUT Sequence contains multiple LUTs, then only the first one is used by default. The other VOI LUTs are selectable.

Image Pixel Attribute Acceptance Criterion for Color Images

The syngo X Workplace Multi-modality Viewing application supports the RGB color image description with the unsigned integer 24-bit color image plane pixel format. This format is not supported for Angio Viewer or Composing display. Accepted values:

- Samples per Pixel (attribute 0028,0002) = 3
- Photometric Interpretation (attribute 0028,0004) = "RGB"
- Pixel Representation (attribute 0028,0103) = 0
- Bits Allocated (attribute 0028,0100) = 8
- Bits Stored (attribute 0028,0101) = 8
- High Bit (attribute 0028,0102) = 7
- Planar Configuration (attribute 0028,0006) = 0 (pixel interleave) or 1 (plane interleave).

The syngo X Workplace Multi-modality Viewing application supports the "Palette Color" color image description with the unsigned integer and 2's complement pixel format. This format is not supported for Angio Viewer or Composing display. Accepted values:

- Samples per Pixel (attribute 0028,0002) = 1
- Photometric Interpretation (attribute 0028,0004) = "PALETTE COLOR"
- Pixel Representation (attribute 0028,0103) = 0
- Bits Allocated (attribute 0028,0100) = 8, 16
- Bits Stored (attribute 0028,0101) = 8, 16
- High Bit (attribute 0028,0102) = 7, 15

Both 8-bit and 16-bit palettes are supported, but NO Segmented Palette Color LUTs.

4.2.3.4.2 Activity – Evaluate Commit Request

4.2.3.4.2.1 Description and Sequencing of Activity

When receiving a Storage Commitment request the syngo X Workplace DICOM application will perform the necessary steps to check the received list Instances against the local database.

4.2.3.4.2.2 Accepted Presentation Context

The syngo X Workplace DICOM application will accept Storage Commitment Presentation Contexts as shown in the following table:

Table 11 - Presentation Context Table "Evaluate Commit Request"

Presentation Context Table – "Evaluate Commit Request"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
Storage Commitment SOP Class detailed in "Table 1 - Network Services" section "Workflow Management".	Explicit VR Little Endian	1.2.840.10008.1.2.1	SCP	None
	Explicit VR Big Endian	1.2.840.10008.1.2.2		
	Implicit VR Little Endian	1.2.840.10008.1.2		

4.2.3.4.2.3 SOP specific Conformance

The syngo X Workplace Storage SCP AE will return success for images that are stored in the local database and failure for images that are not. However, the committed images can later be deleted by the user at the syngo X Workplace without notice!

Note: Storage Media File-Set ID and UID Attributes will not be supported in the N-EVENT-REPORT primitive invoked by the Storage Commitment SCP.

4.2.3.4.3 Activity – Update Flag Information

4.2.3.4.3.1 Description and Sequencing of Activity

After sending a Storage Commitment Request the syngo X Workplace either waits on the same association or, being configured to receive response on a separate association, closes the association and waits for an association request from the Storage Commitment SCP that wants to send the results.

Any incoming Notification will be checked for validity, that is, if the related Transaction UID is still part of the Pending Request Queue.

If the Notification is valid the related Instances are marked with the reported status. The over-all Commit Status of the higher Information Entities in the syngo X Workplace database is derived from propagation of the States of all subordinate Image entities included in a study.

The Status Flags directly affected by Storage Commitment results and indicated in the different entities of the Patient Browser list can be one of

- "AC" or "SC" - Successful Commitment, "A" means archived to configured Archive destination, whereas "S" means sent to any other destination.
- "Af" or "Sf" - Commitment failed.
- "A?" or "S?" - Commitment request is sent, response is pending.

In case of failure the user has to repeat the transfer of images to the Archive destination. Another Storage Commitment will be performed after sending is completed successfully.

Note: Setting of Status Flags is only possible for previously stored images. Any temporary image sent, will not be affected by a Commit Response, due to the fact that there is no permanent dataset to be updated.

4.2.3.4.3.2 Accepted Presentation Context

The syngo X Workplace DICOM application will accept Storage Commitment Presentation Contexts as shown in the following table:

Table 12 - Presentation Context Table "Update Flag Information"

Presentation Context Table – "Update Flag Information"				
Abstract Syntax	Transfer Syntax		Role	Ext. Neg.
Description	Name List	UID List		
1.2.840.10008.1.20.1 Storage Commitment Push Model	Explicit VR Little Endian Explicit VR Big Endian Implicit VR Little Endian	1.2.840.10008.1.2.1 1.2.840.10008.1.2.2 1.2.840.10008.1.2	SCP	None

4.2.3.4.3.3 SOP specific Conformance

If the Commitment response (N-EVENT-REPORT) received has the status of "complete - failure exists", the transaction is marked as "failed", else the transaction is marked as "completed". In both cases, a message is shown to the user.

The related status flags are set for the committed images in the local database.

The syngo X Workplace DICOM application will not support the Storage Media File Set ID attributes.

4.2.4 Query/Retrieve SCU Specification

4.2.4.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" section "Query/Retrieve" in the "Conformance Statement Overview".

4.2.4.2 Association Policies

4.2.4.2.1 General

With the "Search..." function the query data can be entered and the DICOM Query/Retrieve application is initiated. An initial query request will be sent out to one remote node that can be selected from a list of configured Query Providers. Depending on the replies to the initial request, sub-subsequent query requests are issued to gather further data for lower information level entities. The results compiled from the response data will be displayed to the user. Upon request (Import), the retrieval of selected items is initiated.

The default PDU size used will be 528378 bytes.

4.2.4.2.2 Number of Associations

The syngo X Workplace DICOM application initiates several associations at a time.

For Query it initiates a new association to the remote node and issues the C-FIND request to retrieve all the requested patient and study information matching the search criteria. The syngo X Workplace initiates in parallel a second associa-

tion to the destination node to query for all the series information for each study's information returned on the first association.

For the Retrieve request (C-MOVE) only one association is initiated per destination.

4.2.4.2.3 Asynchronous Nature

The syngo X Workplace DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.4.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information" in the "Conformance Statement Overview".

4.2.4.3 Association Initiation Policy

The syngo X Workplace DICOM application will request associations for the following DIMSE-C operations as SCU:

Table 13 - Supported DIMSE-C Operations - Query/Retrieve SCU

Supported DIMSE operations	Cancel Request supported
C-FIND	yes
C-MOVE	n. a.

Extended negotiation (relational query) is not supported for the above listed services.

4.2.4.3.1 Activity – Search for images (Search...)

4.2.4.3.1.1 Description and Sequencing of Activity

The associated activity is to fill out a query form with search data and pass it as query to the network application which issues a C-FIND over a previously built association. The remote SCP will respond with related data-entries that will be passed to a browser application. If needed, further associations are opened for querying data from sub-sequent entities. When data transfer is finished, each association is closed.

If the C-FIND Response from the remote Application contains an error status, the association is aborted.

4.2.4.3.1.2 Proposed Presentation Contexts

The syngo X Workplace DICOM application will propose Presentation Contexts as shown in the following table:

Table 14 - Presentation Context Table "Search..."

Presentation Context Table - "Search..."					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Patient/Study Only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Big Endian	1.2.840.10008.1.2.2		
		Explicit VR Little Endian	1.2.840.10008.1.2.1		

Within the DICOM network configuration it is configurable which of the two query models (or both) are to be used by the syngo X Workplace DICOM Query SCU application for each node. If both Abstract Syntaxes are configured, the Find

SCU will use the Patient Root Model only for C-FIND requests on PATIENT level. For all other levels it will use the Study Root model.

4.2.4.3.1.3 SOP Specific Conformance

The syngo X Workplace DICOM Query/Retrieve SCU supports hierarchical queries with all mandatory search keys. The interactive querying of attributes on IMAGE level is not supported by the Query SCU, hence retrieval of individual Objects is possible. The following table describes the search keys for the different query models that the SCU supports. Matching is either wildcard, which means that the user can supply a string containing wildcards, or universal, which means that the attribute is requested as return value.

Table 15 - C-FIND RQ Search Keys

Attribute Name	Tag	Type	Matching	User Input	Return Value Display
Patient Level³					
Patient's Name	(0010,0010)	R	Wildcard ⁴	Enter value	yes
Patient ID	(0010,0020)	U / R	Wildcard ⁴	Enter value	yes
Patient's Birth Date	(0010,0030)	O	Single value	Enter value	yes
Patient's Sex	(0010,0040)	O	Single value	Enter value	yes
Number of Patient related Studies	(0020,1200)	O	Universal(Null)	--	yes ⁵
Number of Patient related Series	(0020,1202)	O	Universal(Null)	--	no
Number of Patient related Instances	(0020,1204)	O	Universal(Null)	--	no
Study Level					
Patient's Name ⁶	(0010,0010)	R	Wildcard ⁴	Enter value	yes
Patient ID	(0010,0020)	U / R	Wildcard ⁴	Enter value	yes
Patient's Birth Date ⁶	(0010,0030)	O	Single value	Enter value	yes
Patient's Sex ⁶	(0010,0040)	O	Single value	Enter value	yes
Study Instance UID	(0020,000D)	U	Single value	Enter value	yes
Study ID	(0020,0010)	R	Wildcard ⁴	Enter value	yes
Study Date	(0008,0020)	R	Range	Enter value	yes
Study Time	(0008,0030)	R	Range	Enter value	yes
Accession Number	(0008,0050)	R	Wildcard	Enter value	yes
Study Description	(0008,1030)	O	Wildcard ⁴	Enter value	yes
Referring Physician's Name	(0008,0090)	O	Wildcard ⁴	Enter value	yes
Name of Physician Reading Study	(0008,1060)	O	Wildcard ⁴	Enter value	yes
Modalities in Study	(0008,0061)	O	Single Value	Enter value	yes
Number of Patient related Studies	(0020,1200)	O	Universal(Null)	--	no
Number of Patient related Series	(0020,1202)	O	Universal(Null)	--	no
Number of Patient related Instances	(0020,1204)	O	Universal(Null)	--	no
Number of Study related Series	(0020,1206)	O	Universal(Null)	--	yes ⁷
Number of Study related Instances	(0020,1208)	O	Universal(Null)	--	no
Series Level					
Series Instance UID	(0020,000E)	U	Single Value	Enter value	yes
Series Number	(0020,0011)	R	Single Value	Enter value	yes
Modality	(0008,0060)	R	Single Value	Enter value	yes
Series Date	(0008,0021)	O	Universal(Null)	--	yes
Series Time	(0008,0031)	O	Universal(Null)	--	yes
Series Description	(0008,103E)	O	Wildcard ⁴	Enter value	yes

³ Patient Root Information Model only

⁴ Always a "*" is appended to the user-supplied string

⁵ Implicitly visualized in the UI if no study and series search attributes have been entered

⁶ Study Root Information Model only

⁷ Implicitly if no series search attributes have been entered

© Siemens Healthcare GmbH. 2020. All rights reserved.

Attribute Name	Tag	Type	Matching	User Input	Return Value Display
Body Part Examined	(0018,0015)	O	Single Value	Enter value	yes
Performing Physician's Name	(0008,1050)	O	Wildcard ⁴	Enter value	yes
Request Attributes Sequence	(0040,0275)	O	--	--	yes
>Requested Procedure ID	(0040,1001)	O	Wildcard ⁴	Enter value	yes
>Scheduled Procedure Step ID	(0040,0009)	O	Wildcard ⁴	Enter value	yes
Performed Procedure Step Start Date	(0040,0244)	O	Range	Enter value	yes
Performed Procedure Step Start Time	(0040,0245)	O	Range	Enter value	yes
Number of Series related Instances	(0020,1209)	O	Universal(Null)	--	yes
Instance Availability	(0008,0056)	O	Universal(Null)		
Image Level					
SOP Instance UID	(0008,0018)	U	Single Value	--	no
Instance Number	(0020,0013)	R	Universal(Null)	--	yes
SOP Class UID	(0008,0016)	O	Universal(Null)	--	no
Image Comments	(0020,4000)	O	Universal(Null)	--	yes
Number of Frames	(0028,0008)	O	Universal(Null)	--	yes
Content Date	(0008,0023)	O	Universal(Null)	--	yes
Content Time	(0008,0033)	O	Universal(Null)	--	yes

U = Unique Key, R = Required Key, O = Optional Key, - = not supported or applicable

The syngo X Workplace Search application supports a

DIMSE C-FIND-CANCEL

if the user wishes to cancel a running Query request via the syngo X Workplace user interface ("Cancel" button while a "Search..." is active).

The Find SCU interprets following status codes:

Table 16 - Status Codes "Search..."

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

4.2.4.3.2 Activity – Retrieve Images (Import...)

4.2.4.3.2.1 Description and Sequencing of Activity

When selecting a data entry in the Query UI and activating the "Import" function, a retrieval request is passed to the syngo X Workplace DICOM application which issues a C-MOVE service according to the Patient Root or Study Root query model. (The Storage Service Class Conformance Statement describes the C-STORE service, which is generated by processing the C-MOVE service.)

The received image data are processed as described in the Storage class SCP descriptions.

The syngo X Workplace DICOM application will always insert the own Storage SCP AE as "Move Destination".

4.2.4.3.2.2 Proposed Presentation Contexts

The syngo X Workplace Server DICOM application will propose Presentation Contexts as shown in the following table:

Table 17 - Presentation Context Table "Import..."

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Query/Retrieve Model Patient Root – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Query/Retrieve Model Study Root – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None
Query/Retrieve Model Patient/Study Only – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCU	None

Note: C-MOVE Extended Negotiation will not be supported by the SCU.

4.2.4.3.2.3 SOP Specific Conformance

All required keys will be provided in the retrieve request identifier, as defined in DICOM Standard.

The Move SCU interprets following status codes:

Table 18 - C-MOVE RSP Status Codes

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
	Move destination unknown	A801	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	Cxxx	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

4.2.4.4 Association Acceptance Policy

See next section "Query/Retrieve SCP AE Specification".

4.2.5 Query/Retrieve SCP Specification

4.2.5.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" section "Query/Retrieve" in the "Conformance Statement Overview".

4.2.5.2 Association Policies

4.2.5.2.1 General

syngo X Workplace will only accept Associations from known hosts with a known AET ("trusted hosts" concept). Hosts and AETs have to be entered in "Local Service" by a Siemens CSE.

The default PDU size used will be 528378 bytes.

4.2.5.2.2 Number of Associations

The Siemens syngo X Workplace DICOM application is able to accept multiple associations at a time. It can handle up to 10 associations in parallel.

The number of simultaneous DICOM associations can be configured via the Service-UI. The dialog can be found in "Configuration / DICOM / General".

4.2.5.2.3 Asynchronous Nature

The syngo X Workplace DICOM software does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.5.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information".

4.2.5.3 Association Initiation Policy

See previous section "Query/Retrieve SCU AE Specification".

4.2.5.4 Association Acceptance Policy

The syngo X Workplace DICOM application will accept associations for the following DIMSE-C operations as SCP:

- C-FIND
- C-GET
- C-MOVE
- C-FIND-CANCEL
- C-GET-CANCEL
- C-MOVE-CANCEL

Extended negotiation - which is relational query or retrieve - is not supported for the above listed services. The syngo X Workplace DICOM application does support multiple C-FIND requests over the same association, while multiple C-MOVE or C-GET operations are not supported over the same association.

4.2.5.4.1 Activity - Process Search Requests

4.2.5.4.1.1 Description and Sequencing of Activity

The Query SCP AE will respond to incoming query requests from a SCU with the query model Patient Root, Study Root and Patient/Study Only. Relational retrieve operation is not supported. The content records of the local database are used to match the incoming query keys and fill the related return keys. With a C-FIND-CANCEL request the running query can be canceled at any time.

Multiple C-FIND requests over the same association are supported.

4.2.5.4.1.2 Accepted Presentation Contexts

The syngo X Workplace DICOM application will accept Presentation Contexts as shown in the following table:

Table 19 - Presentation Context Table "Process Search Requests"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Study Root Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Patient/Study Only Query/Retrieve Model - FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None

Note: C-FIND Extended Negotiation will not be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

4.2.5.4.1.3 SOP Specific Conformance

The syngo X Workplace DICOM Query/Retrieve SCP supports hierarchical queries for all mandatory and optional search keys.

The syntactical component structure of the attribute (0010,0010) Patient's Name is defined as follows (see [DICOM], Part 5, Definition of PN, Person Name):

<single byte group> =<ideographic group>=<phonetic group>

The Query/Retrieve SCP replies to queries for "Patient Name" as follows:

1. Matching of Patient's Name attribute (0010,0010) is done case insensitive.
2. If a search string matches the complete value of a Patient's Name in the database, a match will be returned.
3. If a search string matches an individual group (single byte, ideographic or phonetic) of a Patient's Name in the database, a match will be returned.
4. If a search string matches two consecutive groups of a data base object's Patients Name, a match will be returned.
5. Redundant group separators "=" or component separators "^" are treated as insignificant for matching.
6. Leading and trailing blanks within a component or a group of Patient's Name are treated as insignificant for matching.

Except for attribute Patient's Name (0010,0010) any queries for text string attributes will be treated case sensitive.

The Find SCP will not differentiate "?" and "*", thus "?abc*" will be treated as "*abc*".

If the value for the patient-level unique key "Patient ID" is not known, it will be returned with zero length. The attribute "Image Comments" will not be included in the C-FIND-RSP, if it is not set in the DB, even if it was requested as return key in the related C-FIND-RQ.

Usage of Storage Media File-Set ID, Retrieve AE Title with C-FIND-RSP message:

- The Storage Media File-Set ID - if available - can be returned at Study/Series/Image Level. Only on Image Level, the values of ONLINE, NEARLINE or OFFLINE are returned to indicate the Storage Location of the related Instance.
- The Retrieve AE Title - if available - can only be returned at Image Level (for Patient Root and Study Root models) or Study Level (for Patient/Study Only model).

Relational Queries are not supported.

A remote DICOM AE can cancel the running query by sending a C-FIND-CANCEL. Matches are possibly continuing (more C-FIND response with status PENDING) until the cancel operation takes effect and query matching has completed.

The supported attributes on the various query levels of the three supported information models are listed in the following table.

Table 20 - Query/Retrieve SCP supported attributes

Attribute Name	Tag	PR	SR	PSo	Matching
Patient Level (PR or PSo) or Study Level (SR)					
Patient's Name	(0010,0010)	R	R	R	Single value, Wildcard, universal
Patient ID	(0010,0020)	U	R	U	Single Value, Wildcard, universal
Patient's Birth Date	(0010,0030)	O	O	O	Single Value, Range, universal
Patient's Birth Time	(0010,0032)	O	O	O	Single Value, Range, universal
Patient's Sex	(0010,0040)	O	O	O	Single Value, Wildcard, universal
Ethnic Group	(0010,2160)	O	-	O	Single Value, Wildcard, universal
Patient Comments	(0010,4000)	O	O	O	Wildcard, universal
Number of Patient related Studies	(0020,1200)	O	O	O	universal
Number of Patient related Series	(0020,1202)	O	O	O	universal
Number of Patient related Instances	(0020,1204)	O	O	O	universal
Study Level					
Study Instance UID	(0020,000D)	U	U	U	Single Value, List of UIDs
Study ID	(0020,0010)	R	R	R	Single Value, Wildcard, universal
Study Date	(0008,0020)	R	R	R	Single Value, Range, universal

Attribute Name	Tag	PR	SR	PSo	Matching
Study Time	(0008,0030)	R	R	R	Single Value, Range, universal
Accession Number	(0008,0050)	R	R	R	Single Value, Wildcard, universal
Referring Physician's Name	(0008,0090)	O	O	O	Single Value, Wildcard, universal
Study Description	(0008,1030)	O	O	O	Single Value, Wildcard, universal
Admitting Diagnosis Description	(0008,1080)	O	O	O	Single Value, Wildcard, universal
Patient's Age	(0010,1010)	O	O	O	Single Value, Wildcard, universal
Patient's Size	(0010,1020)	O	O	O	Single Value, universal
Patient's Weight	(0010,1030)	O	O	O	Single Value, universal
Occupation	(0010,2180)	O	O	O	Single Value, Wildcard, universal
Additional Patient History	(0010,21B0)	O	O	O	Wildcard, universal
Name of Physician reading the Study	(0008,1060)	O	O	O	Single Value, Wildcard, universal
Modalities in Study	(0008,0061)	O	O	O	Multiple values, universal
Number of Study Related Series	(0020,1206)	O	O	O	universal
Number of Study Related Instances	(0020,1208)	O	O	O	universal
Series Level					
Series Instance UID	(0020,000E)	U	U	-	Single Value, List of UIDs
Series Number	(0020,0011)	R	R	-	Single Value, universal
Modality	(0008,0060)	R	R	-	Single Value, Wildcard, universal
Laterality	(0020,0060)	O	O	-	Single Value, Wildcard, universal
Body Part Examined	(0018,0015)	O	O	-	Single Value, Wildcard, universal
Patient Position	(0018,5100)	O	O	-	Single Value, Wildcard, universal
Smallest Pixel Value in Series	(0028,0108)	O	O	-	Single Value, universal
Largest Pixel Value in Series	(0028,0109)	O	O	-	Single Value, universal
Protocol Name	(0018,1030)	O	O	-	Single Value, Wildcard, universal
Series Date	(0008,0021)	O	O	-	Single Value, Range, universal
Series Time	(0008,0031)	O	O	-	Single Value, Range, universal
Series Description	(0008,103E)	O	O	-	Single Value, Wildcard, universal
Operator's Name	(0008,1070)	O	O	-	Single Value, Wildcard, universal
Performing Physician's name	(0008,1050)	O	O	-	Single Value, Wildcard, universal
Performed Procedure Step Start Date	(0040,0244)	O	O	-	universal
Performed Procedure Step Start Time	(0040,0245)	O	O	-	universal
Number of Series related Instances	(0020,1209)	O	O	-	universal
Image or SR Document Level					
SOP Instance UID	(0008,0018)	U	U	-	Single Value, List of UIDs
Instance Number	(0020,0013)	R	R	-	Single Value, universal
Content Date	(0008,0023)	O	O	-	Single Value, Range, universal
Content Time	(0008,0033)	O	O	-	Single Value, Range, universal
Modality	(0008,0060)	O	O	-	Single Value, Wildcard, universal
Image Comments	(0020,4000)	O	O	-	universal
Referenced Request Sequence	(0040,A370)	O	O	-	Sequence matching
>Accession Number	((0008,0050)	O	O	-	Single value, universal
>Requested Procedure ID	(0040,1000)	O	O	-	Single value, universal
Concept Name Code Sequence	(0040,A043)	O	O	-	Sequence matching
>Code Value	(0008,0100)	O	O	-	Single Value, Wildcard, universal
>Coding Scheme Designator	(0008,0102)	O	O	-	Single Value, Wildcard, universal
>Coding Scheme Version	(0008,0103)	O	O	-	Single Value, Wildcard, universal
>Code Meaning	(0008,0104)	O	O	-	Single Value, Wildcard, universal
Template Identifier	(0040,DB00)	O	O	-	Single Value, Wildcard, universal
Completion Flag	(0040,A491)	O	O	-	Single Value, Wildcard, universal
Verification Flag	(0040,A493)	O	O	-	Single Value, Wildcard, universal
Verifying Observer Sequence	(0040,A073)	O	O	-	Sequence matching
>Verifying Organization	(0040,A027)	O	O	-	Single Value, Wildcard, universal

Attribute Name	Tag	PR	SR	PSo	Matching
>Verifying Date Time	(0040,A030)	O	O	-	Single Value, Range, universal
>Verifying Observer Name	(0040,A075)	O	O	-	Single Value, Wildcard, universal
>Verifying Observer Identification Code Sequence	(0040,A088)	O	O	-	Sequence matching
>>Code Value	(0008,0100)	O	O	-	Single Value, Wildcard, universal
>>Coding Scheme Designator	(0008,0102)	O	O	-	Single Value, Wildcard, universal
>>Coding Scheme Version	(0008,0103)	O	O	-	Single Value, Wildcard, universal
>>Code Meaning	(0008,0104)	O	O	-	Single Value, Wildcard, universal

PR = Patient Root Model, SR = Study Root Model, PSo = Patient/Study Only Model
U = Unique Key, R = Required Key, O = Optional Key, - = not supported or applicable

The "Process Search Requests" activity can return the following status codes:

Table 21 - Status Codes Process Search Request

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources	A700	(0000,0902)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Matching terminated due to Cancel request	FE00	None
Success	Matching is complete - No final Identifier is supplied	0000	None
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	Identifier
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this identifier	FF01	Identifier

4.2.5.4.2 Activity - Process Retrieve Requests

4.2.5.4.2.1 Description and Sequencing of Activity

The associated activity is to respond to retrieve requests initiated from a foreign SCU. Relational retrieve operation is not supported.

Multiple C-GET or C-MOVE requests over the same association are not supported.

4.2.5.4.2.1 Accepted Presentation Contexts

The syngo X Workplace DICOM application will accept Presentation Contexts as shown in the following table:

Table 22 - Presentation Context Table "Process Retrieve Requests"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Patient Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.1.3	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Study Root Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.2.3	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Patient/Study Only Query/Retrieve Model - GET	1.2.840.10008.5.1.4.1.2.3.3	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Patient Root Query/	1.2.840.10008.5.1.4.1.2.1.2	Implicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2	SCP	None

Retrieve Model - MOVE		Explicit VR Little Endian	1.2.840.10008.1.2.1		
Study Root Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None
Patient/Study Only Query/Retrieve Model - MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit VR Little Endian Explicit VR Big Endian Explicit VR Little Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.2 1.2.840.10008.1.2.1	SCP	None

Note: C-FIND Extended Negotiation will not be supported.

The order of preference for accepting Transfer Syntaxes is: 1. Explicit VR Little Endian, 2. Explicit VR Big Endian, 3. Implicit VR Little Endian.

4.2.5.4.2.2 SOP Specific Conformance

Relational retrieve operation is not supported.

All unique keys have to be supplied according to the selected Query/Retrieve Level. The related tables in the C-FIND SCP section will give information about "U" marked key attributes.

The C-STORE can only be performed to AEs that are configured in the syngo X Workplace.

The "Process Retrieve Requests" activity can return the following status codes:

Table 23 - Status Codes "Process Retrieve Requests"

Service Status	Meaning	Error Codes	Related Fields
Refused	Out of Resources - Unable to calculate number of matches	A701	(0000,0902)
	Out of Resources - Unable to perform sub operations	A702	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Failed	Identifier does not match SOP Class	A900	(0000,0901) (0000,0902)
	Unable to process	C001	(0000,0901) (0000,0902)
Cancel	Sub-operations terminated due to Cancel Indication	FE00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Warning	Sub-operations Complete - One or more Failures of Warnings	B000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Success	Sub-operations Complete - No Failures or Warning	0000	(0000,1020) (0000,1021) (0000,1022) (0000,1023)
Pending	Sub-operations are continuing	FF00	(0000,1020) (0000,1021) (0000,1022) (0000,1023)

4.2.6 Print SCU Specification

4.2.6.1 SOP Classes

For SOP Classes supported, please refer to "Table 1 - Network Services" section "Print Management" in the "Conformance Statement Overview".

4.2.6.2 Association Policies

4.2.6.2.1 General

Whenever a film-sheet is completely set up and printed by command or automated rule, the job is prepared for processing. As soon as the queue is ready to process the job, it is activated and worked according to the processing data. The Print application will initiate an association to the print destination and process the printing.

The default PDU size used will be 528378 bytes.

4.2.6.2.2 Number of Associations

The syngo X Workplace DICOM application initiates one association at a time for each different print device configured.

4.2.6.2.3 Asynchronous Nature

The syngo X Workplace DICOM print application does not support asynchronous communication (multiple outstanding transactions over a single association).

4.2.6.2.4 Implementation Identifying Information

For Implementation Identifying Information please refer to "Table 3 - Implementation Identifying Information" in the "Conformance Statement Overview".

4.2.6.3 Association Initiation Policy

Triggered by the Print job queue the Print Management SCU establishes an association by using the DICOM association services. An N-GET request determines the printer status prior to printing. If the printer status is "normal", the print job is started.

After the last film is printed from queue, the Print application will leave open the association for another 60 seconds. If a new film job is ready for printing within this time-limit, the job will be immediately processed over the still open association. If there is no new job, the association is closed.

During the "idle-time" (no open association to printer) the Print application will issue a cyclic camera status request (using N-GET of the Printer SOP Class) every 5 minutes.

4.2.6.3.1 Activity - Print Film

4.2.6.3.1.1 Description and Sequencing of Activity

The film sheet is internally processed, converted to a Standard/1-1 page and then the page image is sent. Status is controlled by awaiting any N-EVENT message through the transfer until the last image or film-sheet is sent.

If the response from the remote application contains a status other than Success or Warning the association is aborted.

4.2.6.3.1.2 Proposed Presentation Context

The syngo X Workplace DICOM application will propose Presentation Contexts as shown in the following table:

Table 24 - Presentation Context Table "Print Film"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Basic Grayscale Print Management Meta SOP Class	1.2.840.10008.5.1.1.9	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Color Print Management Meta SOP Class	1.2.840.10008.5.1.1.18	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Film Session SOP Class	1.2.840.10008.5.1.1.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Film Box SOP Class	1.2.840.10008.5.1.1.2	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Grayscale Image Box SOP Class	1.2.840.10008.5.1.1.4	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Basic Color Image Box SOP Class	1.2.840.10008.5.1.1.4.1	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Print Job SOP Class	1.2.840.10008.5.1.1.14	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None
Presentation LUT SOP Class	1.2.840.10008.5.1.1.23	Implicit VR Little Endian Explicit VR Little Endian Explicit VR Big Endian	1.2.840.10008.1.2 1.2.840.10008.1.2.1 1.2.840.10008.1.2.2	SCU	None

4.2.6.3.1.3 SOP Specific Conformance

The syngo X Workplace DICOM print management SCU conforms to the DICOM Basic Grayscale Print Management Meta SOP Class.

The application uses a setting platform to define the properties of the connected DICOM SCP, e.g.:

- maximum number of print jobs in the queue
- maximum number of print copies
- supported film sizes of the connected DICOM SCP
- supported film formats of the DICOM SCP
- lookup table definition.

The printing is only suspended in the case of a failure return status of the SCP.

Basic Film Session SOP Class

The Basic Film Session information object definition describes all the user-defined parameters, which are common for all the films of a film session. The Basic Film Session refers to one or more Basic Film Boxes that are printed on one hard-copy printer.

The syngo X Workplace DICOM print management SCU supports the following DIMSE Service elements for the Basic Film Session SOP Class as SCU:

- N-CREATE
- N-DELETE

The Basic Film Session SOP Class N-CREATE-RQ (SCU) uses the following attributes:

Table 25 - Basic Film Session N-CREATE attributes

Attribute Name	Tag	Usage SCU	Supported Values
Number of Copies	(2000,0010)	U	"1"
Medium Type	(2000,0030)	U	BLUE FILM CLEAR FILM PAPER
Film Destination	(2000,0040)	U	MAGAZINE PROCESSOR

U = User Option

The number of copies sent to the DICOM Printer is always 1, the job is sent n times for n copies.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Session – see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Session

The N-DELETE-RQ on the Basic Film Session SOP Class is used to remove the complete Basic Film Session SOP Instance hierarchy.

The Basic Film Session SOP Class interprets the following status codes (from N-CREATE-RSP, N-DELETE-RSP messages):

Table 26 - Basic Film Session Status Codes

Service Status	Meaning	Error Codes
Failure	Film session SOP instances hierarchy does not contain film box SOP instances	C600
	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603
Warning	Memory allocation not supported	B600
	Film session printing is not supported	B601
	Film box does not contain image box (empty page)	B602
Success	Film belonging to the film session are accepted for printing	0000

Basic Film Box SOP Class

The Basic Film Box information object definition describes all the user-defined parameter of one film of the film session. The Basic Film Box information description defines the presentation parameters, which are common for all images on a given sheet of film.

The Basic Film Box refers to one or more Image Boxes.

Supported Service Elements as SCU are:

- N-CREATE
- N-ACTION
- N-DELETE

The Basic Film Box SOP Class N-CREATE-RQ message uses the following attributes (the actual values for each attribute depend on DICOM printer configuration within the syngo X Workplace DICOM print management SCU):

Table 27 - Basic Film Box N-CREATE attributes

Attribute Name	Tag	Usage SCU	Supported Values
Image Display Format	(2010,0010)	M	STANDARD\1,1
Referenced Film Session Sequence	(2010,0500)	M	n. a.
>Referenced SOP Class UID	(0008,1150)	M	1.2.840.10008.5.1.1.1
>Referenced SOP Instance UID	(0008,1155)	M	
Film Orientation	(2010,0040)	M	PORTRAIT
Film Size ID	(2010,0050)	M	8INX10IN, 10INX12IN, 10INX14IN, 11INX14IN,, 14INX14IN, 14INX17IN, 24CMX24CM, 24CMX30CM
Magnification Type	(2010,0060)	M	BILINEAR, CUBIC, NONE, REPLICATE
Max Density	(2010,0130)	U	> 0
Min Density	(2010,0120)	U	50 > value > 0
Illumination	(2010,015E)	U	> 0 Required if Presentation LUT is present.
Reflective Ambient Light	(2010,0160)	U	> 0 Required if Presentation LUT is present.
Referenced Presentation LUT Sequence	(2050,0500)	U	

M = Mandatory, **U** = User Option

The N-CREATE-RSP message from the Print SCP includes the Referenced Image Box Sequence with SOP Class/Instance UID pairs which will be kept internally and used for the subsequent Basic Image Box SOP Class N-SET-RQ messages.

When all Image Boxes (including parameters) for the film-sheet have been set, the DICOM print manager will issue an N-ACTION-RQ message with the SOP Instance UID of the Basic Film Box and the Action Type ID of 1.

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and used for later requests (e.g. N-DELETE-RQ) on the Basic Film Box - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Basic Film Box

The Basic Film Box SOP Class interprets the following status codes:

Table 28 - Basic Film Box Status Codes

Service Status	Meaning	Error Codes
Failure	Unable to create print job, print queue is full	C601
	Image size is larger than images box size	C603
Warning	Film box does not contain image box (empty page)	B603
	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success	Film accepted for printing	0000

Basic Grayscale Image Box SOP Class

The Basic Grayscale Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Grayscale Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Grayscale Image Box SOP Class uses only the N-SET-RQ with the following attributes:

Table 29 - Basic Grayscale Image Box N-SET attributes

Attribute Name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
BASIC Grayscale Image Sequence	(2020,0110)	M	n.a.
>Samples per Pixel	(0028,0002)	M	1
>Photometric Interpretation	(0028,0004)	M	MONOCHROME2
>Rows	(0028,0010)	M	<Printer/Film config>
>Columns	(0028,0011)	M	<Printer/Film config>
>Pixel Aspect Ratio	(0028,0034)	M	(1:1)
>Bits Allocated	(0028,0100)	M	8, 16
>Bits Stored	(0028,0101)	M	8, 12
>High Bit	(0028,0102)	M	7, 11
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

M = Mandatory

The Grayscale Image Box SOP Class interprets the following status codes:

Table 30 - Basic Grayscale Image Box Status Codes

Service Status	Meaning	Error Codes
Failure	Image contains more pixel than printer can print in Image Box	C603
	Insufficient memory in printer to store the image	C605
Warning	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success		0000

Basic Color Image Box SOP Class

The Basic Color Image Box information object definition is the presentation of an image and image related data in the image area of a film. The Basic Color Image Box information describes the presentation parameters and image pixel data, which apply to a single image of a sheet of film.

The Color Image Box SOP Class uses only the N-SET-RQ with the following attributes:

Table 31 - Basic Color Image Box N-SET attributes

Attribute Name	Tag	Usage SCU	Supported Values
Image Position	(2020,0010)	M	1
BASIC Color Image Sequence	(2020,0111)	M	n.a.
>Samples per Pixel	(0028,0002)	M	3
>Photometric Interpretation	(0028,0004)	M	RGB
>Planar Configuration	(0028,0006)	M	0
>Rows	(0028,0010)	M	<Printer/Film config>
>Columns	(0028,0011)	M	<Printer/Film config>
>Pixel Aspect Ratio	(0028,0034)	M	(1:1)
>Bits Allocated	(0028,0100)	M	8
>Bits Stored	(0028,0101)	M	8
>High Bit	(0028,0102)	M	7
>Pixel Representation	(0028,0103)	M	0
>Pixel Data	(7FE0,0010)	M	

M = Mandatory

The Grayscale Image Box SOP Class interprets the following status codes:

Table 32 - Basic Color Image Box Status Codes

Service Status	Meaning	Error Codes
----------------	---------	-------------

Service Status	Meaning	Error Codes
Failure	Image contains more pixel than printer can print in Image Box	C603
	Insufficient memory in printer to store the image	C605
Warning	Requested MinDensity or MaxDensity outside of Printer's operating range	B605
Success		0000

Presentation LUT SOP Class

The Presentation LUT tailors image hardcopy printing for specific modalities, applications and user preferences.

The output of the Presentation LUT is Presentation Values (P-Values). P-Values are approximately related to human perceptual response. They are intended to facilitate common input for hardcopy. P-Values are intended to be independent of the specific class or characteristics of the hardcopy device.

The Presentation LUT SOP Class uses only the N-CREATE-RQ with the following attributes:

Table 33 - Presentation LUT N-CREATE attribute

Attribute Name	Tag	Usage SCU	Supported Values
Presentation LUT Shape	(2050,0020)	U	IDENTITY

U = User Option

The affected SOP Instance UID received with N-CREATE-RSP message will be kept internally and is used for later requests on the Basic Film Box (N-CREATE-RQ) and on the Presentation LUT (N-DELETE-RQ) - see below:

Attribute Name	Tag	Source of Information
Requested SOP Instance UID	(0000,1000) →(0000,1001)	Affected SOP Instance UID of N-CREATE-RSP on Presentation LUT

The Presentation LUT SOP Class interprets the following status codes:

Table 34 - Presentation LUT Status Codes

Service Status	Meaning	Codes
Success	Presentation LUT successfully created	0000
Warning	Requested MinDensity or MaxDensity outside of printer's operating range. The printer will use its respective minimum or maximum density value instead.	B605

Printer SOP Class

The Printer SOP Class allows monitoring the status of the hardcopy printer in a synchronous and an asynchronous way.

The SCU uses the mandatory N-EVENT Report DIMSE service to monitor the changes of the printer status in an asynchronous way.

The following returned information is supported:

Table 35 - Used Printer N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

U = User Option

Table 36 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

Attribute Name	Tag	Usage SCP	Supported Values
----------------	-----	-----------	------------------

Printer Status	(2110,0010)	M	NORMAL, FAILURE, WARNING
Printer Status Info	(2110,0020)	M	See tables in Annex for details.

M = Mandatory

Note: For a detailed description on how syngo X Workplace reacts on different printer status messages, please refer to the Annex section "8.7 DICOM Print SCU – detailed status displays".

Print Job SOP Class

The Print Job SOP Class allows monitoring the execution of the print process.

The syngo X Workplace DICOM Print Management application supports the optional N-EVENT-REPORT DIMSE Service to receive the changes of the Print Job Status in an asynchronous way.

It can receive Events from the Print SCP asynchronously:

- N-EVENT-REPORT

Note: The underlying syngo DICOM Print AE does not support receiving of N-EVENT-REPORT messages from camera during open print sessions. This is typically configurable in the camera setup.

The following information is supported:

Table 37 - Used Print Job N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Printing	2	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Done	3	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U
Failure	4	Execution Status Info	(2100,0030)	U
		Print Job ID	(2100,0010)	-- (Print Queue Management SOP Class not supported)
		Film Session Label	(2000,0050)	U
		Printer Name	(2110,0030)	U

U = User Option

Note: For a detailed description on how syngo X Workplace reacts on different printer status messages, please refer to the Annex section "8.7 DICOM Print SCU – detailed status displays".

4.2.6.3.2 Activity - Show Device Status

4.2.6.3.2.1 Description and Sequencing of Activity

With no printing activity ongoing ("idle time"), the syngo X Workplace DICOM Print SCU application will cyclically request the printer status to update the related printer state in the Printing UI.

4.2.6.3.2.2 Proposed Presentation Context

The syngo X Workplace DICOM application will propose Presentation Contexts as shown in the following table:

Table 38 - Presentation Context Table "Show Device Status"

Presentation Context Table					
Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name List	UID List		
Printer SOP Class	1.2.840.10008.5.1.1.16	Implicit VR Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit VR Little Endian	1.2.840.10008.1.2.1		
		Explicit VR Big Endian	1.2.840.10008.1.2.2		

4.2.6.3.2.3 SOP Specific Conformance

The Printer SOP Class allows to monitor the status of the hardcopy printer in a synchronous and an asynchronous way.

The Print SCU AE application will cyclically "ask" the Printer (SCP) for its status synchronously:

- N-GET as SCU

The following information is supported:

Table 39 - Used Printer N-EVENT Report attributes

Event-type Name	Event	Attributes	Tag	Usage SCU
Normal	1			
Warning	2	Printer Status Info	(2110,0020)	U
Failure	3	Printer Status Info	(2110,0020)	U

U = User Option

Table 40 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes

Attribute Name	Tag	Usage SCP	Supported Values
Printer Status	(2110,0010)	M	NORMAL, FAILURE, WARNING
Printer Status Info	(2110,0020)	M	See tables in Annex for details.

M = Mandatory

Note: For a detailed description on how syngo X Workplace reacts on different printer status messages, please refer to the Annex section 8.7 DICOM Print SCU – detailed status displays.

4.2.6.4 Association Acceptance Policy

n.a.

4.3 Network Interfaces

4.3.1 Physical Network Interface

The DICOM Interface of the syngo X Workplace provides DICOM TCP/IP Network Communication Support and uses the TCP/IP protocol stack from the operating system. It uses the MergeCOM subroutine library. All available Ethernet interfaces are supported.

4.3.2 Additional Protocols

n.a.

4.4 Configuration

4.4.1 AE Title/Presentation Address Mapping

Local AE Titles

According to the DICOM Standard, the AET string can be up to 16 characters long and must not contain any extended characters, only 7-bit ASCII characters (excluding Control Characters).

Note: The current implementation of *syngo* does not allow Spaces and special characters (like &<> ") in the AE title string. The underscore character "_" may be used in the AE title string.

Change of the default AE Titles chosen by the system can be performed in the Service UI under "Configuration / DICOM / General" item - first page.

Table 41 - Default AET Characteristics

Application Entity	Default AE Title	TCP/IP Port	
Verification SCU	STU_<hostname>	-	
Verification SCP		104 (standard) 2762 (TLS)	
Storage SCU		-	
Storage SCP		104 (standard) 2762 (TLS)	
Query/Retrieve SCU		-	
Query/Retrieve SCP		104 (standard) 2762 (TLS)	
Print SCU		PRI_<hostname>	-

Remote AE Titles

All external AE Titles have to be configured to be able to communicate with *syngo* X Workplace. For each remote AE the following data and capabilities can be configured:

Table 42 - Remote AE Configuration Items

Remote AE configuration item	Comment
Host Name	As defined in the network domain. This has to be configured also for any DICOM AE that wishes to connect to SCP services of <i>syngo</i> X Workplace.
TCP/IP address	As defined in the network domain. This has to be configured also for any DICOM AE that wishes to connect to SCP services of <i>syngo</i> X Workplace.
Logical Name	Name for the AE used in the user interfaces of the <i>syngo</i> X Workplace applications.
AE Title	AET, as provided by network administration
Port Number	Port Number, as provided by network administration
If Storage Service support is checked	
Transfer Syntax	Selection of uncompressed transfer Syntaxes supported by remote AE
Compression	Selection of additional compression Syntaxes supported for remote AE

Default Node	"first default"/"second default"/["no default"] - activating this feature will show "Send to <logical name>" in the Transfer tool menu for quick access.
Preference Node	When checked, the remote AE will be assigned to a keyboard shortcut key.
Archive Node	When checked, sending to remote AET will set status of a (rchived), else s (ent) is indicated.
Default Archive	When checked, the remote AE will be listed as default archive in User interfaces.
Graphics in Pixel Data	When checked, the DICOM overlay will not be encoded in attribute (60xx,3000) Overlay Data, but masked in the "unused bits" of the pixel data (only for uncompressed transfer syntaxes). For backwards compatibility with legacy AE.
Select SC node	Select a previously configured node as target for Storage Commitment when sending DICOM objects to the configured AE. Default is the same node as to which the Objects are sent.
Select SC AET	Select AET that corresponds to the above selected node that receives the Storage Commitment request. Default is the above specified "AE Title".
SC Result in same association	When checked the syngo X Workplace DICOM application will await the Storage Commitment N-EVENT-REPORT on the same association. Default is "not checked" (= different association).
SC result timeout	Timeout in hours and minutes to wait at the open association. Default: 01:00 (hour:minutes).
Encryption	When checked, secure transport connection is used for this AE.
If Storage Commitment Service support is checked	
n. a.	The related Storage Commitment configuration is either in the Storage section of the same AET or different AET (in case the current AET is only Storage Commitment Provider).
If Query Service support is checked	
provides DICOM Query model	The Query models supported by this AET can be selected. When possible, the STUDY ROOT model should preferably be configured
If Retrieve Service support is checked	
n. a.	Checking Retrieve support for an AET is the only needed configuration item. This will allow access to the "Import" feature in the Query result browser.
General	
Trusted Host	When checked, association is only accepted when pair of AET and TCP/IP address is known in the configuration.

4.4.2 Parameters

System parameters can be changed in the Service UI under "Configuration / DICOM / General" item - second page.

Table 43 - General parameter settings and timeouts

Time-out Values				
Parameter	Default Value[sec]	Min [sec]	Max [sec]	Comment
Accepting/Rejecting an Association Request	60	15	600	Wait for an Association Request or wait for a Peer to shut down the Association
Association Open Request	60	15	600	Wait for a reply to an Association Accept Request
Association Close Request	60	15	600	Wait for a reply to an Association Release Request
Accepting a Message over Network	60	15	600	Wait for a Network Write to be accepted
Waiting for Data between TCP/IP Packets	60	15	600	Wait for Data between TCP/IP packets
Response from Remote Node for Storage/Query/Retrieve	600	15	3600	Time between Service Request and Service Response
Accept network connect	60	15	600	Wait for a network connect
General Transfer Setting				

Simultaneous DICOM associations	10	1	10	Number of simultaneous associations running.
Maximum PDU Size	528378 bytes	4kByte	1MByte	Proposed PDU size, each selectable value is doubled from previous, starting with 4kB. Additionally, for optimization for some networks 28kByte are provided.

5 Media Interchange

5.1 Implementation Model

5.1.1 Application Data Flow Diagram

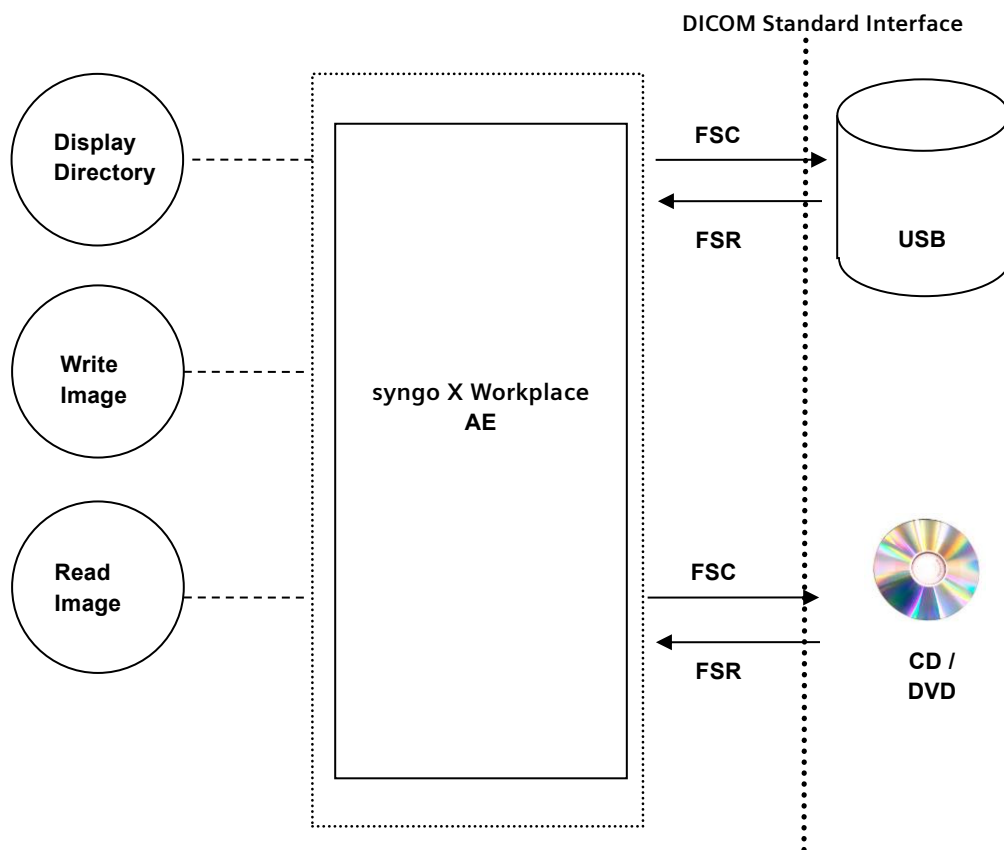


Figure 3: Media Interchange Application Data Flow Diagram

The syngo X Workplace provides the functionality to Import or Export DICOM Instances from and to the File System. During export, a DICOMDIR may also be generated (user selection). A complete ISO Image ready-to-burn can also be generated. All SOP Classes defined in Table 1 are supported for the Import/Export functionality

5.1.2 Functional Definitions of AEs

The syngo X Workplace application is capable of

- creating a new File-set in the File System (Export to ...)
- importing SOP Instances from the medium onto local storage
- writing the File-sets DICOMDIR information into the file system and joining it to an ISO image.

5.1.3 Sequencing of Real-World Activities

Whenever data is written to an external media, syngo X Workplace creates a DICOMDIR from the selected data and creates an ISO image of the selected data on the local hard disk. Depending on the selected data and options (selected media size, with or without compression) either General Purpose CD profile or DVD-J2K profile are used.

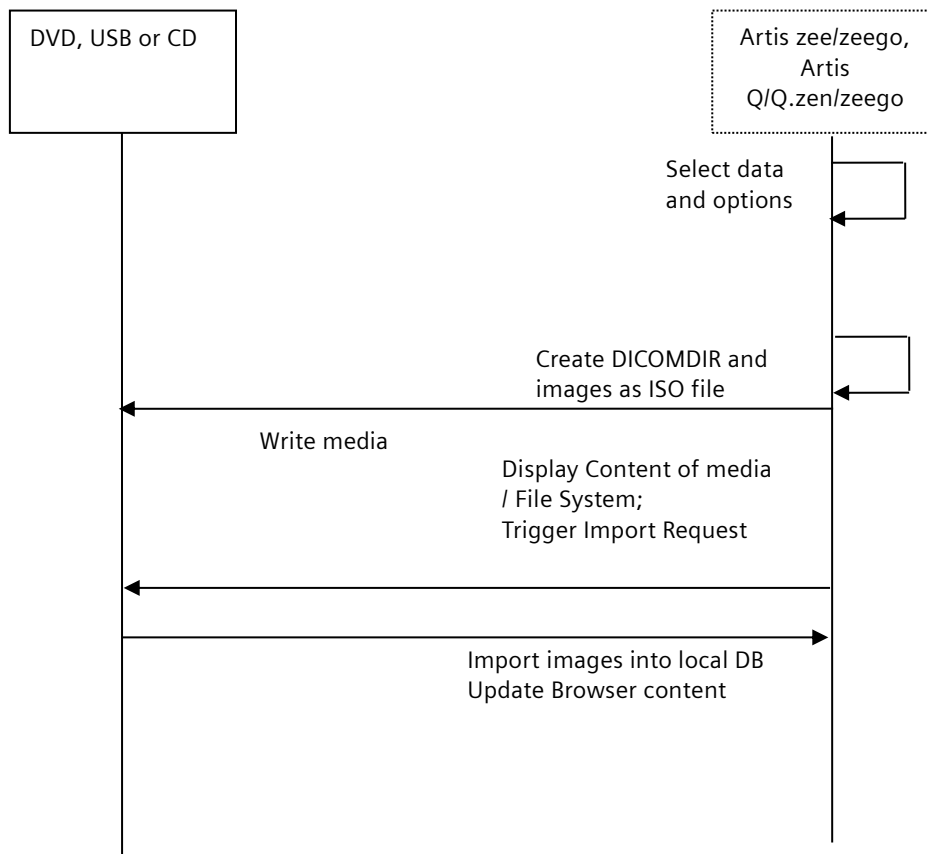


Figure 4: Sequence diagram – Media creation

5.1.4 File Meta Information for Implementation Class and Version

This section describes the values assigned to the File Meta Information attributes (see part PS 3.10) that pertain to the Implementation Class and Version. The implementation Class UID and the Implementation Version name in the File Meta Header are the same as the values specified for networking.

Table 44: Implementation Class/Version Name - Media Interchange

File Meta Information Version	0001
Implementation Class UID	1.3.12.2.1107.5.4.7
Implementation Version Name	"SIEMENSXLEOVD3"

5.2 AE Specifications

5.2.1 Media Storage AE – Specification

The syngo X Workplace provides conformance to the following Application Profiles as an FSC as well as an FSR. The FSU role is only supported only on a non-optical storage device (e.g. USB stick).

Table 45: Media - Application Profiles and Real-World Activities

Application Profiles Supported	Real-World Activity	Role	Service Class Option
STD-GEN-CD	Browse Directory Information Import into Application Export to local Archive Media	FSR , FSC , FSU	Interchange
STD-GEN-DVD			
STD-GEN-DVD-JPEG			
STD_GEN-BD			

5.2.1.1 Real-World Activities

5.2.1.1.1 Activity “Browse Directory Information”

The syngo X Workplace acts as FSR using the interchange option when requested to read the media directory.

The syngo X Workplace will read the DICOMDIR and insert those directory entries that are valid for the application profiles supported, into a local database. The database then is used for browsing media contents.

Note: The “Icon Image Sequence” is also supported in DICOMDIR. But only those Icon Images with “Bits Allocated” (0028,0100) equal to 8 and size of 64x64 or 128x128 pixels are imported into database and are visible in the Browser.

5.2.1.1.2 Real World Activity “Import into Application”

The syngo X Workplace application acts as FSR using the interchange option when requested to read SOP Instances from the medium into the application.

The SOP Instance selected from the media directory will be copied into the running Application. Only SOP Instances, that are valid for the application profile supported and supported by syngo X Workplace, can be retrieved from media.

5.2.1.1.3 Real-World Activity “Export to local Archive Media”

The syngo X Workplace application acts as FSU (for media with existing DICOM file-set) or FSC (media not initialized) using the interchange option when requested to copy SOP Instances from the local storage to local Archive Medium. The activity as FSU is only possible as long as the local burning SW of syngo X Workplace has not already processed the generated ISO file.

The syngo X Workplace application will receive a list of SOP Instances to be copied to the local archive medium. Depending on the profile selected (Standard: uncompressed, with DICOMDIR; Patient: compressed with DICOMDIR) the SOP Instances will be taken, and an ISO file is being generated that includes the DICOMDIR and the corresponding objects.

It is then up to syngo X Workplace local configuration (if equipped with a local media burner) to burn the ISO file to the appropriate media.

5.2.1.2 SOP Classes and Transfer Syntaxes

These Application Profiles are based on the Media Storage Service Class with the Interchange Option. The syngo X Workplace provides Standard Conformance to the SOP Classes listed in "Table 1 - Network Services" section "SOP Classes Created by the syngo X Workplace" and "SOP Classes Managed by the syngo X Workplace" in the "Conformance Statement Overview".

Using the Application Profiles supporting compression (STD-GEN-xxx) the following Transfer Syntaxes are supported:

Table 46: Transfer Syntaxes for STD-GEN-xxx

UID value	Transfer Syntax	Image Objects
1.2.840.10008.1.2.1	Explicit Value Representation Little Endian native	yes
1.2.840.10008.1.2.4.50	JPEG Baseline (Process 1) lossy compressed	yes
1.2.840.10008.1.2.4.51	JPEG Extended (Process 2 & 4) lossy compressed	yes
1.2.840.10008.1.2.4.70	JPEG Lossless, Non-Hierarchical, First-Order Prediction (Process 14) lossless compressed	yes

5.3 Augmented and Private Application Profiles

n.a.

5.4 Media Configuration

5.4.1 Single- / Multi-Session CD burning

Please refer to most recent Service / Configuration documentation of syngo X Workplace for changing between the single-session and multi-session recording modes.

5.4.2 "Viewer on CD"

Please refer to most recent Service / Configuration documentation of syngo X Workplace for changing between the

ACOM.PC Lite 2.0 or **syngo FastView**

as application that is included onto the medium as part of the "Viewer on CD" feature, if the feature is checked in the Media Creation user interface (see also next configuration item).

5.4.3 Auto-Labeling

Please refer to most recent Service / Configuration documentation of syngo X Workplace for activating the auto-labeling of CD media to avoid the label inquiry dialog when using automatic media export. The auto-labeling can be activated with the "Viewer on CD" feature being implicitly checked or not.

6 Support of Extended Character Sets

The syngo X Workplace DICOM application supports the following character sets as defined in the four tables below:

Table 47 - Supported Single-Byte Character Sets (w/o Code Ext.)

Character Set Description	Defined Term	ISO registration number	Character Set
Default repertoire	none	ISO_IR 6	ISO 646:
Latin alphabet No. 1	ISO_IR 100	ISO_IR 100	Supplementary set
		ISO_IR 6	ISO 646:
Latin alphabet No. 2	ISO_IR 101	ISO_IR 101	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 3	ISO_IR 109	ISO_IR 109	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 4	ISO_IR 110	ISO_IR 110	Supplementary set
		ISO_IR 6	ISO 646
Cyrillic	ISO_IR 144	ISO_IR 144	Supplementary set
		ISO_IR 6	ISO 646
Arabic	ISO_IR 127	ISO_IR 127	Supplementary set
		ISO_IR 6	ISO 646
Greek	ISO_IR 126	ISO_IR 126	Supplementary set
		ISO_IR 6	ISO 646
Hebrew	ISO_IR 138	ISO_IR 138	Supplementary set
		ISO_IR 6	ISO 646
Latin alphabet No. 5	ISO_IR 148	ISO_IR 148	Supplementary set
		ISO_IR 6	ISO 646
Japanese	ISO_IR 13	ISO_IR 13	JIS X 0201: Katakana
		ISO_IR 14	JIS X 0201: Romaji

Table 48 - Supported Single-Byte Character Sets (with Code Ext.)

Character Set Description	Defined Term	Standard for Code Extension	ESC sequence	ISO registration number	Character Set
Default repertoire	ISO 2022 IR 6	ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.1	ISO 2022 IR 100	ISO 2022	ESC 02/13 04/01	ISO-IR 100	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.2	ISO 2022 IR 101	ISO 2022	ESC 02/13 04/02	ISO-IR 101	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.3	ISO 2022 IR 109	ISO 2022	ESC 02/13 04/03	ISO-IR 109	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646
Latin alphabet No.4	ISO 2022 IR 110	ISO 2022	ESC 02/13 04/04	ISO-IR 110	Supplementary set
		ISO 2022	ESC 02/08 04/02	ISO-IR 6	ISO 646

Table 49 - Supported Multi-Byte Character Sets (w/o Code Ext.)

Character Set Description	Defined Term	ISO registration number	Character Set
Unicode	ISO_IR 192	ISO 10646	Unicode in UTF-8
Chinese	GB18030	GB18030	GB 18030-2000 (China Association for Standardization)

Table 50 - Supported Multi-Byte Character Sets (with Code Ext.)

Character Set	Defined Term	Standard for	ESC sequence	ISO registra-	Character Set
---------------	--------------	--------------	--------------	---------------	---------------

Description		Code Extension		tion number	
Japanese	ISO 2022 IR 87	ISO 2022	ESC 02/04 04/02	ISO-IR 87	JIS X 0208: Kanji
	ISO 2022 IR 159	ISO 2022	ESC 02/04 02/08 04/04	ISO-IR 159	JIS X 0212: Supplementary Kanji set
Chinese ⁸	ISO 2022 IR 58	ISO 2022	ESC 02/04 04/01	ISO-IR 58	GB2312-80 (China Association for Standardization)

All Special Character Sets (SCS) listed above are supported for incoming Data. When creating new Instances, the system will use the default SCS (or SCS List) configured on the machine.

When there is a mismatch between the given character set in attribute (0008,0005) and the characters in an IOD received by the system, then the following measures are taken to make the characters DICOM conform:

- Convert each illegal character to a '?'.

There are three categories of character sets which have to be differentiated because of their different encoding formats:

- Conventional ISO character sets: ISO_IR 6, ISO 2022 IR 6, ISO_IR 100, etc.
→ encoded in ISO 2022
- ISO IR_192 → encoded in UTF-8
- GB18030 → encoded in GB18030

It is not possible to recognize the following mismatches automatically on receiving or importing:

- An attribute value is encoded in ISO_IR 192 ← → (0008,0005) contains a conventional ISO character set as primary character set.
- An attribute value is encoded in GB18030 ← → (0008,0005) contains a conventional ISO character set as primary character set.
- An attribute value is encoded in ISO 2022 ← → (0008,0005) contains ISO_IR 192.
- An attribute value is encoded in ISO 2022 ← → (0008,0005) contains GB18030

An IOD that contains one of the above-mentioned inconsistencies is not DICOM conform. As these kinds of inconsistencies cannot be recognized by the system, the IOD will not be rejected but the character data might be corrupted.

The syngo X Workplace supports Kanji characters in the byte zones after 74 (79, 7A, 7B and 7C).

7 Security

7.1 Security Profile

The syngo X Workplace DICOM application conforms to the IHE Basic Security Integration Profile that is used for the DICOM Communication.

It allows the use of either a conventional (non-secure) DICOM communication or a secure DICOM communication. For secure DICOM communication the application uses Transport Layer Protocol (TLS v1.1 and TLS v1.2). Following features are supported for the secure DICOM communication. The port in which the application acts as SCP for secure DICOM communication is 2762 (fixed). The port in which the application acts as SCP for unsecure DICOM communication is 104 (fixed).

The following security profile are done in syngo X Workplace DICOM application using TLS protocols

- Secure authentication of node

⁸ Note: This Character Set is an extension of DICOM for the Chinese language.

- Integrity and confidentiality of transmitted data.
- Generation of audit trail records access control and user authentication.

7.1.1 Security Transport Connection Profiles

The syngo X Workplace DICOM application conforms to the Basic TLS Transport Connection Profile.

The syngo X Workplace DICOM application initiates the TLS connections and accepts TLS connections with Storage commitment. It provides a configuration panel by which local systems can configure the certificate that needs to bind for DICOM communication. Secure communication is a “mode of operation” supported by the implementation of the DICOM Basic TLS Secure Transport Connection Profile. This functionality will be used by the nodes that can authenticate each other before they exchange DICOM information. For secure communication the TLS protocol is used which provides message authentication, integrity and confidentiality. The application supports the following protocol versions TLS Protocol v1.1 and v1.2.

The syngo X Workplace DICOM application supports X.509 certificates. The type of X.509 certificates that are supported are:

- 1) Self-Signed certificate
- 2) Certificate for which chain building (Trusted chain building, Trusted CA) is possible.

The following TLS certification checks will be done (TLS Handshake). The machine (either server or client) that will send its certificate will :

- Choose the certificate according to Common Name (CN), if the local self-signed is used. If customer specific certificate needs to be used, then Serial Number of the certificate is used for choosing the certificate.

The server verifies

- that the client certificate is X.509 certificate which is not tampered with
- that the client certificate is in the list of trusted certificates (Trust Chain Building)
- that the client certificate is not in the revoked list.
- that the client certificate is not expired (present time is between “Valid From” and “Valid To” fields of X.509 certificate)
- that the client certificate has the correct purpose (at least the client authentication purpose).

The client verifies

- that the server certificate is a X.509 certificate which is not tampered with
- that the server certificate is in the list of trusted certificates (Trust Chain Building)
- that the server certificate is not in the revoked list.
- that the server certificate is not expired (present time is between “Valid From” and “Valid To” fields of X.509 certificate)
- that the server certificate has the correct purpose (at least the server authentication purpose).

In addition, the following validation is done:

- 1) ‘Direct certificate validation’ for self-signed certificate, i. e. the self-signed certificate of the remote node must be present in the ‘Trusted Root Certificate’ StoreCertificate received from peer have multiple X.509 certificates within the TLS Handshake.

- 2) syngo X Workplace DICOM application can receive X.509 certificate chain(Full certificate chain, Partial certificate chain or only End certificate) in the TLS handshake from peer. For all the cases for successful Trust chain Building all the certificates shall be installed in the Windows certificate Store of the Local Machine. i.e. All The intermediate must be imported to Intermediate Certificate Authorities→Certificates and the root certificate must be imported to the Trusted Root Certificates→Certificates.

The X.509 certificate imported and used for DICOM communication

- 1) must have purpose set for Client and Server Authentication.
- 2) must be exportable to generate the certificate file and private key file.

If intermediate and root X.509 certificates are present, then the intermediate certificate must be imported to Intermediate Certificate Authorities→Certificates. The root certificate must be imported to the Trusted Root Certificates→Certificates.

The syngo X Workplace DICOM application communicates with either of the following Cipher suites for encrypting the data send across the network.

TLS_RSA_WITH_AES_128_CBC_SHA

TLS_RSA_WITH_3DES_EDE_CBC_SHA

Note: Support for NULL Cipher (TLS_RSA_WITH_NULL_SHA) is not there. The secure communication is FIPS mode enabled

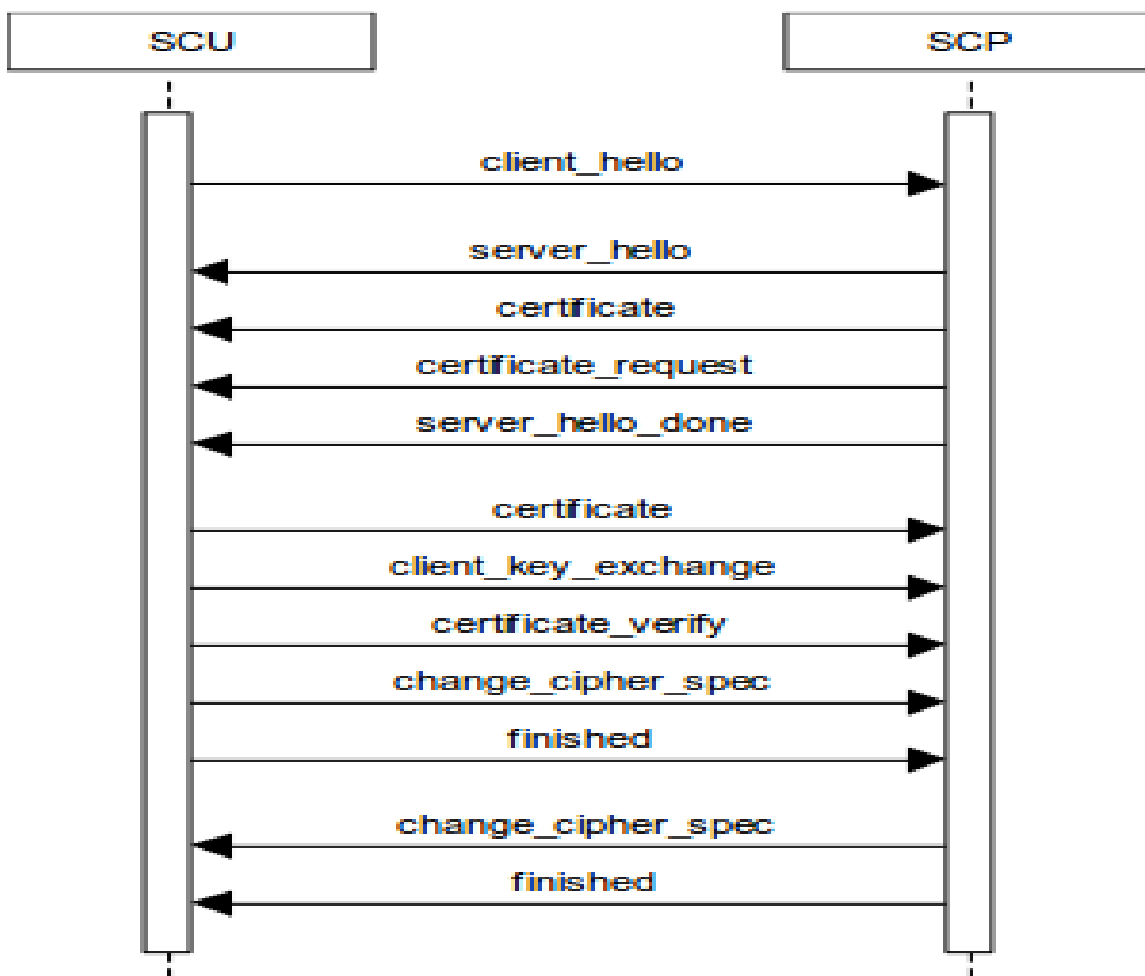


Figure 5: TLS Handshake Message Protocol

7.2 Application Level Confidentiality Profile

Application Level Confidentiality Profiles address the following aspects of security *Data Confidentiality at the application layer*.

These Profiles are targeted toward creating a special purpose, de-identified version of an already existing Data Set. This profile is not intended to replace the original SOP Instance from which the de-identified SOP Instance is created. The de-identified SOP Instances are useful, for example, in creating teaching or research files, performing clinical trials, or submission to registries where the identity of the patient and other individuals is required to be protected.

7.2.1 Anonymization workflow (De-identifier)

syngo provides a functionality to export the DICOM data to configured offline directories (Local Path / Network path / USB). The data exported can be exported anonymous where the Patient Identification parameters like Patient Name, Patient ID etc., are removed or replaced as per the table below.

Table 51: Application Level Confidentiality Profile attributes (standard tags)

DICOM Tag	Attribute Name	Anonymized
(0002,0003)	Media Storage SOP Instance UID	Yes
(0008,0014)	Instance Creator UID	Yes
(0008,0018)	SOP Instance UID	Yes
(0008,0050)	Accession Number	Yes
(0008,0080)	Institution Name	Yes
(0008,0081)	Institution Address	Yes
(0008,0090)	Referring Physician's Name	Yes
(0008,0092)	Referring Physician's Address	Yes
(0008,0094)	Referring Physician's Telephone Numbers	Yes
(0008,1010)	Station Name	Yes
(0008,1030)	Study Description	Yes
(0008,103E)	Series Description	Yes
(0008,1040)	Institutional Department Name	Yes
(0008,1048)	Physician(s) of Record	Yes
(0008,1050)	Performing Physicians' Name	Yes
(0008,1060)	Name of Physician(s) Reading Study	Yes
(0008,1070)	Operators' Name	Yes
(0008,1080)	Admitting Diagnoses Description	Yes
(0008,1120)	Referenced Patient Sequence	Yes
(0008,1155)	Referenced SOP Instance UID	Yes
(0008,1250)	Related Series Sequence	Yes
(0008,2111)	Derivation Description	Yes
(0010,0010)	Patient's Name	Yes
(0010,0020)	Patient ID	Yes
(0010,0030)	Patient's Birth Date	Yes
(0010,0032)	Patient's Birth Time	Yes
(0010,0040)	Patient's Sex	Yes
(0010,1000)	Other Patient IDs	Yes
(0010,1001)	Other Patient Names	Yes
(0010,1005)	Patient's Birth Name	Yes
(0010,1010)	Patient's Age	Yes
(0010,1020)	Patient's Size	Yes
(0010,1030)	Patient's Weight	Yes
(0010,1040)	Patient Address	Yes
(0010,1060)	Patient's Mother's Birth Name	Yes
(0010,1090)	Medical Record Locator	Yes
(0010,2154)	Patient's Telephone Numbers	Yes
(0010,2160)	Ethnic Group	Yes
(0010,2180)	Occupation	Yes
(0010,2180)	Additional Patient's History	Yes
(0010,4000)	Patient Comments	Yes

DICOM Tag	Attribute Name	Anonymized
(0018,1000)	Device Serial Number	Yes
(0018,1030)	Protocol Name	Yes
(0020,000D)	Study Instance UID	Yes
(0020,000E)	Series Instance UID	Yes
(0020,0010)	Study ID	Yes
(0020,0052)	Frame of Reference UID	Yes
(0020,0200)	Synchronization Frame of Reference UID	Yes
(0020,4000)	Image Comments	Yes
(0040,0275)	Request Attributes Sequence	Yes
(0040,A124)	UID	Yes
(0040,A730)	Content Sequence	Yes
(0088,0140)	Storage Media File-set UID	Yes
(3006,0024)	Referenced Frame of Reference UID	Yes
(3006,00C2)	Related Frame of Reference UID	Yes

8 Annexes

8.1 IOD Contents

8.1.1 Created SOP Instances

8.1.1.1 Common Modules

8.1.1.1.1 Supported attributes on Patient level

Table 52 – Patient level attributes

Attribute Name	Tag
Referenced Patient Sequence	(0008,1120)
>Referenced SOP Class UID	(0008,1150)
>Referenced SOP Instance UID	(0008,1155)
Patient's Name	(0010,0010)
Patient ID	(0010,0020)
Patient's Birth Date	(0010,0030)
Patient's Sex	(0010,0040)
Other Patient IDs	(0010,1000)
Other Patient Names	(0010,1001)
Other Patient IDs Sequence	(0010,1002)
>Patient ID	(0010,0020)
>Issuer of Patient ID	(0010,0021)
>Type of Patient ID	(0010,0022)
Ethnic Group	(0010,2160)
Patient Comments	(0010,4000)

8.1.1.1.2 Supported attributes on Study level

Table 53 – Study level attributes

Attribute Name	Tag
Study Date	(0008,0020)
Study Time	(0008,0030)
Accession Number	(0008,0050)
Referring Physician's Name	(0008,0090)
Study Description	(0008,1030)
Procedure Code Sequence	(0008,1032)
>Code Value	(0008,0100)
>Coding Scheme Designator	(0008,0102)
>Coding Scheme Version	(0008,0103)
>Code Meaning	(0008,0104)
Physician(s) of Record	(0008,1048)
Admitting Diagnoses Description	(0008,1080)
Referenced Study Sequence	(0008,1110)

Attribute Name	Tag
>Referenced SOP Class UID	(0008,1150)
>Referenced SOP Instance UID	(0008,1155)
Patient's Age	(0010,1010)
Patient's Size	(0010,1020)
Patient's Weight	(0010,1030)
Occupation	(0010,2180)
Additional Patient History	(0010,2180)
Study Instance UID	(0020,000D)
Study ID	(0020,0010)

8.1.1.2 SC Standard Extended SOP Class

The syngo X Workplace Workstation will create functional images from special applications. Those will be encoded as SC Standard extended SOP Class. Please see the following tables for a complete overview of supplied Type 1/2/3 Standard and Private attributes.

8.1.1.2.1 Composing Result Image

Table 54 - SC Derived Image (Monochrome) from Composing

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	(conf. Character Set is added, if needed)
Image Type	(0008,0008)	DERIVED\SECONDARY\\<algorithm>\<SW version> algorithm = SPINE or COLON or LLEG_ORTHO or LLEG_ANGIO or SPINE DLR or LLEG_ORTHO DLR or SPINE FD or LLEG_ORTHO FD or SPINE OSD or LLEG_ORTHO OSD
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	Derived from original Acquisition/Content Date or <zero length>
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.fffff>
Acquisition Time	(0008,0032)	Derived from original Acquisition/Content Time or <zero length>
Content Time	(0008,0033)	<hhmmss.fffff>
Modality	(0008,0060)	OT
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	(see [0008,0008] 3rd value <algorithm>)
Institutional Department Name	(0008,1040)	from WS configuration
Performing Physician's Name	(0008,1050)	input via "Correct" user interface possible
Manufacturer's Model Name	(0008,1090)	syngoXWP

Attribute Name	Tag	Value
Derivation Description	(0008,2111)	<algorithm> (see [0008,0008])
Device Serial Number	(0018,1000)	from WS Configuration
Secondary Capture Device ID	(0018,1010)	from WS Configuration
Date of Secondary Capture	(0018,1012)	<yyyymmdd>
Time of Secondary Capture	(0018,1014)	<hhmmss.fffff>
Secondary Capture Device Manufacturer	(0018,1016)	"Siemens"
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	"LEONARDO"
Secondary Capture Device Software Version	(0018,1019)	from WS Configuration
Software Versions	(0018,1020)	from WS Configuration
Protocol Name	(0018,1030)	same as Series Description
Series Instance UID	(0020,000E)	
Series Number	(0020,0011)	
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	<zero length>
Laterality	(0020,0060)	<removed>
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME1 or MONOCHROME2
Rows	(0028,0010)	(defined by the number of original images used and the overlap by reconstruction algorithm)
Columns	(0028,0011)	from Original
Pixel Spacing	(0028,0030)	from Calibration, only for "stepping" images
Bits Allocated	(0028,0100)	from Original
Bits Stored	(0028,0101)	from Original
High Bit	(0028,0102)	from Original
Pixel Representation	(0028,0103)	0
Pixel Spacing Calibration Type	(0028,0A02)	only when (0028,0030) exists
Pixel Spacing Calibration Description	(0028,0A04)	only when (0028,0030) exists
Window Center	(0028,1050)	
Window Width	(0028,1051)	
Window Center & Width Explanation	(0028,1055)	
Study Comments	(0032,4000)	from Original
Overlay Rows	(60xx,0010)	
Overlay Columns	(60xx,0011)	
Overlay Description	(60xx,0022)	
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0050)	111
Overlay Bits Allocated	(60xx,0100)	same as (0028,0100) or 1 (if Overlay encoded in [60xx,3000])
Overlay Bit Position	(60xx,0102)	12 or 0 (if Overlay encoded in [60xx,3000])
Overlay Data	[60xx,3000]	Graphics Overlay
Pixel Data	(7FE0,0010)	

8.1.1.2.2 Captured Projection Image

Table 55 - SC Derived Image (RGB) from 3D Projections

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	DERIVED\SECONDARY\OTHER\IAE_PRJ <Filter_Type> <Filter_Type> values: MPR MIP MINIP VRT OVERVIEW
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.ffffff>
Instance Creator UID	(0008,0014)	<implementation_class_uid>.<individual_id>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	from Original
Content Date	(0008,0023)	<yyyymmdd>
Acquisition DateTime	(0008,002A)	from Original
Series Time	(0008,0031)	<hhmmss.ffffff>
Acquisition Time	(0008,0032)	from Original
Content Time	(0008,0033)	<hhmmss.ffffff>
Modality	(0008,0060)	OT or XA or CT (default = OT, can be configured)
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	from Original
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	
Institutional Department Name	(0008,1040)	from WS Configuration
Performing Physician's Name	(0008,1050)	from Original / input via "Correct" possible
Operator's Name	(0008,1070)	from Original
Manufacturer's Model Name	(0008,1090)	from Original
Related Series Sequence	(0008,1250)	from Original
>Study Instance UID	(0020,000D)	from Original
>Series Instance UID	(0020,000E)	from Original
>Purpose of Reference Code Sequence	(0040,A170)	<zero length>
Derivation Description	(0008,2111)	from Original
Source Image Sequence	(0008,2112)	if derived from single image
Body Part Examined	(0018,0015)	from Original
Device Serial Number	(0018,1000)	from Original
Secondary Capture Device ID	(0018,1010)	from WS Configuration
Date of Secondary Capture	(0018,1012)	<yyyymmdd>
Time of Secondary Capture	(0018,1014)	<hhmmss.ffffff>

Attribute Name	Tag	Value
Secondary Capture Device Manufacturer	(0018,1016)	"Siemens"
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	from WS Configuration
Secondary Capture Device Software Version	(0018,1019)	from WS Configuration
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	"Radial Ranges", "Parallel Ranges", "Curved Ranges" or from Original
Patient Position	(0018,5100)	from Original
Series Instance UID	(0020,000E)	
Series Number	(0020,0011)	970
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	n-m (n, m >0) 0 for reference image
Patient Orientation	(0020,0020)	from original (derived from single image) or calculated or <zero length> (derived from multiple images).
Images in Acquisition	(0020,1002)	from Original
Image Comments	(0020,4000)	from Original if derived from single image
Samples per Pixel	(0028,0002)	3
Photometric Interpretation	(0028,0004)	RGB
Planar Configuration	(0028,0006)	0
Rows	(0028,0010)	
Columns	(0028,0011)	
Pixel Spacing	(0028,0030)	If image has been calibrated
Bits Allocated	(0028,0100)	8
Bits Stored	(0028,0101)	8
High Bit	(0028,0102)	7
Pixel Representation	(0028,0103)	0
Burned In Annotation	(0028,0301)	YES, if set to YES in Original or if any text flag is set to "On". Not set otherwise.
Pixel Spacing Calibration Type	(0028,0A02)	from Original
Pixel Spacing Calibration Description	(0028,0A04)	from Original
Lossy Image Compression	(0028,2110)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Performed Protocol Code Sequence	(0040,0260)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason For The Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original

Attribute Name	Tag	Value
Pixel Data	(7FE0,0010)	

8.1.1.2.3 Bookmarks

Table 56 - SC Derived Image (RGB) for 4D Viewer Bookmarks

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	DERIVED\SECONDARY\OTHER\IAE_BOOKMARK
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.fffff>
Instance Creator UID	(0008,0014)	<implementation_class_uid>.<individual_id>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	from Original
Content Date	(0008,0023)	<yyyymmdd>
Acquisition DateTime	(0008,002A)	from Original
Series Time	(0008,0031)	<hhmmss.fffff>
Acquisition Time	(0008,0032)	from Original
Content Time	(0008,0033)	<hhmmss.fffff>
Modality	(0008,0060)	XA
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	from Original
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	
Institutional Department Name	(0008,1040)	from WS Configuration
Performing Physician's Name	(0008,1050)	from Original / input via "Correct" possible
Operator's Name	(0008,1070)	from Original
Manufacturer's Model Name	(0008,1090)	from Original
Related Series Sequence	(0008,1250)	from Original
>Study Instance UID	(0020,000D)	from Original
>Series Instance UID	(0020,000E)	from Original
>Purpose of Reference Code Sequence	(0040,A170)	<zero length>
Derivation Description	(0008,2111)	from Original
Source Image Sequence	(0008,2112)	If derived from single image
Device Serial Number	(0018,1000)	from Original
Secondary Capture Device ID	(0018,1010)	from WS Configuration
Date of Secondary Capture	(0018,1012)	<yyyymmdd>
Time of Secondary Capture	(0018,1014)	<hhmmss.fffff>
Body Part Examined	(0018,0015)	from Original
Secondary Capture Device Manufacturer	(0018,1016)	"Siemens"

Attribute Name	Tag	Value
Secondary Capture Device Manufacturer's Model Name	(0018,1018)	from WS Configuration
Secondary Capture Device Software Version	(0018,1019)	from WS Configuration
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	
Patient Position	(0018,5100)	from Original
Private Creator	(0019,00xx)	"SIEMENS SMS-AX IAE"
Bookmark_XML_File	(0019,xx00)	XML structure
Series Instance UID	(0020,000E)	
Series Number	(0020,0011)	980
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	1 - n
Patient Orientation	(0020,0020)	From original (derived from single image) or calculated or <zero length> (derived from multiple images).
Images in Acquisition	(0020,1002)	from Original
Image Comments	(0020,4000)	from Original if derived from single image
Samples per Pixel	(0028,0002)	3
Photometric Interpretation	(0028,0004)	RGB
Planar Configuration	(0028,0006)	0
Rows	(0028,0010)	
Columns	(0028,0011)	
Bits Allocated	(0028,0100)	8
Bits Stored	(0028,0101)	8
High Bit	(0028,0102)	7
Pixel Representation	(0028,0103)	0
Burned In Annotation	(0028,0301)	YES, if set to YES in Original or if any text flag is set to "On". Not set otherwise.
Pixel Spacing Calibration Type	(0028,0A02)	from Original
Pixel Spacing Calibration Description	(0028,0A04)	from Original
Lossy Image Compression	(0028,2110)	from Original
Private Creator	(0029,00xx)	"SIEMENS MEDCOM HEADER"
Application Header Sequence	(0029,xxxx)	private bookmark data
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Performed Protocol Code Sequence	(0040,0260)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason For The Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original
Pixel Data	(7FE0,0010)	Representative image of image icon.

8.1.1.2.4 EP Segmentation Path Objects

The Segmentation application may create an SC Image (RGB) to contain the Segmentation results for use in a specific workflow only.

The content is only useful in this context and therefore the DICOM content is “tailored” for this special use. It can be identified with the help of the following attributes:

(0008,0008) Image Type is set to “DERIVED\SECONDARY\IINSPACE_EP_SEGMI<SW-Version>”.

(0008,0016) SOP Class UID is set to “1.2.840.10008.5.1.4.1.1.7”.

(0008,103E) Series Description is set to “EP_Segm_<object label>” or “EP_Segm_<object id>”.

8.1.1.2.5 Stored iFlow Images

Table 57 - SC Derived Image (RGB) from iFlow

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	DERIVED\SECONDARY\SINGLE PLANE\SINGLE AI SECONDARY CAPTURE
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.7
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	<yyyymmdd> (set from oldest acquisition or Content Date of input images, if available)
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.ffffff>
Acquisition Time	(0008,0032)	<hhmmss.ffffff> (set from oldest acquisition or image time of input images, if available)
Content Time	(0008,0033)	<hhmmss.ffffff>
Modality	(0008,0060)	from Original
Conversion Type	(0008,0064)	WSD
Manufacturer	(0008,0070)	“Siemens”
Institution Name	(0008,0080)	from WS Configuration
Station Name	(0008,1010)	from Original
Series Description	(0008,103E)	from user input
Performing Physician’s Name	(0008,1050)	from Original
Manufacturer’s Model Name	(0008,1090)	from Original
Referenced Image Sequence	(0008,1140)	Reference to Original (XA multi-frame)
Device Serial Number	(0018,1000)	from Original
Secondary Capture Device ID	(0018,1010)	from WS Configuration
Date of Secondary Capture	(0018,1012)	<yyyymmdd> (same as Content Date)
Time of Secondary Capture	(0018,1014)	<hhmmss.ffffff> (same as Content Time)
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	from Original
Patient Position	(0018,5100)	from Original

Attribute Name	Tag	Value
Series Instance UID	(0020,000E)	1.3.12.2.1107.5.4.7.serialnumber.<individual_uid>
Series Number	(0020,0011)	next available series number, if stored into local database
Instance Number	(0020,0013)	always "1"
Patient Orientation	(0020,0020)	from Original
Laterality	(0020,0060)	from Original
Samples per Pixel	(0028,0002)	3
Photometric Interpretation	(0028,0004)	RGB
Planar Configuration	(0028,0006)	0
Rows	(0028,0010)	1024
Columns	(0028,0011)	1024
Bits Allocated	(0028,0100)	8
Bits Stored	(0028,0101)	8
High Bit	(0028,0102)	7
Pixel Representation	(0028,0103)	0
Window Center	(0028,1050)	2047
Window Width	(0028,1051)	4095
Requesting Physician	(0032,1032)	from Original
Requested Procedure Description	(0032,1060)	from Original
Study Comments	(0032,4000)	from Original
Special Needs	(0038,0050)	from Original
Patient State	(0038,0500)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Confidentiality Constraint on Patient Data Description	(0040,3001)	from Original
Pixel Data	(7FE0,0010)	

8.1.1.3 XA Standard Extended SOP Class

The syngo X Workplace system will create "screen-shots" (Store Monitor images) from the Angio Viewer application. Those will be encoded as XA Standard extended SOP Class. The Angio Viewer only creates XRF images, if this IOD type is base for viewing. Please see the following table for complete overview of supplied Type 1/2/3 Standard and Private attributes:

8.1.1.3.1 Angio Viewer "Store Monitor" Image

Table 58 - XA/XRF Derived Image (Monochrome) Store Monitor

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	(conf. Character Set is added, if needed)

Attribute Name	Tag	Value
Image Type	(0008,0008)	DERIVED\SECONDARY\SINGLE PLANE\SINGLE A(B)\STORE MONITOR
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.12.1 or 1.2.840.10008.5.1.4.1.1.12.2
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	from Original
Acquisition Date	(0008,0022)	Derived from original Acquisition/Content Date or <zero length>
Content Date	(0008,0023)	<yyyymmdd> (date of creation)
Series Time	(0008,0031)	from Original
Acquisition Time	(0008,0032)	Derived from original Acquisition/Content Time or <zero length>
Content Time	(0008,0033)	<hhmmss.ffffff> (time of creation)
Modality	(0008,0060)	XA
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from Original
Institution Address	(0008,0081)	from Original
Station Name	(0008,1010)	from Original
Series Description	(0008,103E)	from Original
Institutional Department Name	(0008,1040)	from Original
Performing Physician's Name	(0008,1050)	input via "Correct" user interface possible
Manufacturer's Model Name	(0008,1090)	from Original
Contrast Bolus Agent	(0018,0010)	from Original
KVP	(0018,0060)	from Original
Device Serial Number	(0018,1000)	from Original
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	from Original
Contrast/Bolus Ingredient	(0018,1048)	from Original
Distance Source to Detector	(0018,1110)	from Original
Distance Source to Patient	(0018,1111)	from Original
Estimated Radiographic Magnification Factor	(0018,1114)	from Original
Exposure Time	(0018,1150)	from Original
X-Ray Tube Current	(0018,1151)	from Original
Average Pulse Width	(0018,1154)	from Original
Radiation Setting	(0018,1155)	from Original
Radiation Mode	(0018,115A)	from Original
Image Area Dose Product	(0018,115E)	from Original
Intensifier Size	(0018,1162)	from Original
Imager Pixel Spacing	(0018,1164)	from Original
Grid	(0018,1166)	from Original
Column Angulation	(0018,1450)	from Original (XRF image only)
Tomo Layer Height	(0018,1460)	from Original (XRF image only)
Tomo Angle	(0018,1470)	from Original (XRF image only)
Tomo Time	(0018,1480)	from Original (XRF image only)
Positioner Motion	(0018,1500)	from Original (XA image only)
Positioner Primary Angle	(0018,1510)	from Original (XA image only)
Positioner Secondary Angle	(0018,1511)	from Original (XA image only)

Attribute Name	Tag	Value
Detector Primary Angle	(0018,1530)	from Original (XA image only)
Detector Secondary Angle	(0018,1531)	from Original (XA image only)
Shutter Shape	(0018,1600)	
Shutter Left Vertical Edge	(0018,1602)	as set
Shutter Right Vertical Edge	(0018,1604)	as set
Shutter Upper Horizontal Edge	(0018,1606)	as set
Shutter Lower Horizontal Edge	(0018,1608)	as set
Center of Circular Shutter	(0018,1610)	from Original
Radius of Circular Shutter	(0018,1612)	from Original
Collimator Shape	(0018,1700)	from Original
Collimator Left Vertical Edge	(0018,1702)	from Original
Collimator Right Vertical Edge	(0018,1704)	from Original
Collimator Upper Horizontal Edge	(0018,1706)	from Original
Collimator Lower Horizontal Edge	(0018,1708)	from Original
Center of Circular Collimator	(0018,1710)	from Original
Radius of Circular Collimator	(0018,1712)	from Original
Vertices of the Polygonal Collimator	(0018,1720)	from Original
Private Creator	(0019,00xx)	"SIEMENS SMS-AX VIEW 1.0"
<i>Attributes according to "8.5.1.1 Angio Viewing Module"</i>		
Series Instance UID	(0020,000E)	from Original
Series Number	(0020,0011)	from Original
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	from Original or <zero length>
Image Comments	(0020,4000)	SM
Private Creator	(0021,00xx)	"SIEMENS SMS-AX ACQ 1.0"
<i>Attributes copied from original AXIOM Artis / Artis zee image</i>		
Private Creator	(0023,00xx)	"SIEMENS SMS-AX QUANT 1.0"
Calibration TOD Value	(0023,xx08)	
Private Creator	(0025,00xx)	"SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0"
<i>Attributes according to "8.5.1.3 Original Image Info Module"</i>		
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	from Original
Columns	(0028,0011)	from Original
Bits Allocated	(0028,0100)	from Original
Bits Stored	(0028,0101)	from Original
High Bit	(0028,0102)	from Original
Pixel Representation	(0028,0103)	0
Pixel Intensity Relationship	(0028,1040)	DISP
Window Center	(0028,1050)	as set
Window Width	(0028,1051)	as set
Representative Frame Number	(0028,6010)	1
Requested Procedure Description	(0032,1060)	from Original
Study Comments	(0032,4000)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original

Attribute Name	Tag	Value
Performed Procedure Step ID	(0040,0253)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Overlay Rows	(60xx,0010)	
Overlay Columns	(60xx,0011)	
Overlay Description	(60xx,0022)	
Overlay Type	(60xx,0040)	G
Overlay Origin	(60xx,0050)	111
Overlay Bits Allocated	(60xx,0100)	same as (0028,0100) or 1 (if Overlay encoded in [60xx,3000])
Overlay Bit Position	(60xx,0102)	12 or 0 (if Overlay encoded in [60xx,3000])
Overlay Data	[60xx,3000]	(with Offline Media Instances) Graphics Overlay
Pixel Data	(7FE0,0010)	

8.1.1.3.2 Quant Report Images - derived XA/XRF IOD

The syngo X Workplace will create result images from performing Quantitative Analysis Functions. To ensure image interchange, the resulting reports are of same type as the input images – XA or XRF.

Table 59 - XA/XRF Derived Quant Report Image (Monochrome)

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	(conf. Character Set is added, if needed)
Image Type	(0008,0008)	DERIVED\SECONDARY\<3 rd to n th value from Original>\QUANT
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.12.1 or 1.2.840.10008.5.1.4.1.1.12.2
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd> (Quant Series)
Acquisition Date	(0008,0022)	Date of original Acquisition
Content Date	(0008,0023)	<yyyymmdd> (date of creation)
Series Time	(0008,0031)	<hhmmss.fyyyy> (Quant Series)
Acquisition Time	(0008,0032)	Time original Acquisition
Content Time	(0008,0033)	<hhmmss.fyyyy> (time of creation)
Modality	(0008,0060)	XA or RF
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from Original
Station Name	(0008,1010)	from WS configuration
Series Description	(0008,103E)	input from Analysis
Performing Physician's Name	(0008,1050)	input via "Correct" user interface possible
Operator's Name	(0008,1070)	from Original
Manufacturer's Model Name	(0008,1090)	
Referenced Patient Sequence	(0008,1120)	from Original
>Referenced SOP Class UID	(0008,1150)	
>Referenced SOP Instance UID	(0008,1155)	
Start Trim	(0008,2142)	<1 st frame to display>

Attribute Name	Tag	Value
Stop Trim	(0008,2143)	<last frame to display>
Recommended Display Frame Rate	(0008,2144)	1
Contrast Bolus Agent	(0018,0010)	from Original
Cine Rate	(0018,0040)	1
KVP	(0018,0060)	from Original
Device Serial Number	(0018,1000)	from WS configuration
Software Versions	(0018,1020)	
Protocol Name	(0018,1030)	from Original
Contrast/Bolus Ingredient	(0018,1048)	from Original
Frame Time	(0018,1063)	1000
Distance Source to Detector	(0018,1110)	from Original
Distance Source to Patient	(0018,1111)	from Original
Exposure Time	(0018,1150)	from Original
X-Ray Tube Current	(0018,1151)	from Original
Average Pulse Width	(0018,1154)	from Original
Radiation Setting	(0018,1155)	from Original
Radiation Mode	(0018,115A)	from Original
Image Area Dose Product	(0018,115E)	from Original
Intensifier Size	(0018,1162)	from Original
Focal Spot	(0018,1190)	from Original
Column Angulation	(0018,1450)	from Original (XRF)
Tomo Layer Height	(0018,1460)	from Original (XRF)
Tomo Angle	(0018,1470)	from Original (XRF)
Tomo Time	(0018,1480)	from Original (XRF)
Tomo Type	(0018,1490)	from Original (XRF)
Positioner Motion	(0018,1500)	from Original (XA)
Positioner Primary Angle	(0018,1510)	from Original (XA)
Positioner Secondary Angle	(0018,1511)	from Original (XA)
Positioner Primary Angle Increment	(0018,1520)	from Original (XA, Only with DYNAMIC)
Positioner Secondary Angle Increment	(0018,1521)	from Original (XA, Only with DYNAMIC)
Patient Position	(0018,5100)	from Original
Series Instance UID	(0020,000E)	<new Quant series will be created>
Series Number	(0020,0011)	
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	from Original or <zero length>
Private Creator	(0023,00xx)	"SIEMENS SMS-AX QUANT 1.0"
<i>Attributes according to "8.5.1.2 Angio Quantification Module" if image was calibrated</i>		
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Number of Frames	(0028,0008)	1 to 4
Frame Increment Pointer	(0028,0009)	(0018,1063)
Rows	(0028,0010)	1024
Columns	(0028,0011)	1024
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	12
High Bit	(0028,0102)	11

Attribute Name	Tag	Value
Pixel Representation	(0028,0103)	0
Pixel Intensity Relationship	(0028,1040)	LIN
Window Center	(0028,1050)	2047
Window Width	(0028,1051)	4095
Lossy Image Compression	(0028,2110)	from Original
Representative Frame Number	(0028,6010)	1
Study Status ID	(0032,000A)	from Original
Scheduled Study Start Date	(0032,1000)	from Original
Scheduled Study Start Time	(0032,1001)	from Original
Scheduled Study Location	(0032,1020)	from Original
Scheduled Study Location AE Title	(0032,1021)	from Original
Requesting Physician	(0032,1032)	from Original
Requested Procedure Description	(0032,1060)	from Original
Requested Contrast Agent	(0032,1060)	from Original
Study Comments	(0032,4000)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Confidentiality Constraint on Patient Data Description	(0040,3001)	from Original
Pixel Data	(7FE0,0010)	

8.1.1.4 CT Standard Extended SOP Class

8.1.1.4.1 DynaCT Reconstructed Volume Data for Artis / syngo X Workplace

The syngo X Workplace will create 3D volume data-sets from 3D reconstruction application package. Those will be encoded as CT Standard extended SOP Class. Please see the following table for complete overview of supplied Type 1/2/3 Standard and Private attributes:

Table 60 - CT Derived Image (Monochrome) from Reconstruction

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	DERIVED\SECONDARY\AXIAL\3DANGIO\<Data_Type> <Data_Type> values: NAT_MASK Images acquired w/o contrast media NAT_FILL Images acquired with contrast media SUB Subtracted acquisition PBV "Parenchymal Blood Volume" acq.
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.ffffff>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2 (CT Image Storage)
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd> (date of creation)

Attribute Name	Tag	Value
Acquisition Date	(0008,0022)	derived from original Acquisition/Content Date
Content Date	(0008,0023)	<yyyymmdd> (date of creation)
Acquisition DateTime	(0008,002A)	from Original or calculated
Series Time	(0008,0031)	<hhmmss.ffffff> (time of creation)
Acquisition Time	(0008,0032)	derived from original Acquisition/Content Time
Content Time	(0008,0033)	<hhmmss.ffffff> (time of creation)
Modality	(0008,0060)	XA or CT (default = XA, can be configured)
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from Original
Institution Address	(0008,0081)	from Original
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	contains information about used reconstruction parameters
Institutional Department Name	(0008,1040)	from WS Configuration
Performing Physician's Name	(0008,1050)	from Original
Operator's Name	(0008,1070)	from Original
Manufacturer's Model Name	(0008,1090)	"AXIOM-Artis"
Derivation Description	(0008,2111)	applied correction algorithms
Contrast/Bolus Agent	(0018,0010)	from Original
Body Part Examined	(0018,0015)	from Original
Scan Options	(0018,0022)	for images created by "Gated Cardiac 3D Acquisition"
Slice Thickness	(0018,0050)	calculated
KVP	(0018,0060)	from Original
Device Serial Number	(0018,1000)	from WS Configuration
Gantry ID	(0018,1008)	from WS Configuration
Software Versions	(0018,1020)	from Original<WS version>\<WS version IAE>
Protocol Name	(0018,1030)	from Original <zoom size(nnn)> <step width(n.nn)> <dose(nn.nn)> <correction(aaa)>
Reconstruction Diameter	(0018,1100)	set for reconstructed slice
Distance Source to Detector	(0018,1110)	from Original
Contrast/Bolus Ingredient	(0018,1048)	from Original
Date of Last Calibration	(0018,1200)	<yyyymmdd> (date of last 3D calibration)
Time of Last Calibration	(0018,1201)	<hhmmss.ffffff> (time of last 3D calibration)
Convolution Kernel	(0018,1210)	<kernel type>\<Image characteristics> Values for kernel type: "EE" (Default for high contrast) "HU" (Default for DynaCT) Values for image characteristics: "Auto", "Sharp", "Normal", "Smooth", "Very Smooth"
Patient Position	(0018,5100)	from Original
Private Creator	(0019,00xx)	"SIEMENS AX DYNACT"
Private Data	(0019,xx02)	private transformation matrix
Private Data	(0019,xx03)	calibration coordinate system ID
Private Data	(0019,xx10)	reconstruction joblist
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	from Original
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	1 (feet) continuous to number of slices (head)
Patient Orientation	(0020,0020)	<removed>

Attribute Name	Tag	Value
Image Position (Patient)	(0020,0032)	calculated during reconstruction
Image Orientation (Patient)	(0020,0037)	calculated during reconstruction
Frame of Reference UID	(0020,0052)	<new UID> (per reconstructed image-set)
Laterality	(0020,0060)	from Original
Position Reference Indicator	(0020,1040)	from Original
Private Creator	(0021,00xx)	"SIEMENS SMS-AX ACQ 1.0"
Private Acquisition Data	(0021,xxxx)	private acquisition data
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	256, 512, 768 or 1024.
Columns	(0028,0011)	256, 512, 768 or 1024.
Pixel Spacing	(0028,0030)	calculated during reconstruction
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	16
High Bit	(0028,0102)	15
Pixel Representation	(0028,0103)	0
Smallest Image Pixel Value	(0028,0106)	
Largest Image Pixel Value	(0028,0107)	
Pixel Padding Value	(0028,0120)	
Burned In Annotation	(0028,0301)	NO
Window Center	(0028,1050)	Value from the "Visualization Preset" configuration
Window Width	(0028,1051)	Value from the "Visualization Preset" configuration
Rescale Intercept	(0028,1052)	0.0 or -1024 (only for HU values)
Rescale Slope	(0028,1053)	1
Rescale Type	(0028,1054)	"HU" for Hounsfield Units, only expected with CT "US" for unspecified
VOI LUT Function	(0028,1056)	
Lossy Image Compression	(0028,2110)	00
VOI LUT Sequence	(0028,3010)	from Original
Requested Procedure Description	(0032,1060)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Performed Protocol Code Sequence	(0040,0260)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason For The Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original
Pixel Data	(7FE0,0010)	

8.1.1.4.2 CT Ranges / Save Image as Derived Volume Data

The syngo X Workplace will save radial, parallel or curved ranges or "Save image" functionality based on CT, XR3D or Enhanced CT Images as CT Standard extended SOP Class.

Please see the following table for complete overview of supplied Type 1/2/3 Standard and Private attributes:

Table 61 – Ranges / Save Image as CT Derived Image (Monochrome)

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	From Original or conf. Character Set
Image Type	(0008,0008)	DERIVED\SECONDARY\ <i>image type</i> >< <i>filter type</i> >\ \ \< <i>range type</i> > < <i>image type</i> > values: AXIAL LOCALIZER < <i>filter type</i> > values: MPR MIP MINIP < <i>range type</i> > values (in case of Range functionality): PARALLEL RADIAL CURVED
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.ffffff>
Instance Creator UID	(0008,0014)	<implementation_class_uid>.<individual_id>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.2 (CT Image Storage)
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd> (date of creation)
Acquisition Date	(0008,0022)	derived from original Acquisition/Content Date
Content Date	(0008,0023)	<yyyymmdd> (date of creation)
Acquisition DateTime	(0008,002A)	derived from original Acquisition Date/Time
Series Time	(0008,0031)	<hhmmss.ffffff> (time of creation)
Acquisition Time	(0008,0032)	derived from original Acquisition/Content Time
Content Time	(0008,0033)	<hhmmss.ffffff> (time of creation)
Modality	(0008,0060)	from Original
Manufacturer	(0008,0070)	from Original
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	
Institutional Department Name	(0008,1040)	from WS Configuration
Performing Physician's Name	(0008,1050)	from Original
Manufacturer's Model Name	(0008,1090)	from Original
Derivation Description	(0008,2111)	Description of how this image was derived.
Scan Options	(0018,0022)	from Original if original is a CT image, not set in case original is XR3D or Enhanced CT image

Attribute Name	Tag	Value
Slice Thickness	(0018,0050)	calculated
KVP	(0018,0060)	from Original
Device Serial Number	(0018,1000)	from Original
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	"Radial Ranges", "Parallel Ranges", "Curved Ranges" or from Original
Reconstruction Diameter	(0018,1100)	from Original
Distance Source to Detector	(0018,1110)	from Original
Date of last Calibration	(0018,1200)	from Original
Time of last Calibration	(0018,1201)	from Original
Convolution Kernel	(0018,1210)	from Original
Patient Position	(0018,5100)	from Original
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	from Original
Acquisition Number	(0020,0012)	from Original
Instance Number	(0020,0013)	n-m (n, m >0) 0 for reference image
Patient Orientation	(0020,0020)	<removed>
Image Position (Patient)	(0020,0032)	calculated during reconstruction
Image Orientation (Patient)	(0020,0037)	calculated during reconstruction
Frame of Reference UID	(0020,0052)	<new UID>
Laterality	(0020,0060)	from Original
Position Reference Indicator	(0020,1040)	
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Rows	(0028,0010)	256 or 512
Columns	(0028,0011)	256 or 512
Pixel Spacing	(0028,0030)	calculated during reconstruction
Bits Allocated	(0028,0100)	from Original
Bits Stored	(0028,0101)	from Original
High Bit	(0028,0102)	from Original
Pixel Representation	(0028,0103)	from Original
Burned In Annotation	(0028,0301)	from Original
Window Center	(0028,1050)	as set
Window Width	(0028,1051)	as set
Rescale Intercept	(0028,1052)	from Original
Rescale Slope	(0028,1053)	
Rescale Type	(0028,1054)	
Window Center & Width Explanation	(0028,1055)	
VOI LUT Function	(0028,1056)	from Original or may be set by application
Lossy Image Compression	(0028,2110)	from Original
VOI LUT Sequence	(0028,3010)	from Original
Requested Procedure Description	(0032,1060)	from Original
Study Comments	(0032,4000)	from Original
Special Needs	(0038,0050)	from Original
Patient State	(0038,0500)	from Original

Attribute Name	Tag	Value
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Performed Protocol Code Sequence	(0040,0260)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason For The Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original
Confidentiality Constraint on Patient Data Description	(0040,3001)	from Original
Pixel Data	(7FE0,0010)	

8.1.1.5 MR Standard Extended SOP Class

8.1.1.5.1 MR Ranges / Save Image as Derived Volume Data

The syngo X Workplace will save radial, parallel or curved ranges or "Save image" functionality based on MR or MR Enhanced Images as MR Standard extended SOP Class.

Please see the following table for complete overview of supplied Type 1/2/3 Standard and Private attributes:

Table 62 – Ranges / Save Image as MR Derived Image (Monochrome)

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original or conf. Character Set
Image Type	(0008,0008)	DERIVED\SECONDARY\ <i><image type></i> copied from original\ <i><filter type></i> copied from original\ <i><range type></i> <i><image type></i> values: Replaced for Localizer image: OTHER <i><filter type></i> values: MPR MIP MINIP <i><range type></i> values (in case of Range functionality): PARALLEL RADIAL CURVED
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.4 (MR Image Storage)
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd> (date of creation)
Acquisition Date	(0008,0022)	derived from original Acquisition/Content Date
Content Date	(0008,0023)	<yyyymmdd> (date of creation)

Attribute Name	Tag	Value
Acquisition DateTime	(0008,002A)	derived from original Acquisition Date/Time
Series Time	(0008,0031)	<hhmmss.fffff> (time of creation)
Acquisition Time	(0008,0032)	derived from original Acquisition/Content Time
Content Time	(0008,0033)	<hhmmss.fffff> (time of creation)
Modality	(0008,0060)	from Original
Manufacturer	(0008,0070)	from Original
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	
Institutional Department Name	(0008,1040)	from WS Configuration
Performing Physician's Name	(0008,1050)	from Original
Manufacturer's Model Name	(0008,1090)	from Original
Derivation Description	(0008,2111)	Description of how this image was derived.
Body Part Examined	(0018,0015)	from Original
Scanning Sequence	(0018,0020)	from Original if original is an MR image, "SE", "GR"; "SE\GR", "IR" or "EP" in case original is an Enhanced MR image
Sequence Variant	(0018,0021)	from Original if original is an MR image; "SP", "MTC", "SS", "OSP" or "SK" in case original is an Enhanced MR image
Scan Options	(0018,0022)	from Original if original is an MR image; "FC", "SP", "PEP", "PEP\PEF", "CG", "RG" or "FS" in case original is an Enhanced MR image
MR Acquisition Type	(0018,0023)	from Original
Slice Thickness	(0018,0050)	calculated
Repetition Time	(0018,0080)	from Original
Echo Time	(0018,0081)	from Original
Inversion Time	(0018,0082)	from Original
Echo Train Length	(0018,0091)	from Original
Device Serial Number	(0018,1000)	from Original
Software Versions	(0018,1020)	from Original
Protocol Name	(0018,1030)	"Radial Ranges", "Parallel Ranges", "Curved Ranges" or from Original
Trigger Time	(0018,1060)	from Original
Date of last Calibration	(0018,1200)	from Original
Time of last Calibration	(0018,1201)	from Original
Patient Position	(0018,5100)	from Original
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	
Instance Number	(0020,0013)	n-m (n, m >0) 0 for reference image
Patient Orientation	(0020,0020)	<removed>
Image Position (Patient)	(0020,0032)	calculated during reconstruction
Image Orientation (Patient)	(0020,0037)	calculated during reconstruction
Frame of Reference UID	(0020,0052)	<new UID>
Laterality	(0020,0060)	from Original
Position Reference Indicator	(0020,1040)	

Attribute Name	Tag	Value
Image Comments	(0020,4000)	
Private Creator	(0021,00xx)	"SIEMENS SMS-AX ACQ 1.0"
Private Acquisition Data	(0021,xxxx)	private acquisition data
Samples per Pixel	(0028,0002)	from Original
Photometric Interpretation	(0028,0004)	from Original
Rows	(0028,0010)	256 or 512
Columns	(0028,0011)	256 or 512
Pixel Spacing	(0028,0030)	calculated during reconstruction
Bits Allocated	(0028,0100)	from Original
Bits Stored	(0028,0101)	from Original
High Bit	(0028,0102)	from Original
Pixel Representation	(0028,0103)	from Original
Burned In Annotation	(0028,0301)	from Original
Window Center	(0028,1050)	as set
Window Width	(0028,1051)	as set
VOI LUT Function	(0028,1056)	from Original or may be set by application
Lossy Image Compression	(0028,2110)	from Original
VOI LUT Sequence	(0028,3010)	from Original
Requested Procedure Description	(0032,1060)	from Original
Study Comments	(0032,4000)	from Original
Special Needs	(0038,0050)	from Original
Patient State	(0038,0500)	from Original
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Performed Protocol Code Sequence	(0040,0260)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason For The Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original
Confidentiality Constraint on Patient Data Description	(0040,3001)	from Original
Pixel Data	(7FE0,0010)	

8.1.1.6 X-Ray 3D Angiographic Image Standard Extended SOP Class

8.1.1.6.1 4D DSA

The syngo X Workplace will save 4D DSA (Dyna4D) reconstructions as X-Ray 3D Angiographic Object Standard extended SOP Class. The 4D DSA data is stored with transfer syntax 1.2.840.1.0008.1.2.4.80 (JPEG-LS Lossless).

Please see the following table for complete overview of supplied Type 1/2/3 Standard and Private attributes:

Table 63 – X-Ray 3D Angiographic Image from 4D DSA Reconstruction

© Siemens Healthcare GmbH. 2020. All rights reserved.

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from Original
Image Type	(0008,0008)	ORIGINAL\PRIMARY\4D_DSA\NONE
Instance Creation	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.ffffff>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.13.1.1
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.ffffff>
Content Time	(0008,0033)	<hhmmss.ffffff>
Modality	(0008,0060)	XA
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from Original
Institution Address	(0008,0081)	from Original
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	contains information about used reconstruction parameters
Institutional Department Name	(0008,1040)	from WS configuration
Performing Physician's Name	(0008,1050)	from Original
Operators' Name	(0008,1070)	from Original
Manufacturer's Model Name	(0008,1090)	"AXIOM-Artis"
Referenced Performed Procedure Step Sequence	(0008,1111)	from Original
Related Series Sequence	(0008,1250)	from Original
Pixel Presentation	(0008,9205)	MONOCHROME
Volumetric Properties	(0008,9206)	VOLUME
Volume Based Calculation Technique	(0008,9207)	NONE
Contrast/Bolus Agent Sequence	(0018,0012)	if contrast media was applied in original images (C-B0300, SRT, "Contrast Agent")
>Contrast/Bolus Administration Route Sequence	(0018,0014)	(R-41198, SRT, "Unknown")
>Contrast/Bolus Volume	(0018,1041)	<zero length>
>Contrast/Bolus Ingredient Concentration	(0018,1049)	<zero length>
>Contrast/Bolus Agent Number	(0018,9337)	
>Contrast/Bolus Ingredient Code Sequence	(0018,9338)	<zero length>
Body Part Examined	(0018,0015)	from Original
Device Serial Number	(0018,1000)	from WS configuration
Software Versions	(0018,1020)	from Original"<WS version>"<WS version IAE>"
Protocol Name	(0018,1030)	"<from Original> <zoom size(nnn)> <step width(n.nn)> <dose(nn.nn)> <correction(aaa)>"
Reconstruction Diameter	(0018,1100)	set for reconstructed slice

Attribute Name	Tag	Value
Convolution Kernel	(0018,1210)	<kernel type>\<Image characteristics> Values for kernel type: "EE" (Default for high contrast) "HU" (Default for DynaCT) Values for image characteristics: "Auto", "Sharp", "Normal", "Smooth", "Very Smooth"
Patient Position	(0018,5100)	from Original
Content Qualification	(0018,9004)	PRODUCT
Contributing Sources Sequence	(0018,9506)	2 items (mask and contrast)
>Acquisition DateTime	(0008,002A)	<yyyymmddhhmmss.ffffff>
>Manufacturer	(0008,0070)	from Original
>Station Name	(0008,1010)	from Original
>Operators' Name	(0008,1070)	from Original
>Operator Identification Sequence	(0008,1072)	from Original
>Manufacturer's Model Name	(0008,1090)	from Original
>Device Serial Number	(0018,1000)	from Original
>Software Versions	(0018,1020)	from Original
>Protocol Name	(0018,1030)	from Original
>Contributing SOP Instances Reference Sequence	(0020,9529)	contains reference to exactly 1 original image on study, series and instance level
>Rows	(0028,0010)	from Original
>Columns	(0028,0011)	from Original
>Bits Stored	(0028,0101)	from Original
>Lossy Image Compression	(0028,2110)	from Original
>Lossy Image Compression Ratio	(0028,2112)	from Original
>Lossy Image Compression Method	(0028,2114)	from Original
>Acquisition Device Processing Description	(0018,1400)	from Original
>Acquisition Device Processing Code	(0018,1401)	from Original
>Acquisition Protocol Name	(0018,9423)	from Original
>Plane Identification	(0018,9457)	derived from Original
>Imager Pixel Spacing	(0018,1164)	from Original
>Performed Protocol Code Sequence	(0040,0260)	from Original
X-Ray 3D Acquisition Sequence	(0018,9507)	2 items (mask and contrast)
>Source Image Sequence	(0008,2112)	points to original image
>>Referenced SOP Class UID	(0008,1150)	
>>Referenced SOP Instance UID	(0008,1155)	
>>Referenced Frame Number	(0008,1160)	if only set of frames was taken as input
>Contrast/Bolus Agent	(0018,0010)	from Original
>KVP	(0018,0060)	from Original
>Distance Source to Detector	(0018,1110)	from Original
>Field of View Shape	(0018,1147)	from Original
>Focal Spot	(0018,1190)	from Original
>Detector Type	(0018,7004)	<zero length>
>Detector Description	(0018,7006)	from Original
>Detector ID	(0018,700A)	from Original
>Exposure Time in ms	(0018,9328)	from Original: attribute (0018,1150)
>X-Ray Tube Current in mA	(0018,9330)	from Original: attribute (0018,1151)
>Exposure in mAs	(0018,9332)	from Original: attribute (0018,1152)

Attribute Name	Tag	Value
X-Ray 3D Reconstruction Sequence	(0018,9530)	1 item
>Application Name	(0018,9524)	"3D Reconstruction"
>Application Version	(0018,9525)	version of reconstruction application
>Application Manufacturer	(0018,9526)	"Siemens"
>Algorithm Type	(0018,9527)	"FILTER_BACK_PROJ"
>Reconstruction Description	(0018,9531)	code for applied correction algorithms
>Acquisition Index	(0020,9518)	112
Private Creator	(0019,00xx)	"SIEMENS AX DYNACT"
Private Data	(0019,xx02)	private Transformation matrix
Private Data	(0019,xx03)	calibration coordinate system ID
Private Data	(0019,xx10)	reconstruction joblist
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	from Original
Instance Number	(0020,0013)	
Frame of Reference UID	(0020,0052)	from Original or <new UID>
Position Reference Indicator	(0020,1040)	from Original
Image Comments	(0020,4000)	from Original
Private Creator	(0021,00xx)	"SIEMENS SMS-AX ACQ 1.0"
Private Acquisition Data	(0021,xxxx)	private acquisition data
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Number of Frames	(0028,0008)	
Rows	(0028,0010)	
Columns	(0028,0011)	
Bits Allocated	(0028,0100)	16
Bits Stored	(0028,0101)	16
High Bit	(0028,0102)	15
Pixel Representation	(0028,0103)	0
Pixel Padding Value	(0028,0120)	0
Burned in Annotation	(0028,0301)	NO
Lossy Image Compression	(0028,2110)	00
Representative Frame Number	(0028,6010)	
Performed Procedure Step Start Date	(0040,0244)	from Original
Performed Procedure Step Start Time	(0040,0245)	from Original
Performed Procedure Step ID	(0040,0253)	from Original
Performed Procedure Step Description	(0040,0254)	from Original
Request Attributes Sequence	(0040,0275)	from Original
>Scheduled Procedure Step Description	(0040,0007)	from Original
>Scheduled Procedure Step ID	(0040,0009)	from Original
>Requested Procedure ID	(0040,1001)	from Original
>Reason for the Requested Procedure	(0040,1002)	from Original
Comments on the Performed Procedure Step	(0040,0280)	from Original
Acquisition Context Sequence	(0040,0555)	<zero length>
Patient Orientation Code Sequence	(0054,0410)	(F-10450, SRT, "recumbent")

Attribute Name	Tag	Value
>Patient Orientation Modifier Code Sequence	(0054,0412)	One of (F-10340, SRT, "supine"), (F-10310, SRT, "prone"), (F-10317, SRT, "right lateral decubitus"), (F-10319, SRT, "left lateral decubitus")
Patient Gantry Relationship Code Sequence	(0054,0414)	One of (F-10470, SRT, "headfirst"), (F-10480, SRT, "feet-first")
Presentation LUT Shape	(2050,0020)	IDENTITY
Shared Functional Groups Sequence	(5200,9229)	
>X-Ray 3D Frame Type Sequence	(0018,9504)	1 item
>>Frame Type	(0008,9007)	ORIGINAL\PRIMARY\4D_DSA\NONE
>>Pixel Presentation	(0008,9205)	MONOCHROME
>>Volumetric Properties	(0008,9206)	VOLUME
>>Volume Based Calculation Technique	(0008,9207)	NONE
>>Reconstruction Index	(0020,9536)	1
>Frame Anatomy Sequence	(0020,9071)	1 item
>>Frame Laterality	(0020,9072)	from Original ("L" or "R", if available)
>>Anatomic Region Sequence	(0008,2218)	(T-D0010, SRT, "Entire body")
>Plane Orientation Sequence	(0020,9116)	1 item
>>Image Orientation (Patient)	(0020,0037)	
>Pixel Measures Sequence	(0028,9110)	1 item
>>Pixel Spacing	(0028,0030)	
>>Slice Thickness	(0018,0050)	
>Frame VOI LUT Sequence	(0028,9132)	
>>Window Center	(0028,1050)	<window 1 center value>\<window 2 center value>
>>Window Width	(0028,1051)	<window 1 width value>\<window 2 width value>
>Real World Value Mapping Sequence	(0040,9096)	
>>LUT Explanation	(0028,3003)	"Linear Mapping"
>>Measurements Units Code Sequence	(0040,08EA)	([hnsfU], UCUM, "Hounsfield unit")
>>LUT Label	(0040,9210)	1
>>Real World Value LUT Last Value Mapped	(0040,9211)	
>>Real World Value LUT First Value Mapped	(0040,9216)	
>>Real World Value Intercept	(0040,9224)	
>>Real World Value Slope	(0040,9225)	
Per-frame Functional Groups Sequence	(5200,9230)	as many items as frames
>Frame Content Sequence	(0020,9111)	1 item
>>Frame Acquisition DateTime	(0018,9074)	from Original: attribute Acquisition DateTime (0008,002A) or calculated from Acquisition Date (0008,0022) and Acquisition Time (0008,0032)
>>Frame Reference DateTime	(0018,9151)	Used to record the time course, computed using original Acquisition Date and Time value and FrameTime resp. FrameTimeVector.
>>Frame Acquisition Duration	(0018,9220)	from Original: private attribute Total Scene Time (0021,xx29) (default: 1000 ms)
>>Stack ID	(0020,9056)	4D_DSA

Attribute Name	Tag	Value
>>In-Stack Position Number	(0020,9057)	ordinal index starting with 1
>Plane Position Sequence	(0020,9113)	1 item
>>Image Position Patient	(0020,0032)	
Pixel Data	(7FE0,0010)	

8.1.1.7 SR Document SOP Class

The syngo X Workplace will create Reports on demand for long-term archival of Scoliosis Analysis. Since there is no public template for orthopedic reports available for this, a Siemens privately defined template for long-term documentation is used. Please refer to next sections to learn about the SR implementation and the definition of the underlying SR template.

8.1.1.7.1 Orthopedic Report Comprehensive SR SOP Class

Table 64 - Private Orthopedic Report Comprehensive SR from Composing

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	(conf. Character Set is added, if needed)
Image Type	(0008,0008)	ORIGINAL\PRIMARY\OTHER\CSA_REPORT
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.88.33
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.ffffff>
Content Time	(0008,0033)	<hhmmss.ffffff>
Modality	(0008,0060)	SR
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	"Composing Report"
Institutional Department Name	(0008,1040)	from WS configuration
Performing Physician's Name	(0008,1050)	input via "Correct" user interface possible
Manufacturer's Model Name	(0008,1090)	from WS configuration
Device Serial Number	(0018,1000)	from WS Configuration
Software Versions	(0018,1020)	from WS Configuration
Series Instance UID	(0020,000E)	
Series Number	(0020,0011)	
Instance Number	(0020,0013)	
Study Status ID	(0032,000A)	from Original
Scheduled Study Start Date	(0032,1000)	from Original
Scheduled Study Start Time	(0032,1001)	from Original
Scheduled Study Location	(0032,1020)	from Original
Scheduled Study Location AE Title	(0032,1021)	from Original
Requesting Physician	(0032,1032)	from Original
Requested Procedure Description	(0032,1060)	from Original

Attribute Name	Tag	Value
Study Comments	(0032,4000)	from Original
Value Type	(0040,A040)	CONTAINER
Concept Name Code Sequence	(0040,A043)	
>Code Value	(0008,0100)	"ORx50001"
>Coding Scheme Designator	(0008,0102)	"99SMS_COMP"
>Code Value	(0008,0104)	"Orthopedic Report"
Continuity of Contents	(0040,A050)	"SEPARATE"
Performed Procedure Code Sequence	(0040,A372)	
Current Requested Procedure Evidence Sequence	(0040,A375)	
>>sequence items		This sequence will contain references to each image referenced in the report.
Completion Flag	(0040,A491)	
Verification Flag	(0040,A493)	
Content Template Sequence	(0040,A504)	See Template Descriptions in section "8.3 Coded Terminology and Templates" for further details on the Orthopedic Report Template.
Content Sequence	(0040,A730)	

8.1.1.8 Segmentation Standard Extended SOP Class

8.1.1.8.1 Segmentation Results

Table 65 - Segmentation Results from 3D Applications

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from WS Configuration
Image Type	(0008,0008)	DERIVED\PRIMARY
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.fffff>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.66.4
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Acquisition Date	(0008,0022)	from Original (0008,0021), if available
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.fffff>
Acquisition Time	(0008,0032)	from Original (0008,0031), if available
Content Time	(0008,0033)	<hhmmss.fffff>
Modality	(0008,0060)	SEG
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	same as Protocol Name
Performing Physician's Name	(0008,1050)	not set, unless input via "Correct"
Operators' name	(0008,1070)	from Original, unless set via "Correct"

Attribute Name	Tag	Value
Manufacturer's Model Name	(0008,1090)	"from WS Configuration
Referenced Series Sequence	(0008,1115)	used, if this instance references instances in this study.
>Referenced Instance Sequence	(0008,114A)	
>Series Instance UID	(0020,000E)	
Studies Containing Other Referenced Instances Sequence	(0008,1200)	used, if this instance references instances in other studies.
>Referenced Series Sequence	(0008,1115)	
>>Referenced Instance Sequence	(0008,114A)	
>>Series Instance UID	(0020,000E)	
>Study Instance UID	(0020,000D)	
Source Image Sequence	(0008,2112)	Reference to the volume/slice object(s) used to generate this segmentation result
Derivation Code Sequence	(0008,9215)	refers to "Segmentation"
Device Serial Number	(0018,1000)	from WS Configuration
Software Versions	(0018,1020)	from WS Configuration
Protocol Name	(0018,1030)	Information on Segmentation
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	from Original
Instance Number	(0020,0013)	
Patient Orientation	(0020,0020)	from Original
Image Comments	(0020,4000)	
Samples per Pixel	(0028,0002)	1
Photometric Interpretation	(0028,0004)	MONOCHROME2
Number of Frames	(0028,0008)	
Rows	(0028,0010)	
Columns	(0028,0011)	
Bits Allocated	(0028,0100)	1
Bits Stored	(0028,0101)	1
High Bit	(0028,0102)	0
Pixel Representation	(0028,0103)	0
Burned In Annotation	(0028,0301)	NO
Lossy Image Compression	(0028,2110)	00
Representative Frame Number	(0028,6010)	
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Segmentation Type	(0062,0001)	BINARY
Segment Sequence	(0062,0002)	
>Anatomic Region Sequence	(0008,2218)	
>Segmented Property Category Code Sequence	(0062,0003)	
>Segment Number	(0062,0004)	
>Segment Label	(0062,0005)	
>Segment Description	(0062,0005)	(optional)
>Segment Algorithm Type	(0062,0008)	

Attribute Name	Tag	Value
>Segment Algorithm Name	(0062,0009)	One of 'Stroke Segmentation', ' Left Atrium Segmentation', 'Model Based Left Atrium Segmentation', 'Hybrid Model Based Left Atrium Segmentation', 'Aortic Root Segmentation' if Segment Algorithm Type is not MANUAL.
>Recommended Display Grayscale Value	(0062,000C)	
>Recommended Display CIELab Value	(0062,000D)	
>Segmented Property Type Code Sequence	(0062,000F)	
Private Creator	(0063,00xx)	"SIEMENS SMS-AX Segmentation Extensions"
<i>Attributes according to "8.5.2.1 Private Segmentation "</i>		
Content Label	(0070,0080)	
Content Description	(0070,0081)	Contains identifier to identify a related segmentation mesh result stored in a Surface Segmentation Object with same identifier
Content Creator's Name	(0070,0084)	<zero length>
Icon Image Sequence	(0088,0200)	optional
Shared Functional Groups Sequence	(5200,9229)	
>Derivation Image Sequence	(0008,9124)	
>>Derivation Code Sequence	(0008,9215)	(113076, DCM, "Segmentation")
>>Source Image Sequence	(0008,2112)	
>>>Referenced SOP Class UID	(0008,1150)	
>>>Referenced SOP Instance UID	(0008,1155)	
>>>Purpose of Reference Code Sequence	(0040,A170)	(121322, DCM, "Image Processing Operation")
>Frame Content Sequence	(0020,9111)	
>Plane Orientation Sequence	(0020,9116)	
>>Image Orientation (Patient)	(0020,0037)	
>Pixel Measure Sequence	(0028,9110)	
>>Slice Thickness	(0018,0050)	
>>Pixel Spacing	(0028,0030)	
>Segmentation Identification Sequence	(0062,000A)	
>>Referenced Segment Number	(0062,000B)	
Per-frame Functional Groups Sequence	(5200,9230)	one item for each frame
>Plane Position Sequence	(0020,9113)	
>>Image Position (Patient)	(0020,0032)	
Pixel Data	(7FE0,0010)	

8.1.1.9 Surface Segmentation Standard Extended SOP Class

8.1.1.9.1 General 3D Graphic Result Storage

Table 66 – General 3D Graphic Results Storage

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from WS Configuration
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.fffff>

Attribute Name	Tag	Value
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.66.5
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.fffff>
Content Time	(0008,0033)	<hhmmss>
Modality	(0008,0060)	SEG
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	same as Protocol Name
Performing Physician's Name	(0008,1050)	not set, unless input via "Correct"
Operators' name	(0008,1070)	from Original, unless set via "Correct"
Manufacturer's Model Name	(0008,1090)	
Referenced Series Sequence	(0008,1115)	used, if this instance references instances in this study.
>Referenced Instance Sequence	(0008,114A)	
>Series Instance UID	(0020,000E)	
Studies Containing Other Referenced Instances Sequence	(0008,1200)	used, if this instance references instances in other studies.
>Referenced Series Sequence	(0008,1115)	
>>Referenced Instance Sequence	(0008,114A)	
>>Series Instance UID	(0020,000E)	
>Study Instance UID	(0020,000D)	
Device Serial Number	(0018,1000)	from WS Configuration
Software Versions	(0018,1020)	from WS Configuration
Protocol Name	(0018,1030)	Information on Surface Segmentation
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	950
Instance Number	(0020,0013)	
Frame of Reference UID	(0020,0052)	Copied from object to which the Surface Segmentation result applies or new UID. Note: In case of 2 volumes with 2 different FoR UIDs stored in same Series the related SSOs are also stored together in same series with FoR of the volume the first SSO is related to.
Laterality	(0020,0060)	n.a. or <zero length>
Position Reference Indicator	(0020,1040)	if applicable, copied from object to which the Surface Segmentation result applies.
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Segment Sequence	(0062,0002)	
>Anatomic Region Sequence	(0008,2218)	

Attribute Name	Tag	Value
>Segmented Property Category Code Sequence	(0062,0003)	One of (T-D0050, SRT, "Tissue"), (T-D000A, SRT, "Anatomical Structure"), (A-00004, SRT, "Physical Object"), (M-01000, SRT, "Morphologically Altered Structure"), (R-42019, SRT, "Function") or private coded term.
>Segment Number	(0062,0004)	
>Segment Label	(0062,0005)	
>Segment Description	(0062,0006)	(optional)
>Segment Algorithm Type	(0062,0008)	
>Recommended Display Grayscale Value	(0062,000C)	
>Recommended Display CIE Lab Value	(0062,000D)	
>Segmented Property Type Code Sequence	(0062,000F)	
>Surface Count	(0066,002A)	number of Surfaces comprising this segment.
>Referenced Surface Sequence	(0066,002B)	
>>Referenced Surface Number	(0062,002C)	
>>>Segment Surface Generation Algorithm Identification Sequence	(0062,002D)	
>>>>Algorithm Family Code Sequence	(0062,002F)	
>>>>Algorithm Version	(0066,0031)	
>>>>Algorithm Name	(0066,0036)	
>>>>Segment Surface Generation Algorithm Identification Sequence	(0066,002D)	
>>>>>Algorithm Family Code Sequence	(0066,002F)	
>>>>>Algorithm Name	(0066,0036)	Identifies workflow/application
>>>>>Algorithm Version	(0066,0031)	
>>>>>>Segmented Surface Source Instance Sequence	(0066,002E)	reference to volume that was viewed while generating this surface segment.
>>>>>>>Referenced SOP Class UID	(0008,1150)	
>>>>>>>Referenced SOP Instance UID	(0008,1155)	
Number of Surfaces	(0066,0001)	
Surface Sequence	(0066,0002)	
>Recommended Display Grayscale Value	(0062,000C)	
>Recommended Display CIE Lab Value	(0062,000D)	
>Surface Number	(0066,0003)	
>Surface Comments	(0066,0004)	
>Surface Processing	(0066,0009)	typically set to NO
>Recommended Presentation Opacity	(0066,000C)	0.0 specifies 100% transparency and 1.0 a 100% opaqueness.
>Recommended Presentation Type	(0066,000D)	DICOM defined values: SURFACE WIREFRAME POINTS Private terms: CONTOUR (only contour of a wireframe) NONE
>Finite Volume	(0066,000E)	
>Manifold	(0066,0010)	
>Surface Points Sequence	(0066,0011)	

Attribute Name	Tag	Value
>>Number of Surface Points	(0066,0015)	
>>Point Coordinates Data	(0066,0016)	
>Surface Points Normals Sequence	(0066,0012)	<zero length>
>Surface Mesh Primitives Sequence	(0066,0013)	
>>Triangle Point Index List	(0066,0023)	
>>Edge Point Index List	(0066,0024)	typically not used
>>Vertex Points Index List	(0066,0025)	
>>Triangle Strip Sequence	(0066,0026)	typically not used
>>Triangle Fan Sequence	(0066,0027)	typically not used
>>Line Sequence	(0066,0028)	
>>>Primitive Point Index List	(0066,0029)	
>>Facet Sequence	(0066,0034)	typically not used
>Recommended Point Radius	(0066,0037)	
>Recommended Line Thickness	(0066,0038)	
Private Creator	(0067,00xx)	"SIEMENS SMS-AX Surface Segmentation Extensions"
<i>Attributes according to "8.5.3.1 Private Surface Segmentation"</i>		
Content Label	(0070,0080)	
Content Description	(0070,0081)	
Content Creator's Name	(0070,0084)	<zero length>

8.1.1.10 Registration SOP Class

8.1.1.10.1 Rigid 3D/3D Registration result

Table 67 – Rigid 3D/3D Registration Result

Attribute Name	Tag	Value
<i>Attributes according to 8.1.1.1.1 Supported attributes on Patient level</i>		
<i>Attributes according to 8.1.1.1.2 Supported attributes on Study level</i>		
Specific Character Set	(0008,0005)	from WS Configuration
Image Type	(0008,0008)	DERIVED\PRIMARY
Instance Creation Date	(0008,0012)	<yyyymmdd>
Instance Creation Time	(0008,0013)	<hhmmss.ffffff>
SOP Class UID	(0008,0016)	1.2.840.10008.5.1.4.1.1.66.1
SOP Instance UID	(0008,0018)	
Series Date	(0008,0021)	<yyyymmdd>
Content Date	(0008,0023)	<yyyymmdd>
Series Time	(0008,0031)	<hhmmss.ffffff>
Content Time	(0008,0033)	<hhmmss.ffffff>
Modality	(0008,0060)	REG
Manufacturer	(0008,0070)	"Siemens"
Institution Name	(0008,0080)	from WS Configuration
Institution Address	(0008,0081)	from WS Configuration
Station Name	(0008,1010)	from WS Configuration
Series Description	(0008,103E)	same as Protocol Name
Performing Physician's Name	(0008,1050)	not set, unless input via "Correct".

Attribute Name	Tag	Value
Operators' name	(0008,1070)	from Original, unless set via "Correct"
Manufacturer's Model Name	(0008,1090)	
Referenced Series Sequence	(0008,1115)	Used if both volumes are in same study. One item for each volume (registered space, registered volume)
>Referenced Instance Sequence	(0008,114A)	
>Series Instance UID	(0020,000E)	
Studies Containing Other Referenced Instances Sequence	(0008,1200)	Used if both volumes are related to different studies.
>Referenced Series Sequence	(0008,1115)	
>>Referenced Instance Sequence	(0008,114A)	
>>Series Instance UID	(0020,000E)	
>Study Instance UID	(0020,000D)	
Device Serial Number	(0018,1000)	from WS Configuration
Software Versions	(0018,1020)	from WS Configuration
Protocol Name	(0018,1030)	"Fusion3D3D"
Series Instance UID	(0020,000E)	<new UID>
Series Number	(0020,0011)	960
Instance Number	(0020,0013)	
Frame of Reference UID	(0020,0052)	Copied from object to which the registration result applies. Note: In case of 2 volumes with 2 different FoR UIDs stored in same Series the related Registrations are also stored together in same series with FoR of the volume the first Registration is related to.
Laterality	(0020,0060)	n.a. or <zero length>
Position Reference Indicator	(0020,1040)	if applicable, copied from object to which the segmentation result applies
Request Attributes Sequence	(0040,0275)	from Original
>item contents as provided		from Original
Content Label	(0070,0080)	
Content Description	(0070,0081)	Contains identifier to identify a related segmentation result stored in a Segmentation Object with same identifier
Content Creator's Name	(0070,0084)	optional, see also <i>Operator's Name</i>
Registration Sequence	(0070,0308)	Two items, one "identity transformation" for the volume in the registered space, to which the volume specified in the second item, is registered to.
<i>Item 1 refers to the volume in the registered space</i>		
>Referenced Image Sequence	(0008,1140)	reference to the volume in the registered space
>Frame of Reference UID	(0020,0052)	
>Matrix Registration Sequence	(0070,0309)	
>>Matrix Sequence	(0070,030A)	
>>>Frame of Reference Transformation Matrix Type	(0070,030C)	
>>>Frame of Reference Transformation Matrix	(3006,00C6)	"identity transformation" specified.
>>Registration Type Code Sequence	(0070,030D)	(125021,DCM,"Frame of Reference Identity")
<i>Item 2 refers to the volume that is registered</i>		

Attribute Name	Tag	Value
>Referenced Image Sequence	(0008,1140)	reference to the volume that is registered to the registered space
>Frame of Reference UID	(0020,0052)	
>Matrix Registration Sequence	(0070,0309)	
>>Matrix Sequence	(0070,030A)	
>>>Frame of Reference Transformation Matrix Type	(0070,030C)	
>>>Frame of Reference Transformation Matrix	(3006,00C6)	
>>Registration Type Code Sequence	(0070,030D)	

8.1.2 Usage of attributes from received IODs

Please refer to the “SOP specific conformance...” sections in the DICOM networking part of this DCS for more details on attribute specific handling.

8.1.3 Attribute mapping

The syngo X Workplace is not an Acquisition Modality that maps schedules to performed procedures. The mapping of attributes for derived SOP Instances is disclosed in the tables of the previous sub-sections of “8.1.1 Created SOP Instances”.

8.1.4 Coerced/Modified fields

The syngo X Workplace DICOM Application is not performing data coercion.

8.2 Data Dictionary of private Attributes

Table 68 - Data Dictionary of Private Attributes

Tag	Private Owner Code	Name	VR	VM
(0019,xx00)	SIEMENS SMS-AX IAE	Bookmark XML Structure	OB	1
(0019,xx00)	SIEMENS AX INSPACE_EP	3D Path List Sequence	SQ	1
(0019,xx01)	SIEMENS AX INSPACE_EP	Point Name	PN	1
(0019,xx02)	SIEMENS AX INSPACE_EP	Position Vector	FL	3
(0019,xx03)	SIEMENS AX INSPACE_EP	Direction Matrix	FL	16
(0019,xx04)	SIEMENS AX INSPACE_EP	Field of View Angle	DS	1
(0019,xx05)	SIEMENS AX INSPACE_EP	Ablated Flag	US	1
(0019,xx20)	SIEMENS AX INSPACE_EP	Ablation Group Sequence	SQ	1
(0019,xx21)	SIEMENS AX INSPACE_EP	Ablation Point Sequence	SQ	1
(0019,xx22)	SIEMENS AX INSPACE_EP	Ablation Group Name	PN	1
(0019,xx23)	SIEMENS AX INSPACE_EP	Ablation Group Color	FL	4
(0019,xx00)	SIEMENS AX DYNACT	Stand Position Matrix 1	DS	12
(0019,xx01)	SIEMENS AX DYNACT	Stand Position Matrix 2	DS	12
(0019,xx02)	SIEMENS AX DYNACT	Transformation to Calibration	DS	16
(0019,xx03)	SIEMENS AX DYNACT	Calibration Coordinate System ID	US	1-n
(0019,xx05)	SIEMENS AX DYNACT	Transformation to Frames	OB	1
(0019,xx06)	SIEMENS AX DYNACT	Independent Transformation to Frames	OB	1-n
(0019,xx10)	SIEMENS AX DYNACT	Reconstruction Joblist	UT	1
(0019,xx01)	SIEMENS AX INSPACE_LC	Graphic Number	SS	1

Tag	Private Owner Code	Name	VR	VM
(0019,xx02)	SIEMENS AX INSPACE_LC	Graphic Description	LO	1
(0019,xx03)	SIEMENS AX INSPACE_LC	Graphic Type	SS	1
(0019,xx04)	SIEMENS AX INSPACE_LC	Graphic Show Flag	SS	1
(0019,xx05)	SIEMENS AX INSPACE_LC	Graphic Vector	FL	3
(0019,xx10)	SIEMENS AX INSPACE_LC	Graphic List Sequence	SQ	1
(0019,xx00)	SIEMENS SMS-AX VIEW 1.0	Description	US	1
(0019,xx01)	SIEMENS SMS-AX VIEW 1.0	Anatomical Background Percent	US	1
(0019,xx02)	SIEMENS SMS-AX VIEW 1.0	Number of Phases	US	1
(0019,xx03)	SIEMENS SMS-AX VIEW 1.0	Apply Anatomical Background	US	1
(0019,xx04)	SIEMENS SMS-AX VIEW 1.0	Pixel Shift Array	SS	4-4n
(0019,xx05)	SIEMENS SMS-AX VIEW 1.0	Brightness	US	1
(0019,xx06)	SIEMENS SMS-AX VIEW 1.0	Contrast	US	1
(0019,xx07)	SIEMENS SMS-AX VIEW 1.0	Enabled Shutters	US	1
(0019,xx08)	SIEMENS SMS-AX VIEW 1.0	Native Edge Enh. Percent Gain	US	1
(0019,xx09)	SIEMENS SMS-AX VIEW 1.0	Native Edge Enh. LUT Index	SS	1
(0019,xx0A)	SIEMENS SMS-AX VIEW 1.0	Native Edge Enh. Kernel Size	SS	1
(0019,xx0B)	SIEMENS SMS-AX VIEW 1.0	Subtr. Edge Enh. Percent Gain	US	1
(0019,xx0C)	SIEMENS SMS-AX VIEW 1.0	Subtr. Edge Enh. LUT Index	SS	1
(0019,xx0D)	SIEMENS SMS-AX VIEW 1.0	Subtr. Edge Enh. Kernel Size	SS	1
(0019,xx0E)	SIEMENS SMS-AX VIEW 1.0	Fade Percent	US	1
(0019,xx0F)	SIEMENS SMS-AX VIEW 1.0	Flipped before Laterality Applied	US	1
(0019,xx10)	SIEMENS SMS-AX VIEW 1.0	Apply Fade	US	1
(0019,xx12)	SIEMENS SMS-AX VIEW 1.0	Zoom	US	1
(0019,xx13)	SIEMENS SMS-AX VIEW 1.0	Pan X	SS	1
(0019,xx14)	SIEMENS SMS-AX VIEW 1.0	Pan Y	SS	1
(0019,xx15)	SIEMENS SMS-AX VIEW 1.0	Native Edge Enh. Adv Percent Gain	SS	1
(0019,xx16)	SIEMENS SMS-AX VIEW 1.0	Subtr. Edge Enh. Adv Percent Gain	SS	1
(0019,xx17)	SIEMENS SMS-AX VIEW 1.0	Invert Flag	US	1
(0019,xx1A)	SIEMENS SMS-AX VIEW 1.0	Quant 1K Overlay	OB	1
(0019,xx1B)	SIEMENS SMS-AX VIEW 1.0	Original Resolution	US	1
(0019,xx1C)	SIEMENS SMS-AX VIEW 1.0	Auto Window Center	DS	1
(0019,xx1D)	SIEMENS SMS-AX VIEW 1.0	Auto Window Width	DS	1
(0019,xx1E)	SIEMENS SMS-AX VIEW 1.0	Auto Window Correct Value	IS	2
(0019,xx1F)	SIEMENS SMS-AX VIEW 1.0	Sigmoid Window Parameter	DS	1
(0019,xx20)	SIEMENS SMS-AX VIEW 1.0	Roadmap Catheter Contrast	DS	1
(0019,xx21)	SIEMENS SMS-AX VIEW 1.0	Roadmap Vessel Contrast	DS	1
(0019,xx23)	SIEMENS SMS-AX VIEW 1.0	CLEARstent ROI Origin	US	2
(0019,xx24)	SIEMENS SMS-AX VIEW 1.0	CLEARstent ROI Size	US	2
(0019,xx30)	SIEMENS SMS-AX VIEW 1.0	Frame # Roadmap - Min Amplification	US	1
(0019,xx31)	SIEMENS SMS-AX VIEW 1.0	Frame # Roadmap - Vessel Map	US	1
(0019,xx41)	SIEMENS SMS-AX VIEW 1.0	Pixel Shift Values	FL	6-6n
(0019,xx42)	SIEMENS SMS-AX VIEW 1.0	Pixel Shift Indicator	US	1
(0019,xx43)	SIEMENS SMS-AX VIEW 1.0	Applied Pixel Shift Values	FL	6-6n
(0019,xx44)	SIEMENS SMS-AX VIEW 1.0	Pixel Shift Validity	US	2-2n
(0019,xx81)	SIEMENS SMS-AX VIEW 1.0	Edge Enhancement LUT Data - nat	DS	1-n
(0019,xx82)	SIEMENS SMS-AX VIEW 1.0	Edge Enhancement LUT Data - sub	DS	1-n
(0019,xx83)	SIEMENS SMS-AX VIEW 1.0	asymmetric Edge Enh. Kernel Size	SS	1
(0021,xx2A)	SIEMENS SMS-AX ACQ 1.0	Cardiac Phase Center	IS	1
(0021,xx2B)	SIEMENS SMS-AX ACQ 1.0	Cardiac Phase Width	IS	1
(0021,xx3B)	SIEMENS SMS-AX ACQ 1.0	mAs Modulation	IS	1
(0021,xx3C)	SIEMENS SMS-AX ACQ 1.0	R-Peaks Datetimes	DT	1
(0021,xx54)	SIEMENS SMS-AX ACQ 1.0	Rotation Angle	SS	1

Tag	Private Owner Code	Name	VR	VM
(0021,xx56)	SIEMENS SMS-AX ACQ 1.0	Table Coordinates	SS	3
(0021,xx57)	SIEMENS SMS-AX ACQ 1.0	Iso Center Table Position	SS	1
(0021,xx5B)	SIEMENS SMS-AX ACQ 1.0	Table Coordinates System	FL	12
(0021,xx81)	SIEMENS SMS-AX ACQ 1.0	Table Tilt	SS	1
(0021,xx82)	SIEMENS SMS-AX ACQ 1.0	Table Rotation	SS	1
(0021,xx83)	SIEMENS SMS-AX ACQ 1.0	Table Cradle Tilt	SS	1
(0021,xxF0)	SIEMENS SMS-AX ACQ 1.0	XML parameters 3D	UT	1
(0023,xx08)	SIEMENS SMS-AX QUANT 1.0	Calibration TOD Value	IS	1
(0025,xx00)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	View Native	US	1
(0025,xx01)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Series Number	US	1
(0025,xx02)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Image Number	US	1
(0025,xx03)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Win Center	US	1
(0025,xx04)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Win Width	US	1
(0025,xx05)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Win Brightness	US	1
(0025,xx06)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Win Contrast	US	1
(0025,xx07)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Frame Number	US	1
(0025,xx08)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Mask Frame Number	US	1
(0025,xx09)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Opac	US	1
(0025,xx0A)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Number of Frames	US	1
(0025,xx0B)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Scene Duration	DS	1
(0025,xx0C)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Identifier LOID	LO	1
(0025,xx0D)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Scene VFR Info	SS	1-n
(0025,xx0E)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Original Frame ECG Position	SS	1
(0025,xx10)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Zoom Flag	SS	1
(0025,xx11)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Flexible Pixel Shift	US	1
(0025,xx12)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Number of Mask Frames	US	1
(0025,xx13)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Number of Fill Frames	US	1
(0025,xx14)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Series Number	IS	1
(0025,xx15)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Image Number	IS	1
(0025,xx16)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	Ready Processing Status	IS	1
(0029,xx08)	SIEMENS MEDCOM HEADER	MedCom Header Type	CS	1
(0029,xx09)	SIEMENS MEDCOM HEADER	MedCom Header Version	LO	1
(0029,xx10)	SIEMENS MEDCOM HEADER	MedCom Header Info	OB	1
(0029,xx20)	SIEMENS MEDCOM HEADER	MedCom History Information	OB	1
(0029,xx31)	SIEMENS MEDCOM HEADER	PMTF Information 1	LO	1
(0029,xx32)	SIEMENS MEDCOM HEADER	PMTF Information 2	UL	1
(0029,xx33)	SIEMENS MEDCOM HEADER	PMTF Information 3	UL	1
(0029,xx34)	SIEMENS MEDCOM HEADER	PMTF Information 4	CS	1
(0029,xx35)	SIEMENS MEDCOM HEADER	PMTF Information 5	UL	1
(0029,xx40)	SIEMENS MEDCOM HEADER	Application Header Sequence	SQ	1
(0029,xx41)	SIEMENS MEDCOM HEADER	Application Header Type	CS	1
(0029,xx42)	SIEMENS MEDCOM HEADER	Application Header ID	LO	1
(0029,xx43)	SIEMENS MEDCOM HEADER	Application Header Version	LO	1
(0029,xx44)	SIEMENS MEDCOM HEADER	Application Header Info	OB	1
(0029,xx50)	SIEMENS MEDCOM HEADER	Workflow Control Flags	LO	8
(0029,xx51)	SIEMENS MEDCOM HEADER	Arch. Management Flag Keep Online	CS	1
(0029,xx52)	SIEMENS MEDCOM HEADER	Arch. Mgmnt Flag Do Not Archive	CS	1
(0029,xx53)	SIEMENS MEDCOM HEADER	Image Location Status	CS	1
(0029,xx54)	SIEMENS MEDCOM HEADER	Estimated Retrieve Time	DS	1
(0029,xx55)	SIEMENS MEDCOM HEADER	Data Size of Retrieved Images	DS	1
(0029,xx08)	SIEMENS MEDCOM OOG	MedCom OOG Type	CS	1
(0029,xx09)	SIEMENS MEDCOM OOG	MedCom OOG Version	LO	1

Tag	Private Owner Code	Name	VR	VM
(0029,xx10)	SIEMENS MEDCOM OOG	MedCom OOG Info	OB	1
(0063,xx42)	SIEMENS SMS-AX Segmentation Extensions	Object GUID	LO	1
(0063,xx48)	SIEMENS SMS-AX Segmentation Extensions	Private Segmentation Sequence	SQ	1
(0067,xx00)	SIEMENS SMS-AX Surface Segmentation Extensions	Object Type	CS	1
(0067,xx01)	SIEMENS SMS-AX Surface Segmentation Extensions	Object IAE Display	CS	1
(0067,xx02)	SIEMENS SMS-AX Surface Segmentation Extensions	Object Live Display	CS	1
(0067,xx03)	SIEMENS SMS-AX Surface Segmentation Extensions	Object Labeling	CS	1
(0067,xx04)	SIEMENS SMS-AX Surface Segmentation Extensions	SSO Version Number	US	1
(0067,xx05)	SIEMENS SMS-AX Surface Segmentation Extensions	EP Point Ablated	CS	1
(0067,xx09)	SIEMENS SMS-AX Surface Segmentation Extensions	Show Length	CS	1
(0067,xx10)	SIEMENS SMS-AX Surface Segmentation Extensions	Polyline Shape	CS	1
(0067,xx11)	SIEMENS SMS-AX Surface Segmentation Extensions	Polyline Style	CS	1
(0067,xx13)	SIEMENS SMS-AX Surface Segmentation Extensions	Clipping	CS	1
(0067,xx14)	SIEMENS SMS-AX Surface Segmentation Extensions	Show Volume	CS	1
(0067,xx27)	SIEMENS SMS-AX Surface Segmentation Extensions	Object Volume Assignment	CS	1
(0067,xx35)	SIEMENS SMS-AX Surface Segmentation Extensions	Group Show	CS	1
(0067,xx36)	SIEMENS SMS-AX Surface Segmentation Extensions	Group IAE Display	CS	1
(0067,xx37)	SIEMENS SMS-AX Surface Segmentation Extensions	Group Live Display	CS	1
(0067,xx38)	SIEMENS SMS-AX Surface Segmentation Extensions	Group Volume Assignment	CS	1
(0067,xx39)	SIEMENS SMS-AX Surface Segmentation Extensions	Object Version Number	US	1
(0067,xx40)	SIEMENS SMS-AX Surface Segmentation Extensions	SSO Owner	LO	1
(0067,xx42)	SIEMENS SMS-AX Surface Segmentation Extensions	Object GUID	LO	1
(0067,xx43)	SIEMENS SMS-AX Surface Segmentation Extensions	Group GUID	LO	1
(0067,xx44)	SIEMENS SMS-AX Surface Segmentation Extensions	SSO GUID	LO	1
(0067,xx47)	SIEMENS SMS-AX Surface Segmentation Extensions	Group Sequence	SQ	1
(0067,xx48)	SIEMENS SMS-AX Surface Segmentation Extensions	Private Surface Segmentation Sequence	SQ	1
(0067,xx49)	SIEMENS SMS-AX Surface Segmentation Extensions	Group Name	LO	1
(0067,xx51)	SIEMENS SMS-AX Surface Segmentation Extensions	Referenced Group GUID	LO	1
(0067,xx53)	SIEMENS SMS-AX Surface Segmentation Extensions	Private Surface Mesh Sequence	SQ	1
(0067,xx54)	SIEMENS SMS-AX Surface Segmentation Extensions	Surface Show	CS	1

(0067,xx56)	SIEMENS SMS-AX Surface Segmentation Extensions	Surface Mean Diameter List	OF	1
(0067,xx57)	SIEMENS SMS-AX Surface Segmentation Extensions	Primary Angle	DS	1
(0067,xx58)	SIEMENS SMS-AX Surface Segmentation Extensions	Secondary Angle	DS	1
(0067,xx59)	SIEMENS SMS-AX Surface Segmentation Extensions	Centerline ID List	LT	1
(0067,xx60)	SIEMENS SMS-AX Surface Segmentation Extensions	Landmark ID List	LT	1
(0067,xx61)	SIEMENS SMS-AX Surface Segmentation Extensions	Surface Text Label	LO	1
(0067,xx62)	SIEMENS SMS-AX Surface Segmentation Extensions	Centerline Visualization Type	CS	1
(0067,xx64)	SIEMENS SMS-AX Surface Segmentation Extensions	MPR Views	UT	1
(0067,xx65)	SIEMENS SMS-AX Surface Segmentation Extensions	Fixed Line Thickness	CS	1
(2121,xx01)	PMI Private Calibration Module Version 2.0	Calibration Method	ST	1
(2121,xx02)	PMI Private Calibration Module Version 2.0	Calibration Method Info	ST	1
(2121,xx03)	PMI Private Calibration Module Version 2.0	Calibration Object Size	FL	1
(2121,xx04)	PMI Private Calibration Module Version 2.0	Calibration Object S Dev	FL	1
(2121,xx05)	PMI Private Calibration Module Version 2.0	Calibration Horizontal Pixel Spacing	FL	1
(2121,xx06)	PMI Private Calibration Module Version 2.0	Calibration Vertical Pixel Spacing	FL	1
(2121,xx08)	PMI Private Calibration Module Version 2.0	Calibration File Name	ST	1
(2121,xx09)	PMI Private Calibration Module Version 2.0	Calibration Frame Number	IS	1
(2121,xx0A)	PMI Private Calibration Module Version 2.0	Calibration Object Unit	SH	1
(2121,xx0B)	PMI Private Calibration Module Version 2.0	Averaged Calibrations Performed	SS	1
(2121,xx0C)	PMI Private Calibration Module Version 2.0	Auto Magnify Factor	FL	1
(2121,xx0D)	PMI Private Calibration Module Version 2.0	Horizontal Pixel S Dev	FL	1
(2121,xx0E)	PMI Private Calibration Module Version 2.0	Vertical Pixel S Dev	FL	1
(2121,xx01)	PMI Private 3D Reconstruction Attributes Version 1.0	Binary 3D Vessel Data	OB	1
(2121,xx02)	PMI Private 3D Reconstruction Attributes Version 1.0	3D Control Displayed Area Sequence	SQ	1
(2121,xx03)	PMI Private 3D Reconstruction Attributes Version 1.0	3D Control Displayed Area Top Left Corner	SL	2
(2121,xx04)	PMI Private 3D Reconstruction Attributes Version 1.0	3D Control Displayed Area Bottom Right Corner	SL	2
(7FE1,xx10)	SIEMENS CSA NON-IMAGE	CSA Data	OB	1

Note: Please be informed that some of the Private Owner Codes contain double-spaces in the name definitions.

The following term (only double-spaces marked) are defined:

SIEMENS SMS-AX<spc><spc>VIEW 1.0

SIEMENS SMS-AX<spc><spc>QUANT 1.0

SIEMENS SMS-AX<spc><spc>ACQ 1.0

(All spaces not specially marked, are single spaces.)

8.3 Coded Terminology and Templates

8.3.1 Context Groups

Context Group	Default Value Set	Configurable	Use
Scoliosis Types	CID Cx01	No	Choose from list

Orthopedic Measurement Types	CID Cx02	No	Choose from list
Vertebra Descriptors	CID Cx03	No	Choose from list
Scoliosis Location	CID Cx04	No	Choose from list
Scoliosis Direction	CID Cx05	No	Choose from list

8.3.1.1 Orthopedic Report Context Groups

CID Cx01 Scoliosis Types

**Table 69 - CID Cx01
Scoliosis Types
Type: Extensible**

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
99SMS_OR	ORx50007-0	Unknown
99SMS_OR	ORx50007-1	Structural
99SMS_OR	ORx50007-2	Functional

CID Cx02 Orthopedic Measurement Types

**Table 70 - CID Cx02
Orthopedic Measurement Types
Type: Extensible**

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
99SMS_OR	ORx50100	Vertical Alignment
99SMS_OR	ORx50200	Cobb Angle
99SMS_OR	ORx50200-1	Cobb Angle Measurement
99SMS_OR	ORx50300	Kyphosis Angle
99SMS_OR	ORx50300-1	Kyphosis Angle Measurement
99SMS_OR	ORx50400	Height Difference
99SMS_OR	ORx50500	Angle
99SMS_OR	ORx50500-1	Angle Measurement
99SMS_OR	ORx50600	Distance
99SMS_OR	ORx50700	Area Measurement

CID Cx03 Vertebra Descriptors

**Table 71 - CID Cx03
Vertebra Descriptors
Type: Extensible**

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
99SMS_OR	ORx50005-0	Unknown
99SMS_OR	ORx50005-1	C1
99SMS_OR	ORx50005-2	C2
99SMS_OR	ORx50005-3	C3
99SMS_OR	ORx50005-4	C4
99SMS_OR	ORx50005-5	C5
99SMS_OR	ORx50005-6	C6
99SMS_OR	ORx50005-7	C7
99SMS_OR	ORx50005-8	T1
99SMS_OR	ORx50005-9	T2

99SMS_OR	ORx50005-10	T3
99SMS_OR	ORx50005-11	T4
99SMS_OR	ORx50005-12	T5
99SMS_OR	ORx50005-13	T6
99SMS_OR	ORx50005-14	T7
99SMS_OR	ORx50005-15	T8
99SMS_OR	ORx50005-16	T9
99SMS_OR	ORx50005-17	T10
99SMS_OR	ORx50005-18	T11
99SMS_OR	ORx50005-19	T12
99SMS_OR	ORx50005-20	L1
99SMS_OR	ORx50005-21	L2
99SMS_OR	ORx50005-22	L3
99SMS_OR	ORx50005-23	L4
99SMS_OR	ORx50005-24	L5

CID Cx04 Scoliosis Location

Table 72 - CID Cx04
Scoliosis Location
Type: Extensible

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
99SMS_OR	ORx50008-0	Unknown
99SMS_OR	ORx50008-1	Cervical
99SMS_OR	ORx50008-2	Thoracic
99SMS_OR	ORx50008-3	Lumbar

CID Cx05 Scoliosis Direction

Table 73 - CID Cx05
Scoliosis Direction
Type: Extensible

Coding Scheme Designator (0008,0102)	Code Value (0008,0100)	Code Meaning (0008,0104)
99SMS_OR	ORx50009-0	Unknown
99SMS_OR	ORx50009-1	Right Convex
99SMS_OR	ORx50009-2	Left Convex

8.3.2 Template Specifications

8.3.2.1 Orthopedic Report Template

The Orthopedic Report Templates are deployed according to the following structure:

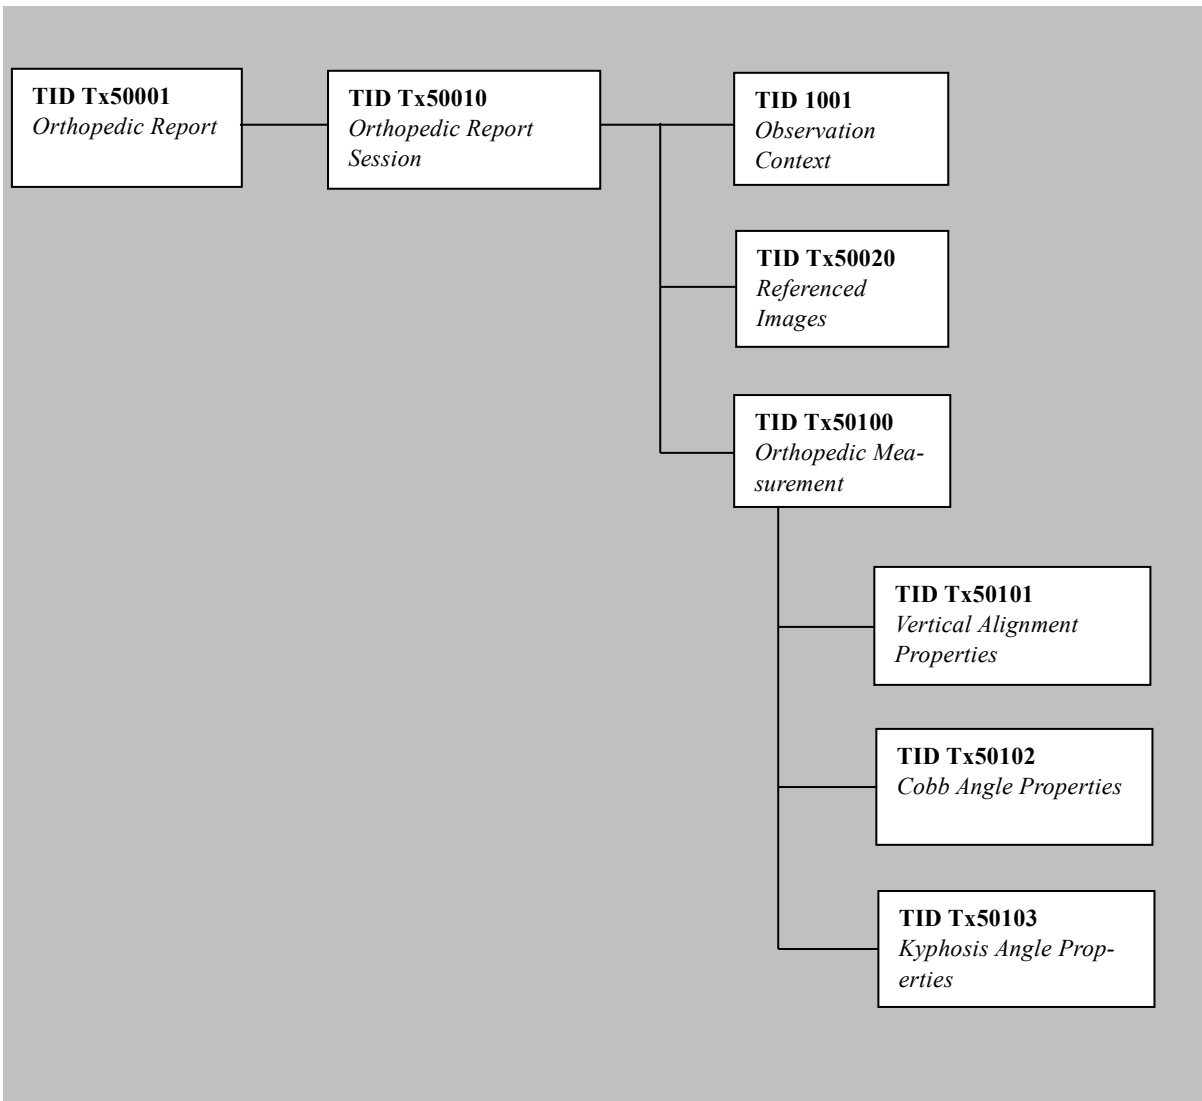


Table 74 - (Private) Orthopedic Report Template

TID Tx50001 Orthopedic Report

This template defines a container (the root) with subsidiary content items, each of which represents a single orthopedic Reporting Session.

Table 75 - TID Tx50001
Orthopedic Report
Type: Extensible

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			CONTAINER	EV (ORx50001, 99SMS_COMP, "Orthopedic Report")	1	M		Root node
2	>	CONTAINS	INCLUDE	DTID (Tx50010) Orthopedic Report Session	1-n	M		

TID Tx50010 Orthopedic Report Session

This general template provides detailed information on an Orthopedic Measurement Session. This includes the Observation Context (Observer as well as Subject and Procedure Context).

**Table 76 - TID Tx50010
Orthopedic Report Session
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			CONTAINER	EV (ORx50002, 99SMS_COMP, "Orthopedic Report Session")	1	M		
2	>	CONTAINS	INCLUDE	DTID(1001) Observation Context	1	M		
3	>	CONTAINS	INCLUDE	DTID (Tx50020) Referenced Images	1	M		
4	>	CONTAINS	INCLUDE	DTID (Tx50100) Orthopedic Measurements	1	U		\$Measurement = DCID (Cx02)
5	>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	1-n	U		

Content Item Descriptions

1	Observation Date Time (0040,A032) of container needs to be flagged with the time of the session performed
3	Only reference to images used in this session.
5	Comment summary for the report session "as a whole" shall be provided in this content item

Observation Context usage

The following templates are extracted from DICOM Part 16 in order to document Content Item Descriptions as those apply for the usage of Observation Context in Orthopedic Reports.

**Table 77 – TID 1002
OBSERVER CONTEXT
Type: Non-Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1		HAS OBS CONTEXT	CODE	EV (121005,DCM, "Observer Type")	1	MC	IF Observer Type is device	DCID (270) Observer Type Defaults to (121006,DCM, "Person")
.

Content Item Descriptions

1	Observer Type used in Orthopedic Report is "Person"
---	---

**Table 78 - TID 1003
PERSON OBSERVER IDENTIFYING ATTRIBUTES
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			PNAME	EV (121008,DCM, "Person Observer Name")	1	M		
.

Content Item Descriptions

1	will be filled with the observer name selected at the creation of the report
---	--

**Table 79 - TID 1005
PROCEDURE CONTEXT
Type: Non-Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			UIDREF	EV (121018, DCM, "Procedure Study Instance UID")	1	U		Defaults to Study Instance UID (0020,000D) of General Study Module
.
5			TEXT	EV(121022,DCM, "Procedure Accession Number")	1	U		Defaults to (0008,0050)
.

Content Item Descriptions

1	will be filled with the Study Instance UID from the first composed image referenced by the report
5	will be filled from the study containing the images referenced by the report session

**Table 80 - TID 1006
SUBJECT CONTEXT
Type: Non-Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			CODE	EV (121024, DCM, "Subject Class")	1	M	IF subject is not the Patient	DCID (271) Observation Subject Class Defaults to (121025, DCM, "Patient")
.

Content Item Descriptions

1	Subject Class used in Orthopedic Report is "Person"
---	---

**Table 81 - TID 1007
SUBJECT CONTEXT, PATIENT
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
.
2			PNAME	EV (121029,DCM, "Subject Name")	1	MC	Required if not inherited	
3			CODE	EV (121030,DCM, "Subject ID")	1	MC	Required if not inherited	
4			DATE	EV (121031,DCM, "Subject Birth Date")	1	U		
5			CODE	EV (121032,DCM, "Subject Sex")	1	U		DCID (7455) Sex
6			NUM	EV (121033,DCM, "Subject Age")				Units DCID (7456) Units of Measure for Age
.

Content Item Descriptions

2	will be filled with Patient's Name of the patient being reported on
3	will be filled with Patient ID of the patient being reported on

4	will be filled with Patient Birth Date of the patient being reported on
5	will be filled with Patient's Sex of the patient being reported on
6	will be filled with Patient's Age of the patient being reported on

TID Tx50020 Referenced Images

This general template provides reference to image instances related to an Orthopedic Measurement Session.

**Table 82 - TID Tx50020
Referenced Images
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			CONTAINER	EV (ORx50003, 99SMS_COMP, "Referenced Images")	1	M		
2	>	CONTAINS	IMAGE	EV(121112, DCM, "Source of Measurement")	1-n	M		
3	>>	HAS CONCEPT MOD	TEXT	EV (ORx50003-1, 99SMS_COMP, "Image Number")	1	U		

Content Item Descriptions

2	One content item for each image referenced
3	Image Number as set in referenced instance

TID Tx50100 Orthopedic Measurements

This general template provides information on the measurement results derived during the performance of an Orthopedic Report Session.

TID Tx50100 Parameters

\$Measurement	Coded Term of Orthopedic Measurement type
---------------	---

**Table 83 - TID Tx50100
Orthopedic Measurements
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1			CONTAINER	EV(121070, DCM, "Findings")	1	M		
2	>	CONTAINS	CONTAINER	EV(ORx50006, 99SMS_COMP, "Scoliosis")	1	MC	IFF Row 6 value = (ORx50200, 99SMS_COMP, "Cobb Angle")	
3	>>	CONTAINS	CODE	EV(ORx50007, 99SMS_COMP, "Scoliosis Type")	1	M		DCID (Cx01) Scoliosis Types
4	>>>	HAS PROPERTIES	TEXT	EV(121106, DCM, "Comment")	1	U		
5	>	CONTAINS	CONTAINER	EV(121424, DCM, "Table of	1-n	M		

				Values")				
6	>>	HAS CONCEPT MOD	CODE	EV(ORx50004, 99SMS_COMP, "Orthopedic Measurement")	1	U		\$Measurement
7	>>		INCLUDE	DTID Tx50101 Vertical Alignment Properties	1-n	MC	IFF Row 6 value = (ORx50100, 99SMS_COMP, "Vertical Alignment"	
8	>>		INCLUDE	DTID Tx50102 Cobb Angle Properties	1-n	MC	IFF Row 6 value = (ORx50200, 99SMS_COMP, "Cobb Angle"	
9	>>		INCLUDE	DTID Tx50103 Kyphosis Angle Properties	1-n	MC	IFF Row 6 value = (ORx50300, 99SMS_COMP, "Kyphosis Angle")	
1 0	>>	CONTAINS	NUM	\$Orthopedic Measurement (CID Cx02)	1-n	MC	XOR Row 6,7,8	
1 1	>>>	R-INFERRED FROM	IMAGE		1	M		
1 2	>>>	HAS PROPERTIES	TEXT	EV (ORx50004- 1, 99SMS_COMP, "Orthopedic Measurement Label")	1	M		
1 3	>>>	HAS PROPERTIES	TEXT	EV (121106, DCM, "Comment")	1	U		
1 4	>>	CONTAINS	TEXT	EV (121106, DCM, "Comment")	1	U		

Content Item Descriptions

5 - 9	includes one container for each type of measurement in the report (i.e. Vertical Alignments, Cobb Angles, Kyphosis Angles, Other Measurements)
10	Value of non-Scoliosis type measurement (e.g. distance measurement in mm or area measurement in cm ²)
11	Reference to image used to measure numeric value specified in Row 10.
12	Label that uniquely identifies the measurement within the image containing it (e.g. HD 1 for a height difference).
13	Free text comment related to this measurement.
14	Free text comment relating to this entire Orthopedic Measurement report

TID Tx50101 Vertical Alignment Properties

This general template provides detailed information on Vertical Alignment Properties derived during an Orthopedic Measurement Session.

**Table 84 - TID Tx50101
Vertical Alignment Properties
Type: Extensible**

NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
----	-----------------	----	--------------	----	----------	-----------	----------------------

1		CONTAINS	NUM	EV (ORx50100, 99SMS_COMP, "Vertical Alignment")	1	M		UNITS = EV (cm, UCUM "centimeter")
2	>	R-INFERRED FROM	IMAGE		1	M		
3	>	HAS PROPERTIES	TEXT	EV (ORx50004-1, 99SMS_COMP, "Orthopedic Measurement Label")	1	M		
4	>	HAS PROPERTIES	CODE	EV (ORx50005, 99SMS_COMP, "Vertebra")	1	U		DCID (Cx03) Vertebra Descriptors
5	>	HAS PROPERTIES	TEXT	EV (121106, DCM, "Comment")	1	U		

Content Item Descriptions

2	Reference to the image this measurement is derived from.
3	Unique identifier for this measurement. "VA 1" to "VA n".
4	Vertebra descriptor indicating the vertebra associated with this vertical alignment.
5	A free-text comment about this vertical alignment measurement.

TID Tx50102 Cobb Angle Properties

This general template provides detailed information on Cobb Angle Properties derived during an Orthopedic Measurement Session.

**Table 85 - TID Tx50102
Cobb Angle Properties
Type: Extensible**

NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1	CONTAINS	NUM	EV (ORx50200, 99SMS_COMP, "Cobb Angle")	1	M		UNITS = EV (deg, UCUM "degrees")
2	>	R-INFERRED FROM	IMAGE	1	M		
3	>	HAS PROPERTIES	TEXT	EV (ORx50004-1, 99SMS_COMP, "Orthopedic Measurement Label")	1	M	
4	>	HAS PROPERTIES	CODE	EV (ORx50005, 99SMS_COMP, "Vertebra")	1	U	DCID (Cx03) Vertebra Descriptors
5	>	HAS PROPERTIES	CODE	EV (ORx50009, 99SMS_COMP, "Scoliosis Direction")	1	U	DCID (Cx05) Scoliosis Direction
6	>	HAS PROPERTIES	TEXT	EV (121106, DCM, "Comment")	1	U	

Content Item Descriptions

2	Reference to the image this measurement is derived from.
3	Unique identifier for this measurement. "CB 1,2", "CB 2,3" to "CB n-1,n".
4	Vertebra descriptor indicating the vertebra associated with this Cobb angle.
5	Indicator of the direction of this scoliosis.
6	A free-text comment about this Cobb angle measurement.

TID Tx50103 Kyphosis Angle Properties

This general template provides detailed information on Kyphosis Angle Properties derived during an Orthopedic Measurement Session.

**Table 86 - TID Tx50103
Kyphosis Angle Properties
Type: Extensible**

	NL	Rel with Parent	VT	Concept Name	VM	Req-Type	Condition	Value Set Constraint
1		CONTAINS	NUM	EV (ORx50300, 99SMS_COMP, "Kyphosis Angle")	1	M		UNITS = EV (deg, UCUM "degrees")
2	>	R-INFERRED FROM	IMAGE		1	M		
3	>	HAS PROPERTIES	TEXT	EV (ORx50004-1, 99SMS_COMP, "Orthopedic Measurement Label")	1	M		
4	>	HAS PROPERTIES	CODE	EV (ORx50005, 99SMS_COMP, "Vertebra")	1	U		DCID (Cx03) Vertebra Descriptors
5	>	HAS PROPERTIES	TEXT	EV (121106, DCM, "Comment")	1	U		

Content Item Descriptions

2	Reference to the image this measurement is derived from.
3	Unique identifier for this measurement. "Ky 1" to "Ky n".
4	Vertebra descriptor indicating the vertebra associated with this Kyphosis angle.
6	A free-text comment about this Kyphosis angle measurement.

8.3.3 Private Code Definitions

Please refer to the Template Specification and Context Groups sections for details on private codes introduced by syngo X Workplace applications.

8.4 Grayscale Image Consistency

The high resolution TFT display monitor option of syngo X Workplace comes with a DICOM Grayscale Standard Display Function (GSDf) compliant factory pre-setting. A typical working environment setup is assumed for ambient light.

8.5 Standard Extended/Specialized/Private SOP Classes

8.5.1 Standard Extended XA

The XA SOP Instances created by syngo X Workplace are standard extended by adding the following private module attributes.

Table 87 - Private Modules for Standard Extended XA

IE	Module	Reference	Usage	Note
Image	Angio Viewing	8.5.1.1	U	private Viewing information

© Siemens Healthcare GmbH. 2020. All rights reserved.

	Angio Quantification	8.5.1.2	U	if image is calibrated for Quant
	Original Image Info	8.5.1.3	U	if derived image

U = User Option

8.5.1.1 Angio Viewing Module

Table 88 - (Private) Angio Viewing Module Attributes

Attribute Name	Tag	Owner	Type	Notes
Review Mode	(0019,xx00)	SIEMENS SMS-AX VIEW 1.0	3	Special Modes for Angio Review. Defined Terms are 1 = REV_MAXFILL, 2 = REV_LOOP, 3 = REV_SCROLL, 4 = REV_STEREO_LOOP
Anatomical Background Percent	(0019,xx01)	SIEMENS SMS-AX VIEW 1.0	3	Percentage of Mix between Subtracted Image Result and Native Mask. Range is from 0 to 100.
Number of Phases	(0019,xx02)	SIEMENS SMS-AX VIEW 1.0	3	1-4 (1 or # of "Variable Frame Rate" acq phases)
Apply Anatomical Background	(0019,xx03)	SIEMENS SMS-AX VIEW 1.0	3	
Pixel Shift Array	(0019,xx04)	SIEMENS SMS-AX VIEW 1.0	3	4 * Number of Frames (0028,0008)
Brightness	(0019,xx05)	SIEMENS SMS-AX VIEW 1.0	3	SUB windowing
Contrast	(0019,xx06)	SIEMENS SMS-AX VIEW 1.0	3	SUB windowing
Enabled Shutter	(0019,xx07)	SIEMENS SMS-AX VIEW 1.0	3	Visualize shutter
Native Edge Enhancement Percent Gain	(0019,xx08)	SIEMENS SMS-AX VIEW 1.0	3	Percent gain for native display of images.
Native Edge Enhancement LUT Index	(0019,xx09)	SIEMENS SMS-AX VIEW 1.0	3	
Native Edge Enhancement Kernel Size	(0019,xx0A)	SIEMENS SMS-AX VIEW 1.0	3	
Subtracted Edge Enhancement Percent Gain	(0019,xx0B)	SIEMENS SMS-AX VIEW 1.0	3	Percent gain for subtracted display of images.
Subtracted Edge Enhancement LUT Index	(0019,xx0C)	SIEMENS SMS-AX VIEW 1.0	3	
Subtracted Edge Enhancement Kernel Size	(0019,xx0D)	SIEMENS SMS-AX VIEW 1.0	3	
Fade Percent	(0019,xx0E)	SIEMENS SMS-AX VIEW 1.0	3	
Flipped before Laterality Applied	(0019,xx0F)	SIEMENS SMS-AX VIEW 1.0	3	
Apply Fade	(0019,xx10)	SIEMENS SMS-AX VIEW 1.0	3	
Zoom	(0019,xx12)	SIEMENS SMS-AX VIEW 1.0	3	
Pan X	(0019,xx13)	SIEMENS SMS-AX VIEW 1.0	3	
Pan Y	(0019,xx14)	SIEMENS SMS-AX VIEW 1.0	3	
Native Edge Enhancement Adverse Percent Gain	(0019,xx15)	SIEMENS SMS-AX VIEW 1.0	3	
Subtracted Edge Enhancement Adverse Percent Gain	(0019,xx16)	SIEMENS SMS-AX VIEW 1.0	3	
Invert Flag	(0019,xx17)	SIEMENS SMS-	3	

Attribute Name	Tag	Owner	Type	Notes
		AX VIEW 1.0		
Quant 1K Overlay	(0019,xx1A)	SIEMENS SMS-AX VIEW 1.0	3	Only Store Monitor and Store Reference Images in Quant (128 kbyte)
Acquisition Size	(0019,xx1B)	SIEMENS SMS-AX VIEW 1.0	3	
Auto Window Center	(0019,xx1C)	SIEMENS SMS-AX VIEW 1.0	3	
Auto Window Width	(0019,xx1D)	SIEMENS SMS-AX VIEW 1.0	3	
Auto Window Correct Value	(0019,xx1E)	SIEMENS SMS-AX VIEW 1.0	3	
Sigmoid Window Parameter	(0019,xx1F)	SIEMENS SMS-AX VIEW 1.0	3	
Roadmap Catheter Contrast	(0019,xx20)	SIEMENS SMS-AX VIEW 1.0	3	
Roadmap Vessel Contrast	(0019,xx21)	SIEMENS SMS-AX VIEW 1.0	3	
CLEARstent ROI Origin	(0019,xx23)	SIEMENS SMS-AX VIEW 1.0	3	
CLEARstent ROI Size	(0019,xx24)	SIEMENS SMS-AX VIEW 1.0	3	
Frame Number Roadmap - Min Amplification	(0019,xx30)	SIEMENS SMS-AX VIEW 1.0	3	
Frame Number Roadmap - Vessel Map	(0019,xx31)	SIEMENS SMS-AX VIEW 1.0	3	
Pixel Shift Values	(0019,xx41)	SIEMENS SMS-AX VIEW 1.0	3	
Pixel Shift Indicator	(0019,xx42)	SIEMENS SMS-AX VIEW 1.0	3	
Applied Pixel Shift Values	(0019,xx43)	SIEMENS SMS-AX VIEW 1.0	3	
Pixel Shift Validity	(0019,xx44)	SIEMENS SMS-AX VIEW 1.0	3	
Edge Enhancement LUT Data - nat	(0019,xx81)	SIEMENS SMS-AX VIEW 1.0	3	LUT data for edge enhancement – native view
Edge Enhancement LUT Data - sub	(0019,xx82)	SIEMENS SMS-AX VIEW 1.0	3	LUT data for edge enhancement – subtracted view
asymmetric Edge Enh. Kernel Size	(0019,xx83)	SIEMENS SMS-AX VIEW 1.0	3	kernel size for asymmetric edge enhancement

8.5.1.2 Angio Quantification Module

The table in this section contains private IOD Elements that describe additional Attributes for advanced Angio Quantification and Calibration Results features.

Table 89 - (Private) Angio Quantification Module Attributes

Attribute Name	Tag	Owner	Type	Notes
Calibration TOD Value	(0023,xx08)	SIEMENS SMS-AX QUANT 1.0	3	Table Object Distance in cm
Calibration Method	(2121,xx01)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Method Info	(2121,xx02)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Object Size	(2121,xx03)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant

Calibration Object S Dev	(2121,xx04)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Horizontal Pixel Spacing	(2121,xx05)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Vertical Pixel Spacing	(2121,xx06)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Frame Number	(2121,xx08)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Object Unit	(2121,xx09)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Averaged Calibrations Performed	(2121,xx0A)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Auto Magnify Factor	(2121,xx0B)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Horizontal Pixel S Dev	(2121,xx0C)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Vertical Pixel S Dev	(2121,xx0D)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Calibration Method	(2121,xx0E)	PMI Private Calibration Module Version 2.0	3	Only for images calibrated for Quant
Binary 3D Vessel Data	(2121,xx01)	PMI Private 3D Reconstruction Attributes Version 1.0	3	Only for Quant 3D models
3D Control Displayed Area Sequence	(2121,xx02)	PMI Private 3D Reconstruction Attributes Version 1.0	3	Only for Quant 3D models
>3D Control Displayed Area Top Left Corner	(2121,xx03)	PMI Private 3D Reconstruction Attributes Version 1.0	3	Only for Quant 3D models
>3D Control Displayed Area Bottom Right Corner	(2121,xx04)	PMI Private 3D Reconstruction Attributes Version 1.0	3	Only for Quant 3D models

8.5.1.3 Original Image Info Module

The table in this section contains private IOD Attributes that describe additional original image data for derived images (e.g. Store Monitor Image).

Table 90 - (Private) Original Image Info Module Attributes

Attribute Name	Tag	Owner	Type	Notes
View Native	(0025,xx00)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Original Series Number	(0025,xx01)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Original Image Number	(0025,xx02)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Win Center	(0025,xx03)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Win Width	(0025,xx04)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Win Brightness	(0025,xx05)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Win Contrast	(0025,xx06)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Original Frame Number	(0025,xx07)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Original Mask Frame Number	(0025,xx08)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Opac	(0025,xx09)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	

Original Number of Frames	(0025,xx0A)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Original Scene Duration	(0025,xx0B)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Image Object ID	(0025,xx0C)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	Set to "AXIM_READY_PROCESSED" when Ready Processing was applied
Original Scene VFR Info	(0025,xx0D)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	Number of phases, then followed by n pairs (Last Frame Number, then Frame Rate)
Original Frame ECG Position	(0025,xx0E)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Zoom Flag	(0025,xx10)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Flexible Pixel Shift	(0025,xx11)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Number of Mask Frames	(0025,xx12)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Number of Fill Frames	(0025,xx13)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Series Number	(0025,xx14)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Image Number	(0025,xx15)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	
Ready Processing Status	(0025,xx16)	SIEMENS SMS-AX ORIGINAL IMAGE INFO 1.0	3	1 = ready processed, 2 = resized, 3 = both 4 = resize 14 to 16 bit (rotational images) 5 = acquired with 16 bit (rotational images)

8.5.2 Standard Extended Segmentation

Any Segmentation SOP Instances created by syngo X Workplace can be standard extended by adding the following syngo private module attributes.

Table 91 - Private Modules for other created SOP Class

IE	Module	Reference	Usage	Note
Image	Private Surface Segmentation	8.5.2.1	U	Private Segmentation information

U = User Option

8.5.2.1 Private Segmentation

The table in this section contains private IOD Attributes that describe the Private Segmentation information:

Table 92 – Private Segmentation Attributes

Attribute Name	Tag	Owner	Type	Notes
SSO GUID	(0063,xx42)	SIEMENS SMS-AX Segmentation Extensions	3	Global ID for the Segmentation object.

8.5.3 Standard Extended Surface Segmentation

Any Surface Segmentation SOP Instances created by syngo X Workplace can be standard extended by adding the following syngo private module attributes.

Table 93 - Private Modules for other created SOP Class

IE	Module	Reference	Usage	Note
Surface	Private Surface Segmentation	8.5.3.1	U	Private Surface Segmentation information

U = User Option

8.5.3.1 Private Surface Segmentation

The table in this section contains private IOD Attributes that describe the Private Surface Segmentation information:

Table 94 – Private Segmentation Attributes

Attribute Name	Tag	Owner	Type	Notes
SSO Version Number	(0067,xx04)	SIEMENS SMS-AX Surface Segmentation Extensions	3	The version is an increasing number.
SSO Owner	(0067,xx40)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines component that created the SSO.
SSO GUID	(0067,xx44)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Global ID for the SSO.
Group Sequence	(0067,xx47)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Shall contain Group related information. Contains at least 1 item
>Recommended Display CIELab Value	(0062,000D)	n.a.	3	Triplet value to define how this Group shall be rendered on a color display. The units are in PCSValues and the value encoding is CIELab.
>Recommended Presentation Opacity	(0066,000C)	n.a.	3	Defines the opacity of the Group in percent. Float value between 0.0 ("0% opaqueness") and 1.0 ("100% opaqueness").
>Group Show	(0067,xx35)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Group is hidden or not. Defined Terms: ON OFF
>Group IAE Display	(0067,xx36)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Group is shown on the IAE image area. Defined Terms: NONE ON OFF
>Group Live Display	(0067,xx37)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Group is shown on the Live image area. Defined Terms: NONE ON OFF
>Group Volume Assignment	(0067,xx38)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Group is shown on the registered volume(s). Defined Terms: REGISTERED PLANNING
>Group GUID	(0067,xx43)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Global ID for the Group
>Group Name	(0067,xx49)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Name of the group.
Private Surface Segmentation Sequence	(0067,xx48)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Sequence which contains private extensions for the Surface Segmentation Module. One Item for each item in the Segment Sequence.
>Object Type	(0067,xx00)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines the type of the Object. Defined Terms

Attribute Name	Tag	Owner	Type	Notes
		tion Extensions		POLYLINE MARKER NEEDLE EP ABLATION PT SEGMENTATION VESSEL VESSEL LANDMARK VERTEBRA CENTER EMPTY_OBJ Note: "EMPTY_OBJ" is used in a (dummy) object version in case all the containing (graphical) objects of this SSO have been deleted by the user.
>Object IAE Display	(0067,xx01)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Object is shown on the IAE image area. Defined Terms: NONE ON OFF
>Object Live Display	(0067,xx02)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Object is shown on the Live image area. Defined Terms: NONE ON OFF
>Object Labeling	(0067,xx03)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines whether the Object labels are shown. Defined Terms: ON OFF
>EP Point Ablated	(0067,xx05)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines whether the EP Point is ablated or not. Defined Terms: ABLATED NOT ABLATED
>Show Length	(0067,xx09)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines whether the display of the length value is shown. Defined Terms: ON OFF
>Polyline Shape	(0067,xx10)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines the shape of a polyline. Defined Terms: LINEAR CURVED".
>Polyline Style	(0067,xx11)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines the style of a polyline. Defined Terms : OPEN CLOSED
>Clipping	(0067,xx13)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines whether clipping affects the Object or not. Defined Terms: ON OFF
>Show Volume	(0067,xx14)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines whether the display of the volume value is shown. Defined Terms: ON OFF
>Object Volume Assignment	(0067,xx27)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Object is shown on the registered volume(s). Defined Terms: REGISTERED PLANNING NONE
>Object Version	(0067,xx39)	SIEMENS SMS-AX	3	The Object version is an increasing number.

Attribute Name	Tag	Owner	Type	Notes
Number		Surface Segmentation Extensions		
>Object GUID	(0067,xx42)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Global ID for the Object
>Referenced Group GUID	(0067,xx51)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Value copied from GUID in the Group GUID (0067,xx43) attribute in the Group Sequence (0067,0047).
>Primary Angle	(0067,xx57)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Primary C-arm angle
>Secondary Angle	(0067,xx58)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Secondary C-arm angle
>Segment Algorithm Name	(0062,0009)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Name of the algorithm that was used to generate the Surface. Defined Terms: Stroke Segmentation Left Atrium Segmentation Model Based Left Atrium Segmentation Hybrid Model Based Left Atrium Segmentation Aortic Root Segmentation Coronary Vessel Aorta Vessel Vessel Tree Definition Vessel Tree Detection Vessel Feeder Detection
>Recommended Display CIE Lab Value	(0062,000D)	n.a.	3	Triplet value to define how this segment shall be rendered on a color display.
>Recommended Presentation Opacity	(0066,000C)	n.a.	3	Single unsigned value to define how the maximum pixel value of this segment shall be rendered on a grayscale display.
>Recommended Point Radius	(0066,0037)	n.a.	3	Specifies the radius of the vertex points defined in the Vertex Point Index List (0066,0025) with which it is recommended that the point be rendered.
>Recommended Line Thickness	(0066,0038)	n.a.	3	Specifies the thickness of each edge or line defined in the Edge Point Index List (0066,0024) or Line Sequence (0066,0028) with which it is recommended that the line be rendered.
Private Surface Mesh Sequence	(0067,xx53)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Sequence which contains private extensions for the Surface Mesh Module. One Item for each item in the Surface Sequence.
>Surface Show	(0067,xx54)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines if the Surface is shown or not. Defined Terms: NONE ON OFF
>Surface Mean Diameter List	(0067,xx56)	SIEMENS SMS-AX Surface Segmentation Extensions	3	List of mean diameters in mm.
>Centerline ID List	(0067,xx59)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Vessel object : 2 values (CenterlineSegID\ParentID)
>Landmark ID List	(0067,xx60)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Vessel Landmarks object: 2 values (LandmarkID\VesselSegmentID)
>Surface Text Label	(0067,xx61)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Text label

Attribute Name	Tag	Owner	Type	Notes
		tion Extensions		
>Centerline Visualization Type	(0067,xx62)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines how a Centerline is visualized. Defined Terms: NONE NORMAL COLOR CODED RULER
>MPR Views	(0067,xx64)	SIEMENS SMS-AX Surface Segmentation Extensions	3	XML structure
>Fixed Line Thickness	(0067,xx65)	SIEMENS SMS-AX Surface Segmentation Extensions	3	Defines a fixed line thickness. Defined Terms: SMALL MEDIUM LARGE

8.5.4 Standard Extended for other created SOP Class

Any SOP Instances created by syngo X Workplace can be standard extended by adding the following *syngo* private module attributes.

Table 95 - Private Modules for other created SOP Class

IE	Module	Reference	Usage	Note
Image	MEDCOM Header	8.5.4.1	U	private <i>syngo</i> information
	MEDCOM OOG	8.5.4.2	U	if object graphics is attached to image

U = User Option

8.5.4.1 MEDCOM Header

The table in this section contains private IOD Attributes that describe the MEDCOM Header:

Table 96 - MEDCOM Header Attributes

Attribute Name	Tag	Owner	Type	Notes
MedCom Header Type	(0029,xx08)	SIEMENS MED-COM HEADER	1C	MedCom Header identification characteristics. Defined Terms: MEDCOM 1 (Required if MedCom Header Info (0029,xx10) present.)
MedCom Header Version	(0029,xx09)	SIEMENS MED-COM HEADER	2C	Version of MedCom Header Info (0029,xx10) format. (Required if MEDCOM Header Info (0029,xx10) present.)
MedCom Header Info	(0029,xx10)	SIEMENS MED-COM HEADER	3	Manufacturer model dependent information. The value of the attribute MedCom Header Info (0029,xx10) can be build up in each user defined format.
MedCom History Information	(0029,xx20)	SIEMENS MED-COM HEADER	3	MedCom defined Patient Registration history information. See 8.5.4.1.1.
PMTF Information 1	(0029,xx31)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 2	(0029,xx32)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 3	(0029,xx33)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 4	(0029,xx34)	SIEMENS MED-COM HEADER	3	Transformation Information
PMTF Information 5	(0029,xx35)	SIEMENS MED-COM HEADER	3	Transformation Information

Attribute Name	Tag	Owner	Type	Notes
Application Header Sequence	(0029,xx40)	SIEMENS MED-COM HEADER	3	Sequence of Application Header items. Zero or more items are possible.
>Application Header Type	(0029,xx41)	SIEMENS MED-COM HEADER	1C	Application Header identification characteristics. Required, if Sequence is sent.
>Application Header ID	(0029,xx42)	SIEMENS MED-COM HEADER	3	Identification of an application header
>Application Header Version	(0029,xx43)	SIEMENS MED-COM HEADER	3	Version of CSA Series Header Info (0029,xx44) format.
>Application Header Info	(0029,xx44)	SIEMENS MED-COM HEADER	3	Application dependent information.
Workflow Control Flags	(0029,xx50)	SIEMENS MED-COM HEADER	3	Eight free definable flags.
Archive Management Flag Keep Online	(0029,xx51)	SIEMENS MED-COM HEADER	3	Flag to control remote archive management system to keep the image always online (also when already archived). Enumerated Values: 00 = remote control not required 01 = keep image online
Archive Management Flag Do Not Archive	(0029,xx52)	SIEMENS MED-COM HEADER	3	Flag to control remote archive management system not to archive the related image. Enumerated Values: 00 = remote control not required 01 = don't archive image
Image Location Status	(0029,xx53)	SIEMENS MED-COM HEADER	3	Image location status to control retrieving. Defined Terms: ONLINE = retrieving has to be done as usual, NEARLINE = move request to SCP and delay according to value of Estimated Retrieve Time (0029,xx54), OFFLINE = invoking a retrieve operation initiates an operator request, INVALID = invoking a retrieve operation would always result in an error.
Estimated Retrieve Time	(0029,xx54)	SIEMENS MED-COM HEADER	3	Estimated retrieve time in seconds. A value less than zero (< 0) indicates location is OFFLINE or INVALID.
Data Size of Retrieved Images	(0029,xx55)	SIEMENS MED-COM HEADER	3	Data size of images in MByte.
Series Workflow Status	(0029,xx60)	SIEMENS MED-COM HEADER2	3	

8.5.4.1.1 MEDCOM History Information

The value of the attribute MEDCOM History Information (0029,xx20) is defined in the following way:

Table 97 - MEDCOM History Information Attributes

Part	Name	Type	Bytes	Notes
header	Identifier	string	32	Always "CSA HISTORY"
	Version	string	32	e.g. "V1.10"
>n Items	Class Name	string	64	
	Modification String	string	1024	

8.5.4.2 MEDCOM OOG

The table in this section contains private IOD Attributes that describe MEDCOM Object Oriented Graphics (OOG). This module is used whenever object graphics is drawn on the image and need to be stored as graphic object properties. Given the condition that the module contents was not removed by other modalities, the graphic objects remain re-animatable if such an image was transferred and is then retrieved back.

Table 98 - MEDCOM OOG Attributes

Attribute Name	Tag	Owner	Type	Notes
CSA Series Header Type	(0029,xx08)	SIEMENS MEDCOM OOG	1	MEDCOM Object Oriented Graphics (OOG) identification characteristics. Defined Terms: MEDCOM OOG 1 MEDCOM OOG 2
CSA Series Header Version	(0029,xx09)	SIEMENS MEDCOM OOG	3	Version of MEDCOM OOG Info (0029,xx10) format.
CSA Series Header Info	(0029,xx10)	SIEMENS MEDCOM OOG	3	MEDCOM Object Oriented Graphics (OOG) data.

The graphics objects are also fully encoded in the Image Overlay Plane for compatibility with other products, which do not support the MedCom OOG module. Any system not supporting the MedCom OOG module shall remove the OOG module and its contents when modifying the image overlay plane content.

8.6 Private Transfer Syntaxes

No private Transfer Syntaxes are defined for or requested by syngo X Workplace DICOM application.

8.7 DICOM Print SCU – detailed status displays

The following tables document the behavior of the syngo X Workplace DICOM Print AE in response to messages received for the Printer SOP class and the Print Job SOP class.

Definition of camera symbols:

- Idle: Camera is installed and ready; idle icon is displayed.
- Interact: The user has to react in near future, but not immediately.
Example: A camera was low in 8x10 clear sheets: LOW 8x10 CLR was sent by N-EVENT-REPORT.
- Queue Stopped: The user has to react immediately. Either the camera needs immediate interaction, or a job has been aborted.
Example: A camera is out of 8x10 clear sheets, or camera is down, or a film job is aborted

Note: different camera symbols are displayed according to the Printer Status Info.

8.7.1 Common Status Information

Table 99 – Print SCU Common Status Information

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
NORMAL	Camera is ready	Camera is ready	<None>/idle
BAD RECEIVE MGZ	There is a problem with the film receive magazine. Films from the printer cannot be transported into the magazine.	Problem with receive magazine.	<None>/interact
BAD SUPPLY MGZ	There is a problem with the film supply magazine. Films from this magazine cannot be transported into the printer.	Problem with supply magazine.	<None>/interact
CALIBRATING	Printer is performing self calibration; it is expected to be available for normal operation shortly.	Self calibration. Please wait.	<None>/idle

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera sym- bol'
CALIBRATION ERR	An error in the printer calibration has been detected, quality of processed films may not be optimal.	Problem in calibration. Film quality may not be optimal.	<None>/interact
CHECK CHEMISTRY	A problem with the processor chemicals has been detected, quality of processed films may not be optimal.	Problem with chemistry. Film quality may not be optimal.	<None>/interact
CHECK SORTER	There is an error in the film sorter	Error in film sorter.	<None>/interact
CHEMICALS EMPTY	There are no processing chemicals in the processor, films will not be printed and processed until the processor is back to normal.	Camera chemistry empty. Please check.	<None>/interact
CHEMICALS LOW	The chemical level in the processor is low, if not corrected, it will probably shut down soon.	Camera chemistry low. Please check.	<None>/interact
COVER OPEN	One or more printer or processor covers, drawers, doors are open.	Camera cover, drawer or door open.	<None>/interact
ELEC CONFIG ERR	Printer configured improperly for this job.	Camera configured improperly for this job. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
ELEC DOWN	Printer is not operating due to some unspecified electrical hardware problem.	Camera electrical hardware Problem.	<None>/interact
ELEC SW ERROR	Printer not operating for some unspecified software error.	Camera software problem. Queue stopped.	Queue for this camera will be STOPPED/ Queue stopped
EMPTY 8x10	The 8x10 inch film supply magazine is empty.	8x10 film supply empty.	<None>/interact
EMPTY 8x10 BLUE	The 8x10 inch blue film supply magazine is empty.	8x10 blue film supply empty.	<None>/interact
EMPTY 8x10 CLR	The 8x10 inch clear film supply magazine is empty.	8x10 clear film supply empty.	<None>/interact
EMPTY 8x10 PAPER	The 8x10 inch paper supply magazine is empty.	8x10 paper supply empty.	<None>/interact
EMPTY 10x12	The 10x12 inch film supply magazine is empty.	10x12 film supply empty.	<None>/interact
EMPTY 10x12 BLUE	The 10x12 inch blue film supply magazine is empty.	10x12 blue film supply empty.	<None>/interact
EMPTY 10x12 CLR	The 10x12 inch clear film supply magazine is empty.	10x12 clear film supply empty.	<None>/interact
EMPTY 10x12 PAPER	The 10x12 inch paper supply magazine is empty.	10x12 paper supply empty.	<None>/interact
EMPTY 10x14	The 10x14 inch film supply magazine is empty.	10x14 film supply empty.	<None>/interact
EMPTY 10x14 BLUE	The 10x14 inch blue film supply magazine is empty.	10x14 blue film supply empty.	<None>/interact
EMPTY 10x14 CLR	The 10x14 inch clear film supply magazine is empty.	10x14 clear film supply empty.	<None>/interact
EMPTY 10x14 PAPER	The 10x14 inch paper supply magazine is empty.	10x14 paper supply empty.	<None>/interact
EMPTY 11x14	The 11x14 inch film supply magazine is empty.	11x14 film supply empty.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera sym- bol'
EMPTY 11x14 BLUE	The 11x14 inch blue film supply magazine is empty.	11x14 blue film supply empty.	<None>/interact
EMPTY 11x14 CLR	The 11x14 inch clear film supply magazine is empty.	11x14 clear film supply empty.	<None>/interact
EMPTY 11x14 PAPR	The 11x14 inch paper supply magazine is empty.	11x14 paper supply empty.	<None>/interact
EMPTY 14x14	The 14x14 inch film supply magazine is empty.	14x14 film supply empty.	<None>/interact
EMPTY 14x14 BLUE	The 14x14 inch blue film supply magazine is empty.	14x14 blue film supply empty.	<None>/interact
EMPTY 14x14 CLR	The 14x14 inch clear film supply magazine is empty.	14x14 clear film supply empty.	<None>/interact
EMPTY 14x14 PAPR	The 14x14 inch paper supply magazine is empty.	14x14 paper supply empty.	<None>/interact
EMPTY 14x17	The 14x17 inch film supply magazine is empty.	14x17 film supply empty.	<None>/interact
EMPTY 14x17 BLUE	The 14x17 inch blue film supply magazine is empty.	14x17 blue film supply empty.	<None>/interact
EMPTY 14x17 CLR	The 14x17 inch clear film supply magazine is empty.	14x17 clear film supply empty.	<None>/interact
EMPTY 14x17 PAPR	The 14x17 inch paper supply magazine is empty.	14x17 paper supply empty.	<None>/interact
EMPTY 24x24	The 24x24 inch film supply magazine is empty.	24x24 film supply empty.	<None>/interact
EMPTY 24x24 BLUE	The 24x24 inch blue film supply magazine is empty.	24x24 blue film supply empty.	<None>/interact
EMPTY 24x24 CLR	The 24x24 inch clear film supply magazine is empty.	24x24 clear film supply empty.	<None>/interact
EMPTY 24x24 PAPR	The 24x24 inch paper supply magazine is empty.	24x24 paper supply empty.	<None>/interact
EMPTY 24x30	The 24x30 inch film supply magazine is empty.	24x30 film supply empty.	<None>/interact
EMPTY 24x30 BLUE	The 24x30 inch blue film supply magazine is empty.	24x30 blue film supply empty.	<None>/interact
EMPTY 24x30 CLR	The 24x30 inch clear film supply magazine is empty.	24x30 clear film supply empty.	<None>/interact
EMPTY 24x30 PAPR	The 24x30 inch paper supply magazine is empty.	24x30 paper supply empty.	<None>/interact
EMPTY A4 PAPR	The A4 paper supply magazine is empty.	A4 paper supply empty.	<None>/interact
EMPTY A4 TRANS	The A4 transparency supply magazine is empty.	A4 transparency supply empty.	<None>/interact
EXPOSURE FAILURE	The exposure device has failed due to some unspecified reason.	Exposure device has failed.	<None>/interact
FILM JAM	A film transport error has occurred and a film is jammed in the printer or processor.	Film jam.	<None>/interact
FILM TRANSP ERR	There is a malfunction with the film transport, there may or may not be a film jam.	Film transport problem.	<None>/interact
FINISHER EMPTY	The finisher is empty.	Finisher is empty.	<None>/interact
FINISHER ERROR	The finisher is not operating due to some unspecified reason.	Finisher problem.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera sym- bol'
FINISHER LOW	The finisher is low on supplies.	Finisher low.	<None>/interact
LOW 8x10	The 8x10 inch film supply magazine is low.	8x10 film supply low.	<None>/interact
LOW 8x10 BLUE	The 8x10 inch blue film supply magazine is low.	8x10 blue film supply low.	<None>/interact
LOW 8x10 CLR	The 8x10 inch clear film supply magazine is low.	8x10 clear film supply low.	<None>/interact
LOW 8x10 PAPR	The 8x10 inch paper supply magazine is low.	8x10 paper supply low.	<None>/interact
LOW 10x12	The 10x12 inch film supply magazine is low.	10x12 film supply low.	<None>/interact
LOW 10x12 BLUE	The 10x12 inch blue film supply magazine is low.	10x12 blue film supply low.	<None>/interact
LOW 10x12 CLR	The 10x12 inch clear film supply magazine is low.	10x12 clear film supply low.	<None>/interact
LOW 10x12 PAPR	The 10x12 inch paper supply magazine is low.	10x12 paper supply low.	<None>/interact
LOW 10x14	The 10x14 inch film supply magazine is low.	10x14 film supply low.	<None>/interact
LOW 10x14 BLUE	The 10x14 inch blue film supply magazine is low.	10x14 blue film supply low.	<None>/interact
LOW 10x14 CLR	The 10x14 inch clear film supply magazine is low.	10x14 clear film supply low.	<None>/interact
LOW 10x14 PAPR	The 10x14 inch paper supply magazine is low.	10x14 paper supply low.	<None>/interact
LOW 11x14	The 11x14 inch film supply magazine is low.	11x14 film supply low.	<None>/interact
LOW 11x14 BLUE	The 11x14 inch blue film supply magazine is low.	11x14 blue film supply low.	<None>/interact
LOW 11x14 CLR	The 11x14 inch clear film supply magazine is low.	11x14 clear film supply low.	<None>/interact
LOW 11x14 PAPR	The 11x14 inch paper supply magazine is low.	11x14 paper supply low.	<None>/interact
LOW 14x14	The 14x14 inch film supply magazine is low.	14x14 film supply low.	<None>/interact
LOW 14x14 BLUE	The 14x14 inch blue film supply magazine is low.	14x14 blue film supply low.	<None>/interact
LOW 14x14 CLR	The 14x14 inch clear film supply magazine is low.	14x14 clear film supply low.	<None>/interact
LOW 14x14 PAPR	The 14x14 inch paper supply magazine is low.	14x14 paper supply low.	<None>/interact
LOW 14x17	The 14x17 inch film supply magazine is low.	14x17 film supply low.	<None>/interact
LOW 14x17 BLUE	The 14x17 inch blue film supply magazine is low.	14x17 blue film supply low.	<None>/interact
LOW 14x17 CLR	The 14x17 inch clear film supply magazine is low.	14x17 clear film supply low.	<None>/interact
LOW 14x17 PAPR	The 14x17 inch paper supply magazine is low.	14x17 paper supply low.	<None>/interact
LOW 24x24	The 24x24 inch film supply magazine is low.	24x24 film supply low.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera sym- bol'
LOW 24x24 BLUE	The 24x24 inch blue film supply magazine is low.	24x24 blue film supply low.	<None>/interact
LOW 24x24 CLR	The 24x24 inch clear film supply magazine is low.	24x24 clear film supply low.	<None>/interact
LOW 24x24 PAPER	The 24x24 inch paper supply magazine is low.	24x24 paper supply low.	<None>/interact
LOW 24x30	The 24x30 inch film supply magazine is low.	24x30 film supply low.	<None>/interact
LOW 24x30 BLUE	The 24x30 inch blue film supply magazine is low.	24x30 blue film supply low.	<None>/interact
LOW 24x30 CLR	The 24x30 inch clear film supply magazine is low.	24x30 clear film supply low.	<None>/interact
LOW 24x30 PAPER	The 24x30 inch paper supply magazine is low.	24x30 paper supply low.	<None>/interact
LOW A4 PAPER	The A4 paper supply magazine is low.	A4 paper supply low.	<None>/interact
LOW A4 TRANS	The A4 transparency supply magazine is low.	A4 transparency supply low.	<None>/interact
NO RECEIVE MGZ	The film receive magazine is not available.	Film receiver not available.	<None>/interact
NO RIBBON	The ribbon cartridge needs to be replaced.	Replace ribbon cartridge.	<None>/interact
NO SUPPLY MGZ	The film supply magazine is not available.	Film supply not available.	<None>/interact
CHECK PRINTER	The printer is not ready at this time, operator intervention is required to make the printer available.	Check camera.	<None>/interact
CHECK PROC	The processor is not ready at this time, operator intervention is required to make the printer available.	Check processor.	<None>/interact
PRINTER DOWN	The printer is not operating due to some unspecified reason.	Camera down.	<None>/interact
PRINTER INIT	The printer is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Camera initializing.	<None>/Idle
PRINTER OFFLINE	The printer has been disabled by an operator or service person.	Camera off-line.	<None>/interact
PROC DOWN	The processor is not operating due to some unspecified reason.	Processor down.	<None>/interact
PROC INIT	The processor is not ready at this time, it is expected to become available without intervention. For example, it may be in a normal warm-up state.	Processor initializing.	<None>/Idle
PROC OVERFLOW FL	Processor chemicals are approaching the overflow full mark.	Processor chemicals near overflow.	<None>/interact
PROC OVERFLOW HI	Processor chemicals have reached the overflow full mark.	Processor chemicals overflow.	<None>/interact
QUEUED	Print job in Queue	--	<None>/Idle
RECEIVER FULL	The film receive magazine is full.	Receiver full.	<None>/interact

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
REQ MED NOT INST	The requested film, paper, or other media supply magazine is installed in the printer but may be available with operator intervention.	Install media supply.	<None>/interact
REQ MED NOT AVAI	The requested film, paper, or other media requested is not available on this printer.	Media supply not available on this camera. Queue stopped. Change camera.	Queue for this camera will be STOPPED/ Queue stopped
RIBBON ERROR	There is an unspecified problem with the print ribbon.	Error with print ribbon.	<None>/interact
SUPPLY EMPTY	The printer is out of film.	Camera out of film.	<None>/interact
SUPPLY LOW	The film supply is low.	Film supply low.	<None>/interact
UNKNOWN	There is an unspecified problem.	Unspecified problem with camera.	<None>/interact

8.7.2 Additional DICOM Execution Status Information

Table 100 – Print SCU Additional DICOM Execution Status Evaluation

Printer Status Info/ Execution Status Info	Description	Message string visible in 'Status Bar'	Other action for UI/ 'camera symbol'
INVALID PAGE DES	The specified page layout cannot be printed, or other page description errors have been detected.	Film Job cannot be printed on this camera. Queue stopped. Please redirect film job.	Queue for this camera will be STOPPED/ Queue stopped
INSUFFICIENT MEMORY	There is not enough memory available to complete this job.	Not enough memory available in camera. Queue stopped. Please continue queue or change camera.	Queue for this camera will be STOPPED/ Queue stopped
NONE	General printer warning, no specific information is available. Spooling of print jobs to disk is still possible.	--	<None>/Idle

8.7.3 Unknown DICOM Execution Status Information

Printer Status Info and Execution Status Info are defined terms and can therefore be extended or reduced by camera manufacturers. Therefore syngo X Workplace Print AE shall be flexible.

If any other printer status info or execution status info is received, syngo X Workplace will react as shown in the following table:

Table 101 – Print SCU Unknown DICOM Execution Status Information

Printer Status/ Execution	Printer / Execution Status Info	Description	Message string visible in the HCD 'Status Bar'	Other action for UI/ 'camera symbol'
WARNING	<any other>	<not defined status info>	Camera Info: <status info>	<none>/interact>

Printer Status/ Execution	Printer / Execution Status Info	Description	Message string visible in the HCD 'Status Bar'	Other action for UI/ 'camera symbol'
FAILURE	<any other>	<not defined status info>	Camera Info: <status info> Queue stopped	Queue for this camera will be STOPPED/ Queue stopped

Annex A: Index of Tables

Table 1 - Network Services	2
Table 2 - Media Services.....	3
Table 3 - Implementation Identifying Information	3
Table 4 - Revision History	6
Table 5 - Presentation Context Table "Verification"	13
Table 6 - Presentation Context Table "Send to ..."	15
Table 7 - Presentation Context Table "Return Commitment Result"	17
Table 8 - Status codes "Save to local disk"	17
Table 9 - Presentation Context Table "Save to local disk"	19
Table 10 - Order of Preference Transfer Syntax	19
Table 11 - Presentation Context Table "Evaluate Commit Request"	22
Table 12 - Presentation Context Table "Update Flag Information"	23
Table 13 - Supported DIMSE-C Operations - Query/Retrieve SCU	24
Table 14 - Presentation Context Table "Search..."	24
Table 15 - C-FIND RQ Search Keys	25
Table 16 - Status Codes "Search..."	26
Table 17 - Presentation Context Table "Import..."	27
Table 18 - C-MOVE RSP Status Codes.....	27
Table 19 - Presentation Context Table "Process Search Requests"	29
Table 20 - Query/Retrieve SCP supported attributes	30
Table 21 - Status Codes Process Search Request	32
Table 22 - Presentation Context Table "Process Retrieve Requests"	32
Table 23 - Status Codes "Process Retrieve Requests"	33
Table 24 - Presentation Context Table "Print Film"	34
Table 25 - Basic Film Session N-CREATE attributes	36
Table 26 - Basic Film Session Status Codes	36
Table 27 - Basic Film Box N-CREATE attributes	36
Table 28 - Basic Film Box Status Codes	37
Table 29 - Basic Grayscale Image Box N-SET attributes.....	37
Table 30 - Basic Grayscale Image Box Status Codes.....	38
Table 31 - Basic Color Image Box N-SET attributes	38
Table 32 - Basic Color Image Box Status Codes	38
Table 33 - Presentation LUT N-CREATE attribute	39
Table 34 - Presentation LUT Status Codes	39
Table 35 - Used Printer N-EVENT Report attributes	39
Table 36 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes.....	39
Table 37 - Used Print Job N-EVENT Report attributes.....	40
Table 38 - Presentation Context Table "Show Device Status"	41
Table 39 - Used Printer N-EVENT Report attributes	41
Table 40 - Mandatory Printer N-GET-RSP, N-EVENT-REPORT-RQ attributes.....	41
Table 41 - Default AET Characteristics	42
Table 42 - Remote AE Configuration Items.....	42
Table 43 - General parameter settings and timeouts	43
Table 44: Implementation Class/Version Name - Media Interchange	46
Table 45: Media - Application Profiles and Real-World Activities	47
Table 46: Transfer Syntaxes for STD-GEN-xxx	48
Table 47 - Supported Single-Byte Character Sets (w/o Code Ext.).....	49
Table 48 - Supported Single-Byte Character Sets (with Code Ext.)	49
Table 49 - Supported Multi-Byte Character Sets (w/o Code Ext.)	49
Table 50 - Supported Multi-Byte Character Sets (with Code Ext.)	49
Table 51: Application Level Confidentiality Profile attributes (standard tags)	53
Table 52 – Patient level attributes	55
Table 53 – Study level attributes	55
Table 54 - SC Derived Image (Monochrome) from Composing	56
Table 55 - SC Derived Image (RGB) from 3D Projections	58
Table 56 - SC Derived Image (RGB) for 4D Viewer Bookmarks	60
Table 57 - SC Derived Image (RGB) from iFlow	62
Table 58 - XA/XRF Derived Image (Monochrome) Store Monitor	63
Table 59 - XA/XRF Derived Quant Report Image (Monochrome)	66
Table 60 - CT Derived Image (Monochrome) from Reconstruction	68
Table 61 – Ranges / Save Image as CT Derived Image (Monochrome)	71
Table 62 – Ranges / Save Image as MR Derived Image (Monochrome)	73
Table 63 – X-Ray 3D Angiographic Image from 4D DSA Reconstruction	75
Table 64 - Private Orthopedic Report Comprehensive SR from Composing	80
Table 65 - Segmentation Results from 3D Applications	81

Table 66 – General 3D Graphic Results Storage	83
Table 67 – Rigid 3D/3D Registration Result.....	86
Table 68 - Data Dictionary of Private Attributes	88
Table 69 - CID Cx01 Scoliosis Types Type: Extensible	93
Table 70 - CID Cx02 Orthopedic Measurement Types Type: Extensible	93
Table 71 - CID Cx03 Vertebra Descriptors Type: Extensible	93
Table 72 - CID Cx04 Scoliosis Location Type: Extensible.....	94
Table 73 - CID Cx05 Scoliosis Direction Type: Extensible.....	94
Table 74 - (Private) Orthopedic Report Template	95
Table 75 - TID Tx50001 Orthopedic Report Type: Extensible.....	95
Table 76 - TID Tx50010 Orthopedic Report Session Type: Extensible	96
Table 77 – TID 1002 OBSERVER CONTEXT Type: Non-Extensible	96
Table 78 - TID 1003 PERSON OBSERVER IDENTIFYING ATTRIBUTES Type: Extensible	96
Table 79 - TID 1005 PROCEDURE CONTEXT Type: Non-Extensible	96
Table 80 - TID 1006 SUBJECT CONTEXT Type: Non-Extensible.....	97
Table 81 - TID 1007 SUBJECT CONTEXT, PATIENT Type: Extensible	97
Table 82 - TID Tx50020 Referenced Images Type: Extensible.....	98
Table 83 - TID Tx50100 Orthopedic Measurements Type: Extensible.....	98
Table 84 - TID Tx50101 Vertical Alignment Properties Type: Extensible.....	99
Table 85 - TID Tx50102 Cobb Angle Properties Type: Extensible.....	100
Table 86 - TID Tx50103 Kyphosis Angle Properties Type: Extensible	101
Table 87 - Private Modules for Standard Extended XA.....	101
Table 88 - (Private) Angio Viewing Module Attributes	102
Table 89 - (Private) Angio Quantification Module Attributes.....	103
Table 90 - (Private) Original Image Info Module Attributes.....	104
Table 91 - Private Modules for other created SOP Class.....	105
Table 92 – Private Segmentation Attributes	105
Table 93 - Private Modules for other created SOP Class.....	106
Table 94 – Private Segmentation Attributes	106
Table 95 - Private Modules for other created SOP Class.....	109
Table 96 - MEDCOM Header Attributes.....	109
Table 97 - MEDCOM History Information Attributes.....	110
Table 98 - MEDCOM OOG Attributes	111
Table 99 – Print SCU Common Status Information	111
Table 100 – Print SCU Additional DICOM Execution Status Evaluation	116
Table 101 – Print SCU Unknown DICOM Execution Status Information.....	116

On account of certain regional limitations of sales rights and service availability, we cannot guarantee that all products included in this brochure are available through the Siemens sales organization worldwide. Availability and packaging may vary by country and are subject to change without prior notice.

Some/All of the features and products described herein may not be available in the United States or other countries.

The information in this document contains general technical descriptions of specifications and options as well as standard and optional features that do not always have to be present in individual cases.

Siemens reserves the right to modify the design, packaging, specifications and options described herein without prior notice. Please contact your local Siemens sales representative for the most current information.

In the interest of complying with legal requirements concerning the environmental compatibility of our products (protection of natural resources and waste conservation), we recycle certain components. Using the same extensive quality assurance measures as for factory-new components, we guarantee the quality of these recycled components.

Note: Any technical data contained in this document may vary within defined tolerances. Original images always lose a certain amount of detail when reproduced.

Caution: Federal law restricts this device to sale by or on the order of a physician.

Siemens Healthineers Headquarters

Siemens Healthcare GmbH
Henkestr. 127
91052 Erlangen, Germany
Phone: +49 9131 84-0
siemens-healthineers.com

Published by Siemens Healthcare GmbH · Doc-Ident. 11275126-ESK-001-00 · ©Siemens Healthcare GmbH, 2020